

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
 Data File : PS015865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2021 05:24
 Operator : DD\AJ
 Sample : M2639-02
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 01:51:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.766	779.6E6	258.9E6	469.240	513.875
Target Compounds							
1) T	Dalapon	2.975f	2.481	26574095	36861043	13.166	56.755 #
2) T	3,5-DICHL...	0.000	5.982	0	73256051	N.D.	97.135
3) T	4-Nitroph...	7.026	0.000	4485136	0	4.933	N.D. #
6) T	MCP	7.544	0.000	7397817	0	1.362	N.D. #
8) T	DICHLORPROP	0.000	7.569	0	22486500	N.D.	43.432
10) T	Pentachlo...	8.610	8.266	15669108	8007565	<MDL	1.140 #
12) T	2,4,5-T	9.388f	9.075f	47734117	11750314	5.407	4.166
13) T	2,4-DB	9.964	0.000	59158995	0	28.921	N.D. #
14) T	DINOSEB	11.119f	9.878	52758708	70196124	8.146	34.852 #
15) T	Picloram	10.972	10.821	38924766	12633473	2.847	3.004
16) T	DCPA	0.000	10.821f	0	12633473	N.D.	3.005



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
Data File : PS015865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2021 05:24
Operator : DD\AJ
Sample : M2639-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 01:51:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

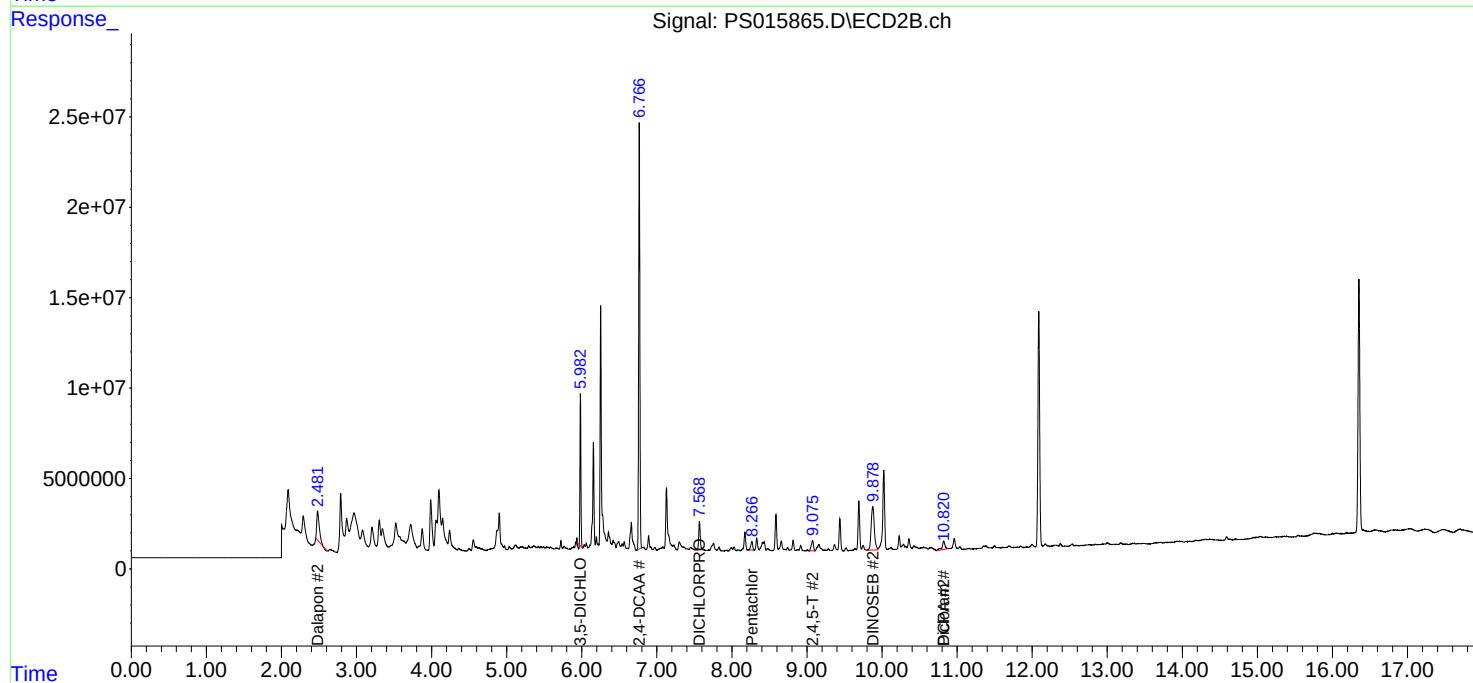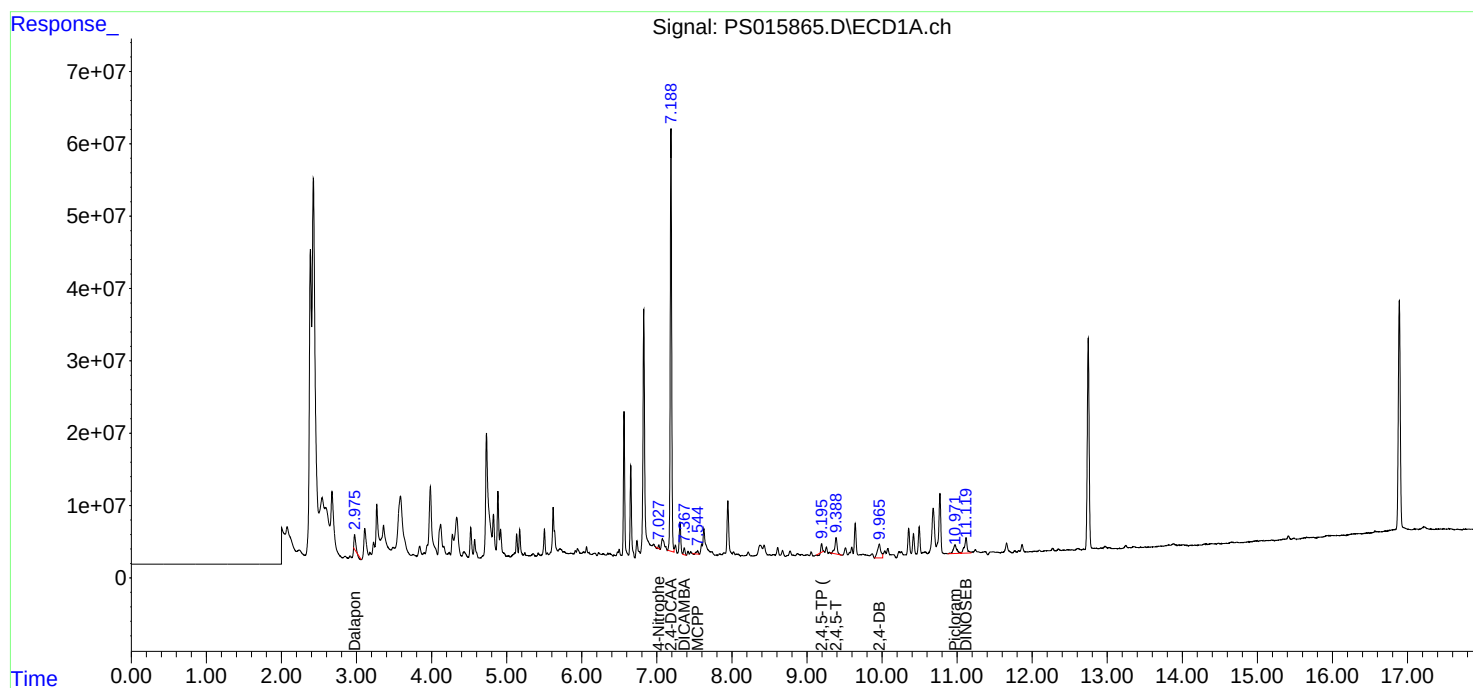


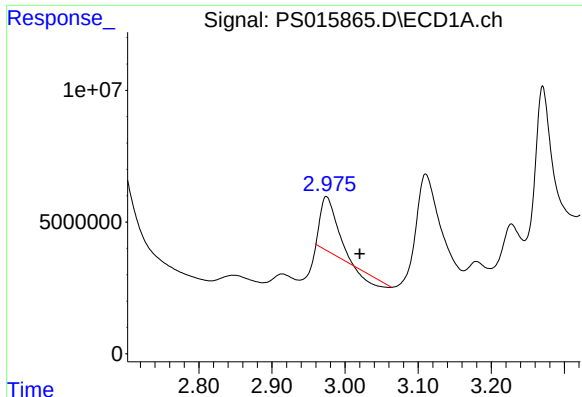

#1 Dalapon


R.T.: 2.975 min
Delta R.T.: -0.045 min
Response: 26574095
Conc: 13.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

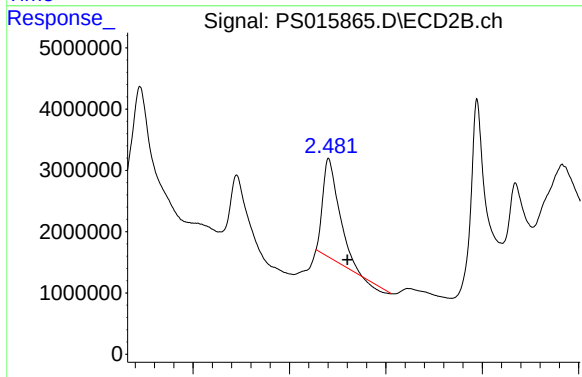


#1 Dalapon

R.T.: 2.481 min
Delta R.T.: -0.040 min
Response: 36861043
Conc: 56.75 ng/ml

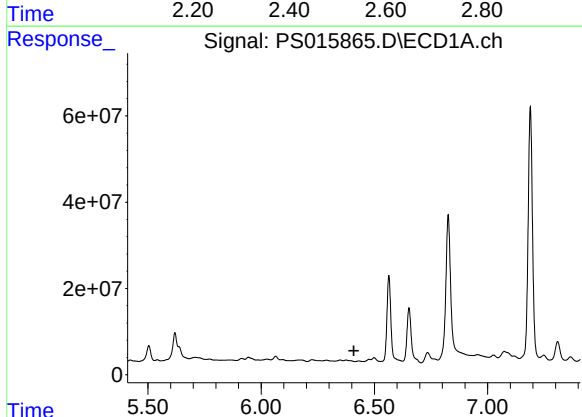


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

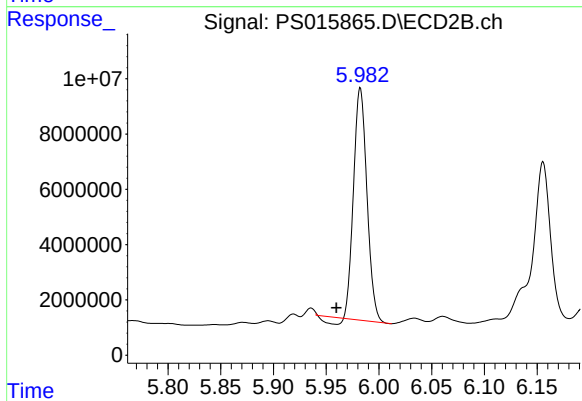

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.982 min
Delta R.T.: 0.023 min
Response: 73256051
Conc: 97.14 ng/ml

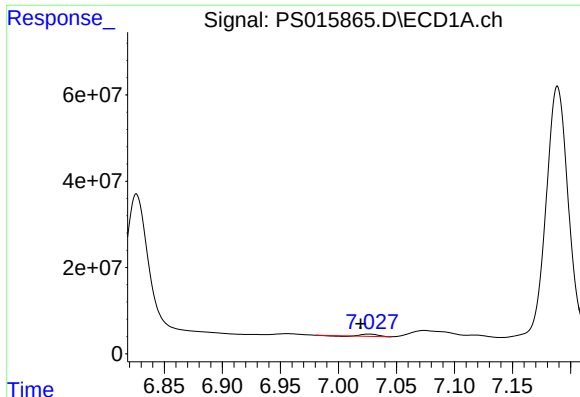

#3 4-Nitrophenol


R.T.: 7.026 min
Delta R.T.: 0.007 min
Response: 4485136
Conc: 4.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

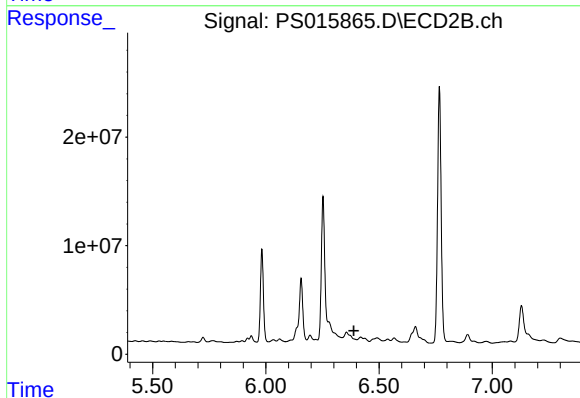


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

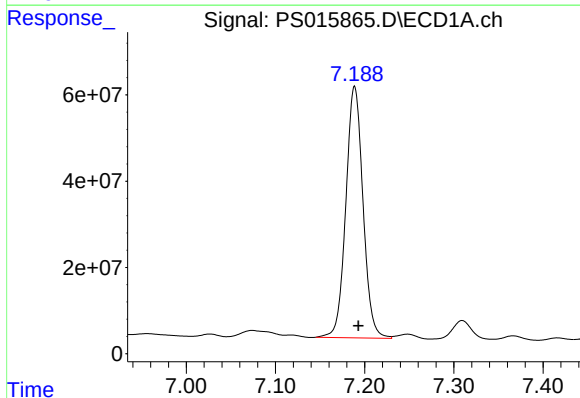


#4 2,4-DCAA

R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 779617141
Conc: 469.24 ng/ml

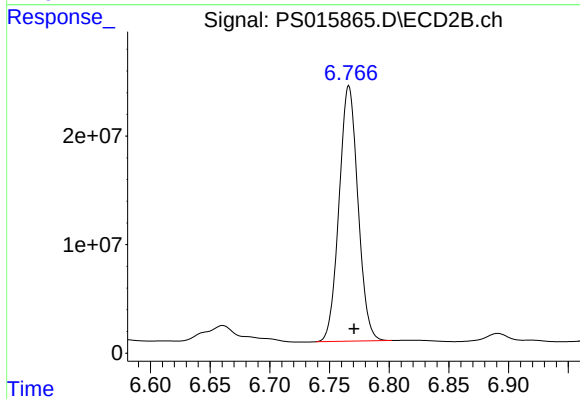

#4 2,4-DCAA


R.T.: 6.766 min
Delta R.T.: -0.004 min
Response: 258916681
Conc: 513.87 ng/ml

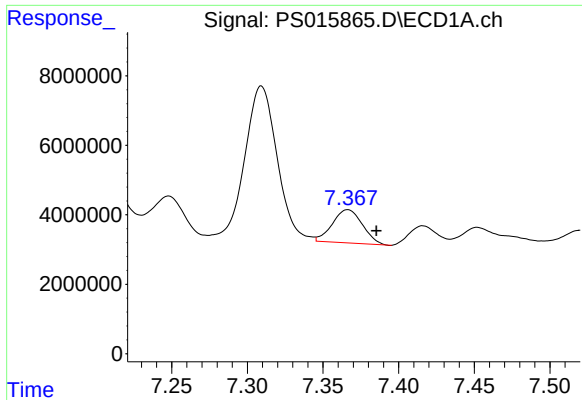

#5 DICAMBA


R.T.: 7.366 min
Delta R.T.: -0.019 min
Response: 13248601
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

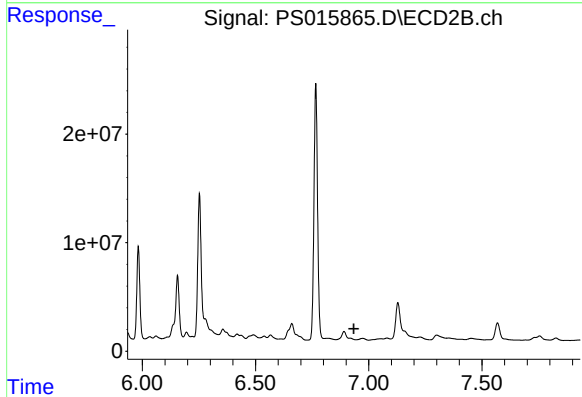


#5 DICAMBA

R.T.: 6.891 min
Delta R.T.: -0.044 min
Response: -6980831
Conc: N.D.

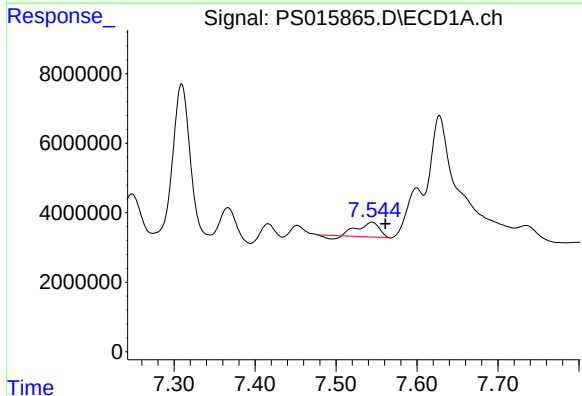


#6 MCP

R.T.: 7.544 min
Delta R.T.: -0.017 min
Response: 7397817
Conc: 1.36 ug/ml

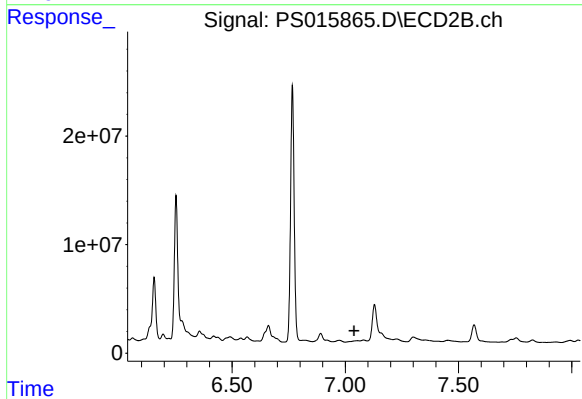

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.038 min
Response: 0
Conc: N.D.

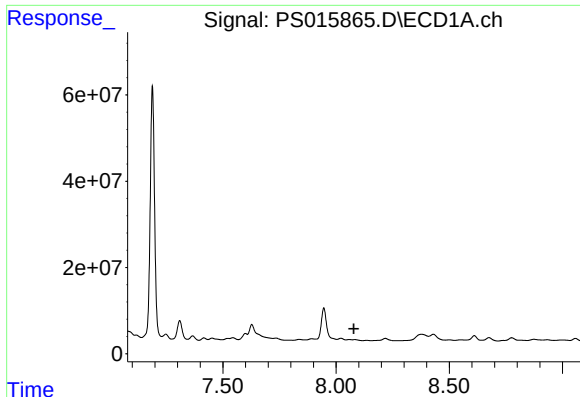

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

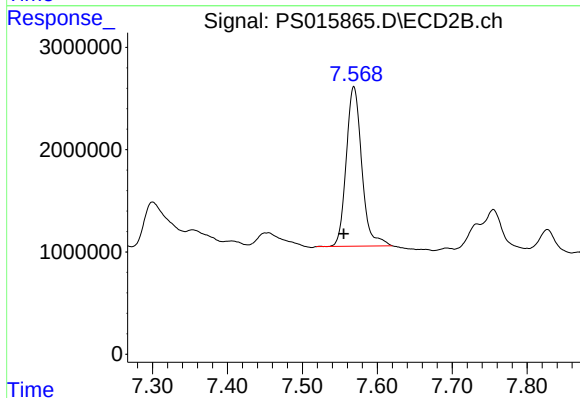


#8 DICHLORPROP

R.T.: 7.569 min
Delta R.T.: 0.013 min
Response: 22486500
Conc: 43.43 ng/ml

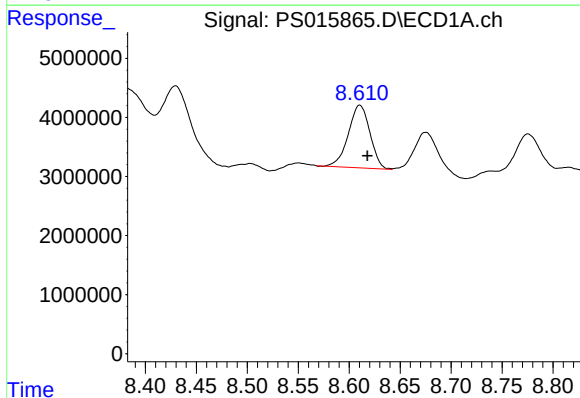


#10 Pentachlorophenol

R.T.: 8.610 min
Delta R.T.: -0.007 min
Response: 15669108
Conc: N.D.

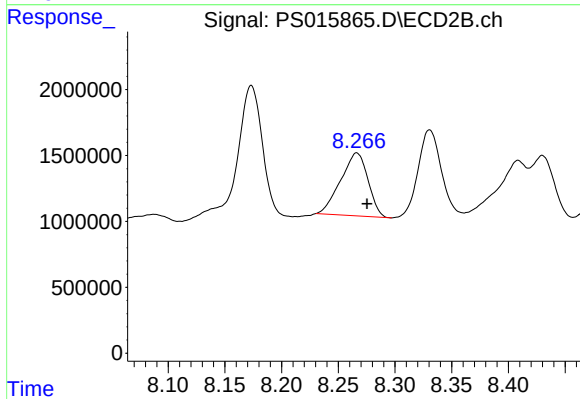

#10 Pentachlorophenol


R.T.: 8.266 min
Delta R.T.: -0.009 min
Response: 8007565
Conc: 1.14 ng/ml

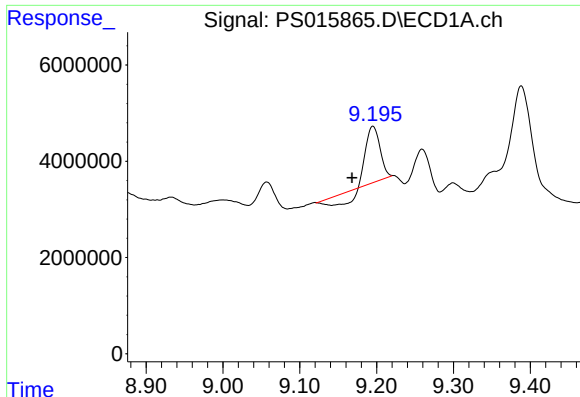

#11 2,4,5-TP (SILVEX)


R.T.: 9.195 min
Delta R.T.: 0.027 min
Response: 11750312
Conc: 1.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

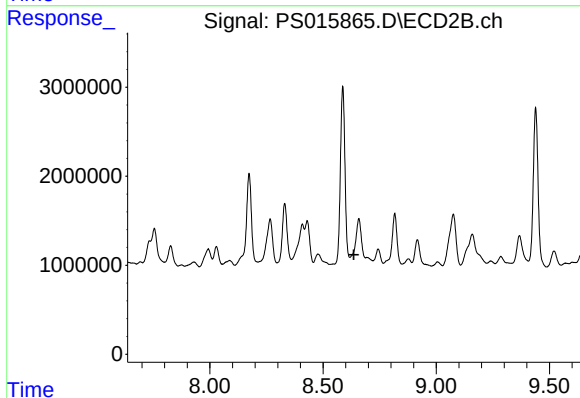


#11 2,4,5-TP (SILVEX)

R.T.: 8.658 min
Delta R.T.: 0.022 min
Response: -7602492
Conc: N.D.

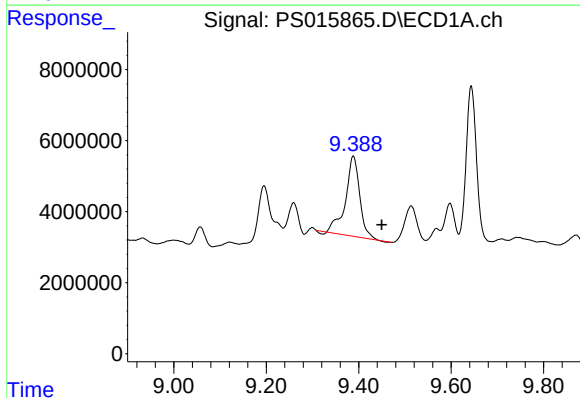


#12 2,4,5-T

R.T.: 9.388 min
Delta R.T.: -0.062 min
Response: 47734117
Conc: 5.41 ng/ml

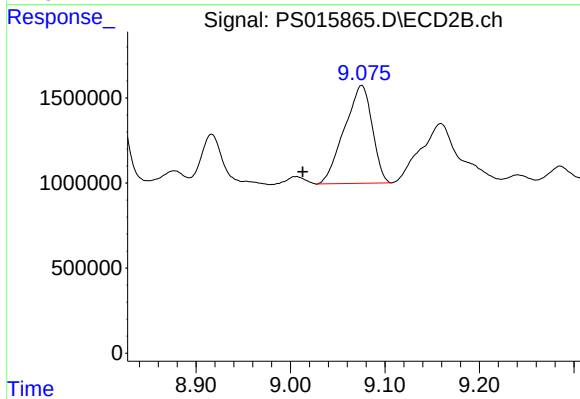

#12 2,4,5-T


R.T.: 9.075 min
Delta R.T.: 0.062 min
Response: 11750314
Conc: 4.17 ng/ml

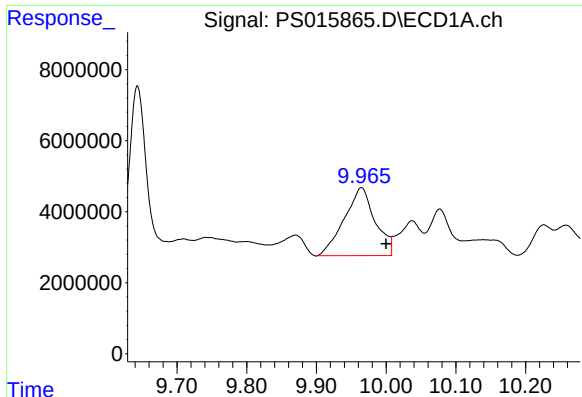

#13 2,4-DB


R.T.: 9.964 min
Delta R.T.: -0.036 min
Response: 59158995
Conc: 28.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

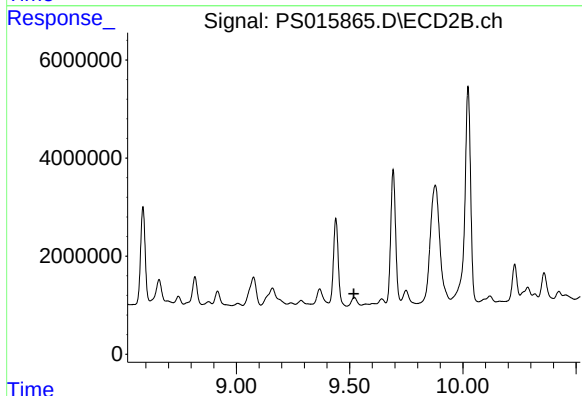


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.519 min
Response: 0
Conc: N.D.

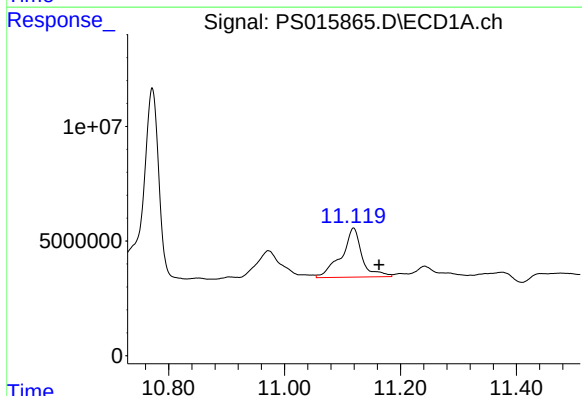


#14 DINOSEB

R.T.: 11.119 min
Delta R.T.: -0.044 min
Response: 52758708
Conc: 8.15 ng/ml

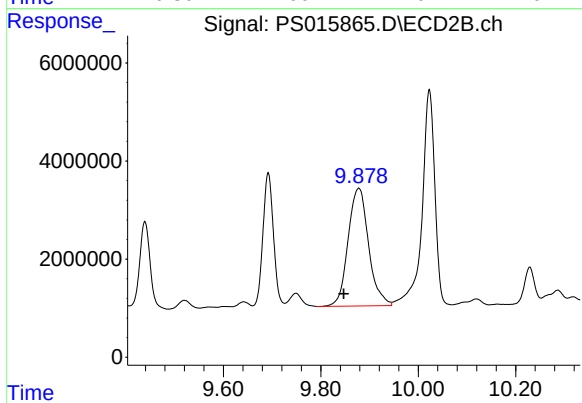

#14 DINOSEB


R.T.: 9.878 min
Delta R.T.: 0.031 min
Response: 70196124
Conc: 34.85 ng/ml

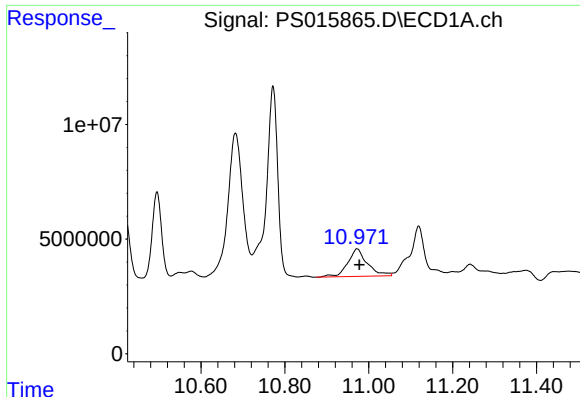

#15 Picloram


R.T.: 10.972 min
Delta R.T.: -0.006 min
Response: 38924766
Conc: 2.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

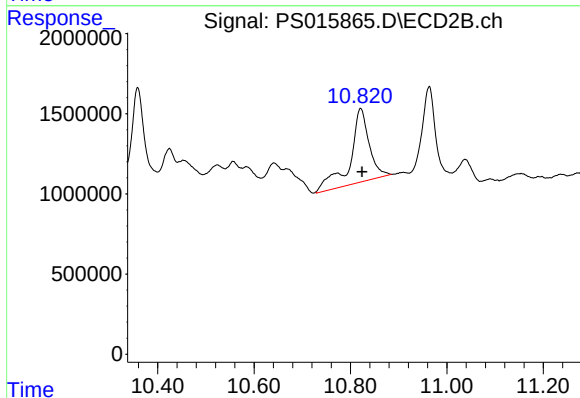


#15 Picloram

R.T.: 10.821 min
Delta R.T.: -0.003 min
Response: 12633473
Conc: 3.00 ng/ml

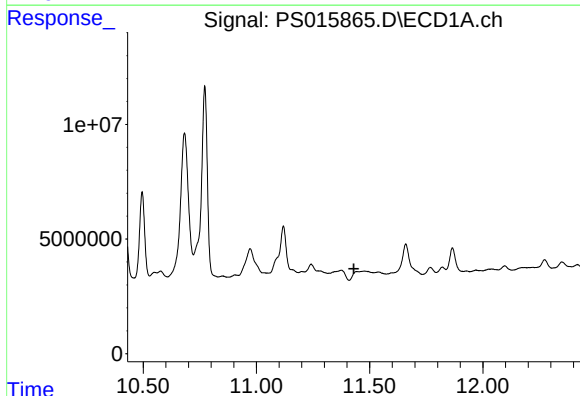

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.431 min
Response: 0
Conc: N.D.

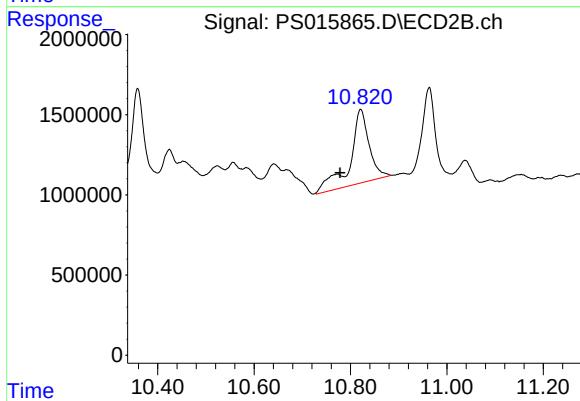

#16 DCPA

R.T.: 10.821 min
Delta R.T.: 0.043 min
Response: 12633473
Conc: 3.00 ng/ml