

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
 Data File : PS015873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2021 08:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 01:54:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.766	781.6E6	276.4E6	470.408	548.641
Target Compounds							
12) T	2,4,5-T	9.447	9.059f	13263228	6944474	1.502	2.462 #
15) T	Picloram	10.977	10.819	61839484	27506739	4.523	6.541 #
16) T	DCPA	11.419	10.819f	12326732	27506739	<MDL	6.543 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
Data File : PS015873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2021 08:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 01:54:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

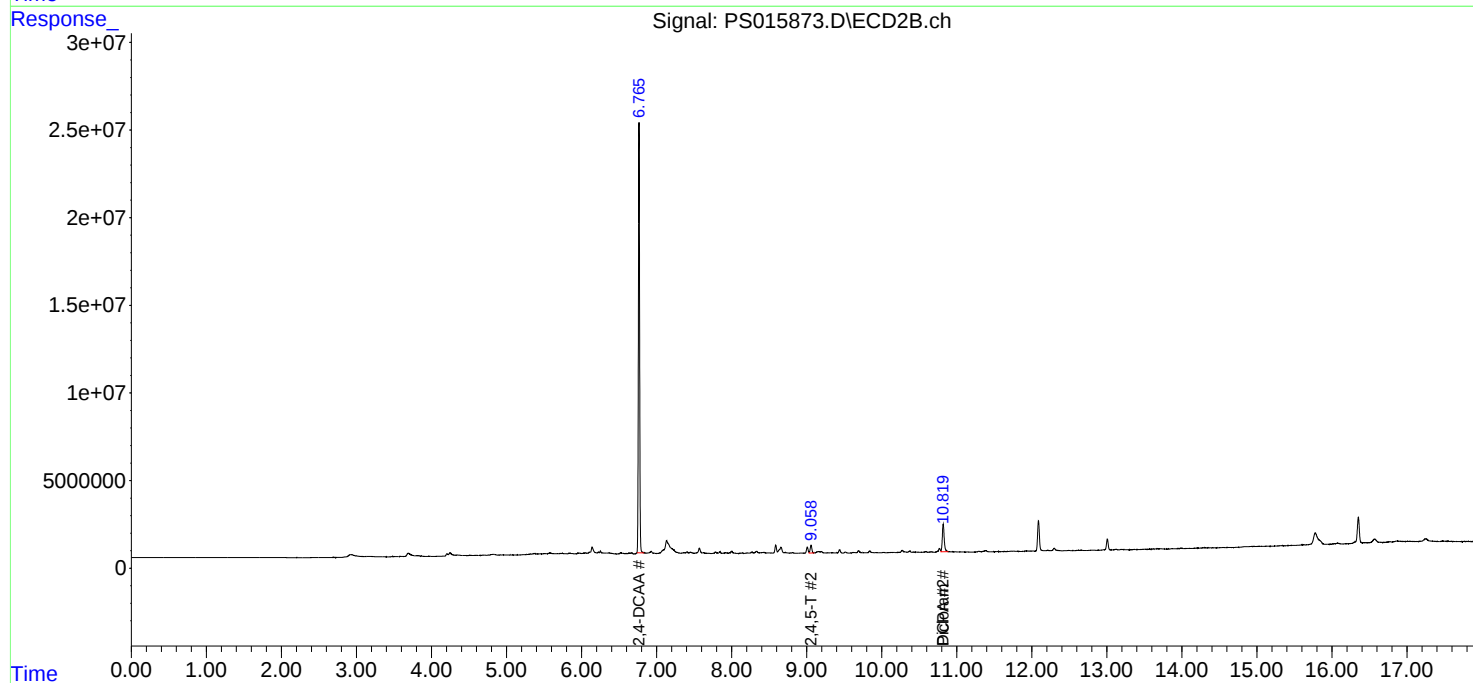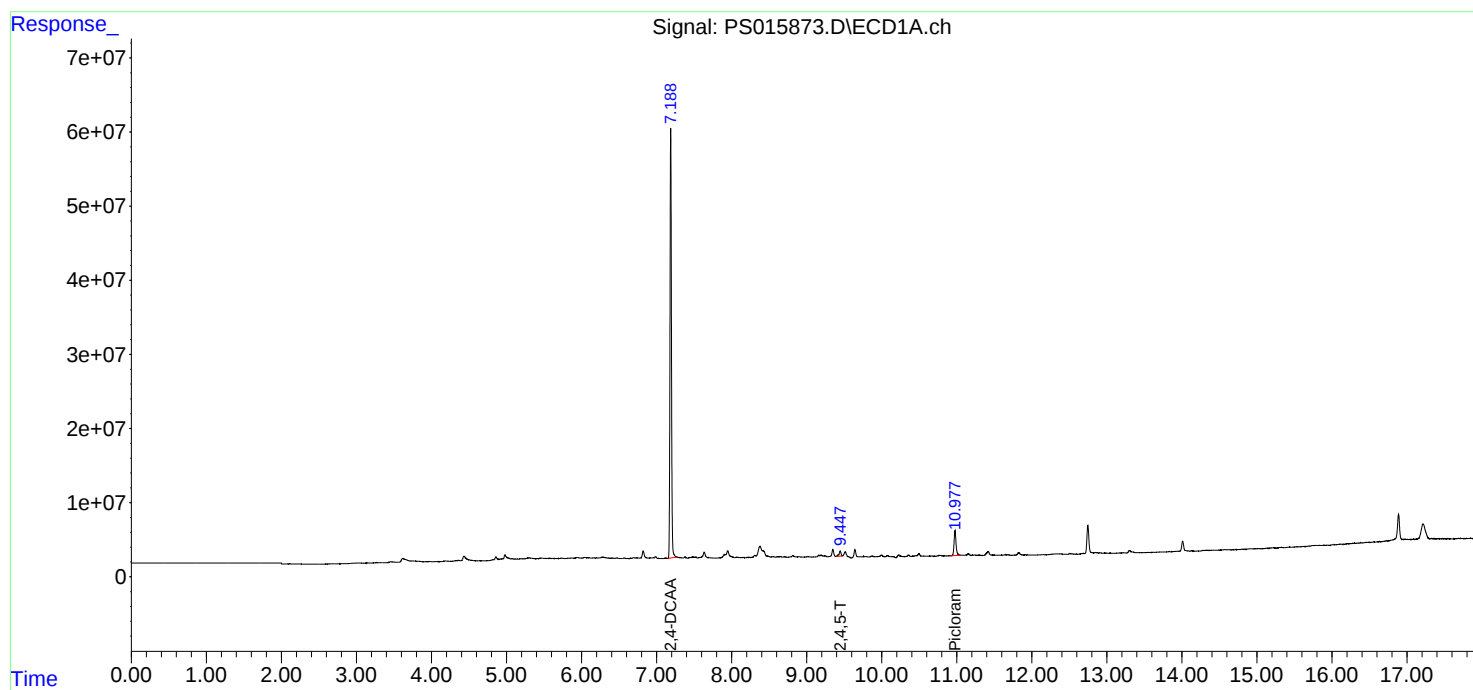


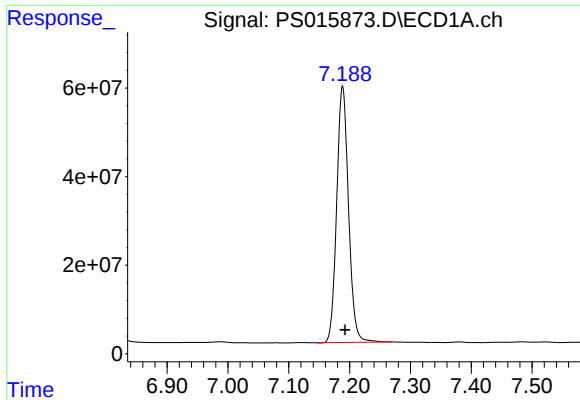

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 781557360
Conc: 470.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

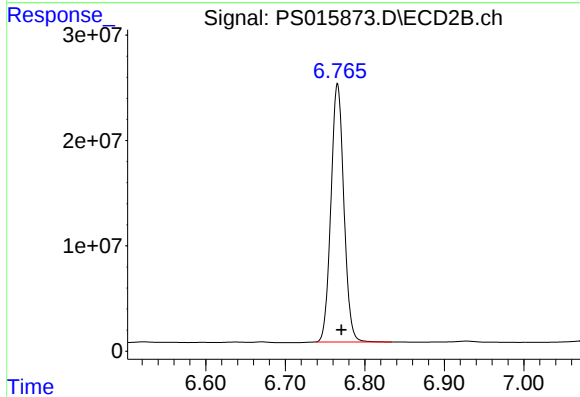


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: -0.005 min
Response: 276433790
Conc: 548.64 ng/ml

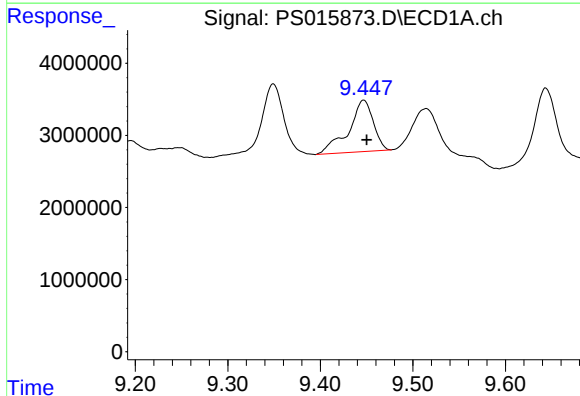


#12 2,4,5-T

R.T.: 9.447 min
Delta R.T.: -0.003 min
Response: 13263228
Conc: 1.50 ng/ml

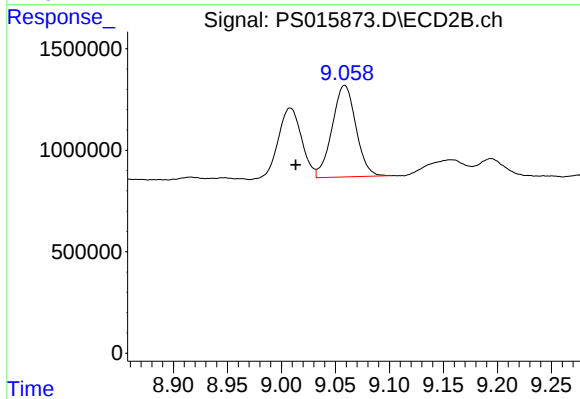

#12 2,4,5-T


R.T.: 9.059 min
Delta R.T.: 0.045 min
Response: 6944474
Conc: 2.46 ng/ml

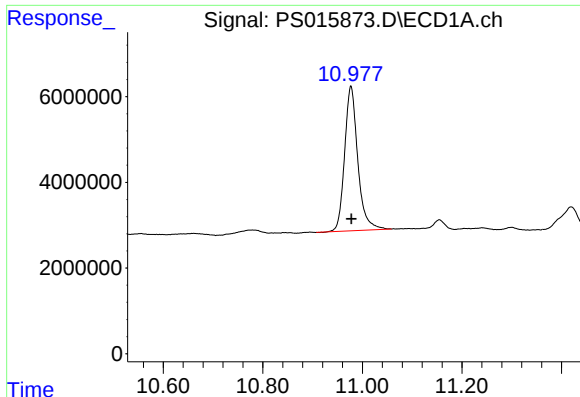

#15 Picloram


R.T.: 10.977 min
Delta R.T.: 0.000 min
Response: 61839484
Conc: 4.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

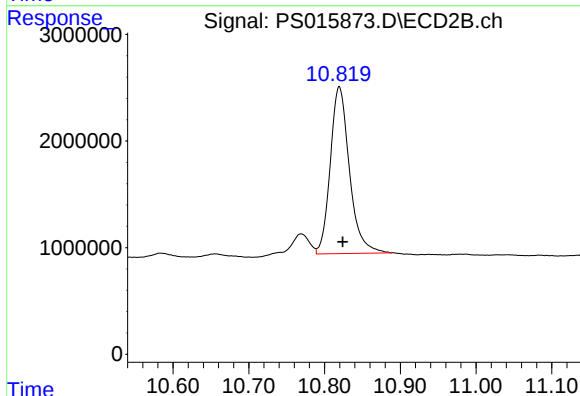


#15 Picloram

R.T.: 10.819 min
Delta R.T.: -0.004 min
Response: 27506739
Conc: 6.54 ng/ml

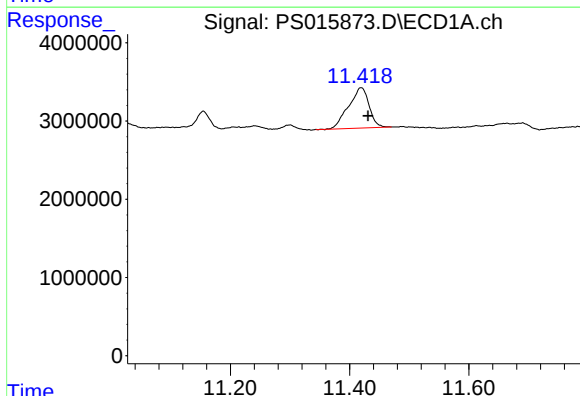

#16 DCPA

R.T.: 11.419 min
Delta R.T.: -0.012 min
Response: 12326732
Conc: N.D.

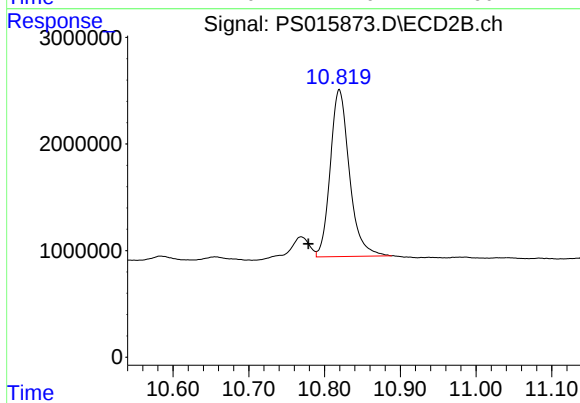

#16 DCPA

R.T.: 10.819 min
Delta R.T.: 0.041 min
Response: 27506739
Conc: 6.54 ng/ml