

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
 Data File : PS015885.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2021 13:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 01:59:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.767	777.3E6	277.7E6	467.864	551.174
Target Compounds							
12) T	2,4,5-T	0.000	9.061f	0	9548597	N.D.	3.385
15) T	Picloram	10.981	10.821	117.6E6	47310402	8.603	11.249 #
16) T	DCPA	0.000	10.821f	0	47310402	N.D.	11.253



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
Data File : PS015885.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2021 13:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 01:59:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

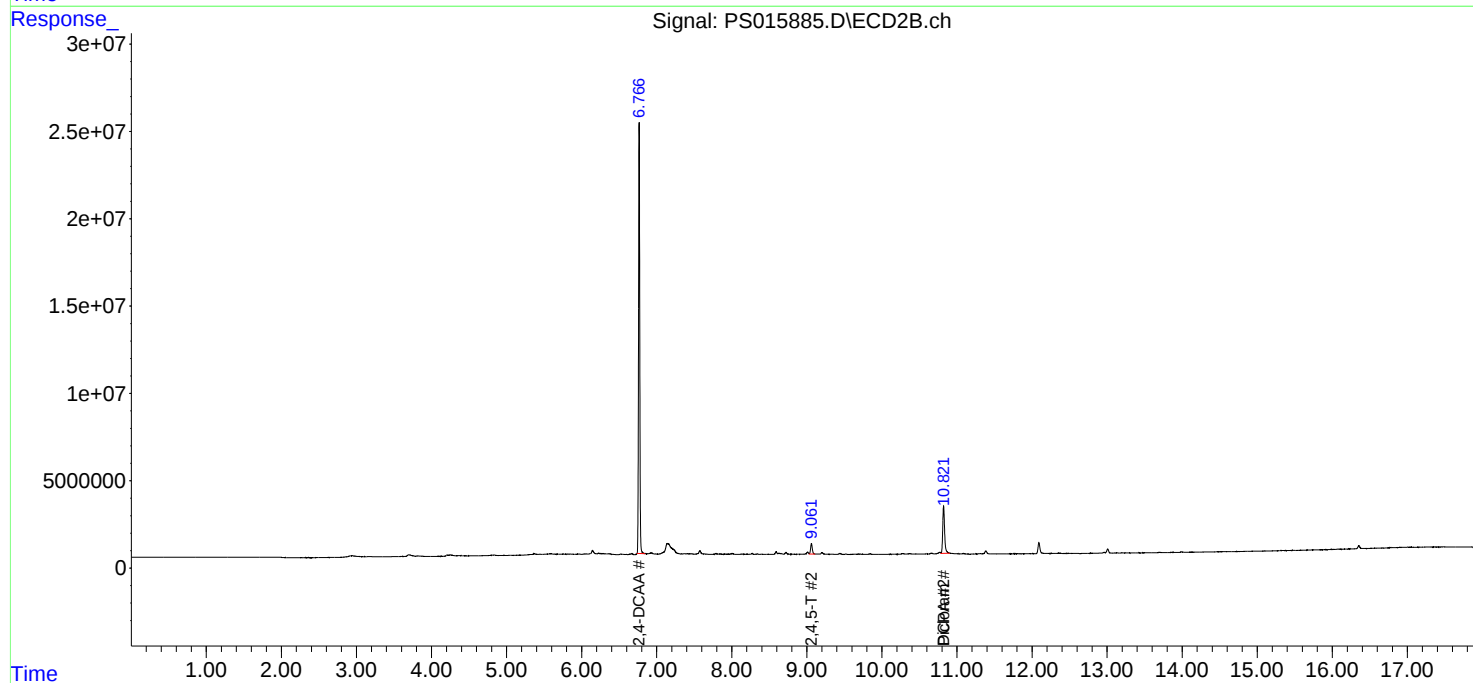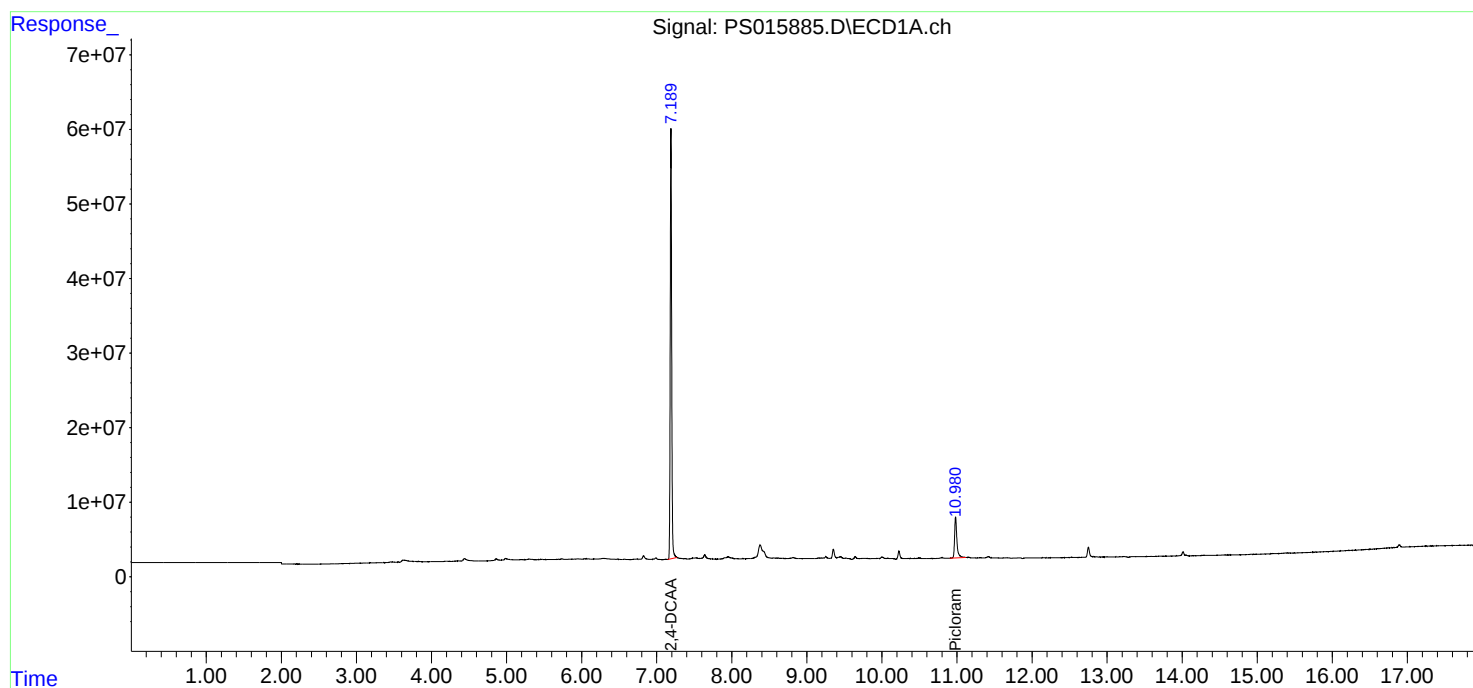


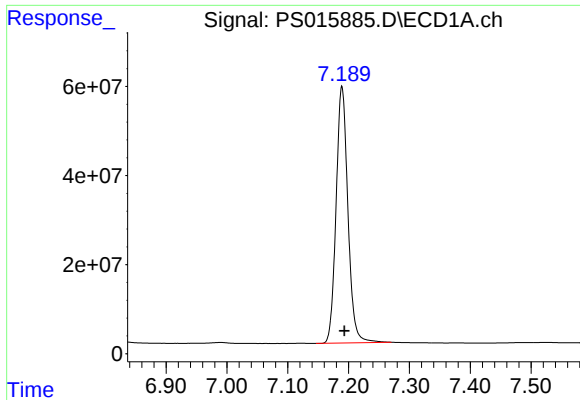

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 777331208
Conc: 467.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

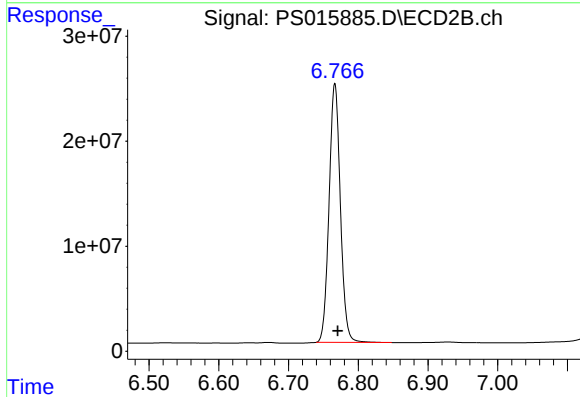


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.004 min
Response: 277710120
Conc: 551.17 ng/ml

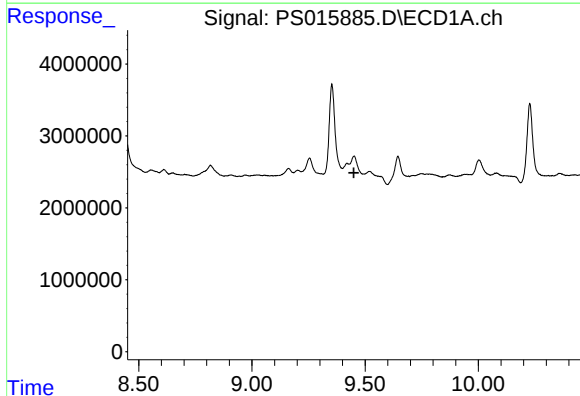


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.450 min
Response: 0
Conc: N.D.

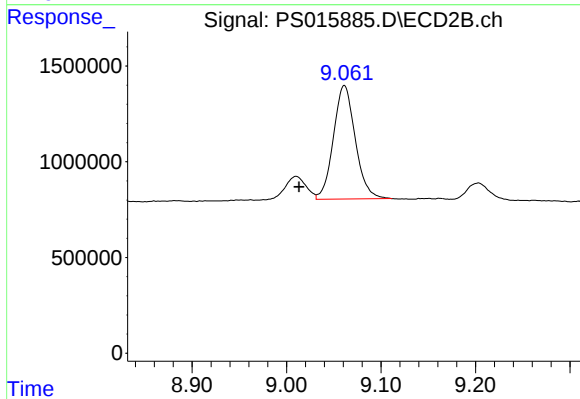

#12 2,4,5-T


R.T.: 9.061 min
Delta R.T.: 0.048 min
Response: 9548597
Conc: 3.39 ng/ml

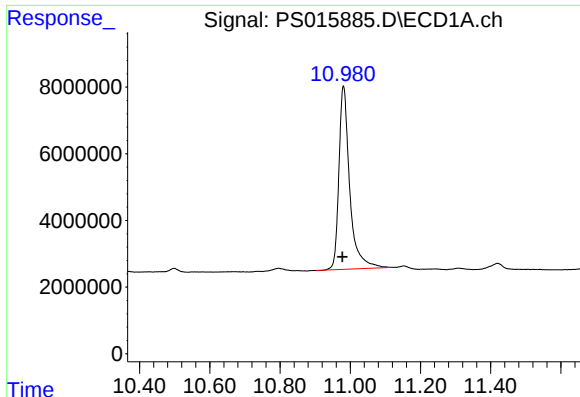

#15 Picloram


R.T.: 10.981 min
Delta R.T.: 0.003 min
Response: 117608675
Conc: 8.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

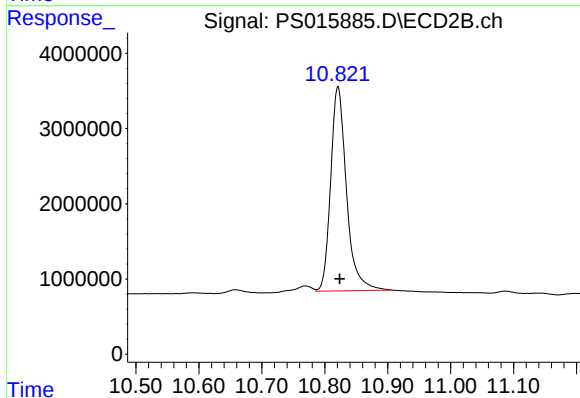


#15 Picloram

R.T.: 10.821 min
Delta R.T.: -0.003 min
Response: 47310402
Conc: 11.25 ng/ml

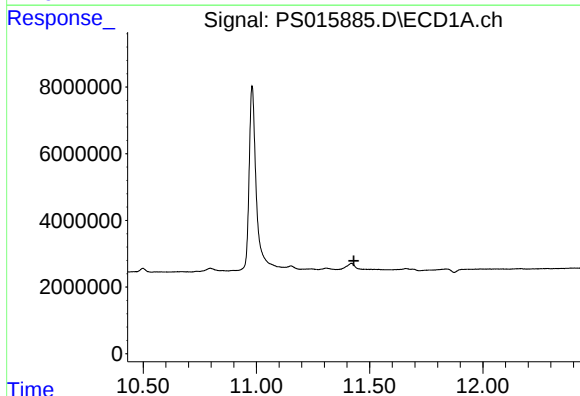

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.431 min
Response: 0
Conc: N.D.

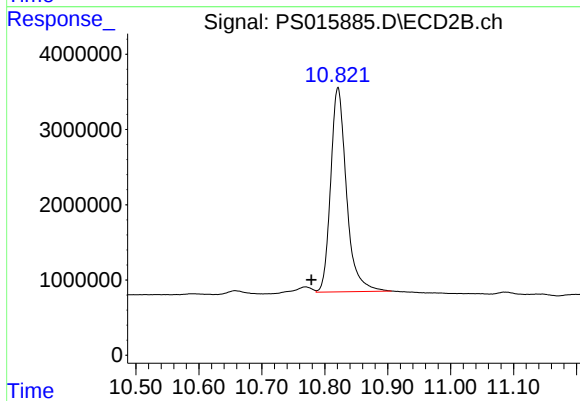

#16 DCPA

R.T.: 10.821 min
Delta R.T.: 0.042 min
Response: 47310402
Conc: 11.25 ng/ml