

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061923\
 Data File : PS023313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 10:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 13:31:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.481	6.853	916.2E6	285.3E6	517.832	502.559
Target Compounds							
3) T	4-Nitroph...	6.317	0.000	5780197	0	4.485	N.D. #
6) T	MCP	6.820	0.000	185030	0	<MDL	N.D. #
7) T	MCPA	6.856f	7.300	-703547	13467181	N.D.	5.011
8) T	DICHLORPROP	7.288f	0.000	673093	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.211	0.000	4380552	0	<MDL	N.D. #
12) T	2,4,5-T	8.479	0.000	1749603	0	<MDL	N.D. #
13) T	2,4-DB	8.935f	0.000	8046941	0	3.418	N.D. #
14) T	DINOSEB	10.061	0.000	682932	0	<MDL	N.D. #
15) T	Picloram	9.895	10.895	16333514	2963263	<MDL	<MDL #
16) T	DCPA	10.332	10.895	1782829	2963263	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061923\
Data File : PS023313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 10:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 13:31:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

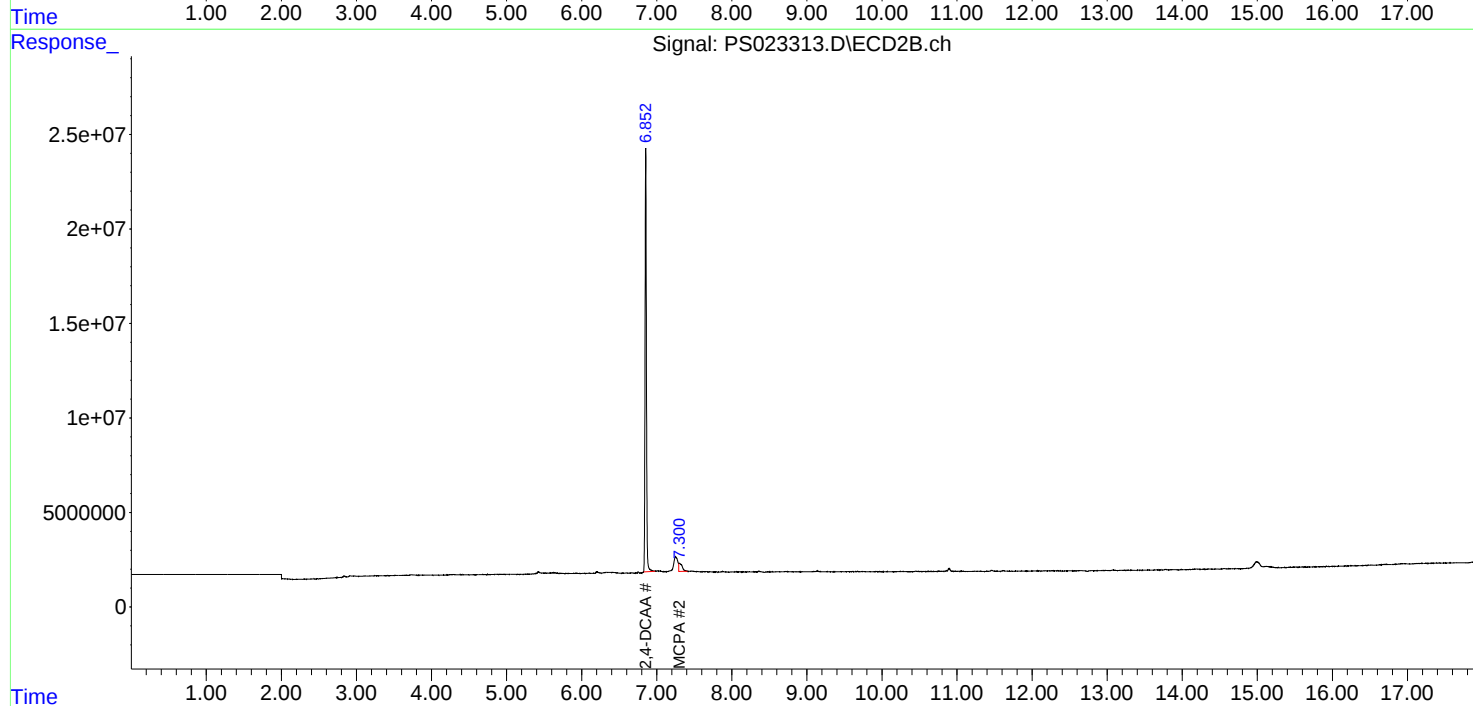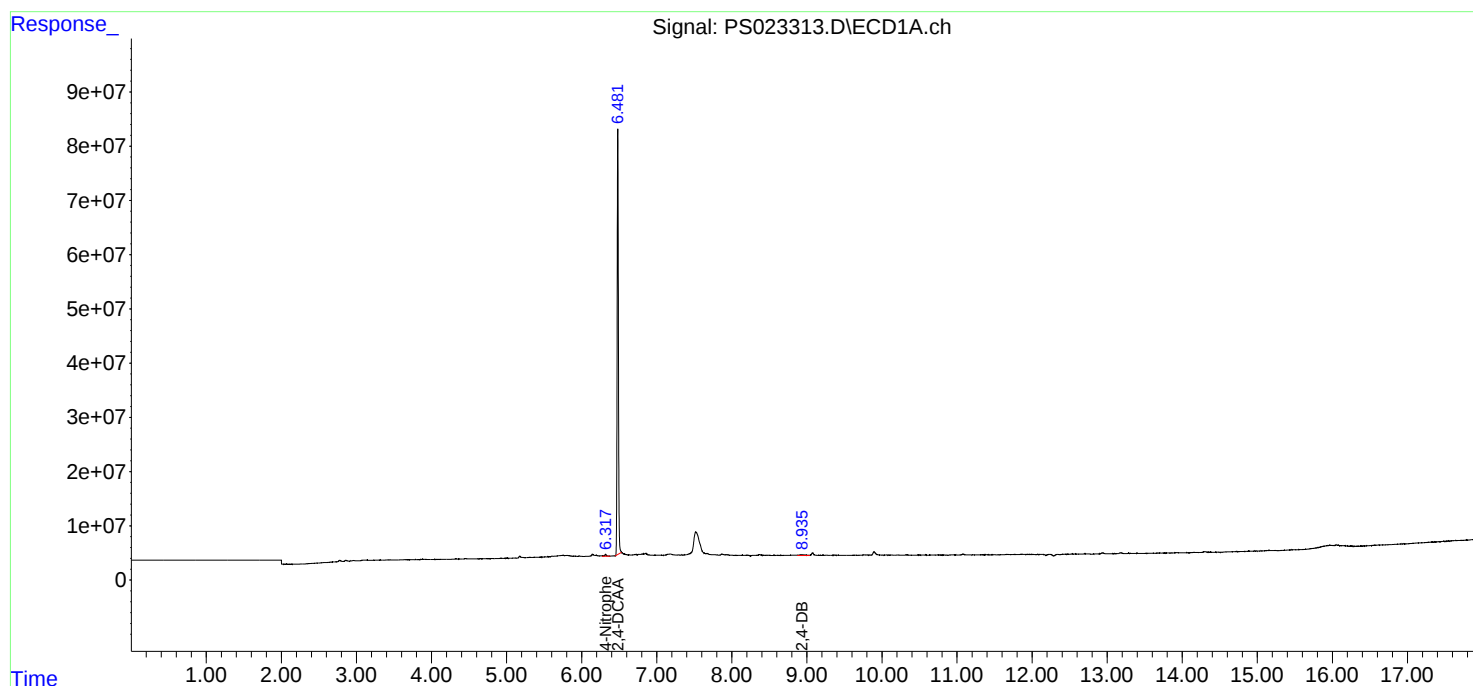


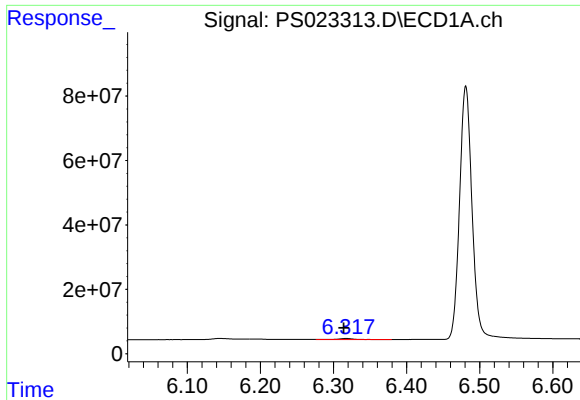

#3 4-Nitrophenol


R.T.: 6.317 min
Delta R.T.: 0.004 min
Response: 5780197
Conc: 4.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

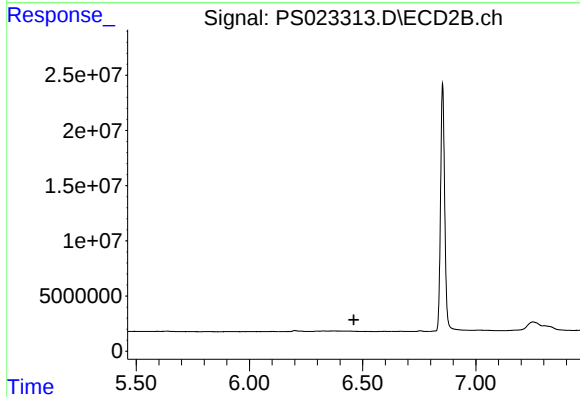


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

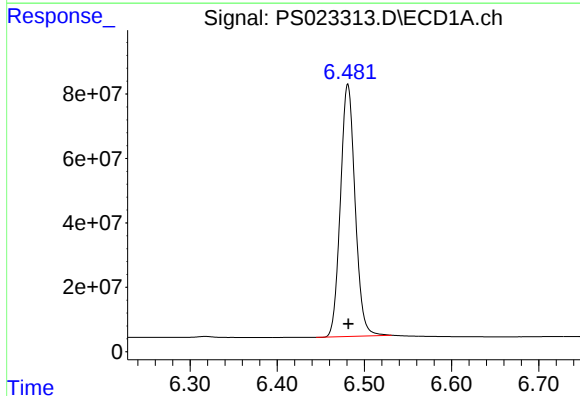


#4 2,4-DCAA

R.T.: 6.481 min
Delta R.T.: 0.000 min
Response: 916176735
Conc: 517.83 ng/ml

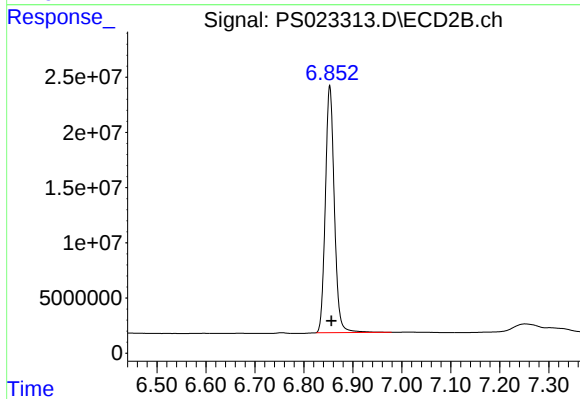

#4 2,4-DCAA


R.T.: 6.853 min
Delta R.T.: -0.003 min
Response: 285300244
Conc: 502.56 ng/ml

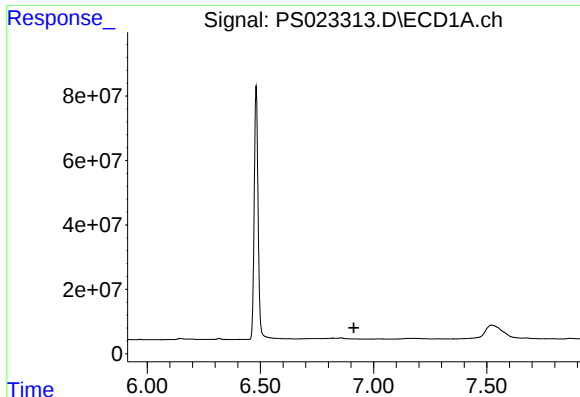

#7 MCPA


R.T.: 6.856 min
Delta R.T.: -0.057 min
Response: -703547
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

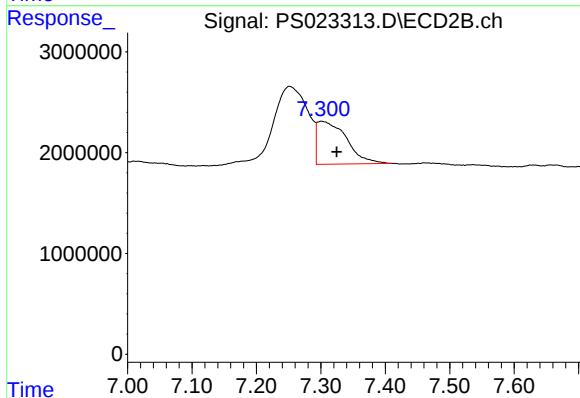


#7 MCPA

R.T.: 7.300 min
Delta R.T.: -0.025 min
Response: 13467181
Conc: 5.01 ug/ml

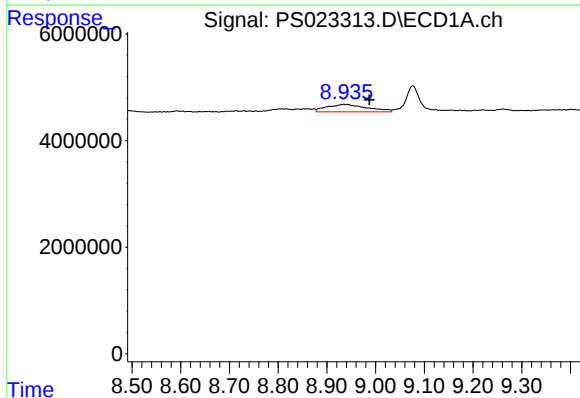

#13 2,4-DB

R.T.: 8.935 min
Delta R.T.: -0.052 min
Response: 8046941
Conc: 3.42 ng/ml

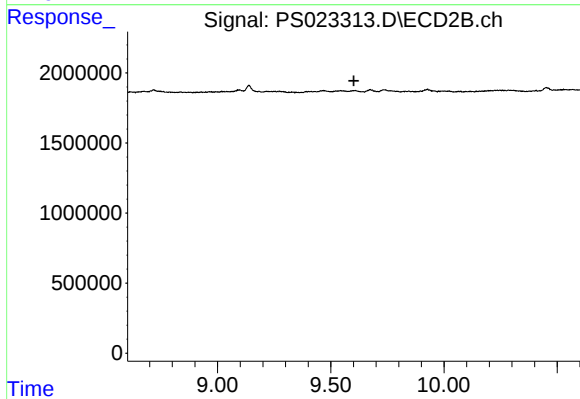

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.