

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061923\
 Data File : PS023325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 15:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:34:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.480	6.856	904.9E6	288.4E6	511.484	507.950
Target Compounds							
2) T	3,5-DICHL...	5.799	0.000	320163	0	<MDL	N.D. #
3) T	4-Nitroph...	6.317	0.000	5252387	0	4.075	N.D. #
5) T	DICAMBA	6.630	7.019	232567	673736	<MDL	<MDL #
6) T	MCP	6.818	0.000	1583513	0	<MDL	N.D. #
7) T	MCPA	6.924	7.260f	302602	78727521	<MDL	29.293 #
8) T	DICHLORPROP	7.287f	7.662	767228	991556	<MDL	1.603 #
11) T	2,4,5-TP ...	8.206	0.000	5364211	0	<MDL	N.D. #
12) T	2,4,5-T	8.473	0.000	3837435	0	<MDL	N.D. #
13) T	2,4-DB	8.931f	0.000	5618180	0	2.387	N.D. #
14) T	DINOSEB	10.053	0.000	666871	0	<MDL	N.D. #
15) T	Picloram	9.887	10.896	9996807	1827504	<MDL	<MDL #
16) T	DCPA	10.324	10.896	1942355	1827504	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061923\
Data File : PS023325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 15:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:34:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

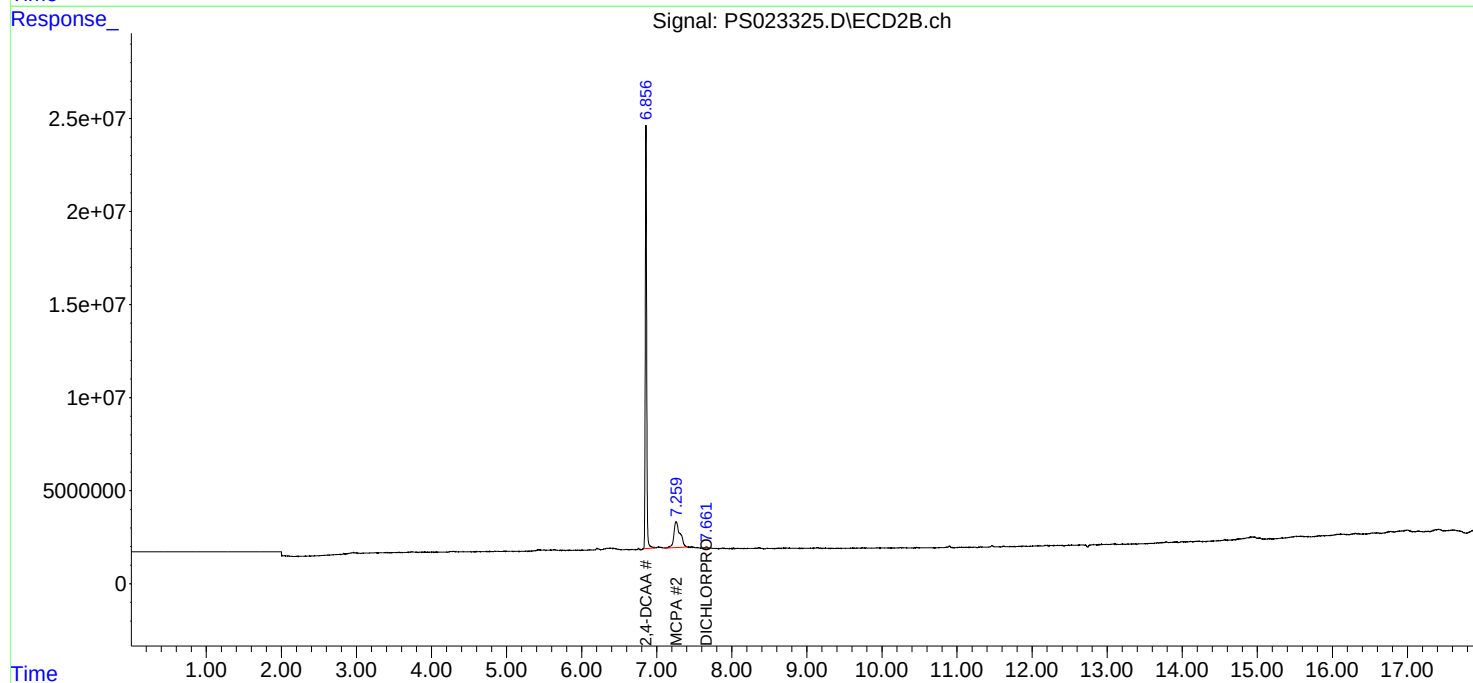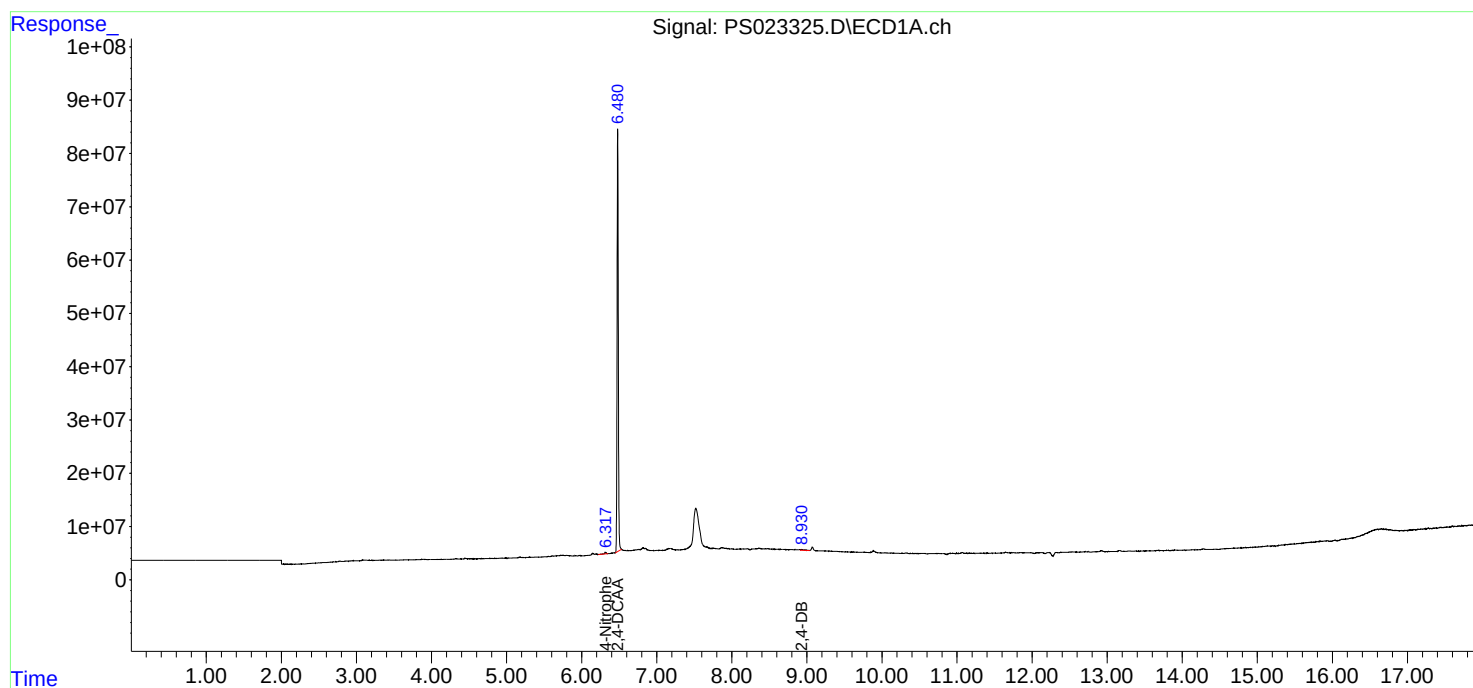


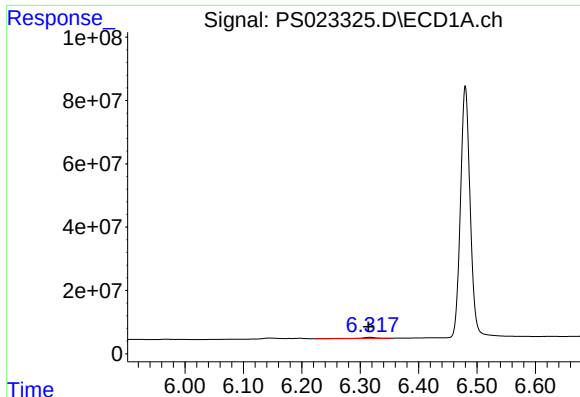

#3 4-Nitrophenol


R.T.: 6.317 min
Delta R.T.: 0.003 min
Response: 5252387
Conc: 4.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

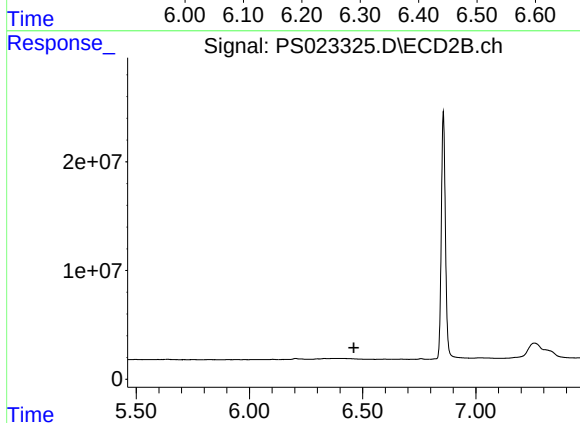


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

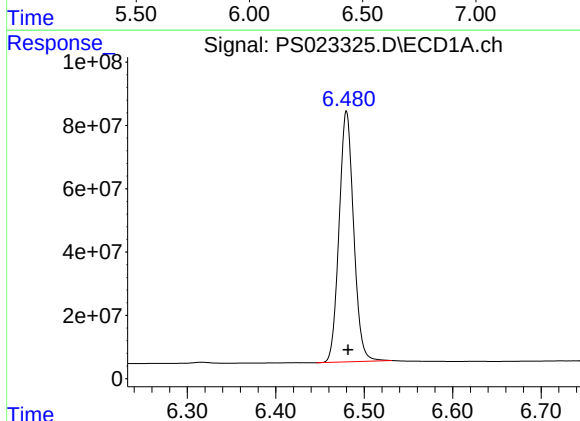


#4 2,4-DCAA

R.T.: 6.480 min
Delta R.T.: -0.002 min
Response: 904946345
Conc: 511.48 ng/ml

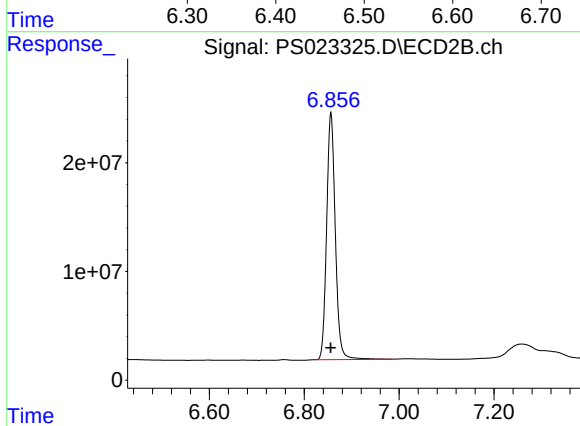

#4 2,4-DCAA


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 288360894
Conc: 507.95 ng/ml

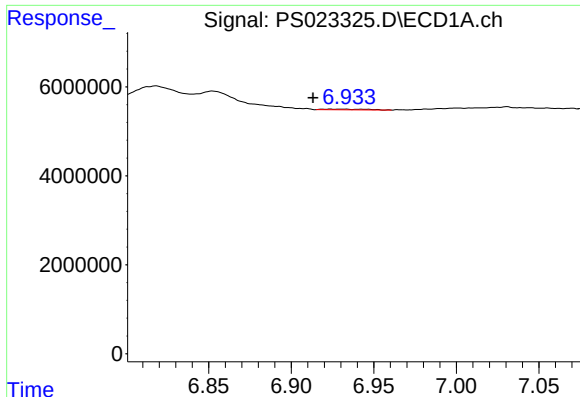

#7 MCPA


R.T.: 6.924 min
Delta R.T.: 0.011 min
Response: 302602
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

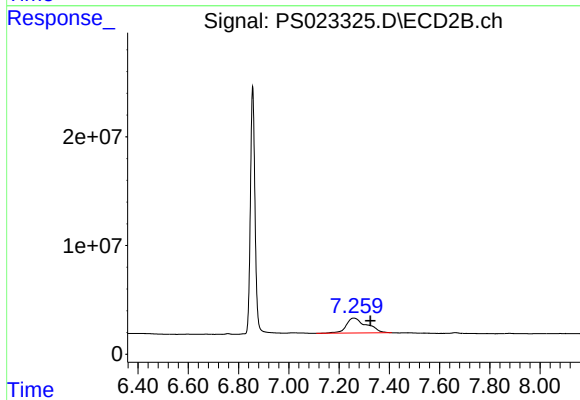


#7 MCPA

R.T.: 7.260 min
Delta R.T.: -0.065 min
Response: 78727521
Conc: 29.29 ug/ml

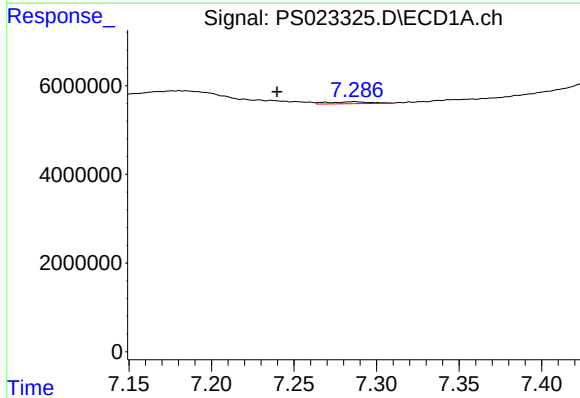


#8 DICHLORPROP

R.T.: 7.287 min
Delta R.T.: 0.047 min
Response: 767228
Conc: N.D.

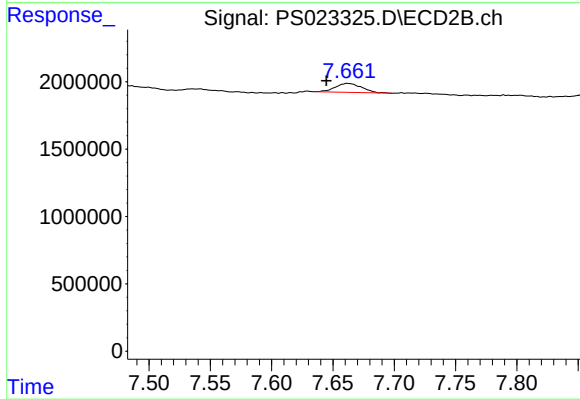

#8 DICHLORPROP


R.T.: 7.662 min
Delta R.T.: 0.017 min
Response: 991556
Conc: 1.60 ng/ml

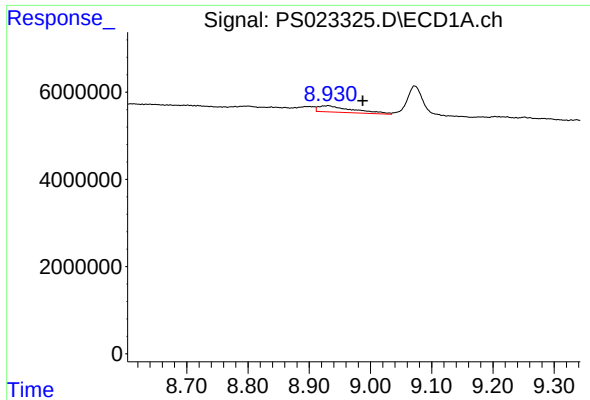

#13 2,4-DB

R.T.: 8.931 min
Delta R.T.: -0.056 min
Response: 5618180
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

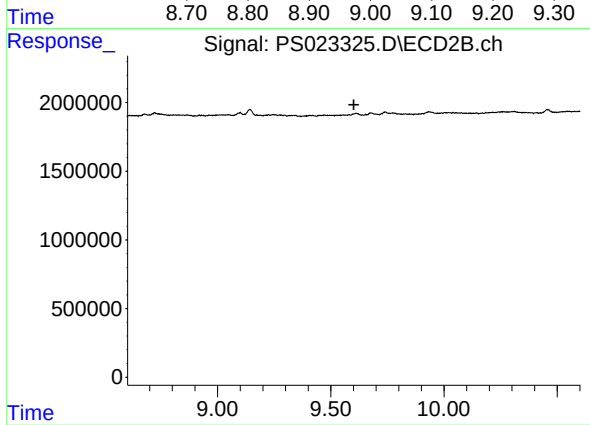

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.