

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062018\
 Data File : PS000481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 09:32
 Operator : UA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 14:37:47 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	3.220	2.598	561118	251151	1.097	0.576 #
6) T	MCP	12.527	0.000	66338	0	0.059	N.D. #
10) T	Pentachlo...	14.113	13.659	1015556	734707	0.193	0.155
11) T	2,4,5-TP ...	14.981	14.268	466761	416844	0.215	0.214
12) T	2,4,5-T	15.379	14.842	664604	529127	0.309	0.313
14) T	DINOSEB	17.642	15.925	665565	370369	0.447	0.284 #
15) T	Picloram	17.400	17.170	1963293	1092346	0.672	0.438 #
16) T	DCPA	17.981	17.112	1272424	1146377	0.497	0.497



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062018\
Data File : PS000481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 09:32
Operator : UA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 14:37:47 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

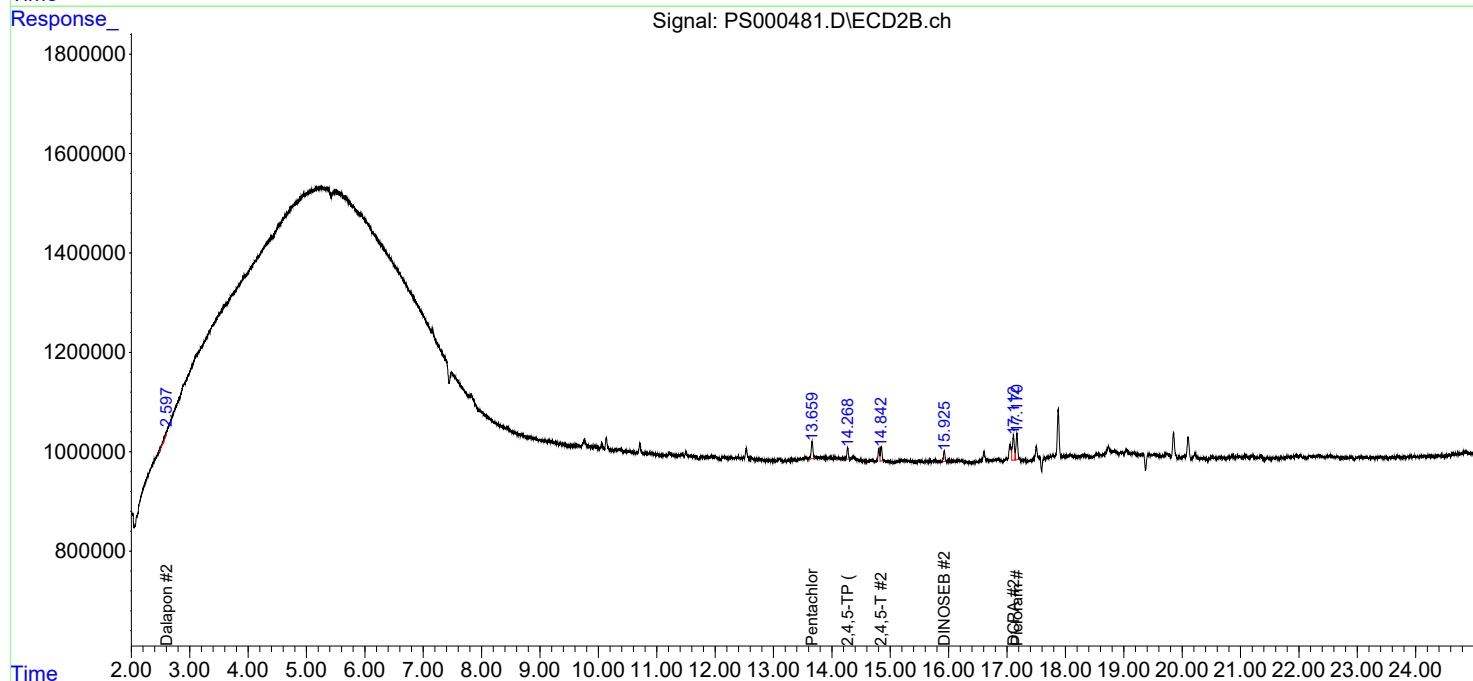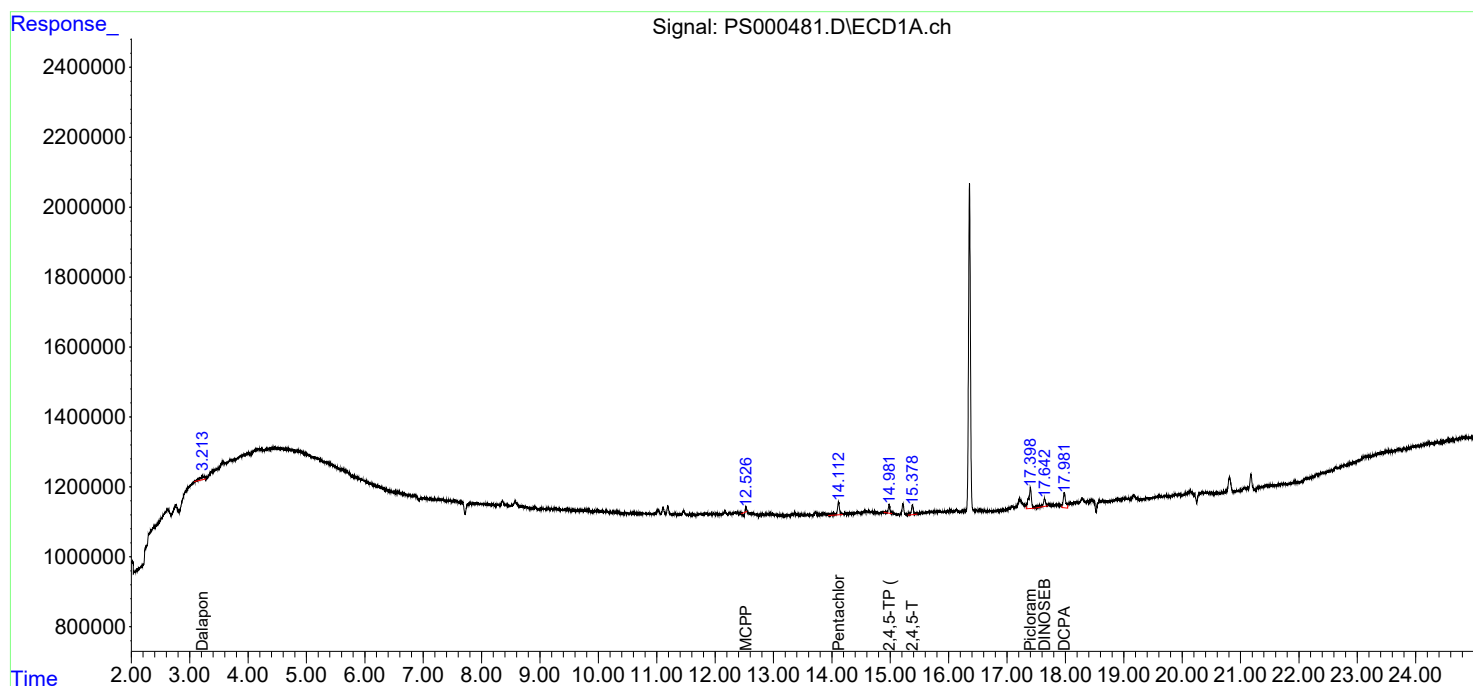


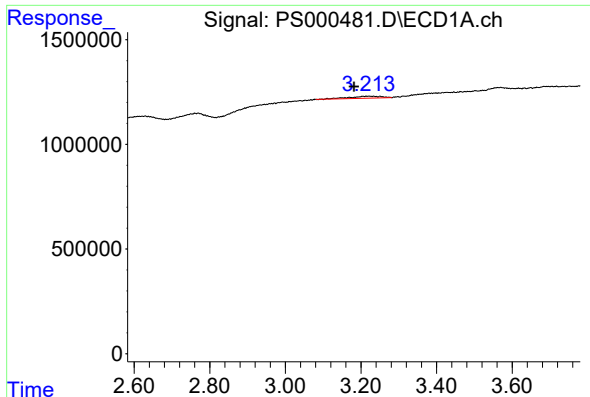

#1 Dalapon


R.T.: 3.220 min
Delta R.T.: 0.038 min
Response: 561118
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

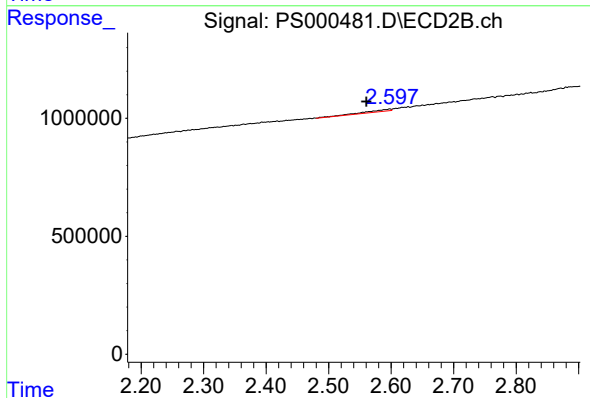


#1 Dalapon

R.T.: 2.598 min
Delta R.T.: 0.037 min
Response: 251151
Conc: 0.58 ng/ml

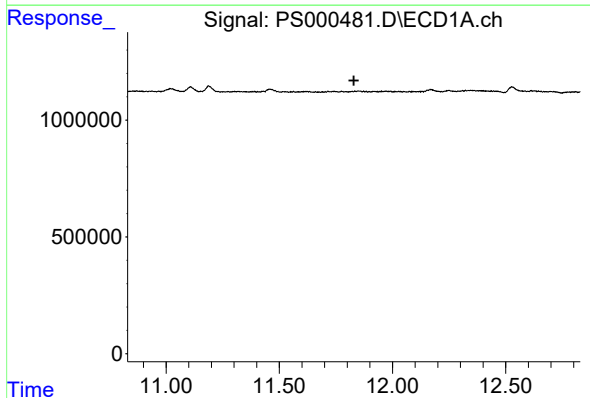


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.829 min
Response: 0
Conc: N.D.

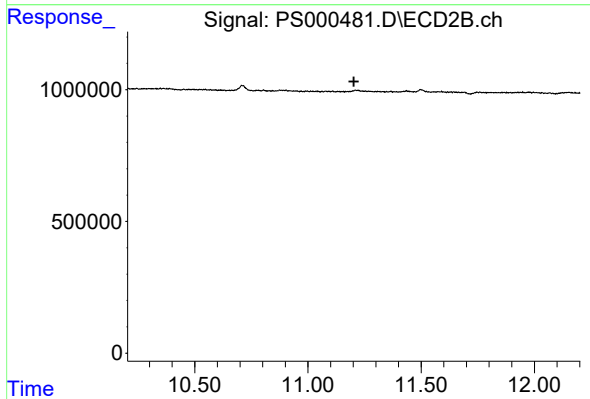

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.203 min
Response: 0
Conc: N.D.

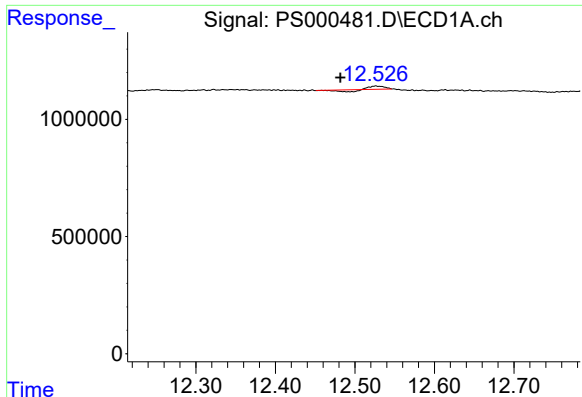

#6 MCP


R.T.: 12.527 min
Delta R.T.: 0.046 min
Response: 66338
Conc: 0.06 ug/ml

Instrument :
ECD_S
ClientSampleId :

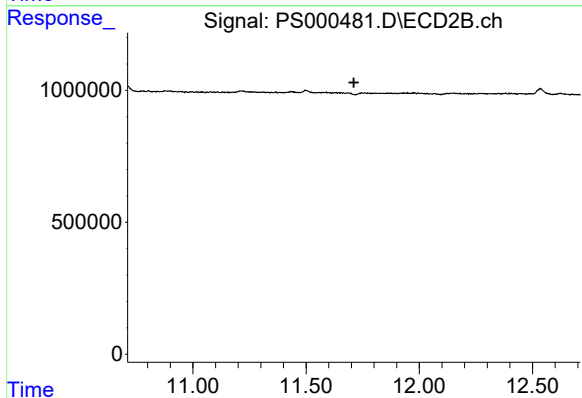


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

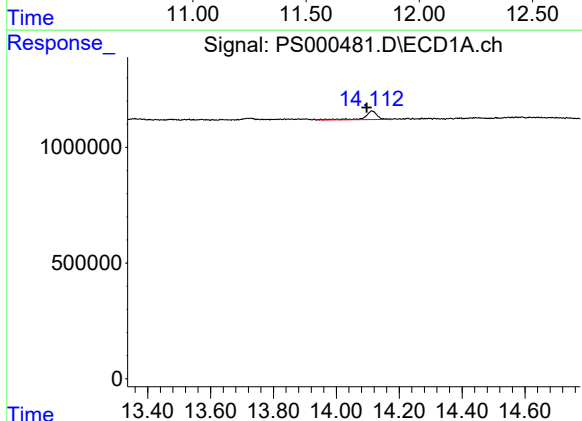


#10 Pentachlorophenol

R.T.: 14.113 min
Delta R.T.: 0.016 min
Response: 1015556
Conc: 0.19 ng/ml

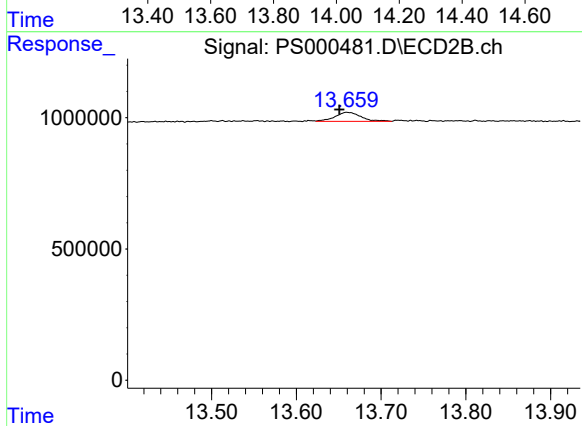

#10 Pentachlorophenol


R.T.: 13.659 min
Delta R.T.: 0.008 min
Response: 734707
Conc: 0.16 ng/ml

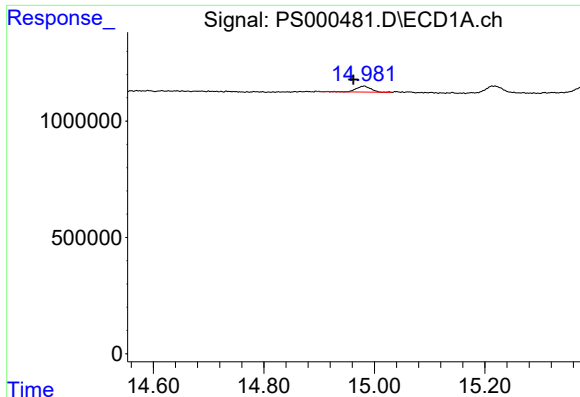

#11 2,4,5-TP (SILVEX)


R.T.: 14.981 min
Delta R.T.: 0.019 min
Response: 466761
Conc: 0.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

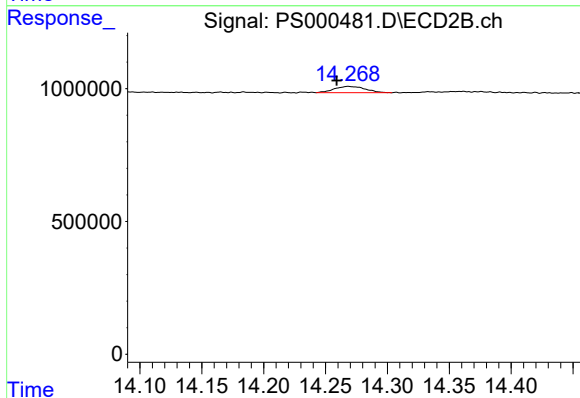


#11 2,4,5-TP (SILVEX)

R.T.: 14.268 min
Delta R.T.: 0.009 min
Response: 416844
Conc: 0.21 ng/ml

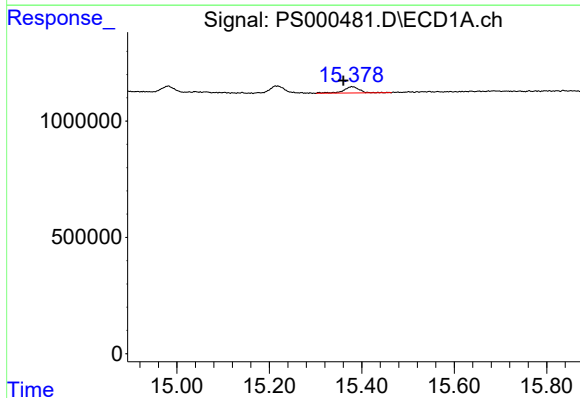


#12 2,4,5-T

R.T.: 15.379 min
Delta R.T.: 0.019 min
Response: 664604
Conc: 0.31 ng/ml

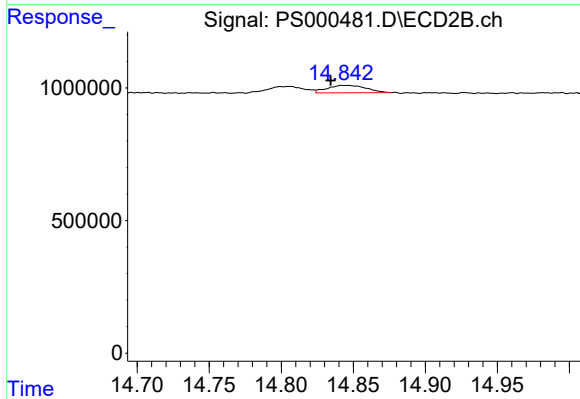

#12 2,4,5-T


R.T.: 14.842 min
Delta R.T.: 0.008 min
Response: 529127
Conc: 0.31 ng/ml

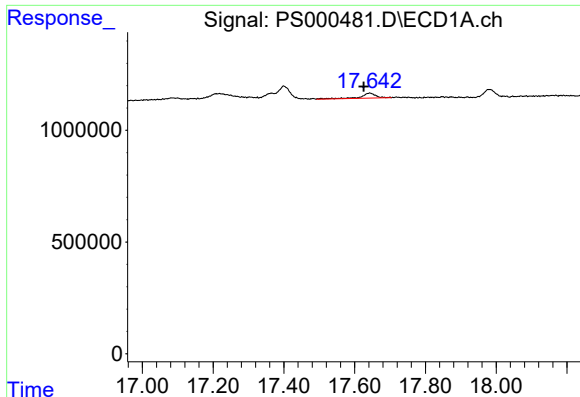

#14 DINOSEB


R.T.: 17.642 min
Delta R.T.: 0.017 min
Response: 665565
Conc: 0.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

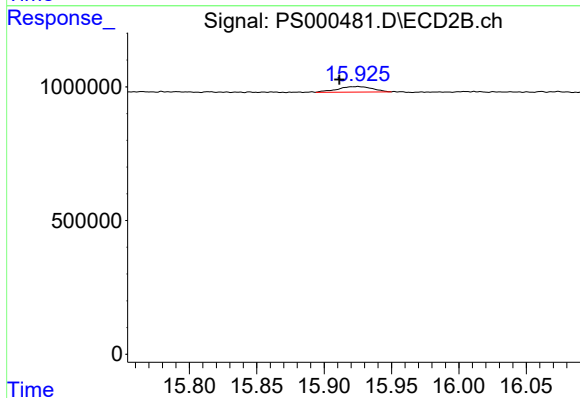


#14 DINOSEB

R.T.: 15.925 min
Delta R.T.: 0.014 min
Response: 370369
Conc: 0.28 ng/ml

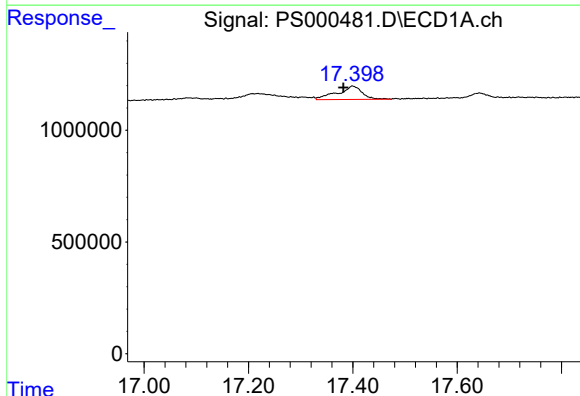


#15 Picloram

R.T.: 17.400 min
Delta R.T.: 0.018 min
Response: 1963293
Conc: 0.67 ng/ml

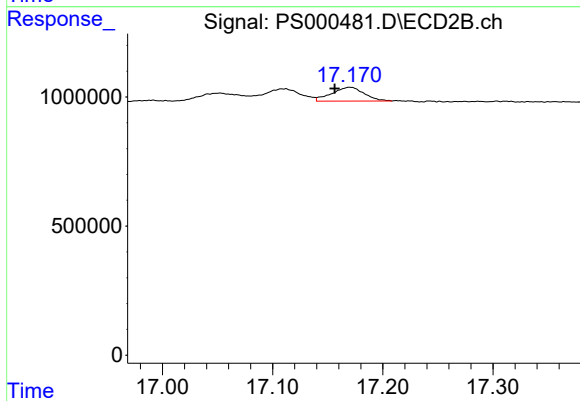

#15 Picloram


R.T.: 17.170 min
Delta R.T.: 0.014 min
Response: 1092346
Conc: 0.44 ng/ml

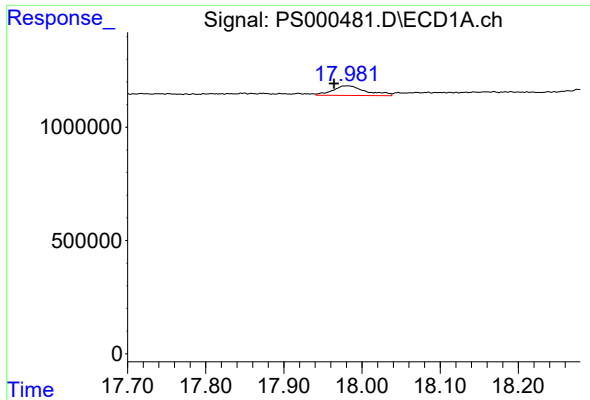

#16 DCPA

R.T.: 17.981 min
Delta R.T.: 0.016 min
Response: 1272424
Conc: 0.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

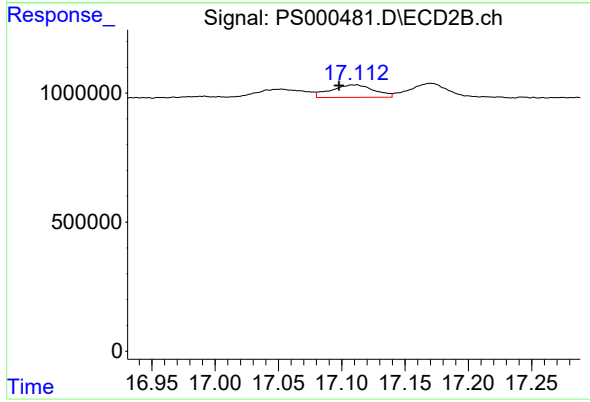

#16 DCPA

R.T.: 17.112 min
Delta R.T.: 0.014 min
Response: 1146377
Conc: 0.50 ng/ml