

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062018\
 Data File : PS000515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 05:49
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 07:54:22 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	11.851	11.229	205.2E6	76024216	544.699	223.398	#
Target Compounds								
3) T	4-Nitroph...	11.473	0.000	679862	0	2.892	N.D.	#
6) T	MCP	12.531	0.000	447567	0	0.395	N.D.	#
8) T	DICHLORPROP	0.000	12.554	0	605835	N.D.	1.882	#
10) T	Pentachlo...	0.000	13.676	0	36493	N.D.	0.008	#
15) T	Picloram	17.366	17.177	311950	-3298	0.107	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062018\
Data File : PS000515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 05:49
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 07:54:22 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

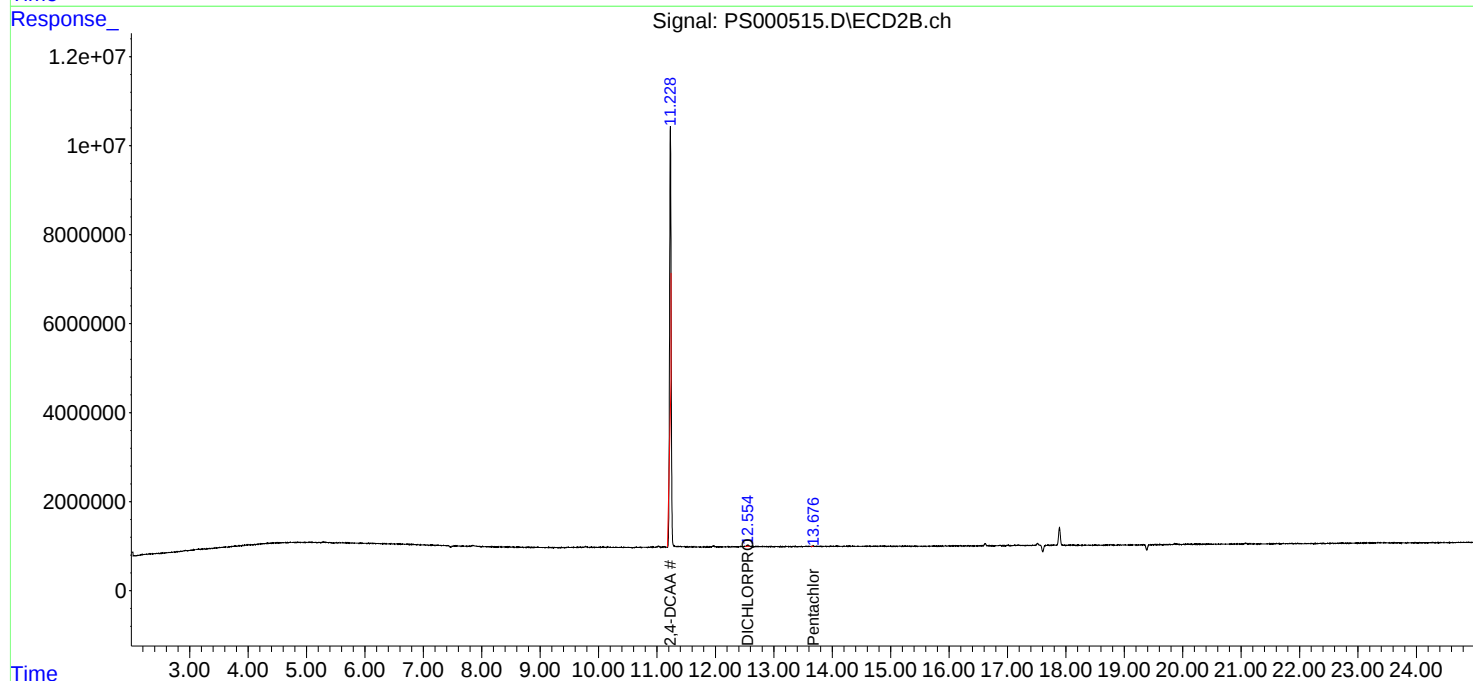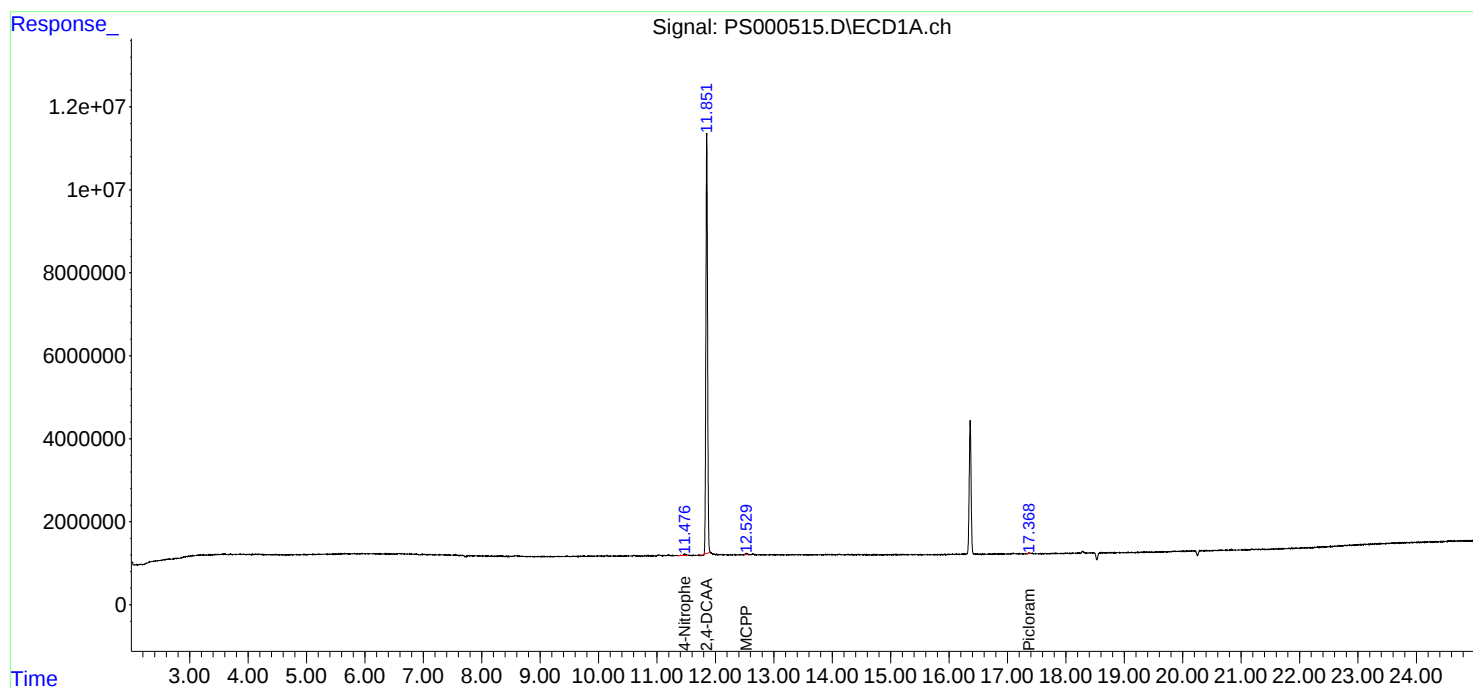


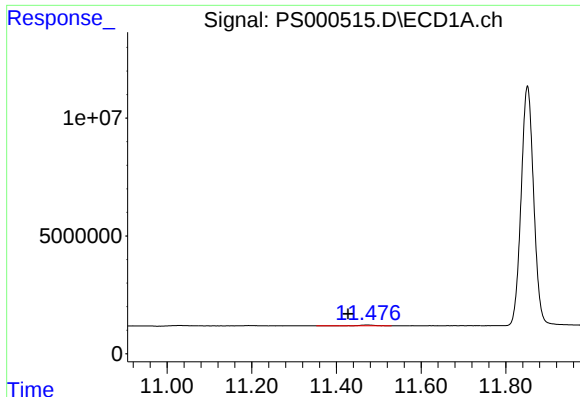

#3 4-Nitrophenol


R.T.: 11.473 min
Delta R.T.: 0.045 min
Response: 679862
Conc: 2.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

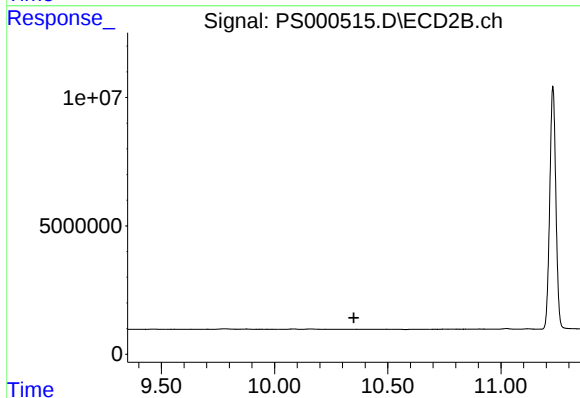


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.350 min
Response: 0
Conc: N.D.

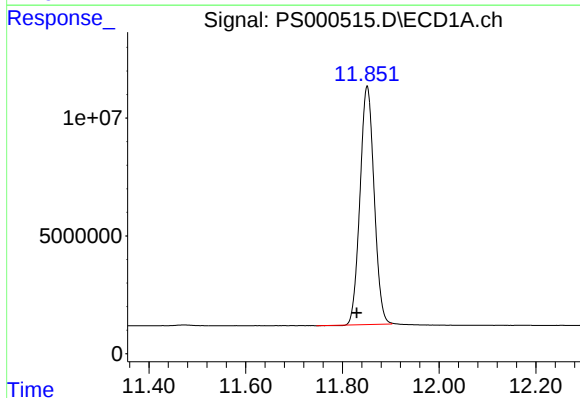


#4 2,4-DCAA

R.T.: 11.851 min
Delta R.T.: 0.022 min
Response: 205163433
Conc: 544.70 ng/ml

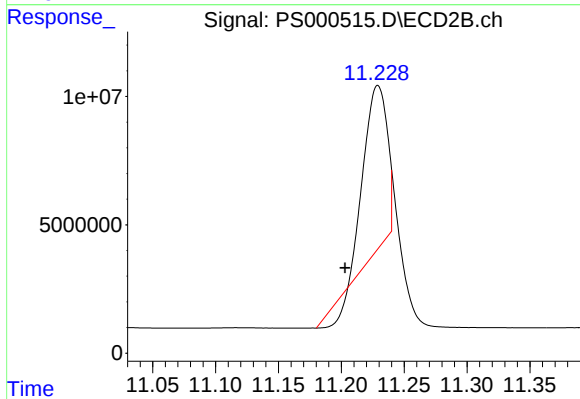

#4 2,4-DCAA


R.T.: 11.229 min
Delta R.T.: 0.026 min
Response: 76024216
Conc: 223.40 ng/ml

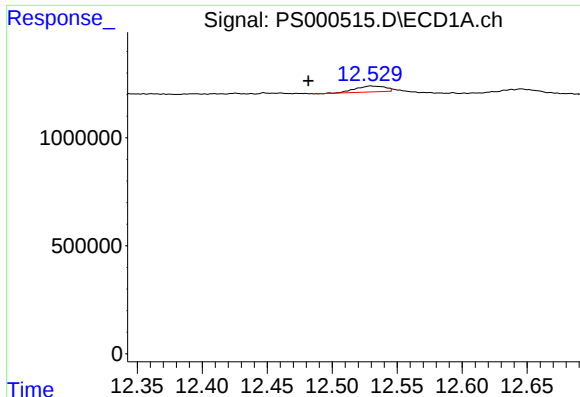

#6 MCP


R.T.: 12.531 min
Delta R.T.: 0.049 min
Response: 447567
Conc: 0.40 ug/ml

Instrument :
ECD_S
ClientSampleId :

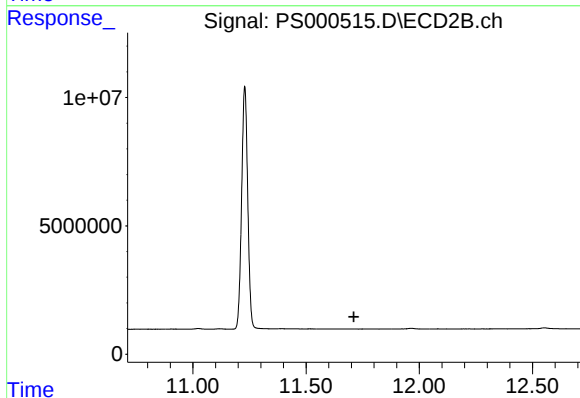


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

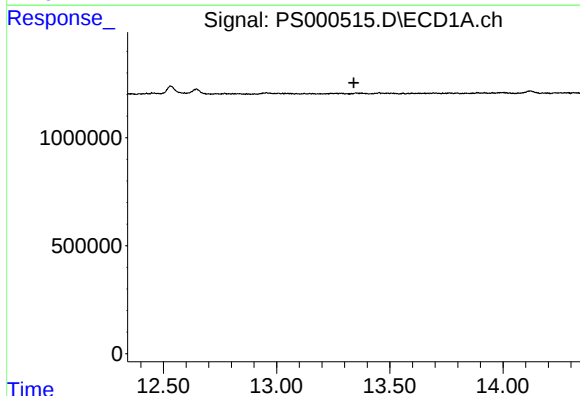


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.341 min
Response: 0
Conc: N.D.

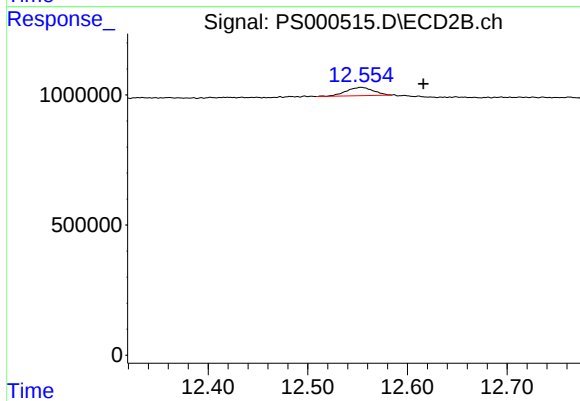

#8 DICHLORPROP


R.T.: 12.554 min
Delta R.T.: -0.062 min
Response: 605835
Conc: 1.88 ng/ml

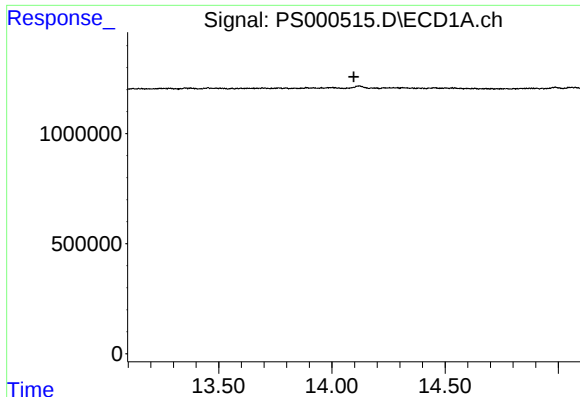

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 14.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

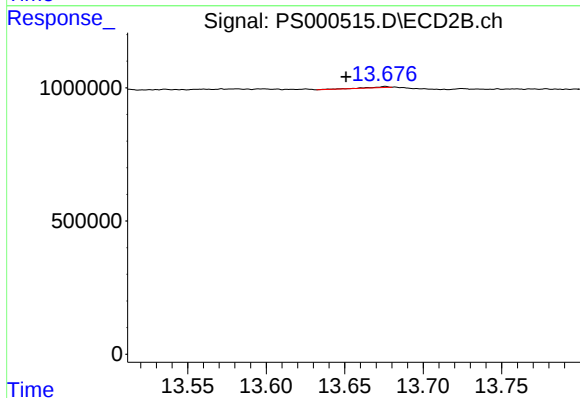


#10 Pentachlorophenol

R.T.: 13.676 min
Delta R.T.: 0.025 min
Response: 36493
Conc: 0.01 ng/ml

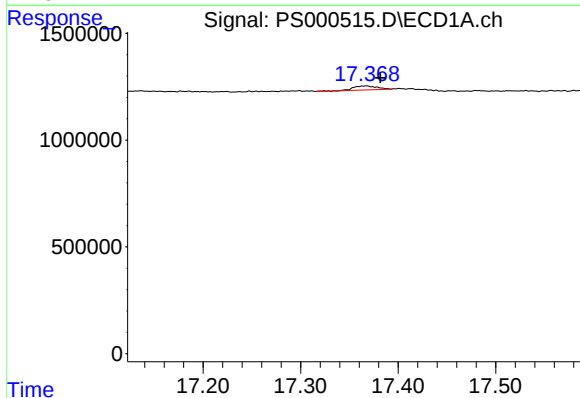

#15 Picloram

R.T.: 17.366 min
Delta R.T.: -0.015 min
Response: 311950
Conc: 0.11 ng/ml

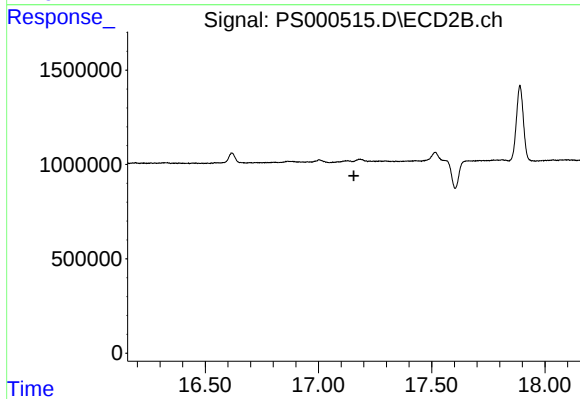

#15 Picloram

R.T.: 17.177 min
Delta R.T.: 0.020 min
Response: -3298
Conc: N.D.