

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062018\
 Data File : PS000492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 17:20
 Operator : UA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:49:25 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.820	11.195	273.3E6	252.7E6	725.494	742.564
Target Compounds							
1) T	Dalapon	3.174	2.554	335.5E6	292.5E6	655.921	670.989
2) T	3,5-DICHL...	10.234	9.340	371.3E6	321.7E6	687.991	699.309
3) T	4-Nitroph...	11.418	10.343	162.8E6	138.3E6	692.477	705.928
5) T	DICAMBA	12.139	11.485	989.6E6	891.4E6	700.150	719.482
6) T	MCPD	12.478	11.711	78357991	67206956	69.195	70.047
7) T	MCPA	12.730	12.089	120.5E6	100.9E6	68.534	72.889
8) T	DICHLORPROP	13.332	12.609	259.3E6	227.0E6	689.255	705.009
9) T	2,4-D	13.690	13.080	334.9E6	306.4E6	700.194	720.837
10) T	Pentachlo...	14.088	13.645	3696.8E6	3447.0E6	704.159	728.647
11) T	2,4,5-TP ...	14.954	14.253	1531.9E6	1413.0E6	705.675	726.080
12) T	2,4,5-T	15.352	14.827	1513.8E6	1143.9E6	703.007	676.409
13) T	2,4-DB	16.106	15.472	206.3E6	179.0E6	700.547	723.136
14) T	DINOSEB	17.617	15.904	1017.7E6	917.8E6	683.402	703.498
15) T	Picloram	17.375	17.150	2031.2E6	1800.6E6	695.500	721.861
16) T	DCPA	17.956	17.092	1833.9E6	1715.0E6	715.662	743.746



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062018\
Data File : PS000492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 17:20
Operator : UA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:49:25 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

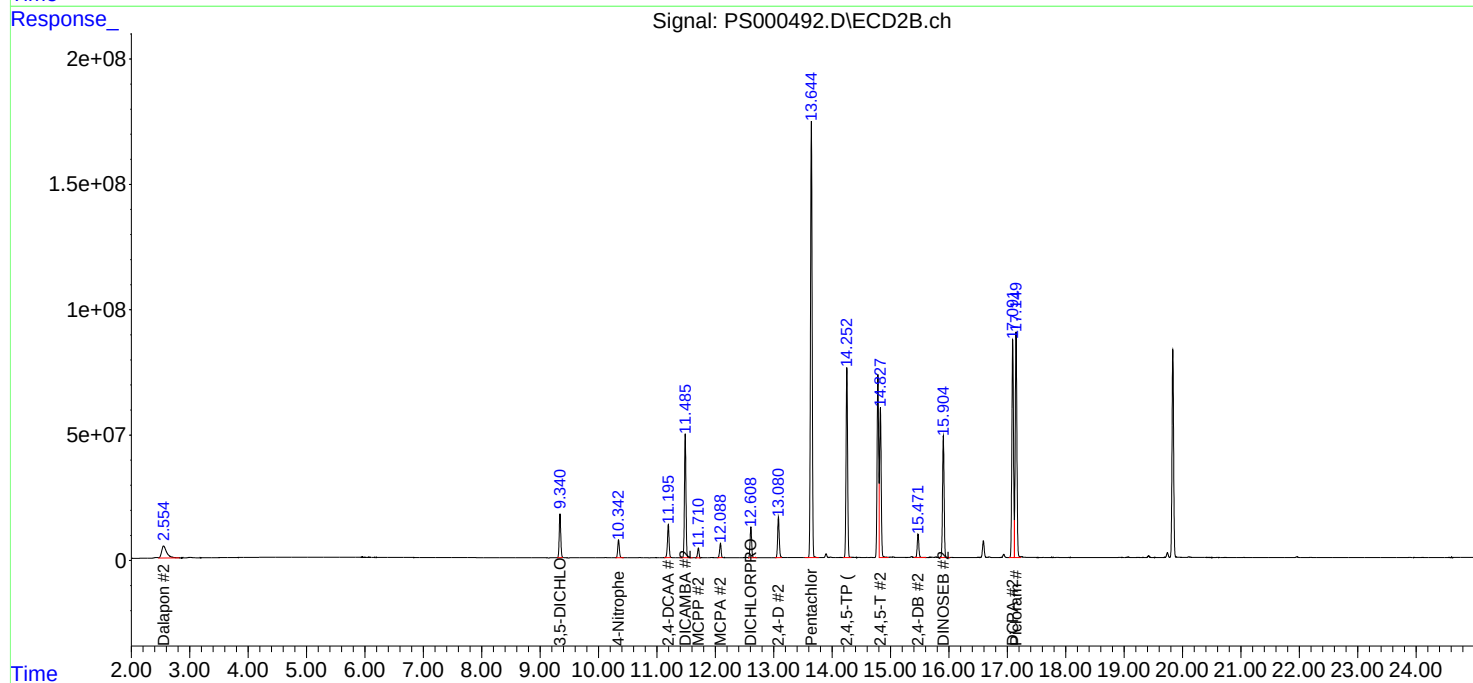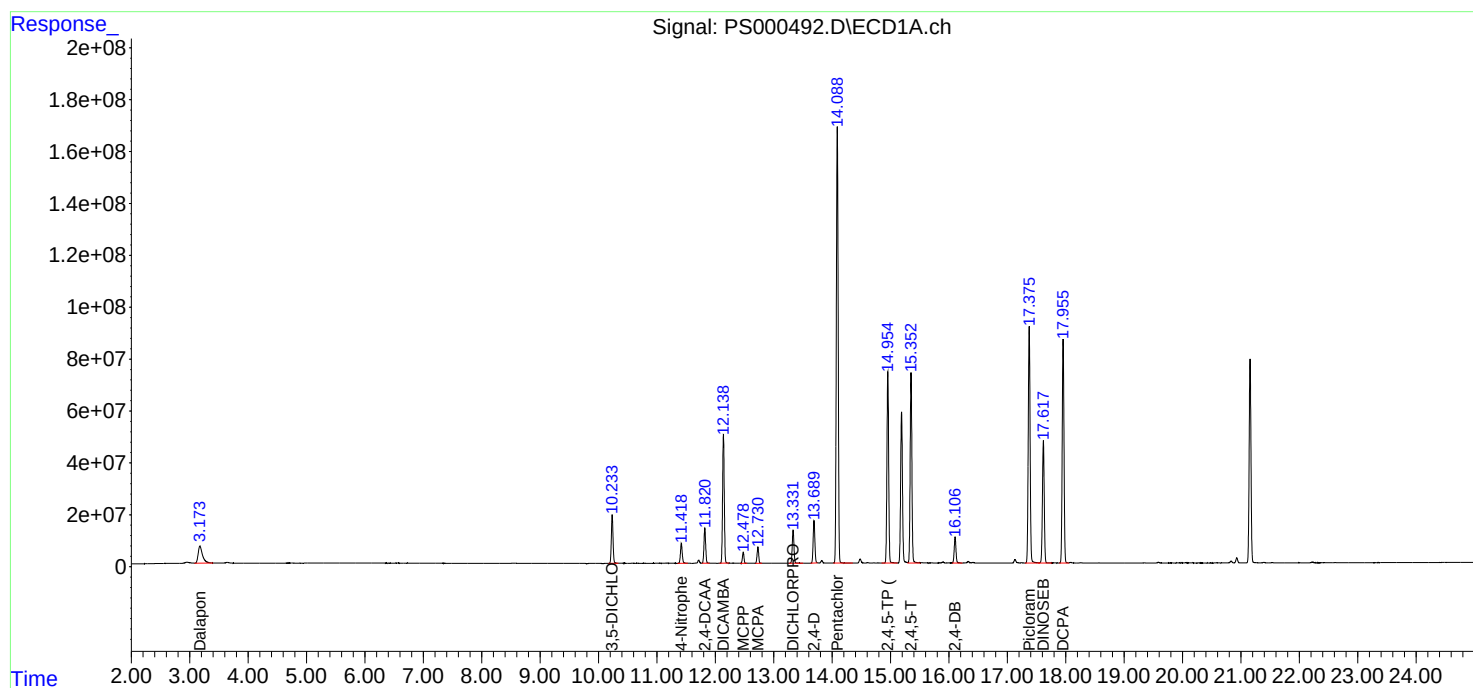


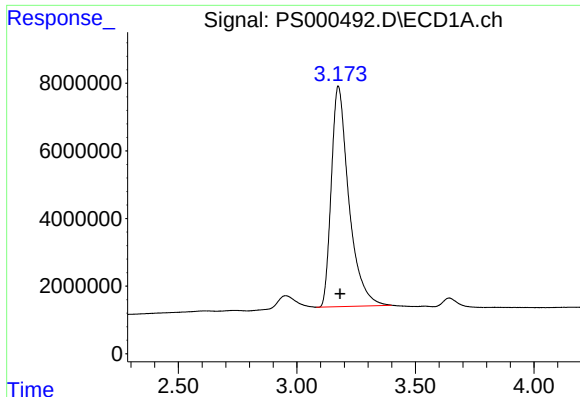

#1 Dalapon


R.T.: 3.174 min
Delta R.T.: -0.008 min
Response: 335477784
Conc: 655.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

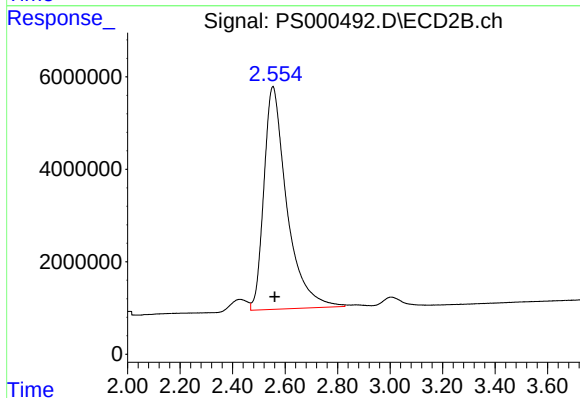


#1 Dalapon

R.T.: 2.554 min
Delta R.T.: -0.006 min
Response: 292506038
Conc: 670.99 ng/ml

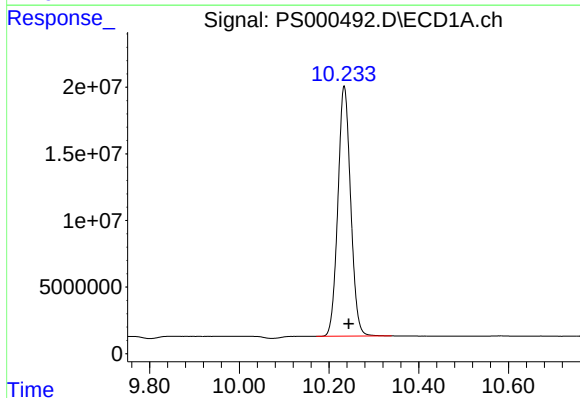


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.234 min
Delta R.T.: -0.010 min
Response: 371292333
Conc: 687.99 ng/ml

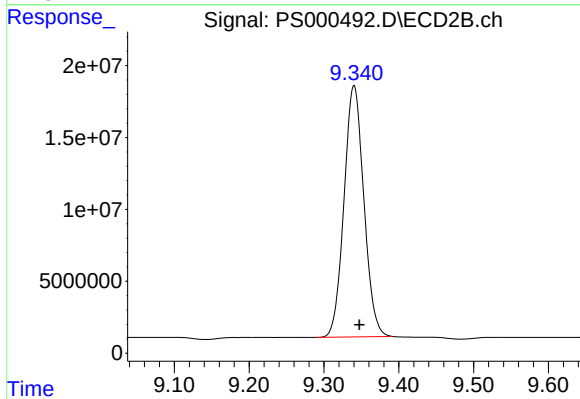

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.340 min
Delta R.T.: -0.007 min
Response: 321711155
Conc: 699.31 ng/ml

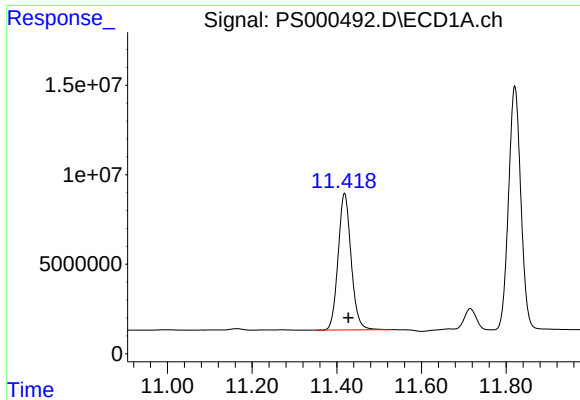

#3 4-Nitrophenol


R.T.: 11.418 min
Delta R.T.: -0.009 min
Response: 162780807
Conc: 692.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

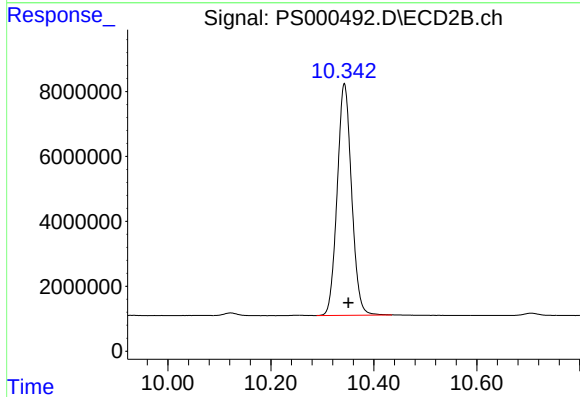


#3 4-Nitrophenol

R.T.: 10.343 min
Delta R.T.: -0.008 min
Response: 138334992
Conc: 705.93 ng/ml

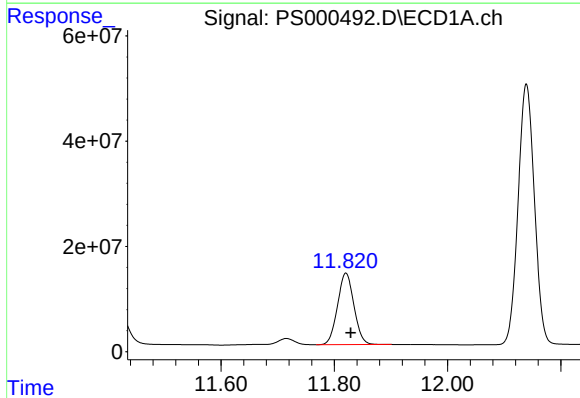


#4 2,4-DCAA

R.T.: 11.820 min
Delta R.T.: -0.009 min
Response: 273260798
Conc: 725.49 ng/ml

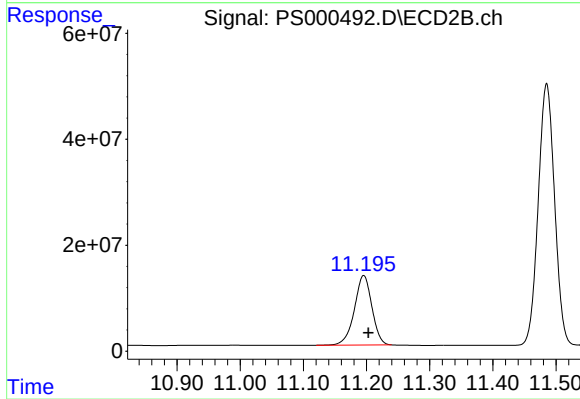

#4 2,4-DCAA


R.T.: 11.195 min
Delta R.T.: -0.007 min
Response: 252701149
Conc: 742.56 ng/ml

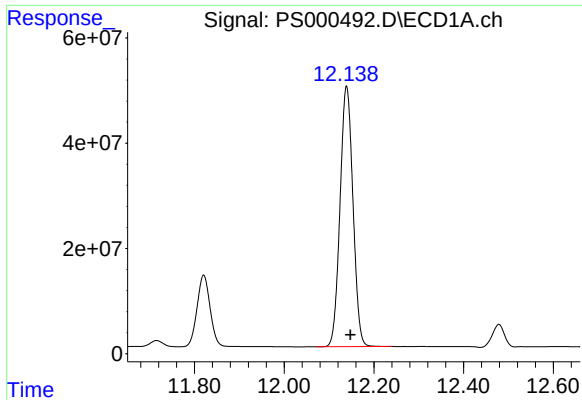

#5 DICAMBA


R.T.: 12.139 min
Delta R.T.: -0.008 min
Response: 989628370
Conc: 700.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

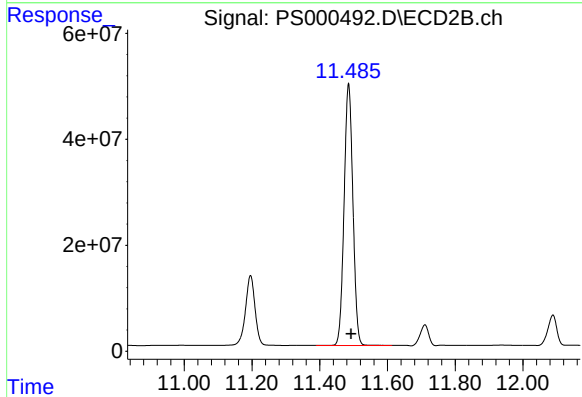


#5 DICAMBA

R.T.: 11.485 min
Delta R.T.: -0.008 min
Response: 891409066
Conc: 719.48 ng/ml

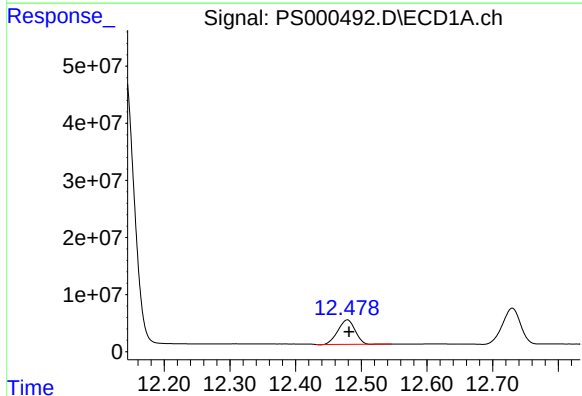


#6 MCP

R.T.: 12.478 min
Delta R.T.: -0.003 min
Response: 78357991
Conc: 69.20 ug/ml

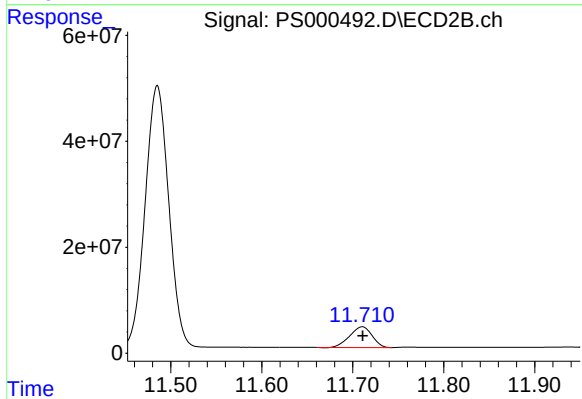

#6 MCP


R.T.: 11.711 min
Delta R.T.: 0.000 min
Response: 67206956
Conc: 70.05 ug/ml

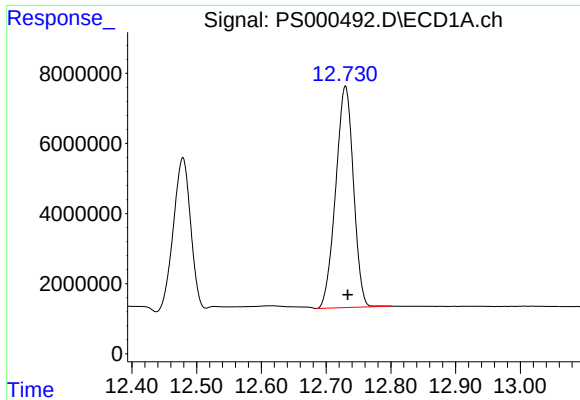

#7 MCPA


R.T.: 12.730 min
Delta R.T.: -0.004 min
Response: 120463130
Conc: 68.53 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

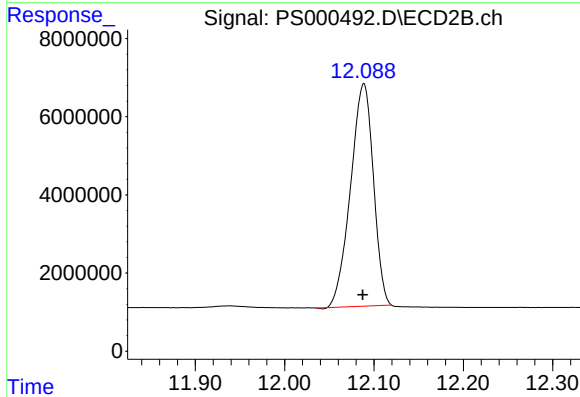


#7 MCPA

R.T.: 12.089 min
Delta R.T.: 0.001 min
Response: 100948510
Conc: 72.89 ug/ml

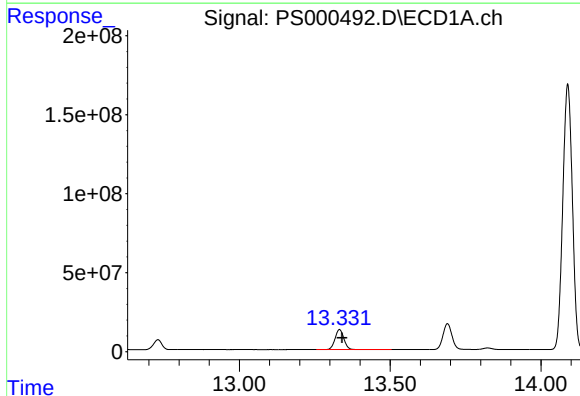


#8 DICHLORPROP

R.T.: 13.332 min
Delta R.T.: -0.009 min
Response: 259269260
Conc: 689.25 ng/ml

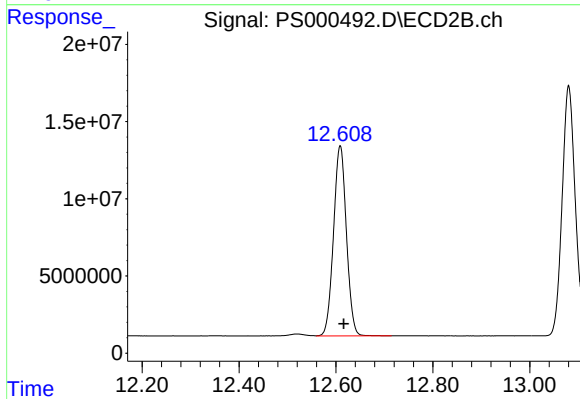

#8 DICHLORPROP


R.T.: 12.609 min
Delta R.T.: -0.007 min
Response: 226993026
Conc: 705.01 ng/ml

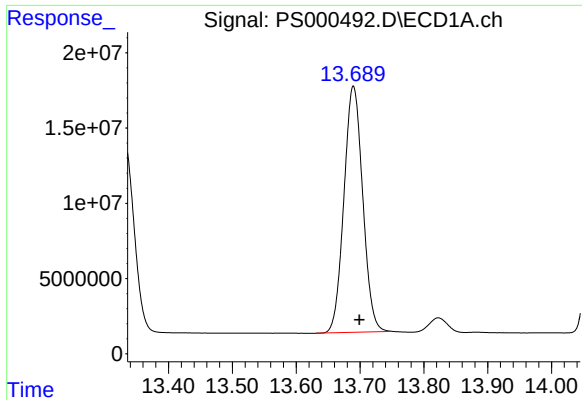

#9 2,4-D


R.T.: 13.690 min
Delta R.T.: -0.009 min
Response: 334905746
Conc: 700.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

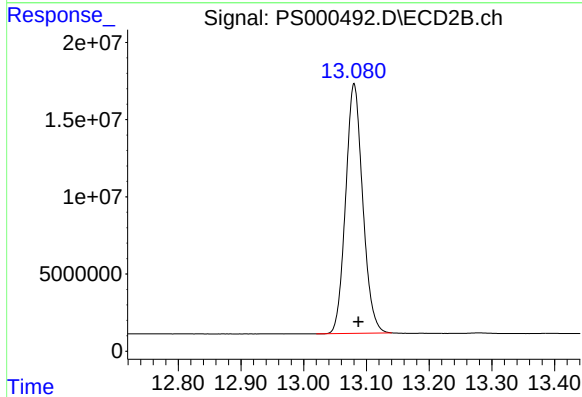


#9 2,4-D

R.T.: 13.080 min
Delta R.T.: -0.007 min
Response: 306355285
Conc: 720.84 ng/ml

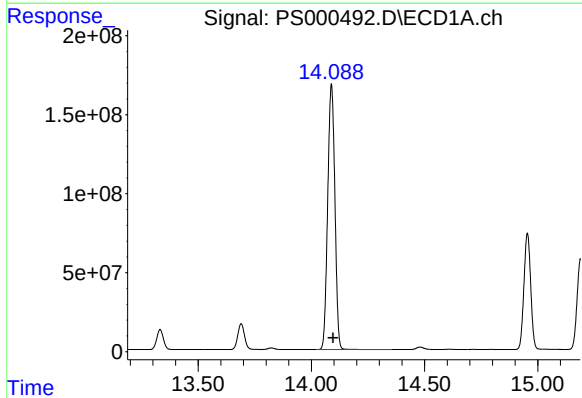


#10 Pentachlorophenol

R.T.: 14.088 min
Delta R.T.: -0.008 min
Response: 3696810289
Conc: 704.16 ng/ml

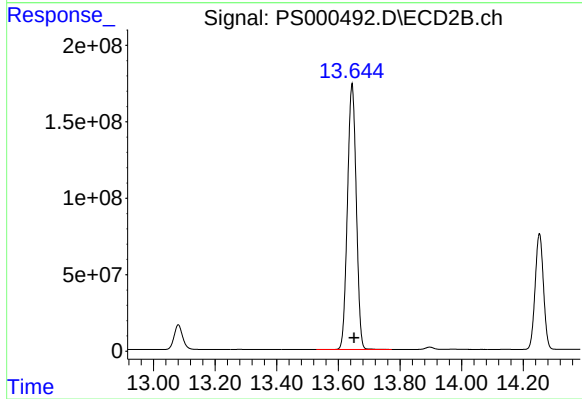

#10 Pentachlorophenol


R.T.: 13.645 min
Delta R.T.: -0.006 min
Response: 3446988215
Conc: 728.65 ng/ml

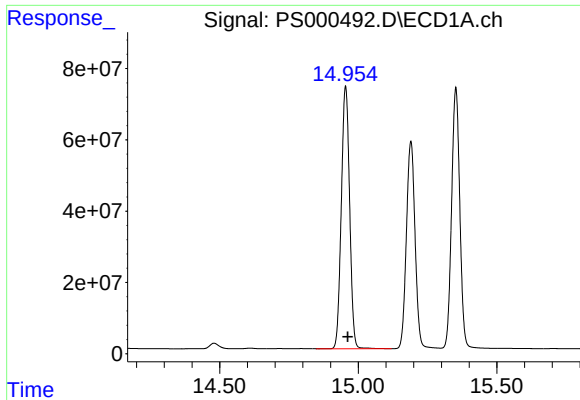

#11 2,4,5-TP (SILVEX)


R.T.: 14.954 min
Delta R.T.: -0.008 min
Response: 1531907520
Conc: 705.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

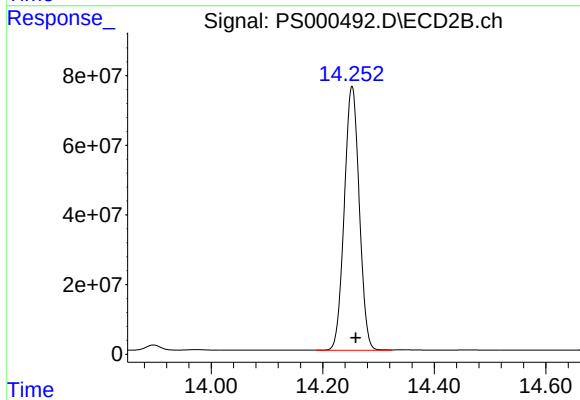


#11 2,4,5-TP (SILVEX)

R.T.: 14.253 min
Delta R.T.: -0.007 min
Response: 1412961019
Conc: 726.08 ng/ml

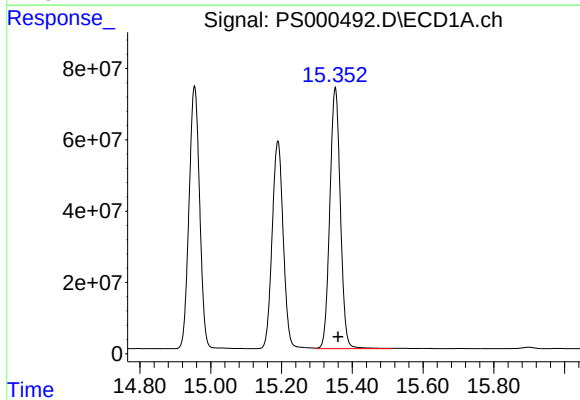


#12 2,4,5-T

R.T.: 15.352 min
Delta R.T.: -0.008 min
Response: 1513768744
Conc: 703.01 ng/ml

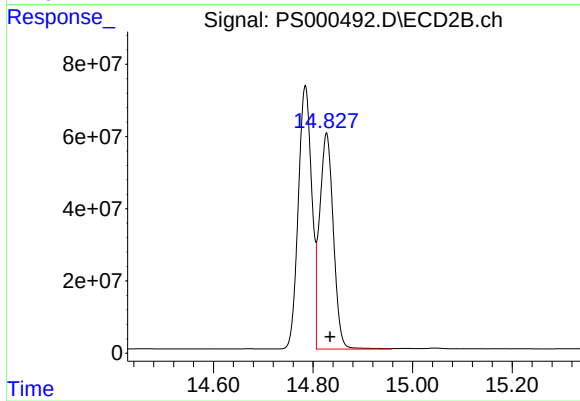

#12 2,4,5-T


R.T.: 14.827 min
Delta R.T.: -0.007 min
Response: 1143898196
Conc: 676.41 ng/ml

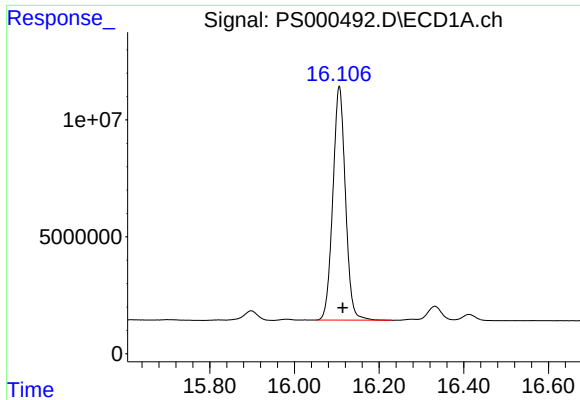

#13 2,4-DB


R.T.: 16.106 min
Delta R.T.: -0.008 min
Response: 206253700
Conc: 700.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

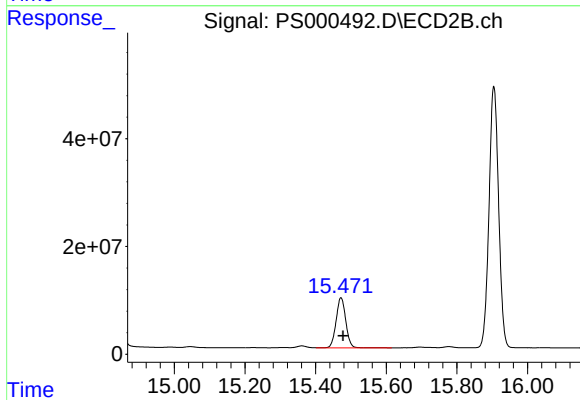


#13 2,4-DB

R.T.: 15.472 min
Delta R.T.: -0.006 min
Response: 179010479
Conc: 723.14 ng/ml

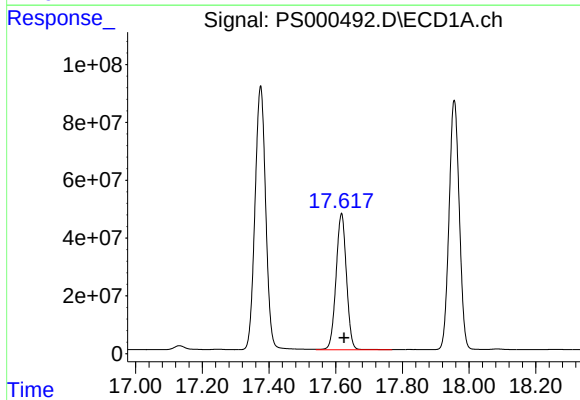


#14 DINOSEB

R.T.: 17.617 min
Delta R.T.: -0.008 min
Response: 1017670090
Conc: 683.40 ng/ml

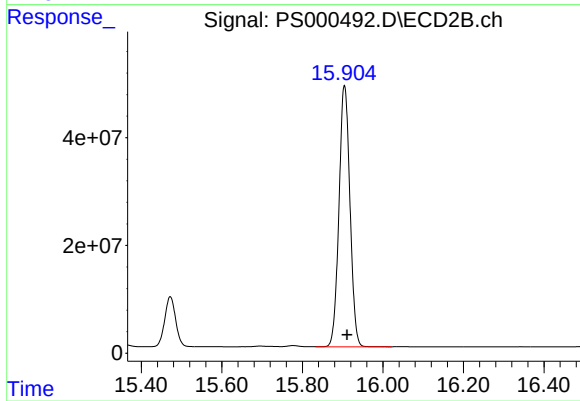

#14 DINOSEB


R.T.: 15.904 min
Delta R.T.: -0.007 min
Response: 917761263
Conc: 703.50 ng/ml

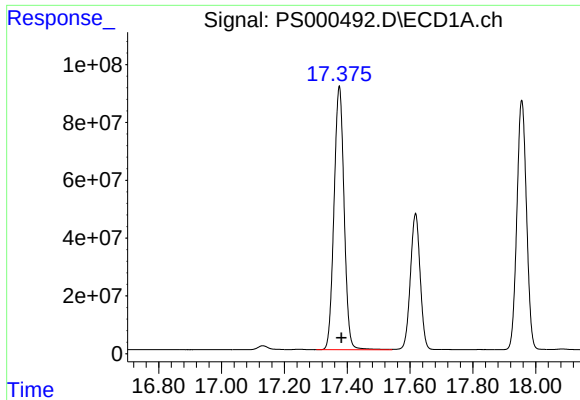

#15 Picloram


R.T.: 17.375 min
Delta R.T.: -0.007 min
Response: 2031192703
Conc: 695.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

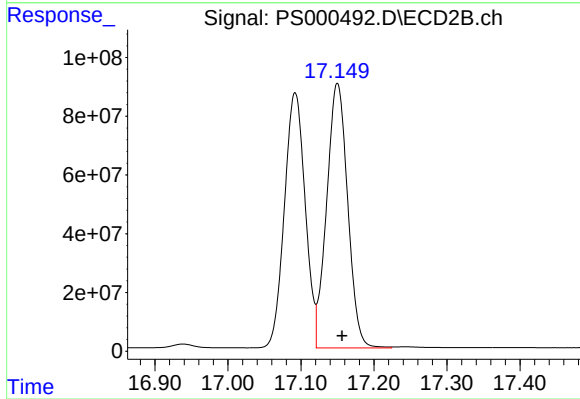


#15 Picloram

R.T.: 17.150 min
Delta R.T.: -0.006 min
Response: 1800577620
Conc: 721.86 ng/ml

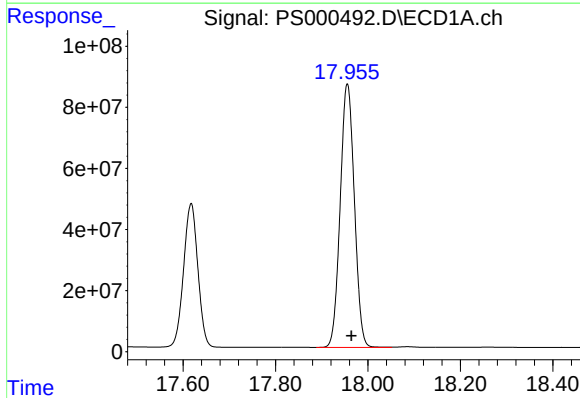

#16 DCPA

R.T.: 17.956 min
Delta R.T.: -0.009 min
Response: 1833862659
Conc: 715.66 ng/ml

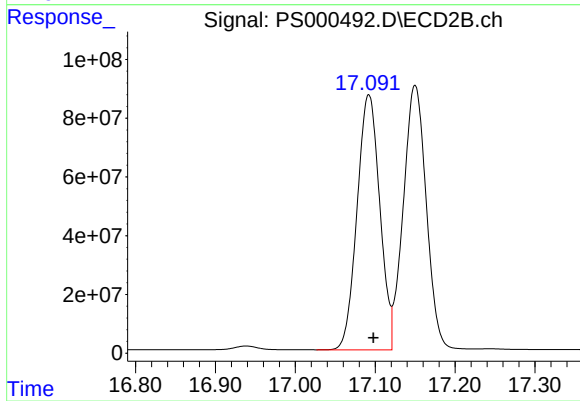

#16 DCPA

R.T.: 17.092 min
Delta R.T.: -0.006 min
Response: 1715049258
Conc: 743.75 ng/ml