

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
 Data File : PS005140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2019 08:03
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 12:00:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.586	5.283	531.6E6	364.8E6	362.152	363.965
Target Compounds							
12) T	2,4,5-T	7.593	7.392	31982276	31988776	3.974	6.271 #
15) T	Picloram	9.154	9.095	223.8E6	169.9E6	19.477	22.520
16) T	DCPA	0.000	9.095	0	169.9E6	N.D.	24.964



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
Data File : PS005140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 08:03
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 12:00:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

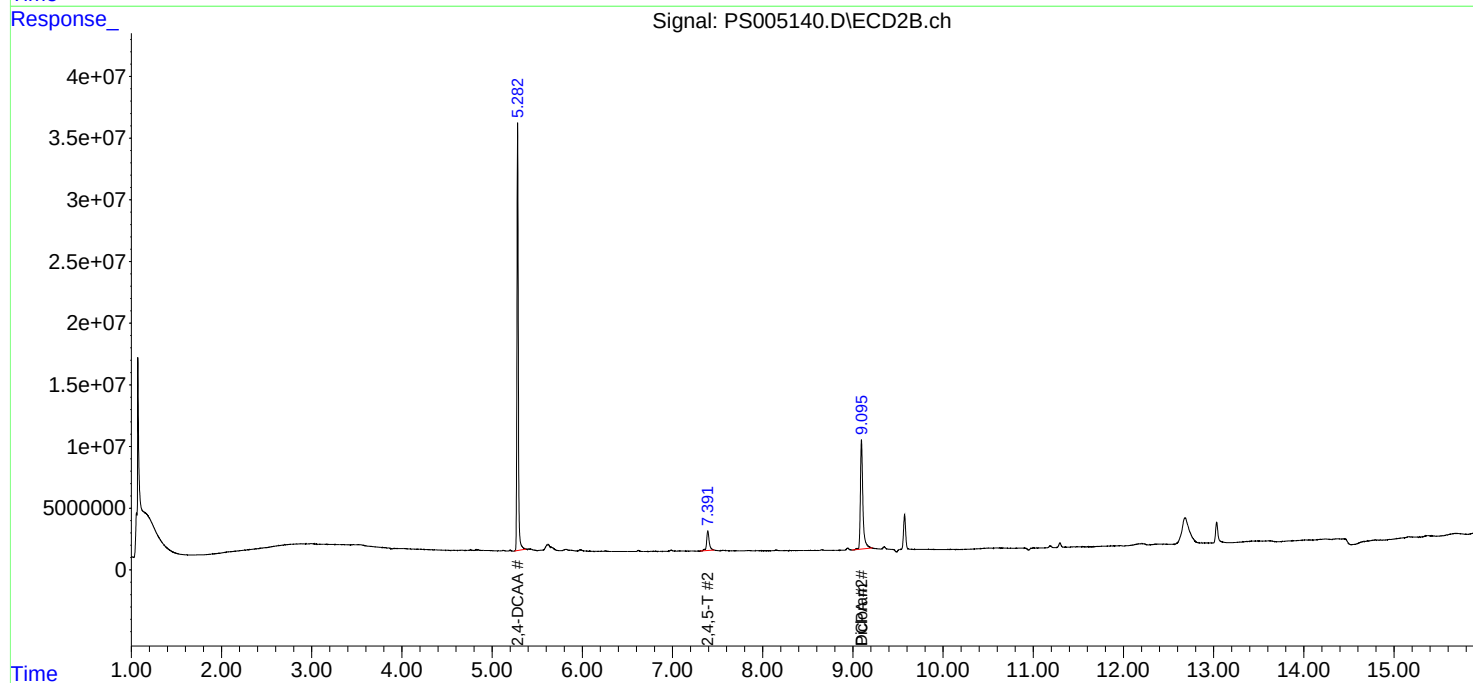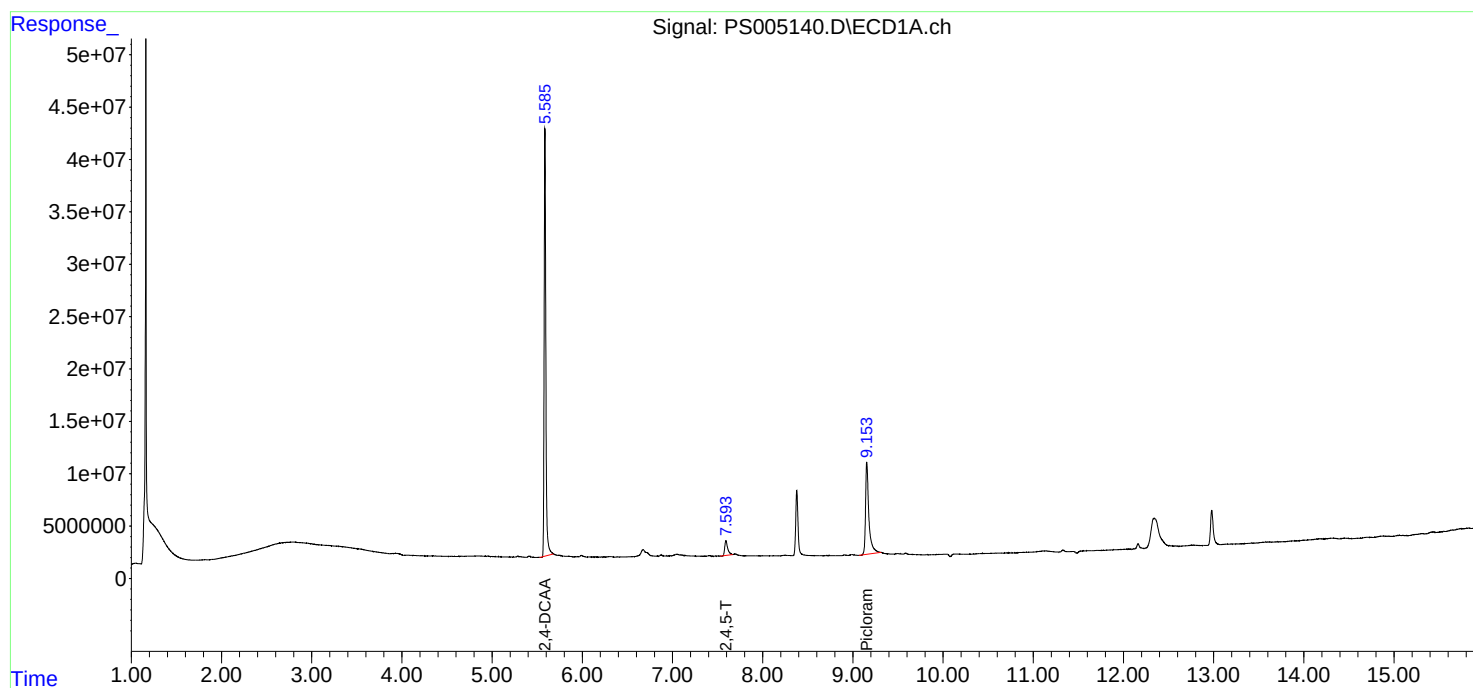


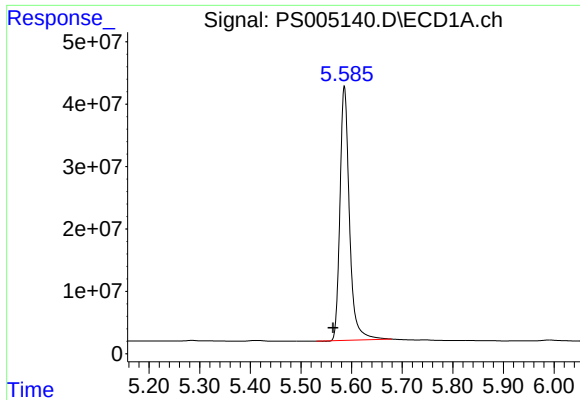

#4 2,4-DCAA


R.T.: 5.586 min
Delta R.T.: 0.022 min
Response: 531600327
Conc: 362.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

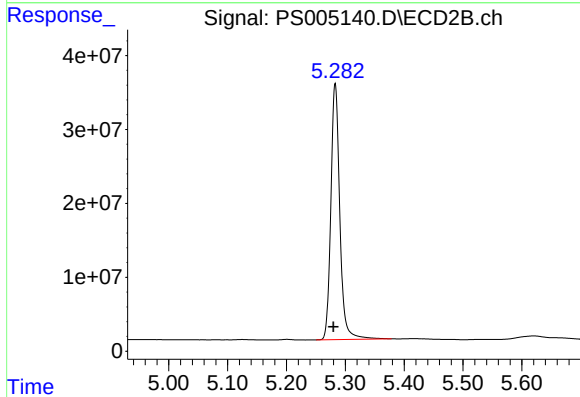


#4 2,4-DCAA

R.T.: 5.283 min
Delta R.T.: 0.003 min
Response: 364827016
Conc: 363.96 ng/ml

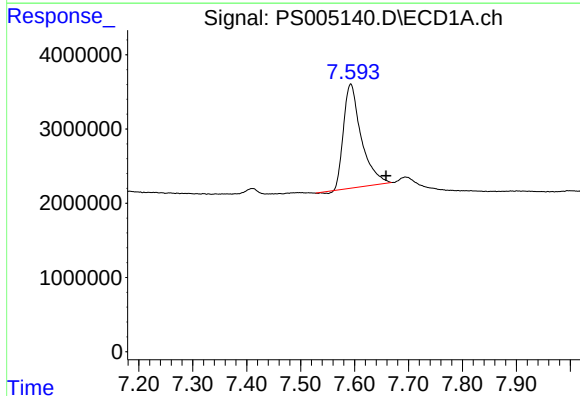


#12 2,4,5-T

R.T.: 7.593 min
Delta R.T.: -0.066 min
Response: 31982276
Conc: 3.97 ng/ml

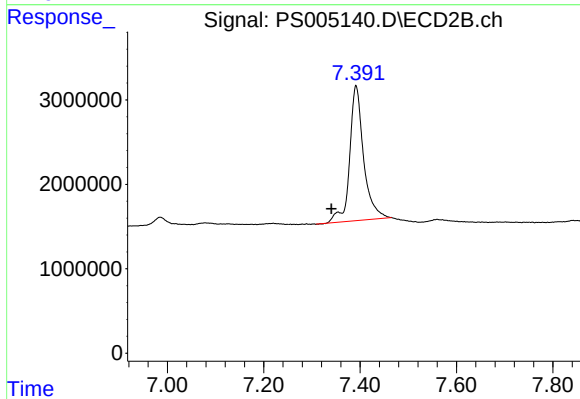

#12 2,4,5-T


R.T.: 7.392 min
Delta R.T.: 0.051 min
Response: 31988776
Conc: 6.27 ng/ml

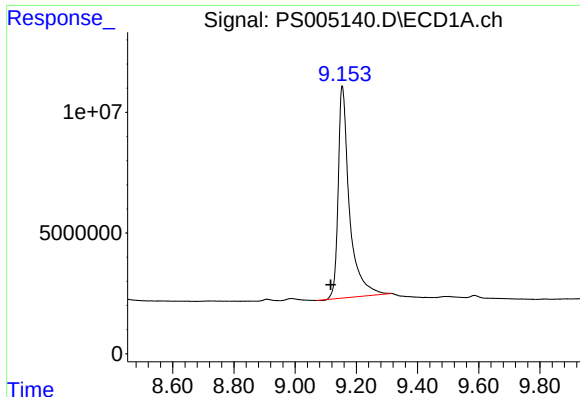

#15 Picloram


R.T.: 9.154 min
Delta R.T.: 0.038 min
Response: 223814545
Conc: 19.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

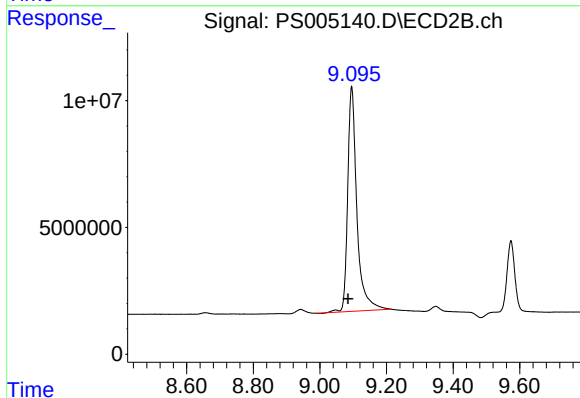


#15 Picloram

R.T.: 9.095 min
Delta R.T.: 0.011 min
Response: 169943244
Conc: 22.52 ng/ml

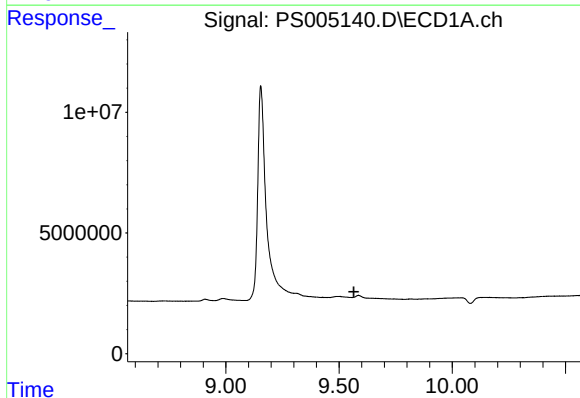

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

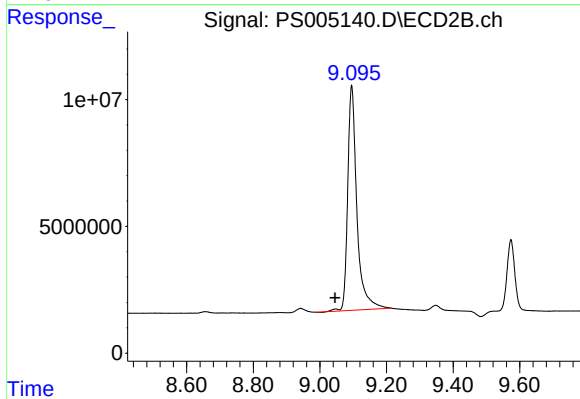

#16 DCPA

R.T.: 9.095 min
Delta R.T.: 0.050 min
Response: 169943244
Conc: 24.96 ng/ml