

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
 Data File : PS005151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2019 12:51
 Operator : SM\AJ
 Sample : K3439-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-0D015-03-006

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 14:33:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.567	5.281	99222082	54738170	67.595	54.609
Target Compounds							
1) T	Dalapon	2.070	0.000	54640601	0	29.643	N.D. #
2) T	3,5-DICHL...	0.000	4.599	0	198.3E6	N.D.	150.356
3) T	4-Nitroph...	5.369	0.000	30781017	0	42.498	N.D. #
5) T	DICAMBA	5.664	5.387	13024136	28122593	2.283	7.513 #
6) T	MCPD	5.878	0.000	12648446	0	2.889	N.D. #
7) T	MCPA	6.059	5.673	25100819	24277845	3.997	5.993 #
9) T	2,4-D	0.000	6.229	0	22095346	N.D.	19.811
11) T	2,4,5-TP ...	0.000	6.935	0	57442204	N.D.	10.787
13) T	2,4-DB	8.210	7.842	219.6E6	152.1E6	189.075	233.027
14) T	DINOSEB	0.000	8.170	0	62683440	N.D.	15.503
15) T	Picloram	9.058	0.000	23507233	0	2.046	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
Data File : PS005151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 12:51
Operator : SM\AJ
Sample : K3439-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 14:33:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

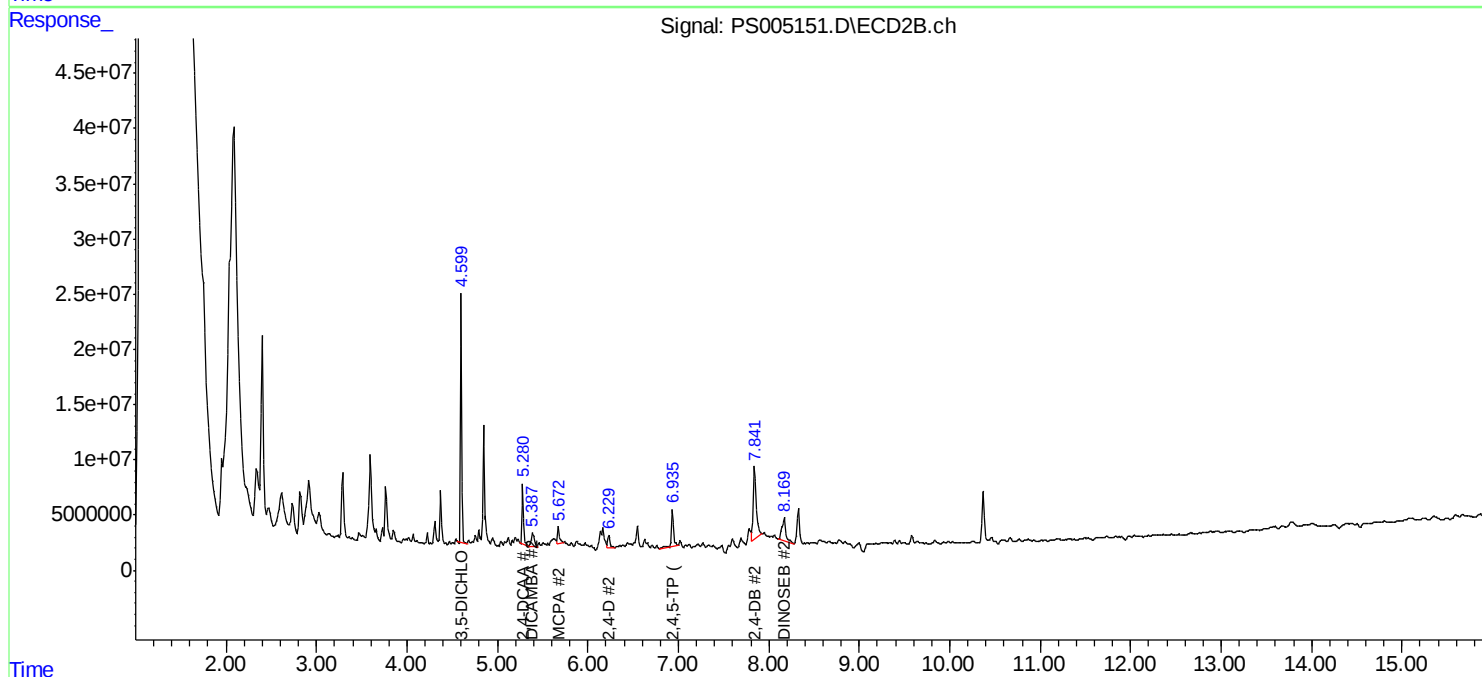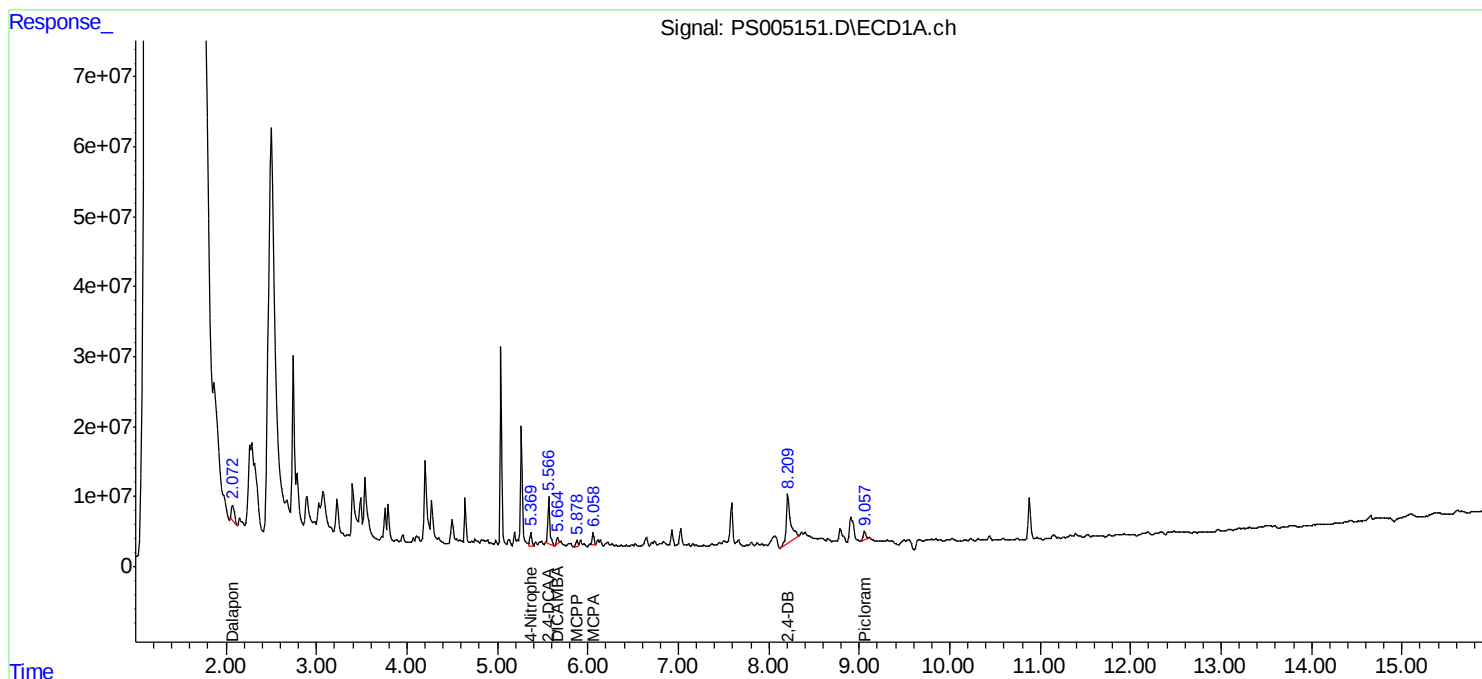


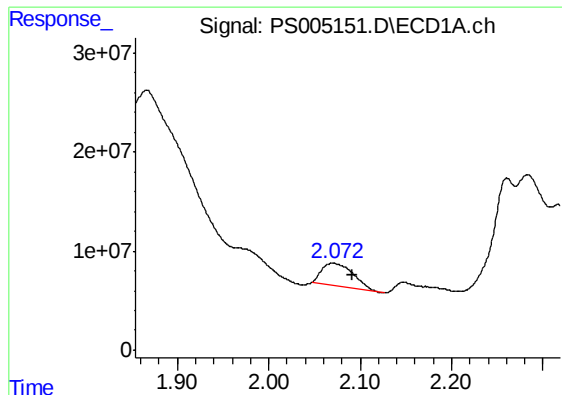

#1 Dalapon


R.T.: 2.070 min
Delta R.T.: -0.022 min
Response: 54640601
Conc: 29.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006

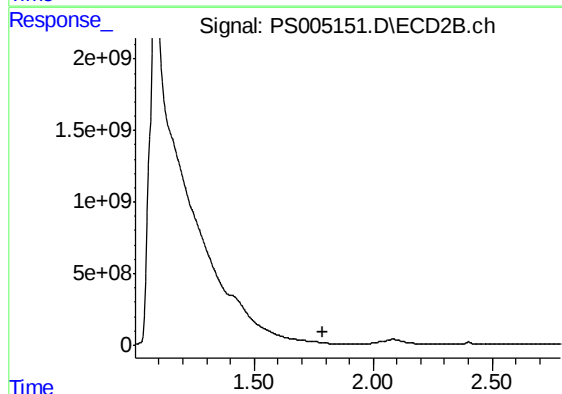


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

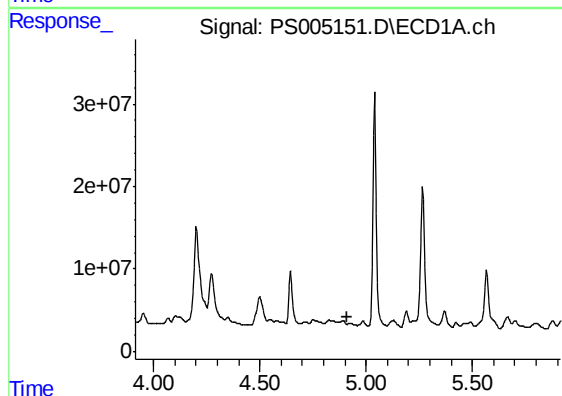


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

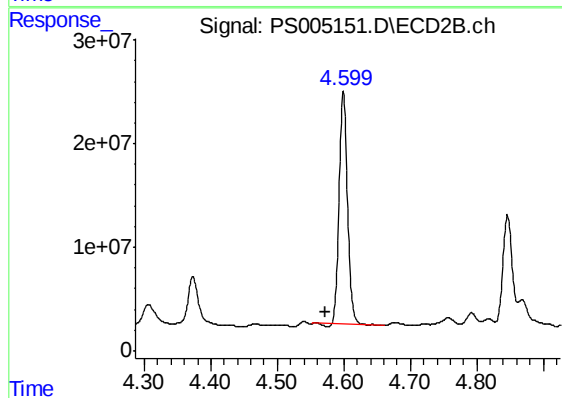

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.599 min
Delta R.T.: 0.027 min
Response: 198276403
Conc: 150.36 ng/ml

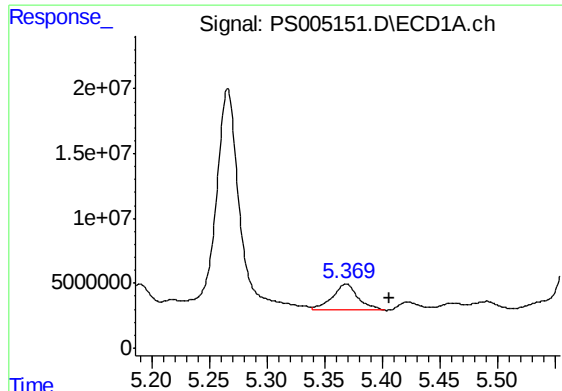

#3 4-Nitrophenol


R.T.: 5.369 min
Delta R.T.: -0.038 min
Response: 30781017
Conc: 42.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006

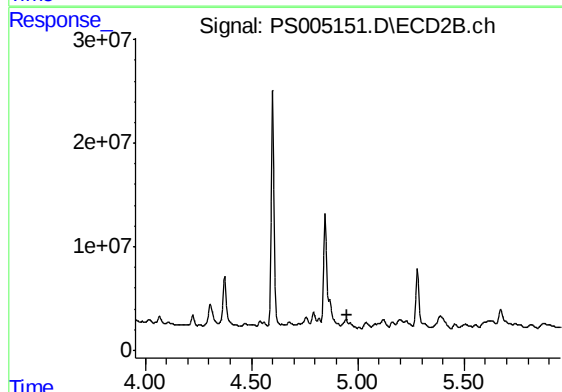


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

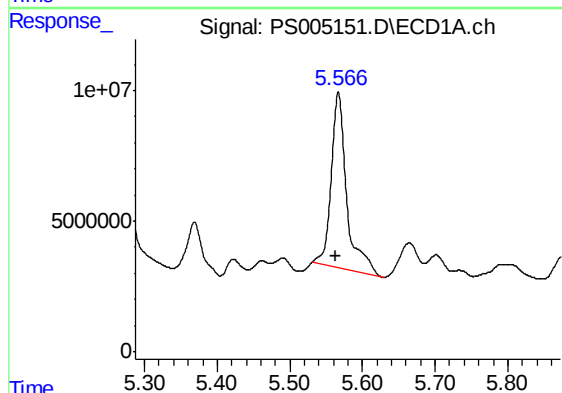


#4 2,4-DCAA

R.T.: 5.567 min
Delta R.T.: 0.003 min
Response: 99222082
Conc: 67.59 ng/ml

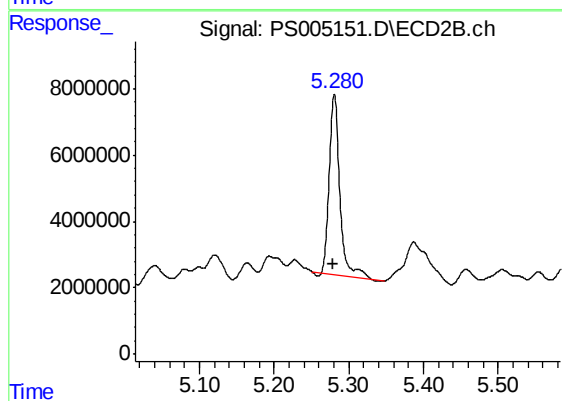

#4 2,4-DCAA


R.T.: 5.281 min
Delta R.T.: 0.000 min
Response: 54738170
Conc: 54.61 ng/ml

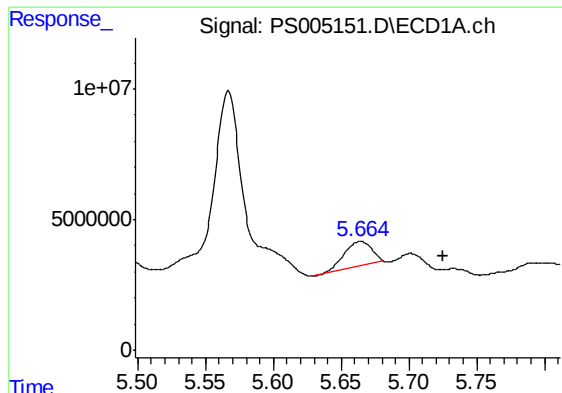

#5 DICAMBA


R.T.: 5.664 min
Delta R.T.: -0.061 min
Response: 13024136
Conc: 2.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006

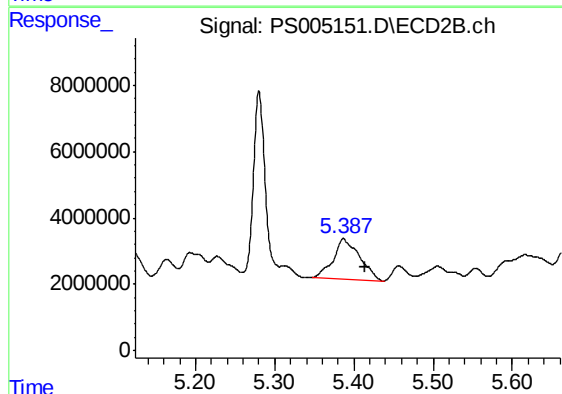


#5 DICAMBA

R.T.: 5.387 min
Delta R.T.: -0.027 min
Response: 28122593
Conc: 7.51 ng/ml

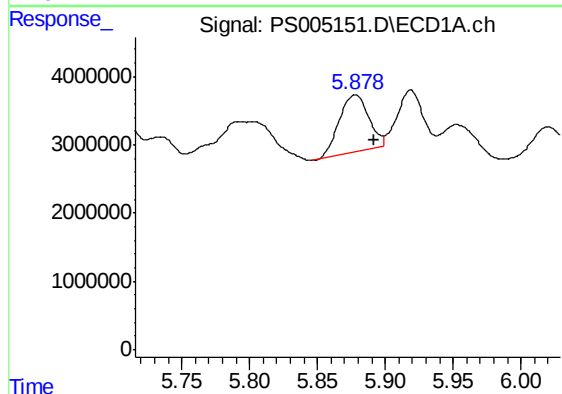


#6 MCPP

R.T.: 5.878 min
Delta R.T.: -0.014 min
Response: 12648446
Conc: 2.89 ug/ml

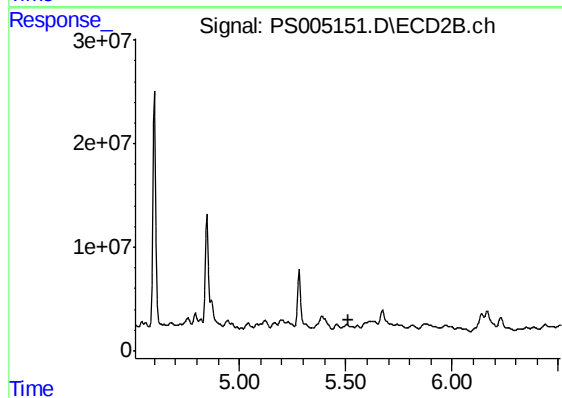

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

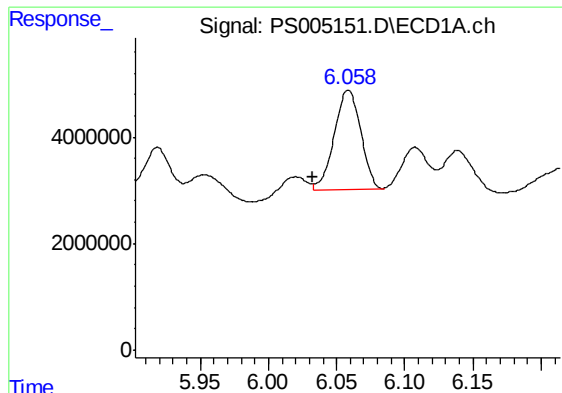

#7 MCPA


R.T.: 6.059 min
Delta R.T.: 0.027 min
Response: 25100819
Conc: 4.00 ug/ml

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006

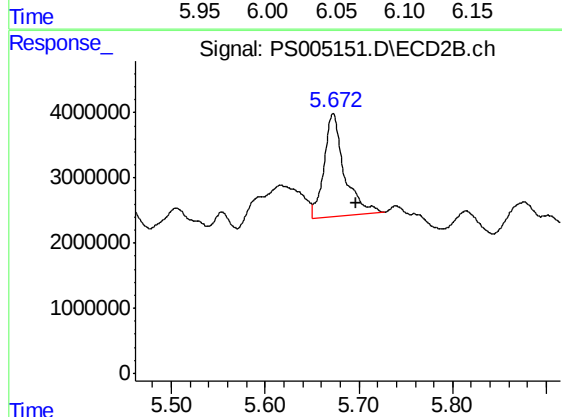


#7 MCPA

R.T.: 5.673 min
Delta R.T.: -0.025 min
Response: 24277845
Conc: 5.99 ug/ml

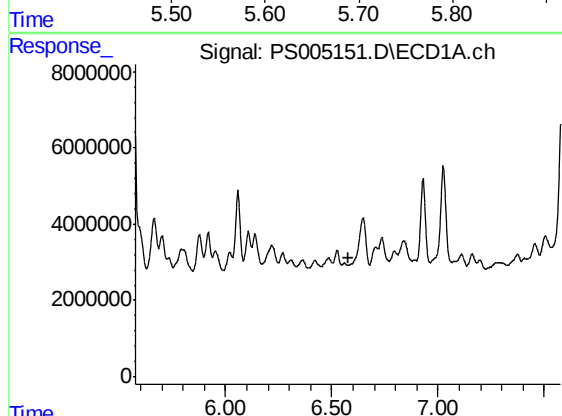


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.576 min
Response: 0
Conc: N.D.

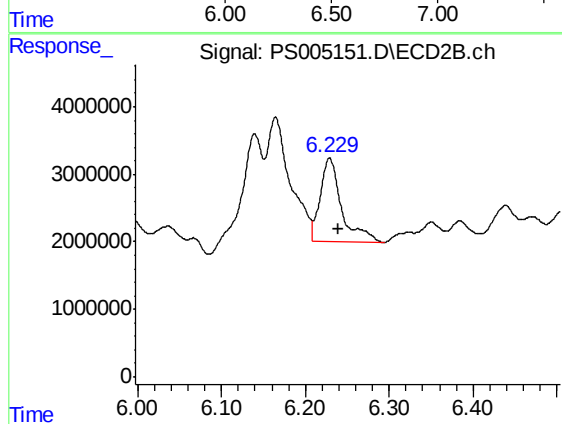

#9 2,4-D


R.T.: 6.229 min
Delta R.T.: -0.011 min
Response: 22095346
Conc: 19.81 ng/ml

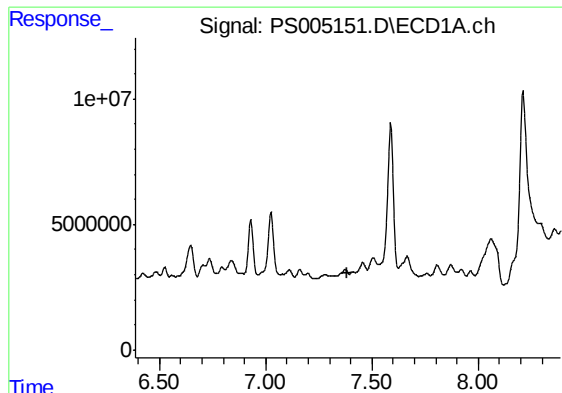

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006

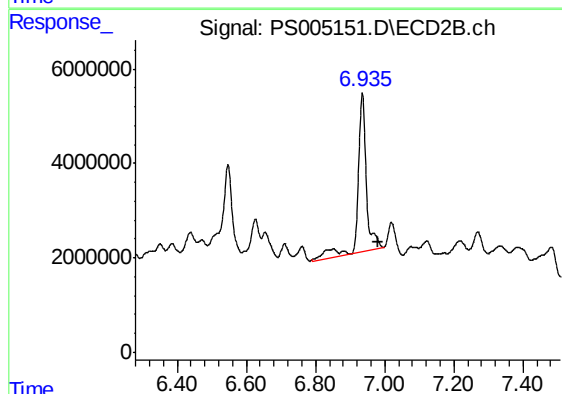


#11 2,4,5-TP (SILVEX)

R.T.: 6.935 min
Delta R.T.: -0.045 min
Response: 57442204
Conc: 10.79 ng/ml

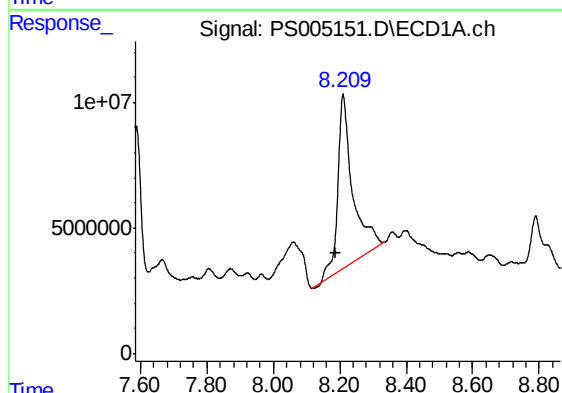


#13 2,4-DB

R.T.: 8.210 min
Delta R.T.: 0.021 min
Response: 219619217
Conc: 189.07 ng/ml

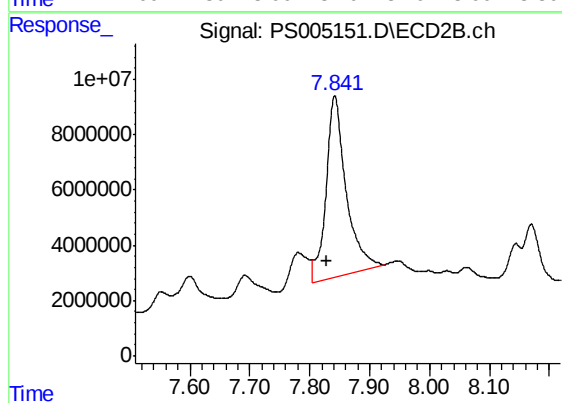

#13 2,4-DB


R.T.: 7.842 min
Delta R.T.: 0.012 min
Response: 152132276
Conc: 233.03 ng/ml

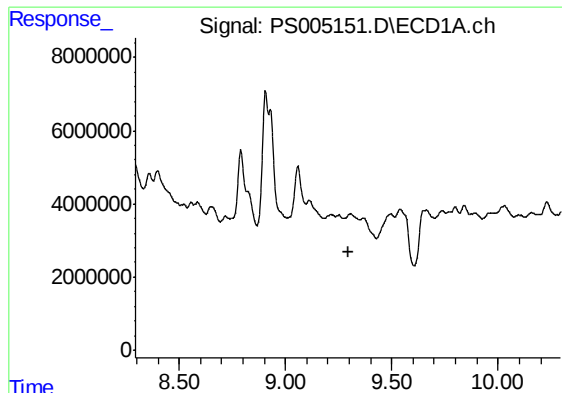

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006

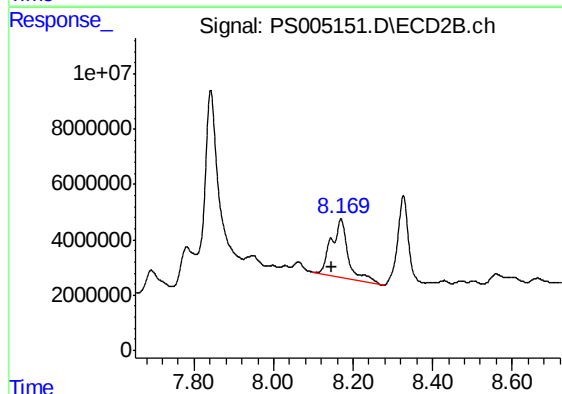


#14 DINOSEB

R.T.: 8.170 min
Delta R.T.: 0.024 min
Response: 62683440
Conc: 15.50 ng/ml

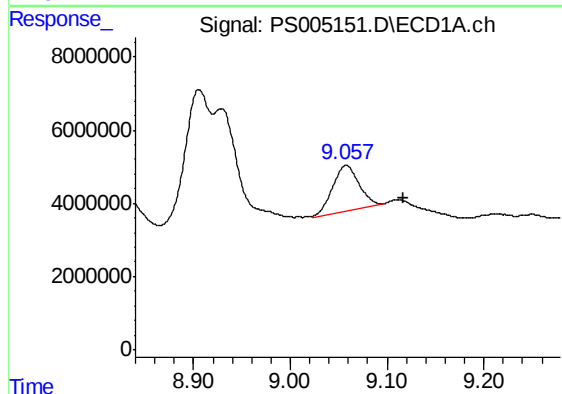

#15 Picloram

R.T.: 9.058 min
Delta R.T.: -0.059 min
Response: 23507233
Conc: 2.05 ng/ml

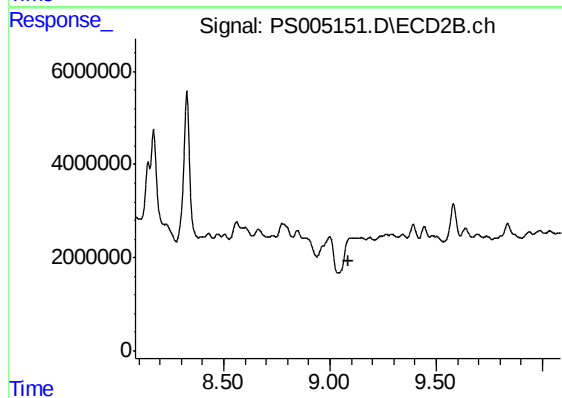

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.