

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
 Data File : PS005144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2019 10:17
 Operator : SM\AJ
 Sample : K3420-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BAT-B12

Manual Integrations
 APPROVED

Ankita
 6/21/2019 2:31:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 12:01:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.567	5.282	490.2E6	281.6E6	333.972m	280.967m
Target Compounds							
10) T	Pentachlo...	6.842	6.581	599.0E6	682.7E6	30.445	53.105m#
13) T	2,4-DB	8.210	7.835	120.1E6	109.0E6	103.371	166.949m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
Data File : PS005144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 10:17
Operator : SM\AJ
Sample : K3420-02
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
BAT-B12


Manual Integrations
APPROVED

Ankita
6/21/2019 2:31:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 12:01:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

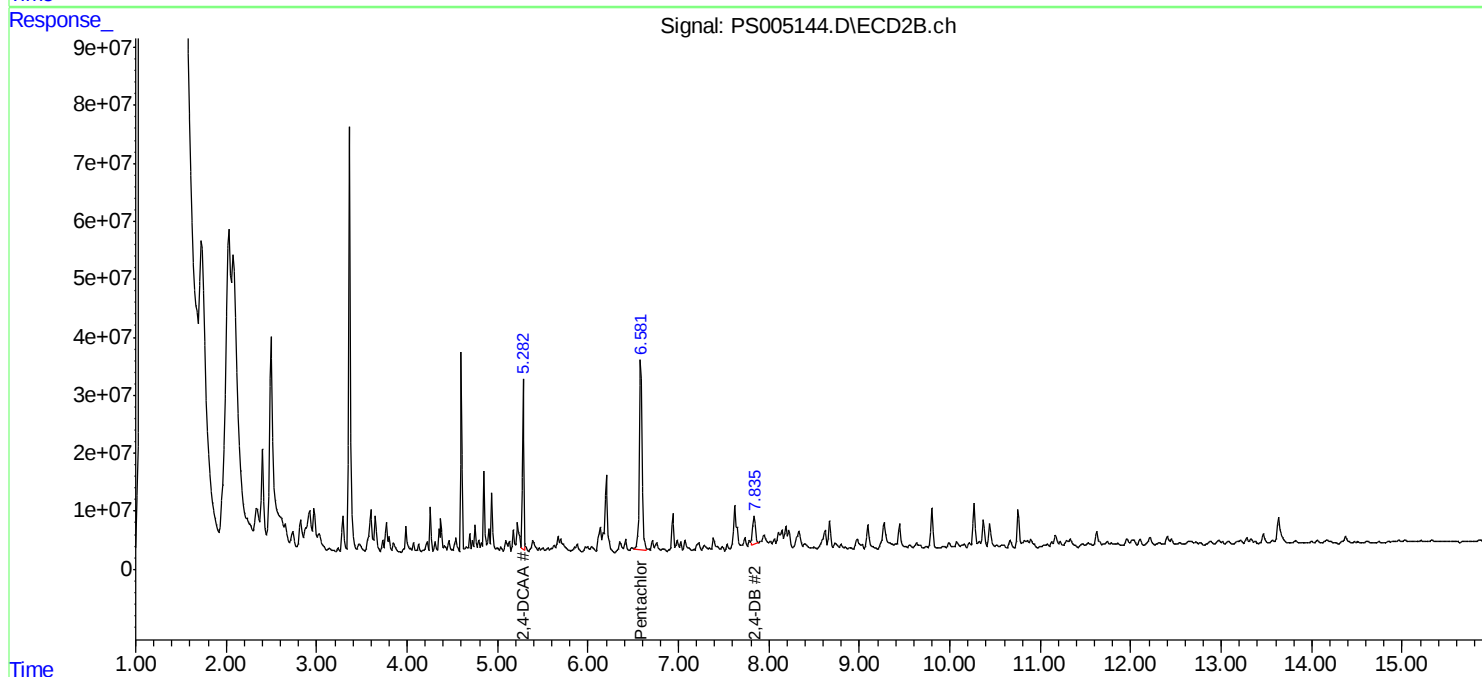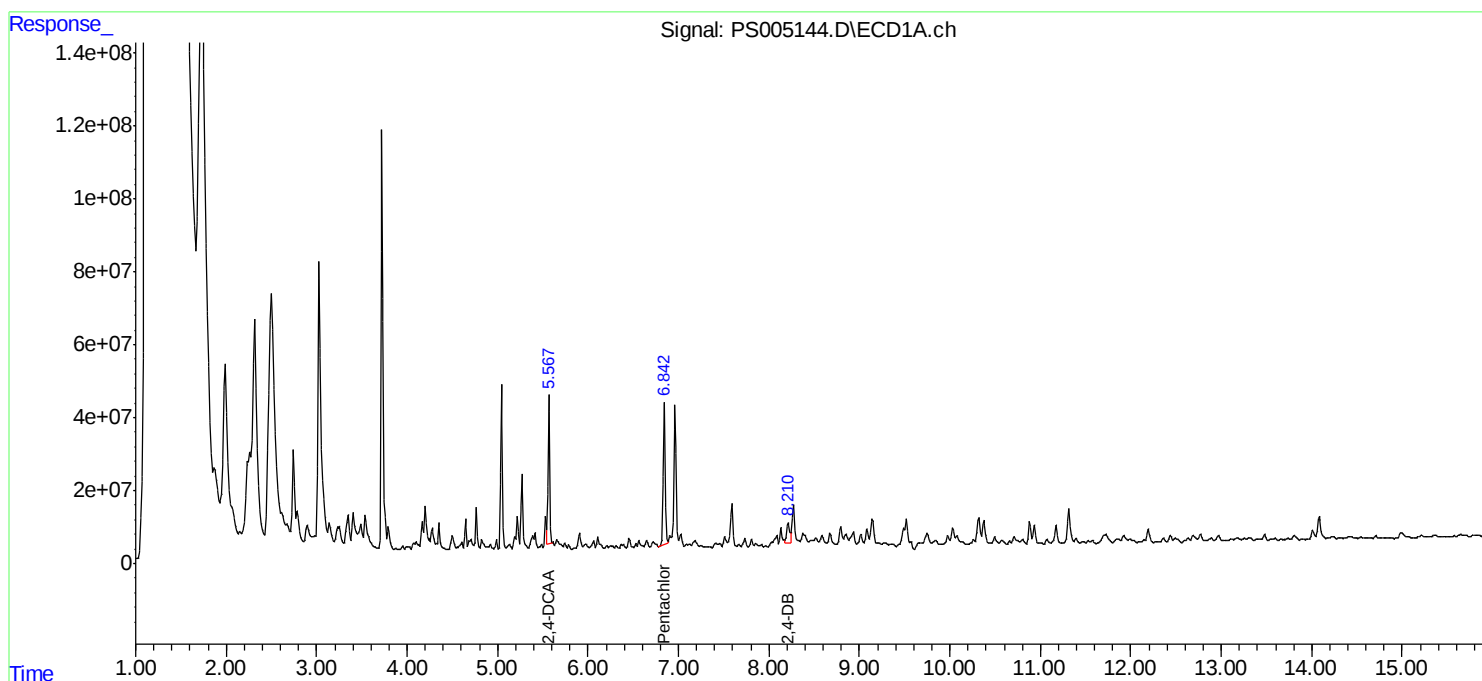

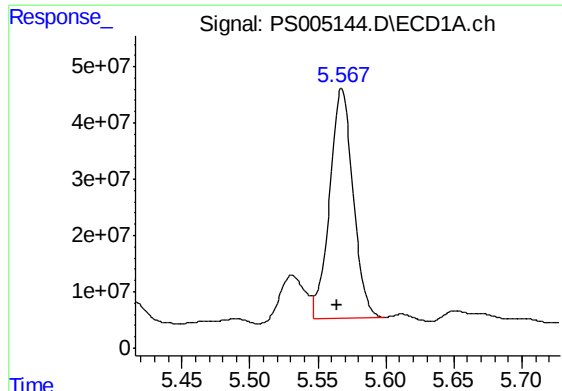


#4 2,4-DCAA

R.T.: 5.567 min
Delta R.T.: 0.003 min
Response: 490234874
Conc: 333.97 ng/ml m

Instrument :
ECD_S
ClientSampleId :
BAT-B12


Manual Integrations
APPROVED

Ankita
6/21/2019 2:31:51 PM

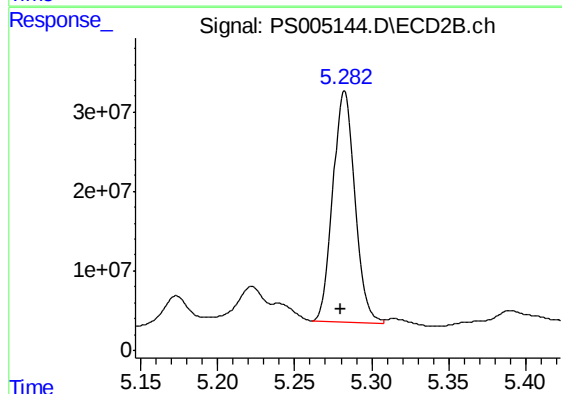


#4 2,4-DCAA

R.T.: 5.282 min
Delta R.T.: 0.002 min
Response: 281632380
Conc: 280.97 ng/ml m

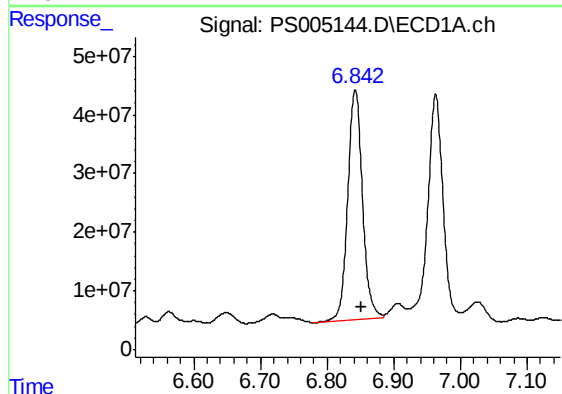


#10 Pentachlorophenol

R.T.: 6.842 min
Delta R.T.: -0.009 min
Response: 599041417
Conc: 30.45 ng/ml

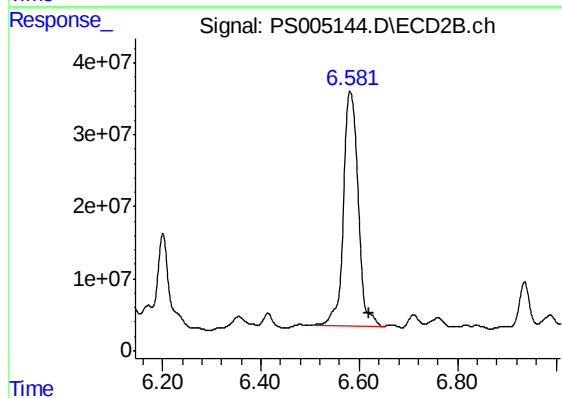

#10 Pentachlorophenol

R.T.: 6.581 min
Delta R.T.: -0.038 min
Response: 682730769
Conc: 53.10 ng/ml m

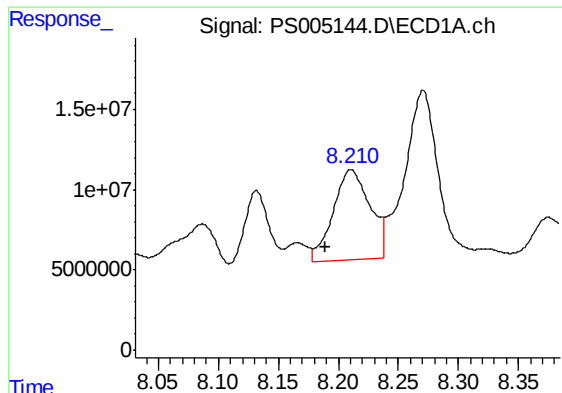


#13 2,4-DB

R.T.: 8.210 min
Delta R.T.: 0.021 min
Response: 120069663
Conc: 103.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B12

Manual Integrations
APPROVED

Ankita
6/21/2019 2:31:51 PM

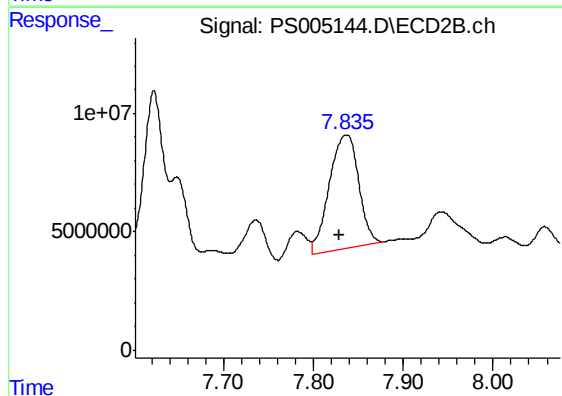

#13 2,4-DB

R.T.: 7.835 min
Delta R.T.: 0.005 min
Response: 108993225
Conc: 166.95 ng/ml m