

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
 Data File : PS005151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2019 12:51
 Operator : SM\AJ
 Sample : K3439-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-0D015-03-006

Manual Integrations
 APPROVED

Ankita
 6/21/2019 2:32:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 16:52:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.566	5.280	113.0E6	57708229	76.962m	57.572m#
Target Compounds							
13) T	2,4-DB	8.210	7.842	219.6E6	152.1E6	189.075	233.027

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
Data File : PS005151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 12:51
Operator : SM\AJ
Sample : K3439-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006


Manual Integrations
APPROVED

Ankita
6/21/2019 2:32:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 16:52:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

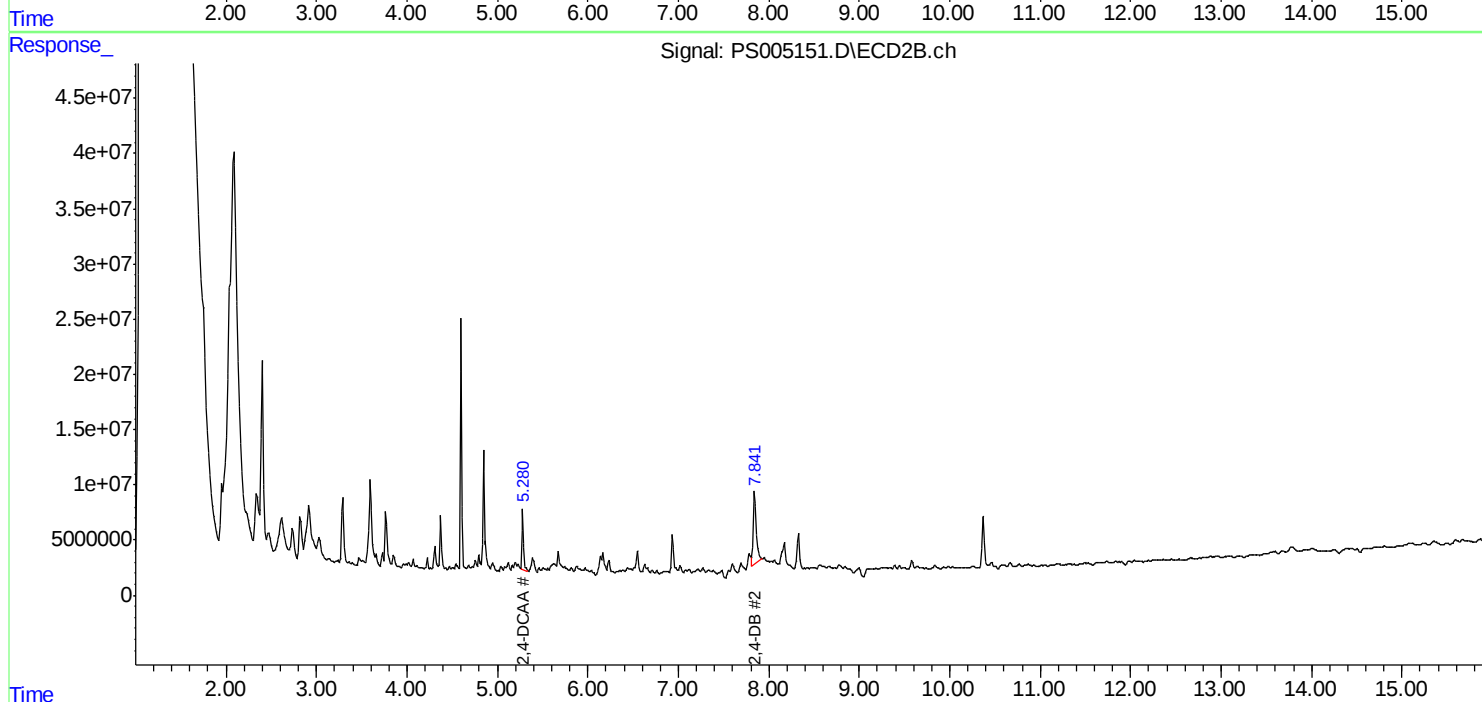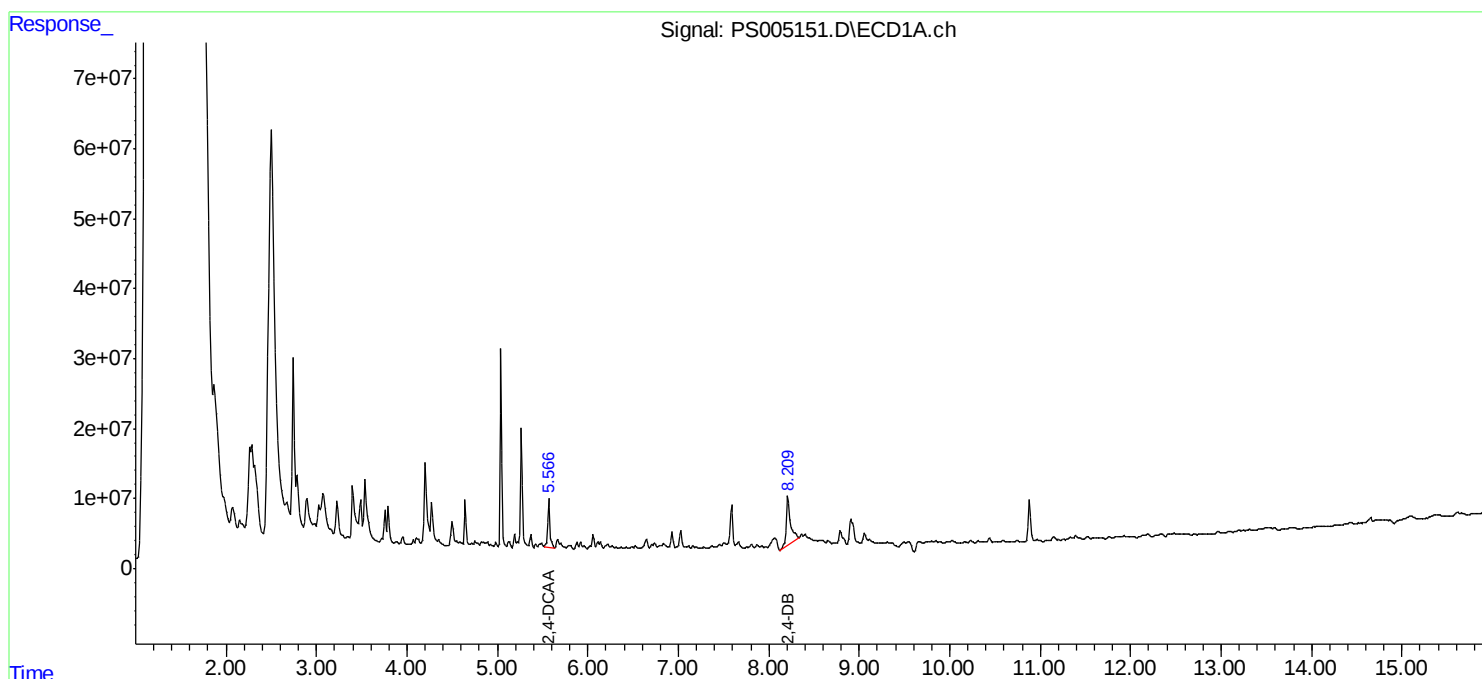

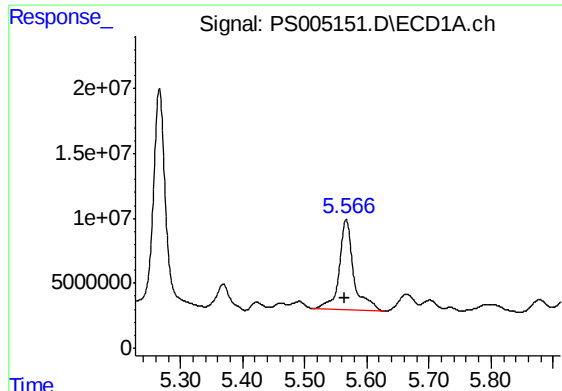


#4 2,4-DCAA

R.T.: 5.566 min
Delta R.T.: 0.003 min
Response: 112971579
Conc: 76.96 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-006


Manual Integrations
APPROVED

Ankita
6/21/2019 2:32:01 PM

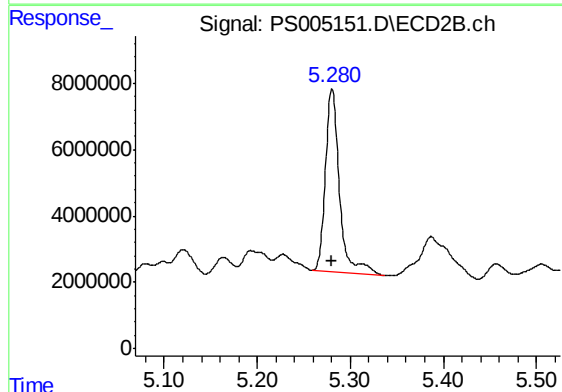


#4 2,4-DCAA

R.T.: 5.280 min
Delta R.T.: 0.000 min
Response: 57708229
Conc: 57.57 ng/ml m

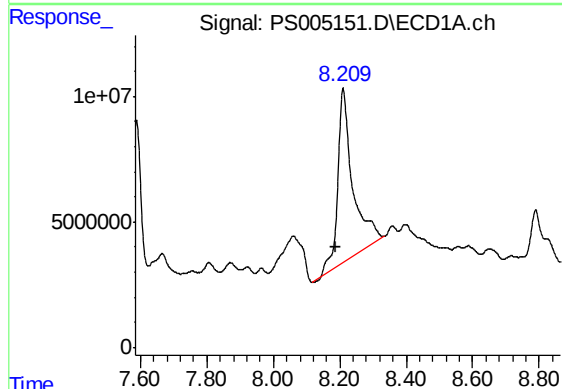

#13 2,4-DB

R.T.: 8.210 min
Delta R.T.: 0.021 min
Response: 219619217
Conc: 189.07 ng/ml

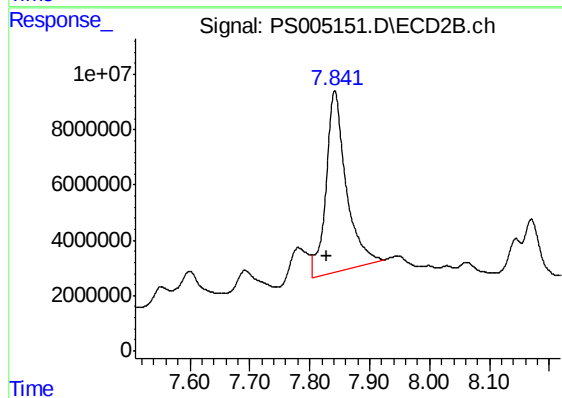

#13 2,4-DB

R.T.: 7.842 min
Delta R.T.: 0.012 min
Response: 152132276
Conc: 233.03 ng/ml