

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
 Data File : PS005154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2019 13:57
 Operator : SM\AJ
 Sample : K3440-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-SF-03-008-A

Manual Integrations
 APPROVED

Ankita
 6/21/2019 2:32:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 14:34:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.567	5.282	330.7E6	207.1E6	225.264m	206.592
Target Compounds							
13) T	2,4-DB	8.212	7.843	229.1E6	163.5E6	197.202	250.373 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062019\
Data File : PS005154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 13:57
Operator : SM\AJ
Sample : K3440-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-SF-03-008-A


Manual Integrations
APPROVED

Ankita
6/21/2019 2:32:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 14:34:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

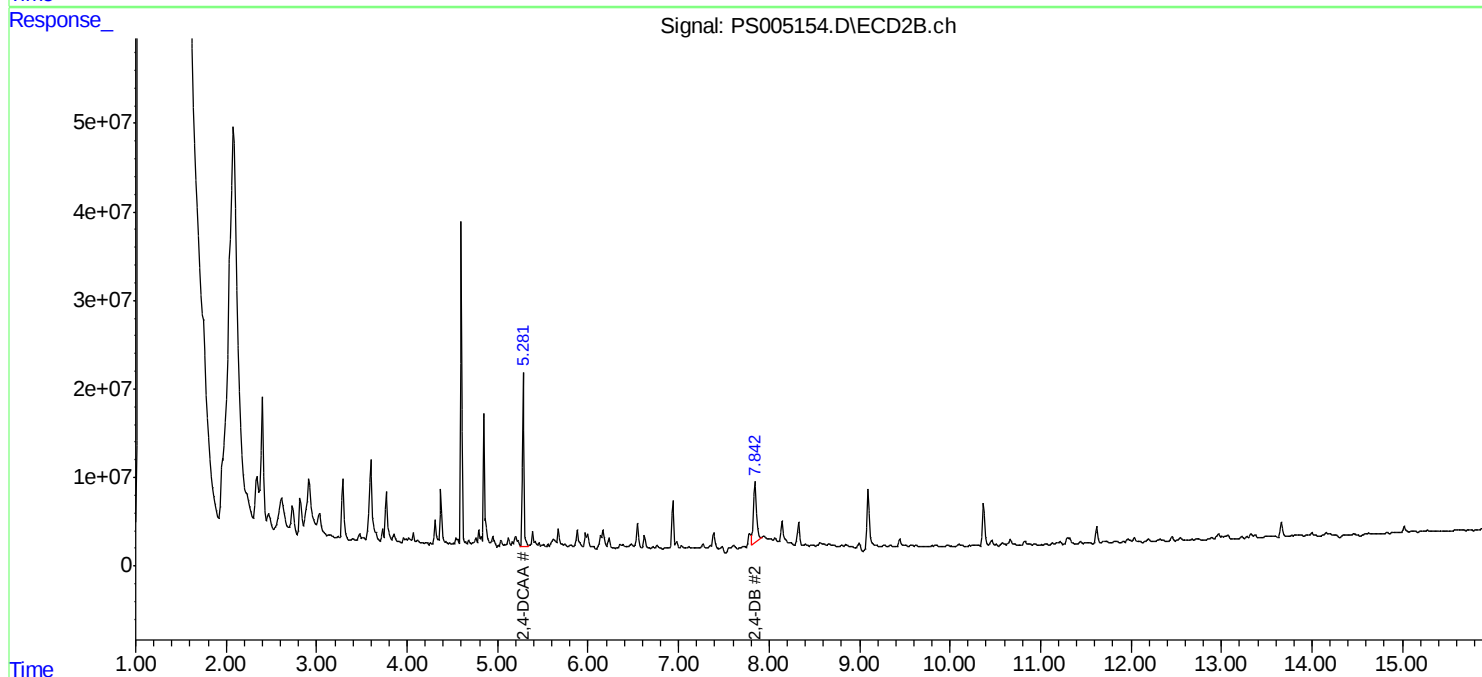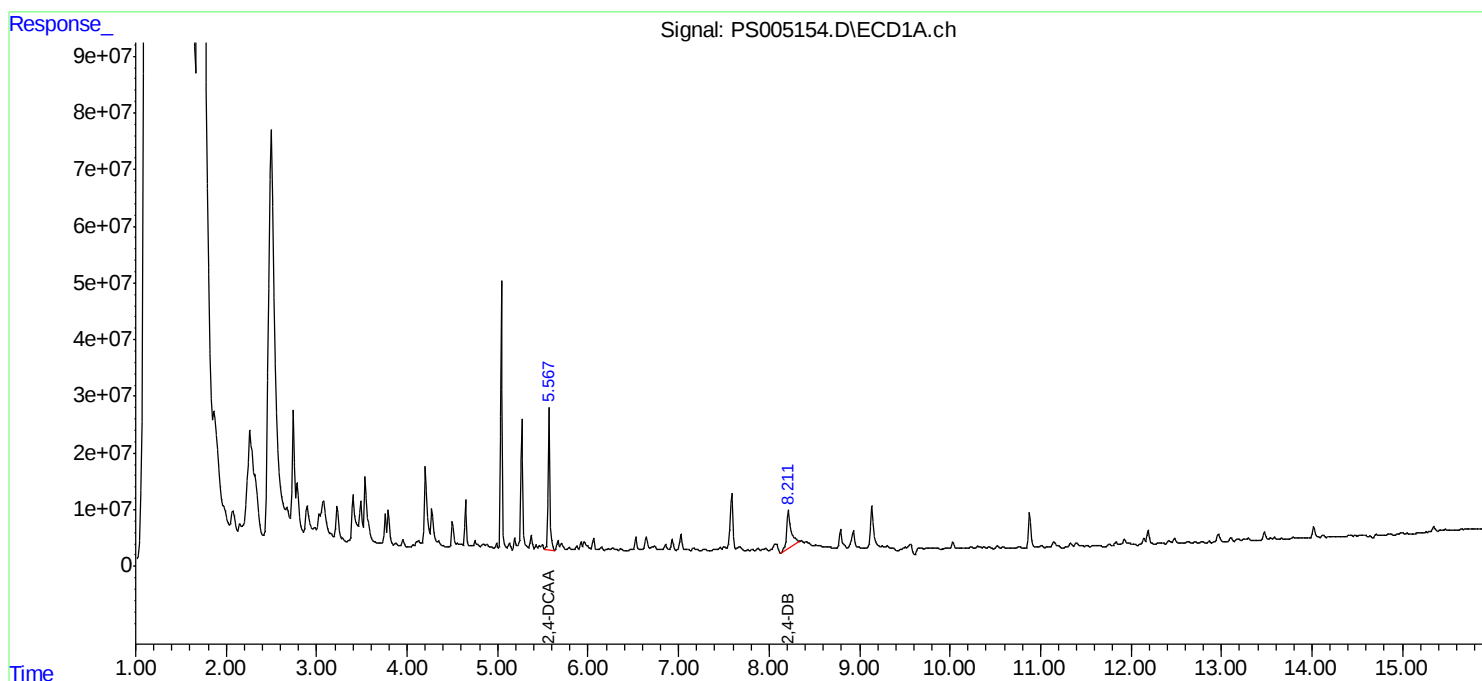

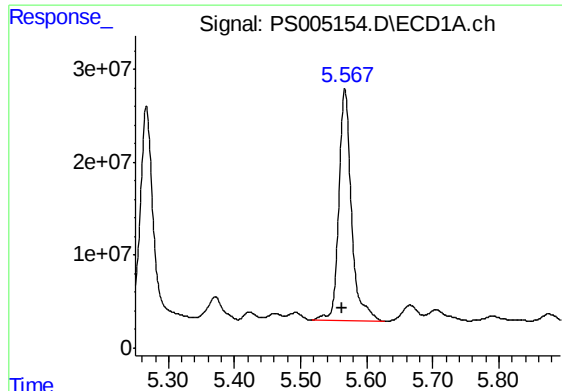


#4 2,4-DCAA

R.T.: 5.567 min
Delta R.T.: 0.003 min
Response: 330663189
Conc: 225.26 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-SF-03-008-A


Manual Integrations
APPROVED

Ankita
6/21/2019 2:32:05 PM

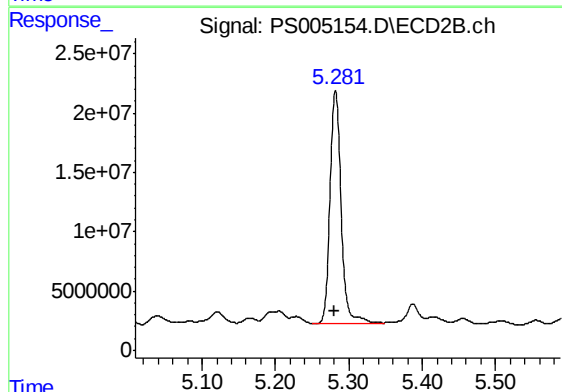


#4 2,4-DCAA

R.T.: 5.282 min
Delta R.T.: 0.002 min
Response: 207081322
Conc: 206.59 ng/ml

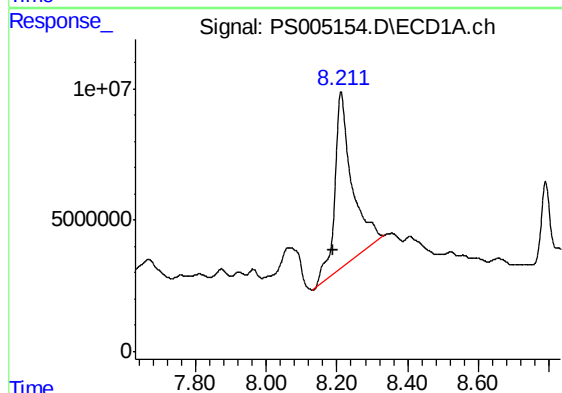

#13 2,4-DB

R.T.: 8.212 min
Delta R.T.: 0.022 min
Response: 229058954
Conc: 197.20 ng/ml

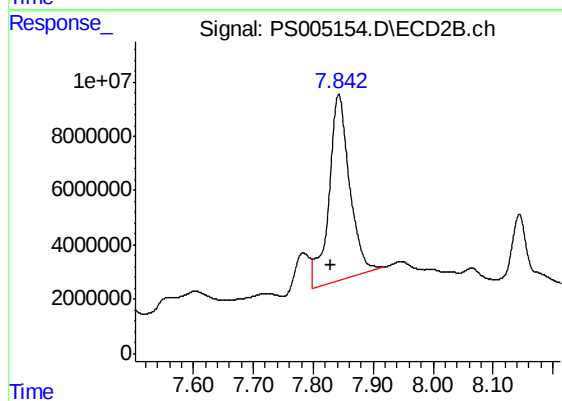

#13 2,4-DB

R.T.: 7.843 min
Delta R.T.: 0.013 min
Response: 163456207
Conc: 250.37 ng/ml