

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062118\
 Data File : PS000538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 21:22
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 00:46:45 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.823	11.201	213.8E6	177.2E6	567.602	520.824
Target Compounds							
1) T	Dalapon	3.195	2.592	167793	63784	0.328	0.146 #
3) T	4-Nitroph...	11.442	0.000	889319	0	3.783	N.D. #
6) T	MCP	12.504	0.000	751030	0	0.663	N.D. #
8) T	DICHLORPROP	13.320	0.000	148918	0	0.396	N.D. #
10) T	Pentachlo...	14.099	0.000	314131	0	0.060	N.D. #
15) T	Picloram	17.338	17.156	20971254	42752	7.181	0.017 #
16) T	DCPA	17.957	17.156	20103910	42752	7.846	0.019 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062118\
Data File : PS000538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 21:22
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 00:46:45 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

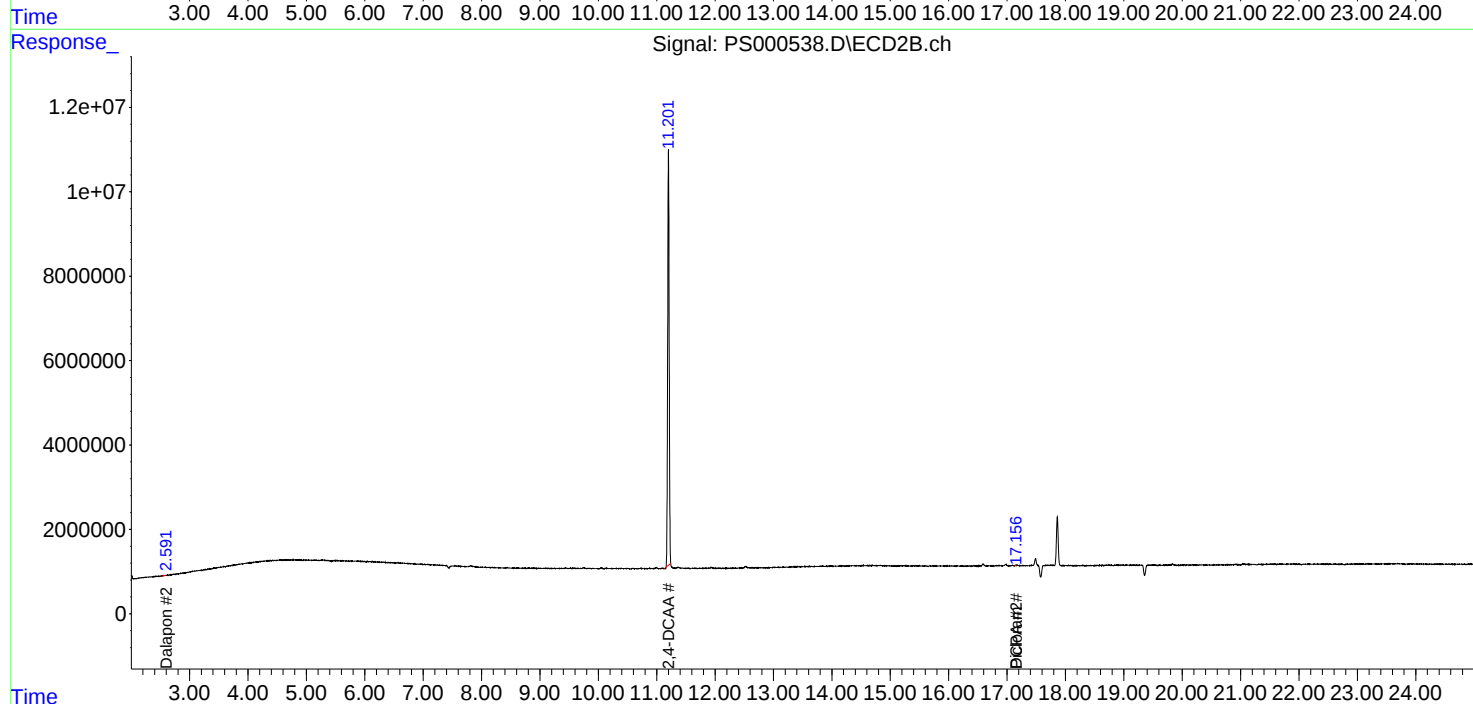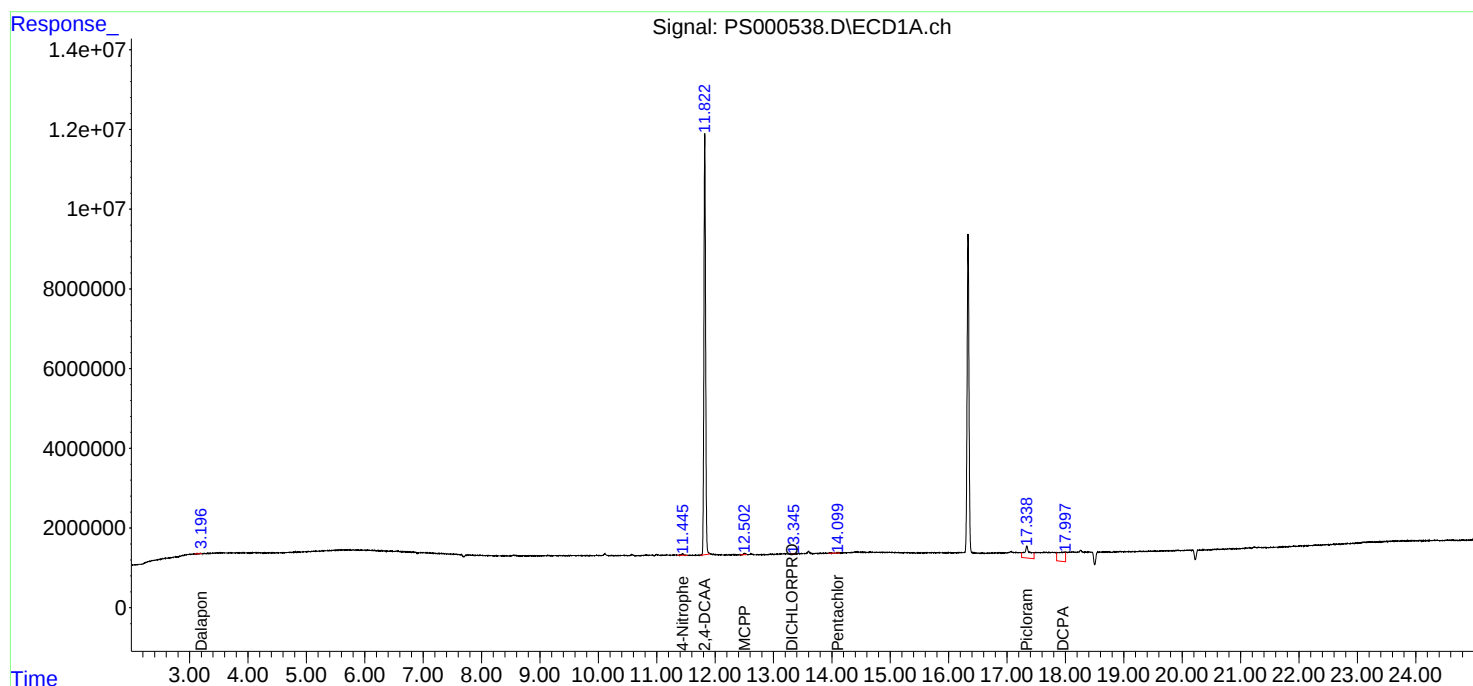


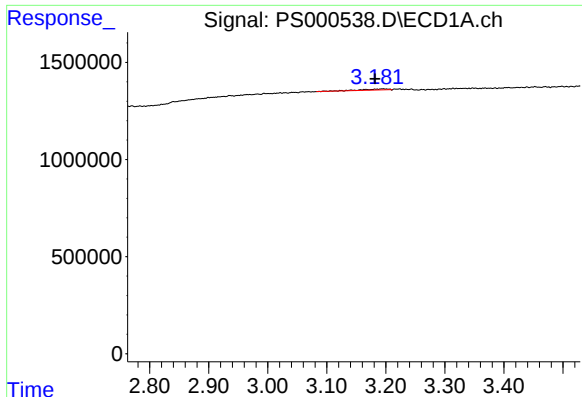

#1 Dalapon


R.T.: 3.195 min
Delta R.T.: 0.013 min
Response: 167793
Conc: 0.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

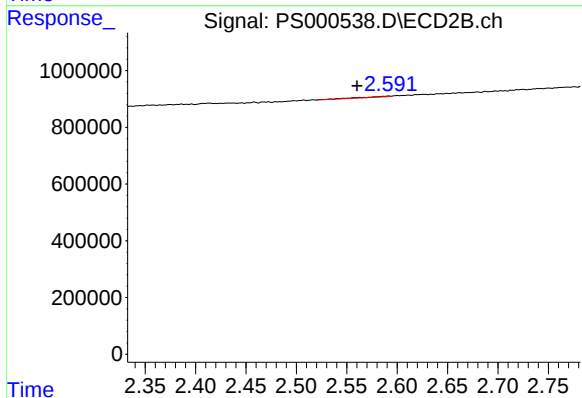


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: 0.031 min
Response: 63784
Conc: 0.15 ng/ml

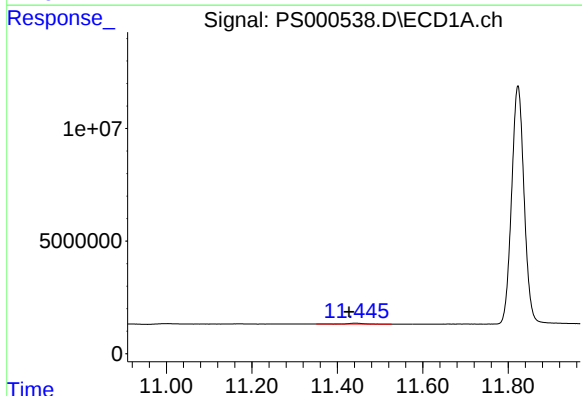


#3 4-Nitrophenol

R.T.: 11.442 min
Delta R.T.: 0.015 min
Response: 889319
Conc: 3.78 ng/ml

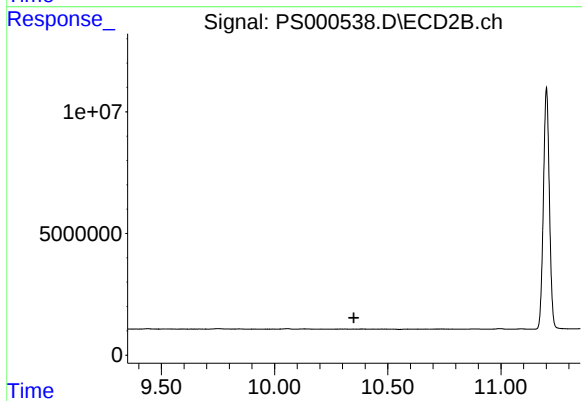

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.350 min
Response: 0
Conc: N.D.

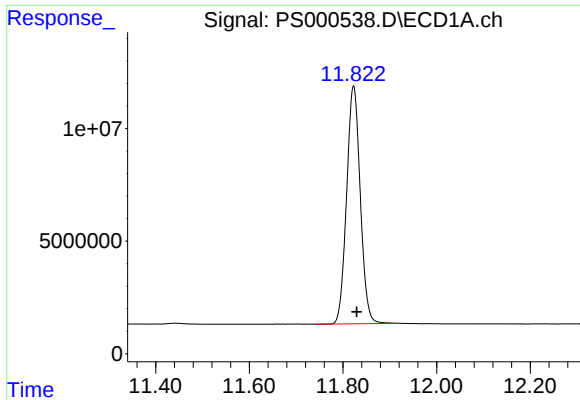

#4 2,4-DCAA


R.T.: 11.823 min
Delta R.T.: -0.007 min
Response: 213790125
Conc: 567.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

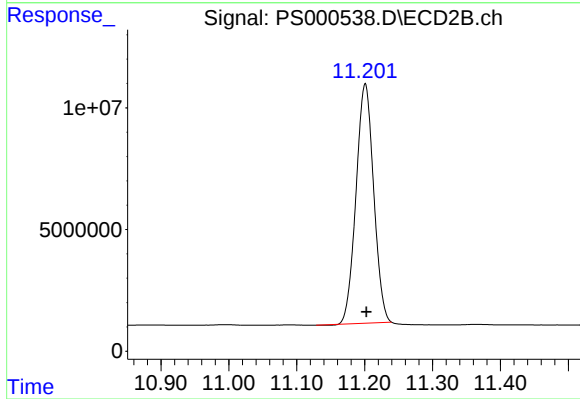


#4 2,4-DCAA

R.T.: 11.201 min
Delta R.T.: -0.002 min
Response: 177241007
Conc: 520.82 ng/ml

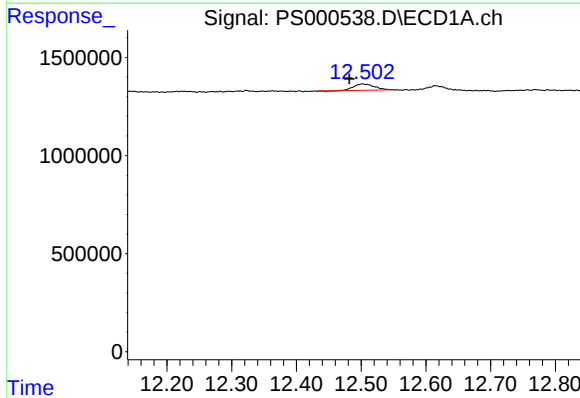


#6 MCP

R.T.: 12.504 min
Delta R.T.: 0.022 min
Response: 751030
Conc: 0.66 ug/ml

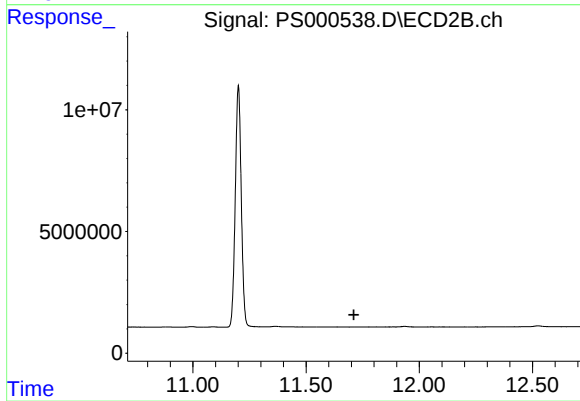

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.711 min
Response: 0
Conc: N.D.

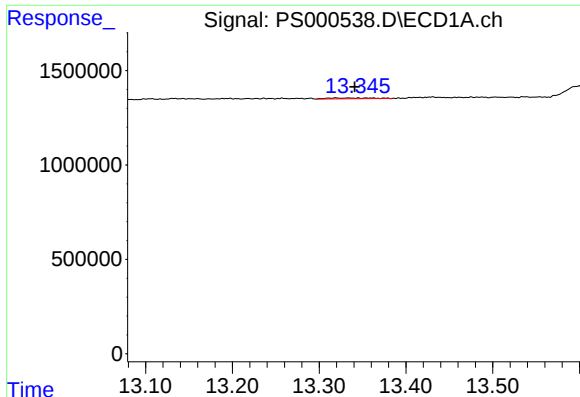

#8 DICHLORPROP


R.T.: 13.320 min
Delta R.T.: -0.021 min
Response: 148918
Conc: 0.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

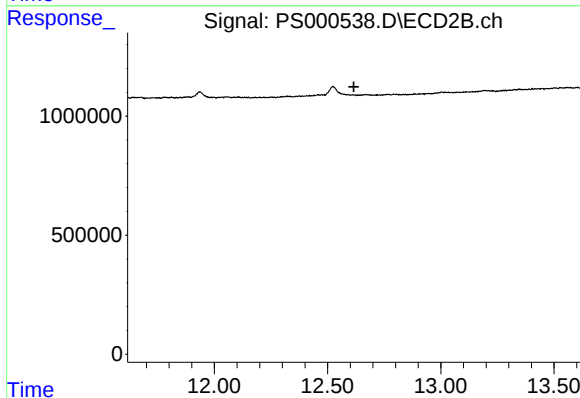


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.616 min
Response: 0
Conc: N.D.

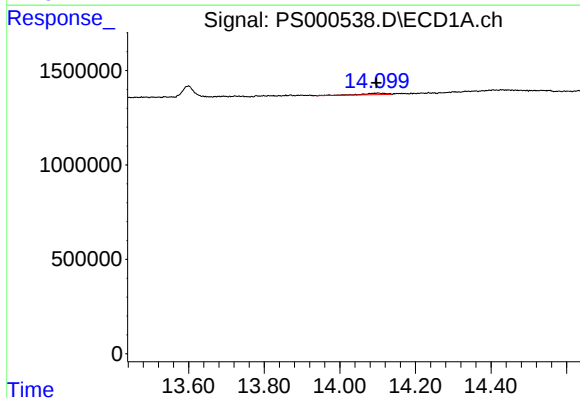


#10 Pentachlorophenol

R.T.: 14.099 min
Delta R.T.: 0.002 min
Response: 314131
Conc: 0.06 ng/ml

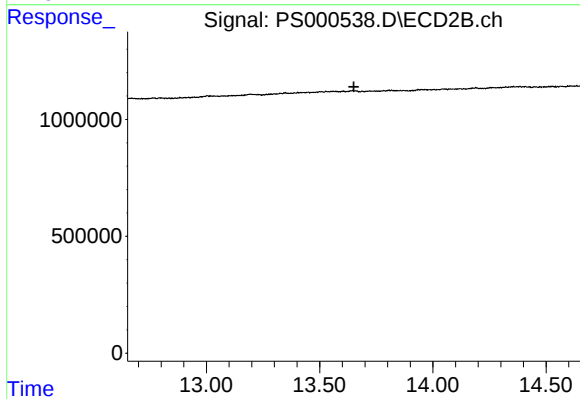

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.651 min
Response: 0
Conc: N.D.

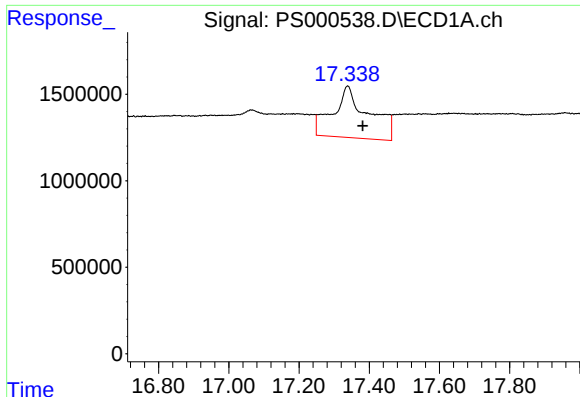

#15 Picloram


R.T.: 17.338 min
Delta R.T.: -0.044 min
Response: 20971254
Conc: 7.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

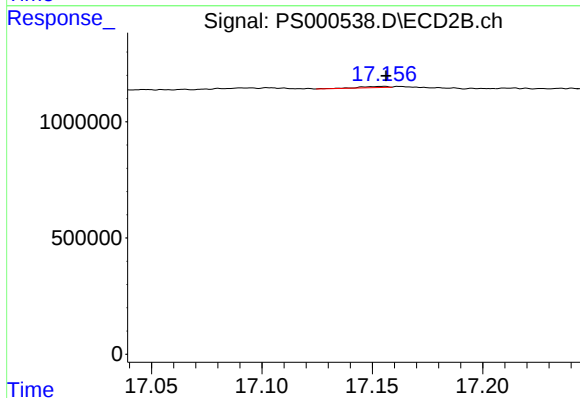


#15 Picloram

R.T.: 17.156 min
Delta R.T.: 0.000 min
Response: 42752
Conc: 0.02 ng/ml

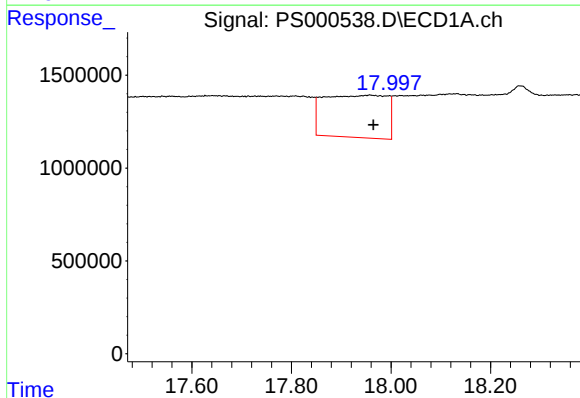

#16 DCPA

R.T.: 17.957 min
Delta R.T.: -0.007 min
Response: 20103910
Conc: 7.85 ng/ml

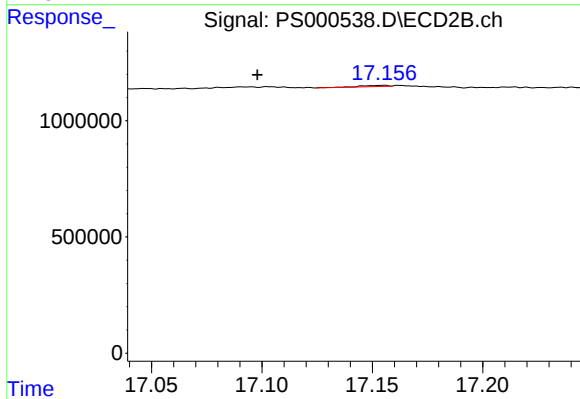

#16 DCPA

R.T.: 17.156 min
Delta R.T.: 0.058 min
Response: 42752
Conc: 0.02 ng/ml