

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062118\
 Data File : PS000550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 03:33
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 04:14:47 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.804	11.182	213.7E6	181.4E6	567.389	532.945
Target Compounds							
3) T	4-Nitroph...	11.424	0.000	1134181	0	4.825	N.D. #
6) T	MCP	12.485	0.000	1133481	0	1.001	N.D. #
11) T	2,4,5-TP ...	14.936	0.000	390383	0	0.180	N.D. #
15) T	Picloram	17.320	17.132	2251196	31541	0.771	0.013 #
16) T	DCPA	0.000	17.132	0	31541	N.D.	0.014 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062118\
Data File : PS000550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 03:33
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 04:14:47 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

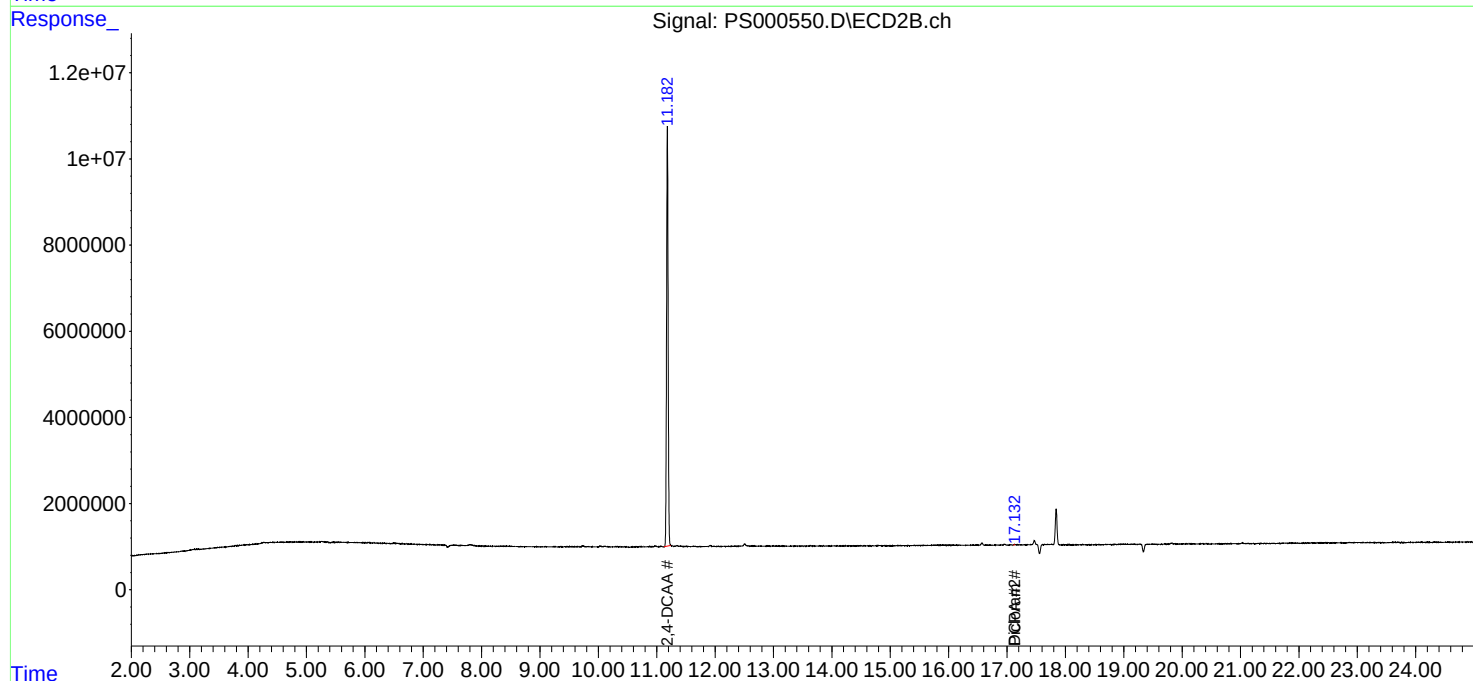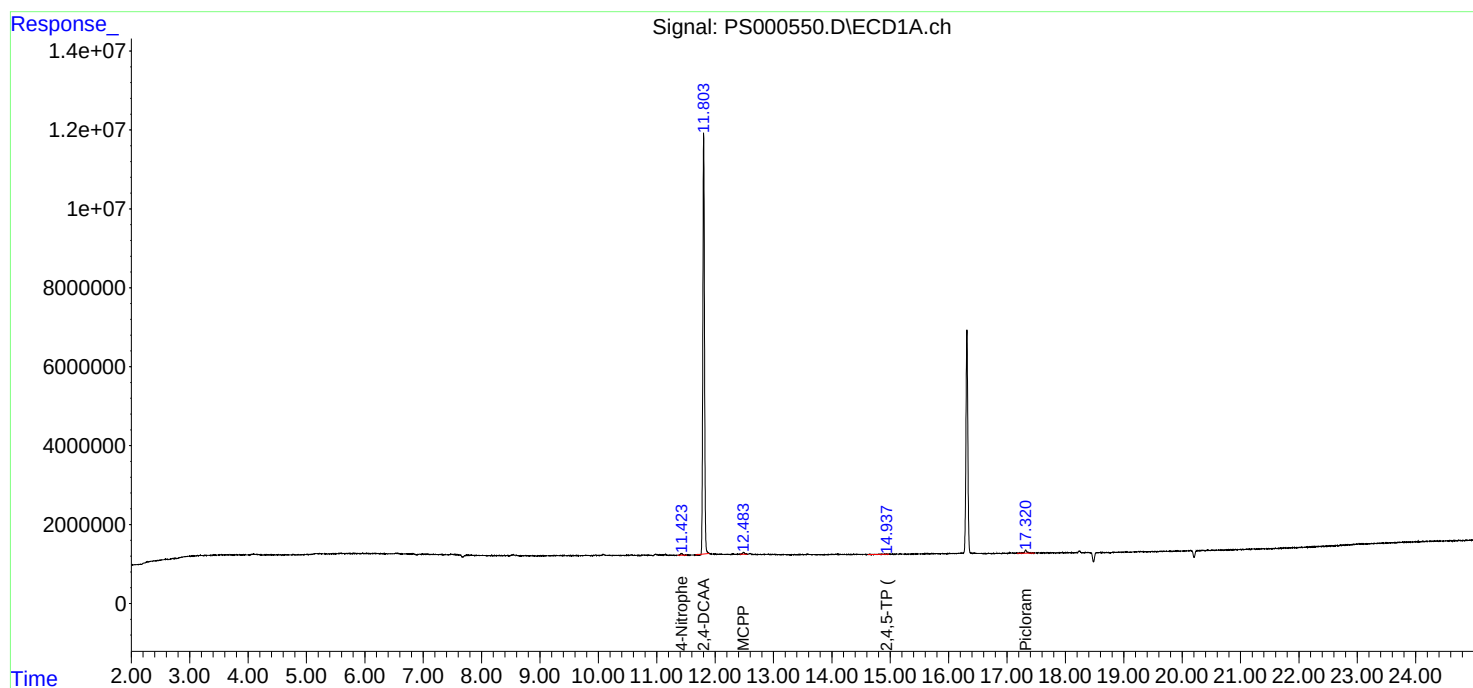


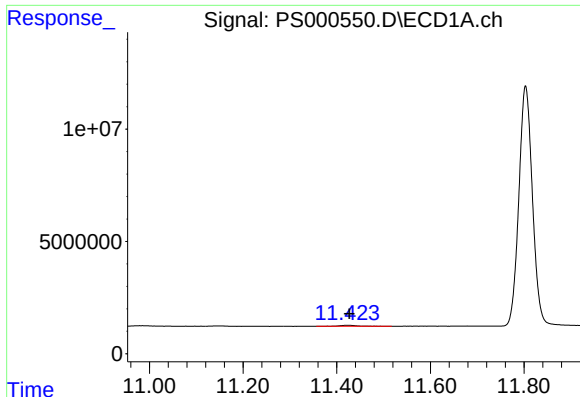

#3 4-Nitrophenol


R.T.: 11.424 min
Delta R.T.: -0.004 min
Response: 1134181
Conc: 4.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

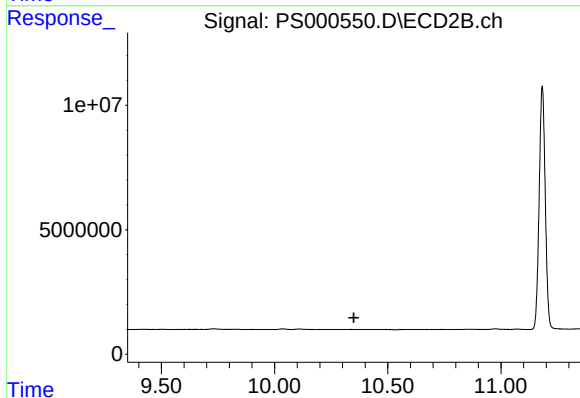


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.350 min
Response: 0
Conc: N.D.

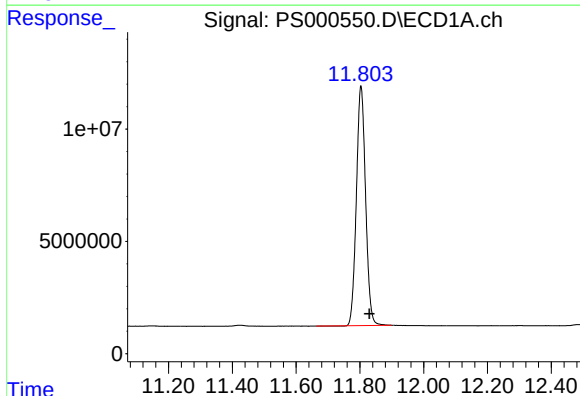


#4 2,4-DCAA

R.T.: 11.804 min
Delta R.T.: -0.026 min
Response: 213709804
Conc: 567.39 ng/ml

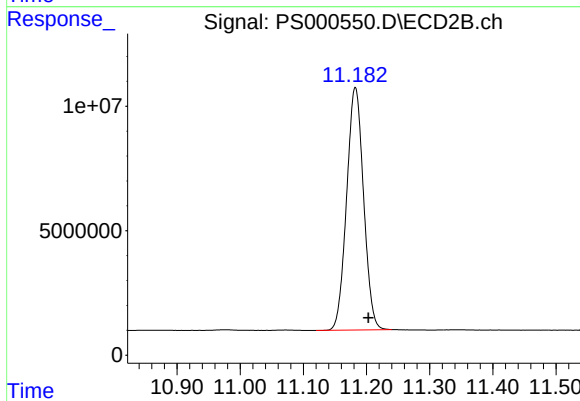

#4 2,4-DCAA


R.T.: 11.182 min
Delta R.T.: -0.021 min
Response: 181366061
Conc: 532.95 ng/ml

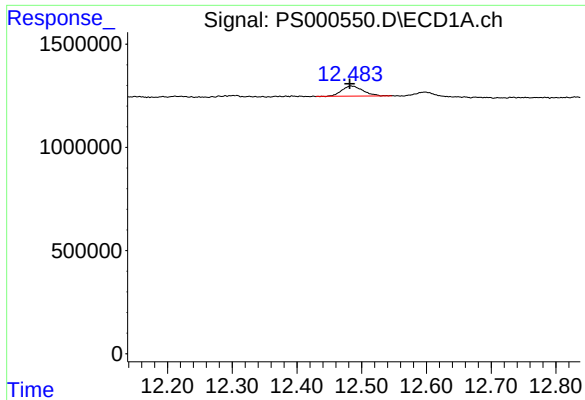

#6 MCP


R.T.: 12.485 min
Delta R.T.: 0.003 min
Response: 1133481
Conc: 1.00 ug/ml

Instrument :
ECD_S
ClientSampleId :

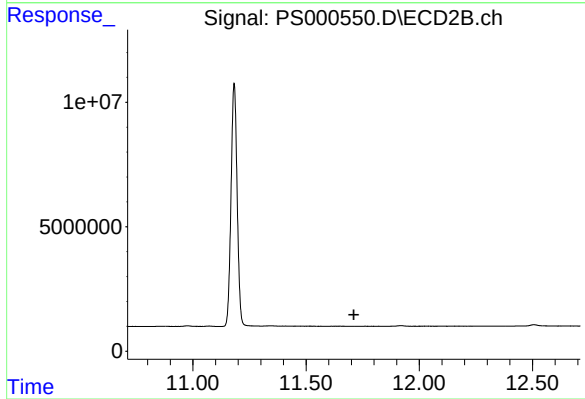


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

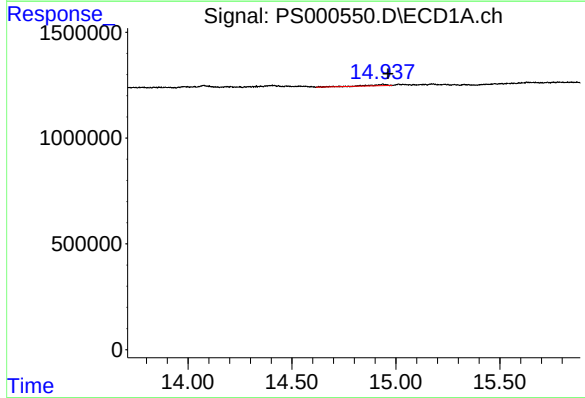


#11 2,4,5-TP (SILVEX)

R.T.: 14.936 min
Delta R.T.: -0.026 min
Response: 390383
Conc: 0.18 ng/ml

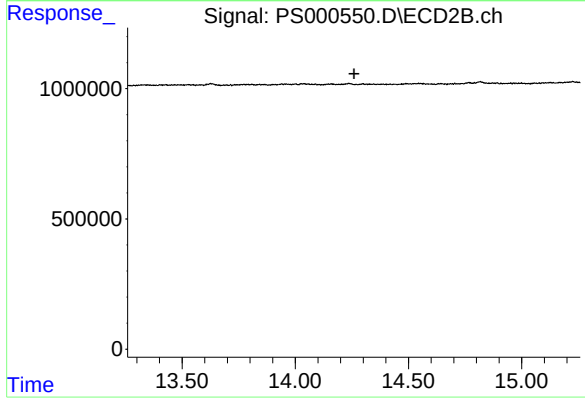

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.259 min
Response: 0
Conc: N.D.

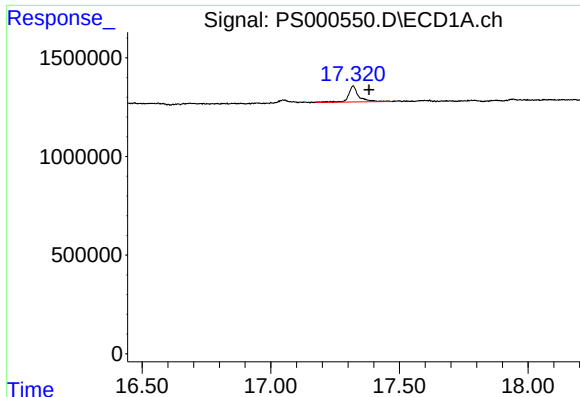

#15 Picloram


R.T.: 17.320 min
Delta R.T.: -0.062 min
Response: 2251196
Conc: 0.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

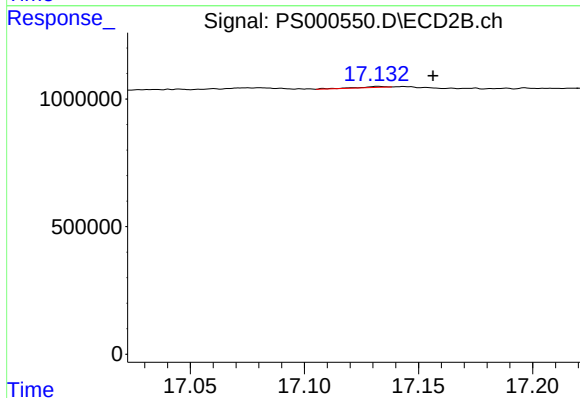


#15 Picloram

R.T.: 17.132 min
Delta R.T.: -0.024 min
Response: 31541
Conc: 0.01 ng/ml

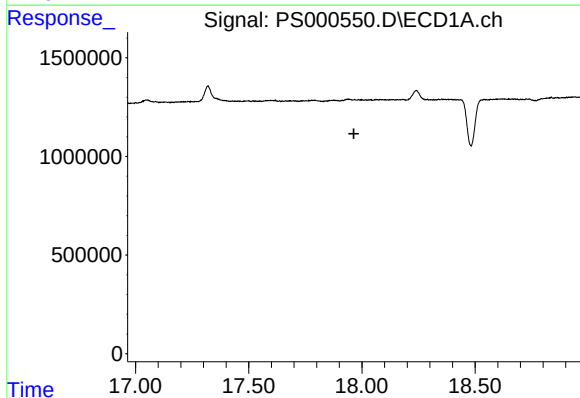

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.964 min
Response: 0
Conc: N.D.

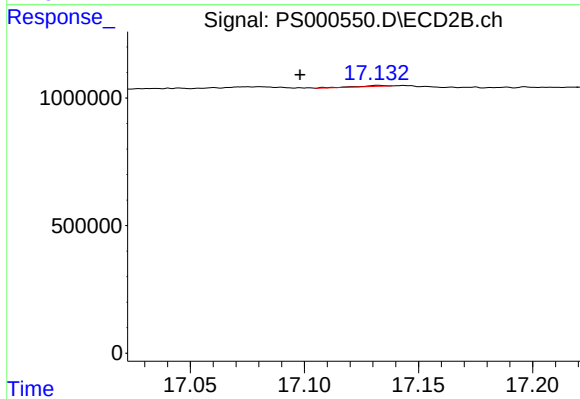

#16 DCPA

R.T.: 17.132 min
Delta R.T.: 0.034 min
Response: 31541
Conc: 0.01 ng/ml