

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062118\
 Data File : PS000559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 08:11
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 11:39:06 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.804	11.183	218.9E6	185.9E6	581.069	546.182
Target Compounds							
1) T	Dalapon	0.000	2.581	0	44802	N.D.	0.103 #
3) T	4-Nitroph...	11.424	0.000	1107968	0	4.713	N.D. #
6) T	MCP	12.486	0.000	1076201	0	0.950	N.D. #
10) T	Pentachlo...	14.072	13.629	871600	500080	0.166	0.106 #
11) T	2,4,5-TP ...	14.938	14.237	408079	229968	0.188	0.118 #
12) T	2,4,5-T	0.000	14.774	0	147352	N.D.	0.087 #
14) T	DINOSEB	17.598	0.000	6235875	0	4.188	N.D. #
15) T	Picloram	17.319	17.136	8339424	306481	2.855	0.123 #
16) T	DCPA	17.939	17.083	24510140	242974	9.565	0.105 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062118\
Data File : PS000559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 08:11
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 11:39:06 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

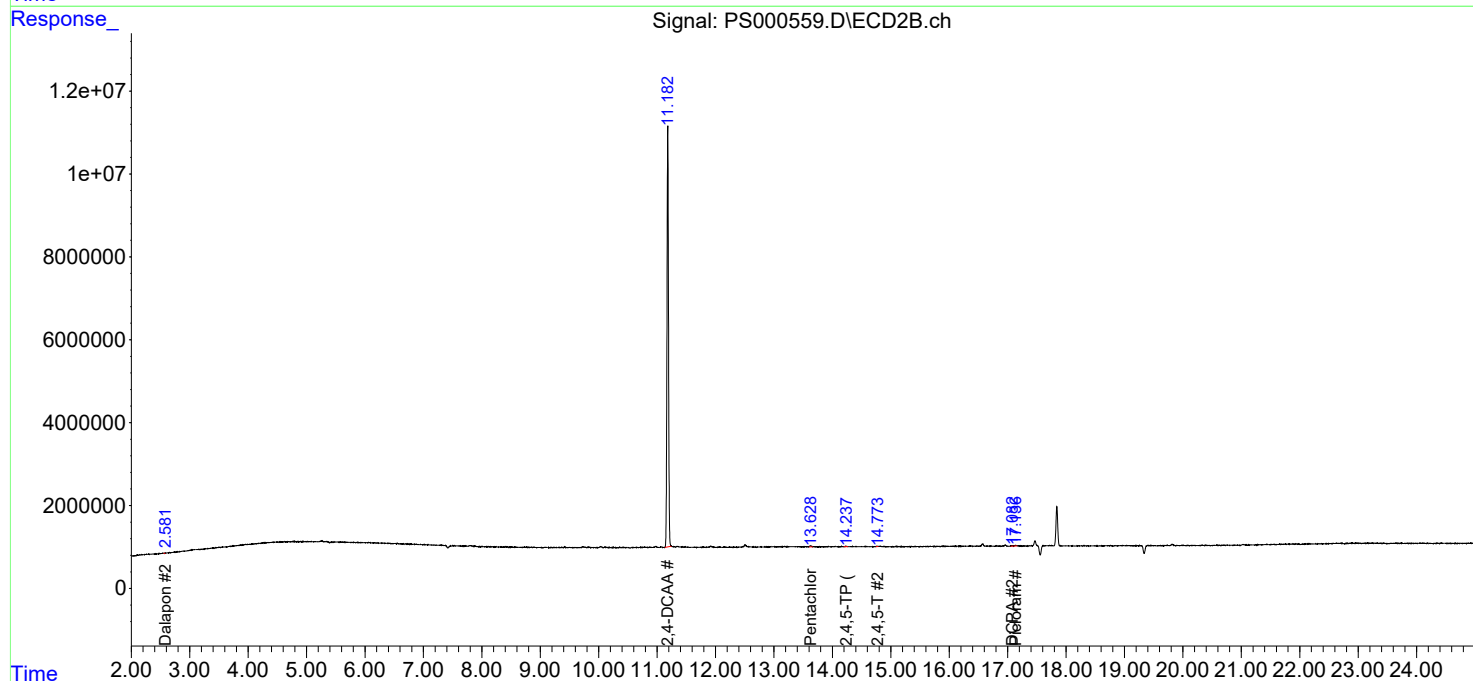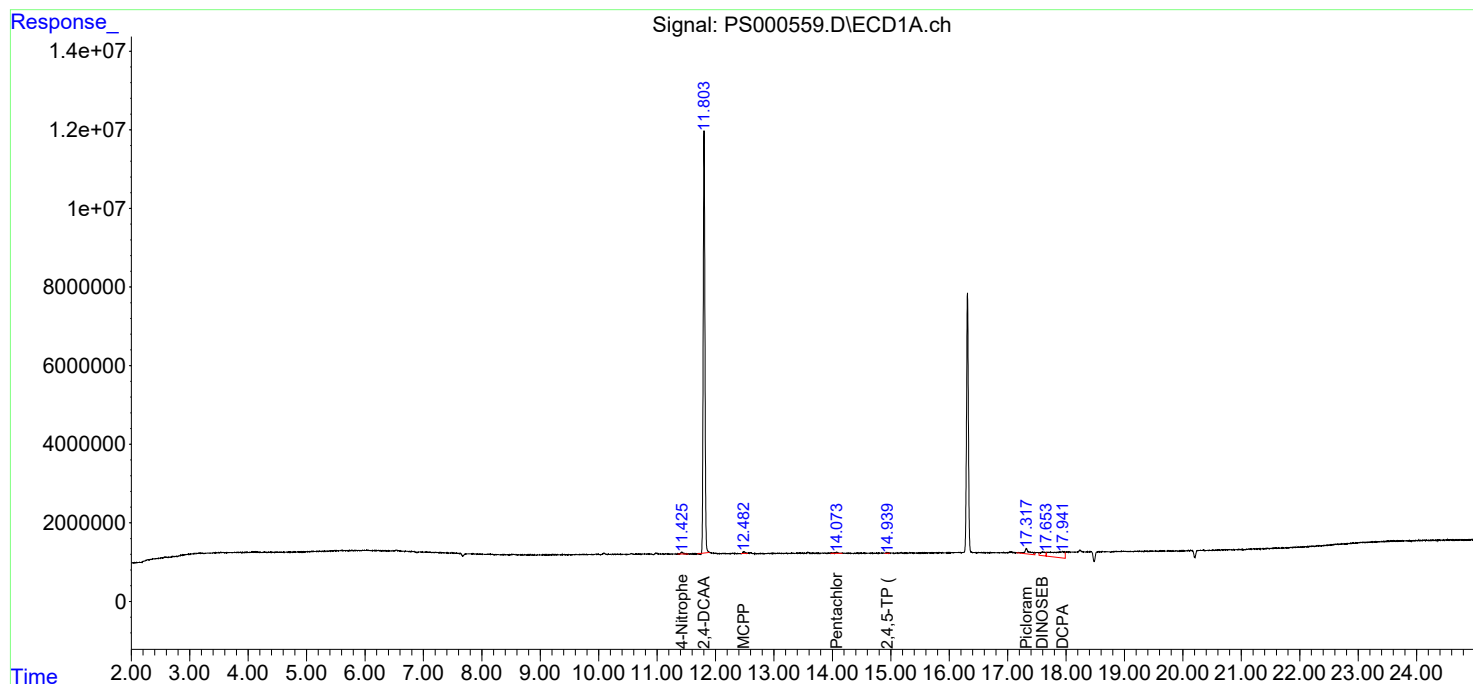


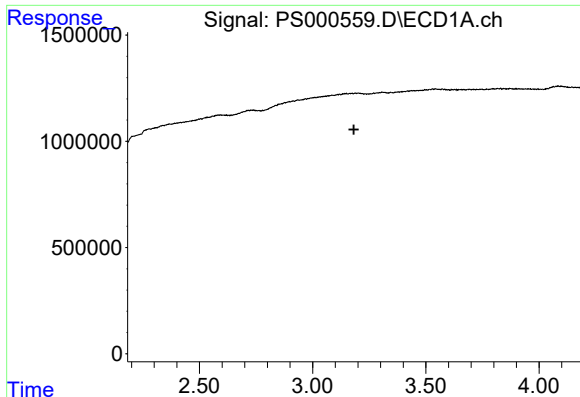

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

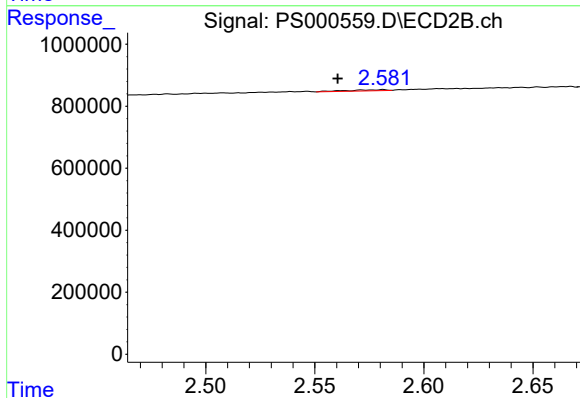


#1 Dalapon

R.T.: 2.581 min
Delta R.T.: 0.021 min
Response: 44802
Conc: 0.10 ng/ml

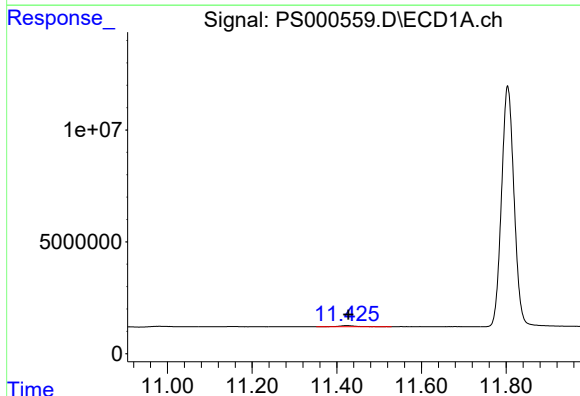


#3 4-Nitrophenol

R.T.: 11.424 min
Delta R.T.: -0.004 min
Response: 1107968
Conc: 4.71 ng/ml

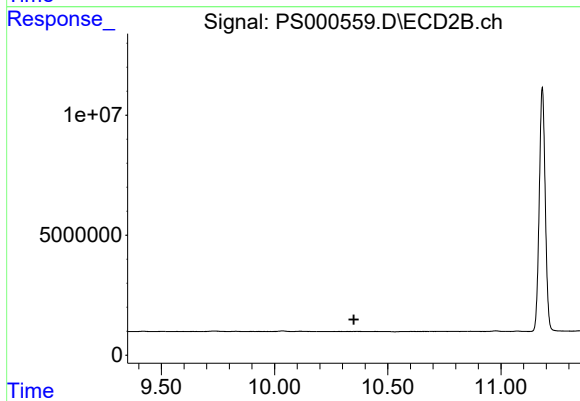

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

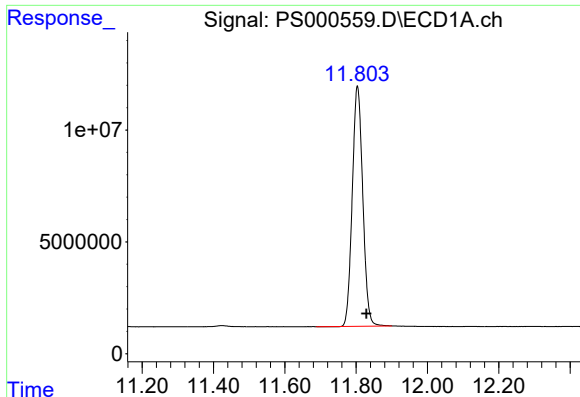

#4 2,4-DCAA


R.T.: 11.804 min
Delta R.T.: -0.025 min
Response: 218862327
Conc: 581.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

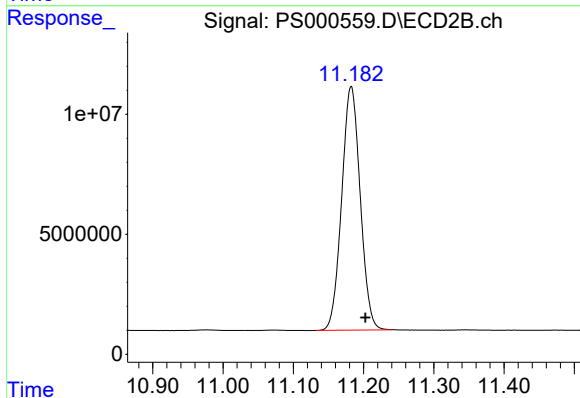


#4 2,4-DCAA

R.T.: 11.183 min
Delta R.T.: -0.020 min
Response: 185870703
Conc: 546.18 ng/ml

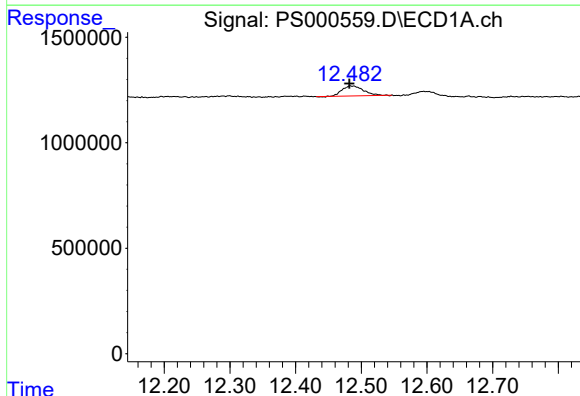


#6 MCP

R.T.: 12.486 min
Delta R.T.: 0.004 min
Response: 1076201
Conc: 0.95 ug/ml

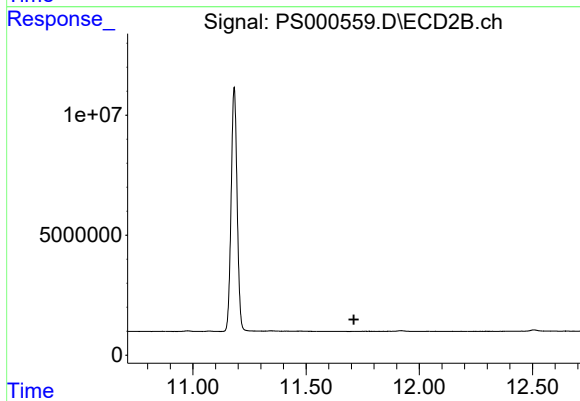

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

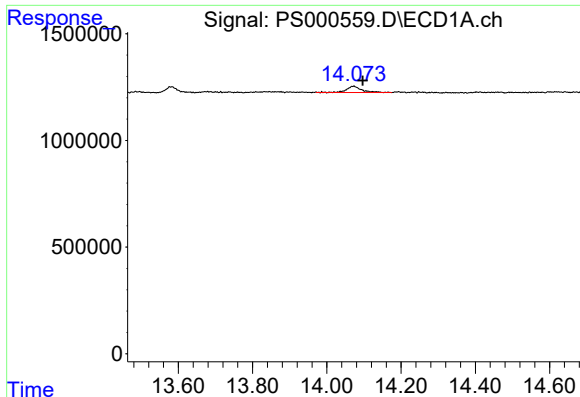

#10 Pentachlorophenol


R.T.: 14.072 min
Delta R.T.: -0.025 min
Response: 871600
Conc: 0.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

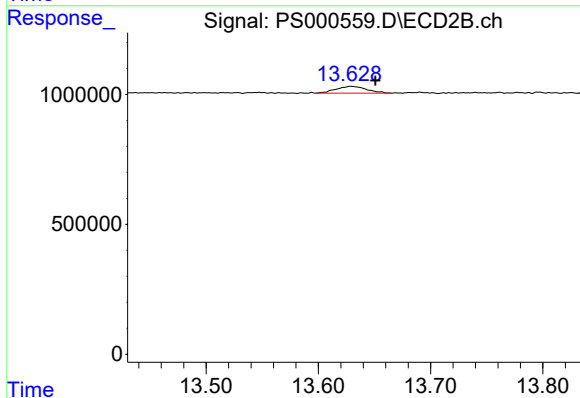


#10 Pentachlorophenol

R.T.: 13.629 min
Delta R.T.: -0.022 min
Response: 500080
Conc: 0.11 ng/ml

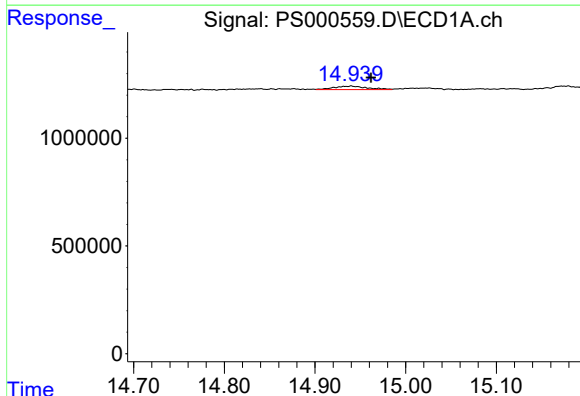


#11 2,4,5-TP (SILVEX)

R.T.: 14.938 min
Delta R.T.: -0.024 min
Response: 408079
Conc: 0.19 ng/ml

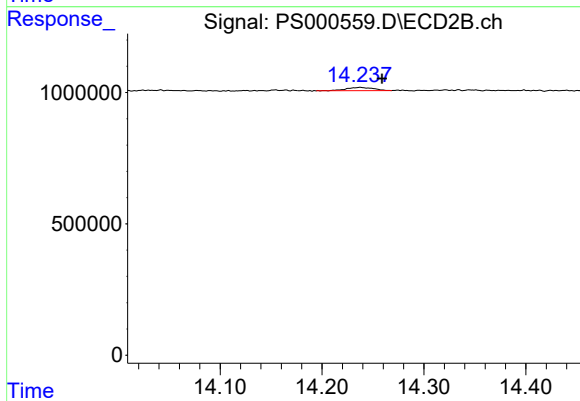

#11 2,4,5-TP (SILVEX)


R.T.: 14.237 min
Delta R.T.: -0.022 min
Response: 229968
Conc: 0.12 ng/ml

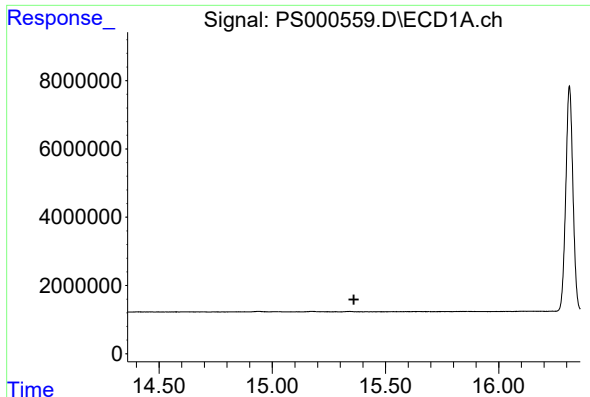

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.360 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

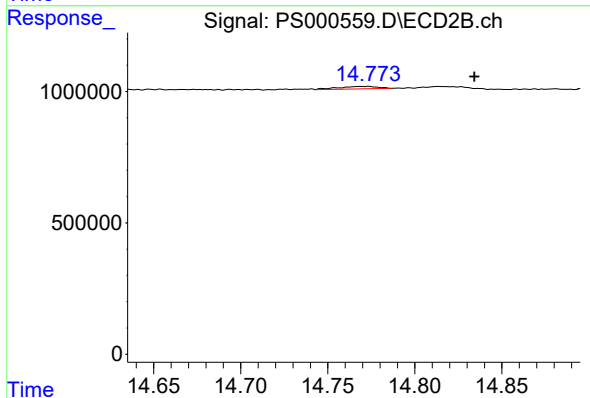


#12 2,4,5-T

R.T.: 14.774 min
Delta R.T.: -0.061 min
Response: 147352
Conc: 0.09 ng/ml

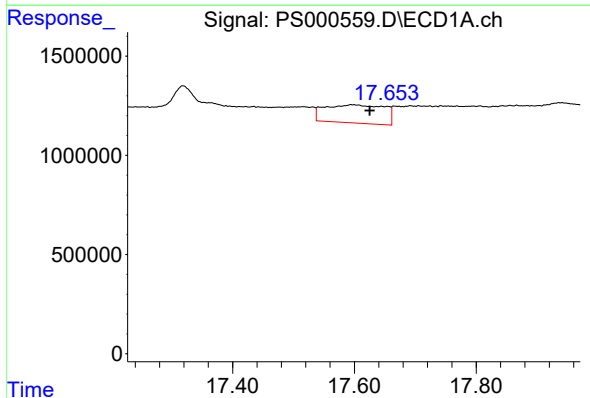


#14 DINOSEB

R.T.: 17.598 min
Delta R.T.: -0.027 min
Response: 6235875
Conc: 4.19 ng/ml

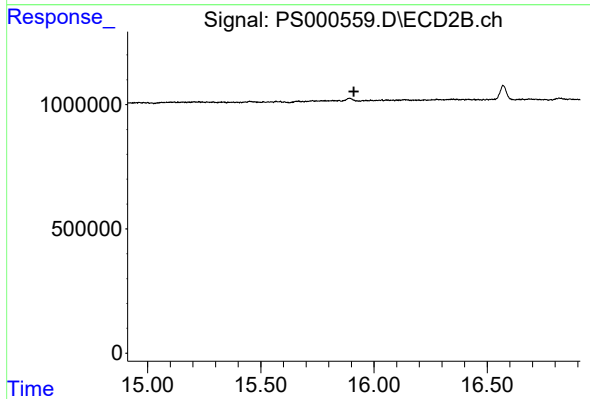

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 15.911 min
Response: 0
Conc: N.D.

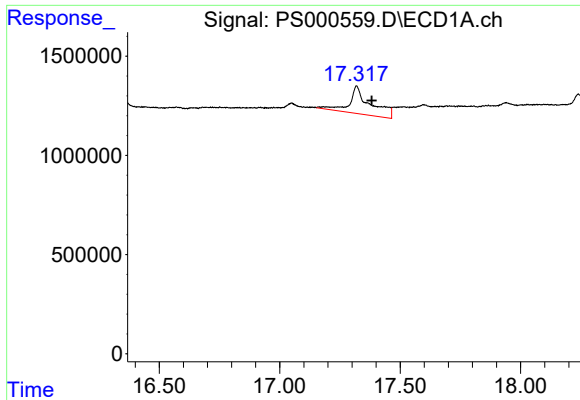

#15 Picloram


R.T.: 17.319 min
Delta R.T.: -0.063 min
Response: 8339424
Conc: 2.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

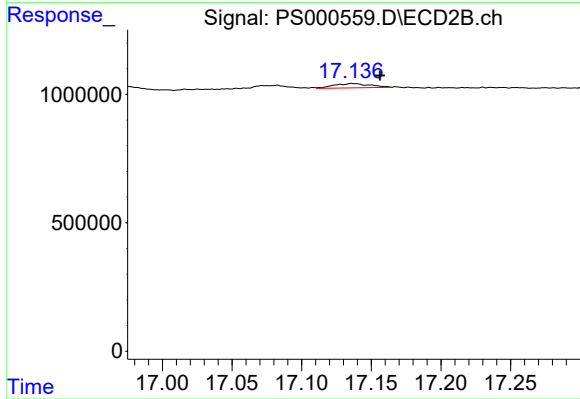


#15 Picloram

R.T.: 17.136 min
Delta R.T.: -0.020 min
Response: 306481
Conc: 0.12 ng/ml

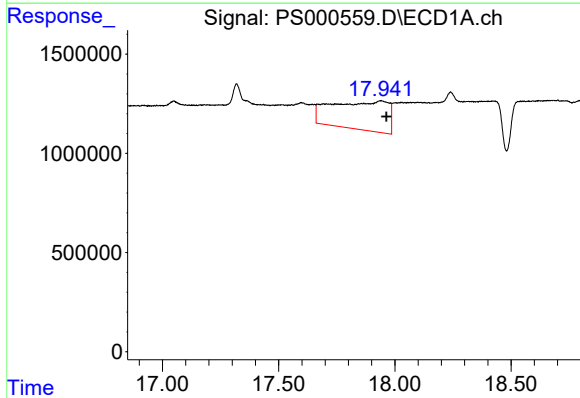

#16 DCPA

R.T.: 17.939 min
Delta R.T.: -0.025 min
Response: 24510140
Conc: 9.57 ng/ml

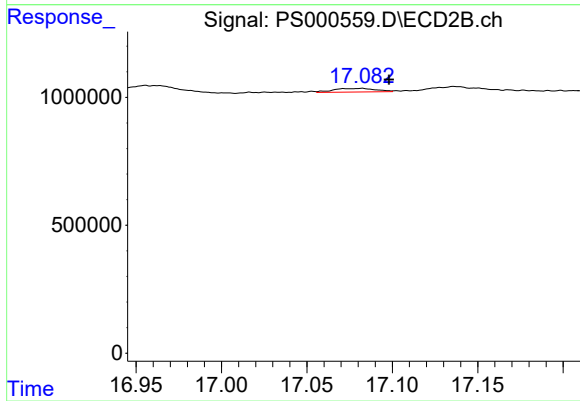

#16 DCPA

R.T.: 17.083 min
Delta R.T.: -0.015 min
Response: 242974
Conc: 0.11 ng/ml