

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062121\
 Data File : PS015891.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 08:18
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 12:10:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.443	0.000	148.8E6	0	66.304	N.D. #
5) T	DICAMBA	0.000	6.987f	0	50643608	N.D.	24.407
6) T	MCCP	0.000	6.987f	0	50643608	N.D.	30.384
9) T	2,4-D	8.365f	0.000	137.8E6	0	78.648	N.D. #
15) T	Picloram	10.981	10.821	38304204	15784496	2.802	3.753 #
16) T	DCPA	0.000	10.821f	0	15784496	N.D.	3.754


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062121\
Data File : PS015891.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 08:18
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 12:10:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

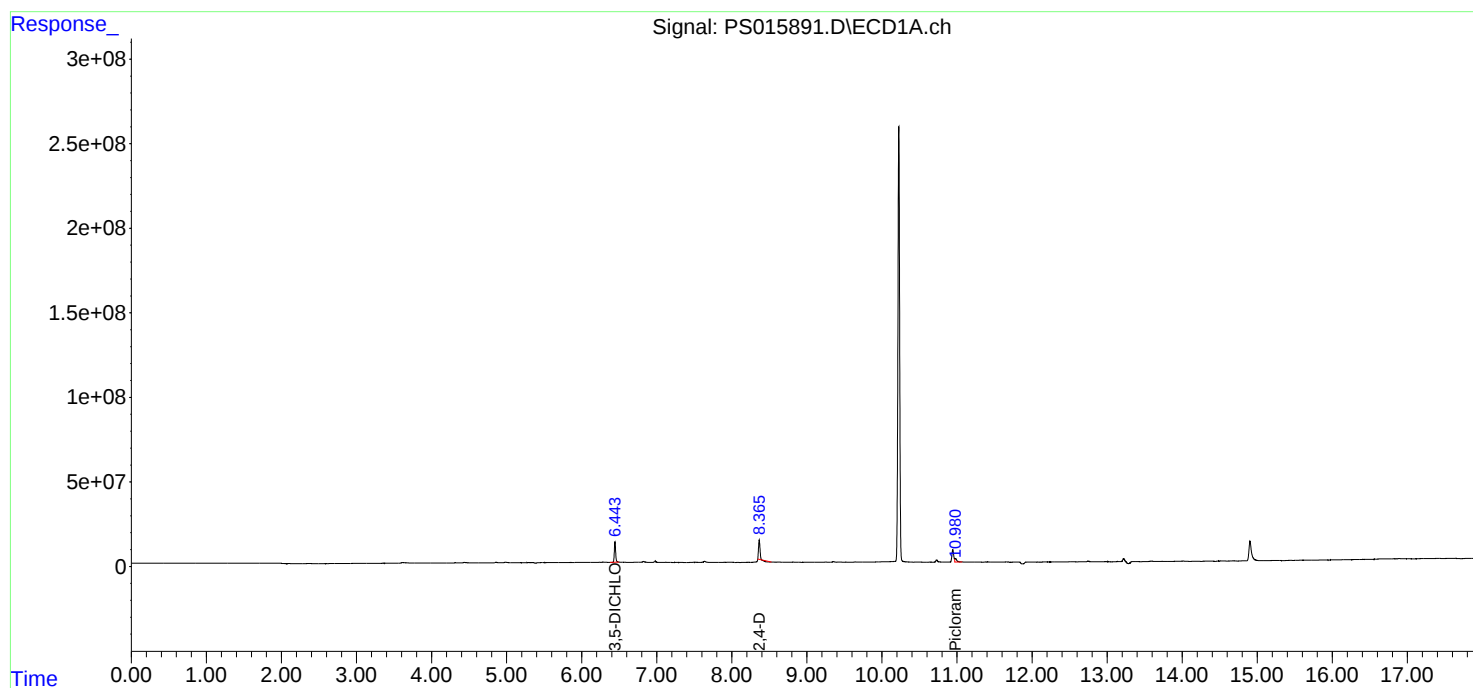


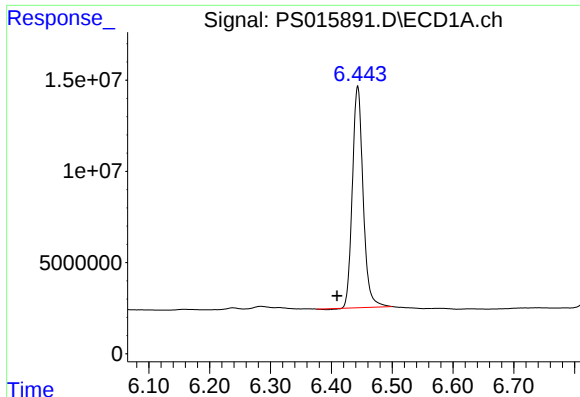

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.443 min
Delta R.T.: 0.034 min
Response: 148814425
Conc: 66.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

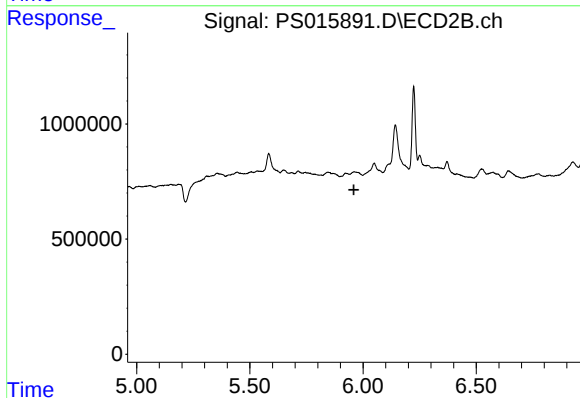


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.960 min
Response: 0
Conc: N.D.

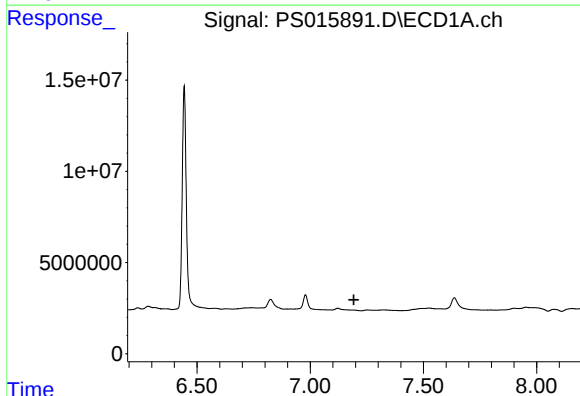


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

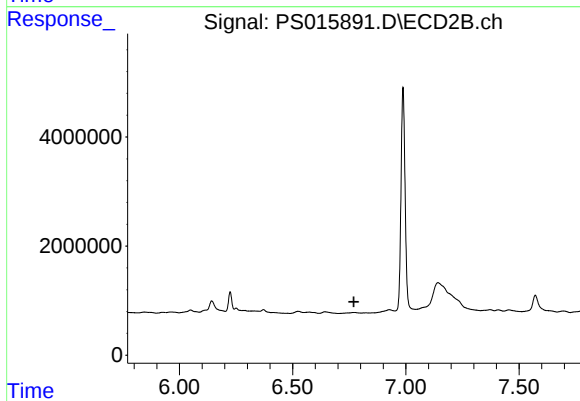

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

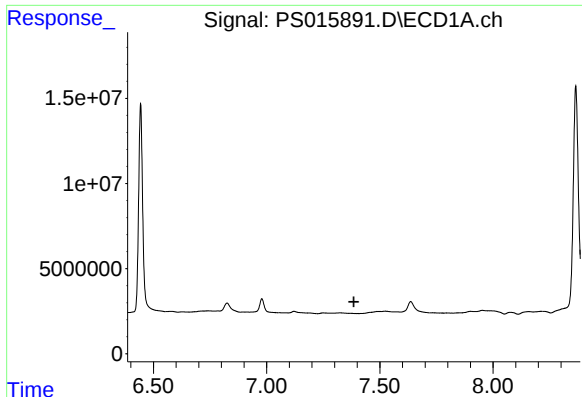

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

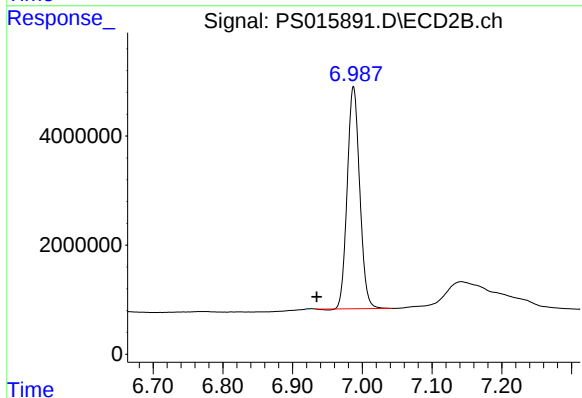


#5 DICAMBA

R.T.: 6.987 min
Delta R.T.: 0.053 min
Response: 50643608
Conc: 24.41 ng/ml

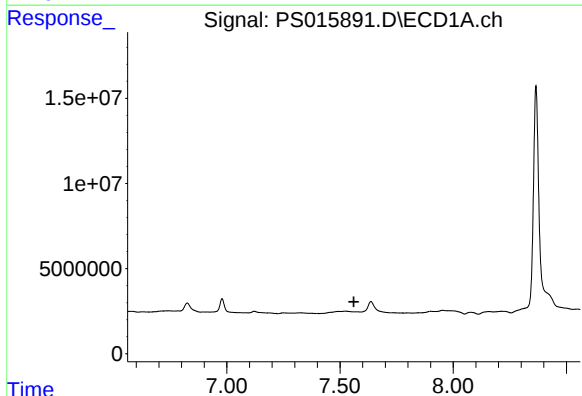


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.561 min
Response: 0
Conc: N.D.

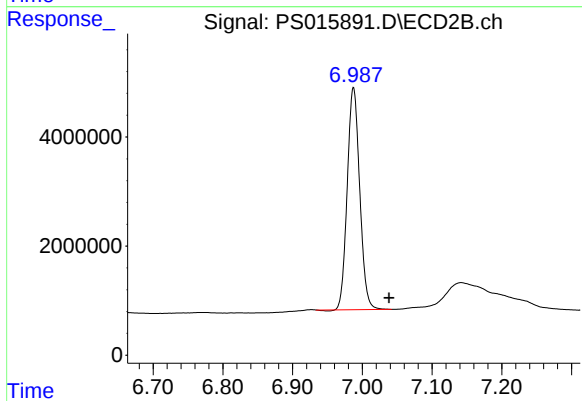

#6 MCP


R.T.: 6.987 min
Delta R.T.: -0.051 min
Response: 50643608
Conc: 30.38 ug/ml

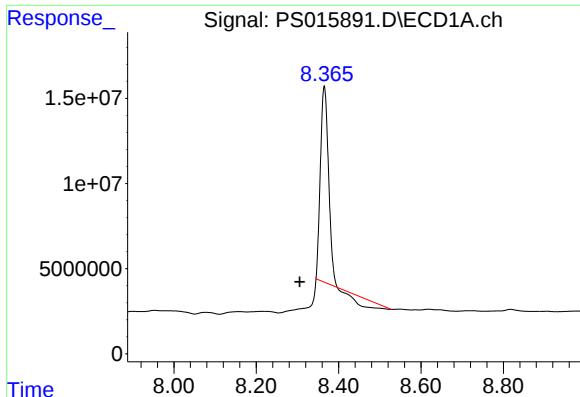

#9 2,4-D


R.T.: 8.365 min
Delta R.T.: 0.060 min
Response: 137835246
Conc: 78.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

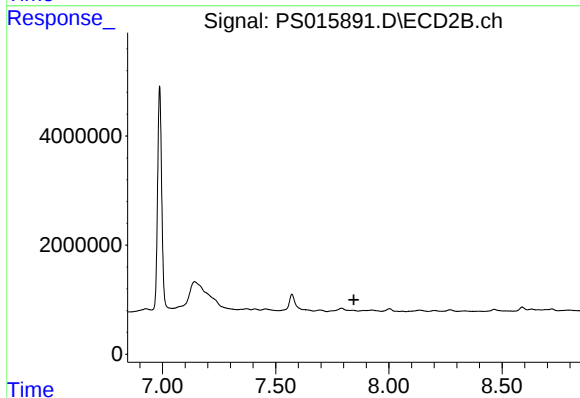


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

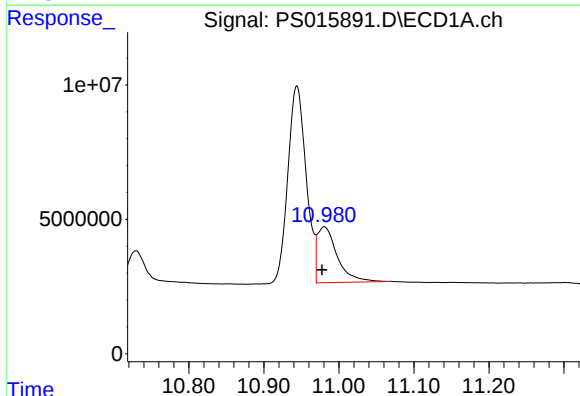


#15 Picloram

R.T.: 10.981 min
Delta R.T.: 0.003 min
Response: 38304204
Conc: 2.80 ng/ml

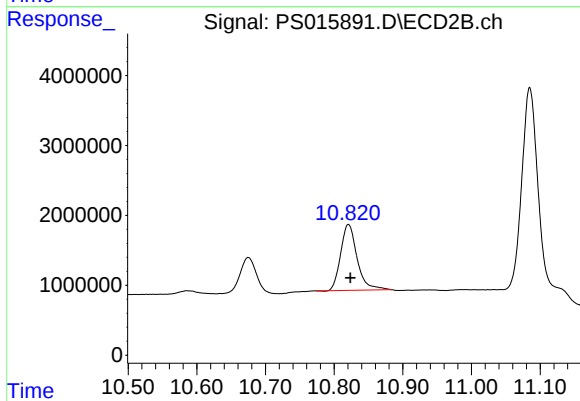

#15 Picloram


R.T.: 10.821 min
Delta R.T.: -0.003 min
Response: 15784496
Conc: 3.75 ng/ml

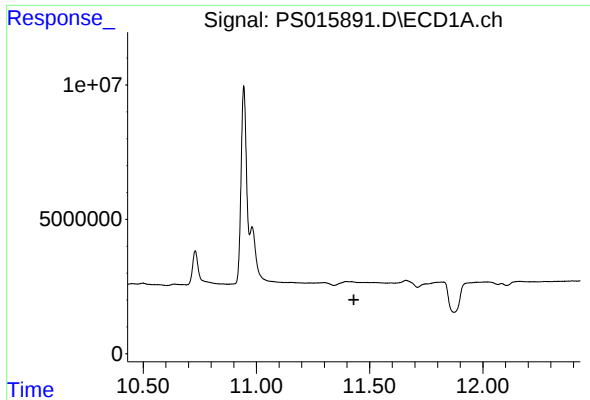

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

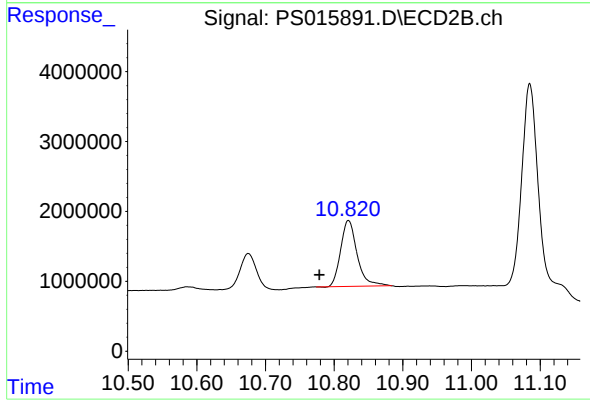

#16 DCPA

R.T.: 10.821 min
Delta R.T.: 0.042 min
Response: 15784496
Conc: 3.75 ng/ml