

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062218\
Data File : PS000591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2018 01:26
Operator : UA
Sample : J3584-20RE
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-1-SRE

Manual Integrations
APPROVED

ugo
6/25/2018 5:09:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:26:31 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	11.798	11.177	81070717	69167039	215.239m	203.248

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062218\
Data File : PS000591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2018 01:26
Operator : UA
Sample : J3584-20RE
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-1-SRE


Manual Integrations
APPROVED

ugo
6/25/2018 5:09:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:26:31 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

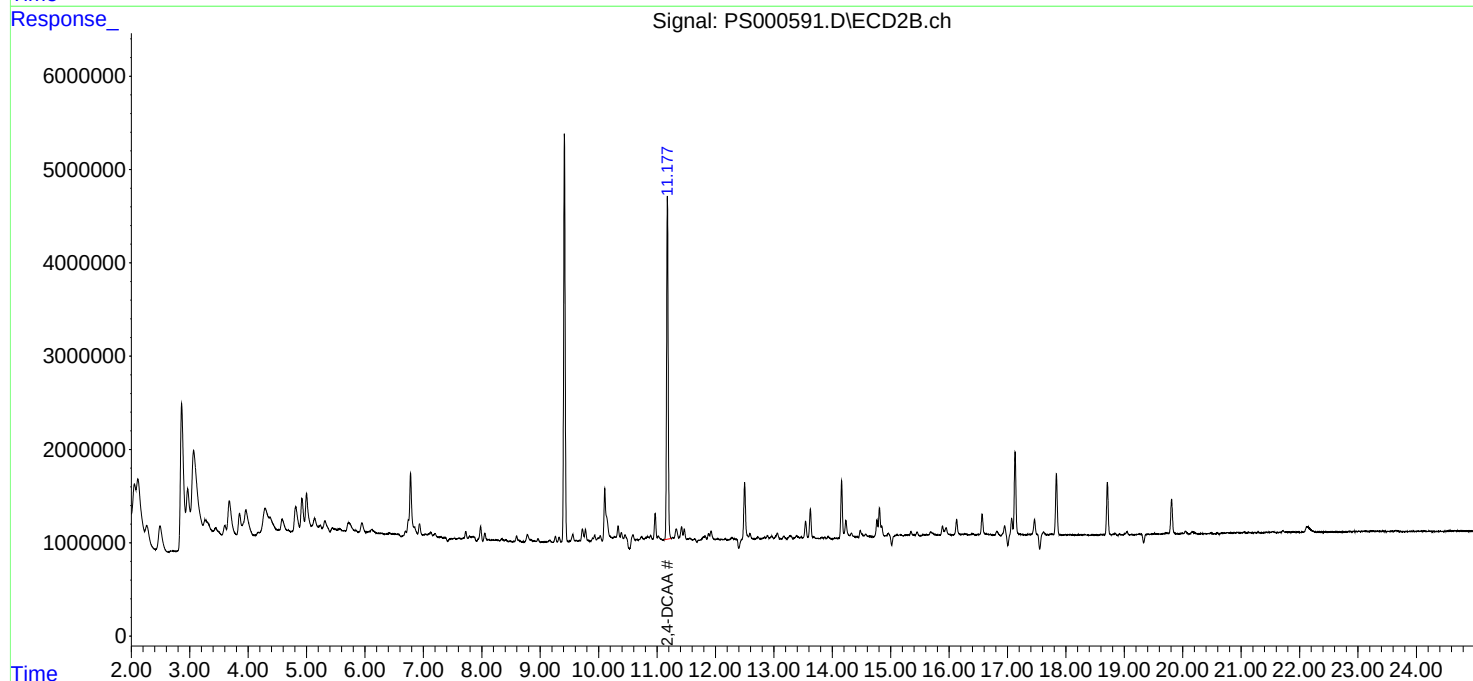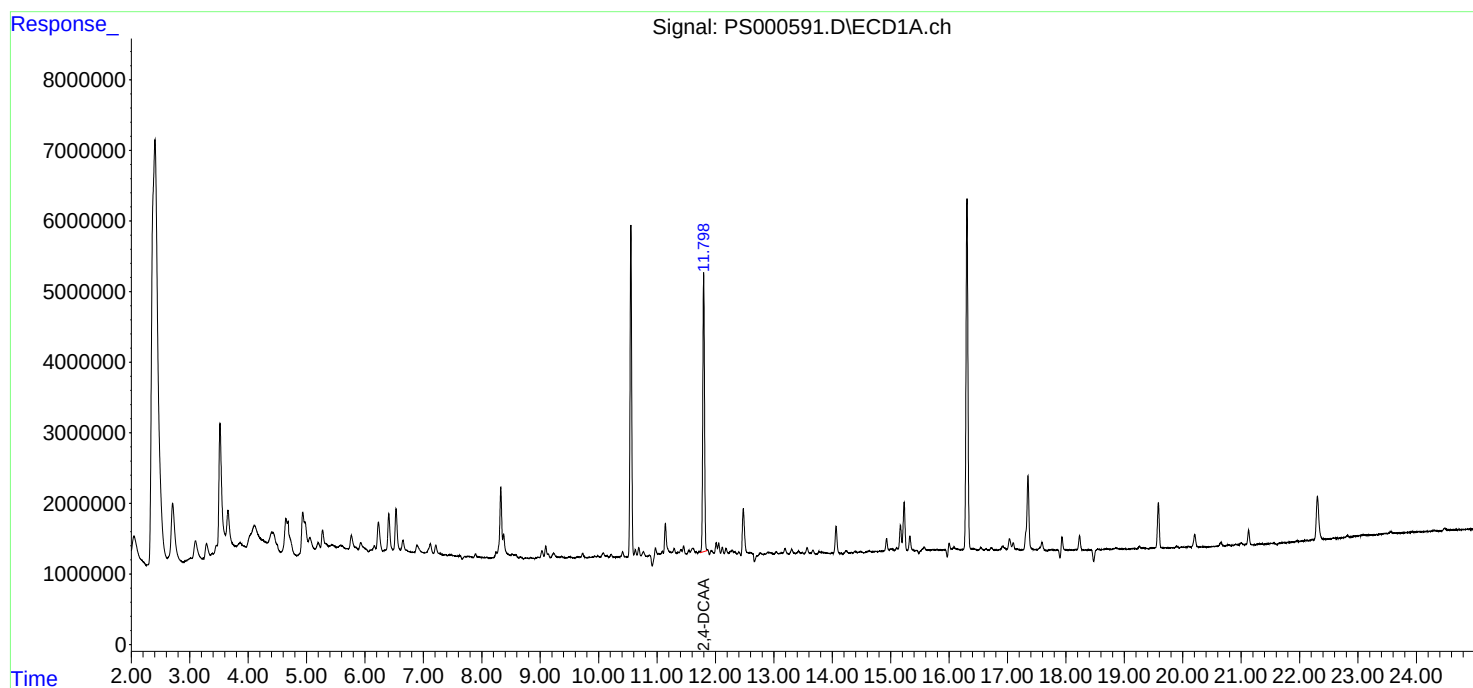

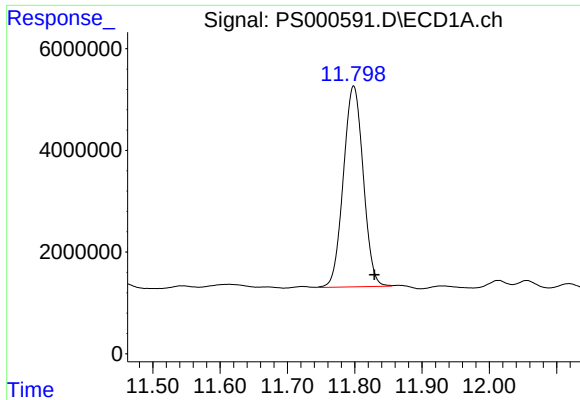


#4 2,4-DCAA

R.T.: 11.798 min
Delta R.T.: -0.031 min
Response: 81070717
Conc: 215.24 ng/ml m

Instrument :
ECD_S
ClientSampleId :
TP-1-SRE

Manual Integrations
APPROVED

ugo
6/25/2018 5:09:30 PM

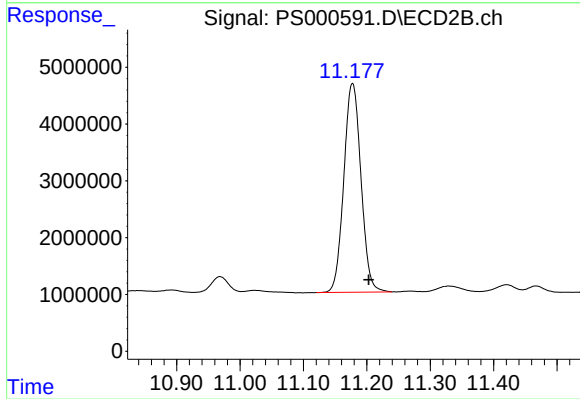

#4 2,4-DCAA

R.T.: 11.177 min
Delta R.T.: -0.025 min
Response: 69167039
Conc: 203.25 ng/ml