

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062221\
 Data File : PS015901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 08:29
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 13:33:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.443	0.000	172.4E6	0	76.815	N.D. #
3) T	4-Nitroph...	6.979f	0.000	3661724	0	4.028	N.D. #
5) T	DICAMBA	0.000	6.987f	0	65876969	N.D.	31.748
6) T	MCP	0.000	6.987f	0	65876969	N.D.	39.523
9) T	2,4-D	8.366f	0.000	179.8E6	0	102.599	N.D. #
15) T	Picloram	10.985	10.824	23661078	8379019	1.731	1.992
16) T	DCPA	0.000	10.824f	0	8379019	N.D.	1.993



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062221\
Data File : PS015901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 08:29
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 13:33:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

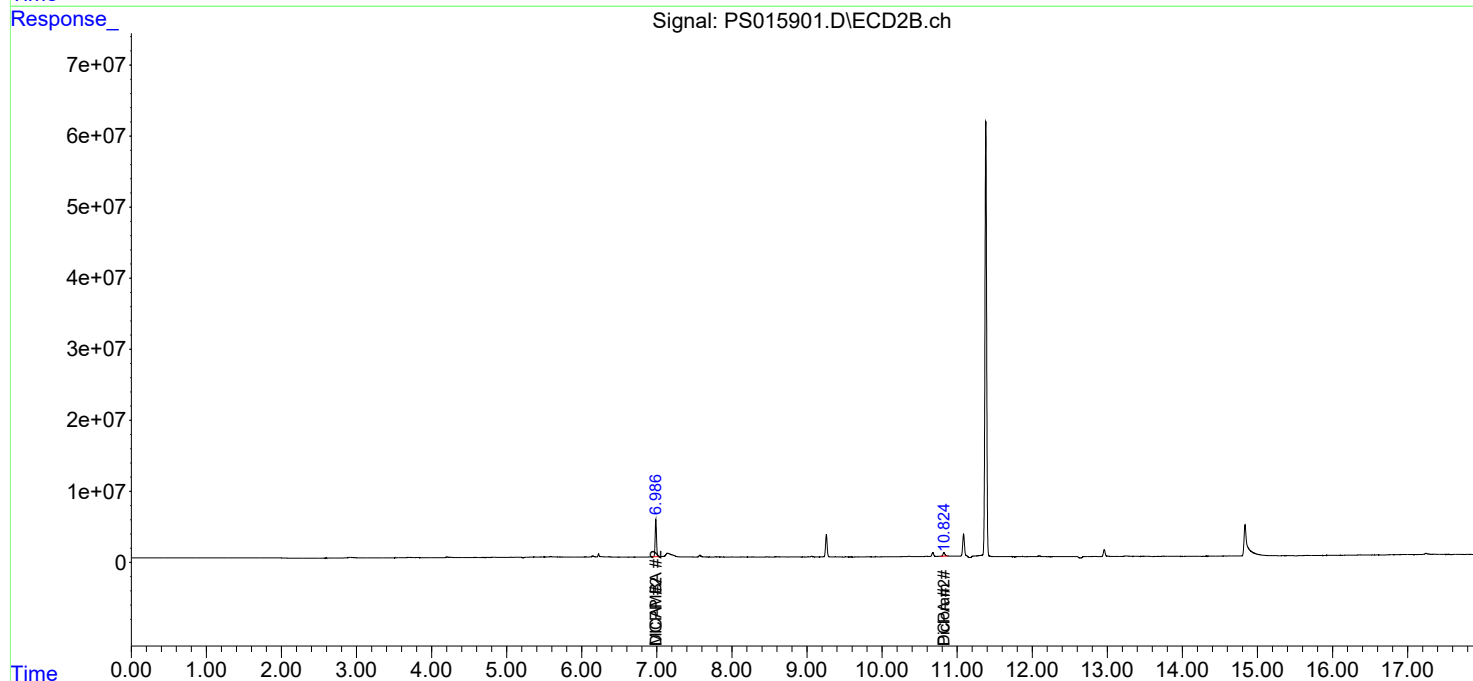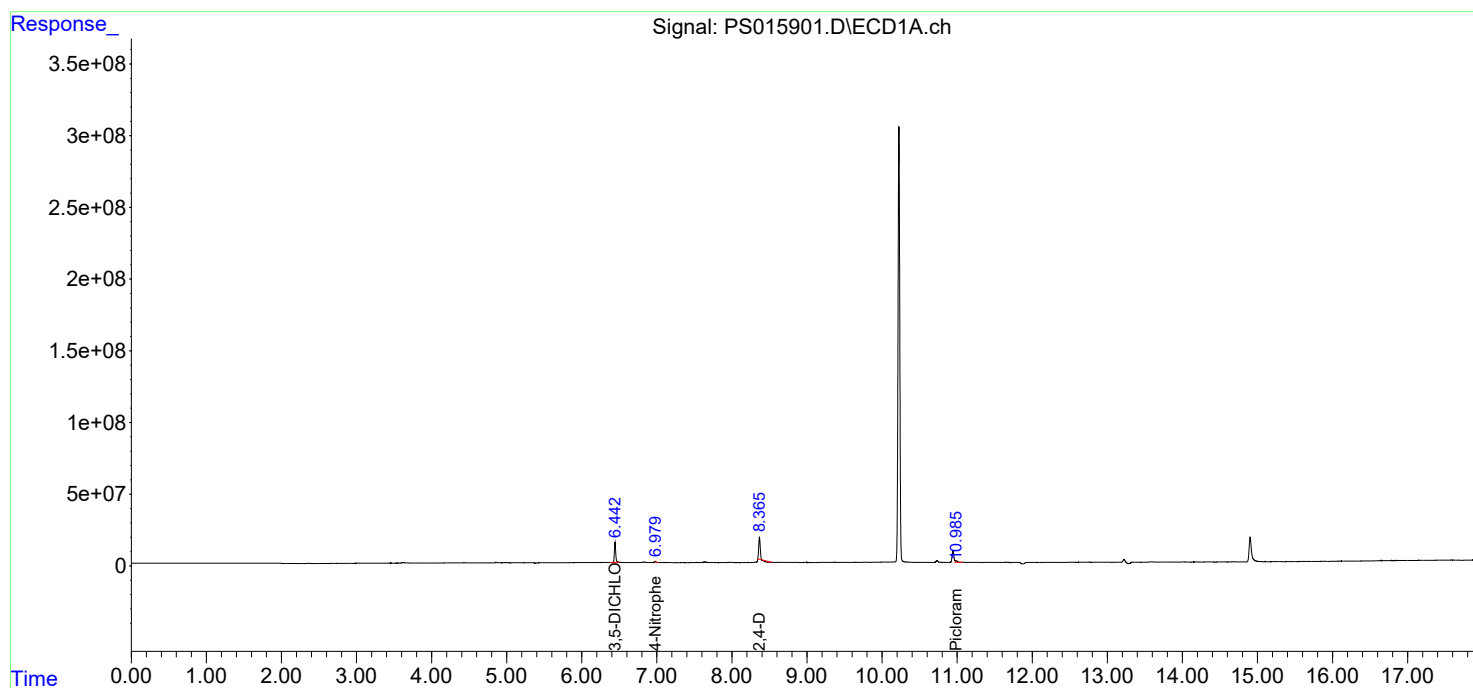


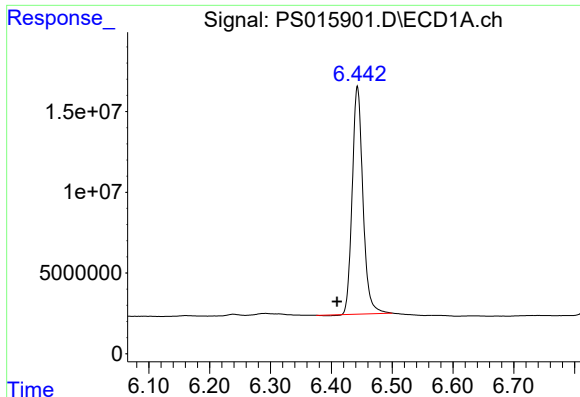

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.443 min
Delta R.T.: 0.033 min
Response: 172407490
Conc: 76.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

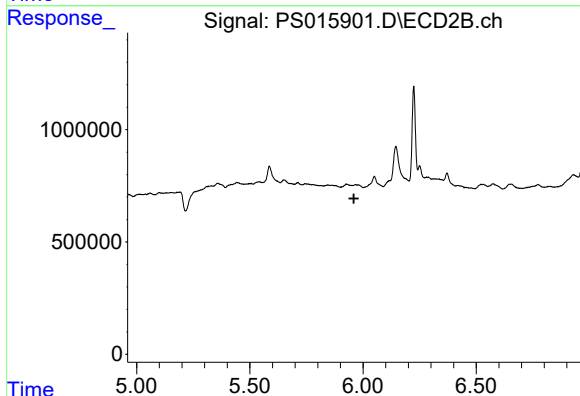


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

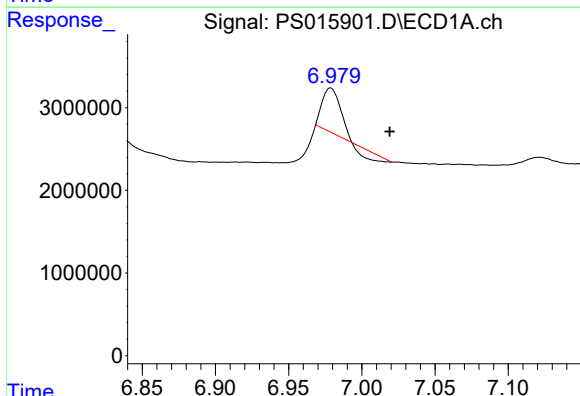


#3 4-Nitrophenol

R.T.: 6.979 min
Delta R.T.: -0.040 min
Response: 3661724
Conc: 4.03 ng/ml

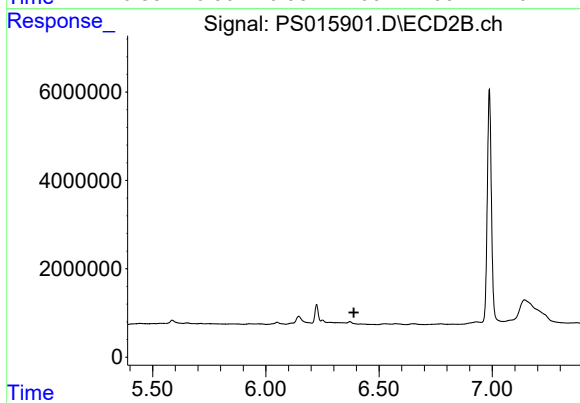

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

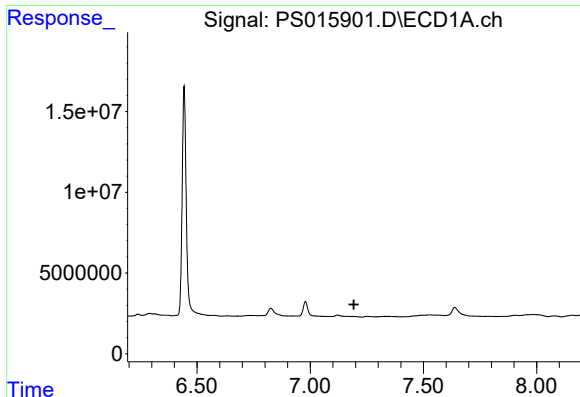

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

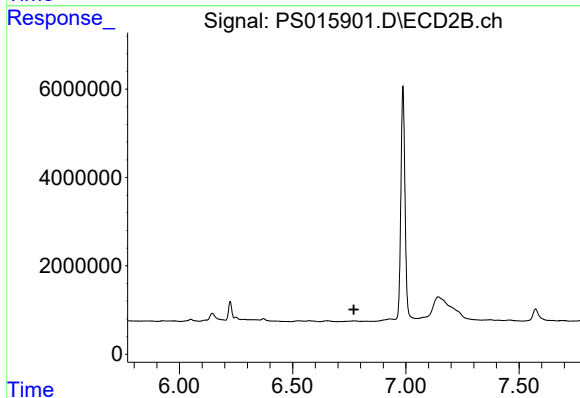


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

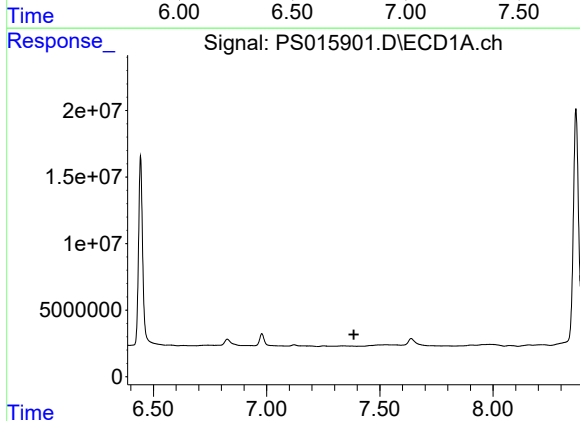


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

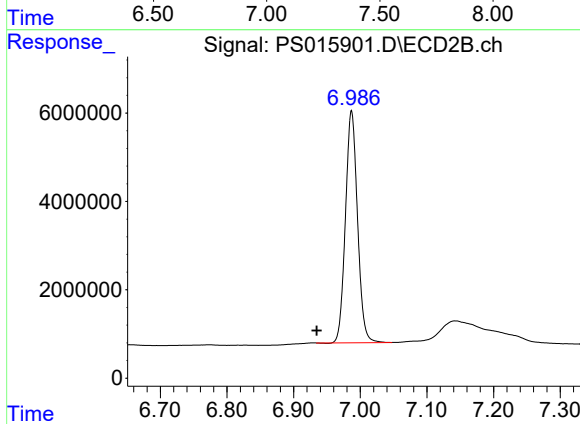

#5 DICAMBA


R.T.: 6.987 min
Delta R.T.: 0.052 min
Response: 65876969
Conc: 31.75 ng/ml

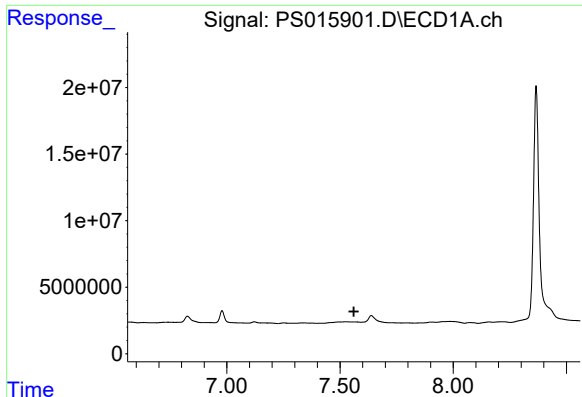

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.561 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

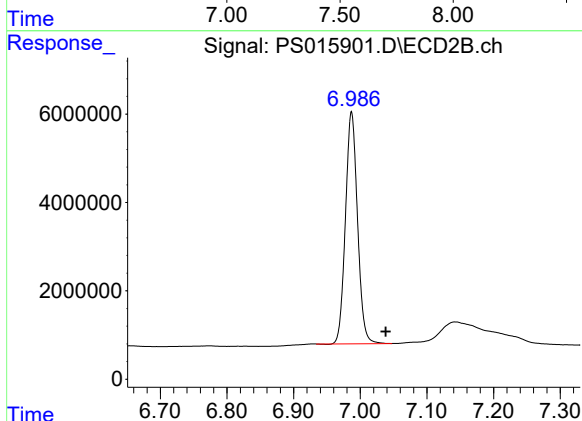


#6 MCPP

R.T.: 6.987 min
Delta R.T.: -0.051 min
Response: 65876969
Conc: 39.52 ug/ml

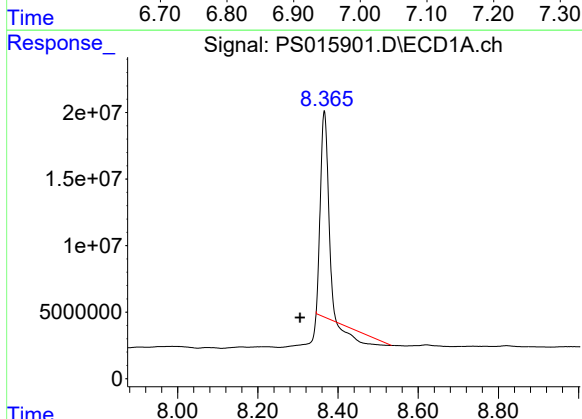


#9 2,4-D

R.T.: 8.366 min
Delta R.T.: 0.061 min
Response: 179811440
Conc: 102.60 ng/ml

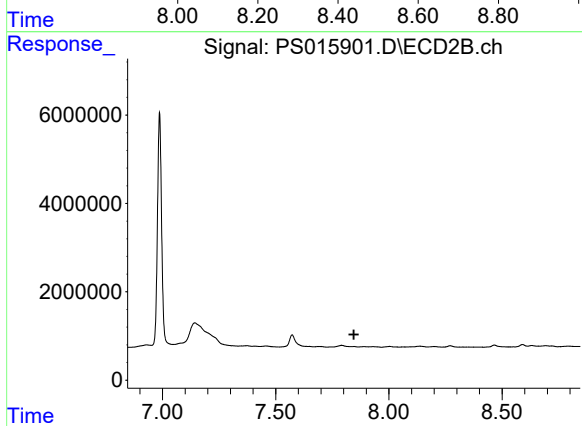

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

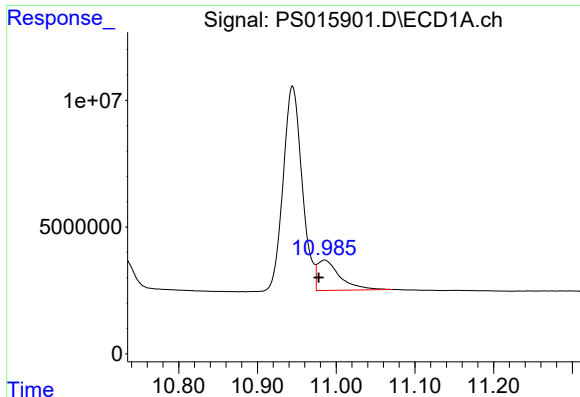

#15 Picloram


R.T.: 10.985 min
Delta R.T.: 0.007 min
Response: 23661078
Conc: 1.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

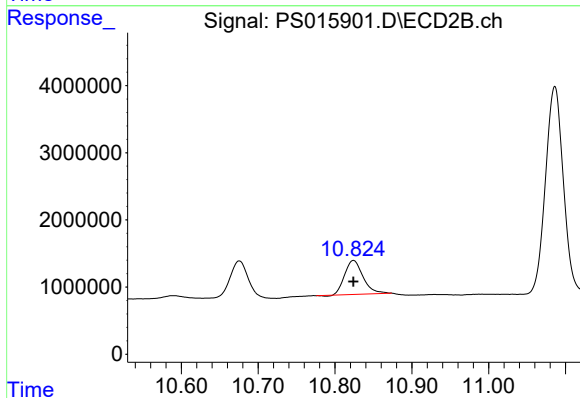


#15 Picloram

R.T.: 10.824 min
Delta R.T.: 0.000 min
Response: 8379019
Conc: 1.99 ng/ml

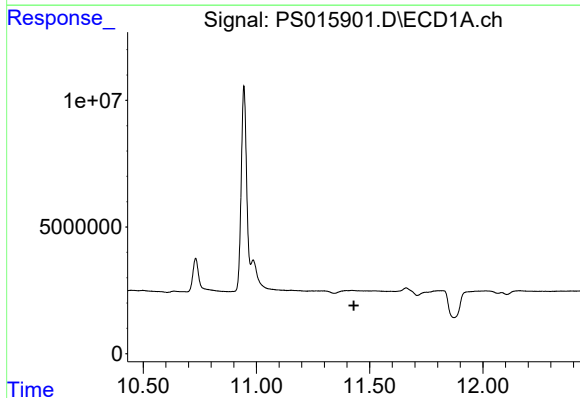

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.431 min
Response: 0
Conc: N.D.

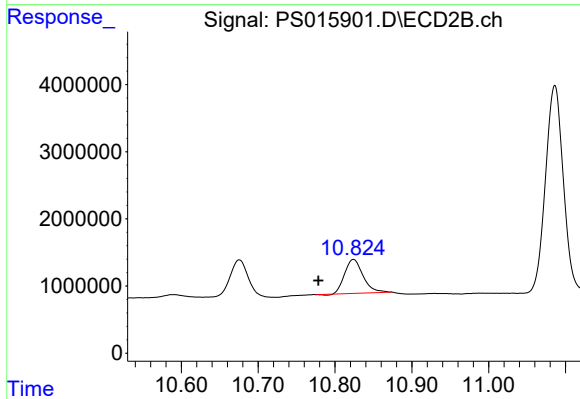

#16 DCPA

R.T.: 10.824 min
Delta R.T.: 0.045 min
Response: 8379019
Conc: 1.99 ng/ml