

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062221\
 Data File : PS015912.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2021 13:28
 Operator : DD\AJ
 Sample : M2764-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 14:21:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.188	6.765	394.2E6	138.0E6	237.273m	273.961m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_S
 ClientSampleId :
 PHC-250EM-001

Manual Integrations
 APPROVED

Ankita
 6/23/2021 2:18:53 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062221\
Data File : PS015912.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2021 13:28
Operator : DD\AJ
Sample : M2764-01
Misc :
ALS Vial : 12 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 14:21:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation


Instrument :
ECD_S
ClientSampleId :
PHC-250EM-001

Manual Integrations
APPROVED

Ankita
6/23/2021 2:18:53 PM

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

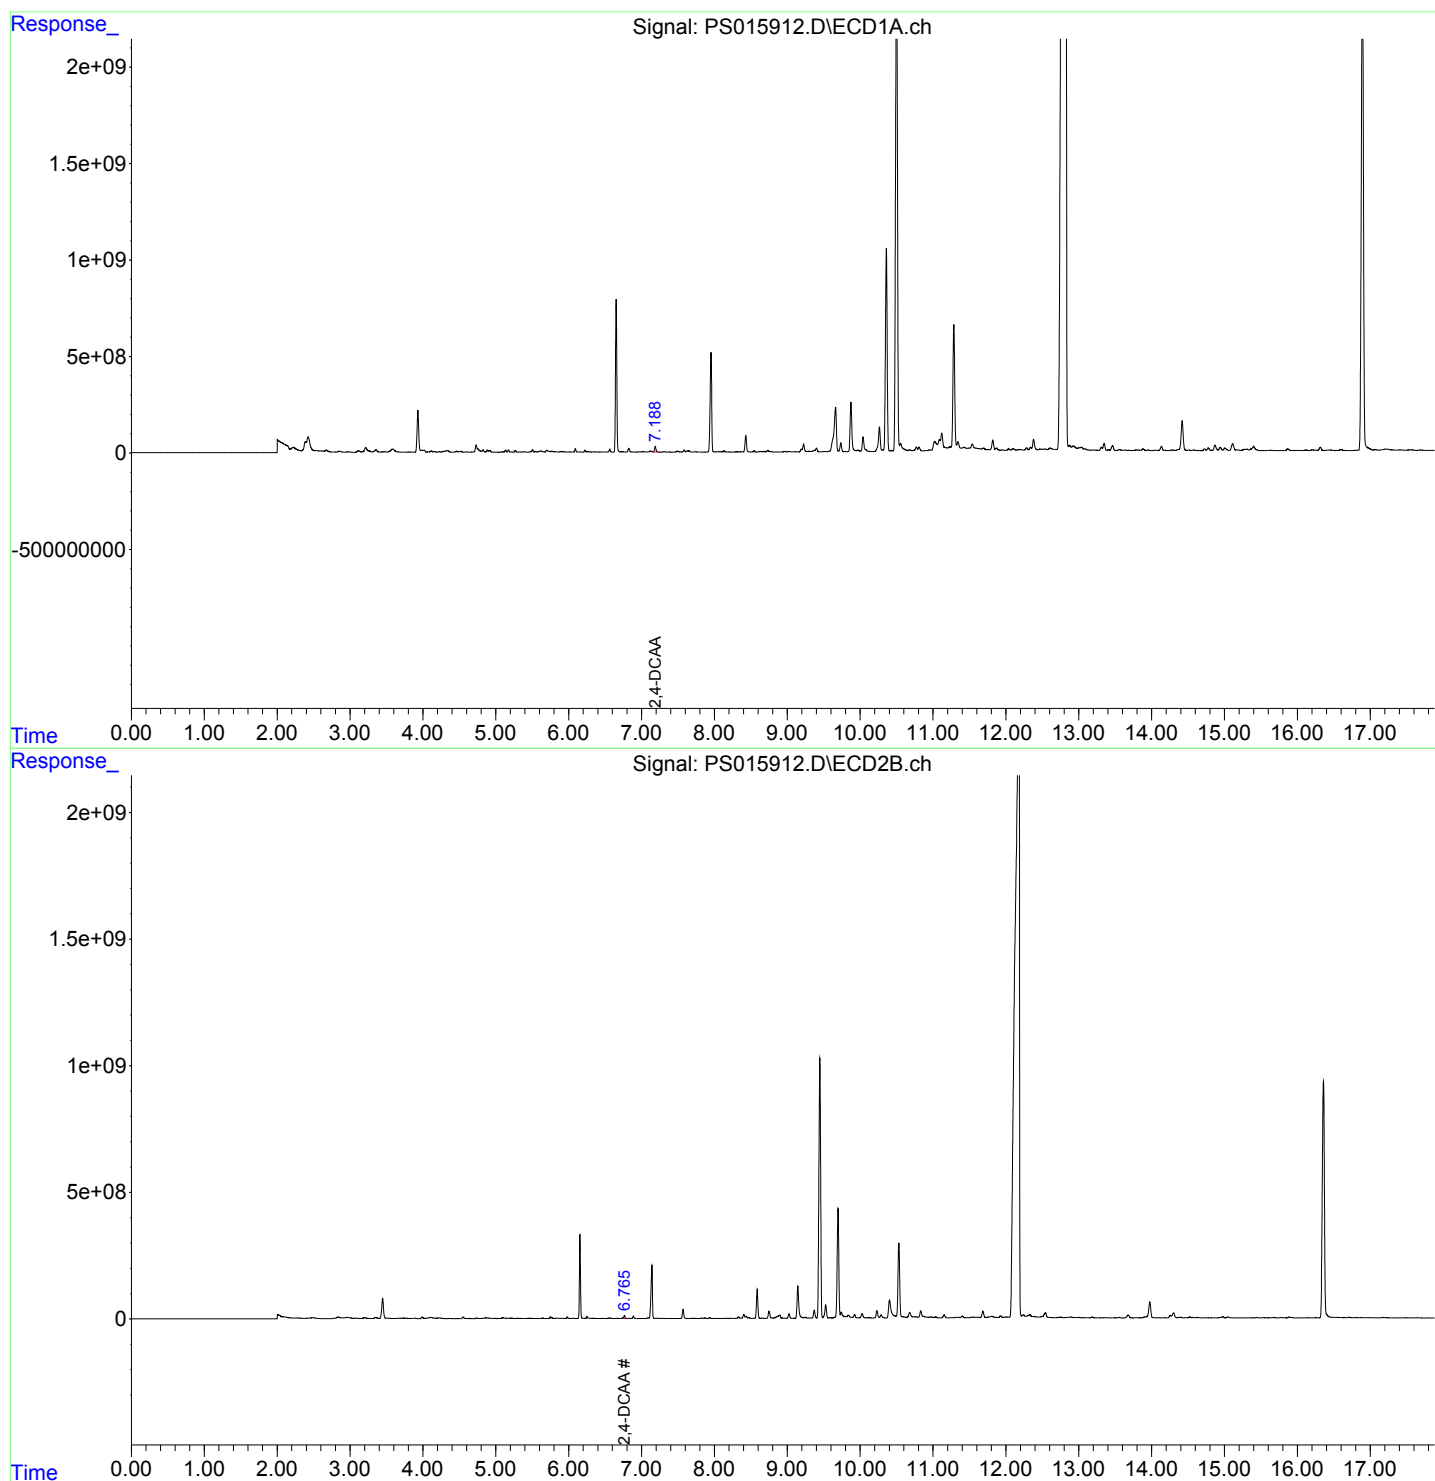

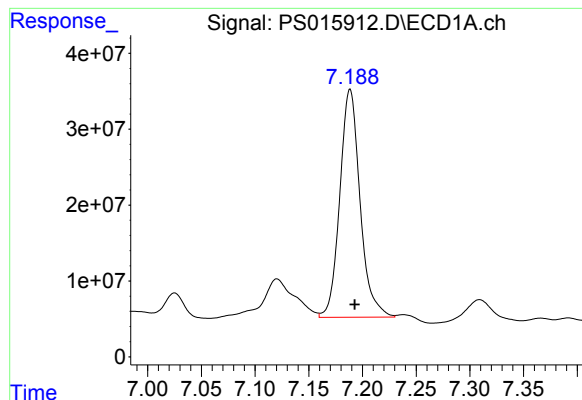


#4 2,4-DCAA

R.T.: 7.188 min
Delta R.T.: -0.005 min
Response: 394216850
Conc: 237.27 ng/ml m

Instrument :
ECD_S
ClientSampleId :
PHC-250EM-001

Manual Integrations
APPROVED

Ankita
6/23/2021 2:18:53 PM

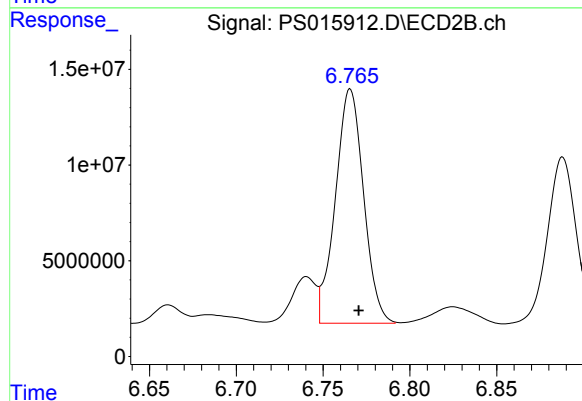

#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.005 min
Response: 138035794
Conc: 273.96 ng/ml m