

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062222\
 Data File : PS019752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 09:29
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 18:32:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) T	3,5-DICHL...	6.454	5.915f	64543476	98084	20.421 <MDL #
3) T	4-Nitroph...	6.986f	6.386	4150961	421434	4.230 <MDL #
5) T	DICAMBA	0.000	7.004f	0	20470829	N.D. 5.988
6) T	MCP	0.000	7.004	0	20470829	N.D. 7.562
7) T	MCPA	7.736	0.000	5123642	0	<MDL N.D. #
8) T	DICHLORPROP	0.000	7.633f	0	1063063	N.D. 1.203
9) T	2,4-D	0.000	7.833	0	345391	N.D. <MDL
10) T	Pentachlo...	8.641	0.000	3329087	0	<MDL N.D. #
11) T	2,4,5-TP ...	9.117f	8.642	5014038	255811	<MDL <MDL #
12) T	2,4,5-T	9.447	9.053	6128444	312613	<MDL <MDL #
13) T	2,4-DB	10.033	9.467f	26080435	2000892	6.446 3.238 #
14) T	DINOSEB	0.000	9.857	0	439594	N.D. <MDL
15) T	Picloram	10.958	10.880f	201.3E6	19068849	6.781 2.965 #
16) T	DCPA	11.428	0.000	1580676	0	<MDL N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062222\
Data File : PS019752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 09:29
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 18:32:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

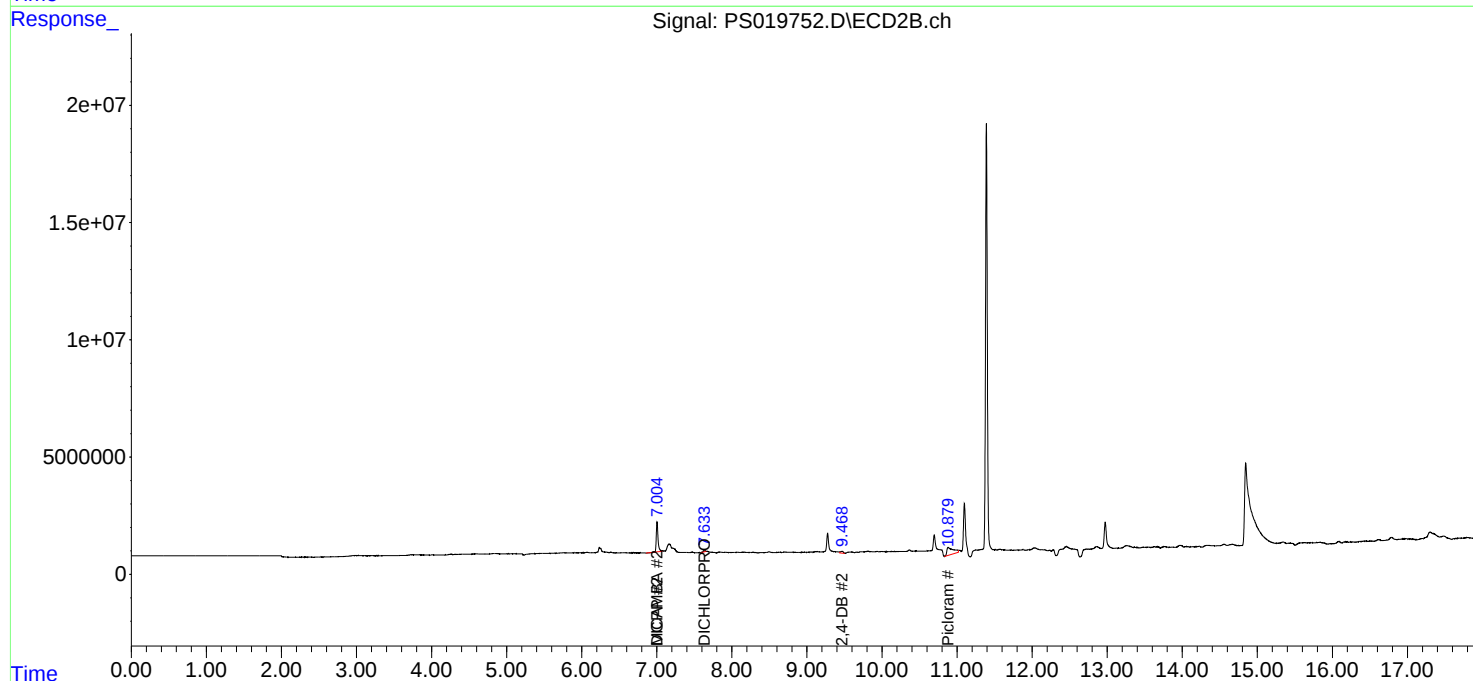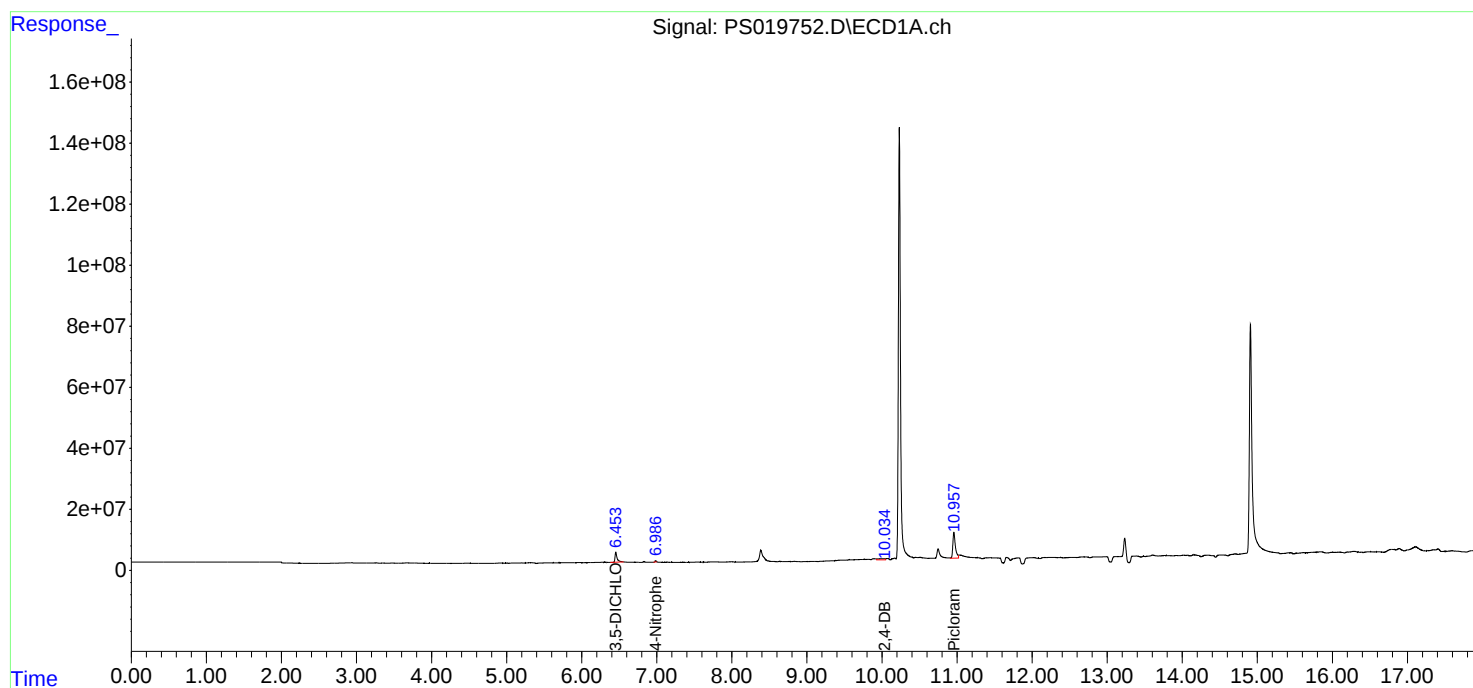


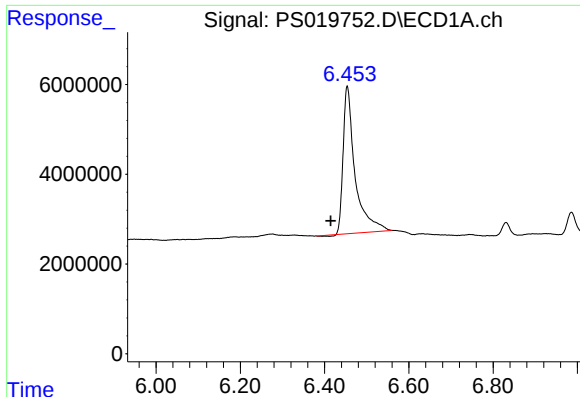

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.454 min
Delta R.T.: 0.040 min
Response: 64543476
Conc: 20.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

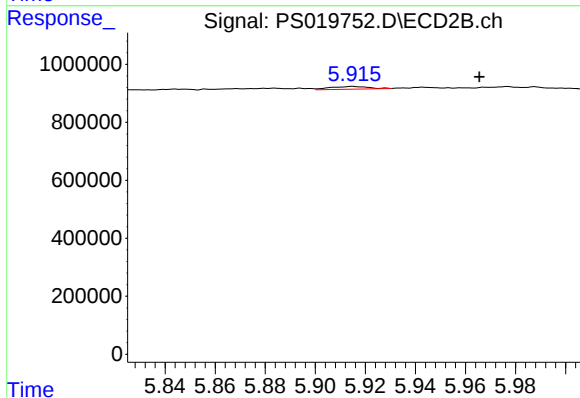


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.915 min
Delta R.T.: -0.051 min
Response: 98084
Conc: N.D.

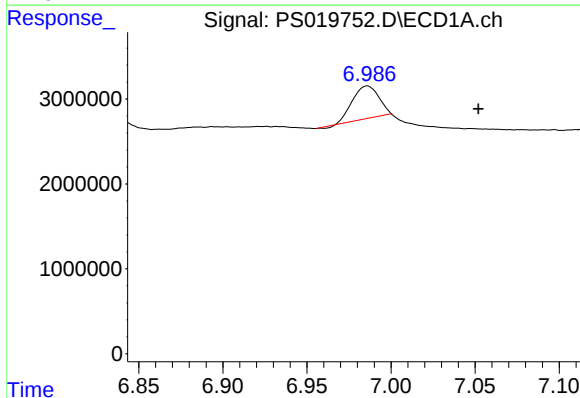


#3 4-Nitrophenol

R.T.: 6.986 min
Delta R.T.: -0.066 min
Response: 4150961
Conc: 4.23 ng/ml

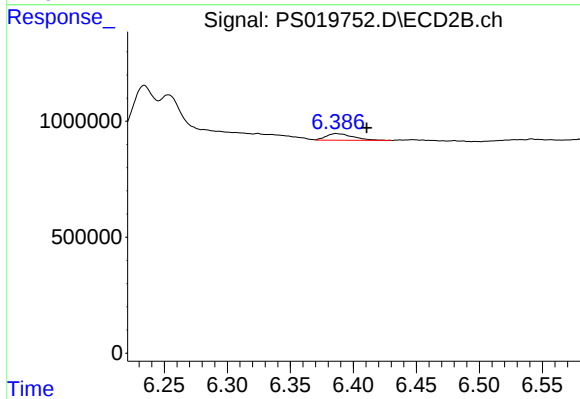

#3 4-Nitrophenol


R.T.: 6.386 min
Delta R.T.: -0.024 min
Response: 421434
Conc: N.D.

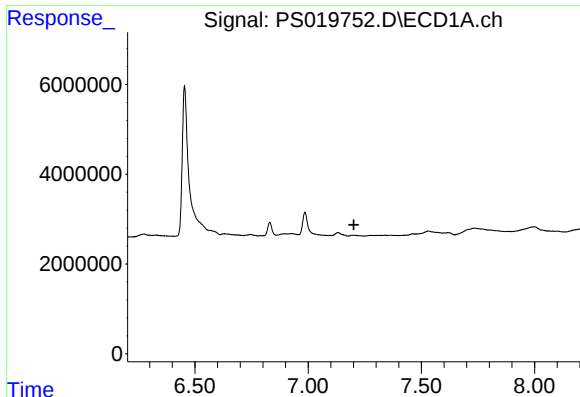

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: -0.001 min
Response: -188744
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

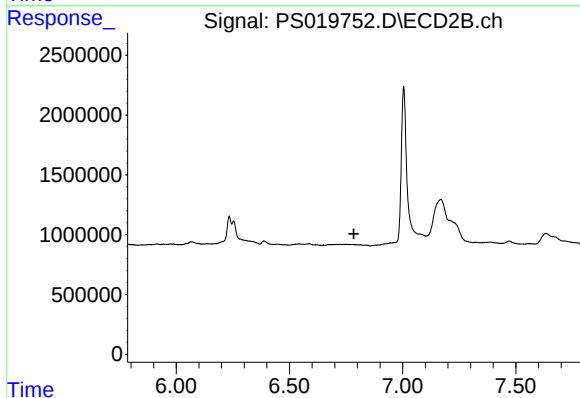


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

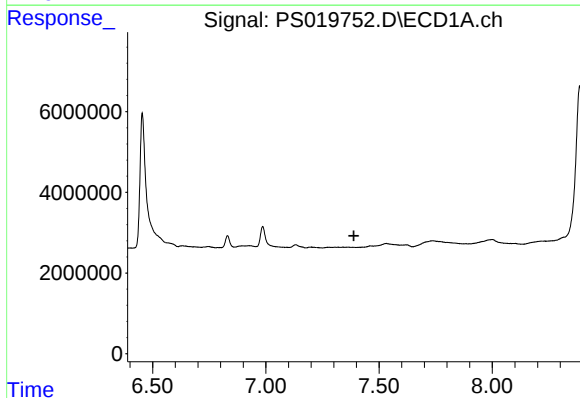


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

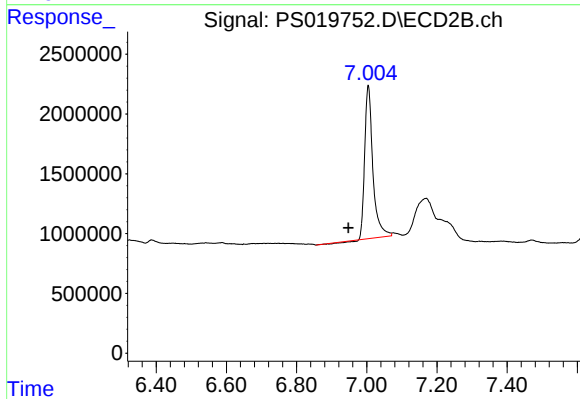

#5 DICAMBA


R.T.: 7.004 min
Delta R.T.: 0.056 min
Response: 20470829
Conc: 5.99 ng/ml

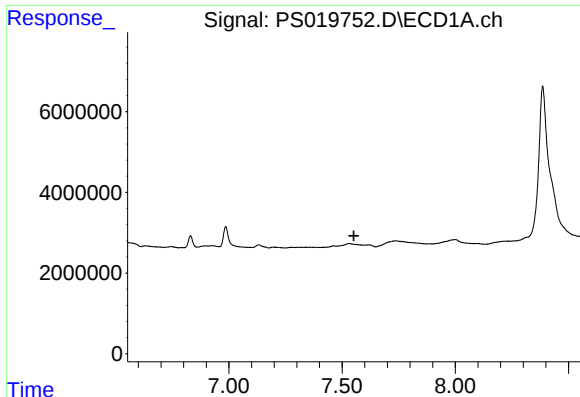

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

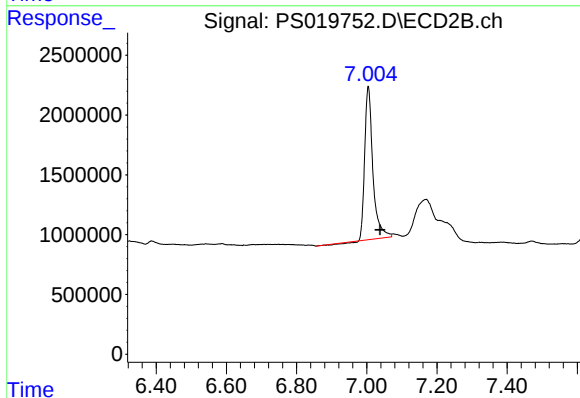


#6 MCP

R.T.: 7.004 min
Delta R.T.: -0.034 min
Response: 20470829
Conc: 7.56 ug/ml

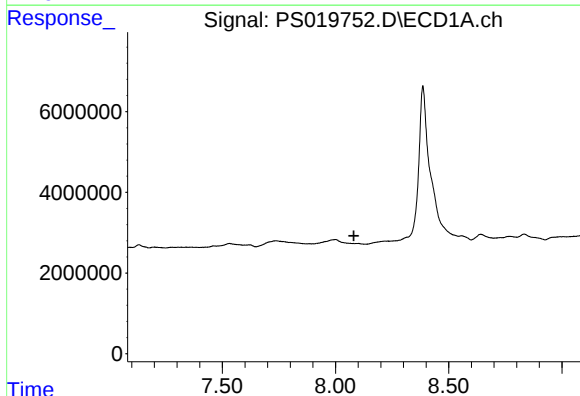


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.081 min
Response: 0
Conc: N.D.

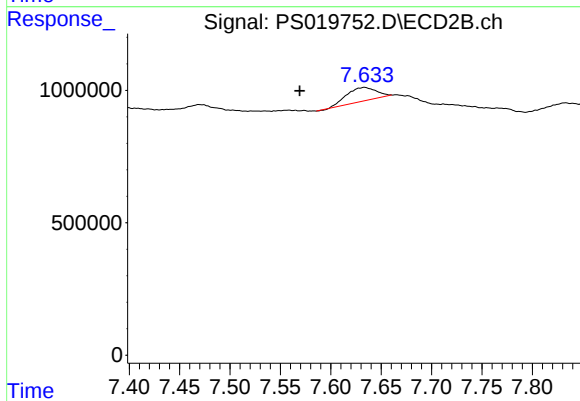

#8 DICHLORPROP


R.T.: 7.633 min
Delta R.T.: 0.064 min
Response: 1063063
Conc: 1.20 ng/ml

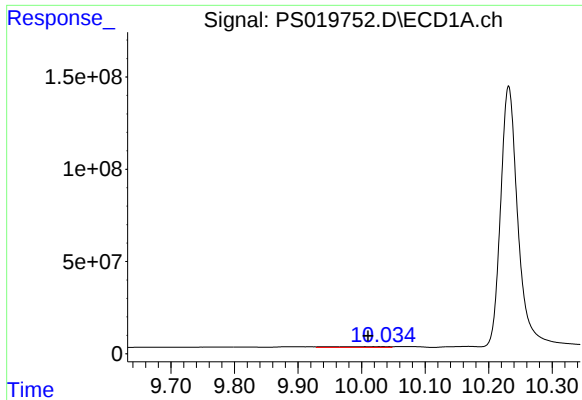

#13 2,4-DB


R.T.: 10.033 min
Delta R.T.: 0.023 min
Response: 26080435
Conc: 6.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

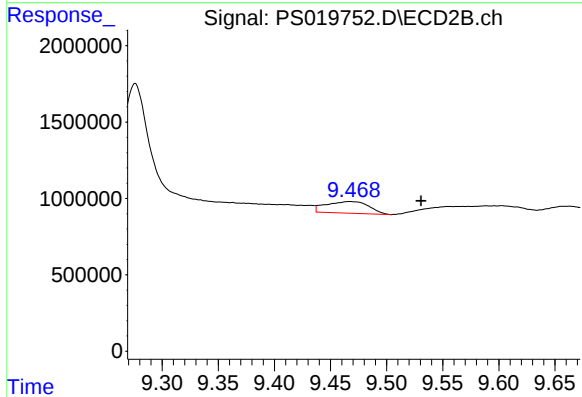


#13 2,4-DB

R.T.: 9.467 min
Delta R.T.: -0.064 min
Response: 2000892
Conc: 3.24 ng/ml

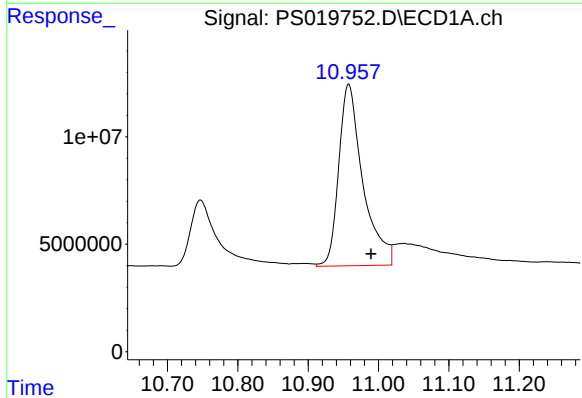

#15 Picloram

R.T.: 10.958 min
Delta R.T.: -0.032 min
Response: 201255637
Conc: 6.78 ng/ml

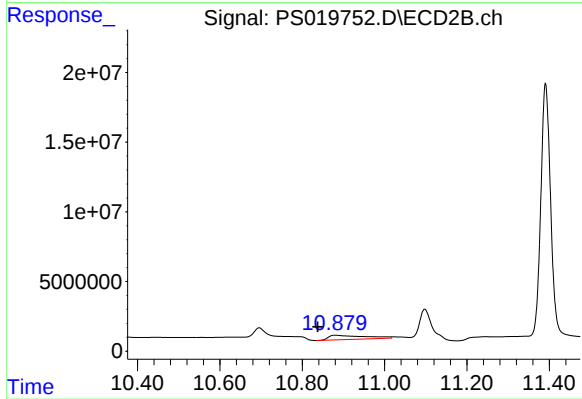

#15 Picloram

R.T.: 10.880 min
Delta R.T.: 0.042 min
Response: 19068849
Conc: 2.96 ng/ml