

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062223\
 Data File : PS023357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 11:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 12:46:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.482	6.853	909.6E6	284.7E6	514.090	501.506
Target Compounds							
1) T	Dalapon	2.583	0.000	1891144	0	1.034	N.D. #
3) T	4-Nitroph...	6.317	0.000	7322365	0	5.681	N.D. #
6) T	MCP	6.749	0.000	864892	0	<MDL	N.D. #
7) T	MCPA	6.855f	7.309	-2398690	9741302	N.D.	3.625
8) T	DICHLORPROP	7.291f	0.000	854470	0	<MDL	N.D. #
10) T	Pentachlo...	7.674	0.000	1385705	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.212	0.000	2306192	0	<MDL	N.D. #
12) T	2,4,5-T	8.480	9.138f	2024674	1578473	<MDL	<MDL #
13) T	2,4-DB	8.939f	0.000	9776095	0	4.153	N.D. #
14) T	DINOSEB	10.062	0.000	459092	0	<MDL	N.D. #
15) T	Picloram	9.895	10.894	53297404	8786010	3.071	1.925 #
16) T	DCPA	10.336	10.894	1877144	8786010	<MDL	2.190 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062223\
Data File : PS023357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 11:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 12:46:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

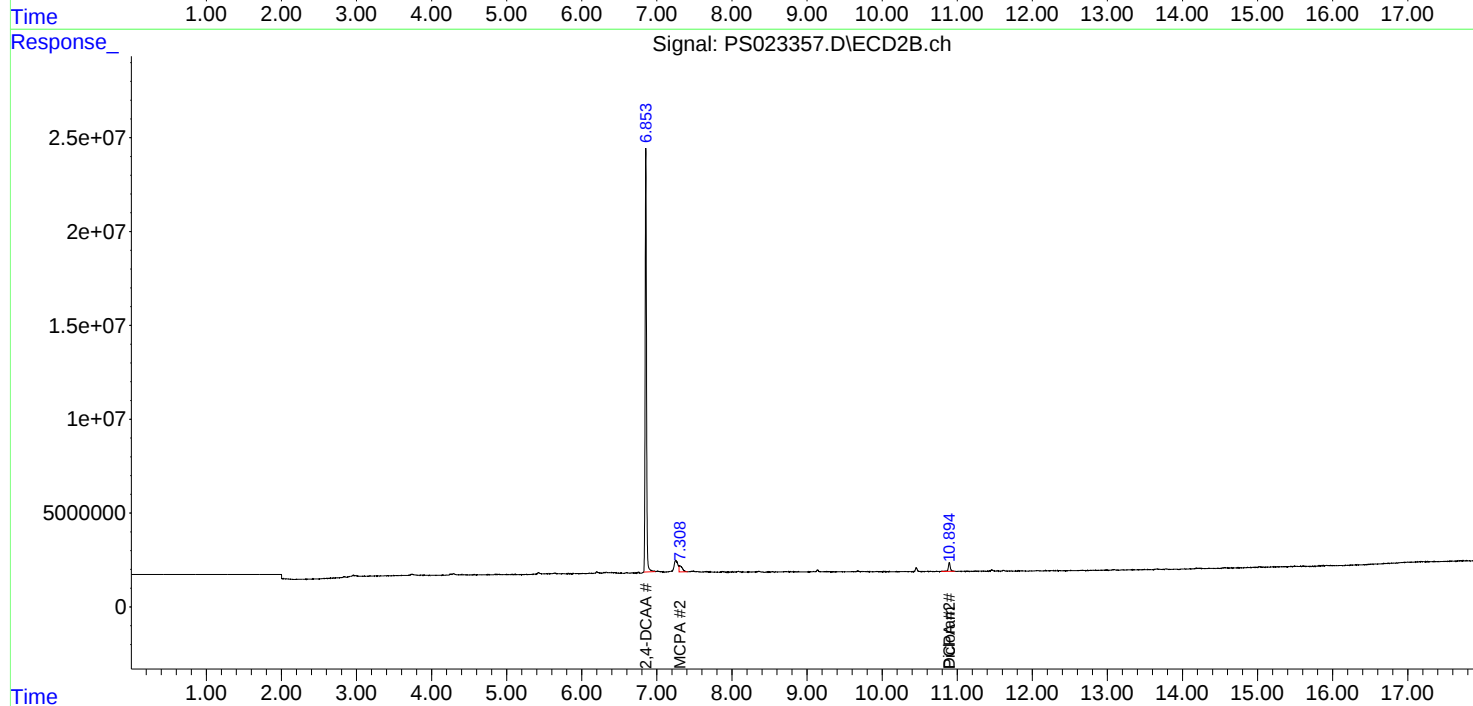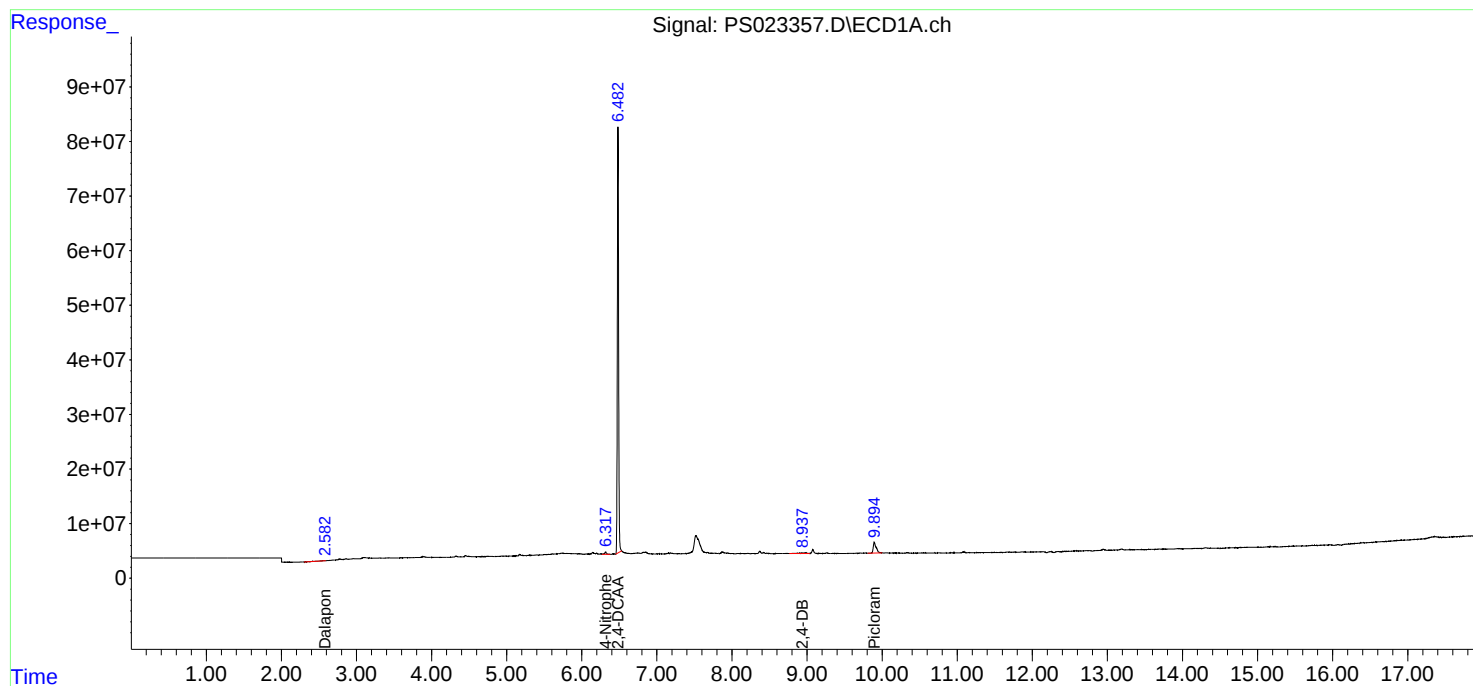


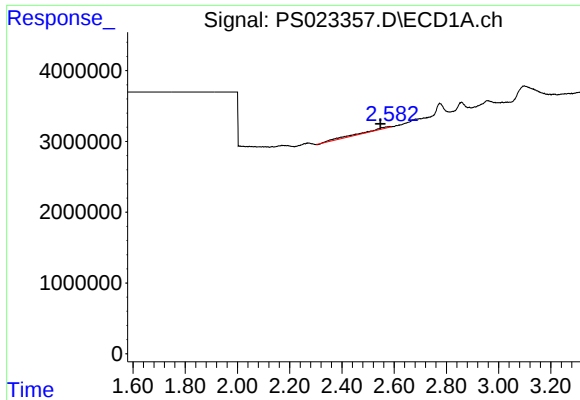

#1 Dalapon


R.T.: 2.583 min
Delta R.T.: 0.036 min
Response: 1891144
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

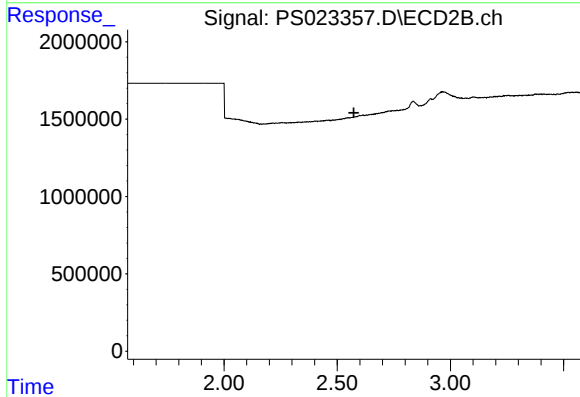


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

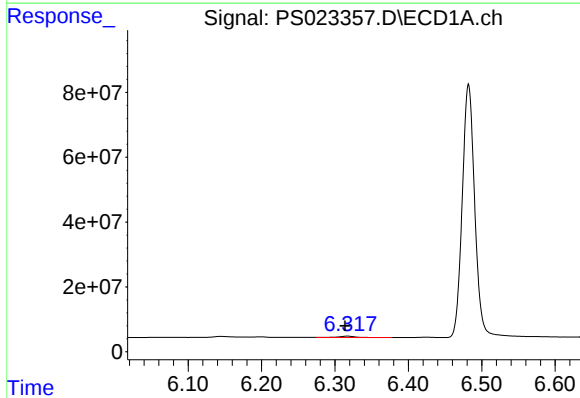


#3 4-Nitrophenol

R.T.: 6.317 min
Delta R.T.: 0.003 min
Response: 7322365
Conc: 5.68 ng/ml

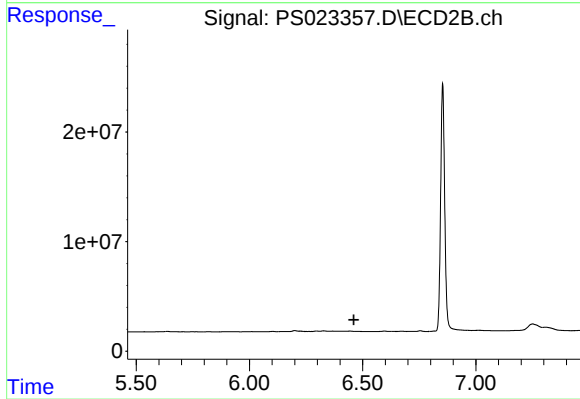

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

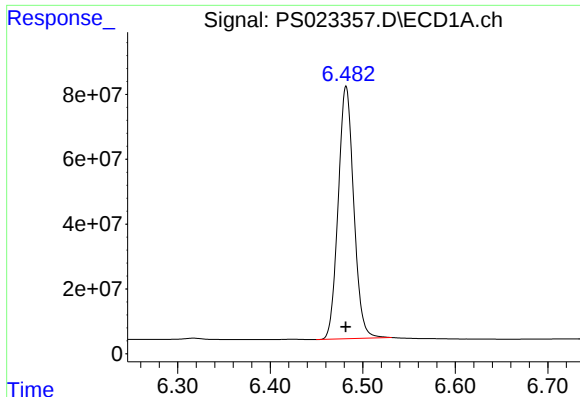

#4 2,4-DCAA


R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 909557483
Conc: 514.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

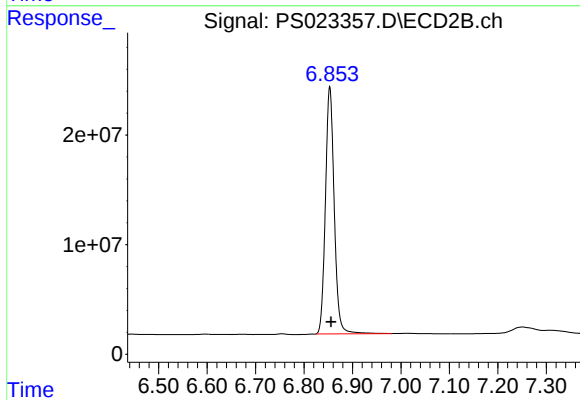


#4 2,4-DCAA

R.T.: 6.853 min
Delta R.T.: -0.003 min
Response: 284702667
Conc: 501.51 ng/ml

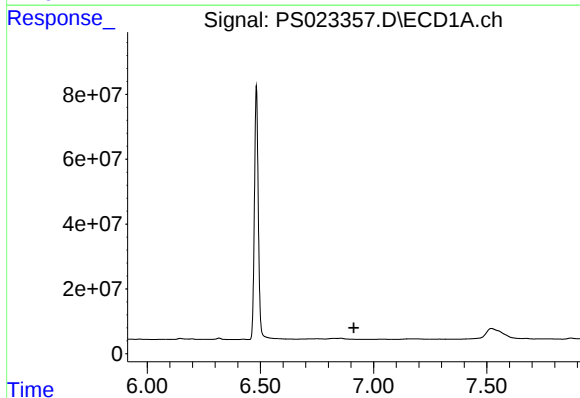


#7 MCPA

R.T.: 6.855 min
Delta R.T.: -0.058 min
Response: -2398690
Conc: N.D.

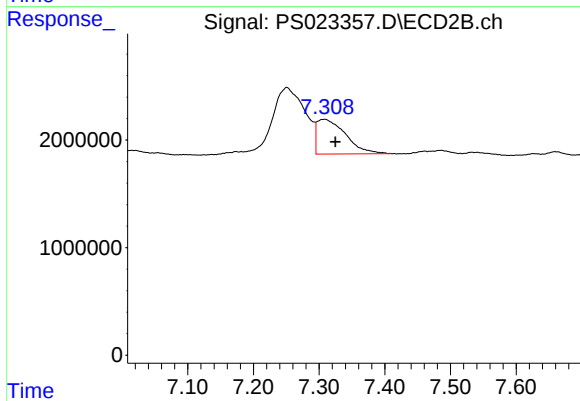

#7 MCPA


R.T.: 7.309 min
Delta R.T.: -0.016 min
Response: 9741302
Conc: 3.62 ug/ml

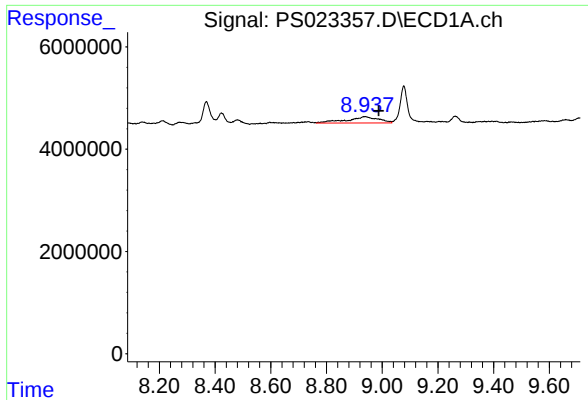

#13 2,4-DB


R.T.: 8.939 min
Delta R.T.: -0.049 min
Response: 9776095
Conc: 4.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

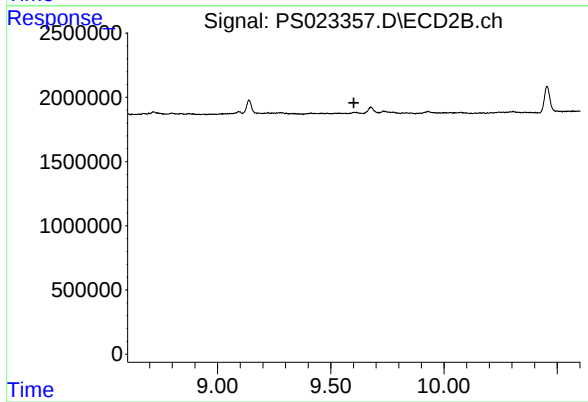


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.

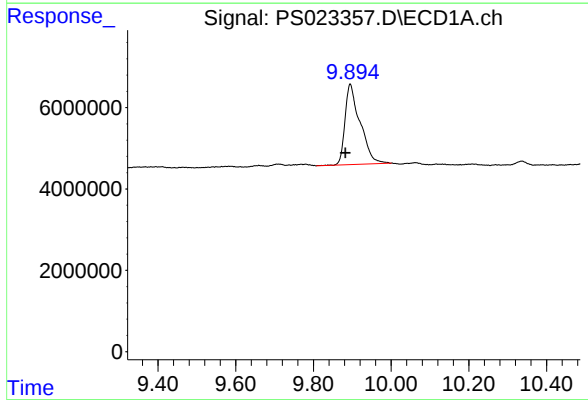


#15 Picloram

R.T.: 9.895 min
Delta R.T.: 0.013 min
Response: 53297404
Conc: 3.07 ng/ml

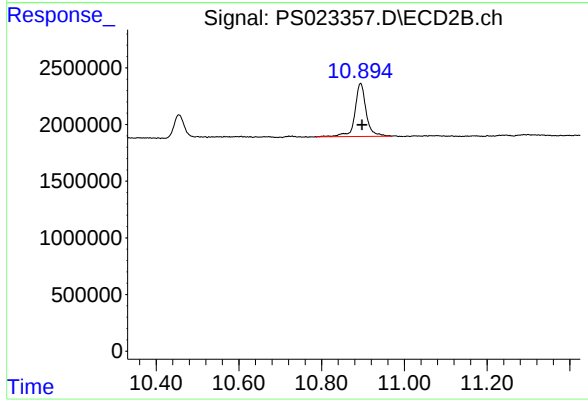

#15 Picloram


R.T.: 10.894 min
Delta R.T.: -0.004 min
Response: 8786010
Conc: 1.93 ng/ml

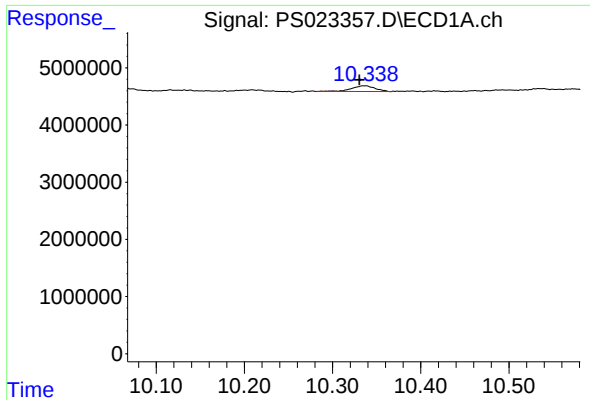

#16 DCPA

R.T.: 10.336 min
Delta R.T.: 0.006 min
Response: 1877144
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

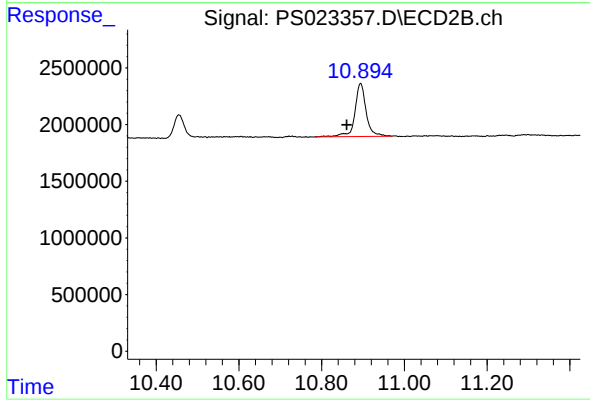

#16 DCPA

R.T.: 10.894 min
Delta R.T.: 0.034 min
Response: 8786010
Conc: 2.19 ng/ml