

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062223\
 Data File : PS023370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 19:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:14:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.479	6.854	925.7E6	295.9E6	523.236	521.227
Target Compounds							
3) T	4-Nitroph...	6.314	0.000	5924737	0	4.597	N.D. #
5) T	DICAMBA	6.625	7.014	-155712	679420	N.D.	<MDL
6) T	MCP	6.814	0.000	8173930	0	1.483	N.D. #
7) T	MCPA	0.000	7.302	0	16855249	N.D.	6.271
8) T	DICHLORPROP	7.254	7.659	1361472	5549908	<MDL	8.972 #
9) T	2,4-D	0.000	7.873f	0	1006737	N.D.	1.452
10) T	Pentachlo...	7.668	0.000	1375255	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.205	8.721	6041873	778242	<MDL	<MDL #
12) T	2,4,5-T	8.472	9.138f	3988165	926625	<MDL	<MDL #
13) T	2,4-DB	8.979	0.000	11766191	0	4.998	N.D. #
14) T	DINOSEB	10.048	0.000	1164962	0	<MDL	N.D. #
15) T	Picloram	9.879	10.892	14848757	3120756	<MDL	<MDL #
16) T	DCPA	10.323	10.892	1942786	3120756	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062223\
Data File : PS023370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 19:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:14:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

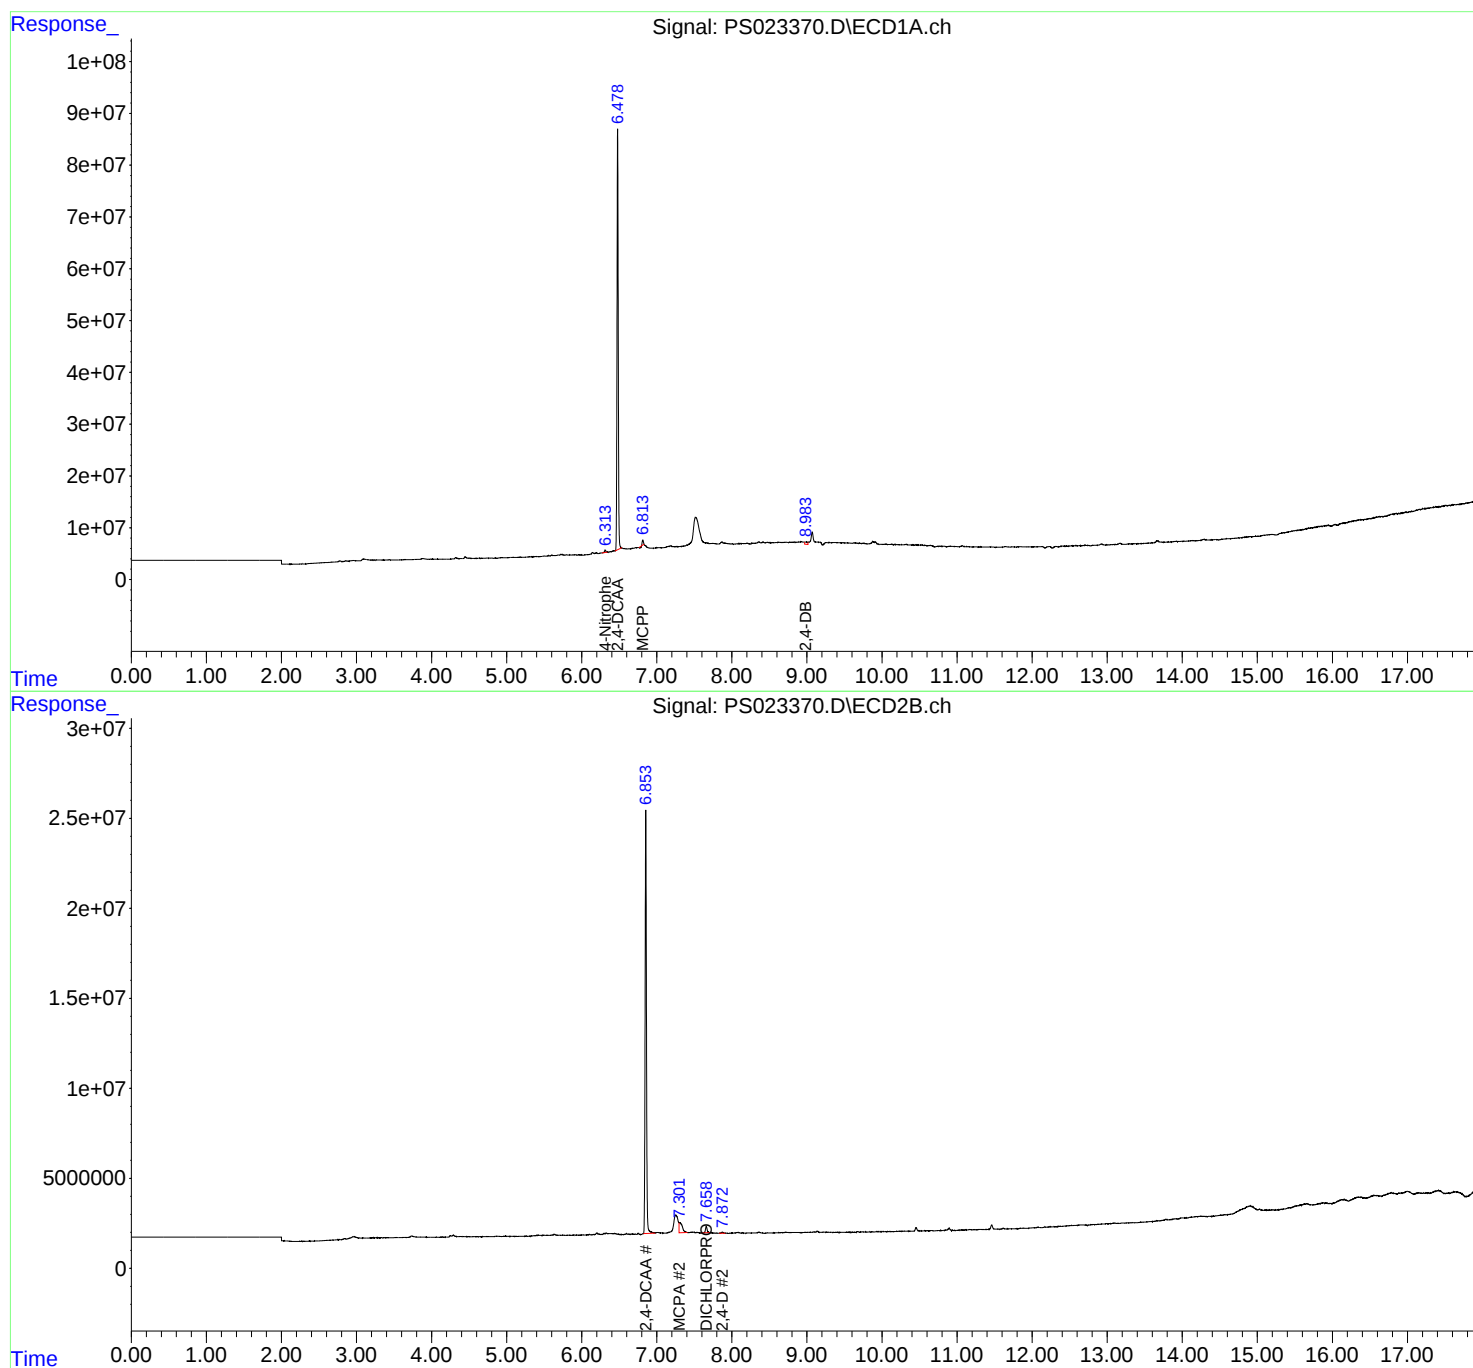


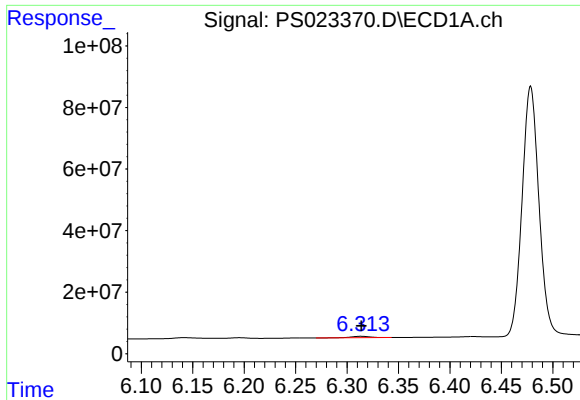

#3 4-Nitrophenol


R.T.: 6.314 min
Delta R.T.: 0.000 min
Response: 5924737
Conc: 4.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

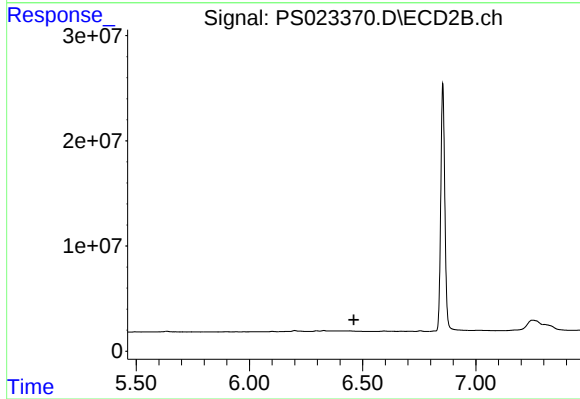


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

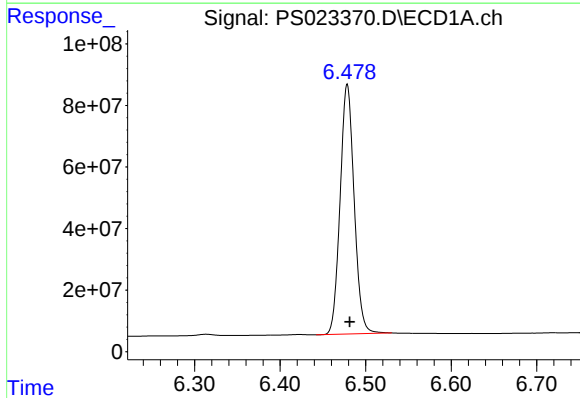


#4 2,4-DCAA

R.T.: 6.479 min
Delta R.T.: -0.003 min
Response: 925738215
Conc: 523.24 ng/ml

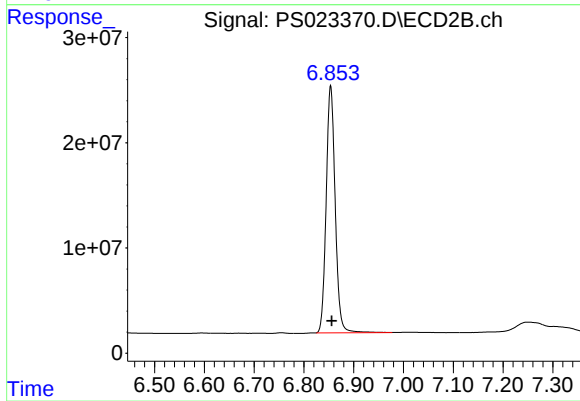

#4 2,4-DCAA


R.T.: 6.854 min
Delta R.T.: -0.002 min
Response: 295898491
Conc: 521.23 ng/ml

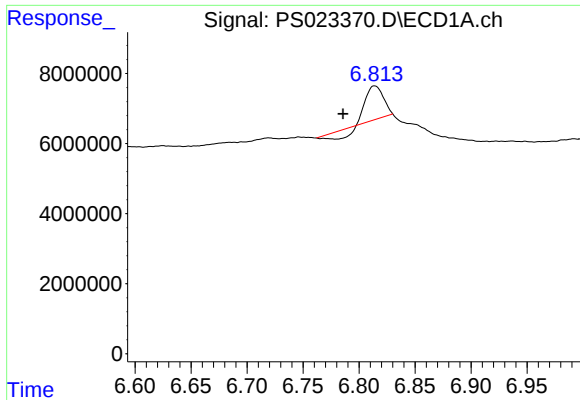

#6 MCPP


R.T.: 6.814 min
Delta R.T.: 0.029 min
Response: 8173930
Conc: 1.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

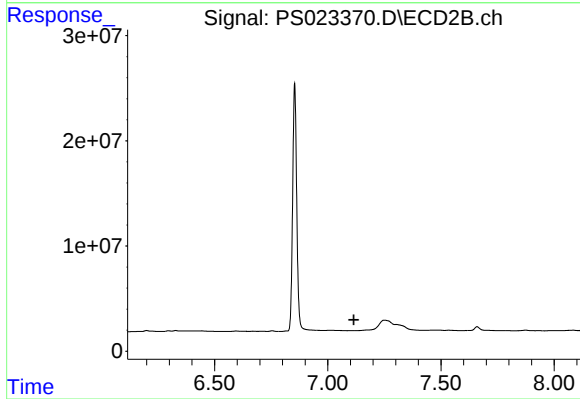


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

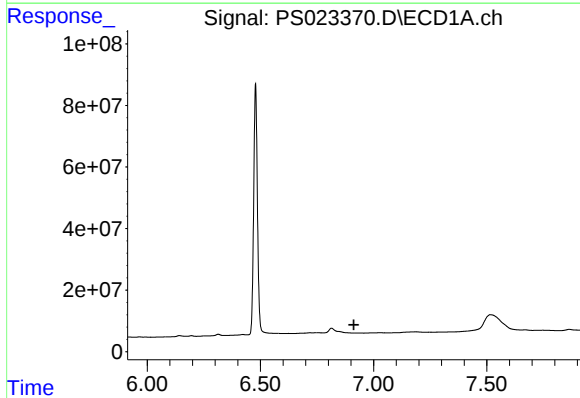


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.913 min
Response: 0
Conc: N.D.

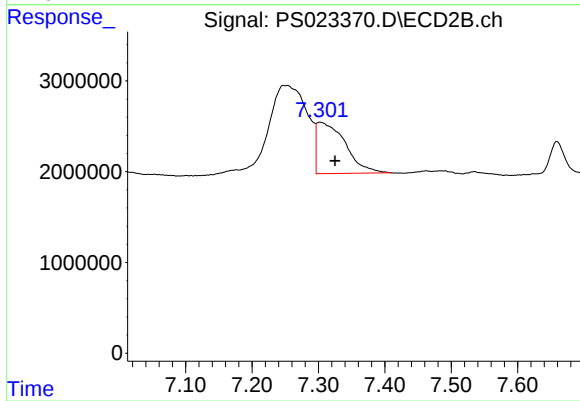

#7 MCPA


R.T.: 7.302 min
Delta R.T.: -0.023 min
Response: 16855249
Conc: 6.27 ug/ml

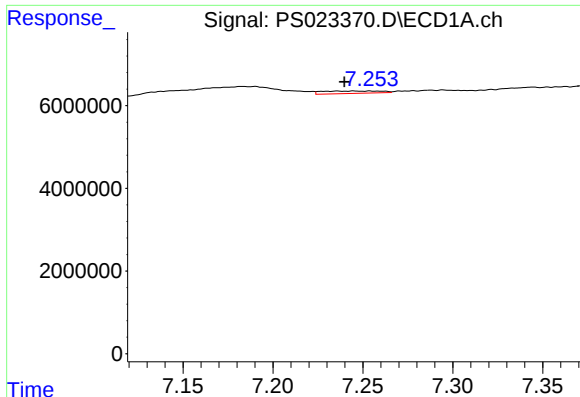

#8 DICHLORPROP


R.T.: 7.254 min
Delta R.T.: 0.015 min
Response: 1361472
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

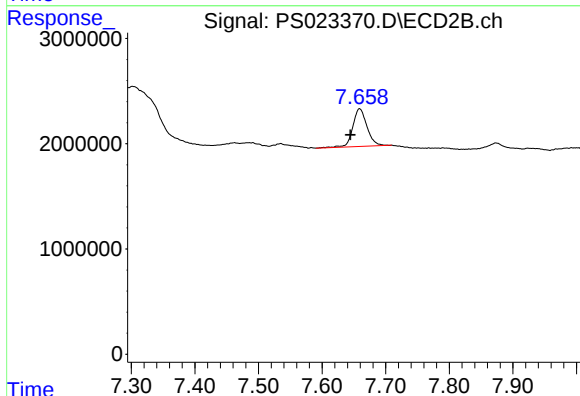


#8 DICHLORPROP

R.T.: 7.659 min
Delta R.T.: 0.014 min
Response: 5549908
Conc: 8.97 ng/ml

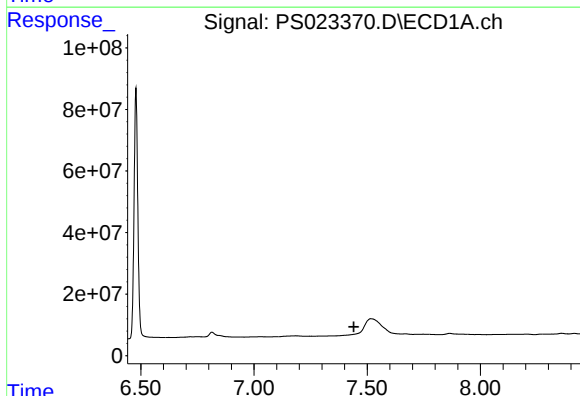


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.442 min
Response: 0
Conc: N.D.

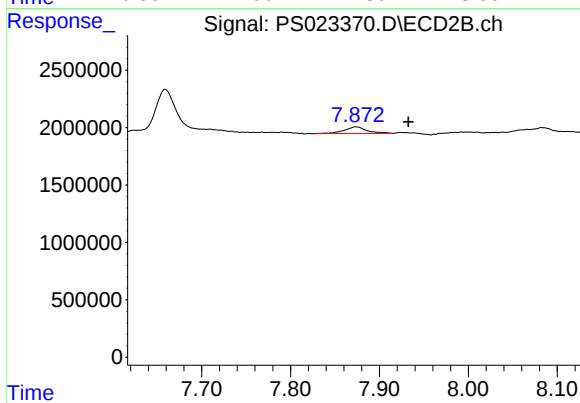

#9 2,4-D


R.T.: 7.873 min
Delta R.T.: -0.059 min
Response: 1006737
Conc: 1.45 ng/ml

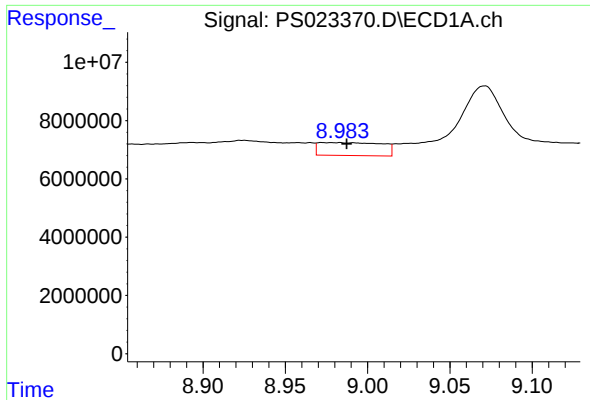

#13 2,4-DB

R.T.: 8.979 min
Delta R.T.: -0.009 min
Response: 11766191
Conc: 5.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

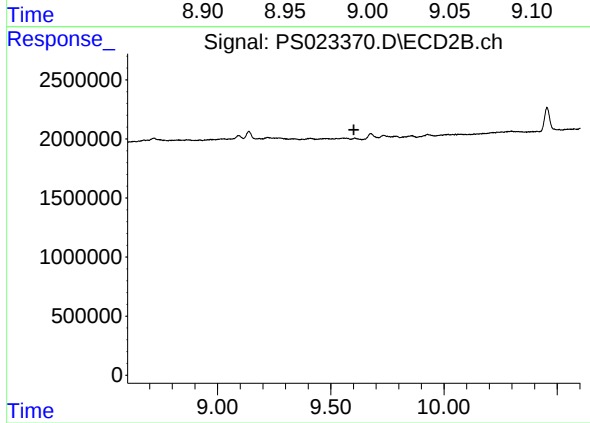

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.