

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062318\
 Data File : PS000612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2018 16:19
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:20:21 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.817	11.197	205.7E6	173.2E6	546.251	508.893
Target Compounds							
3) T	4-Nitroph...	11.442	0.000	642538	0	2.733	N.D. #
6) T	MCP	12.505	0.000	287250	0	0.254	N.D. #
10) T	Pentachlo...	14.085	13.645	1390739	585481	0.265	0.124 #
11) T	2,4,5-TP ...	14.952	0.000	706894	0	0.326	N.D. #
12) T	2,4,5-T	15.355	14.829	427319	303162	0.198	0.179
14) T	DINOSEB	17.612	0.000	1842455	0	1.237	N.D. #
15) T	Picloram	17.382	17.153	7300360	307293	2.500	0.123 #
16) T	DCPA	17.951	17.090	6690878	214913	2.611	0.093 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062318\
Data File : PS000612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2018 16:19
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:20:21 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

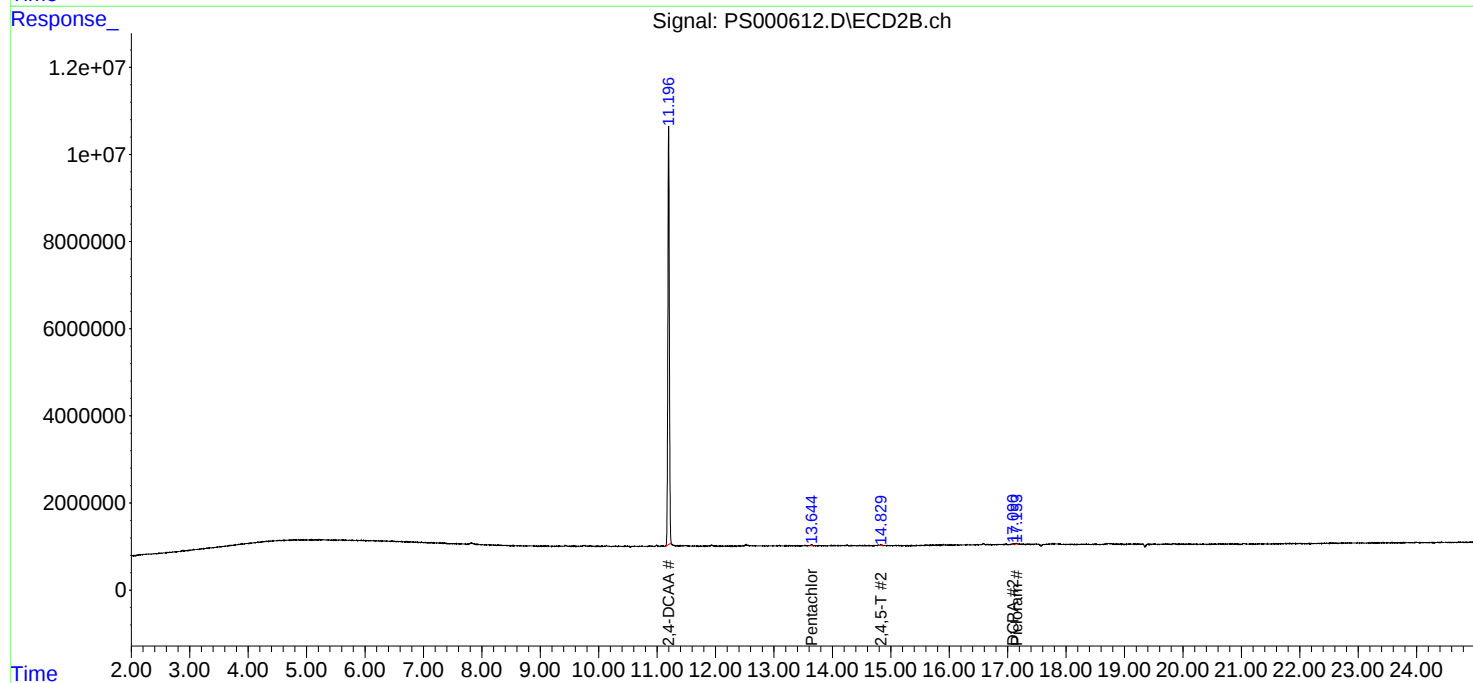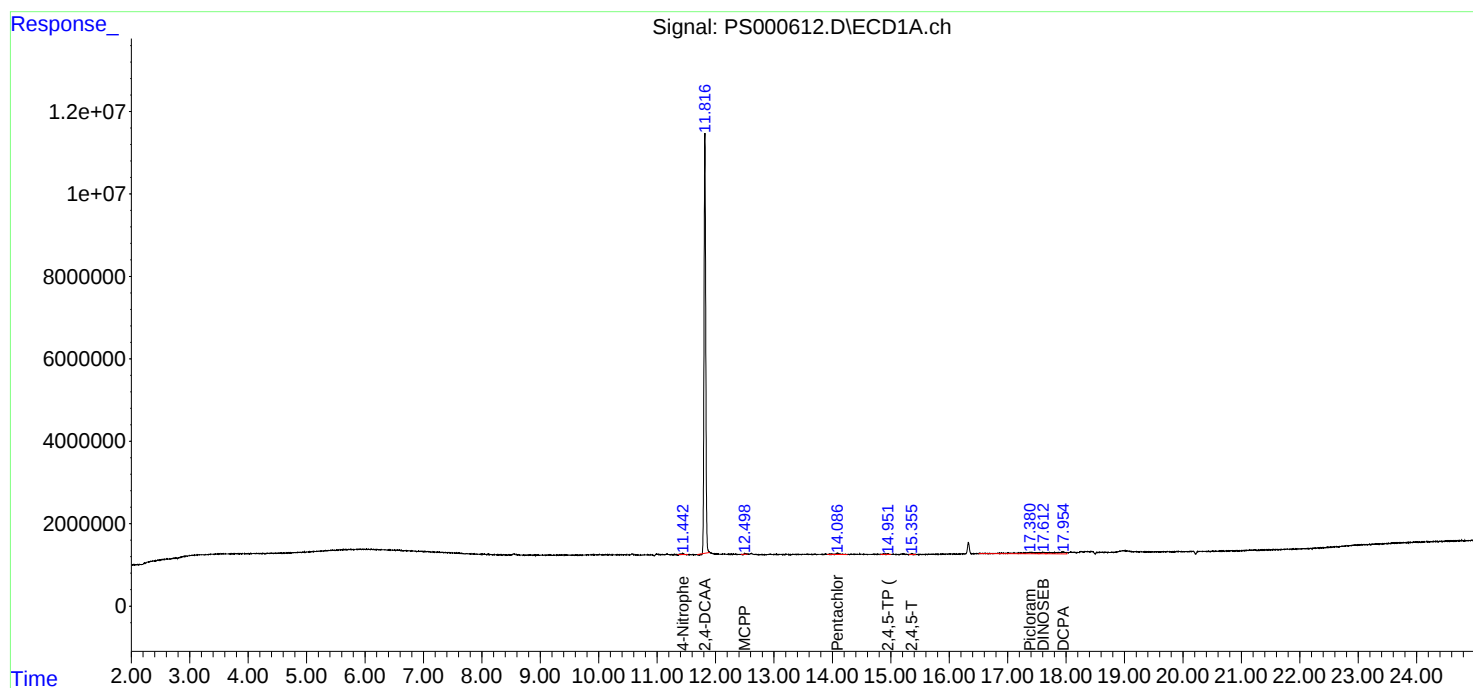


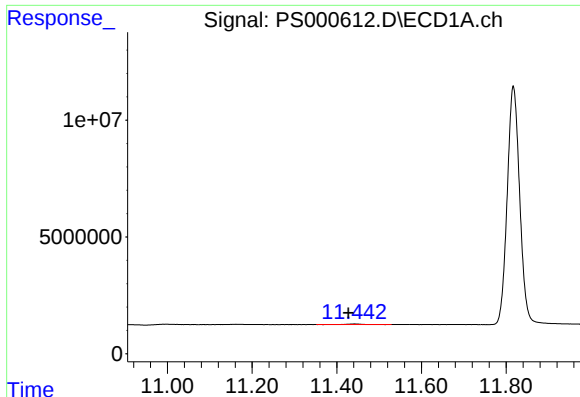

#3 4-Nitrophenol


R.T.: 11.442 min
Delta R.T.: 0.015 min
Response: 642538
Conc: 2.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

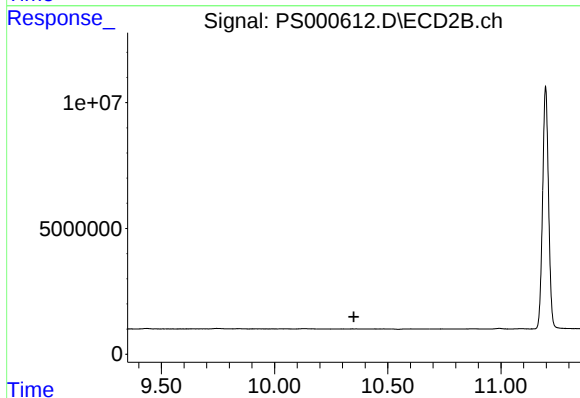


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.350 min
Response: 0
Conc: N.D.

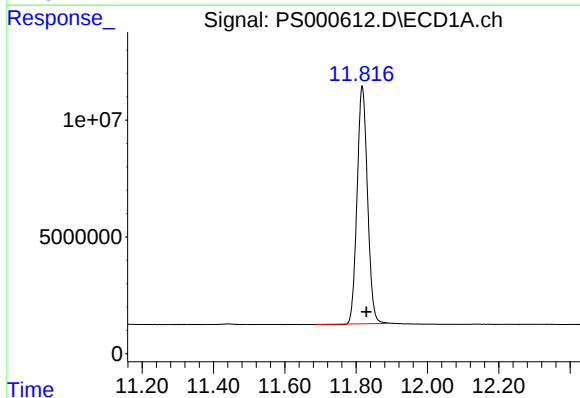


#4 2,4-DCAA

R.T.: 11.817 min
Delta R.T.: -0.012 min
Response: 205748052
Conc: 546.25 ng/ml

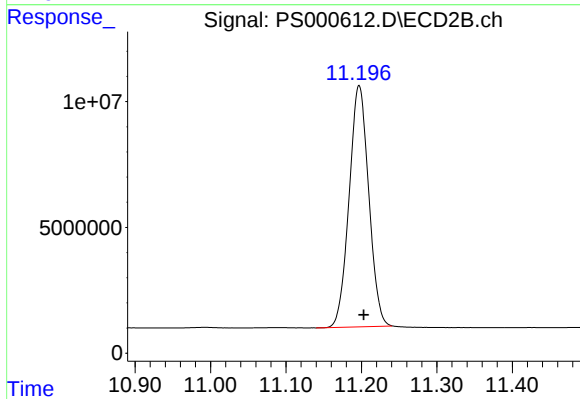

#4 2,4-DCAA


R.T.: 11.197 min
Delta R.T.: -0.006 min
Response: 173180944
Conc: 508.89 ng/ml

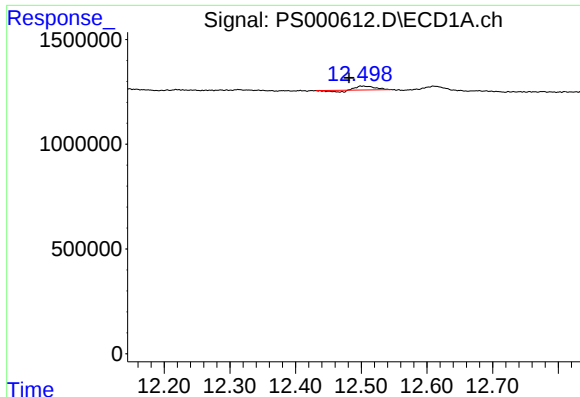

#6 MCPP


R.T.: 12.505 min
Delta R.T.: 0.023 min
Response: 287250
Conc: 0.25 ug/ml

Instrument :
ECD_S
ClientSampleId :

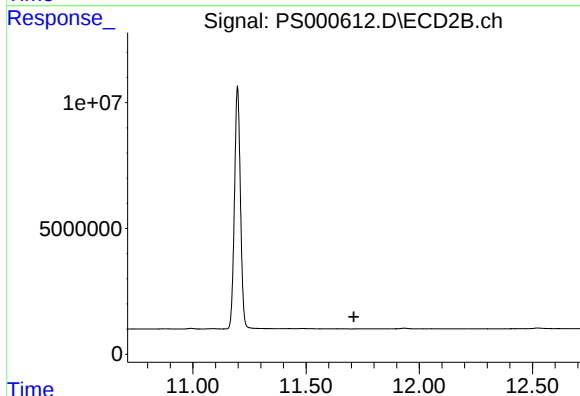


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

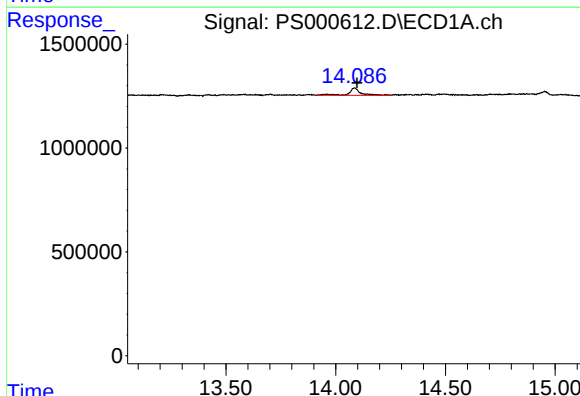


#10 Pentachlorophenol

R.T.: 14.085 min
Delta R.T.: -0.012 min
Response: 1390739
Conc: 0.26 ng/ml

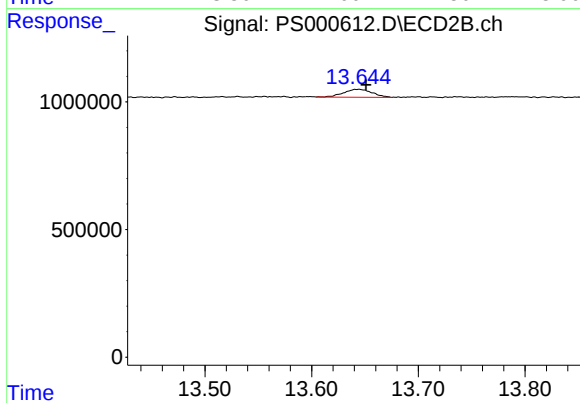

#10 Pentachlorophenol


R.T.: 13.645 min
Delta R.T.: -0.006 min
Response: 585481
Conc: 0.12 ng/ml

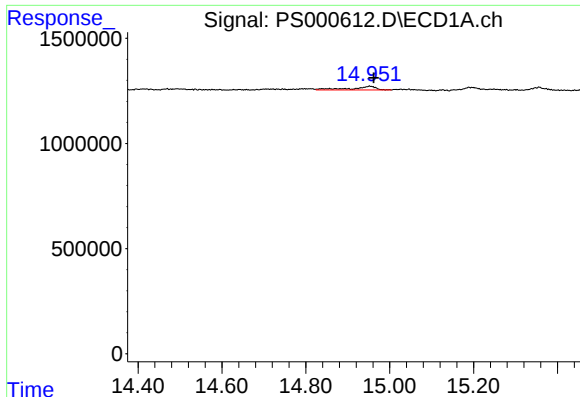

#11 2,4,5-TP (SILVEX)


R.T.: 14.952 min
Delta R.T.: -0.010 min
Response: 706894
Conc: 0.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

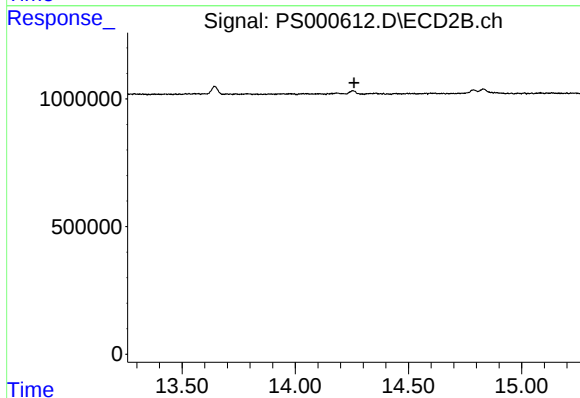


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.259 min
Response: 0
Conc: N.D.

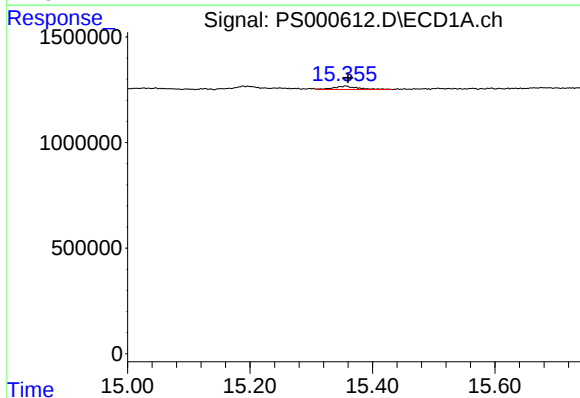


#12 2,4,5-T

R.T.: 15.355 min
Delta R.T.: -0.005 min
Response: 427319
Conc: 0.20 ng/ml

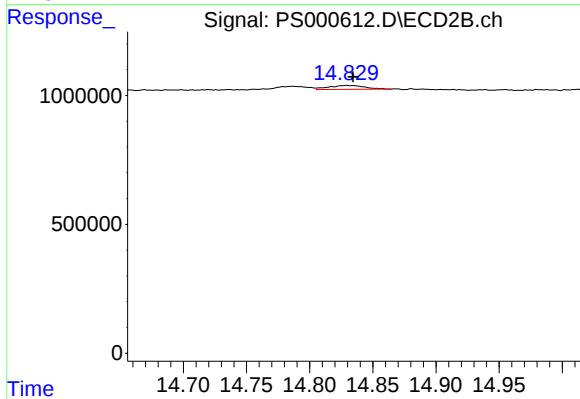

#12 2,4,5-T


R.T.: 14.829 min
Delta R.T.: -0.005 min
Response: 303162
Conc: 0.18 ng/ml

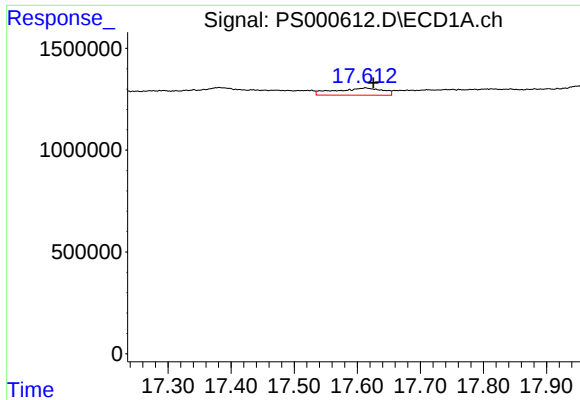

#14 DINOSEB


R.T.: 17.612 min
Delta R.T.: -0.013 min
Response: 1842455
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

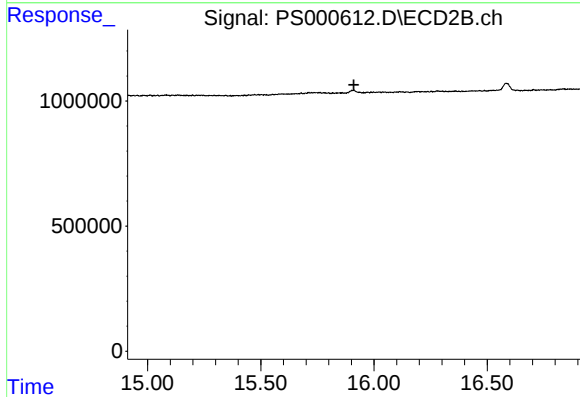


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.911 min
Response: 0
Conc: N.D.

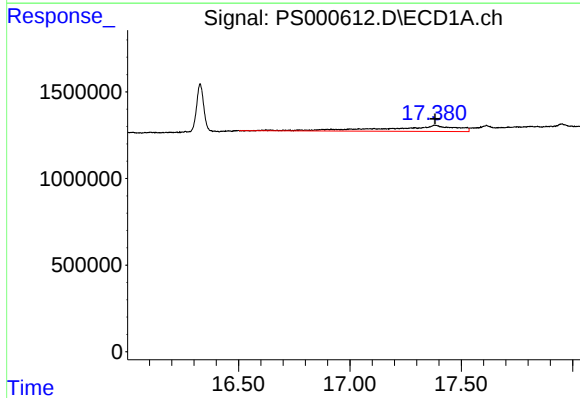


#15 Picloram

R.T.: 17.382 min
Delta R.T.: 0.000 min
Response: 7300360
Conc: 2.50 ng/ml

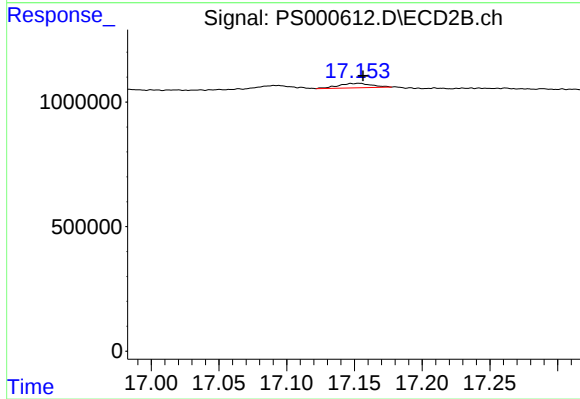

#15 Picloram


R.T.: 17.153 min
Delta R.T.: -0.003 min
Response: 307293
Conc: 0.12 ng/ml

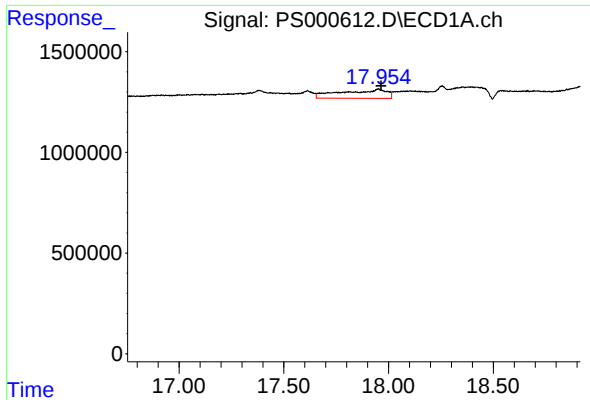

#16 DCPA

R.T.: 17.951 min
Delta R.T.: -0.014 min
Response: 6690878
Conc: 2.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

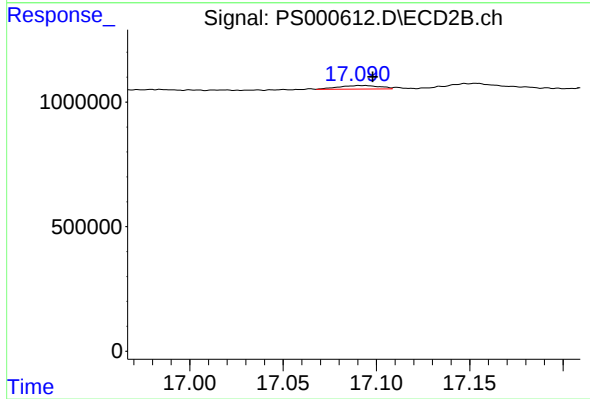

#16 DCPA

R.T.: 17.090 min
Delta R.T.: -0.008 min
Response: 214913
Conc: 0.09 ng/ml