

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062318\
 Data File : PS000623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2018 21:59
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:25:05 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.815	11.179	208.8E6	177.3E6	554.443	521.087
Target Compounds							
3) T	4-Nitroph...	11.439	0.000	667472	0	2.839	N.D. #
6) T	MCP	12.497	0.000	6657645	0	5.879	N.D. #
10) T	Pentachlo...	14.084	13.629	1452242	332330	0.277	0.070 #
11) T	2,4,5-TP ...	14.949	0.000	696132	0	0.321	N.D. #
12) T	2,4,5-T	15.356	14.816	531933	138406	0.247	0.082 #
14) T	DINOSEB	17.609	0.000	1442525	0	0.969	N.D. #
15) T	Picloram	17.381	17.133	5568953	258830	1.907	0.104 #
16) T	DCPA	17.950	17.072	2139065	194415	0.835	0.084 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062318\
Data File : PS000623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2018 21:59
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:25:05 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

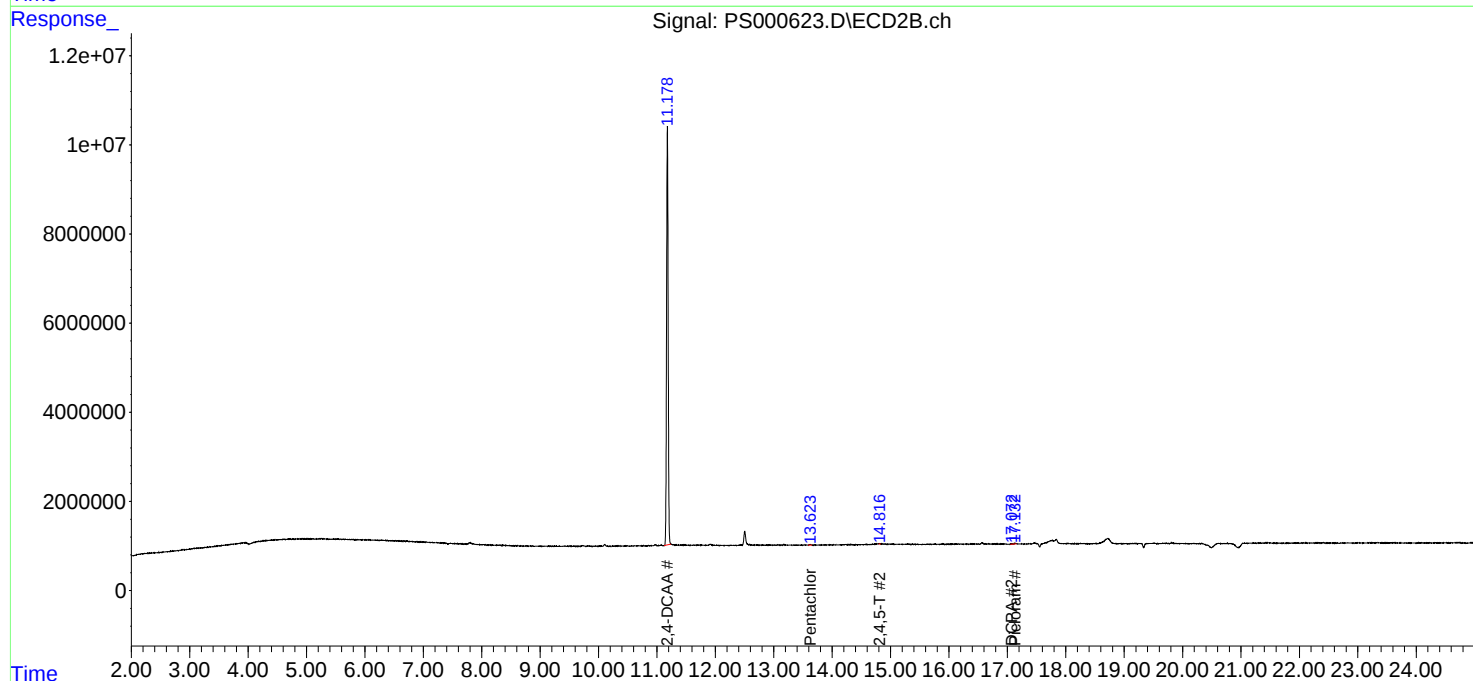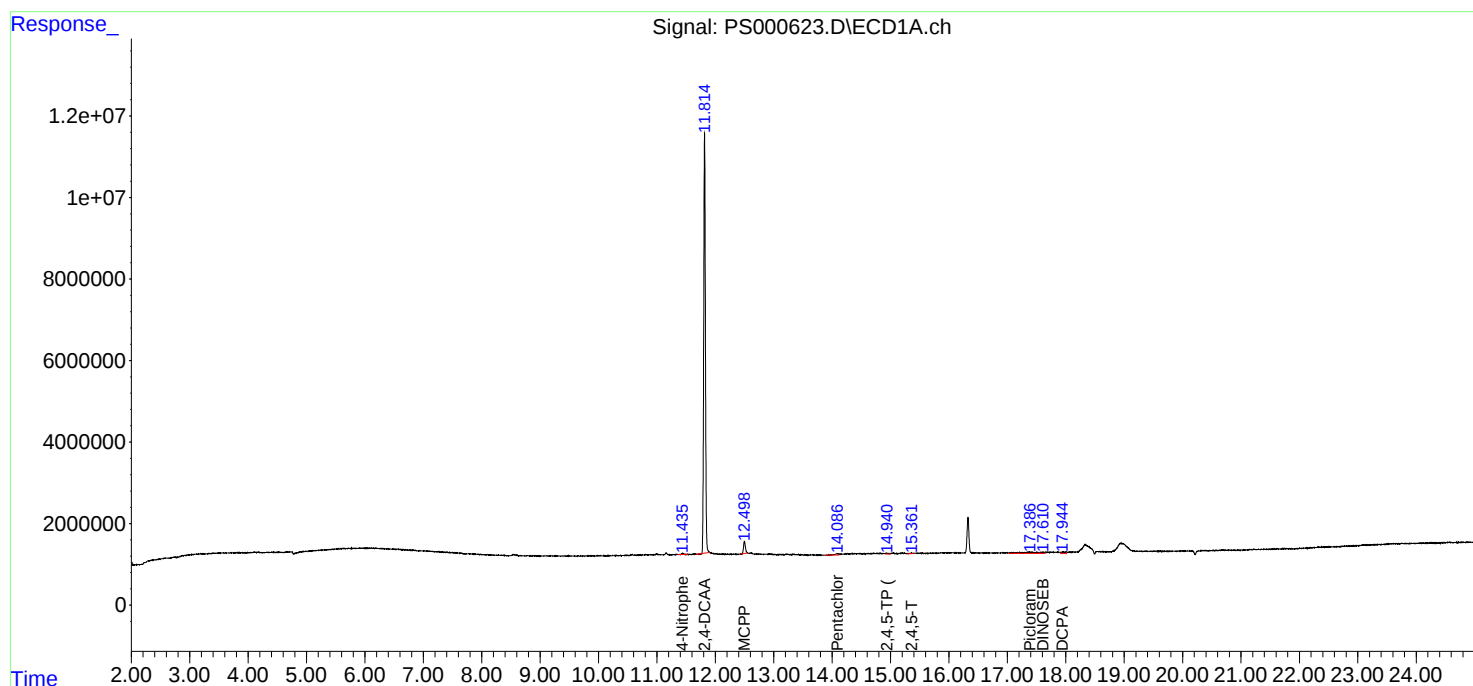


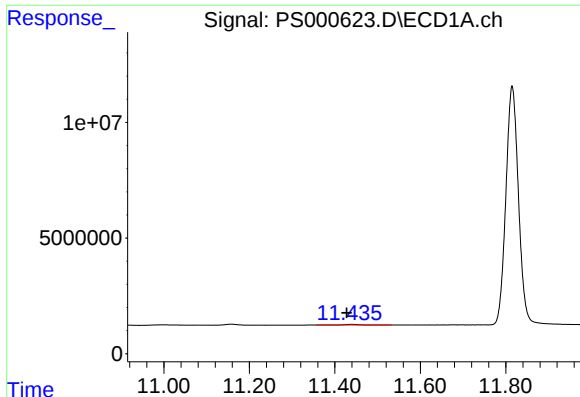

#3 4-Nitrophenol


R.T.: 11.439 min
Delta R.T.: 0.011 min
Response: 667472
Conc: 2.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

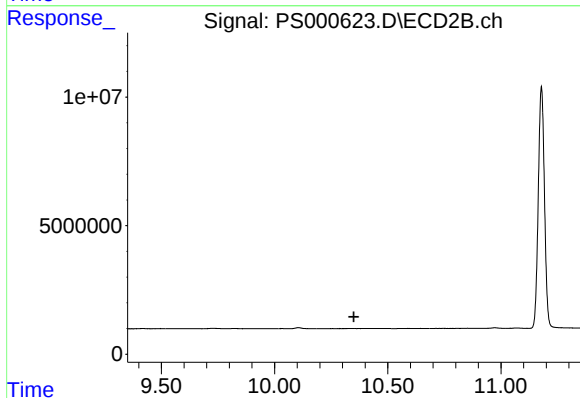


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.350 min
Response: 0
Conc: N.D.

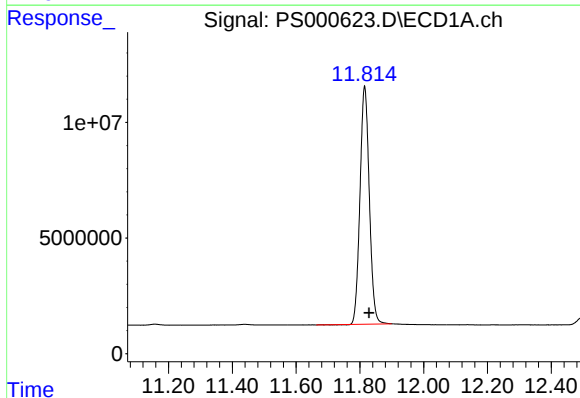


#4 2,4-DCAA

R.T.: 11.815 min
Delta R.T.: -0.014 min
Response: 208833786
Conc: 554.44 ng/ml

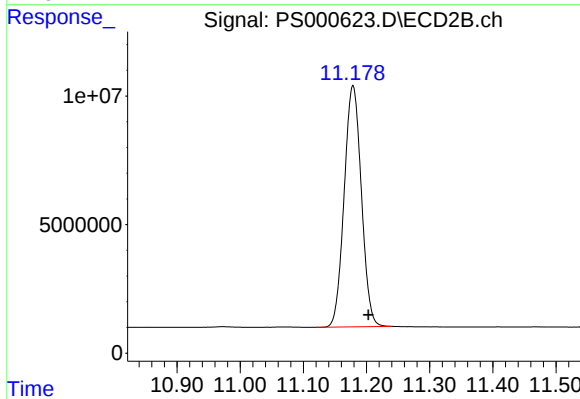

#4 2,4-DCAA


R.T.: 11.179 min
Delta R.T.: -0.024 min
Response: 177330667
Conc: 521.09 ng/ml

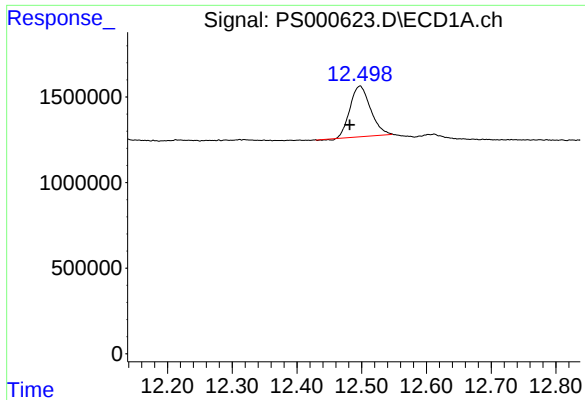

#6 MCP


R.T.: 12.497 min
Delta R.T.: 0.016 min
Response: 6657645
Conc: 5.88 ug/ml

Instrument :
ECD_S
ClientSampleId :

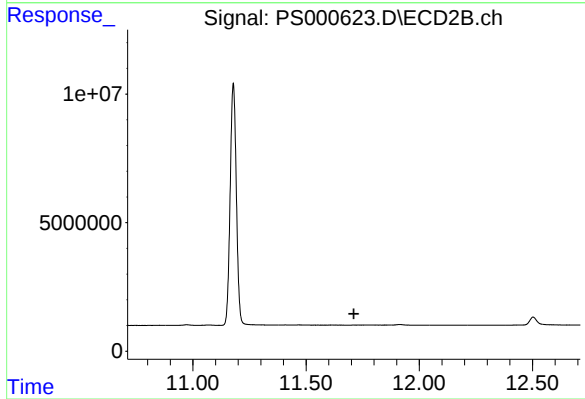


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

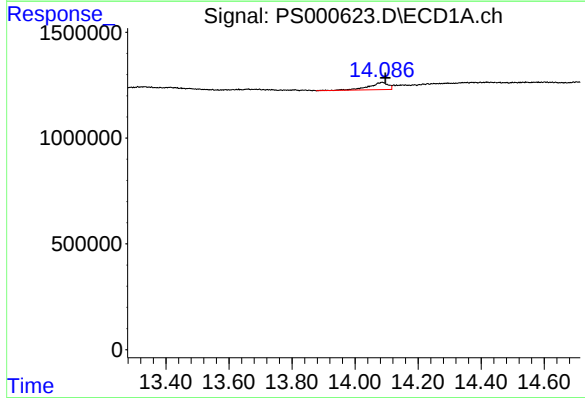


#10 Pentachlorophenol

R.T.: 14.084 min
Delta R.T.: -0.013 min
Response: 1452242
Conc: 0.28 ng/ml

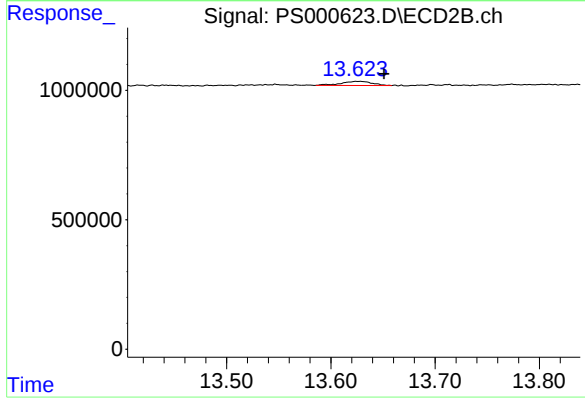

#10 Pentachlorophenol


R.T.: 13.629 min
Delta R.T.: -0.022 min
Response: 332330
Conc: 0.07 ng/ml

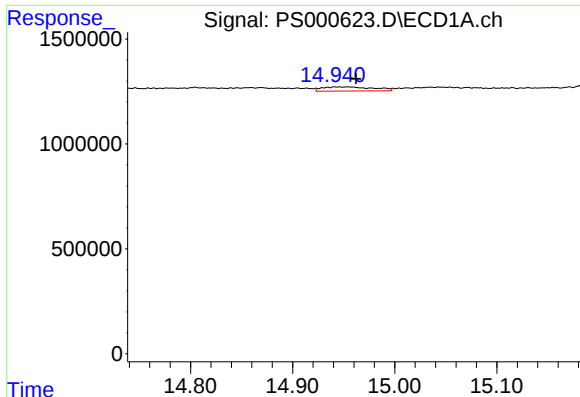

#11 2,4,5-TP (SILVEX)


R.T.: 14.949 min
Delta R.T.: -0.013 min
Response: 696132
Conc: 0.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

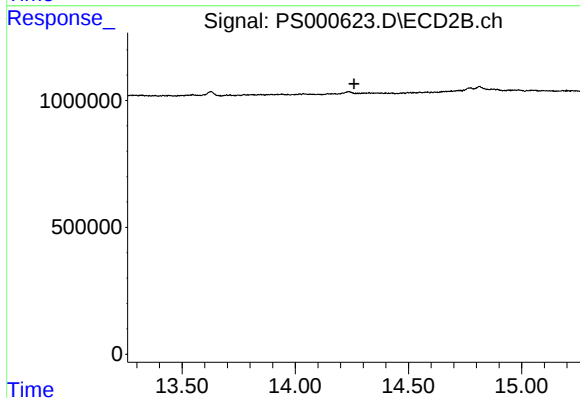


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.259 min
Response: 0
Conc: N.D.

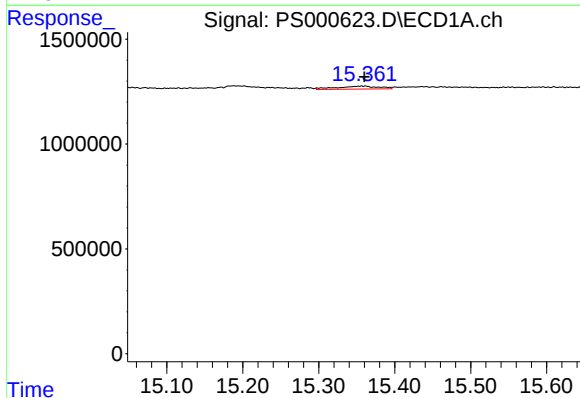


#12 2,4,5-T

R.T.: 15.356 min
Delta R.T.: -0.004 min
Response: 531933
Conc: 0.25 ng/ml

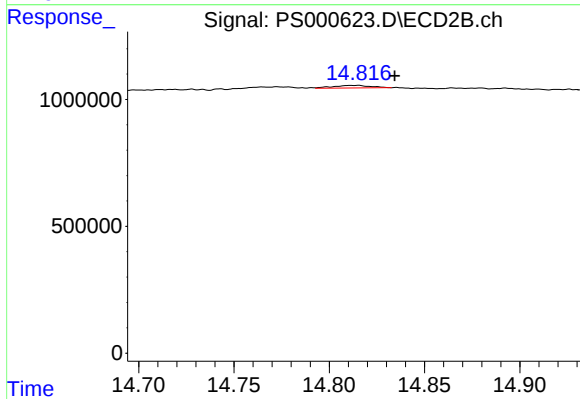

#12 2,4,5-T


R.T.: 14.816 min
Delta R.T.: -0.019 min
Response: 138406
Conc: 0.08 ng/ml

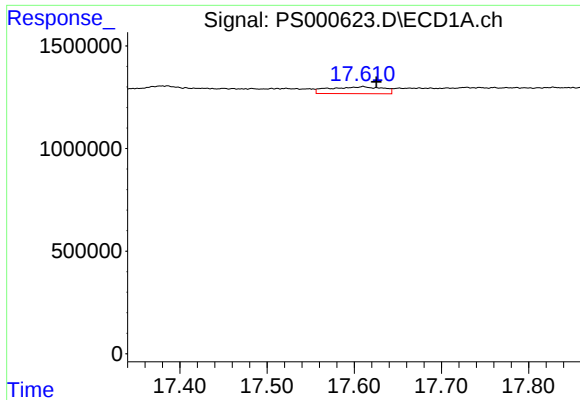

#14 DINOSEB


R.T.: 17.609 min
Delta R.T.: -0.017 min
Response: 1442525
Conc: 0.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

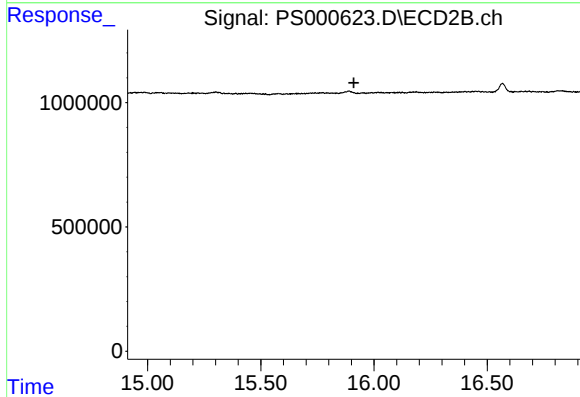


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.911 min
Response: 0
Conc: N.D.

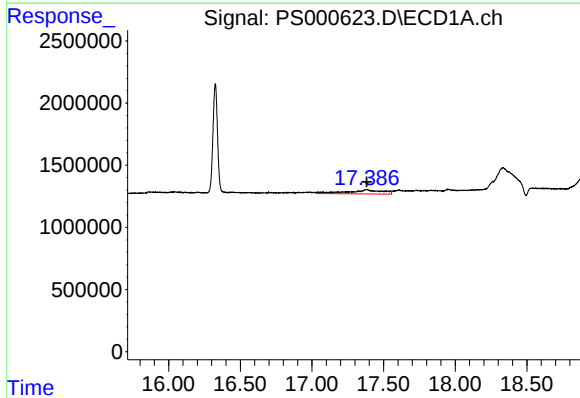


#15 Picloram

R.T.: 17.381 min
Delta R.T.: -0.001 min
Response: 5568953
Conc: 1.91 ng/ml

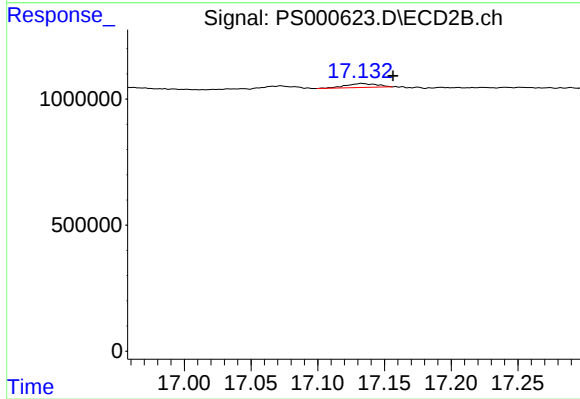

#15 Picloram


R.T.: 17.133 min
Delta R.T.: -0.024 min
Response: 258830
Conc: 0.10 ng/ml

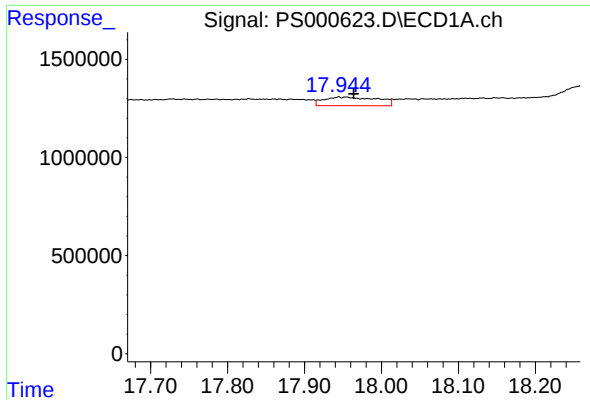

#16 DCPA

R.T.: 17.950 min
Delta R.T.: -0.014 min
Response: 2139065
Conc: 0.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

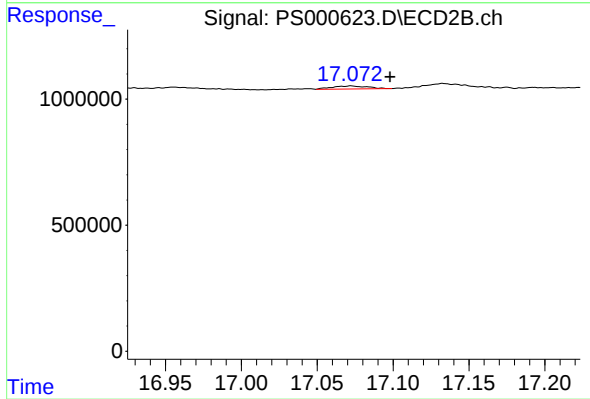

#16 DCPA

R.T.: 17.072 min
Delta R.T.: -0.026 min
Response: 194415
Conc: 0.08 ng/ml