

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062323\
 Data File : PS023373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 09:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 14:20:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.481	6.853	925.2E6	290.0E6	522.945	510.758
Target Compounds							
3) T	4-Nitroph...	6.316	0.000	7214246	0	5.598	N.D. #
6) T	MCP	6.819	0.000	1123981	0	<MDL	N.D. #
7) T	MCPA	6.854f	0.000	121476	0	<MDL	N.D. #
8) T	DICHLORPROP	7.290f	7.660	724208	1125069	<MDL	1.819 #
11) T	2,4,5-TP ...	8.211	0.000	2654139	0	<MDL	N.D. #
12) T	2,4,5-T	8.479	9.138f	1929940	1432354	<MDL	<MDL #
13) T	2,4-DB	8.932f	0.000	12778496	0	5.428	N.D. #
14) T	DINOSEB	10.065	0.000	1017189	0	<MDL	N.D. #
15) T	Picloram	9.889	10.894	46518334	8298572	2.680	1.818 #
16) T	DCPA	10.331	10.894	1983225	8298572	<MDL	2.069 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062323\
Data File : PS023373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 09:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 14:20:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

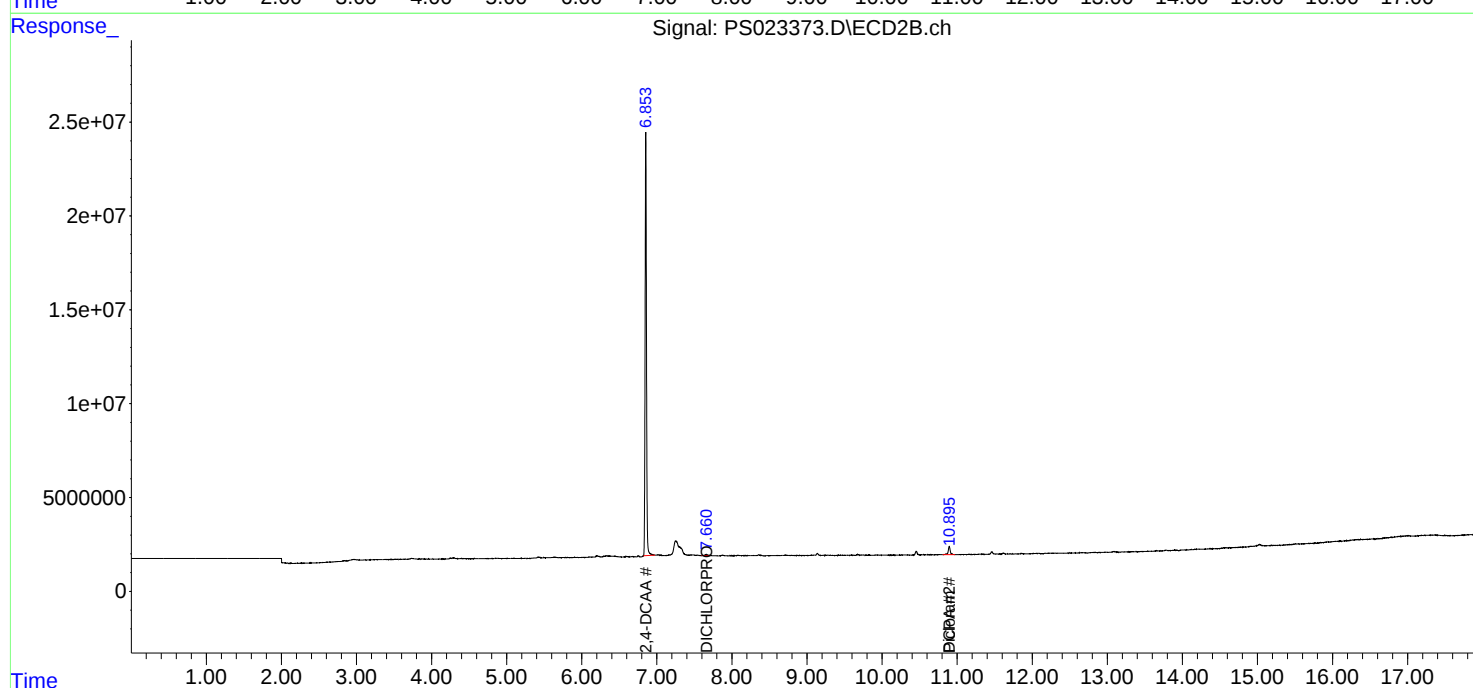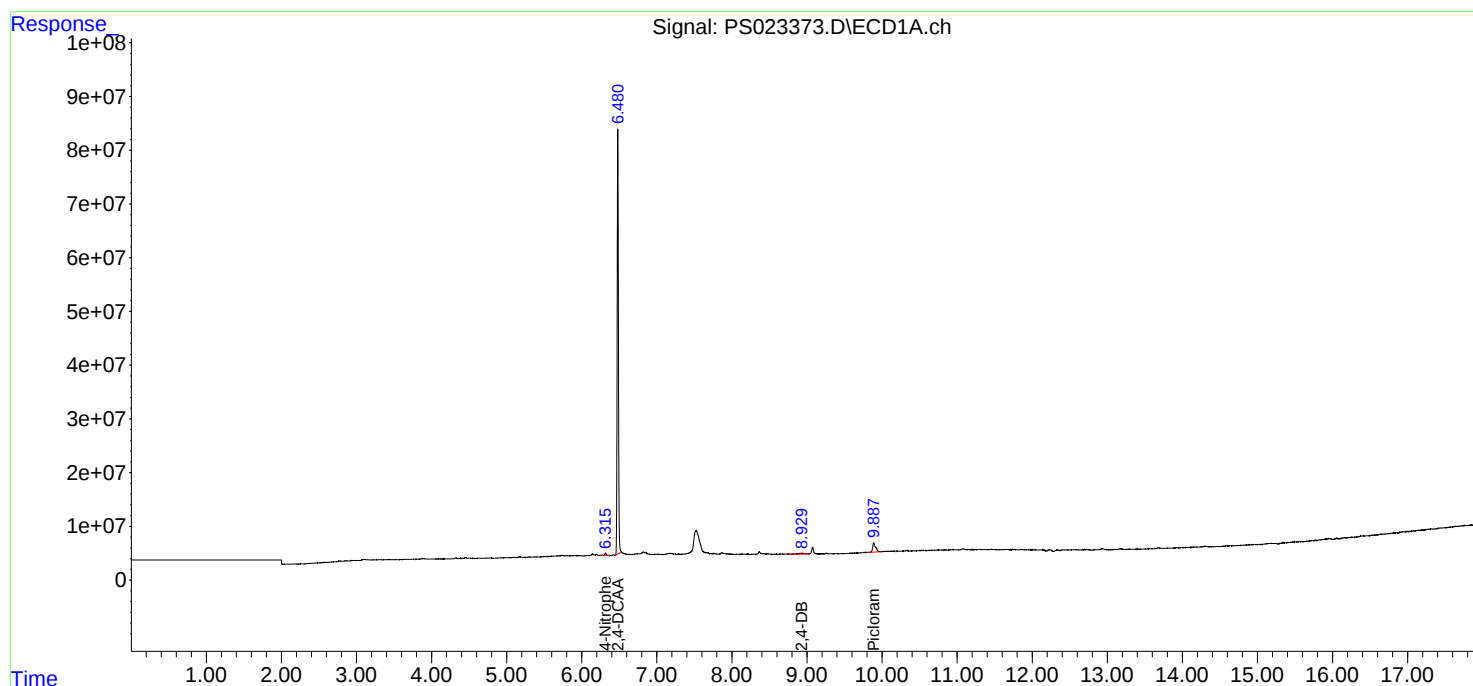


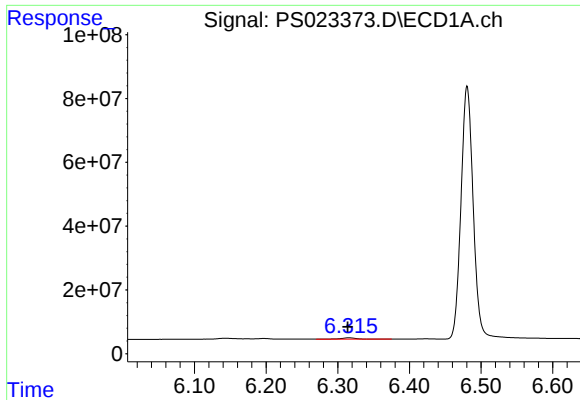

#3 4-Nitrophenol


R.T.: 6.316 min
Delta R.T.: 0.002 min
Response: 7214246
Conc: 5.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

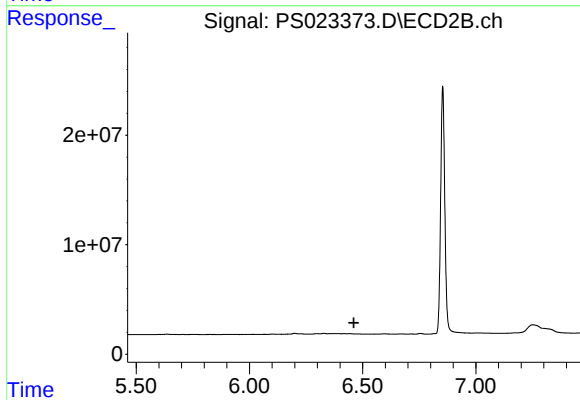


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

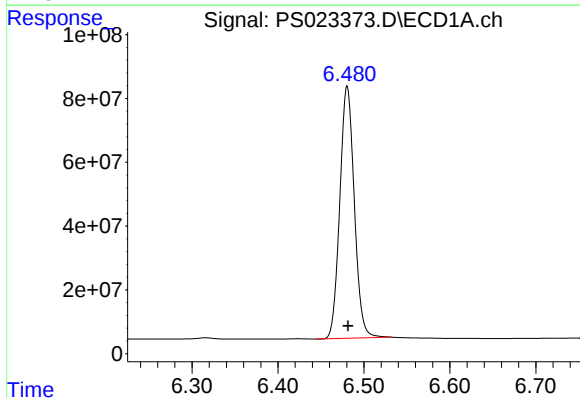


#4 2,4-DCAA

R.T.: 6.481 min
Delta R.T.: -0.001 min
Response: 925223552
Conc: 522.94 ng/ml

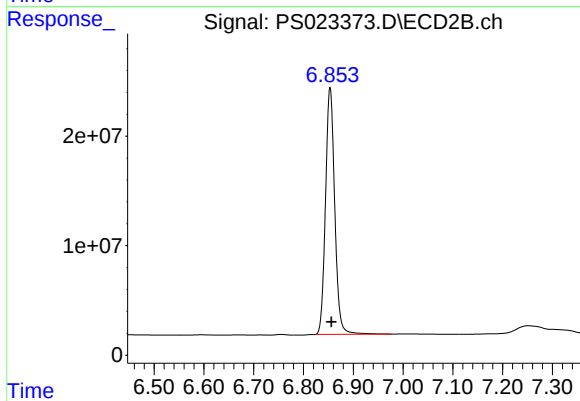

#4 2,4-DCAA


R.T.: 6.853 min
Delta R.T.: -0.003 min
Response: 289955141
Conc: 510.76 ng/ml

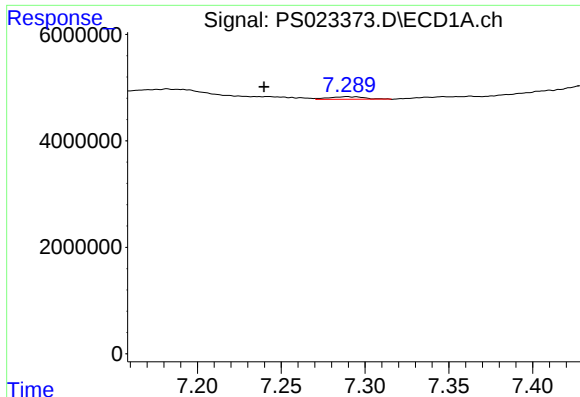

#8 DICHLORPROP


R.T.: 7.290 min
Delta R.T.: 0.050 min
Response: 724208
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

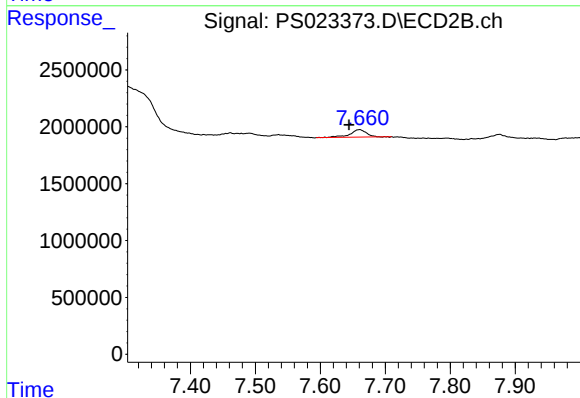


#8 DICHLORPROP

R.T.: 7.660 min
Delta R.T.: 0.016 min
Response: 1125069
Conc: 1.82 ng/ml

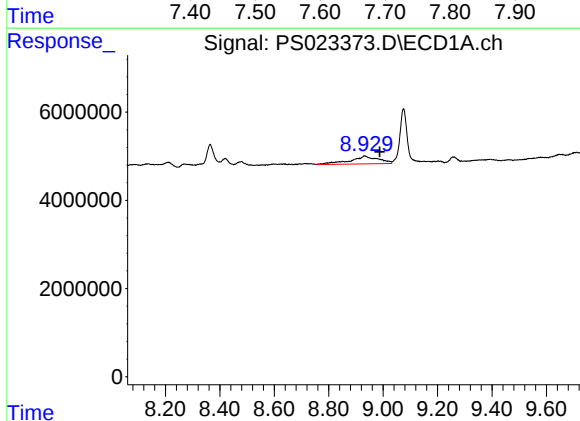


#13 2,4-DB

R.T.: 8.932 min
Delta R.T.: -0.055 min
Response: 12778496
Conc: 5.43 ng/ml

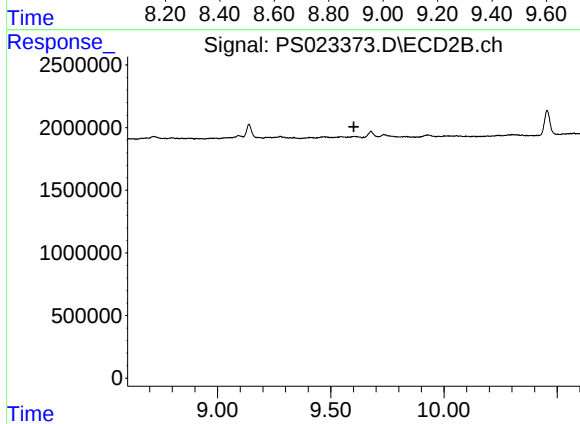

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.

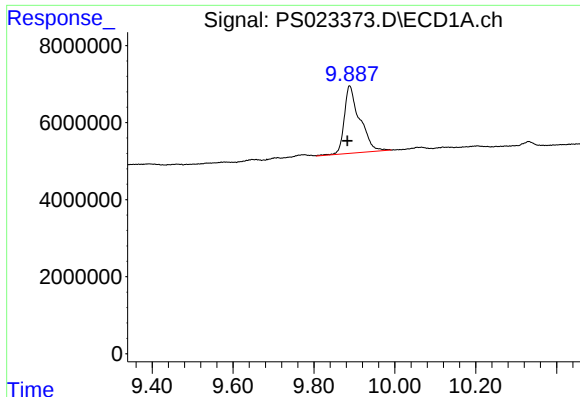

#15 Picloram


R.T.: 9.889 min
Delta R.T.: 0.006 min
Response: 46518334
Conc: 2.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

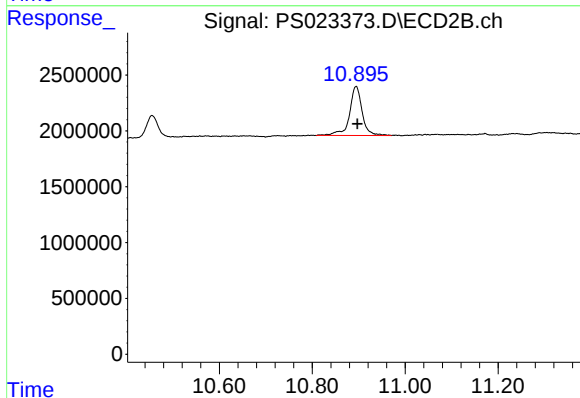


#15 Picloram

R.T.: 10.894 min
Delta R.T.: -0.003 min
Response: 8298572
Conc: 1.82 ng/ml

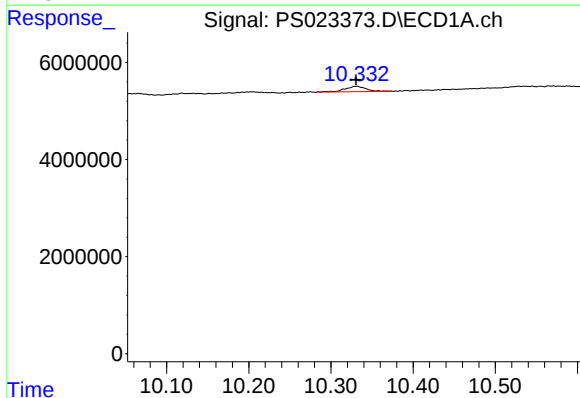

#16 DCPA

R.T.: 10.331 min
Delta R.T.: 0.000 min
Response: 1983225
Conc: N.D.

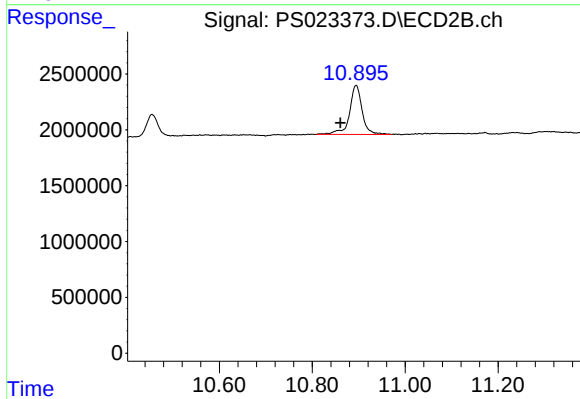

#16 DCPA

R.T.: 10.894 min
Delta R.T.: 0.034 min
Response: 8298572
Conc: 2.07 ng/ml