

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062323\
 Data File : PS023378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 13:13
 Operator : AR\AJ
 Sample : 03327-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 14:22:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.479	6.853	496.3E6	87903258	280.489	154.842 #
Target Compounds							
1) T	Dalapon	2.513	0.000	57925191	0	31.679	N.D. #
3) T	4-Nitroph...	6.335	6.484	5607084	17634909	4.351	51.691 #
5) T	DICAMBA	6.652	7.002	662910	3445012	<MDL	1.344 #
6) T	MCP	6.809	7.100	62608298	4616135	11.360	2.582 #
7) T	MCPA	6.923	7.322	-22942762	14244750	N.D.	5.300
8) T	DICHLORPROP	7.221	7.655	14707712	16776902	7.127	27.121 #
9) T	2,4-D	7.443	7.930	34708794	3770403	14.206	5.437 #
10) T	Pentachlo...	7.680	8.383	76615735	3389989	2.719	<MDL #
11) T	2,4,5-TP ...	8.201	8.720	57911230	4592776	5.008	1.376 #
12) T	2,4,5-T	8.498	9.079	58610466	14432196	5.159	4.708
13) T	2,4-DB	8.989	9.595	119.9E6	16958019	50.950	45.733
15) T	Picloram	9.884	10.895	66555677	12076419	3.835	2.646 #
16) T	DCPA	10.391f	10.856	40521918	7254414	2.907	1.808 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062323\
Data File : PS023378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 13:13
Operator : AR\AJ
Sample : 03327-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 14:22:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

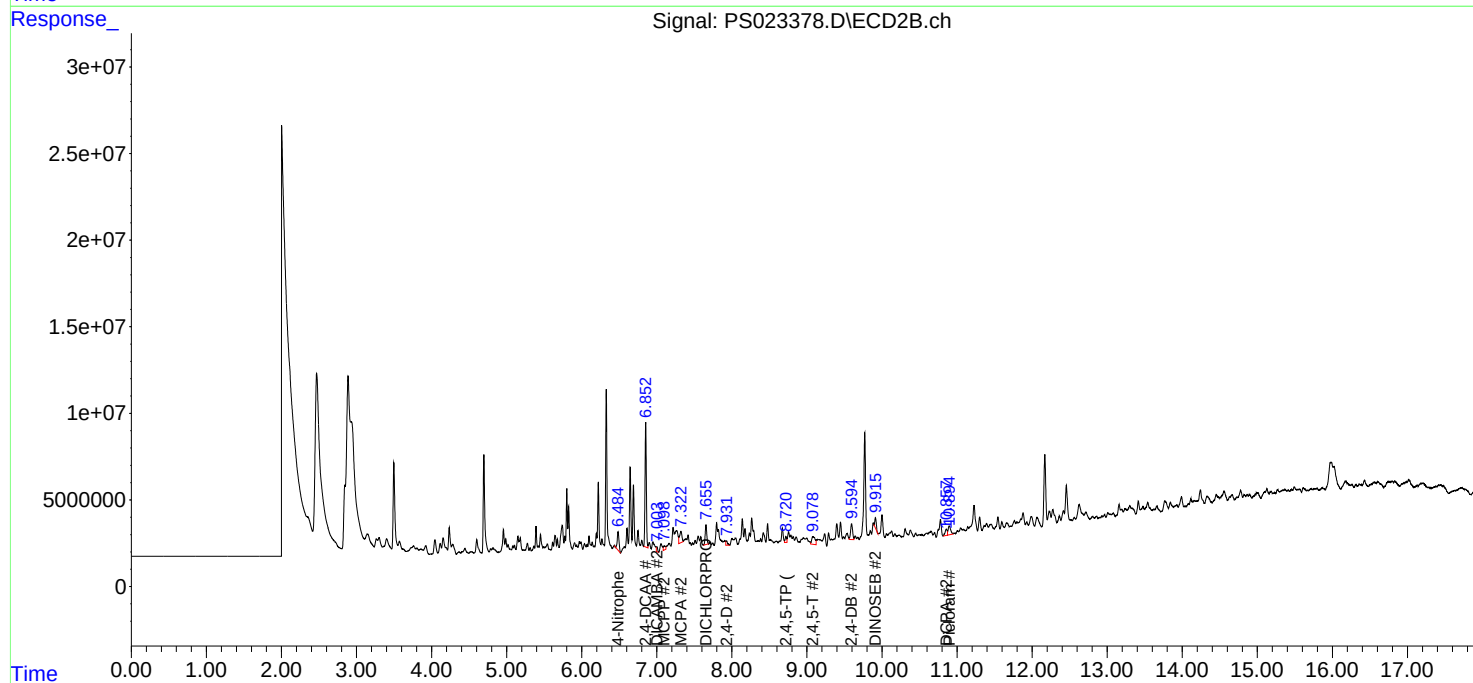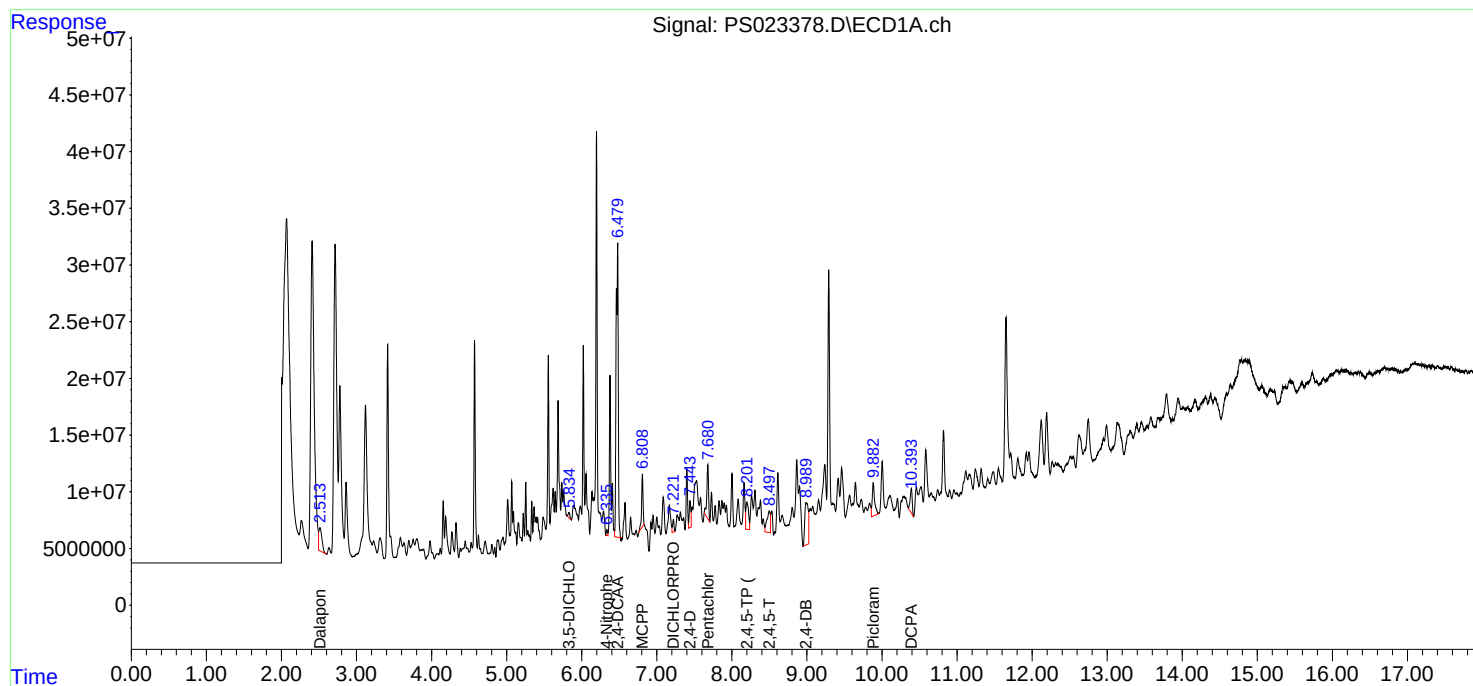


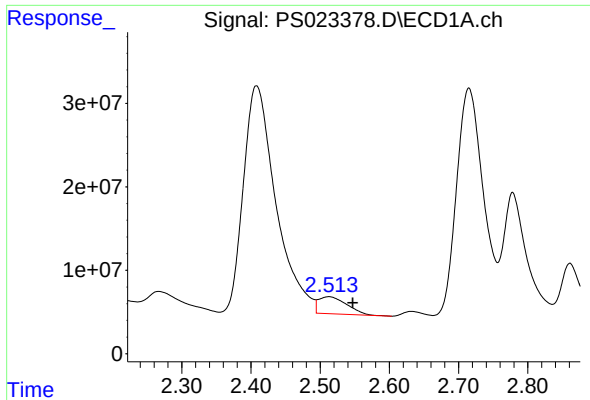

#1 Dalapon


R.T.: 2.513 min
Delta R.T.: -0.034 min
Response: 57925191
Conc: 31.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

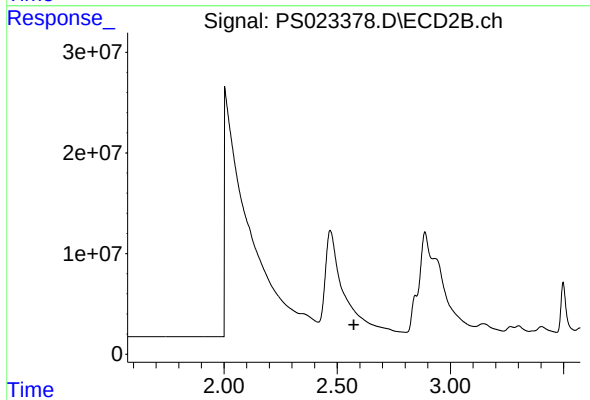


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

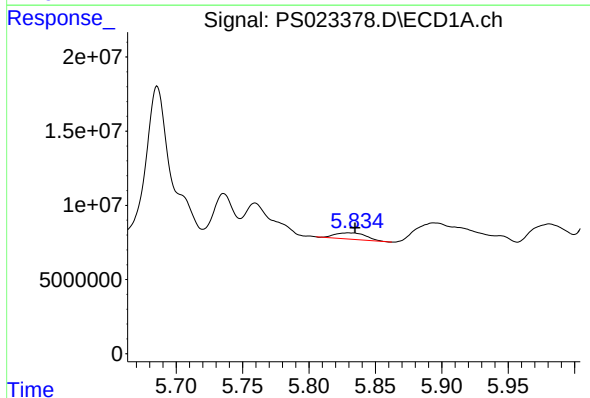


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.830 min
Delta R.T.: -0.004 min
Response: 6921874
Conc: 2.58 ng/ml

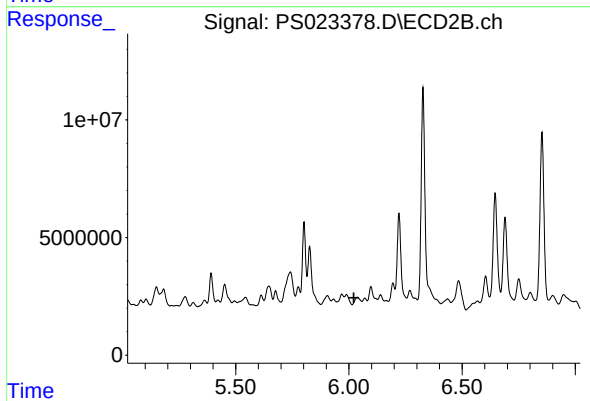

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.037 min
Delta R.T.: 0.015 min
Response: -2360023
Conc: N.D.

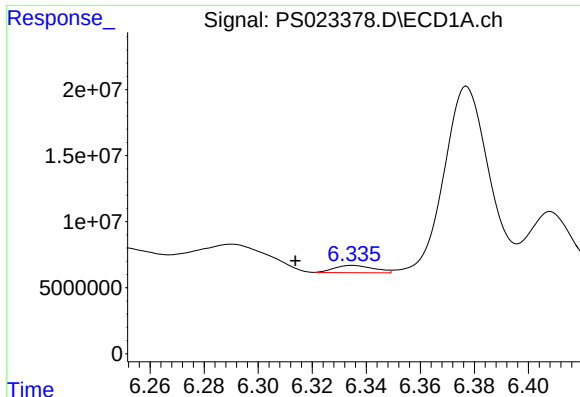

#3 4-Nitrophenol


R.T.: 6.335 min
Delta R.T.: 0.021 min
Response: 5607084
Conc: 4.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

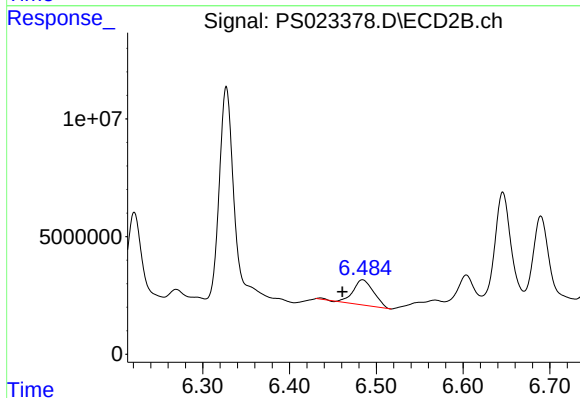


#3 4-Nitrophenol

R.T.: 6.484 min
Delta R.T.: 0.023 min
Response: 17634909
Conc: 51.69 ng/ml

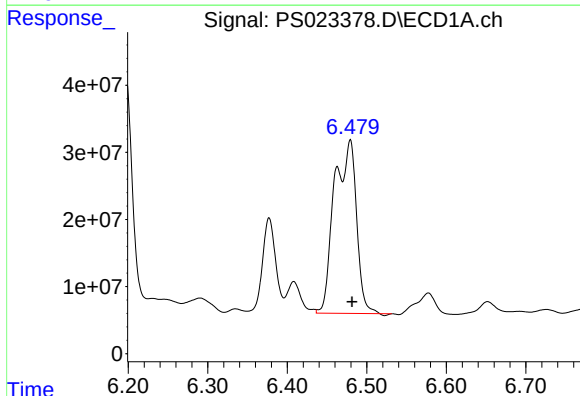


#4 2,4-DCAA

R.T.: 6.479 min
Delta R.T.: -0.003 min
Response: 496256558
Conc: 280.49 ng/ml

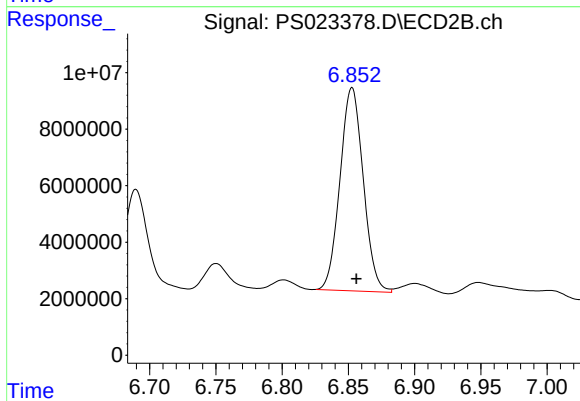

#4 2,4-DCAA


R.T.: 6.853 min
Delta R.T.: -0.003 min
Response: 87903258
Conc: 154.84 ng/ml

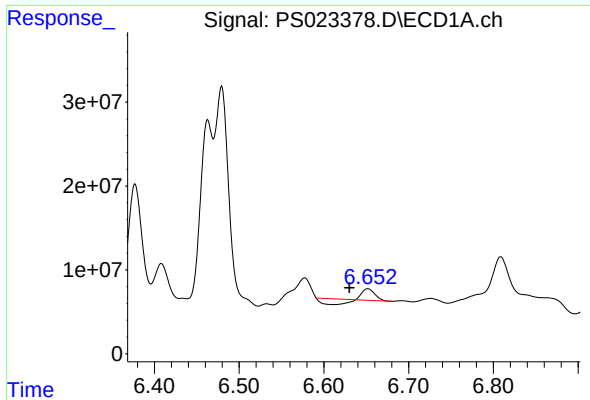

#5 DICAMBA


R.T.: 6.652 min
Delta R.T.: 0.022 min
Response: 662910
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

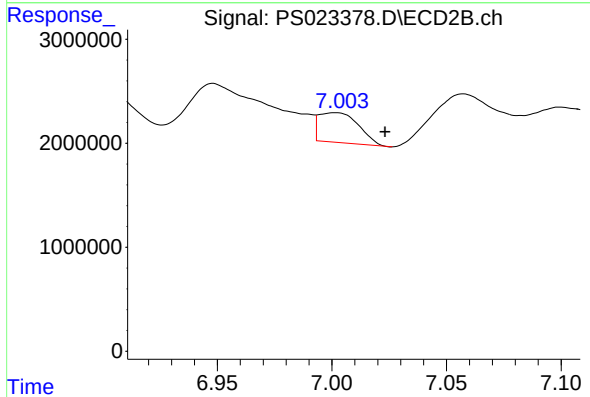


#5 DICAMBA

R.T.: 7.002 min
Delta R.T.: -0.021 min
Response: 3445012
Conc: 1.34 ng/ml

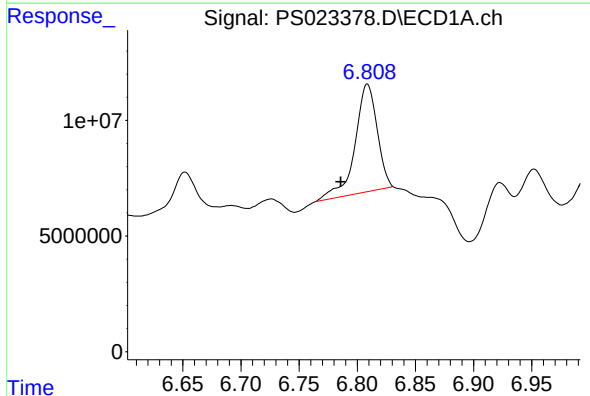


#6 MCP

R.T.: 6.809 min
Delta R.T.: 0.023 min
Response: 62608298
Conc: 11.36 ug/ml

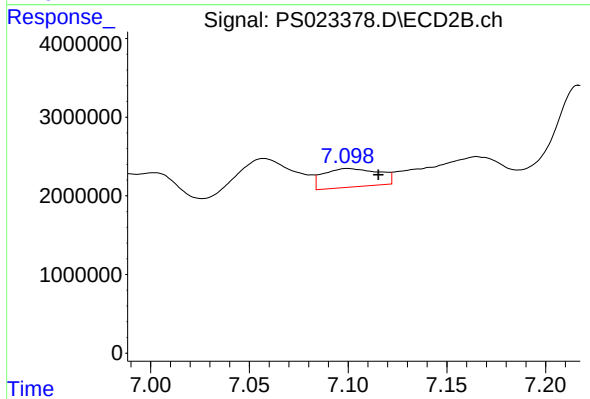

#6 MCP


R.T.: 7.100 min
Delta R.T.: -0.016 min
Response: 4616135
Conc: 2.58 ug/ml

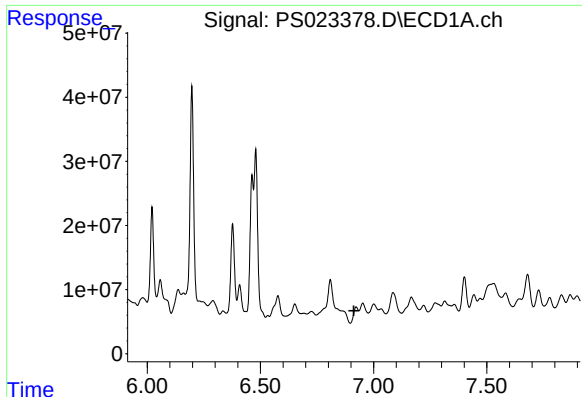

#7 MCPA


R.T.: 6.923 min
Delta R.T.: 0.010 min
Response: -22942762
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

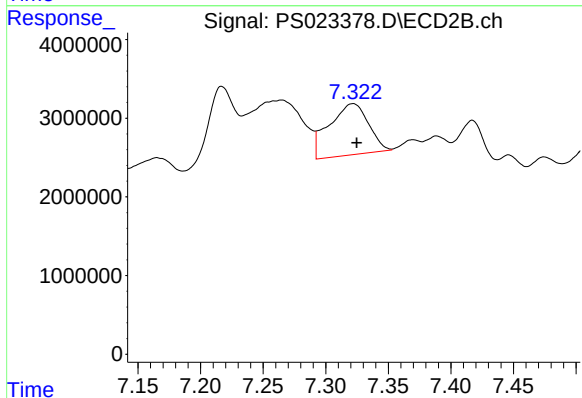


#7 MCPA

R.T.: 7.322 min
Delta R.T.: -0.003 min
Response: 14244750
Conc: 5.30 ug/ml

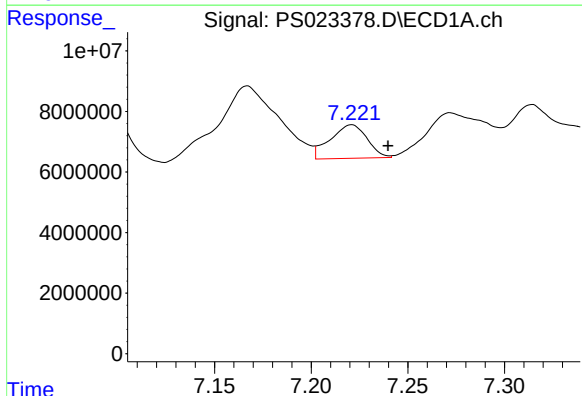


#8 DICHLORPROP

R.T.: 7.221 min
Delta R.T.: -0.019 min
Response: 14707712
Conc: 7.13 ng/ml

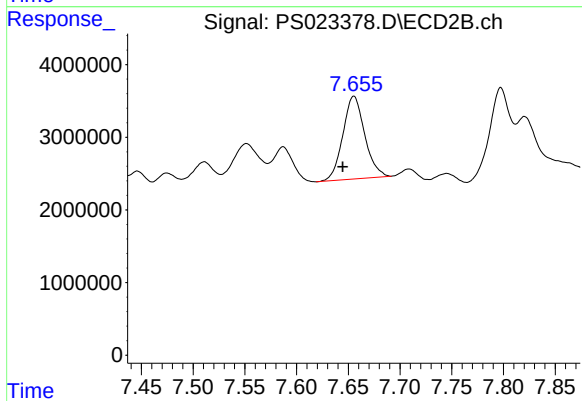

#8 DICHLORPROP


R.T.: 7.655 min
Delta R.T.: 0.011 min
Response: 16776902
Conc: 27.12 ng/ml

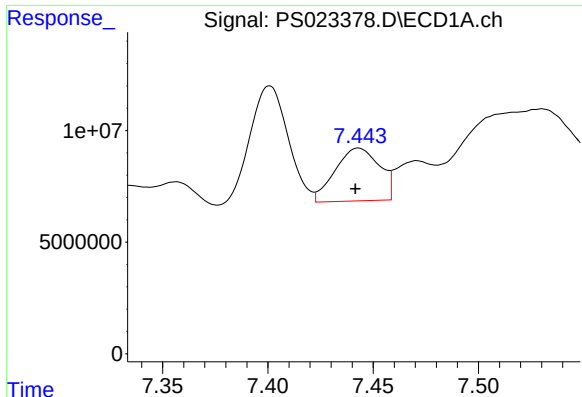

#9 2,4-D


R.T.: 7.443 min
Delta R.T.: 0.002 min
Response: 34708794
Conc: 14.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

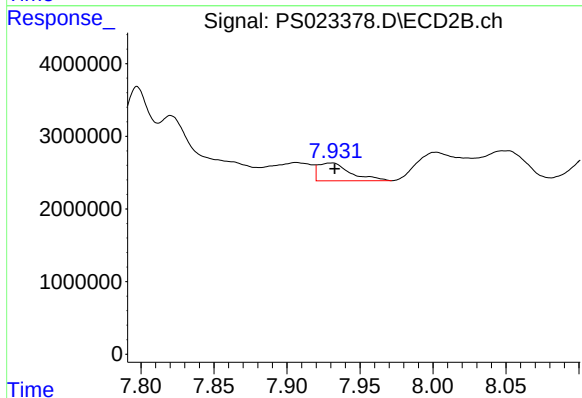


#9 2,4-D

R.T.: 7.930 min
Delta R.T.: -0.003 min
Response: 3770403
Conc: 5.44 ng/ml

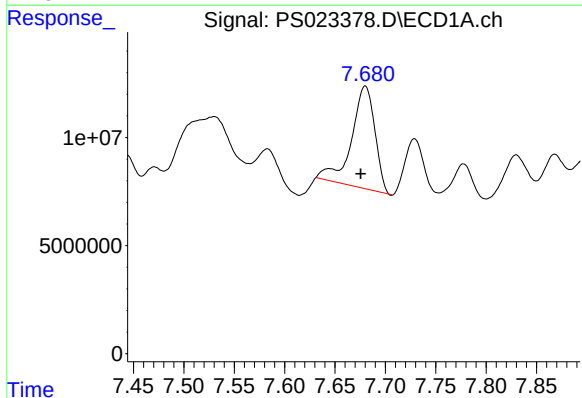


#10 Pentachlorophenol

R.T.: 7.680 min
Delta R.T.: 0.004 min
Response: 76615735
Conc: 2.72 ng/ml

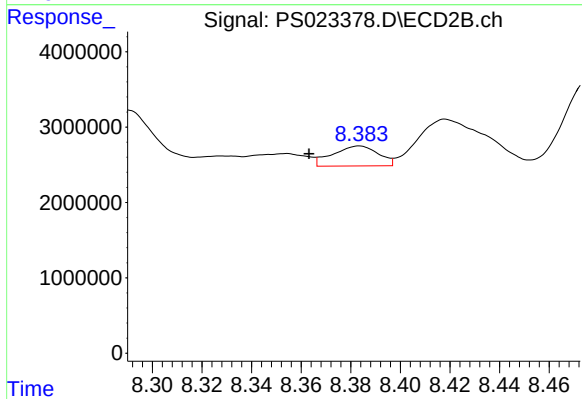

#10 Pentachlorophenol


R.T.: 8.383 min
Delta R.T.: 0.020 min
Response: 3389989
Conc: N.D.

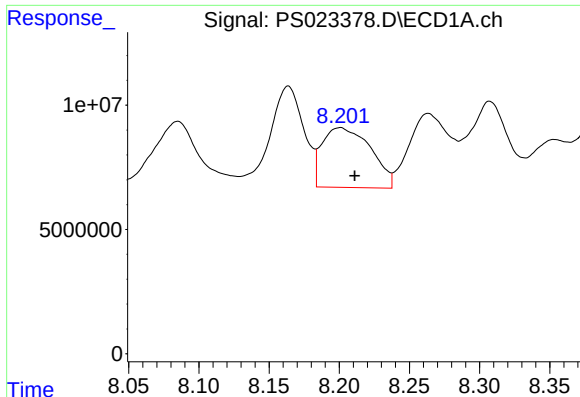

#11 2,4,5-TP (SILVEX)


R.T.: 8.201 min
Delta R.T.: -0.010 min
Response: 57911230
Conc: 5.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

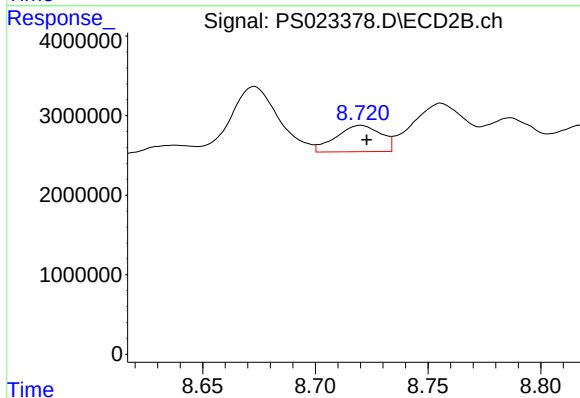


#11 2,4,5-TP (SILVEX)

R.T.: 8.720 min
Delta R.T.: -0.003 min
Response: 4592776
Conc: 1.38 ng/ml

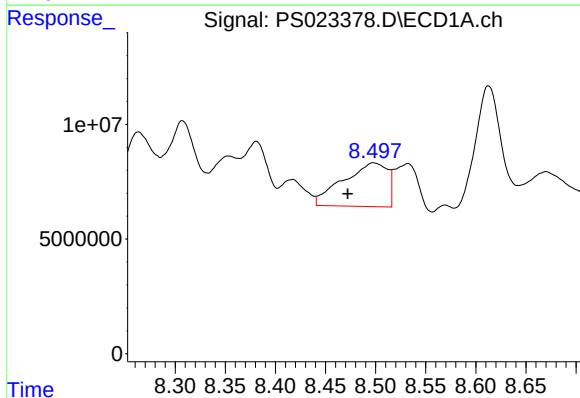


#12 2,4,5-T

R.T.: 8.498 min
Delta R.T.: 0.026 min
Response: 58610466
Conc: 5.16 ng/ml

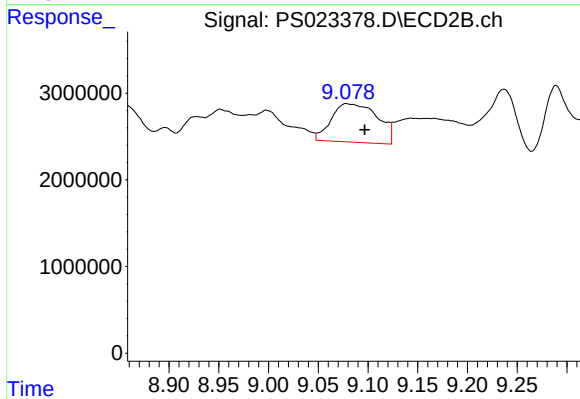

#12 2,4,5-T


R.T.: 9.079 min
Delta R.T.: -0.017 min
Response: 14432196
Conc: 4.71 ng/ml

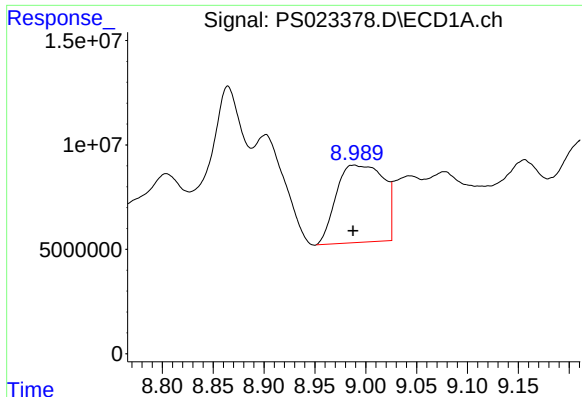

#13 2,4-DB


R.T.: 8.989 min
Delta R.T.: 0.001 min
Response: 119942072
Conc: 50.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

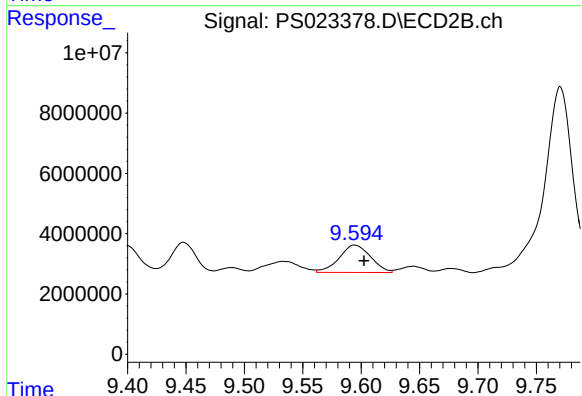


#13 2,4-DB

R.T.: 9.595 min
Delta R.T.: -0.008 min
Response: 16958019
Conc: 45.73 ng/ml

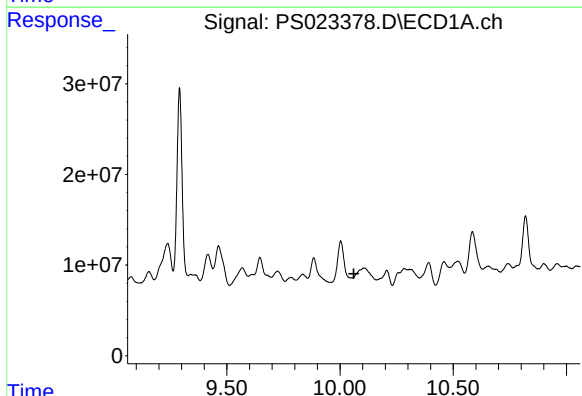


#14 DINOSEB

R.T.: 10.107 min
Delta R.T.: 0.045 min
Response: -83606362
Conc: N.D.

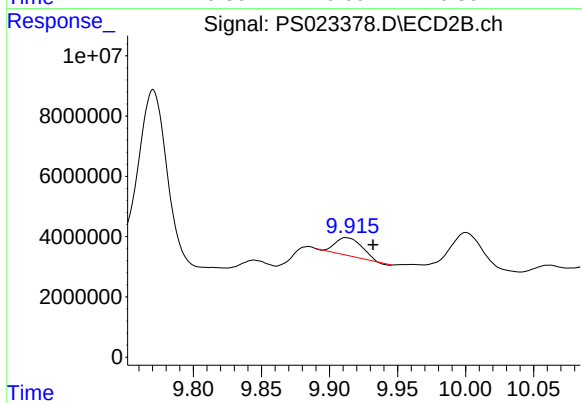

#14 DINOSEB


R.T.: 9.913 min
Delta R.T.: -0.020 min
Response: 7943203
Conc: 3.35 ng/ml

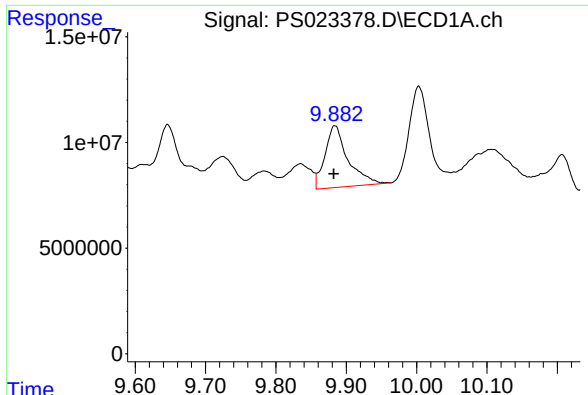

#15 Picloram


R.T.: 9.884 min
Delta R.T.: 0.001 min
Response: 66555677
Conc: 3.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

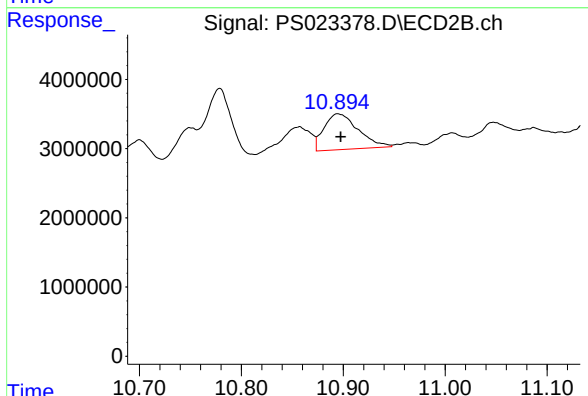


#15 Picloram

R.T.: 10.895 min
Delta R.T.: -0.002 min
Response: 12076419
Conc: 2.65 ng/ml

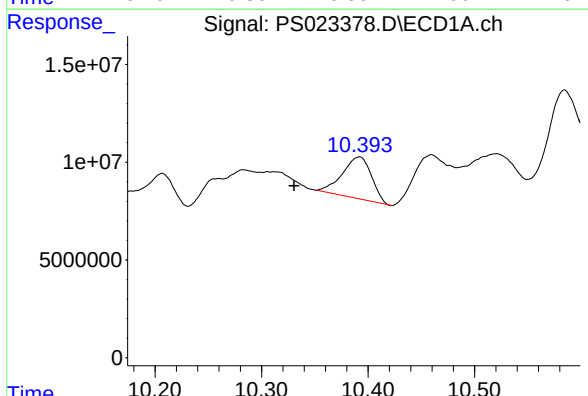

#16 DCPA

R.T.: 10.391 min
Delta R.T.: 0.061 min
Response: 40521918
Conc: 2.91 ng/ml

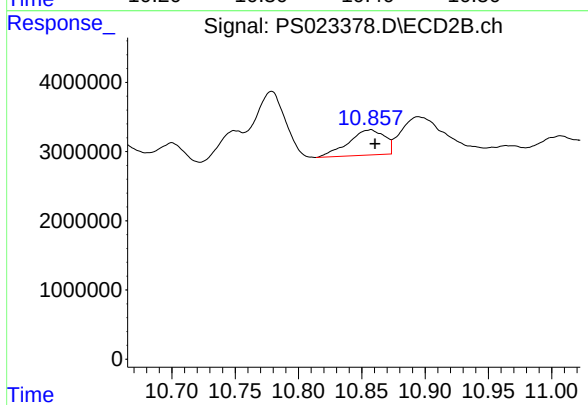

#16 DCPA

R.T.: 10.856 min
Delta R.T.: -0.004 min
Response: 7254414
Conc: 1.81 ng/ml