

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062323\
 Data File : PS023385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 16:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 17:41:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.478	6.853	931.4E6	295.1E6	526.436	519.775
Target Compounds							
2) T	3,5-DICHL...	5.797	0.000	472497	0	<MDL	N.D. #
3) T	4-Nitroph...	6.314	0.000	6027908	0	4.677	N.D. #
6) T	MCP	6.816	0.000	2274556	0	<MDL	N.D. #
7) T	MCPA	6.928	0.000	334120	0	<MDL	N.D. #
8) T	DICHLORPROP	7.241	7.659	823294	1998230	<MDL	3.230 #
10) T	Pentachlo...	7.668	0.000	995920	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.207	0.000	5381670	0	<MDL	N.D. #
12) T	2,4,5-T	8.472	9.137f	3275737	925402	<MDL	<MDL #
13) T	2,4-DB	8.924f	0.000	15941775	0	6.772	N.D. #
14) T	DINOSEB	10.050	0.000	932926	0	<MDL	N.D. #
15) T	Picloram	9.883	10.894	9146969	1776154	<MDL	<MDL #
16) T	DCPA	10.322	10.894	1776769	1776154	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062323\
Data File : PS023385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 16:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 17:41:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

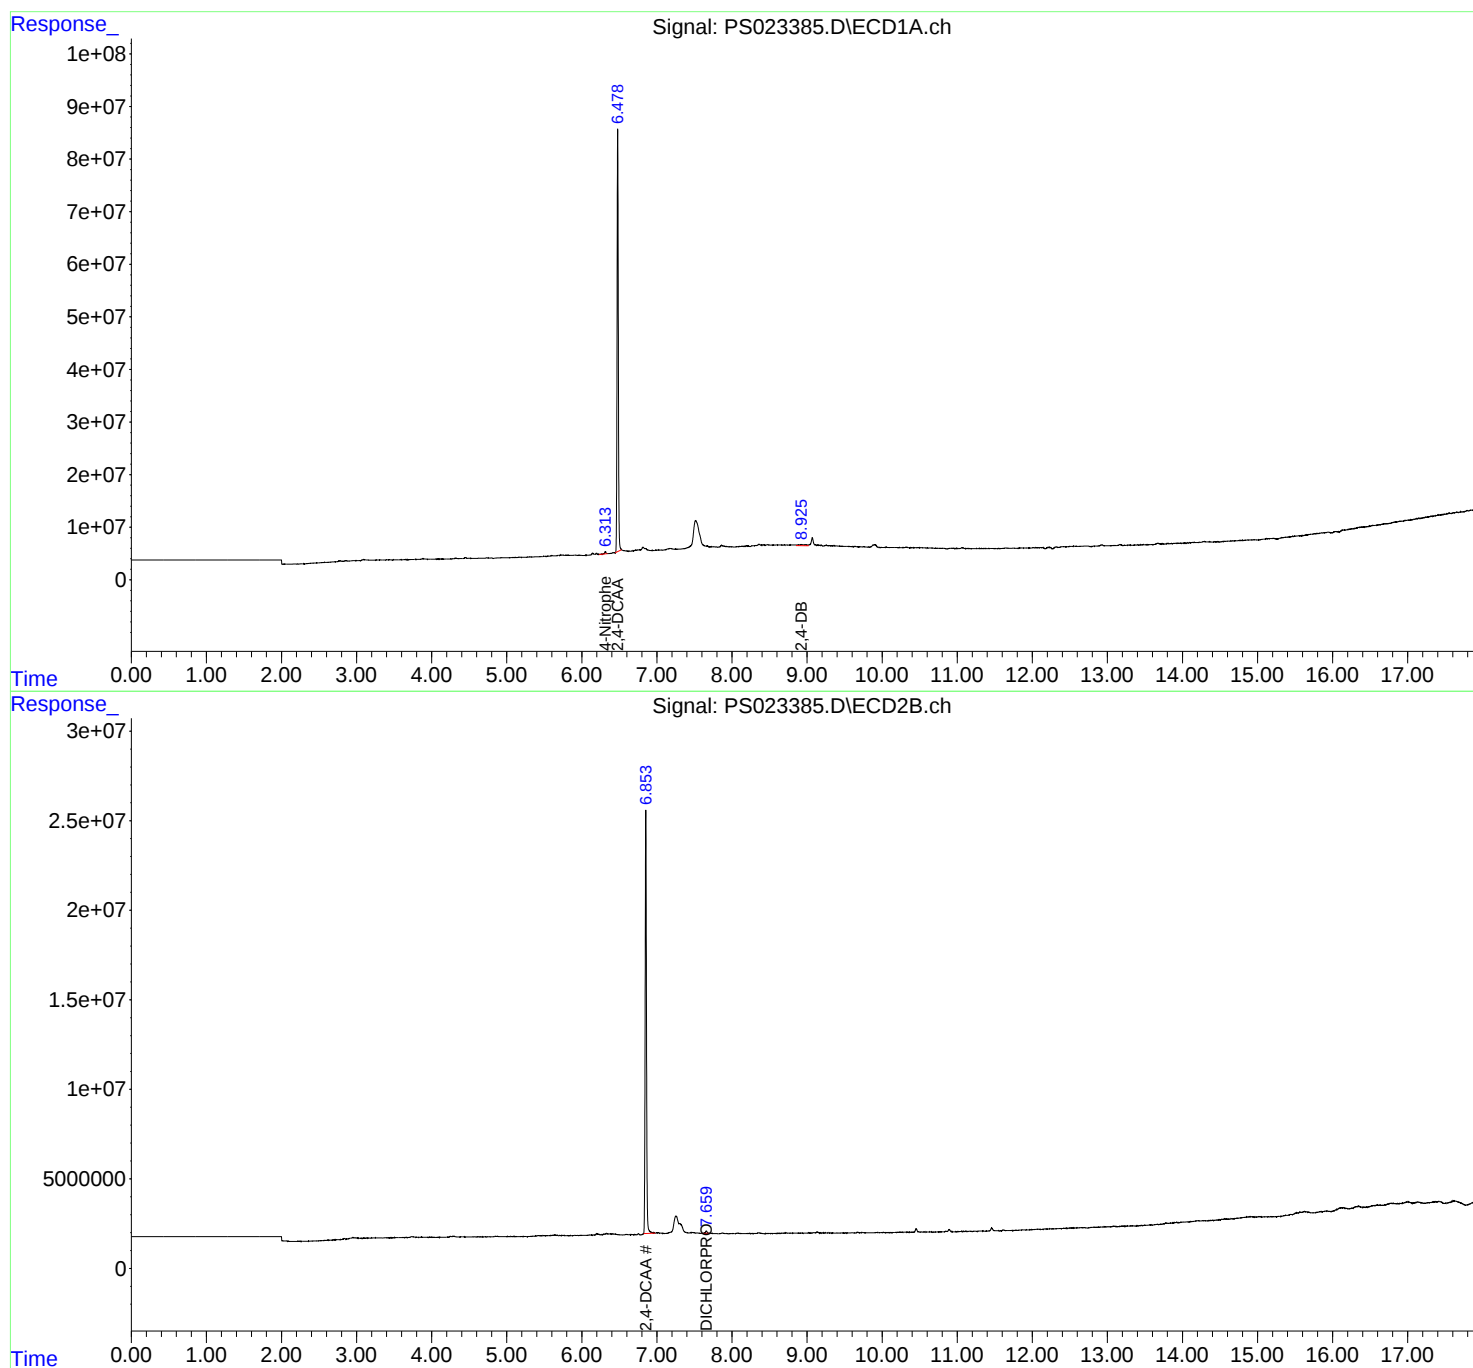


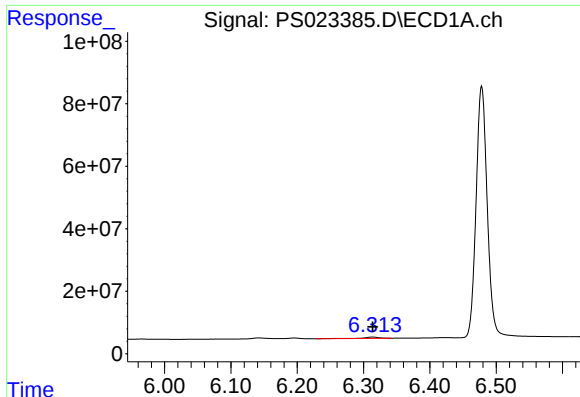

#3 4-Nitrophenol


R.T.: 6.314 min
Delta R.T.: 0.000 min
Response: 6027908
Conc: 4.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

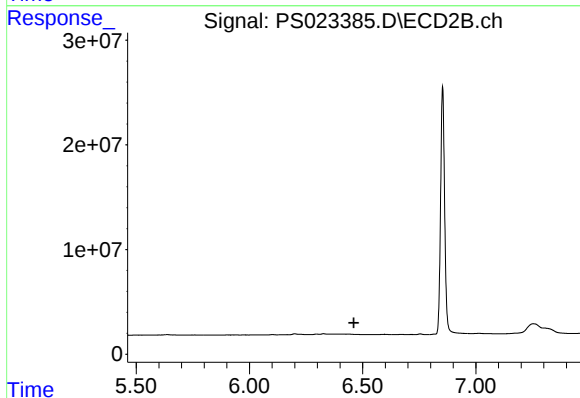


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

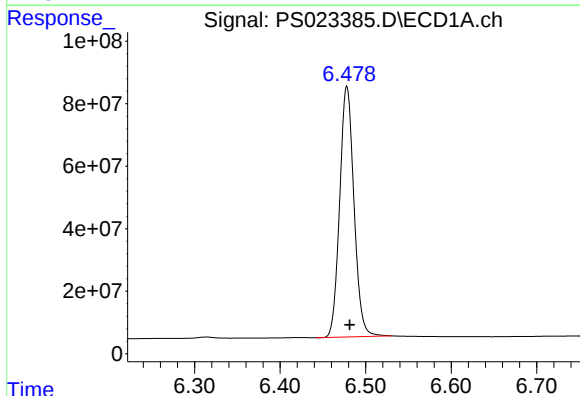


#4 2,4-DCAA

R.T.: 6.478 min
Delta R.T.: -0.003 min
Response: 931399512
Conc: 526.44 ng/ml

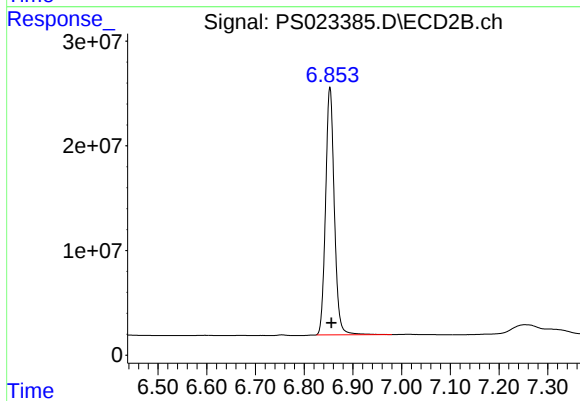

#4 2,4-DCAA


R.T.: 6.853 min
Delta R.T.: -0.003 min
Response: 295073784
Conc: 519.77 ng/ml

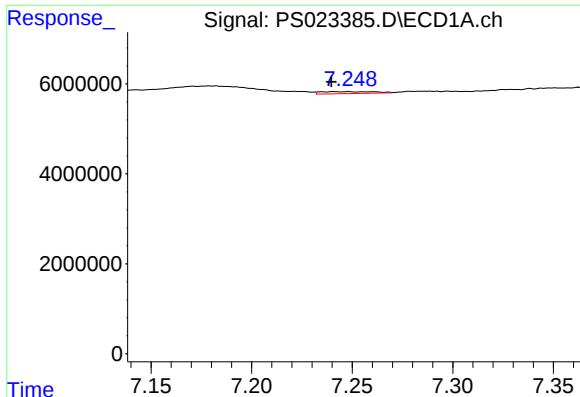

#8 DICHLORPROP


R.T.: 7.241 min
Delta R.T.: 0.001 min
Response: 823294
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

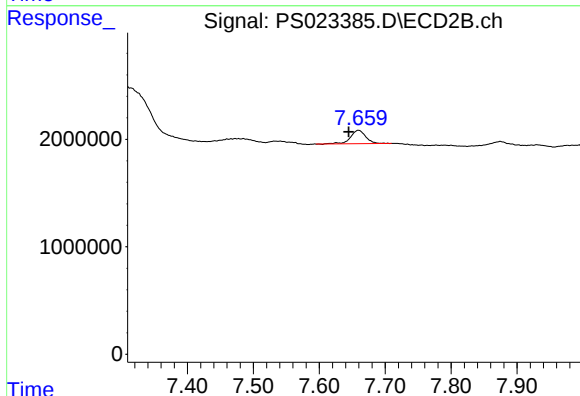


#8 DICHLORPROP

R.T.: 7.659 min
Delta R.T.: 0.015 min
Response: 1998230
Conc: 3.23 ng/ml

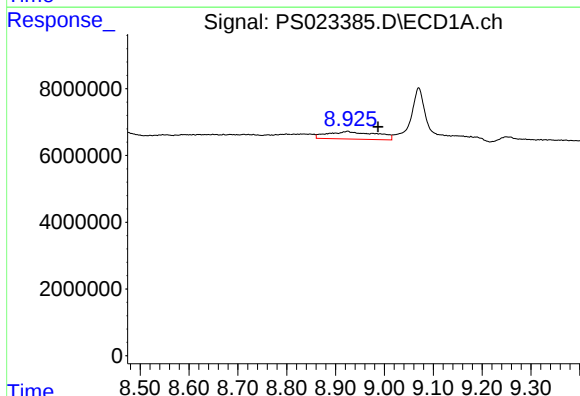

#13 2,4-DB

R.T.: 8.924 min
Delta R.T.: -0.063 min
Response: 15941775
Conc: 6.77 ng/ml

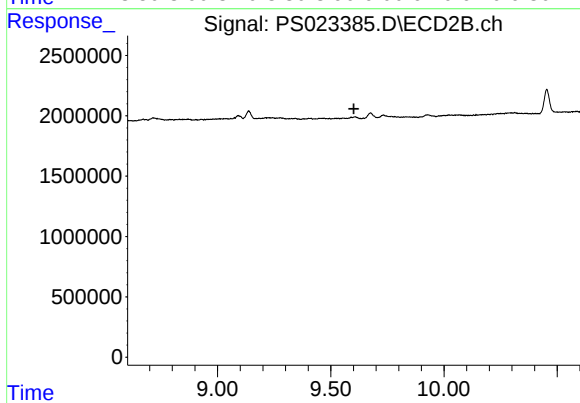

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.