

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
 Data File : PS019772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2022 11:49
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 23:19:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.196	6.781	1088.4E6	430.9E6	453.652	556.117
Target Compounds							
2) T	3,5-DICHL...	6.453	0.000	755707	0	<MDL	N.D. #
3) T	4-Nitroph...	6.987f	0.000	1397966	0	1.425	N.D. #
5) T	DICAMBA	0.000	7.005f	0	1152736	N.D.	<MDL
6) T	MCP	0.000	7.005	0	1152736	N.D.	<MDL
7) T	MCPA	7.656f	0.000	949040	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.636f	0	1477826	N.D.	1.673
10) T	Pentachlo...	8.614	8.284	1312376	1490880	<MDL	<MDL #
11) T	2,4,5-TP ...	9.178	8.649	1873389	351960	<MDL	<MDL #
12) T	2,4,5-T	9.480	9.053	3085137	435875	<MDL	<MDL #
13) T	2,4-DB	10.032	9.471f	5663158	700275	1.400	1.133
15) T	Picloram	10.969	10.880f	27103434	21501973	<MDL	3.343 #
16) T	DCPA	11.423	10.780	3894227	6817680	<MDL	1.105 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
Data File : PS019772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2022 11:49
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 23:19:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

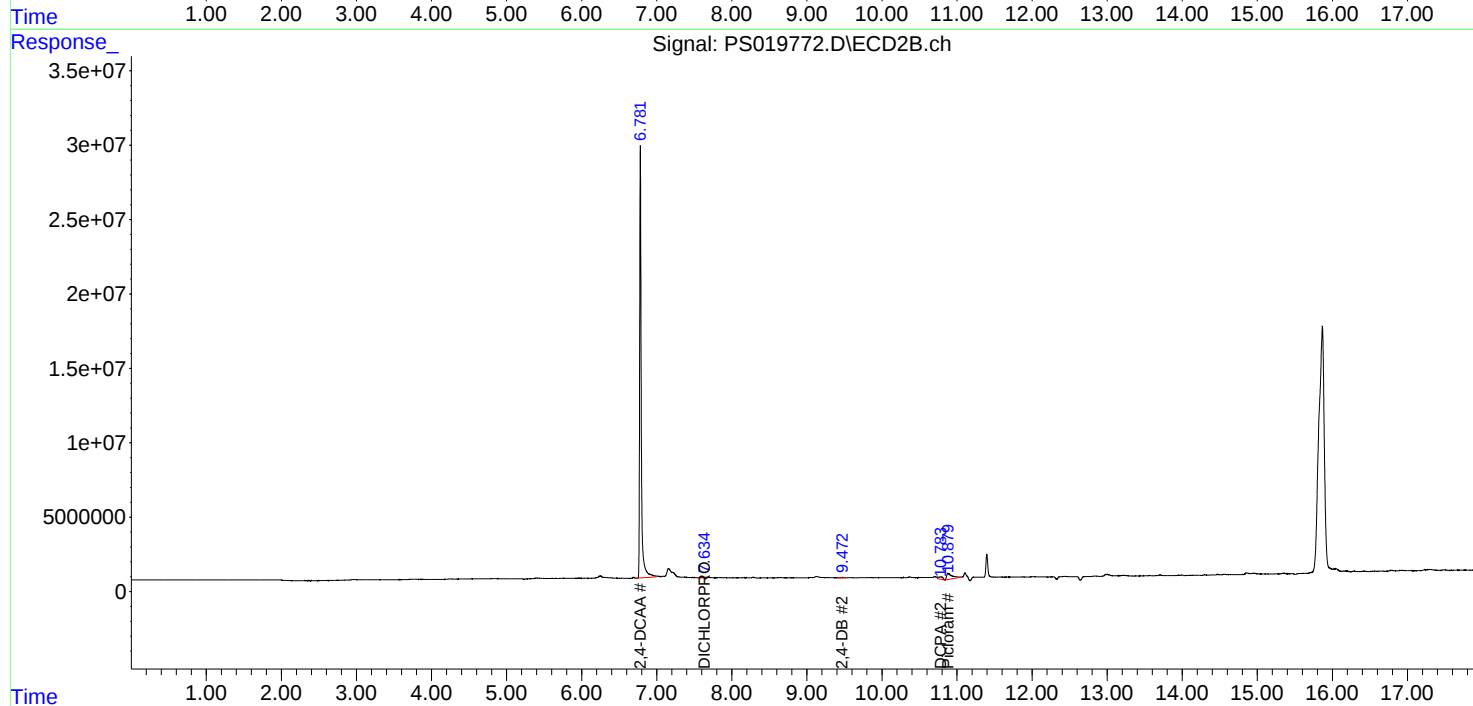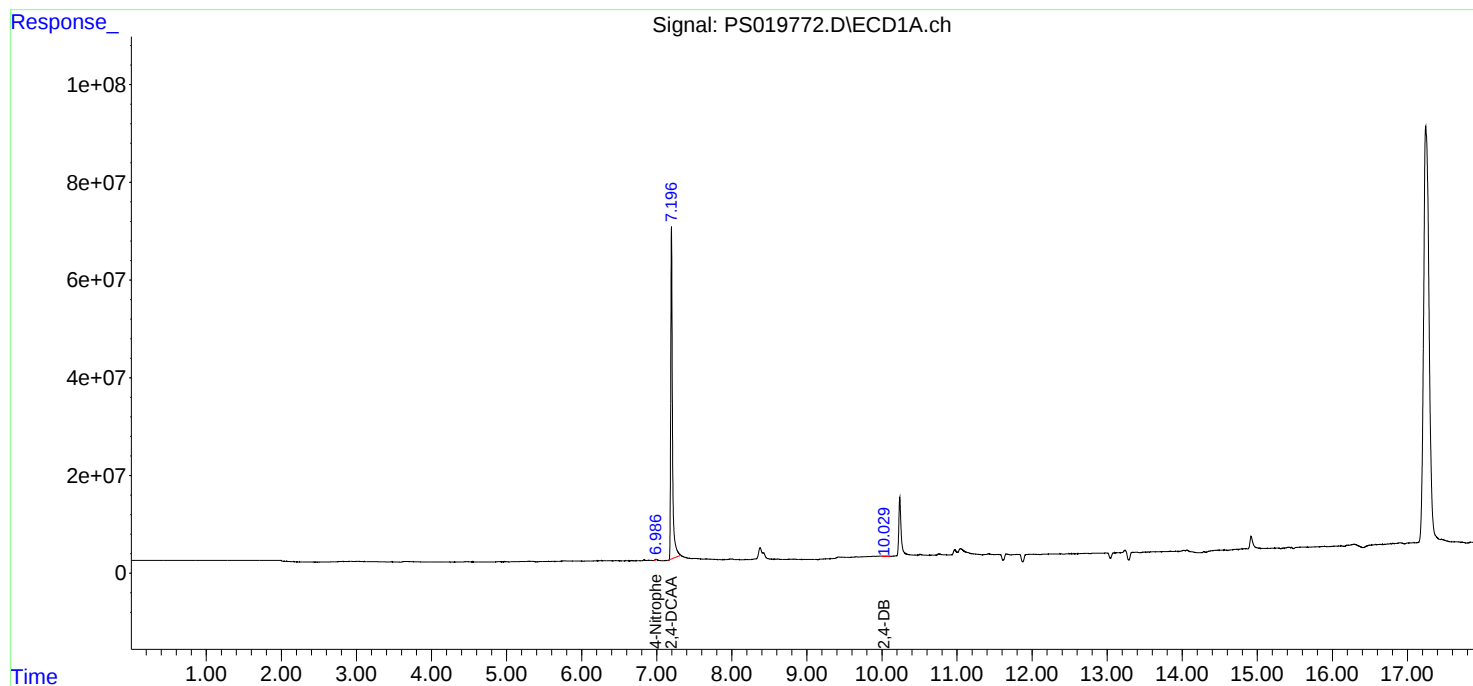


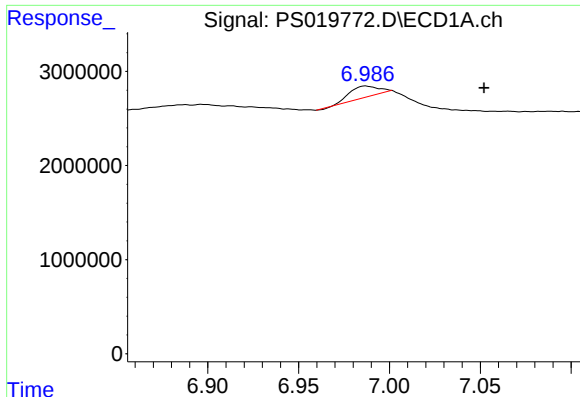

#3 4-Nitrophenol


R.T.: 6.987 min
Delta R.T.: -0.065 min
Response: 1397966
Conc: 1.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

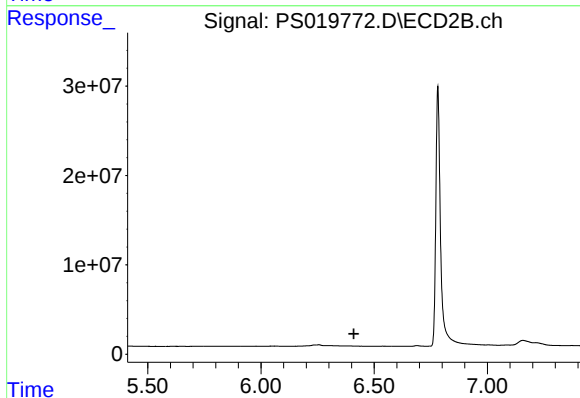


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

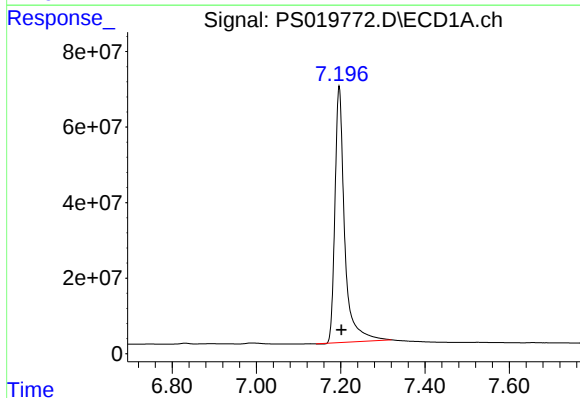


#4 2,4-DCAA

R.T.: 7.196 min
Delta R.T.: -0.006 min
Response: 1088386662
Conc: 453.65 ng/ml

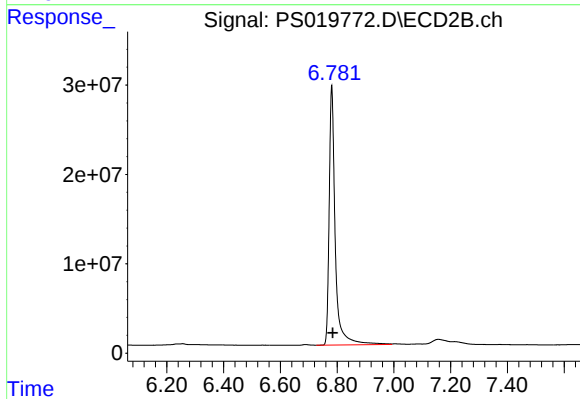

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: -0.004 min
Response: 430918724
Conc: 556.12 ng/ml

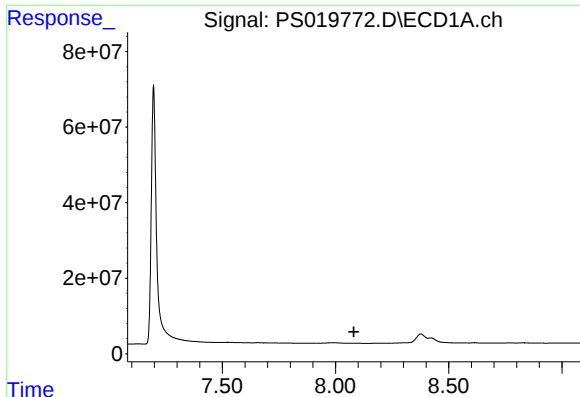

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.081 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

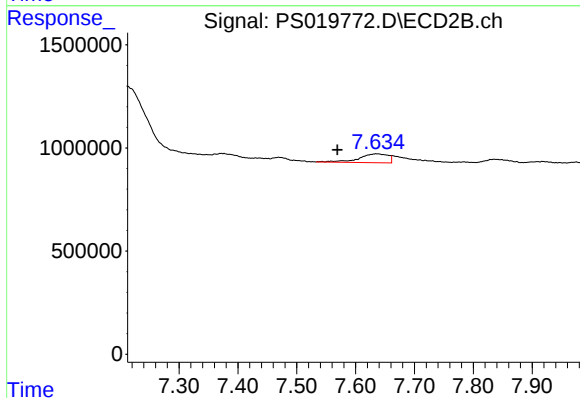


#8 DICHLORPROP

R.T.: 7.636 min
Delta R.T.: 0.067 min
Response: 1477826
Conc: 1.67 ng/ml

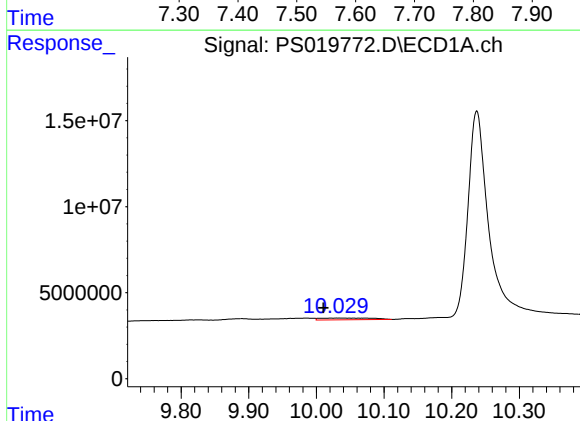


#13 2,4-DB

R.T.: 10.032 min
Delta R.T.: 0.022 min
Response: 5663158
Conc: 1.40 ng/ml

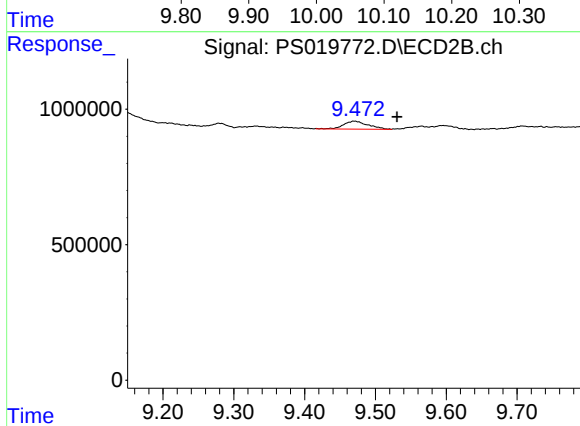

#13 2,4-DB


R.T.: 9.471 min
Delta R.T.: -0.060 min
Response: 700275
Conc: 1.13 ng/ml

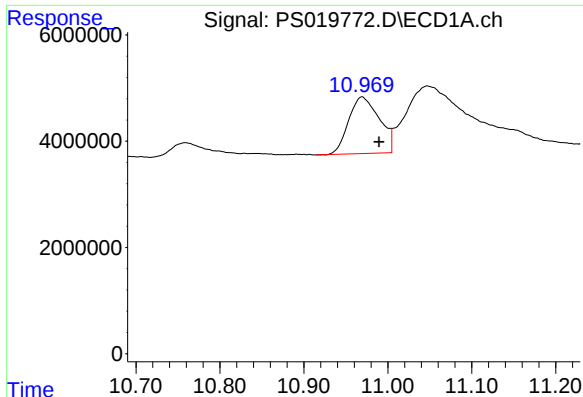

#15 Picloram


R.T.: 10.969 min
Delta R.T.: -0.020 min
Response: 27103434
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

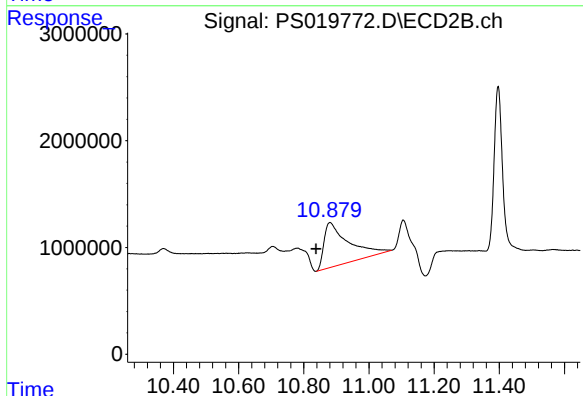


#15 Picloram

R.T.: 10.880 min
Delta R.T.: 0.043 min
Response: 21501973
Conc: 3.34 ng/ml

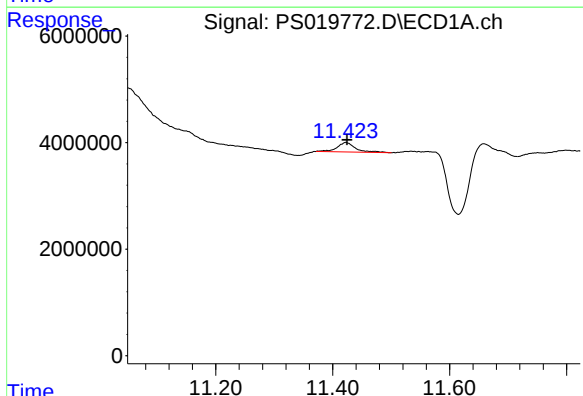

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.002 min
Response: 3894227
Conc: N.D.

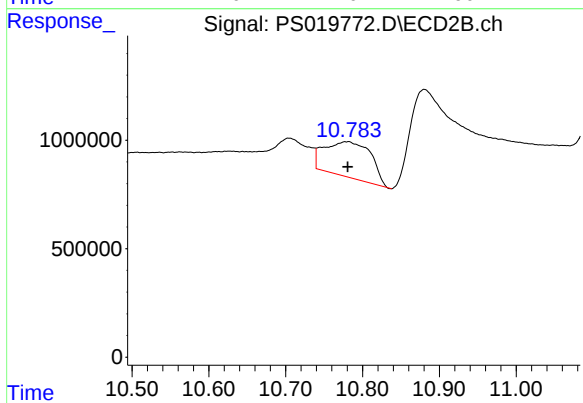

#16 DCPA

R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 6817680
Conc: 1.10 ng/ml