

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
 Data File : PS019778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2022 18:17
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 23:21:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.196	6.781	1124.4E6	444.2E6	468.677	573.246
Target Compounds							
2) T	3,5-DICHL...	6.452	0.000	1109755	0	<MDL	N.D. #
3) T	4-Nitroph...	6.986f	0.000	1774992	0	1.809	N.D. #
5) T	DICAMBA	0.000	7.003f	0	1272961	N.D.	<MDL
6) T	MCP	0.000	7.003	0	1272961	N.D.	<MDL
7) T	MCPA	7.653f	0.000	2514247	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.628f	0	2028079	N.D.	2.296
10) T	Pentachlo...	8.613	8.283	1737247	2392117	<MDL	<MDL #
11) T	2,4,5-TP ...	9.177	8.648	2465004	336781	<MDL	<MDL #
12) T	2,4,5-T	9.485	9.050	4478181	-320706	<MDL	N.D. #
13) T	2,4-DB	10.026	9.470f	5301508	828220	1.310	1.340
14) T	DINOSEB	0.000	9.855	0	412513	N.D.	<MDL
15) T	Picloram	10.964	10.882f	43213449	18926360	1.456	2.942 #
16) T	DCPA	11.423	10.779	4351898	10011496	<MDL	1.622 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
Data File : PS019778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2022 18:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 23:21:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

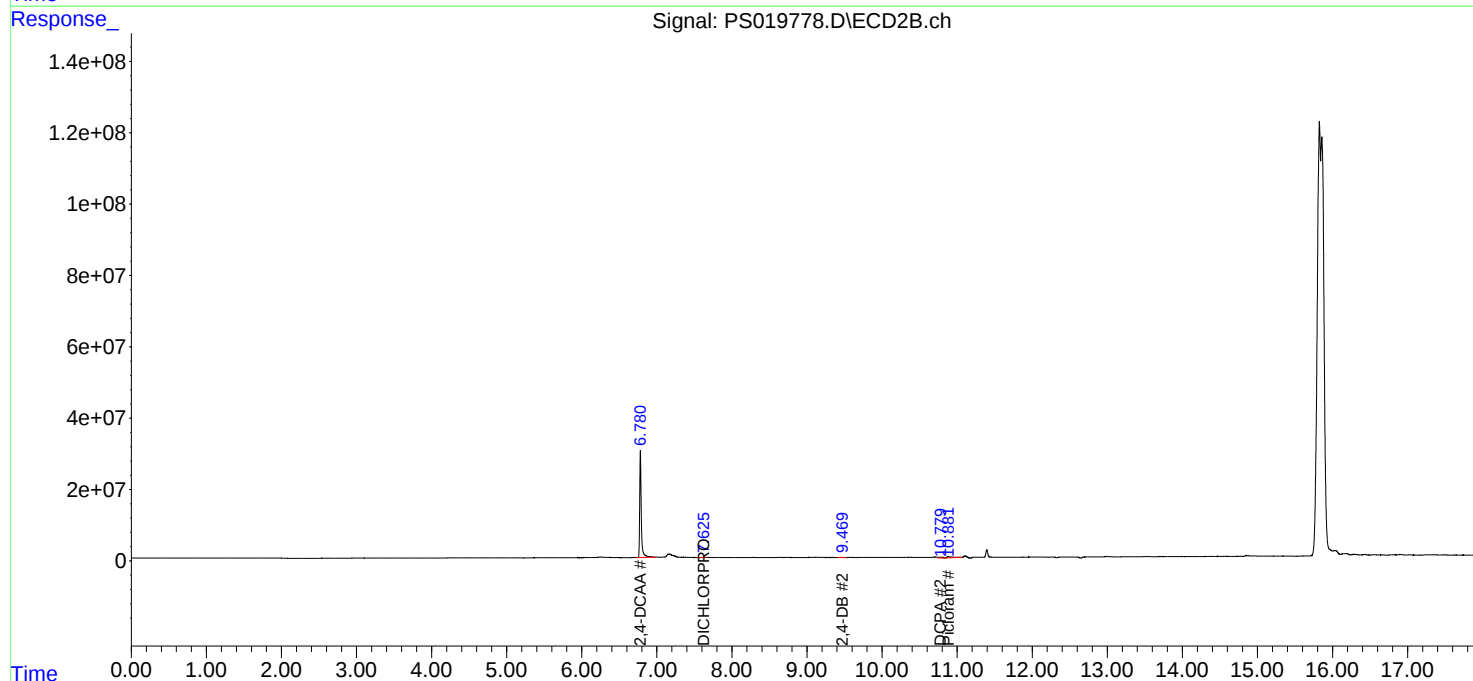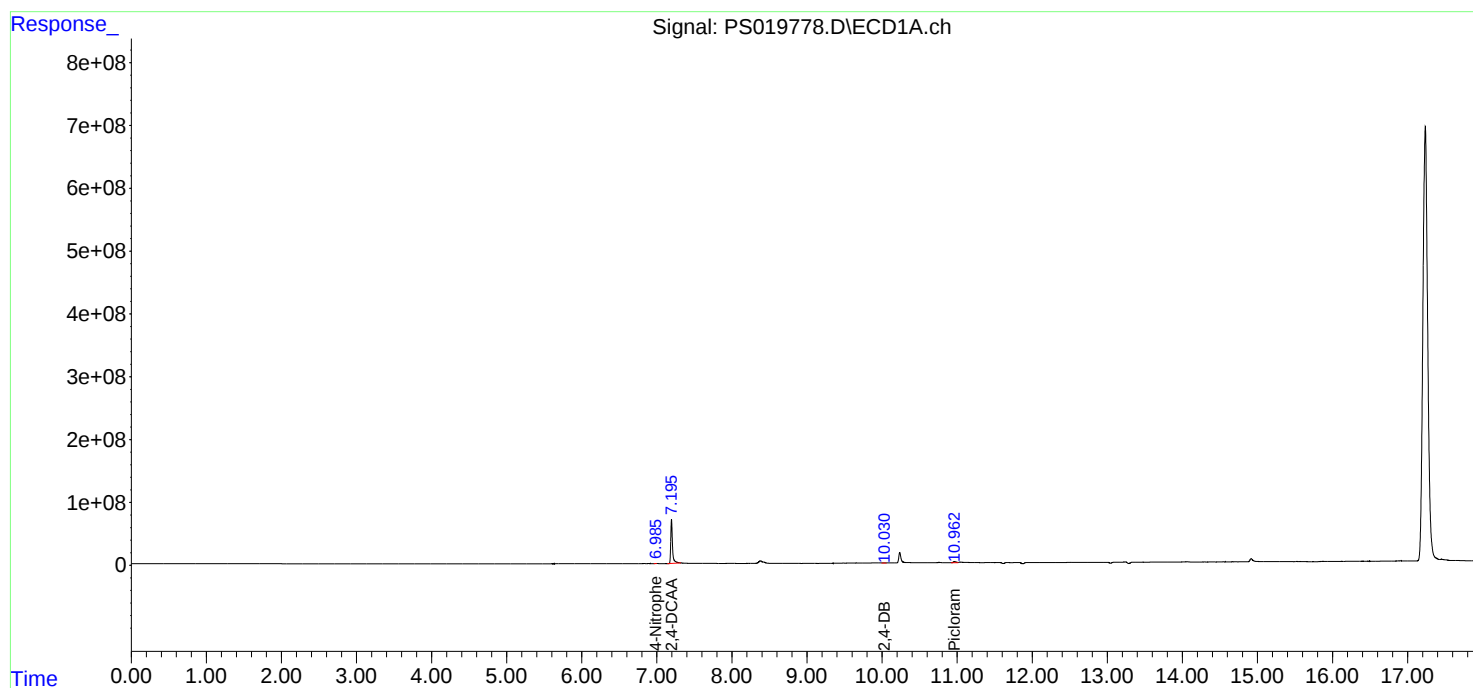


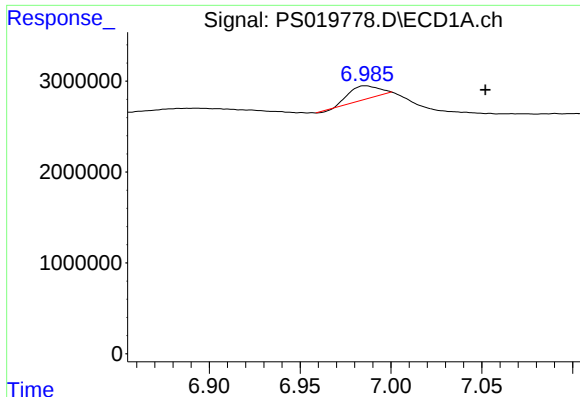

#3 4-Nitrophenol


R.T.: 6.986 min
Delta R.T.: -0.066 min
Response: 1774992
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

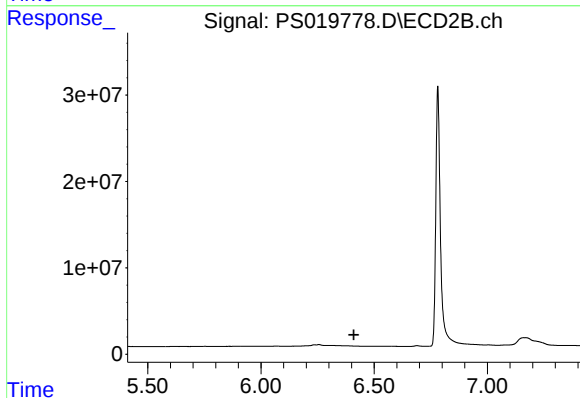


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

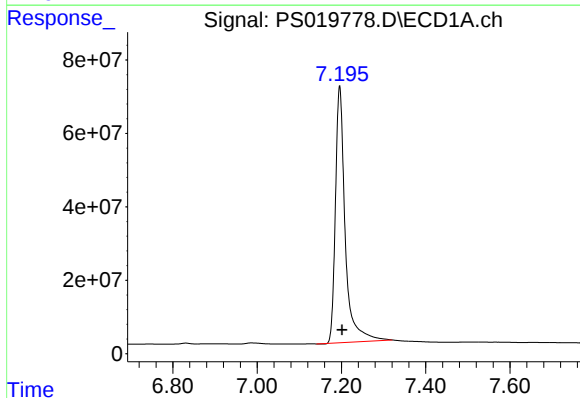


#4 2,4-DCAA

R.T.: 7.196 min
Delta R.T.: -0.006 min
Response: 1124434422
Conc: 468.68 ng/ml

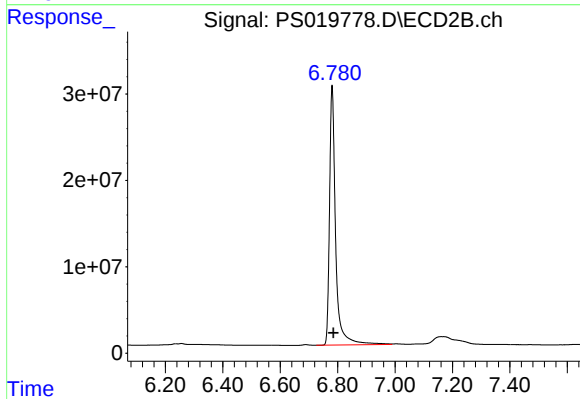

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: -0.004 min
Response: 444191561
Conc: 573.25 ng/ml

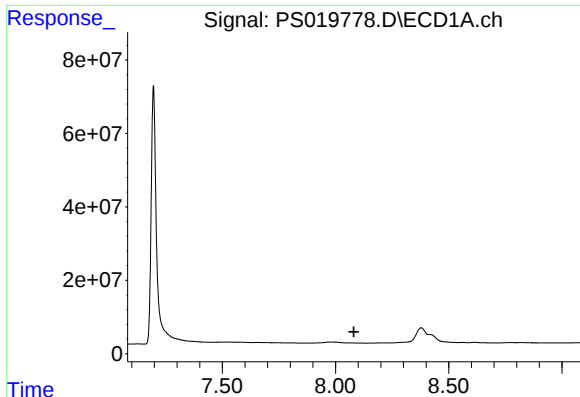

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.081 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

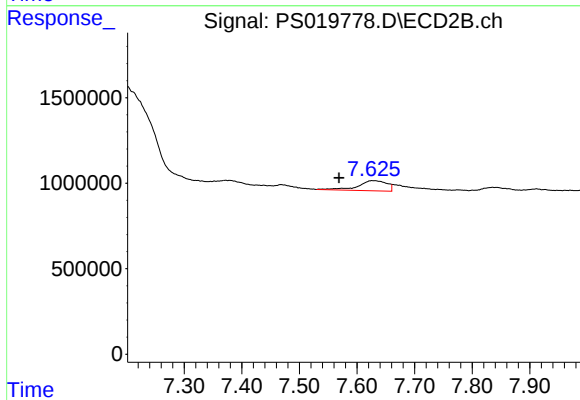


#8 DICHLORPROP

R.T.: 7.628 min
Delta R.T.: 0.059 min
Response: 2028079
Conc: 2.30 ng/ml

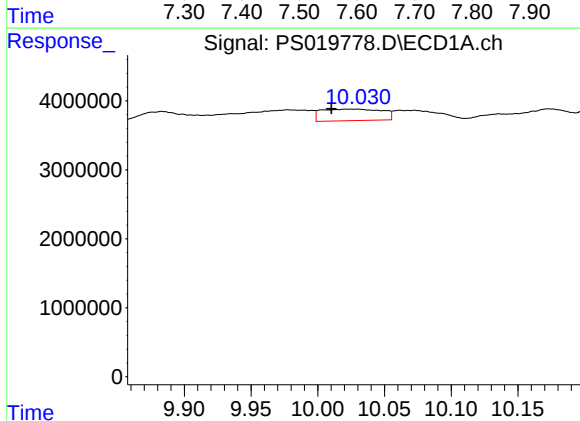


#13 2,4-DB

R.T.: 10.026 min
Delta R.T.: 0.016 min
Response: 5301508
Conc: 1.31 ng/ml

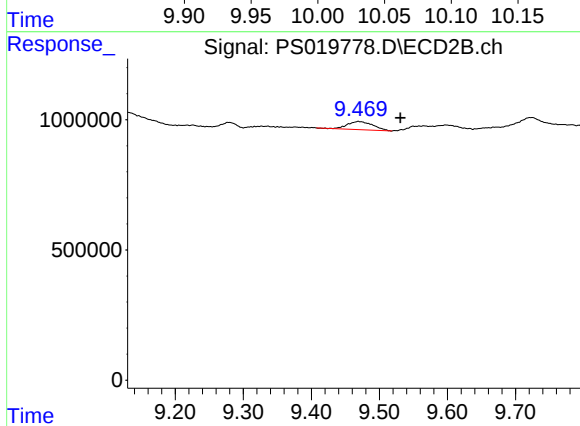

#13 2,4-DB


R.T.: 9.470 min
Delta R.T.: -0.061 min
Response: 828220
Conc: 1.34 ng/ml

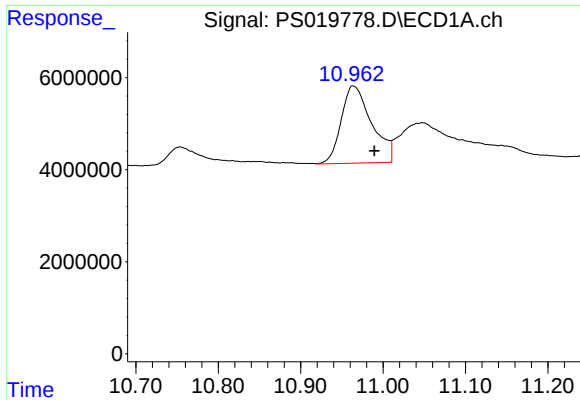

#15 Picloram


R.T.: 10.964 min
Delta R.T.: -0.025 min
Response: 43213449
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

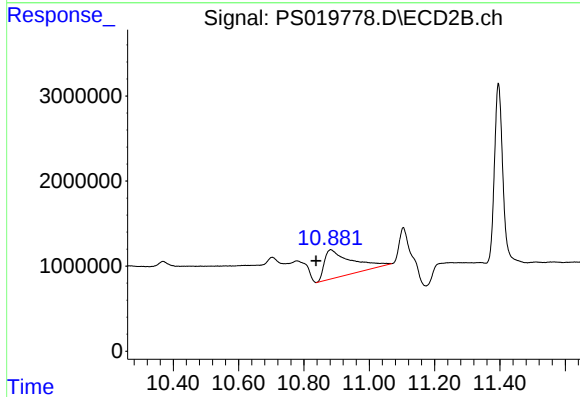


#15 Picloram

R.T.: 10.882 min
Delta R.T.: 0.045 min
Response: 18926360
Conc: 2.94 ng/ml

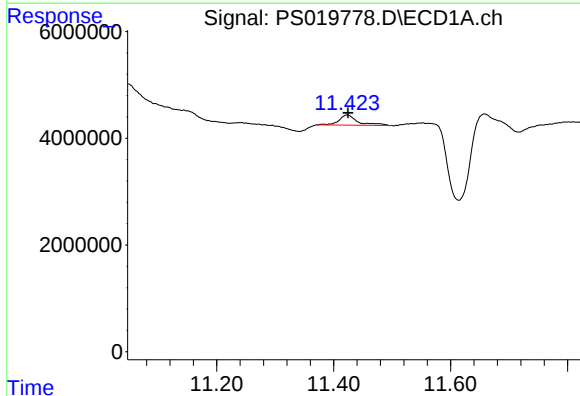

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.001 min
Response: 4351898
Conc: N.D.

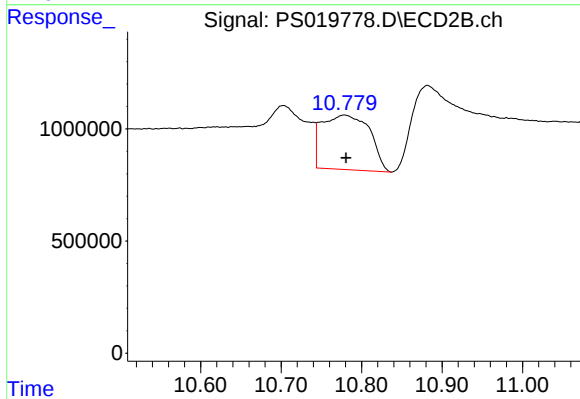

#16 DCPA

R.T.: 10.779 min
Delta R.T.: -0.002 min
Response: 10011496
Conc: 1.62 ng/ml