

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062518\
 Data File : PS000639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2018 18:14
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 00:49:23 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.806	11.173	216.6E6	183.8E6	575.040	540.141
Target Compounds							
1) T	Dalapon	3.179	2.551	494059	514185	0.966	1.180
3) T	4-Nitroph...	11.428	0.000	764738	0	3.253	N.D. #
6) T	MCP	12.491	0.000	420926	0	0.372	N.D. #
10) T	Pentachlo...	14.073	13.622	680080	451388	0.130	0.095 #
11) T	2,4,5-TP ...	14.938	14.236	679285	244940	0.313	0.126 #
12) T	2,4,5-T	15.341	14.804	792013	12305	0.368	0.007 #
14) T	DINOSEB	17.602	0.000	2993427	0	2.010	N.D. #
15) T	Picloram	17.363	17.134	6443134	573572	2.206	0.230 #
16) T	DCPA	17.939	17.077	3997809	441077	1.560	0.191 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062518\
Data File : PS000639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2018 18:14
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 00:49:23 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

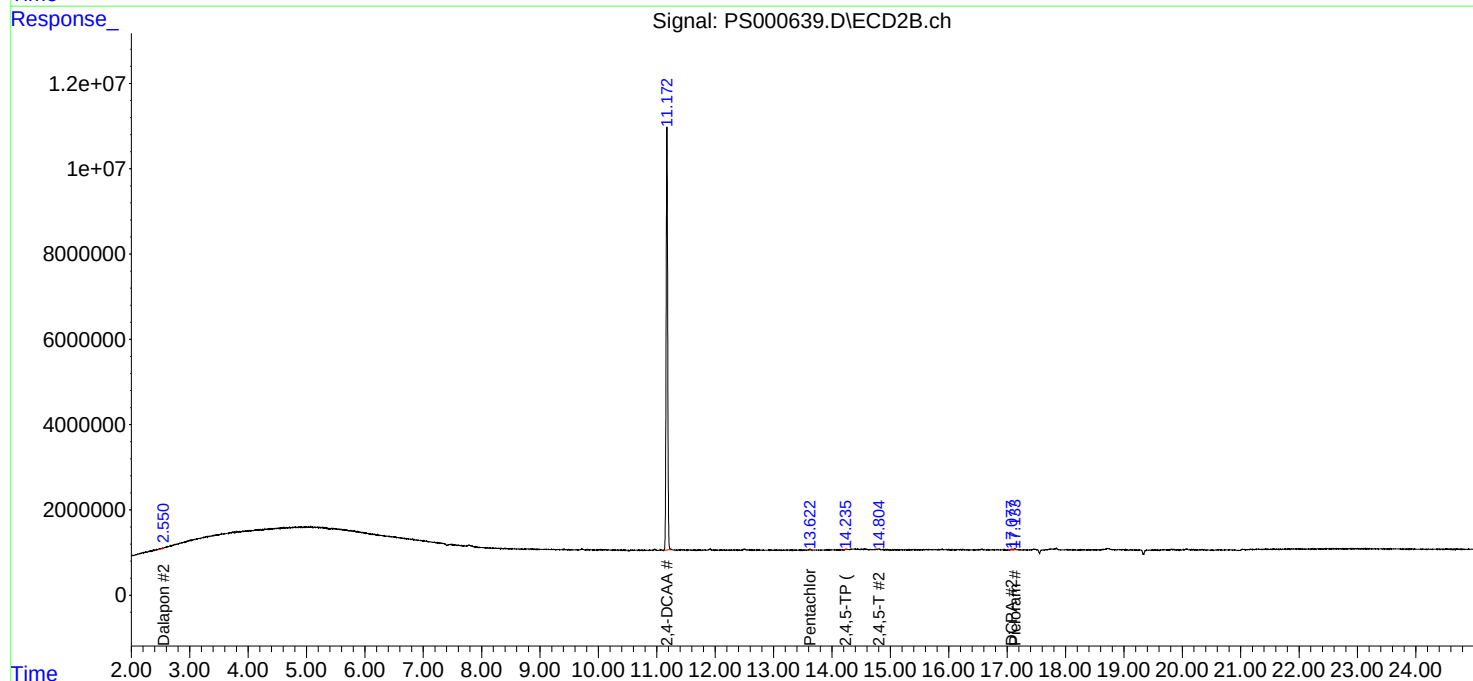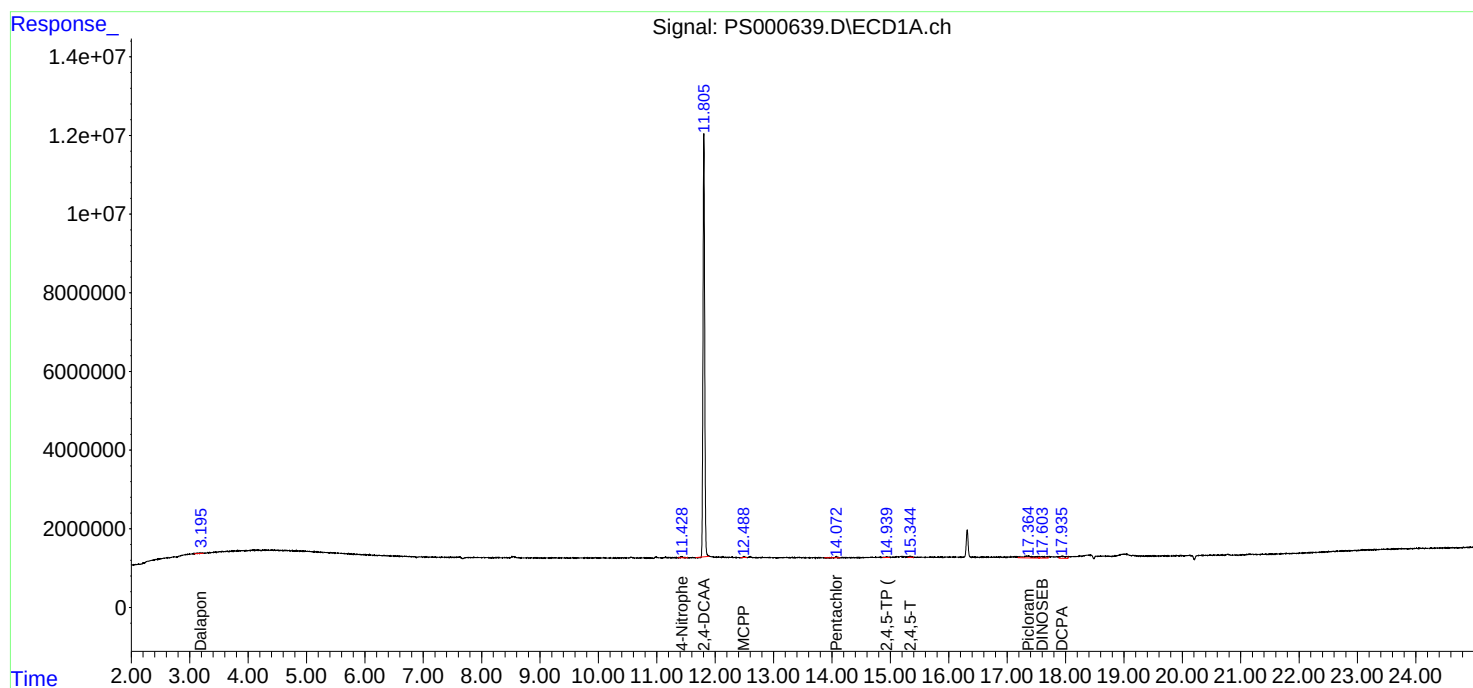


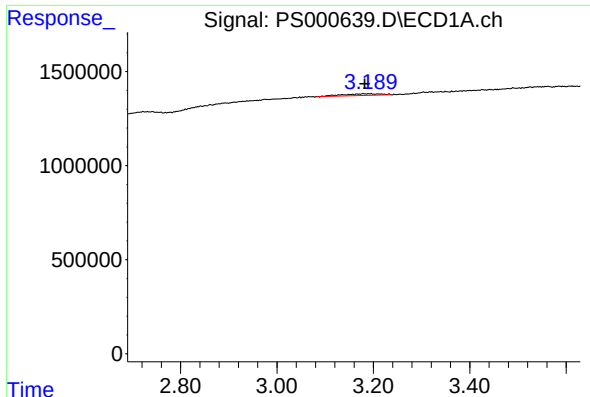

#1 Dalapon


R.T.: 3.179 min
Delta R.T.: -0.003 min
Response: 494059
Conc: 0.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

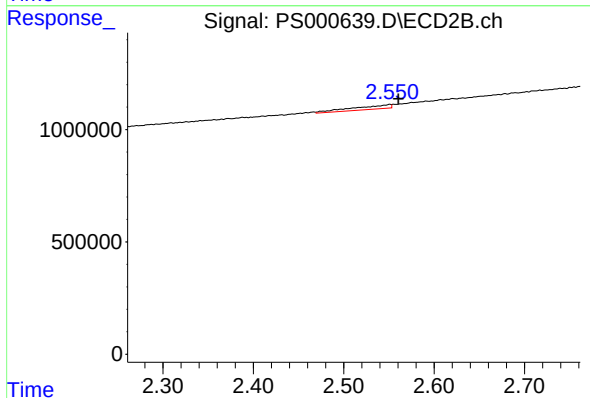


#1 Dalapon

R.T.: 2.551 min
Delta R.T.: -0.010 min
Response: 514185
Conc: 1.18 ng/ml

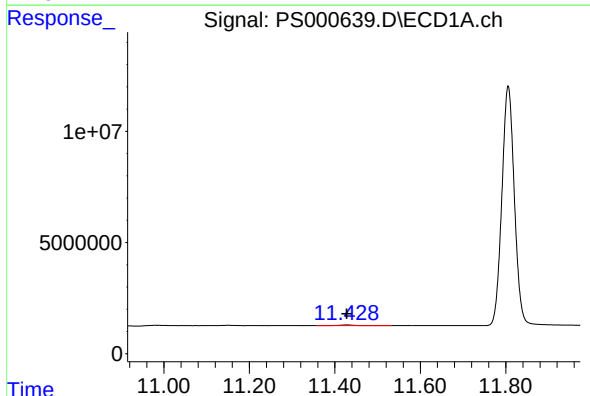


#3 4-Nitrophenol

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 764738
Conc: 3.25 ng/ml

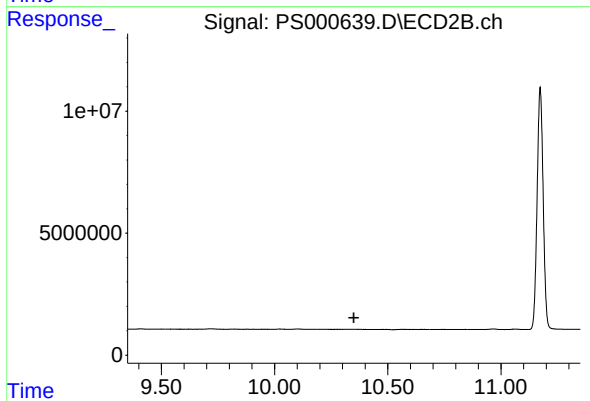

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

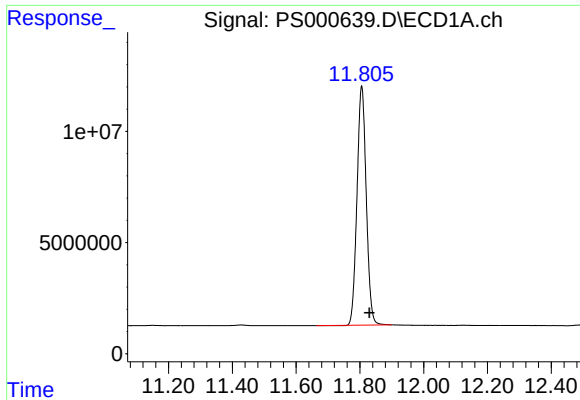

#4 2,4-DCAA


R.T.: 11.806 min
Delta R.T.: -0.024 min
Response: 216591680
Conc: 575.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

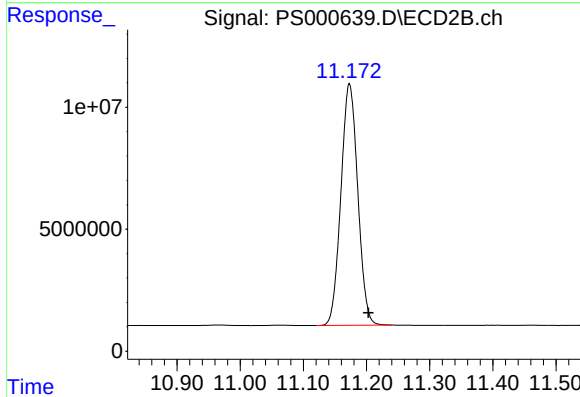


#4 2,4-DCAA

R.T.: 11.173 min
Delta R.T.: -0.030 min
Response: 183814969
Conc: 540.14 ng/ml

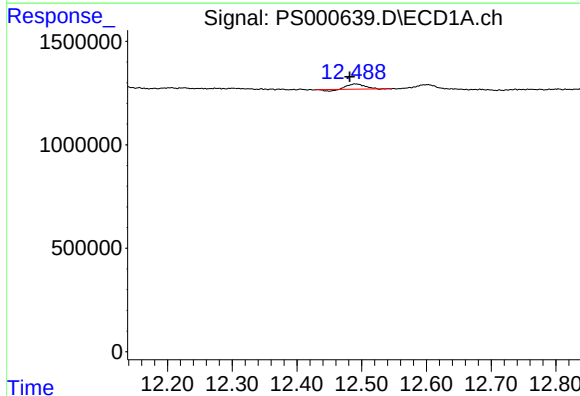


#6 MCP

R.T.: 12.491 min
Delta R.T.: 0.009 min
Response: 420926
Conc: 0.37 ug/ml

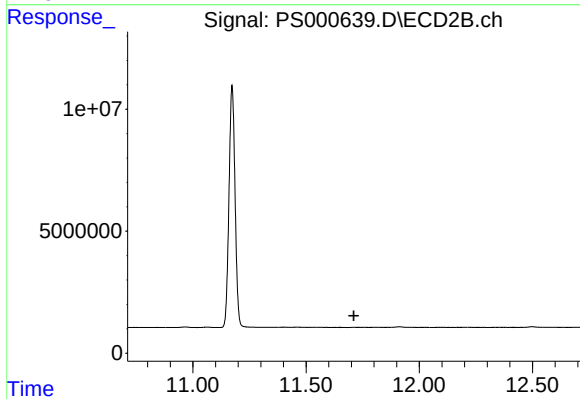

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

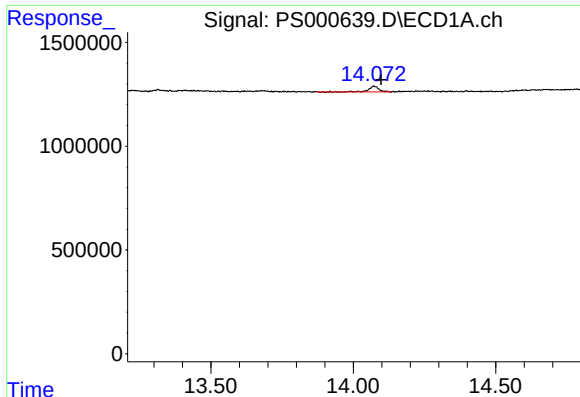

#10 Pentachlorophenol


R.T.: 14.073 min
Delta R.T.: -0.024 min
Response: 680080
Conc: 0.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

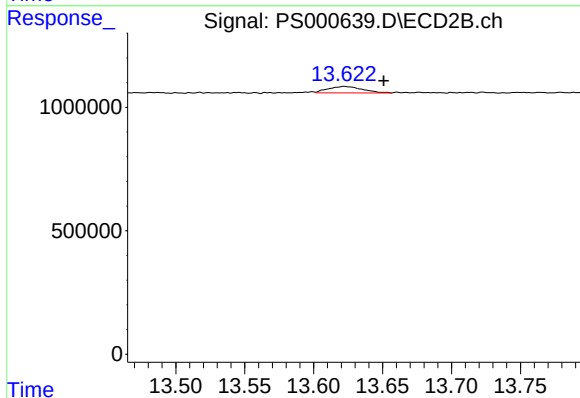


#10 Pentachlorophenol

R.T.: 13.622 min
Delta R.T.: -0.029 min
Response: 451388
Conc: 0.10 ng/ml

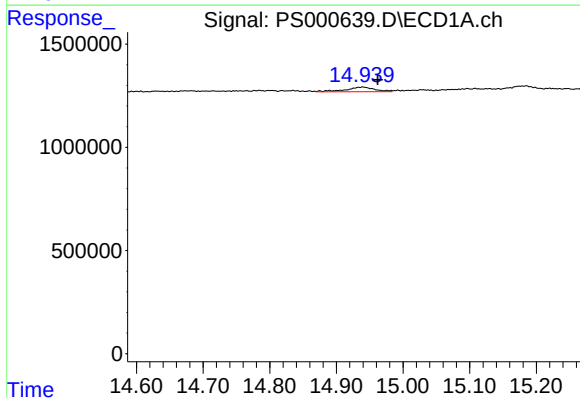


#11 2,4,5-TP (SILVEX)

R.T.: 14.938 min
Delta R.T.: -0.024 min
Response: 679285
Conc: 0.31 ng/ml

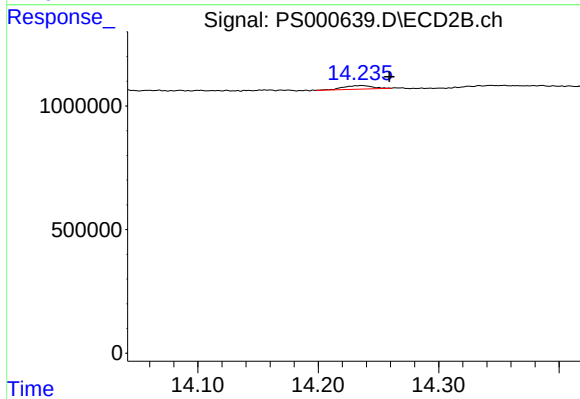

#11 2,4,5-TP (SILVEX)


R.T.: 14.236 min
Delta R.T.: -0.023 min
Response: 244940
Conc: 0.13 ng/ml

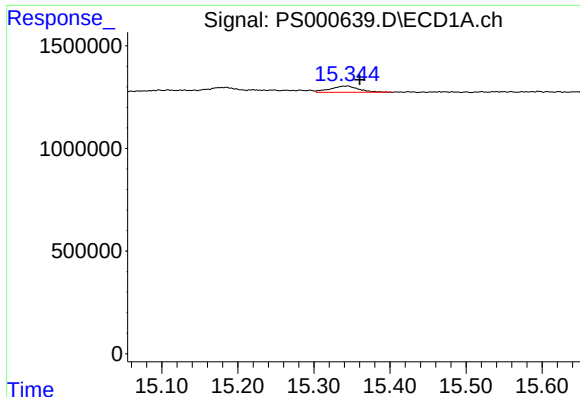

#12 2,4,5-T


R.T.: 15.341 min
Delta R.T.: -0.019 min
Response: 792013
Conc: 0.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

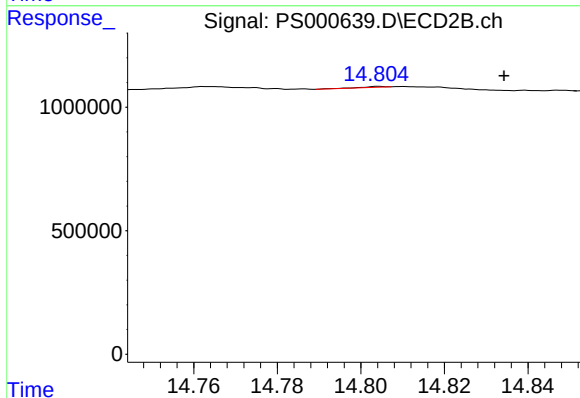


#12 2,4,5-T

R.T.: 14.804 min
Delta R.T.: -0.030 min
Response: 12305
Conc: 0.01 ng/ml

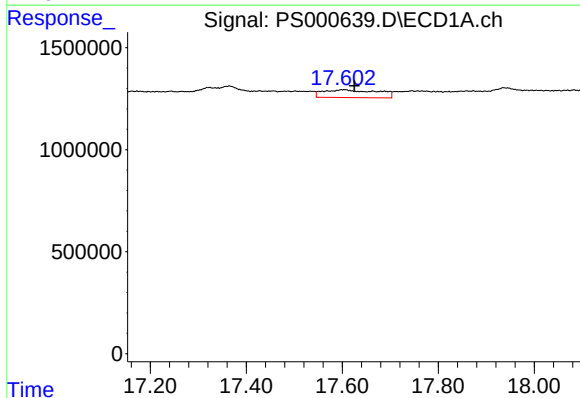


#14 DINOSEB

R.T.: 17.602 min
Delta R.T.: -0.024 min
Response: 2993427
Conc: 2.01 ng/ml

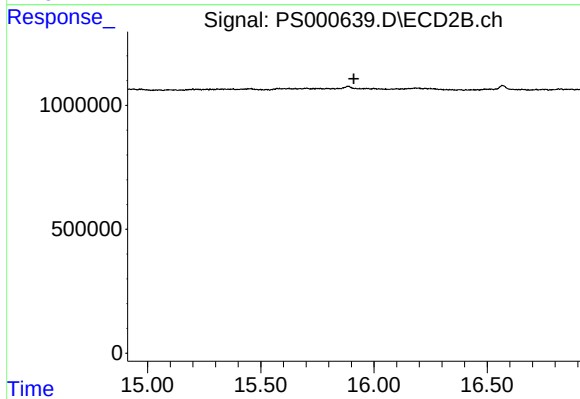

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.911 min
Response: 0
Conc: N.D.

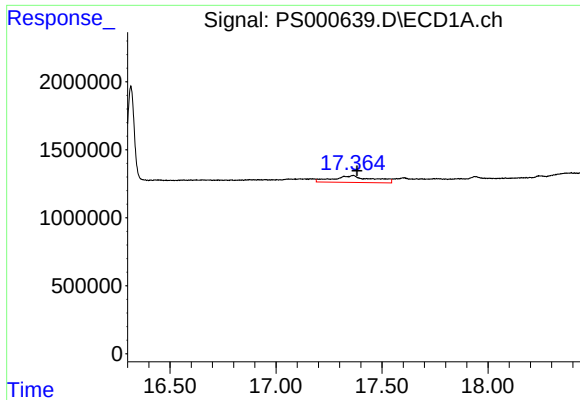

#15 Picloram


R.T.: 17.363 min
Delta R.T.: -0.019 min
Response: 6443134
Conc: 2.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

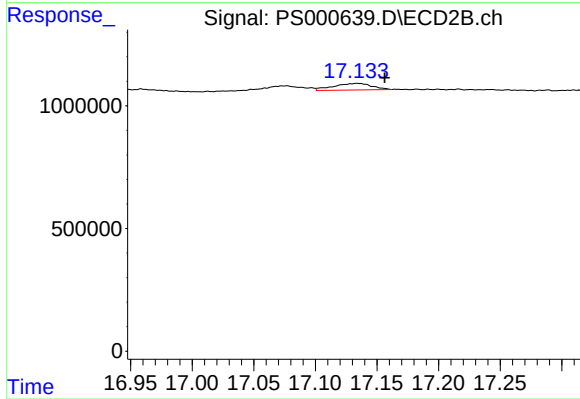


#15 Picloram

R.T.: 17.134 min
Delta R.T.: -0.023 min
Response: 573572
Conc: 0.23 ng/ml

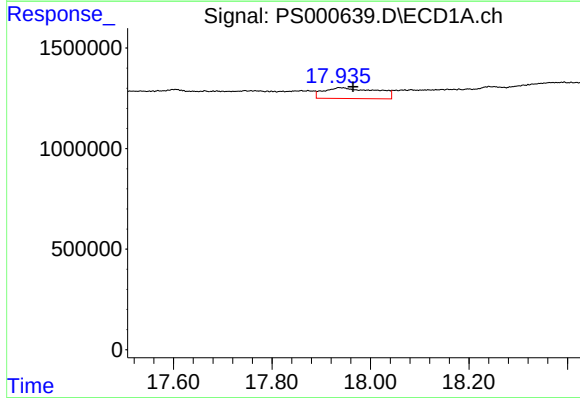

#16 DCPA

R.T.: 17.939 min
Delta R.T.: -0.025 min
Response: 3997809
Conc: 1.56 ng/ml

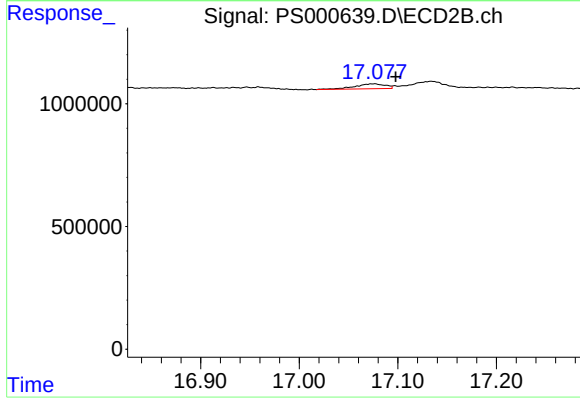

#16 DCPA

R.T.: 17.077 min
Delta R.T.: -0.021 min
Response: 441077
Conc: 0.19 ng/ml