

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062520\
 Data File : PS010925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2020 14:03
 Operator : DD\AJ
 Sample : PB129734BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB129734BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 15:38:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	407.5E6	274.7E6	449.358	495.792
Target Compounds							
1) T	Dalapon	2.993	2.584	38346699	118.5E6	34.247	157.144 #
2) T	3,5-DICHL...	0.000	6.100	0	21116443	N.D.	25.355
3) T	4-Nitroph...	7.004	0.000	3047492	0	7.634	N.D. #
7) T	MCPA	7.777	7.384	50724409	37813092	12.737	13.700
8) T	DICHLORPROP	0.000	7.742	0	9577522	N.D.	16.312
10) T	Pentachlo...	8.710	0.000	14047123	0	1.130	N.D. #
11) T	2,4,5-TP ...	9.269	0.000	3035782	0	<MDL	N.D. #
12) T	2,4,5-T	9.509	0.000	7245715	0	1.556	N.D. #
14) T	DINOSEB	0.000	10.039	0	9719659	N.D.	4.668
15) T	Picloram	10.996	0.000	56349806	0	10.051	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062520\
Data File : PS010925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2020 14:03
Operator : DD\AJ
Sample : PB129734BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB129734BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 15:38:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

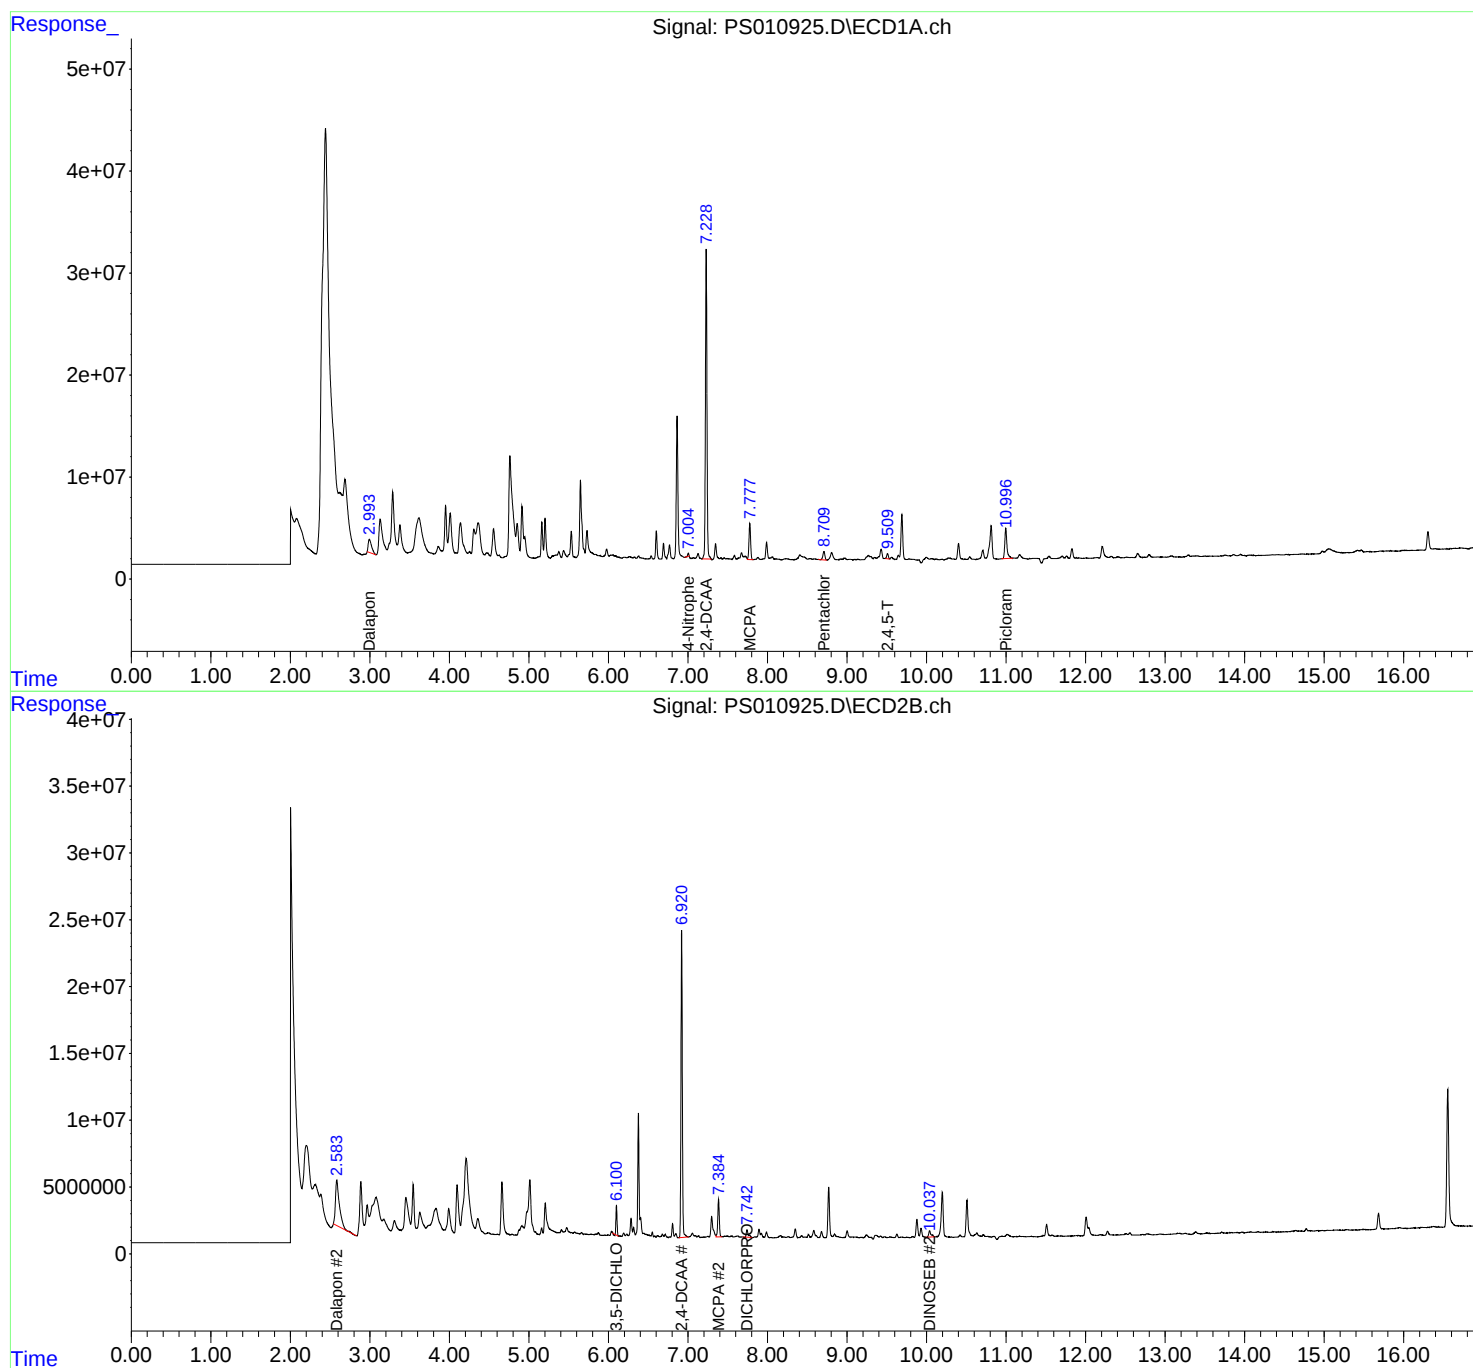


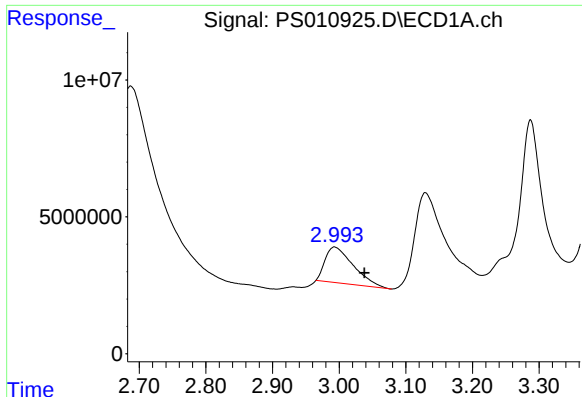

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.045 min
Response: 38346699
Conc: 34.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129734BL

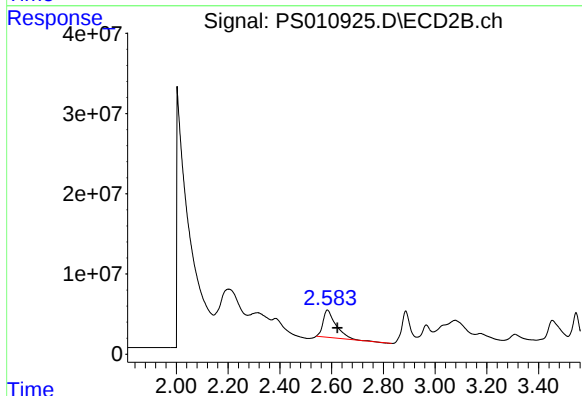


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.038 min
Response: 118543134
Conc: 157.14 ng/ml

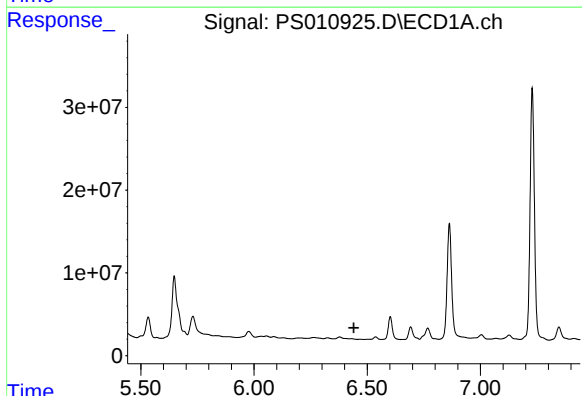


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

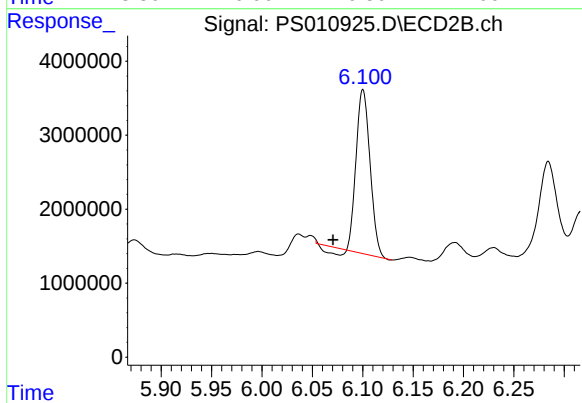

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 21116443
Conc: 25.36 ng/ml

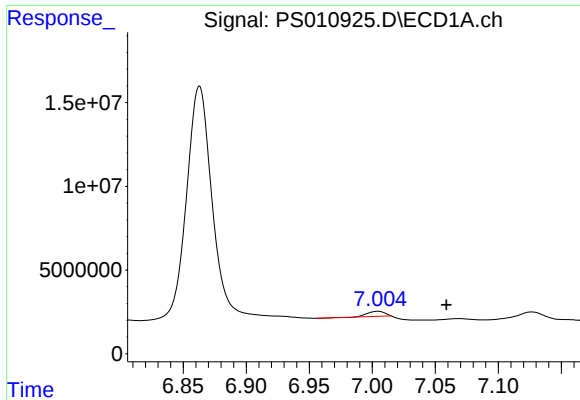

#3 4-Nitrophenol


R.T.: 7.004 min
Delta R.T.: -0.055 min
Response: 3047492
Conc: 7.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129734BL

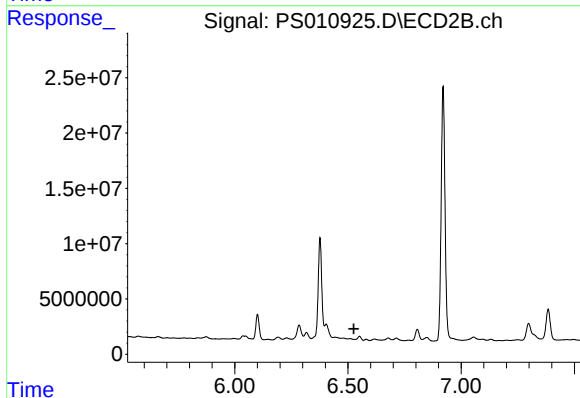


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.526 min
Response: 0
Conc: N.D.

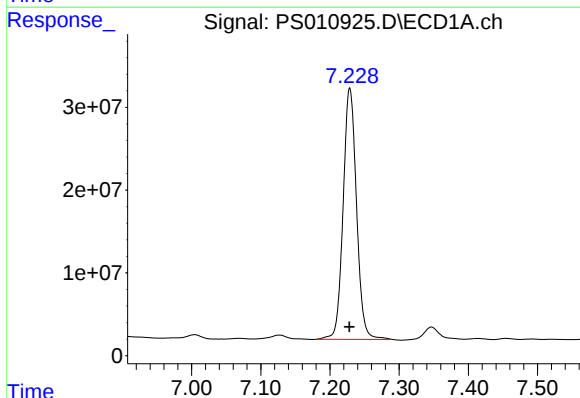


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 407486518
Conc: 449.36 ng/ml

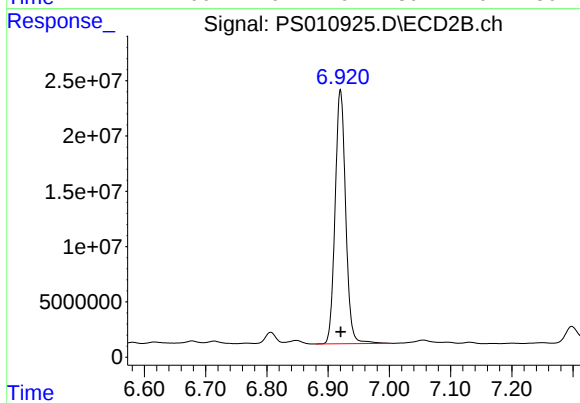

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 274706436
Conc: 495.79 ng/ml

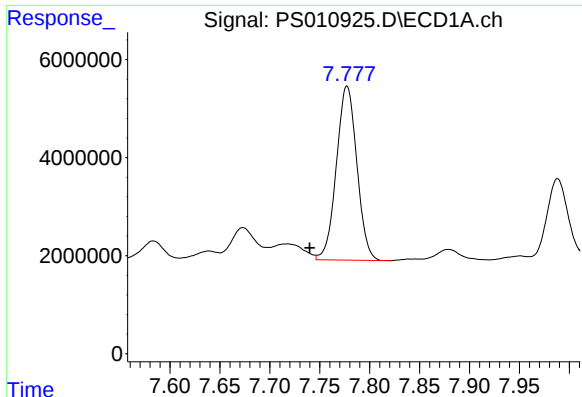

#7 MCPA


R.T.: 7.777 min
Delta R.T.: 0.037 min
Response: 50724409
Conc: 12.74 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB129734BL

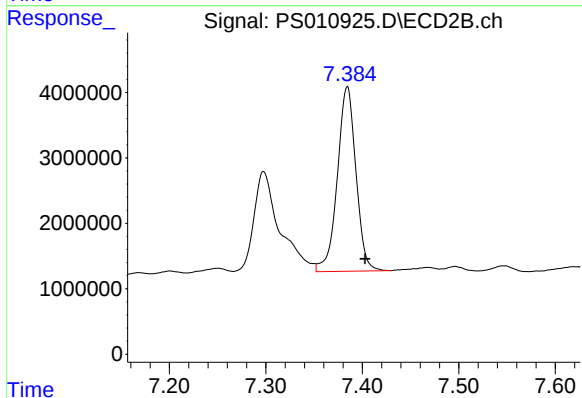


#7 MCPA

R.T.: 7.384 min
Delta R.T.: -0.019 min
Response: 37813092
Conc: 13.70 ug/ml

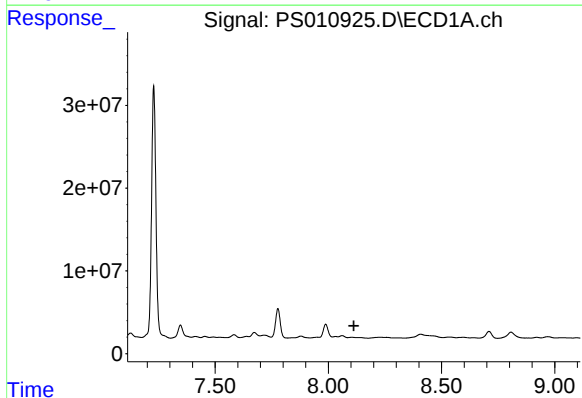


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

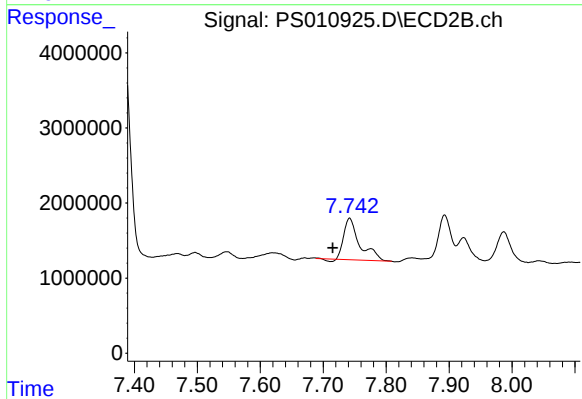

#8 DICHLORPROP


R.T.: 7.742 min
Delta R.T.: 0.027 min
Response: 9577522
Conc: 16.31 ng/ml

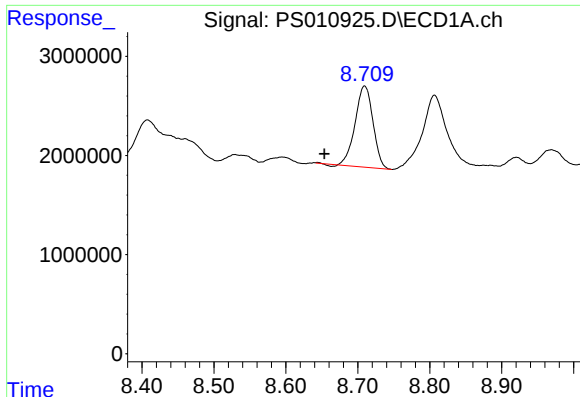

#10 Pentachlorophenol


R.T.: 8.710 min
Delta R.T.: 0.056 min
Response: 14047123
Conc: 1.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129734BL

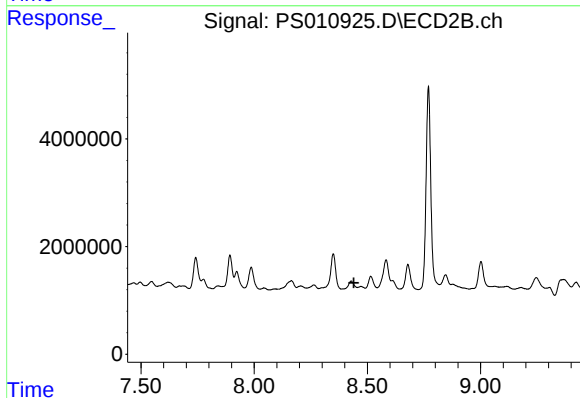


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.440 min
Response: 0
Conc: N.D.

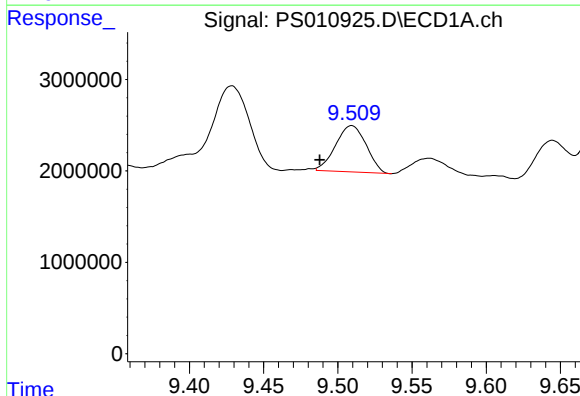


#12 2,4,5-T

R.T.: 9.509 min
Delta R.T.: 0.022 min
Response: 7245715
Conc: 1.56 ng/ml

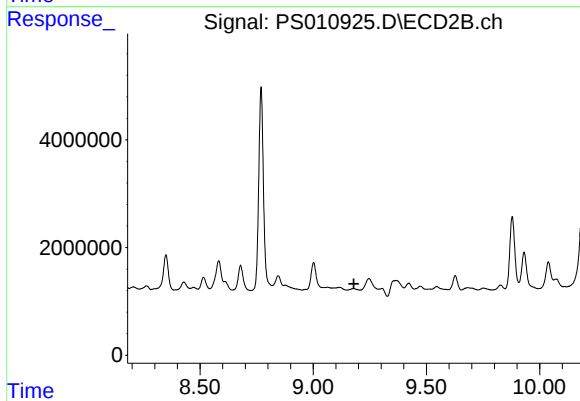

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

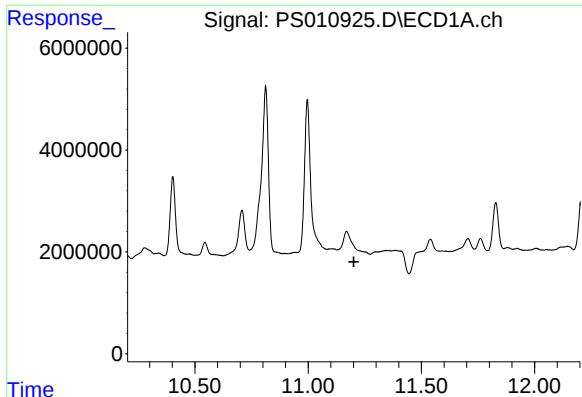

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.202 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB129734BL

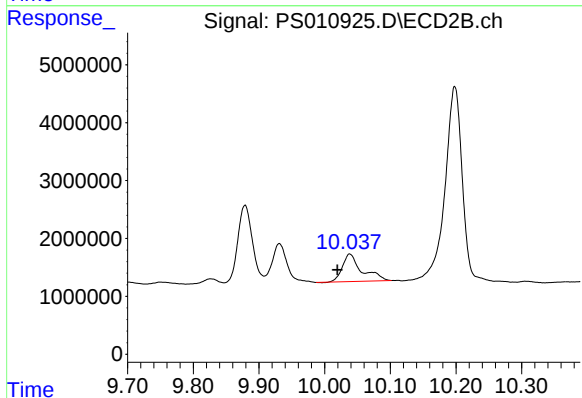


#14 DINOSEB

R.T.: 10.039 min
Delta R.T.: 0.019 min
Response: 9719659
Conc: 4.67 ng/ml

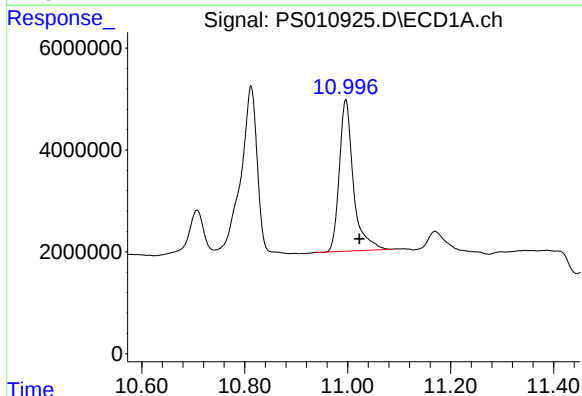

#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.026 min
Response: 56349806
Conc: 10.05 ng/ml

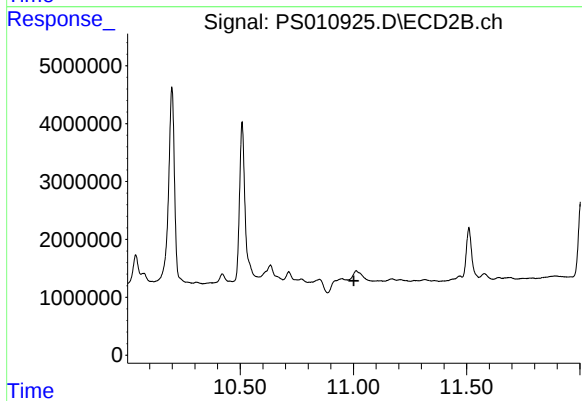

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.002 min
Response: 0
Conc: N.D.