

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062520\
 Data File : PS010935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2020 17:52
 Operator : DD\AJ
 Sample : PB129751BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB129751BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:38:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.920	458.9E6	312.5E6	506.103	563.992
Target Compounds							
1) T	Dalapon	2.996	2.582	37924461	80501421	33.870	106.715 #
2) T	3,5-DICHL...	0.000	6.101	0	48735085	N.D.	58.518
3) T	4-Nitroph...	7.004	0.000	3610576	0	9.045	N.D. #
7) T	MCPA	7.721	7.385	9814918	39433797	2.465	14.288 #
8) T	DICHLORPROP	0.000	7.743	0	10533454	N.D.	17.940
10) T	Pentachlo...	8.710	0.000	11907663	0	<MDL	N.D. #
12) T	2,4,5-T	9.510	0.000	8221303	0	1.765	N.D. #
14) T	DINOSEB	0.000	10.038	0	9762629	N.D.	4.689
15) T	Picloram	11.033	11.013	12898769	15561712	2.301	3.714 #
16) T	DCPA	0.000	11.013	0	15561712	N.D.	4.178



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062520\
Data File : PS010935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2020 17:52
Operator : DD\AJ
Sample : PB129751BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB129751BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:38:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

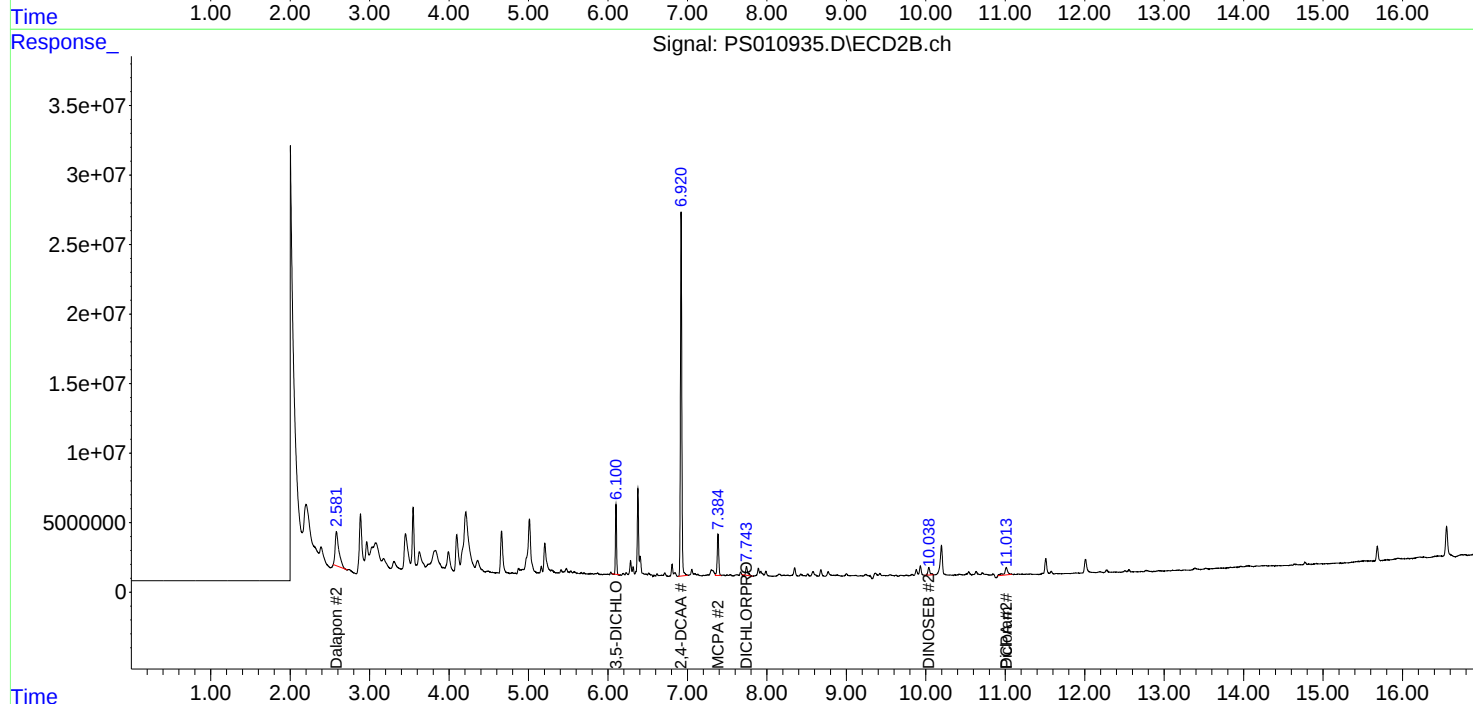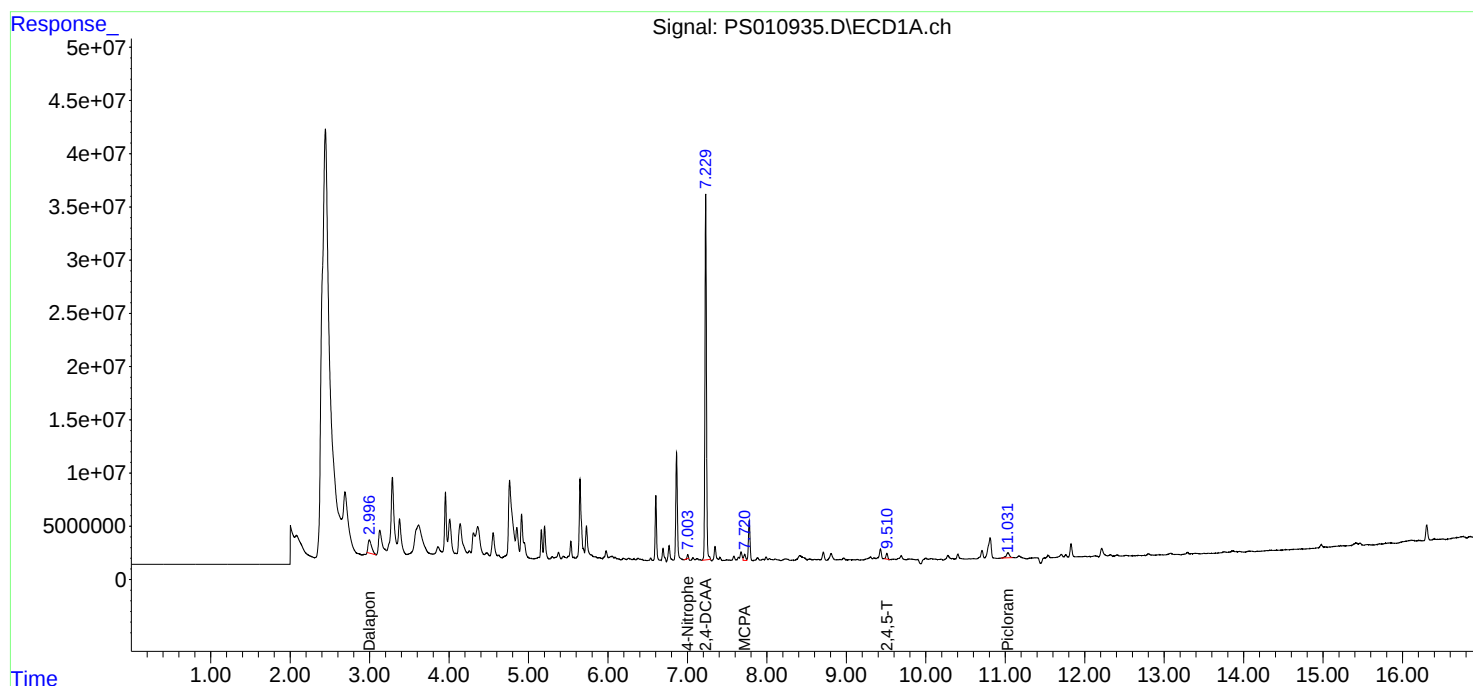


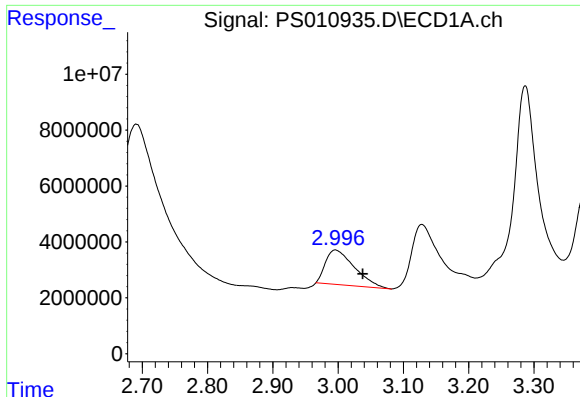

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 37924461
Conc: 33.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129751BL

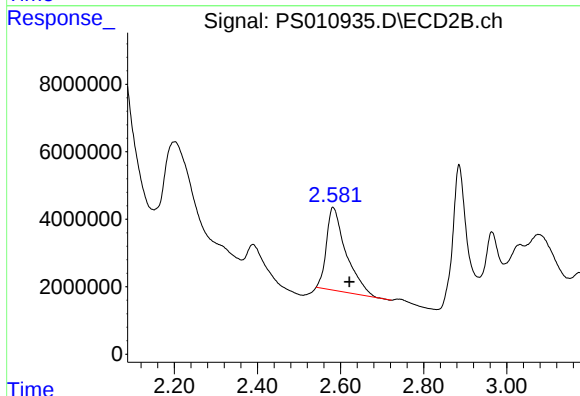


#1 Dalapon

R.T.: 2.582 min
Delta R.T.: -0.040 min
Response: 80501421
Conc: 106.71 ng/ml

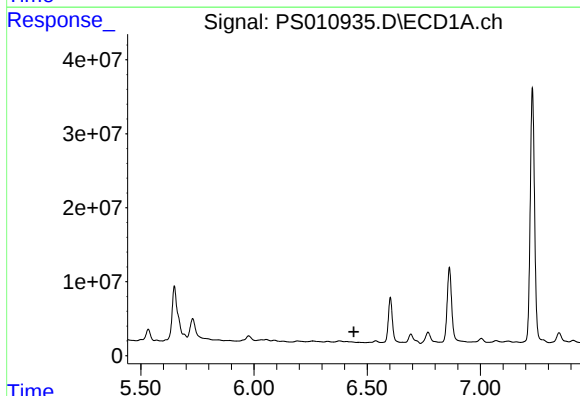


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

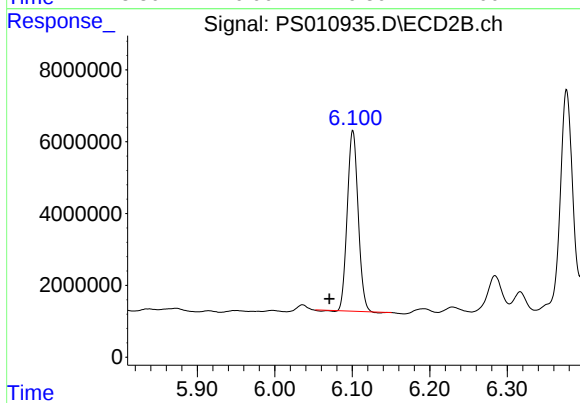

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 48735085
Conc: 58.52 ng/ml

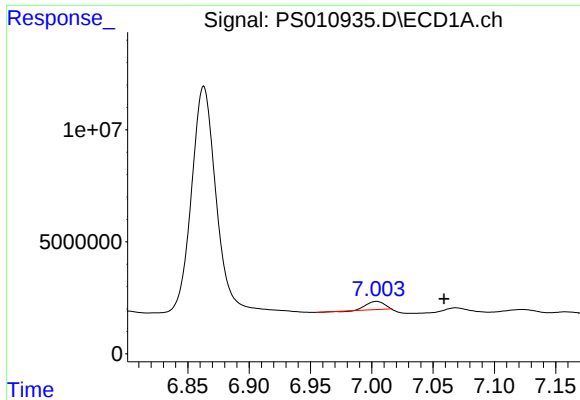

#3 4-Nitrophenol


R.T.: 7.004 min
Delta R.T.: -0.055 min
Response: 3610576
Conc: 9.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129751BL

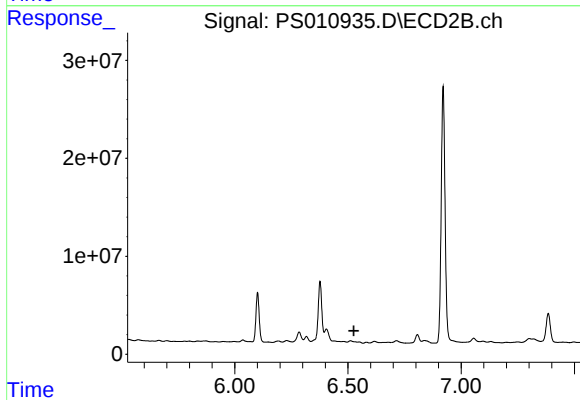


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.526 min
Response: 0
Conc: N.D.

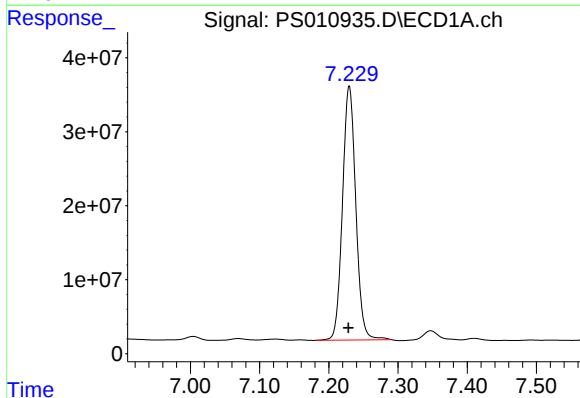


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.001 min
Response: 458943397
Conc: 506.10 ng/ml

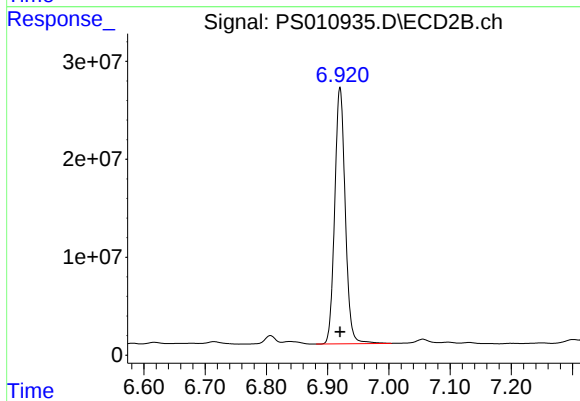

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 312494663
Conc: 563.99 ng/ml

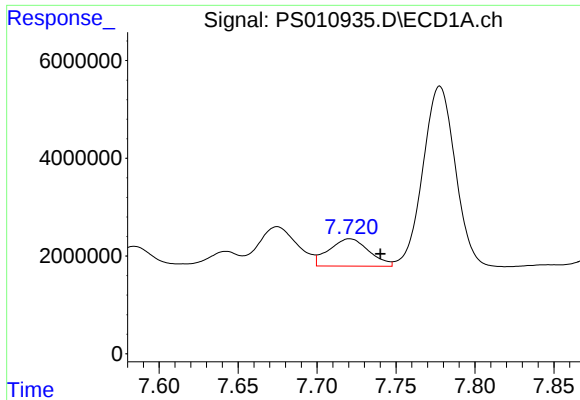

#7 MCPA


R.T.: 7.721 min
Delta R.T.: -0.019 min
Response: 9814918
Conc: 2.46 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB129751BL

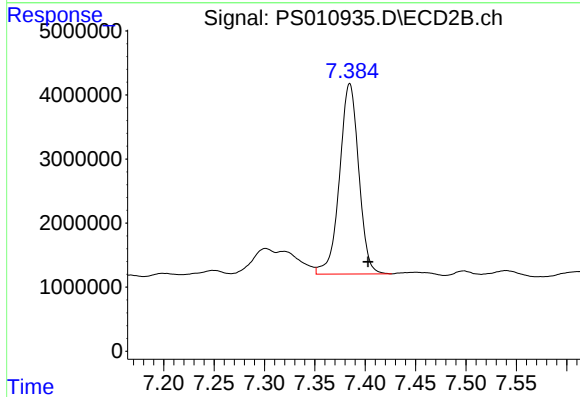


#7 MCPA

R.T.: 7.385 min
Delta R.T.: -0.018 min
Response: 39433797
Conc: 14.29 ug/ml

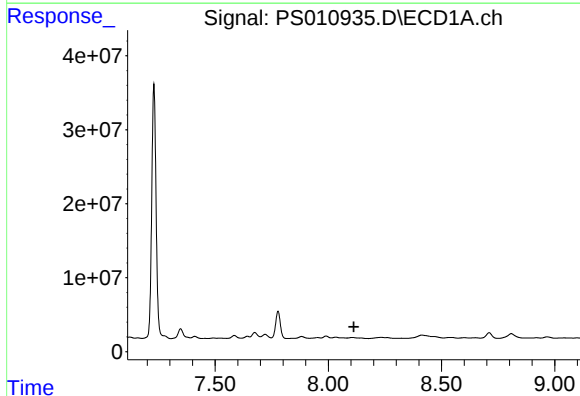


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

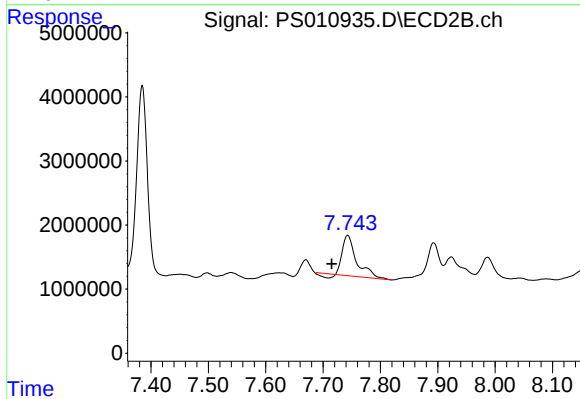

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.028 min
Response: 10533454
Conc: 17.94 ng/ml

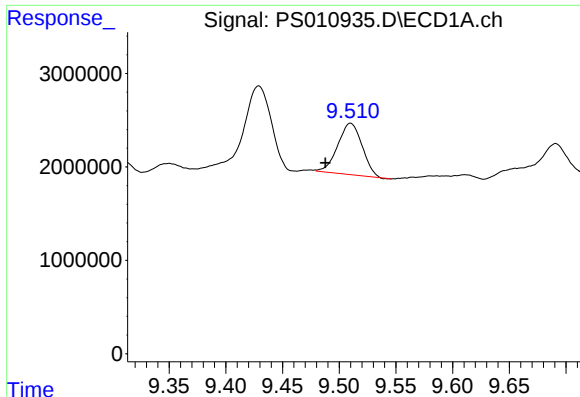

#12 2,4,5-T


R.T.: 9.510 min
Delta R.T.: 0.022 min
Response: 8221303
Conc: 1.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129751BL

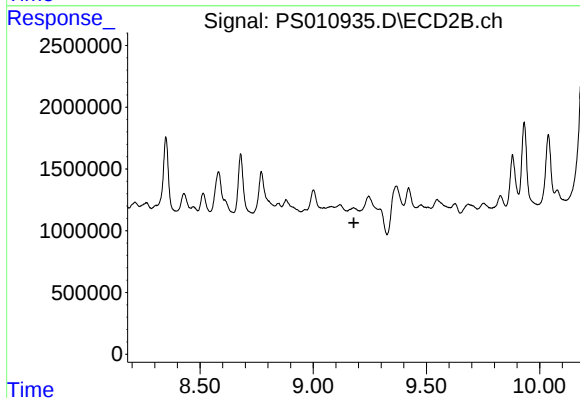


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

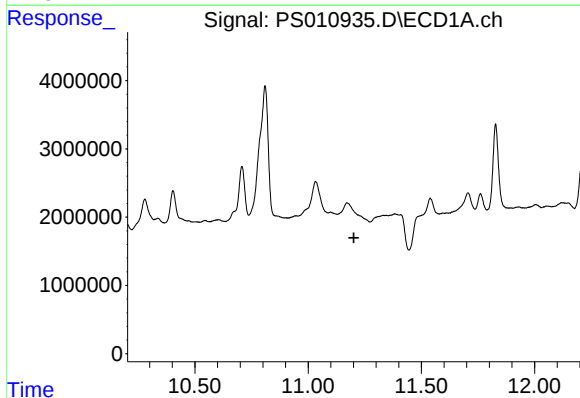


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.202 min
Response: 0
Conc: N.D.

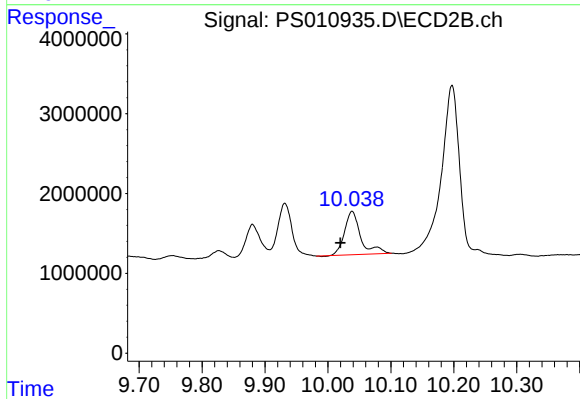

#14 DINOSEB


R.T.: 10.038 min
Delta R.T.: 0.019 min
Response: 9762629
Conc: 4.69 ng/ml

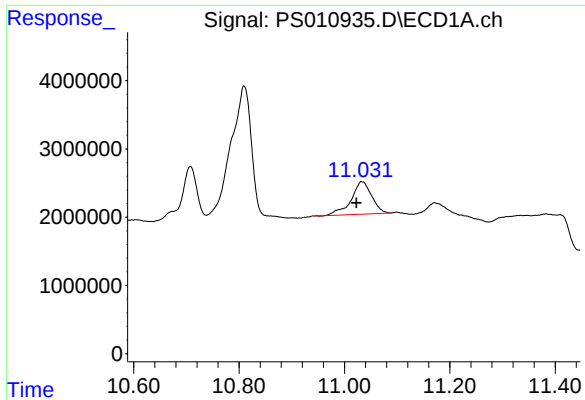

#15 Picloram


R.T.: 11.033 min
Delta R.T.: 0.010 min
Response: 12898769
Conc: 2.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129751BL

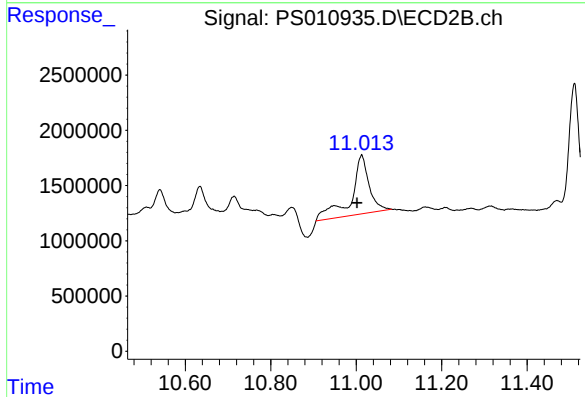


#15 Picloram

R.T.: 11.013 min
Delta R.T.: 0.011 min
Response: 15561712
Conc: 3.71 ng/ml

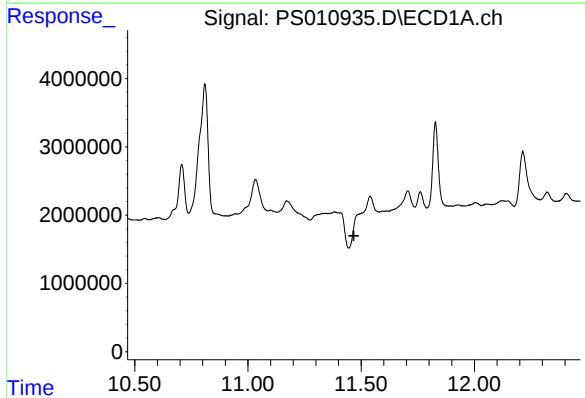

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.468 min
Response: 0
Conc: N.D.

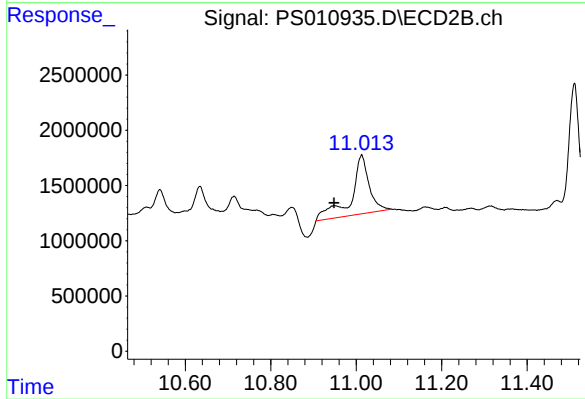

#16 DCPA

R.T.: 11.013 min
Delta R.T.: 0.064 min
Response: 15561712
Conc: 4.18 ng/ml