

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062520\
 Data File : PS010937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2020 18:38
 Operator : DD\AJ
 Sample : PB129751TB
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB129751TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:39:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	364.0E6	256.3E6	401.416	462.527
Target Compounds							
1) T	Dalapon	2.995	2.583	38303806	91688354	34.208	121.544 #
2) T	3,5-DICHL...	0.000	6.100	0	62311872	N.D.	74.820
5) T	DICAMBA	7.409	0.000	5916805	0	1.623	N.D. #
6) T	MCP	7.642	0.000	6168119	0	2.163	N.D. #
7) T	MCPA	7.694	7.465	70469957	42900668	17.695	15.544
8) T	DICHLORPROP	0.000	7.741	0	22286291	N.D.	37.958
10) T	Pentachlo...	8.710	0.000	9998686	0	<MDL	N.D. #
12) T	2,4,5-T	9.427	0.000	16577052	0	3.559	N.D. #
15) T	Picloram	11.026	0.000	12355307	0	2.204	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062520\
Data File : PS010937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2020 18:38
Operator : DD\AJ
Sample : PB129751TB
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB129751TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:39:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

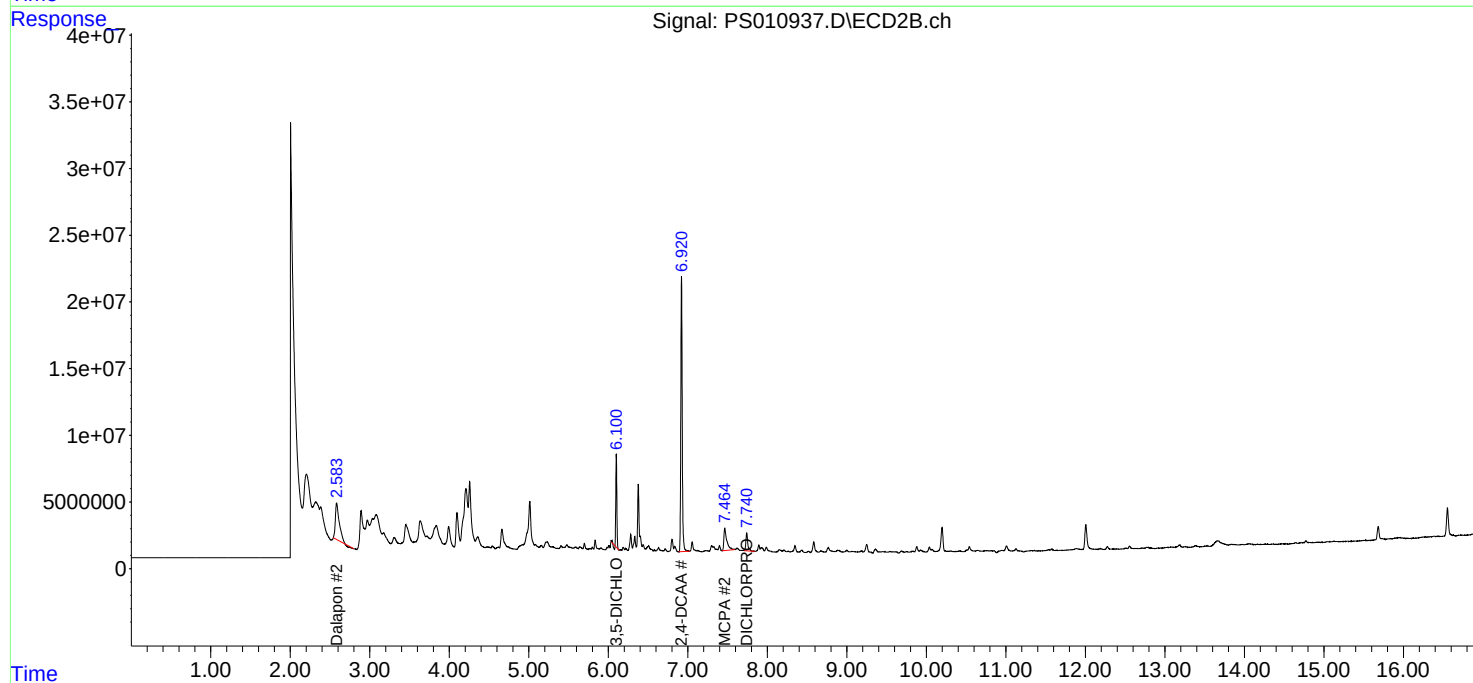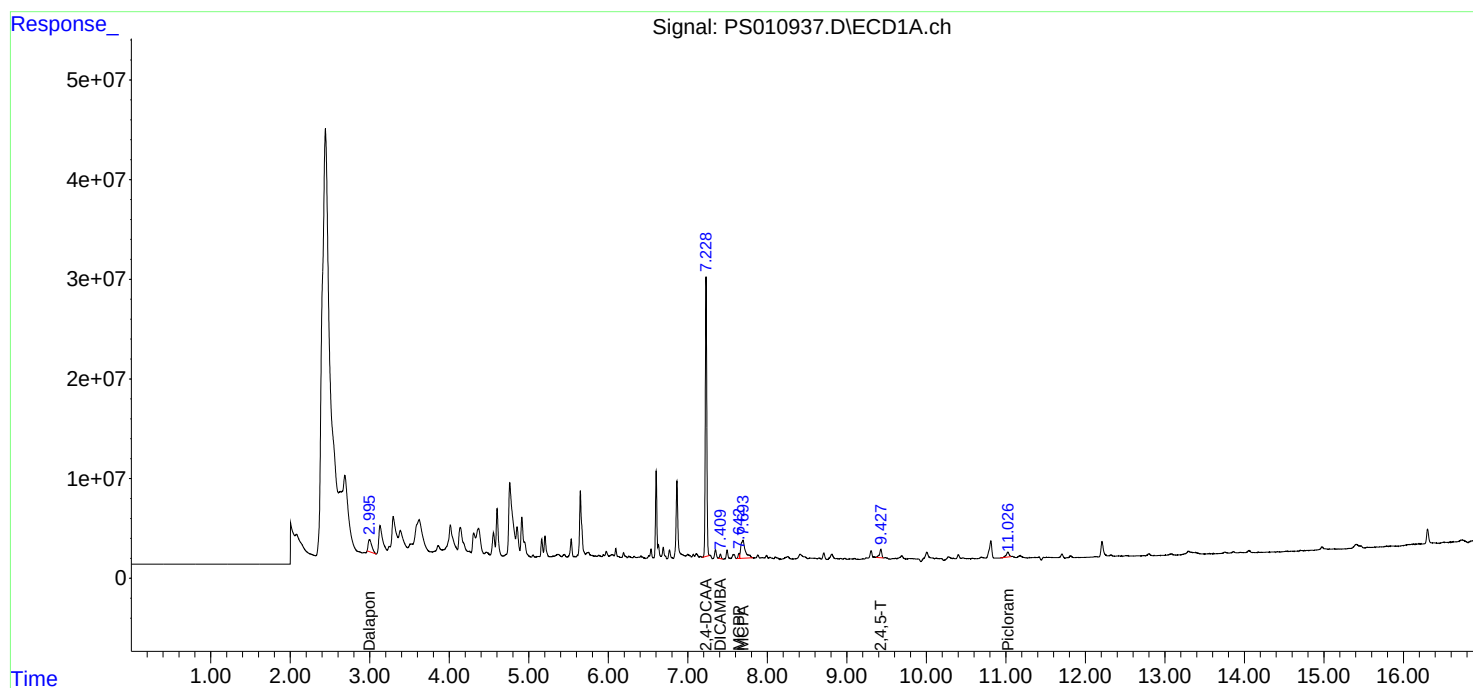


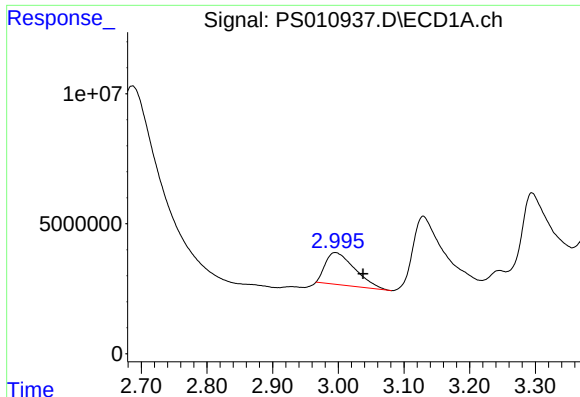

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.043 min
Response: 38303806
Conc: 34.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129751TB

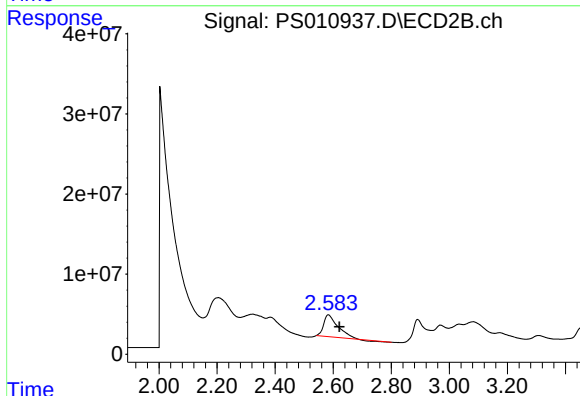


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.039 min
Response: 91688354
Conc: 121.54 ng/ml

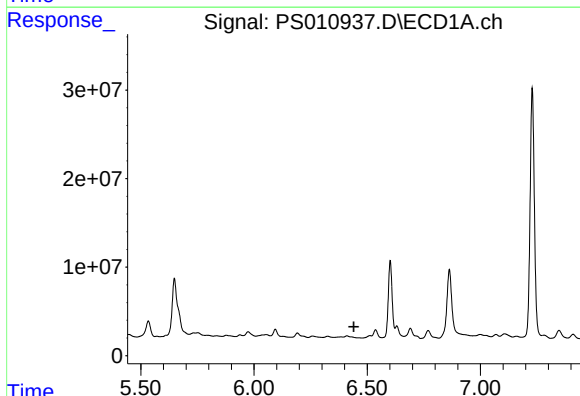


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

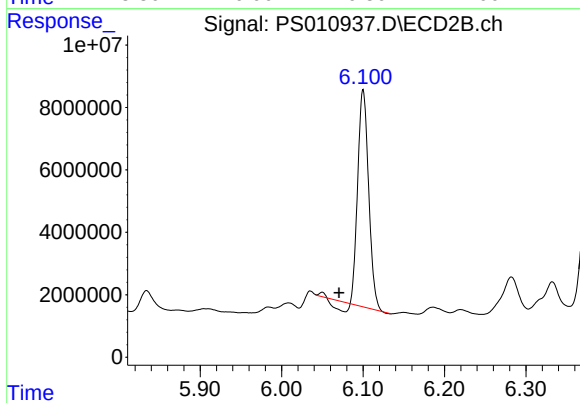

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 62311872
Conc: 74.82 ng/ml

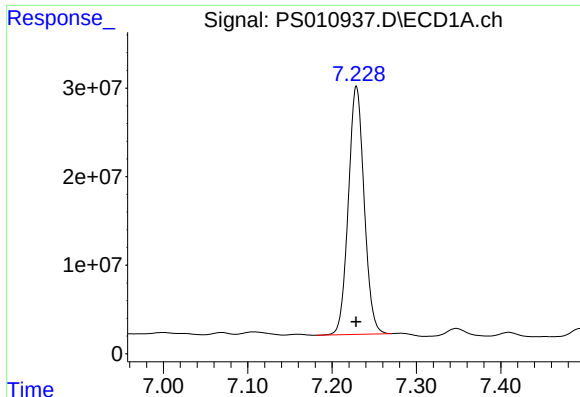

#4 2,4-DCAA


R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 364011579
Conc: 401.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129751TB

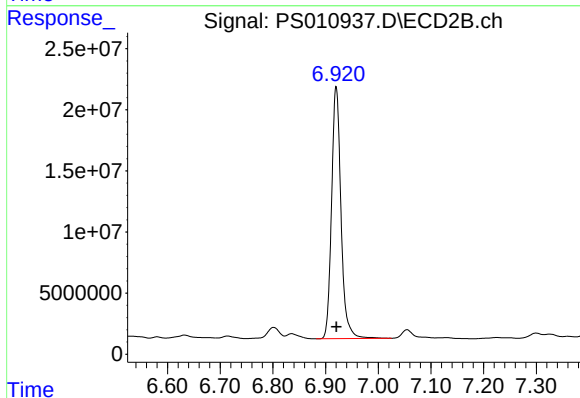


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 256275368
Conc: 462.53 ng/ml

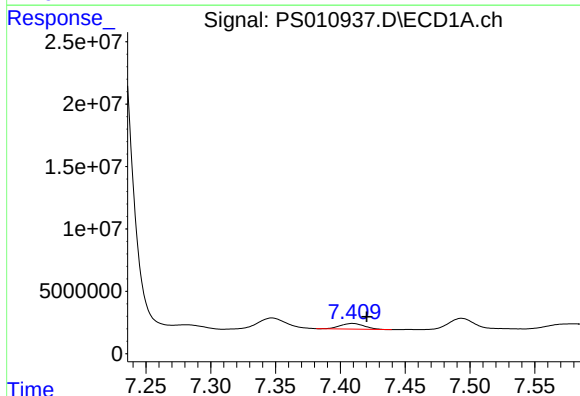


#5 DICAMBA

R.T.: 7.409 min
Delta R.T.: -0.011 min
Response: 5916805
Conc: 1.62 ng/ml

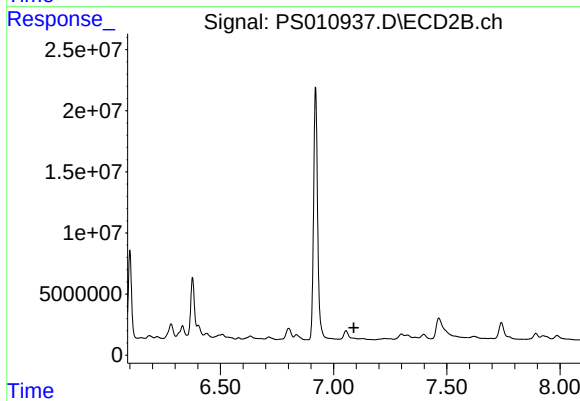

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.089 min
Response: 0
Conc: N.D.

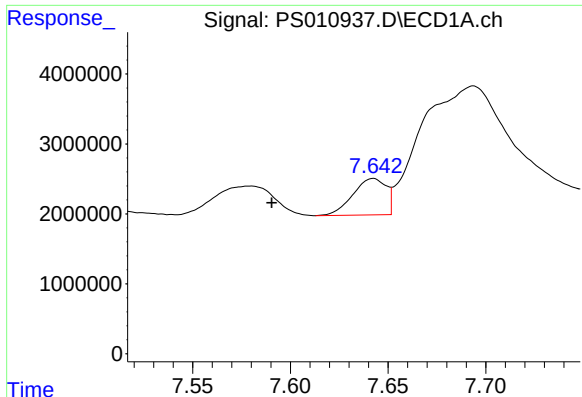

#6 MCP


R.T.: 7.642 min
Delta R.T.: 0.052 min
Response: 6168119
Conc: 2.16 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB129751TB

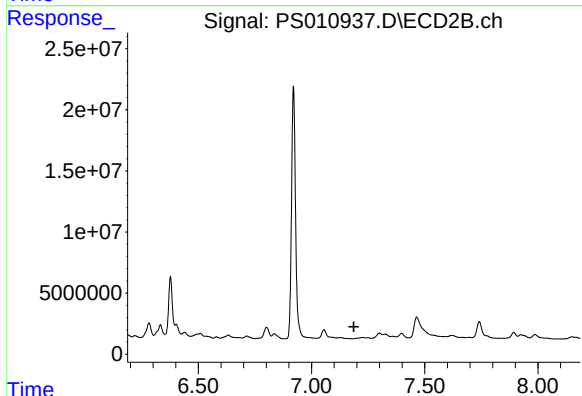


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

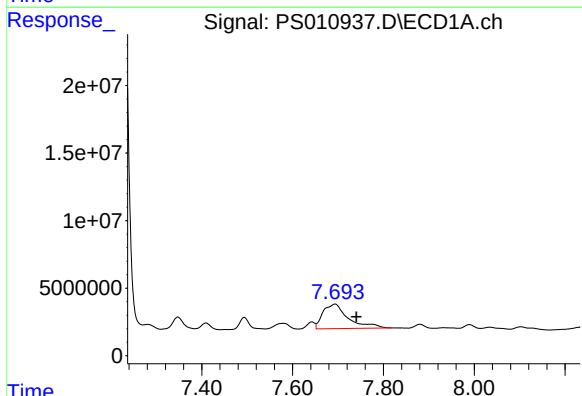


#7 MCP

R.T.: 7.694 min
Delta R.T.: -0.046 min
Response: 70469957
Conc: 17.70 ug/ml

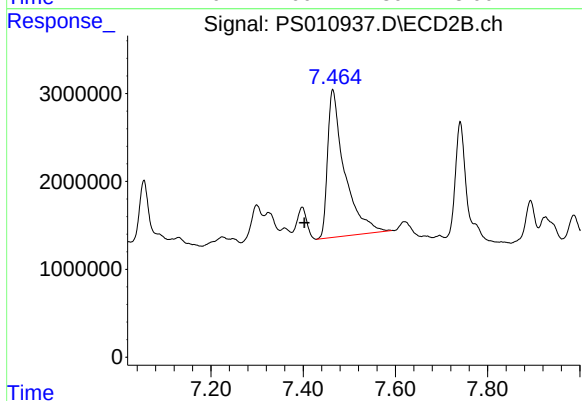

#7 MCP


R.T.: 7.465 min
Delta R.T.: 0.062 min
Response: 42900668
Conc: 15.54 ug/ml

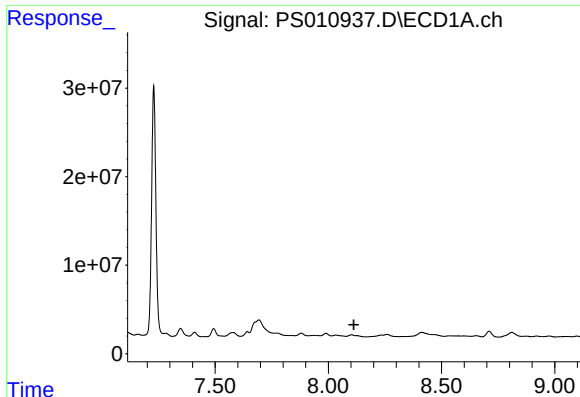

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB129751TB

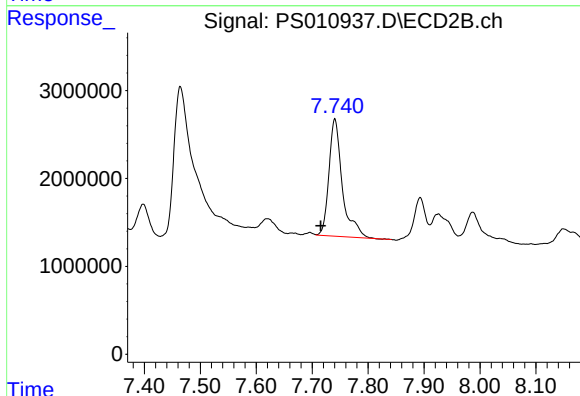


#8 DICHLORPROP

R.T.: 7.741 min
Delta R.T.: 0.025 min
Response: 22286291
Conc: 37.96 ng/ml

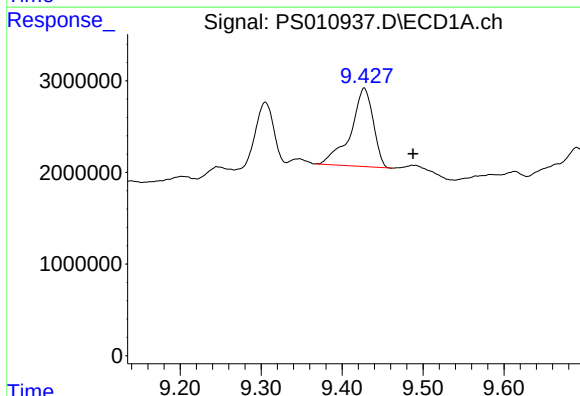


#12 2,4,5-T

R.T.: 9.427 min
Delta R.T.: -0.060 min
Response: 16577052
Conc: 3.56 ng/ml

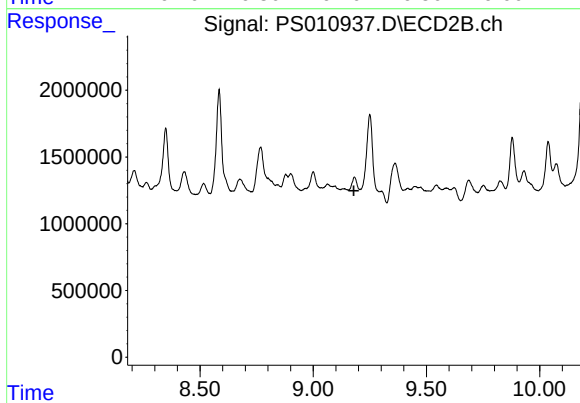

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

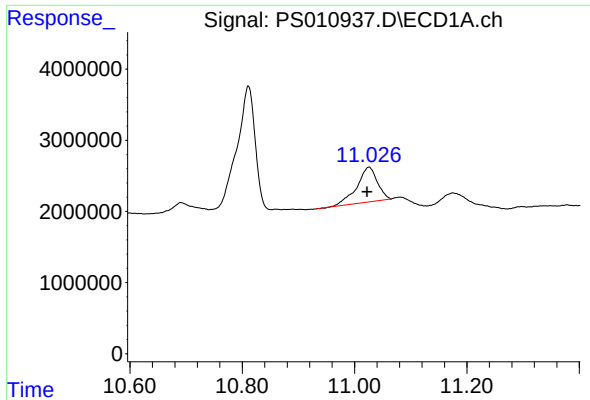

#15 Picloram

R.T.: 11.026 min
Delta R.T.: 0.003 min
Response: 12355307
Conc: 2.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129751TB

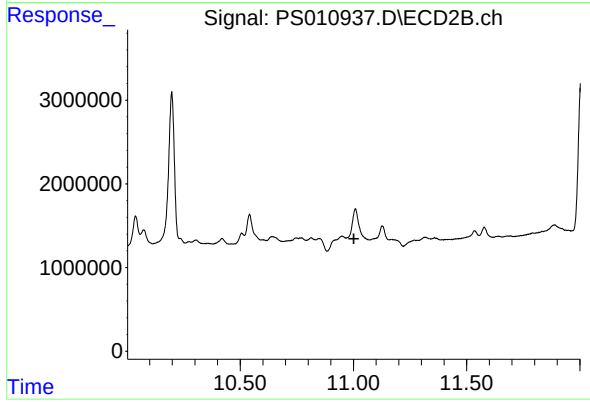

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.