

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062521\
 Data File : PS015932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 13:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 02:27:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.766	910.1E6	336.3E6	547.787	667.367
Target Compounds							
9) T	2,4-D	8.372f	0.000	46625113	0	26.604	N.D. #
12) T	2,4,5-T	0.000	9.062f	0	10959997	N.D.	3.886
15) T	Picloram	10.983	10.822	115.5E6	41525085	8.450	9.874
16) T	DCPA	0.000	10.822f	0	41525085	N.D.	9.877



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062521\
Data File : PS015932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 13:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 02:27:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

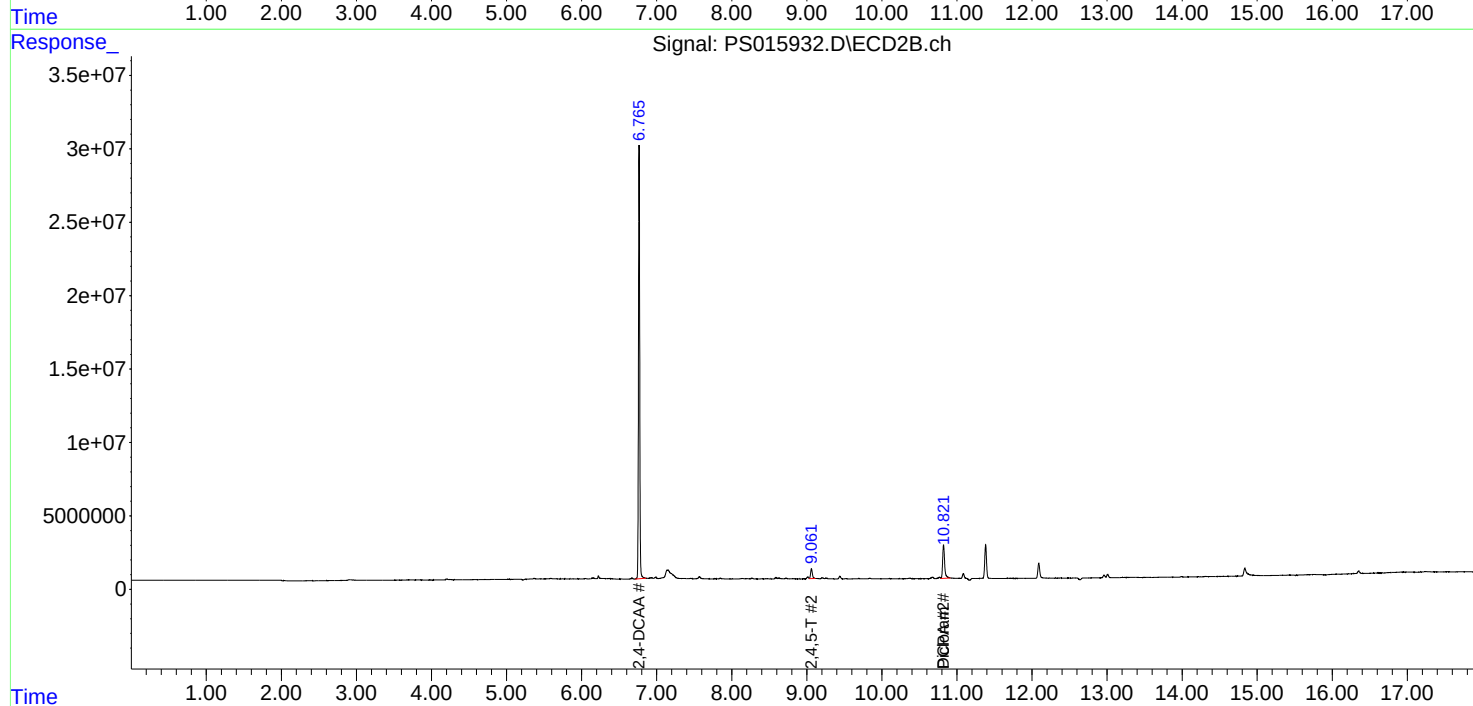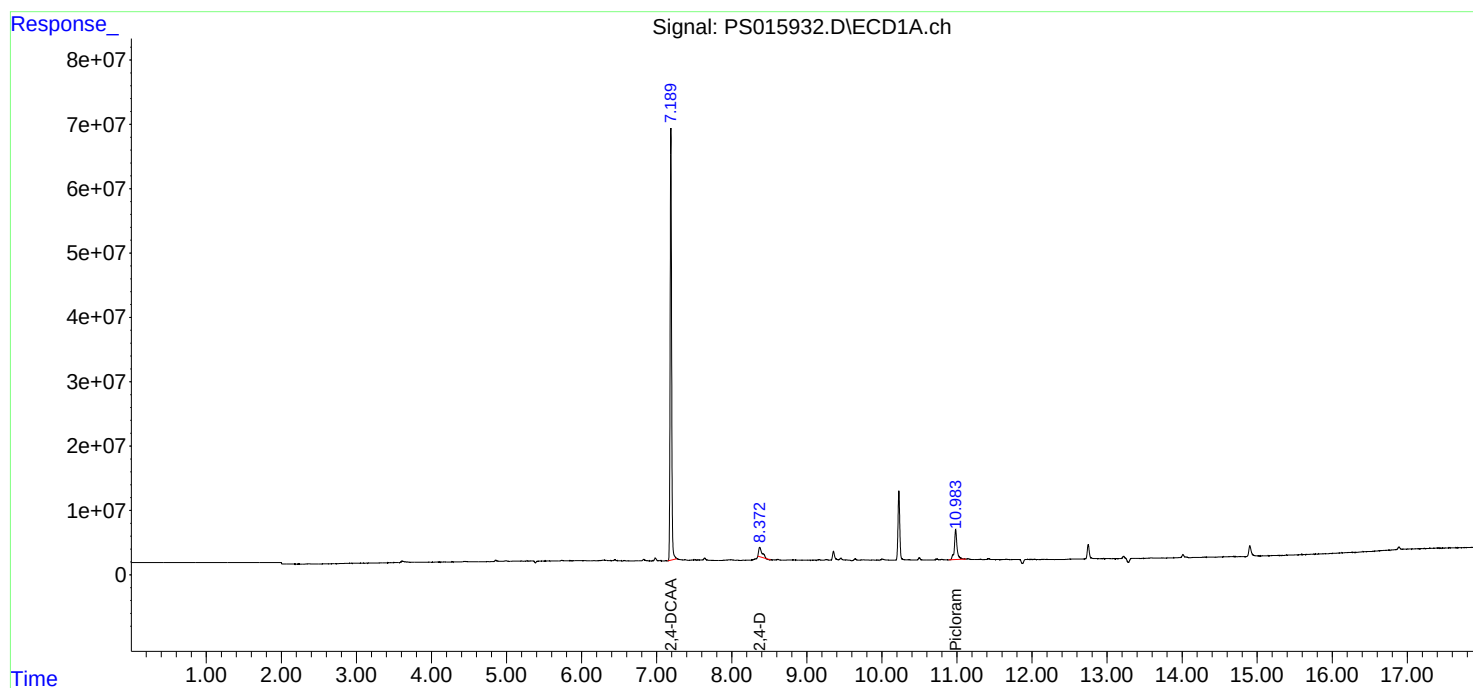


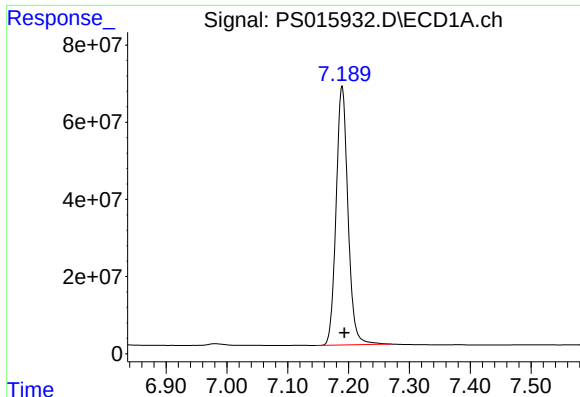

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 910119508
Conc: 547.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

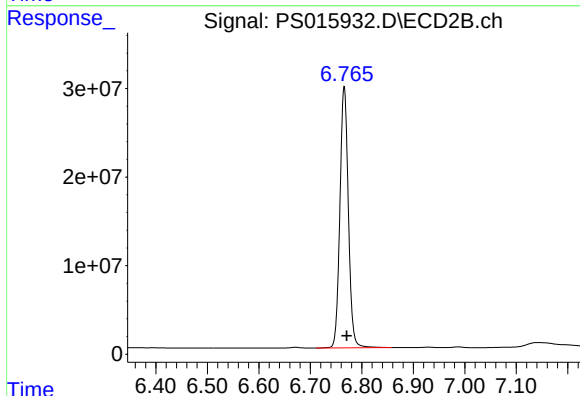


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: -0.005 min
Response: 336254239
Conc: 667.37 ng/ml

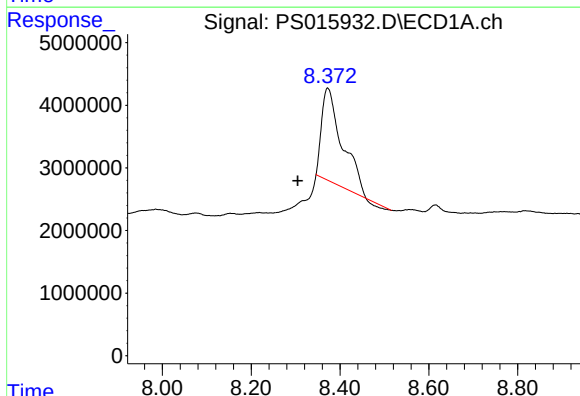


#9 2,4-D

R.T.: 8.372 min
Delta R.T.: 0.067 min
Response: 46625113
Conc: 26.60 ng/ml

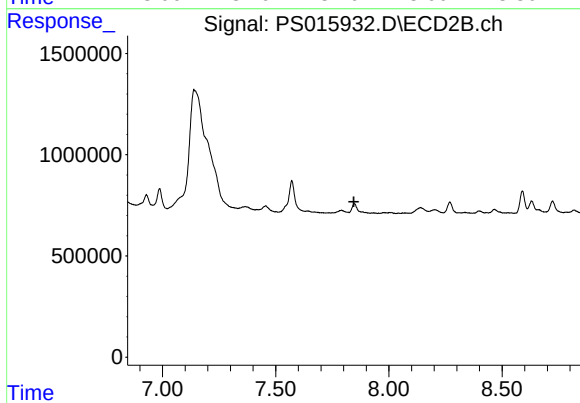

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

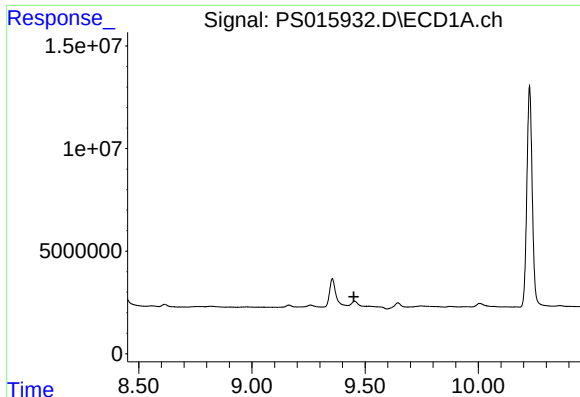

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.450 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

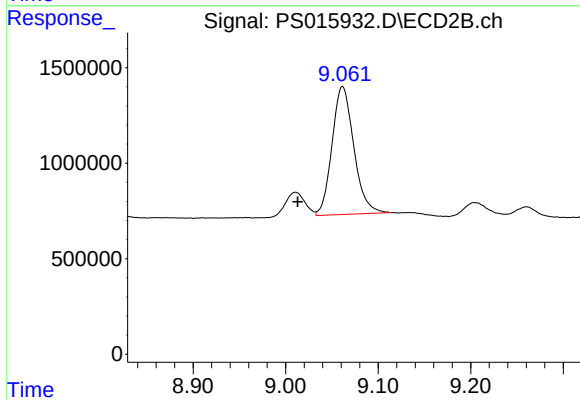


#12 2,4,5-T

R.T.: 9.062 min
Delta R.T.: 0.048 min
Response: 10959997
Conc: 3.89 ng/ml

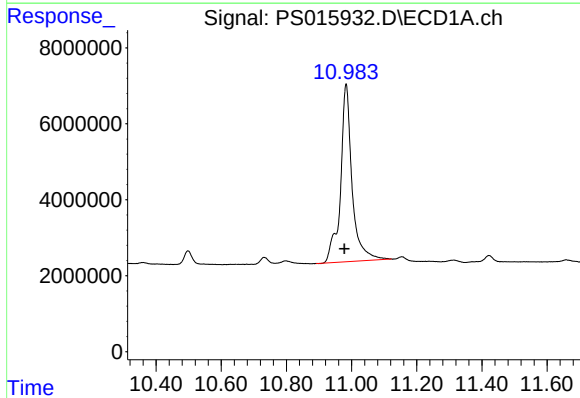


#15 Picloram

R.T.: 10.983 min
Delta R.T.: 0.005 min
Response: 115513093
Conc: 8.45 ng/ml

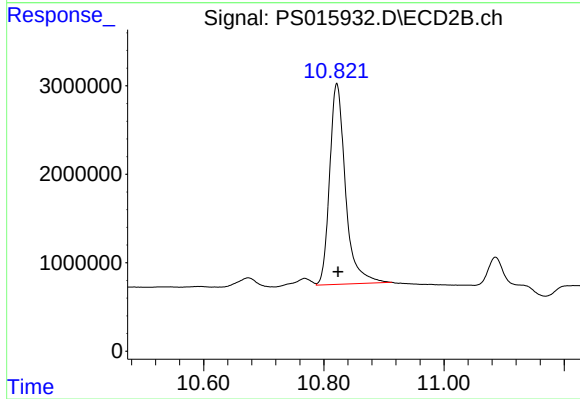

#15 Picloram


R.T.: 10.822 min
Delta R.T.: -0.002 min
Response: 41525085
Conc: 9.87 ng/ml

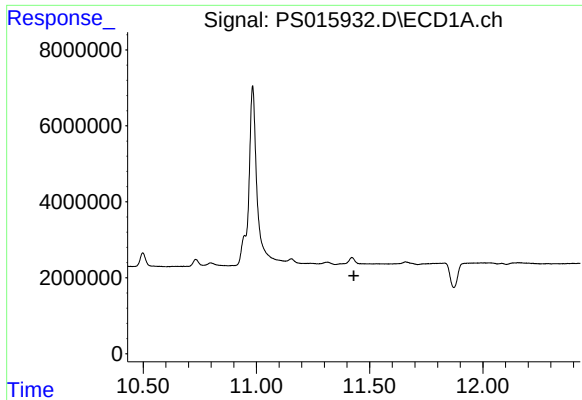

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

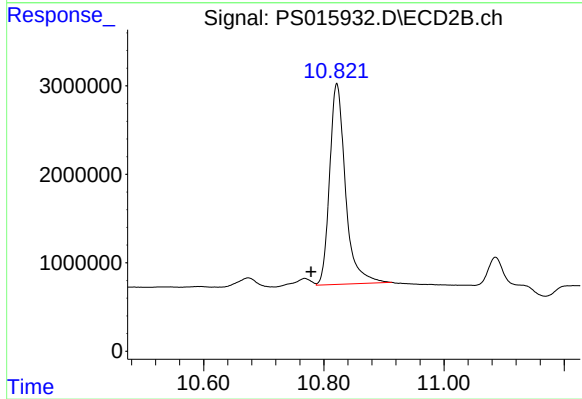

#16 DCPA

R.T.: 10.822 min
Delta R.T.: 0.043 min
Response: 41525085
Conc: 9.88 ng/ml