

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062521\
 Data File : PS015934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 16:00
 Operator : DD\AJ
 Sample : PB137334BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 02:27:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.766	406.1E6	137.2E6	244.453	272.360
Target Compounds							
1) T	Dalapon	2.988	2.500	39301199	30160936	19.472	46.438 #
2) T	3,5-DICHL...	0.000	5.983	0	20844007	N.D.	27.639
3) T	4-Nitroph...	7.089f	0.000	11687989	0	12.856	N.D. #
5) T	DICAMBA	7.372	0.000	6241406	0	<MDL	N.D. #
6) T	MCPD	7.596	0.000	3980754	0	<MDL	N.D. #
7) T	MCPA	0.000	7.226	0	9711368	N.D.	3.785
8) T	DICHLORPROP	8.021f	7.568	7445391	17623094	4.702	34.038 #
13) T	2,4-DB	10.036	0.000	12754347	0	6.235	N.D. #
14) T	DINOSEB	11.191	0.000	18851672	0	2.911	N.D. #
15) T	Picloram	10.973	10.818	176.4E6	43749646	12.900	10.403
16) T	DCPA	11.433	10.818	9675212	43749646	<MDL	10.406 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062521\
Data File : PS015934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 16:00
Operator : DD\AJ
Sample : PB137334BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 02:27:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

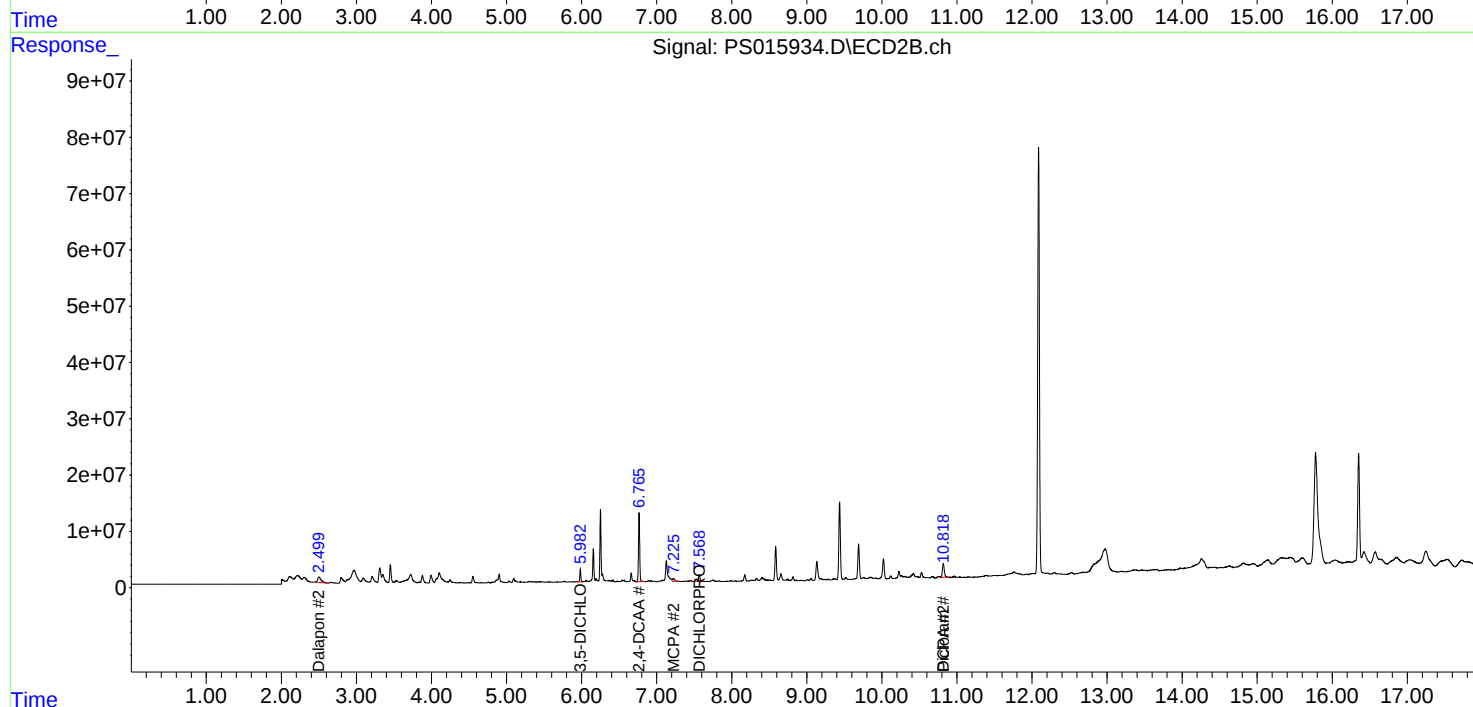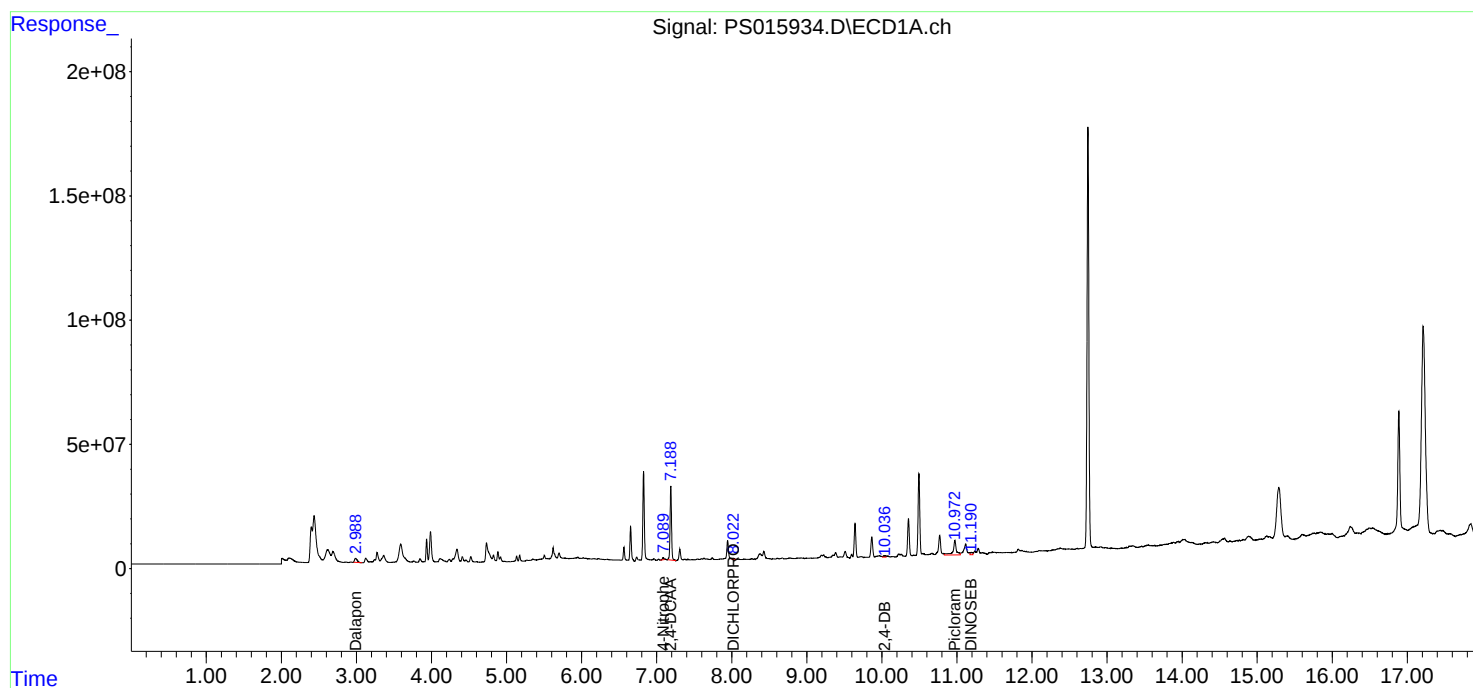


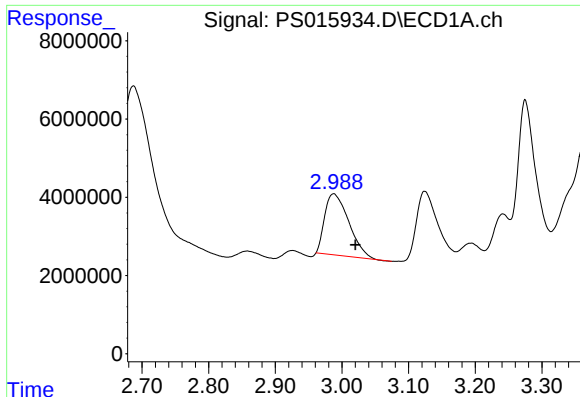

#1 Dalapon


R.T.: 2.988 min
Delta R.T.: -0.032 min
Response: 39301199
Conc: 19.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

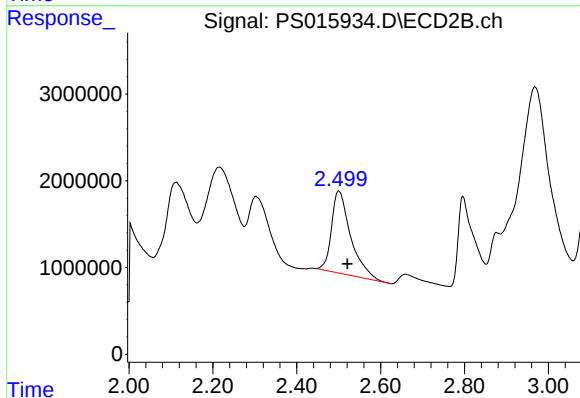


#1 Dalapon

R.T.: 2.500 min
Delta R.T.: -0.020 min
Response: 30160936
Conc: 46.44 ng/ml

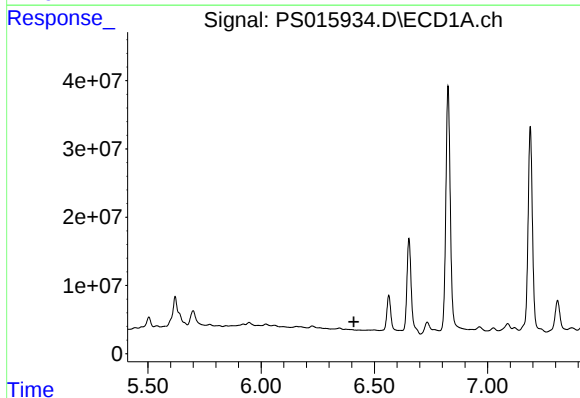


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

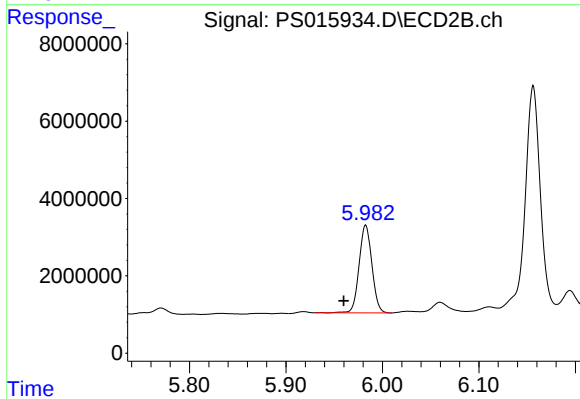

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.983 min
Delta R.T.: 0.023 min
Response: 20844007
Conc: 27.64 ng/ml

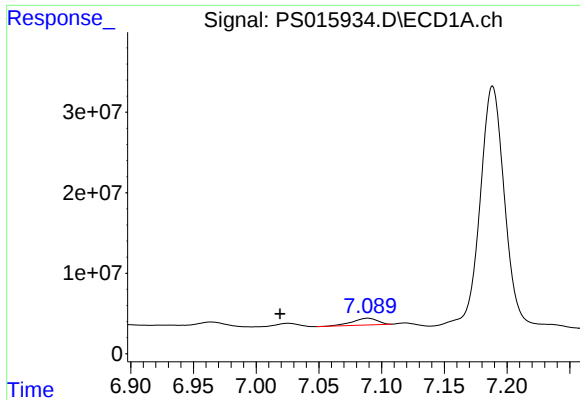

#3 4-Nitrophenol


R.T.: 7.089 min
Delta R.T.: 0.070 min
Response: 11687989
Conc: 12.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

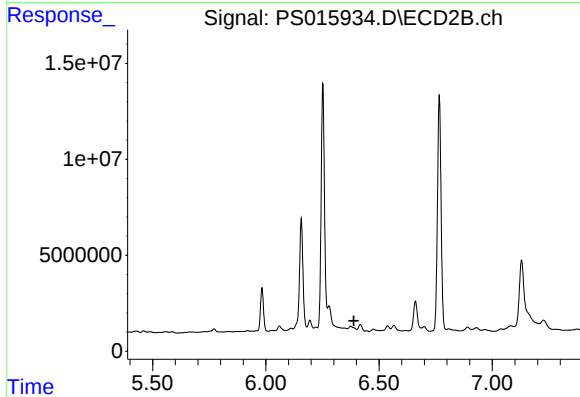


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

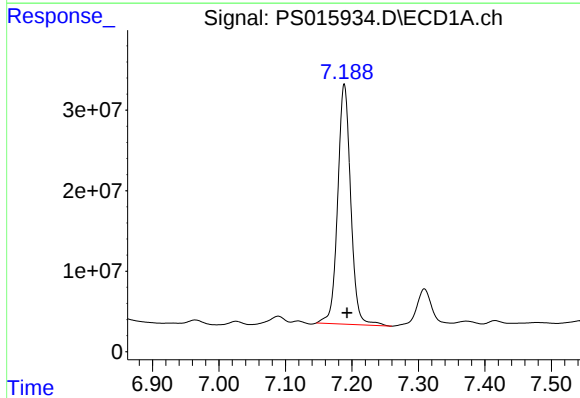


#4 2,4-DCAA

R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 406145076
Conc: 244.45 ng/ml

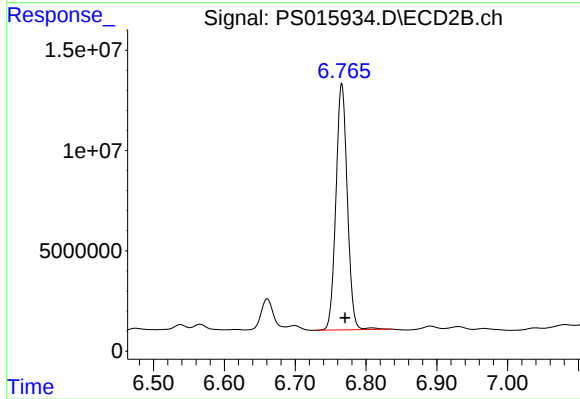

#4 2,4-DCAA


R.T.: 6.766 min
Delta R.T.: -0.005 min
Response: 137228900
Conc: 272.36 ng/ml

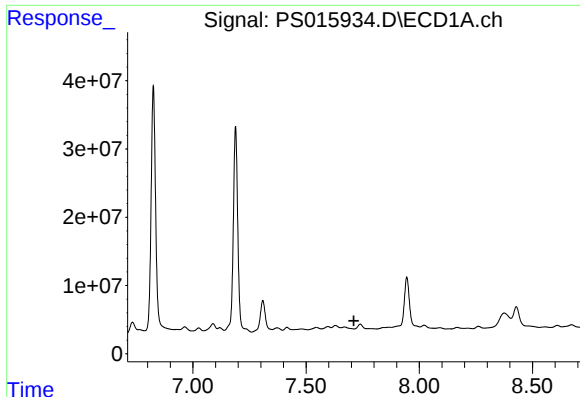

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

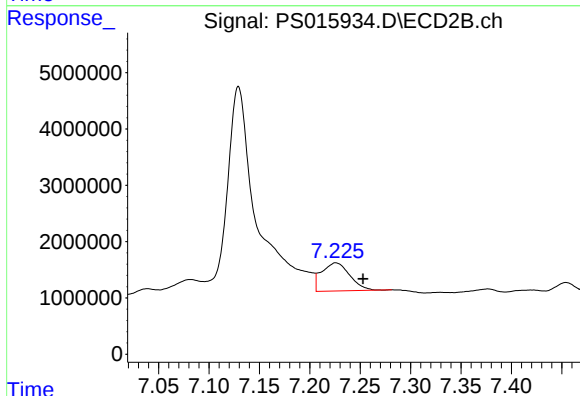


#7 MCPA

R.T.: 7.226 min
Delta R.T.: -0.027 min
Response: 9711368
Conc: 3.79 ug/ml

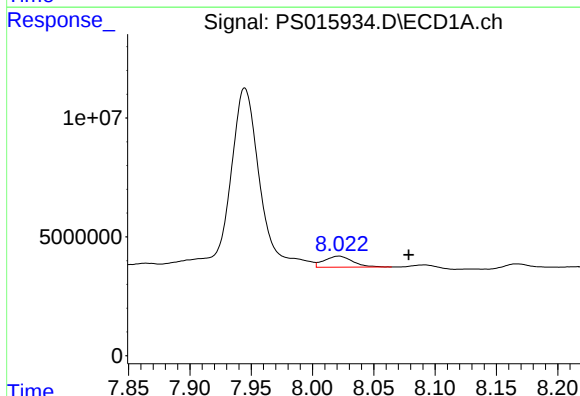


#8 DICHLORPROP

R.T.: 8.021 min
Delta R.T.: -0.057 min
Response: 7445391
Conc: 4.70 ng/ml

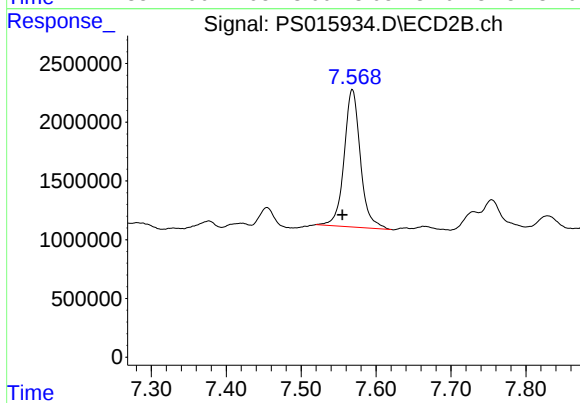

#8 DICHLORPROP


R.T.: 7.568 min
Delta R.T.: 0.013 min
Response: 17623094
Conc: 34.04 ng/ml

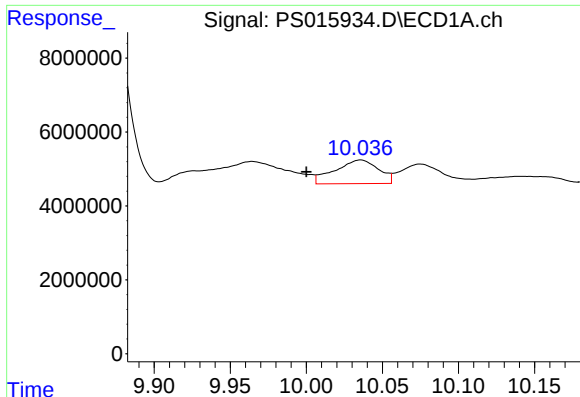

#13 2,4-DB


R.T.: 10.036 min
Delta R.T.: 0.036 min
Response: 12754347
Conc: 6.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

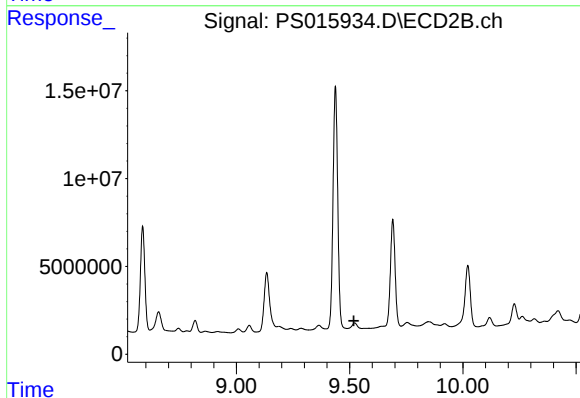


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.519 min
Response: 0
Conc: N.D.

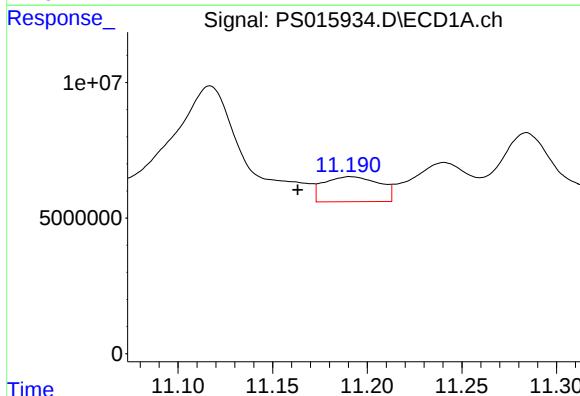


#14 DINOSEB

R.T.: 11.191 min
Delta R.T.: 0.028 min
Response: 18851672
Conc: 2.91 ng/ml

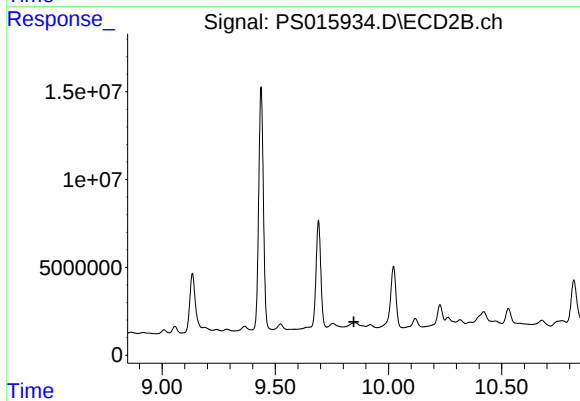

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.847 min
Response: 0
Conc: N.D.

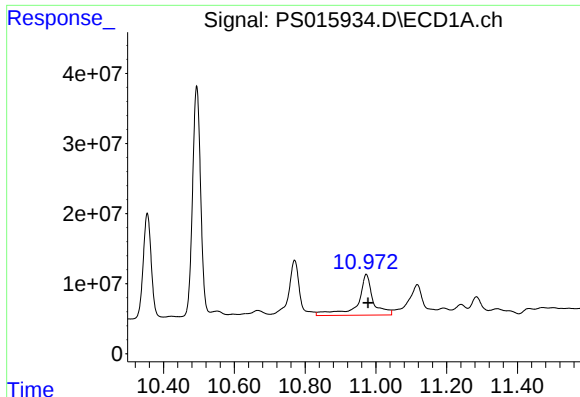

#15 Picloram


R.T.: 10.973 min
Delta R.T.: -0.005 min
Response: 176352515
Conc: 12.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

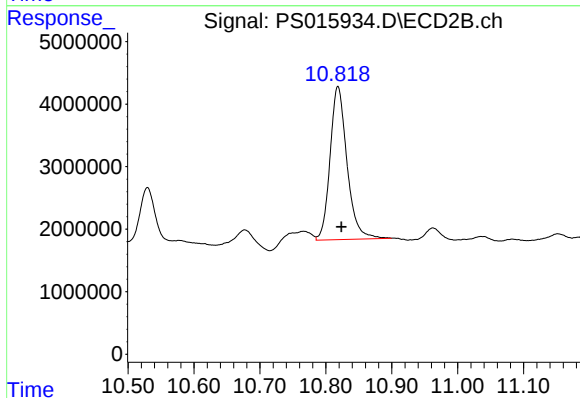


#15 Picloram

R.T.: 10.818 min
Delta R.T.: -0.005 min
Response: 43749646
Conc: 10.40 ng/ml

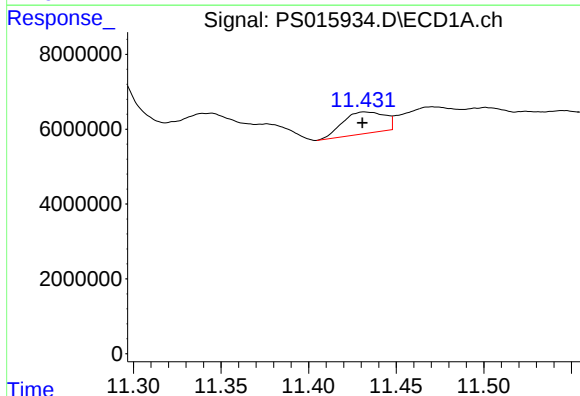

#16 DCPA

R.T.: 11.433 min
Delta R.T.: 0.002 min
Response: 9675212
Conc: N.D.

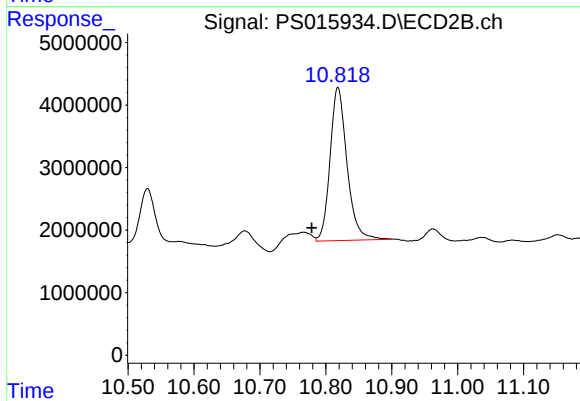

#16 DCPA

R.T.: 10.818 min
Delta R.T.: 0.040 min
Response: 43749646
Conc: 10.41 ng/ml