

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062521\
 Data File : PS015938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2021 17:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 02:28:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.765	915.2E6	333.2E6	550.834	661.237
Target Compounds							
8) T	DICHLORPROP	0.000	7.568	0	13759552	N.D.	26.576
9) T	2,4-D	8.374f	0.000	45447262	0	25.932	N.D. #
10) T	Pentachlo...	8.612	0.000	5913270	0	<MDL	N.D. #
12) T	2,4,5-T	9.445	0.000	10337177	0	1.171	N.D. #
14) T	DINOSEB	11.108f	0.000	12085338	0	1.866	N.D. #
15) T	Picloram	10.974	10.818	85859875	29374431	6.281	6.985
16) T	DCPA	11.419	10.818	9070494	29374431	<MDL	6.987 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062521\
Data File : PS015938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2021 17:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 02:28:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

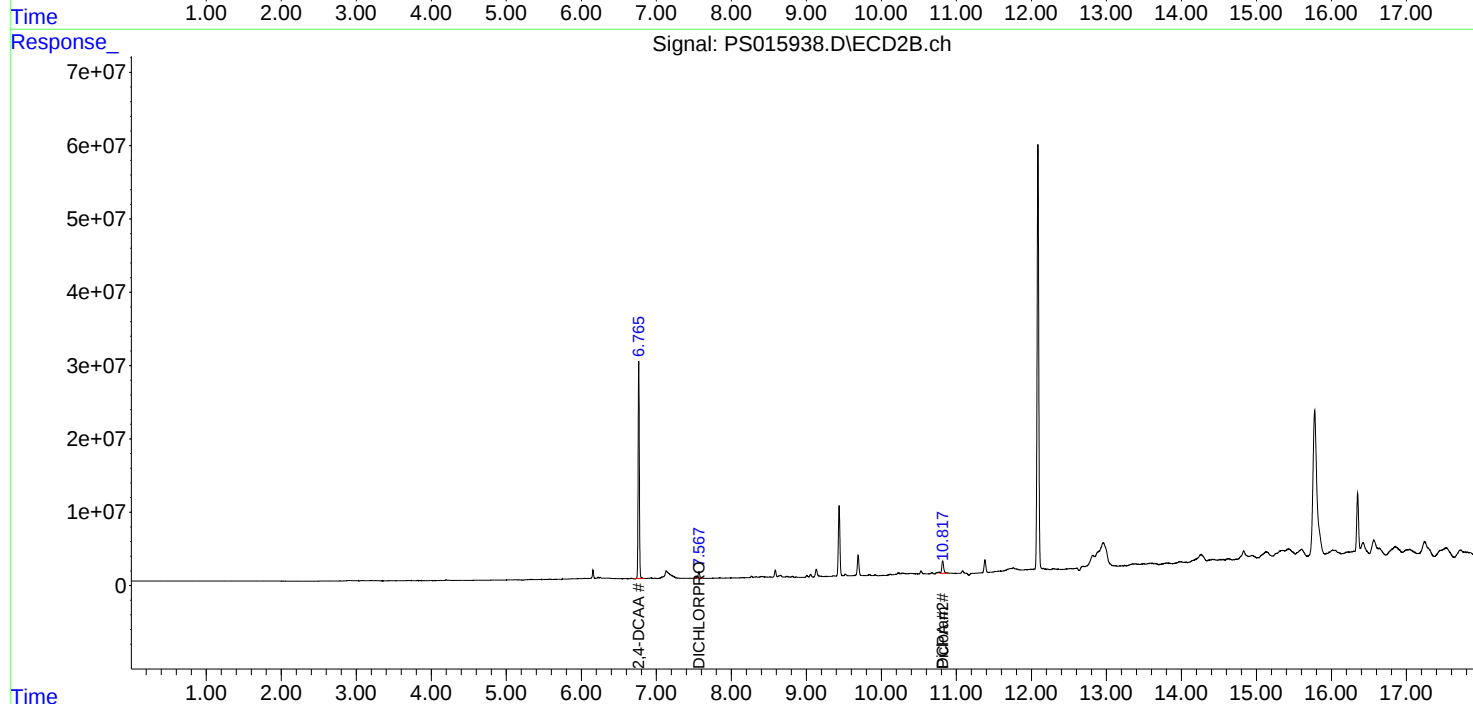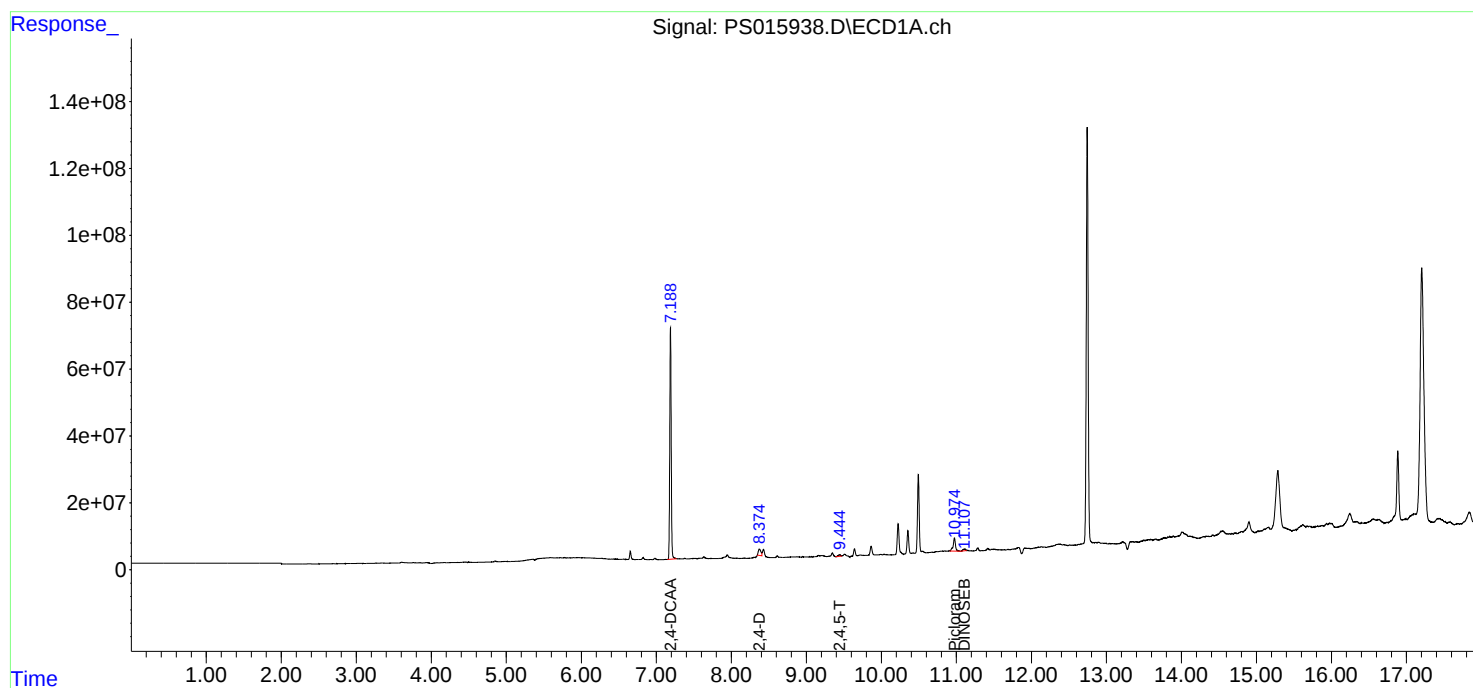


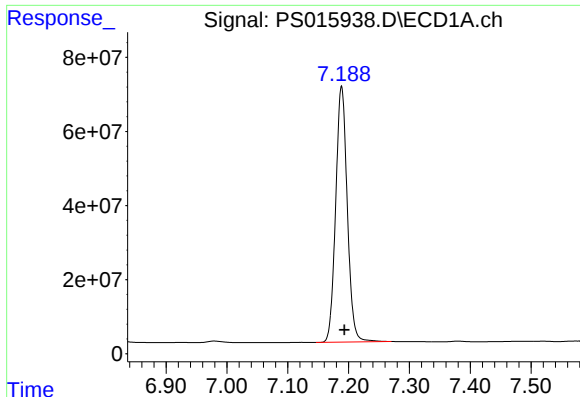

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 915181679
Conc: 550.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

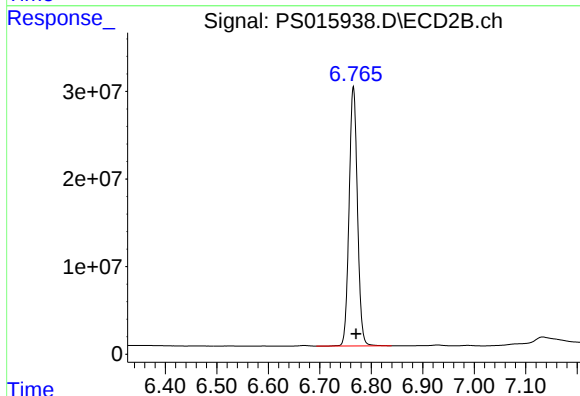


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.005 min
Response: 333165588
Conc: 661.24 ng/ml

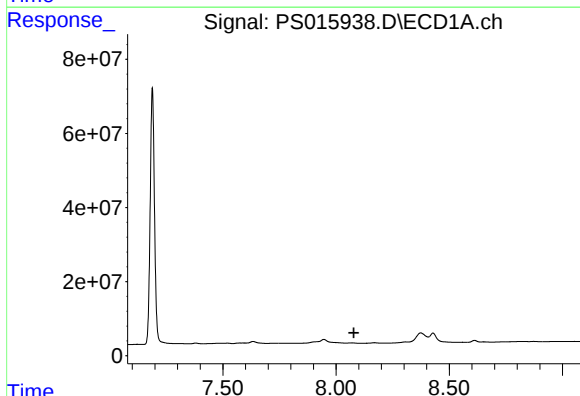


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.079 min
Response: 0
Conc: N.D.

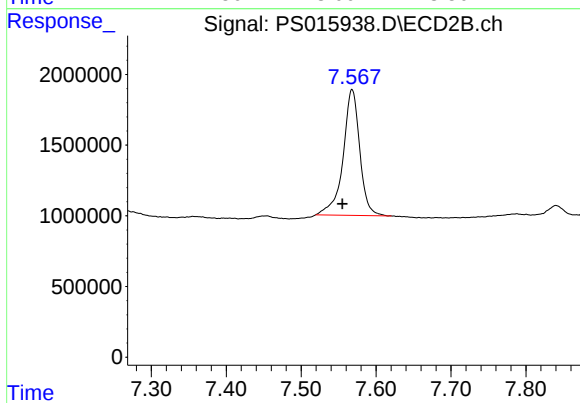

#8 DICHLORPROP


R.T.: 7.568 min
Delta R.T.: 0.013 min
Response: 13759552
Conc: 26.58 ng/ml

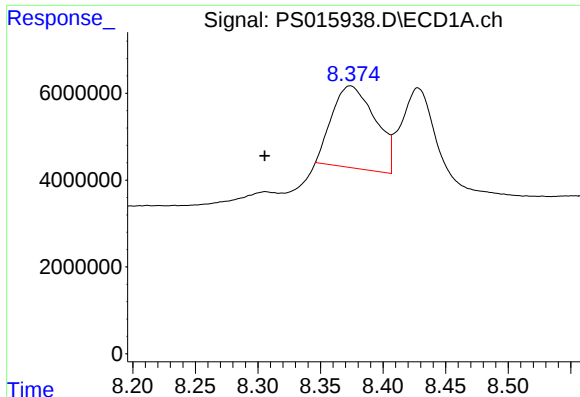

#9 2,4-D


R.T.: 8.374 min
Delta R.T.: 0.069 min
Response: 45447262
Conc: 25.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

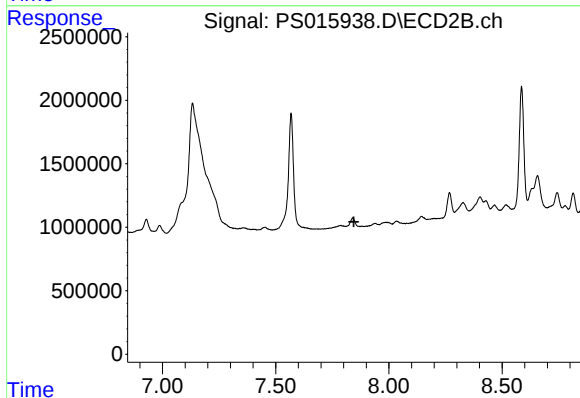


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

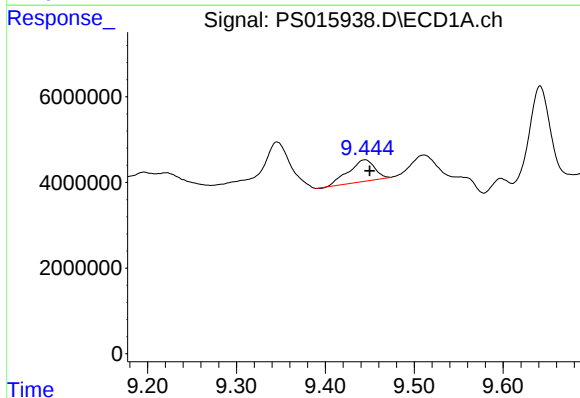


#12 2,4,5-T

R.T.: 9.445 min
Delta R.T.: -0.005 min
Response: 10337177
Conc: 1.17 ng/ml

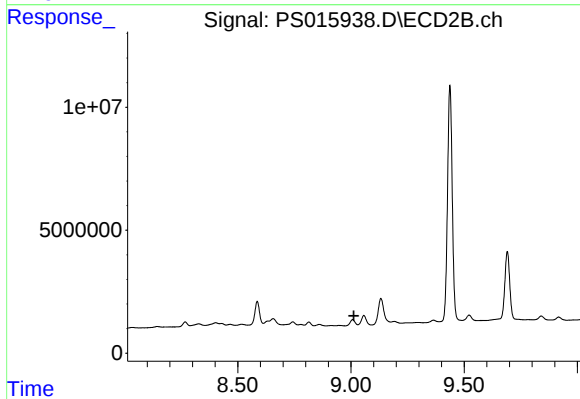

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.013 min
Response: 0
Conc: N.D.

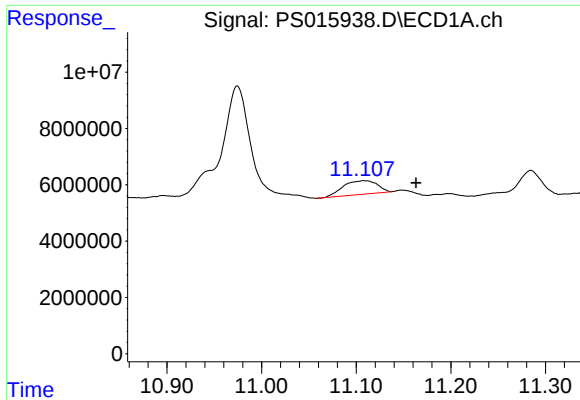

#14 DINOSEB


R.T.: 11.108 min
Delta R.T.: -0.055 min
Response: 12085338
Conc: 1.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

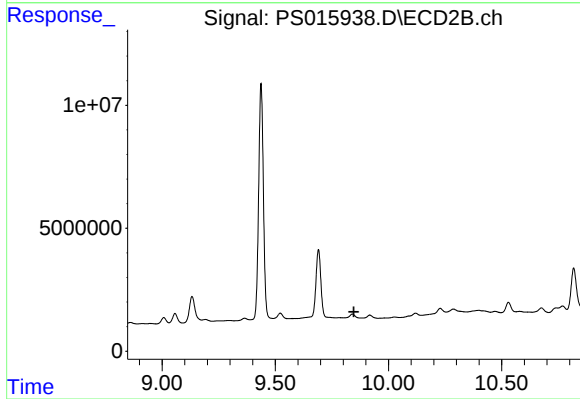


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.847 min
Response: 0
Conc: N.D.

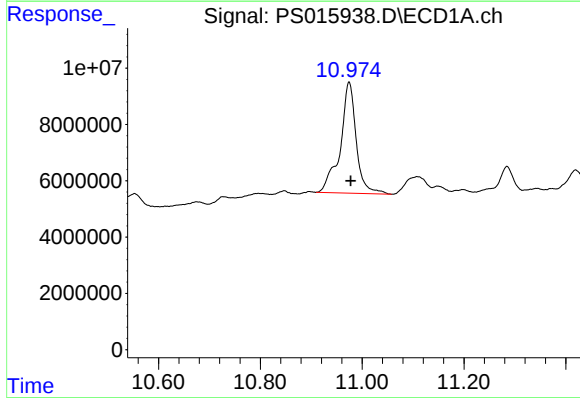


#15 Picloram

R.T.: 10.974 min
Delta R.T.: -0.004 min
Response: 85859875
Conc: 6.28 ng/ml

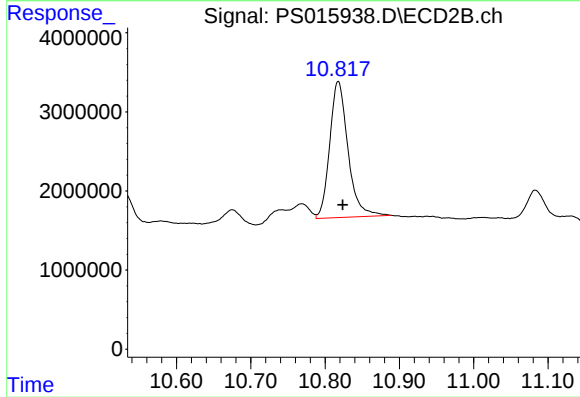

#15 Picloram


R.T.: 10.818 min
Delta R.T.: -0.006 min
Response: 29374431
Conc: 6.98 ng/ml

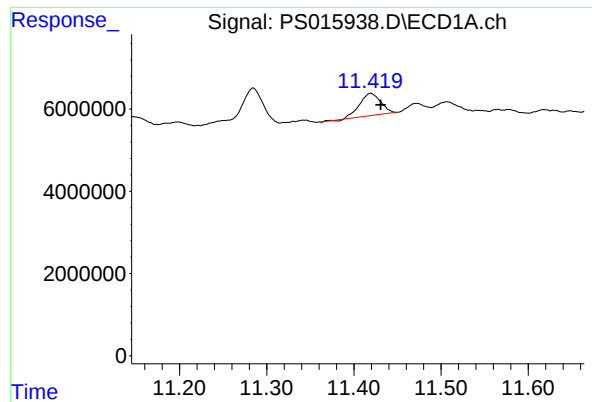

#16 DCPA

R.T.: 11.419 min
Delta R.T.: -0.011 min
Response: 9070494
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

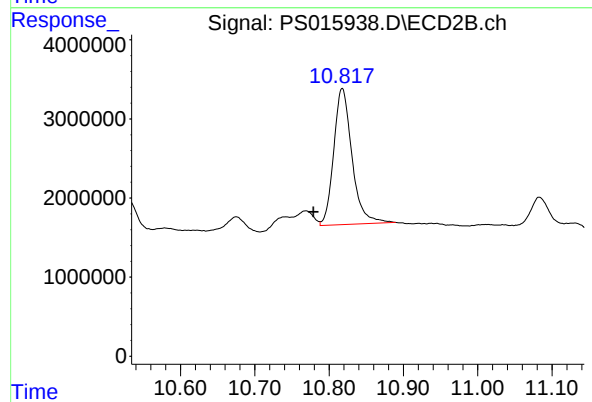

#16 DCPA

R.T.: 10.818 min
Delta R.T.: 0.039 min
Response: 29374431
Conc: 6.99 ng/ml