

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062523\
 Data File : PS023421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2023 23:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:26:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.479	6.851	984.1E6	314.0E6	556.196	553.063
Target Compounds							
1) T	Dalapon	2.575	0.000	4568039	0	2.498	N.D. #
2) T	3,5-DICHL...	5.827	0.000	327012	0	<MDL	N.D. #
3) T	4-Nitroph...	6.310	6.442	12845121	615767	9.967	1.805 #
5) T	DICAMBA	6.677f	0.000	196481	0	<MDL	N.D. #
6) T	MCP	6.813	0.000	1700906	0	<MDL	N.D. #
7) T	MCPA	6.940	0.000	488205	0	<MDL	N.D. #
8) T	DICHLORPROP	7.255	7.656	1489069	1613241	<MDL	2.608 #
9) T	2,4-D	0.000	7.871f	0	2101755	N.D.	3.031
10) T	Pentachlo...	7.668	8.356	2068690	1375485	<MDL	<MDL #
11) T	2,4,5-TP ...	8.205	0.000	3779037	0	<MDL	N.D. #
12) T	2,4,5-T	8.471	9.134	3630554	1021336	<MDL	<MDL #
13) T	2,4-DB	8.984	0.000	8335671	0	3.541	N.D. #
14) T	DINOSEB	10.043	0.000	789574	0	<MDL	N.D. #
15) T	Picloram	9.879	10.891	17612383	4391546	1.015	<MDL #
16) T	DCPA	10.323	10.891	1868888	4391546	<MDL	1.095 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062523\
Data File : PS023421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2023 23:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:26:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

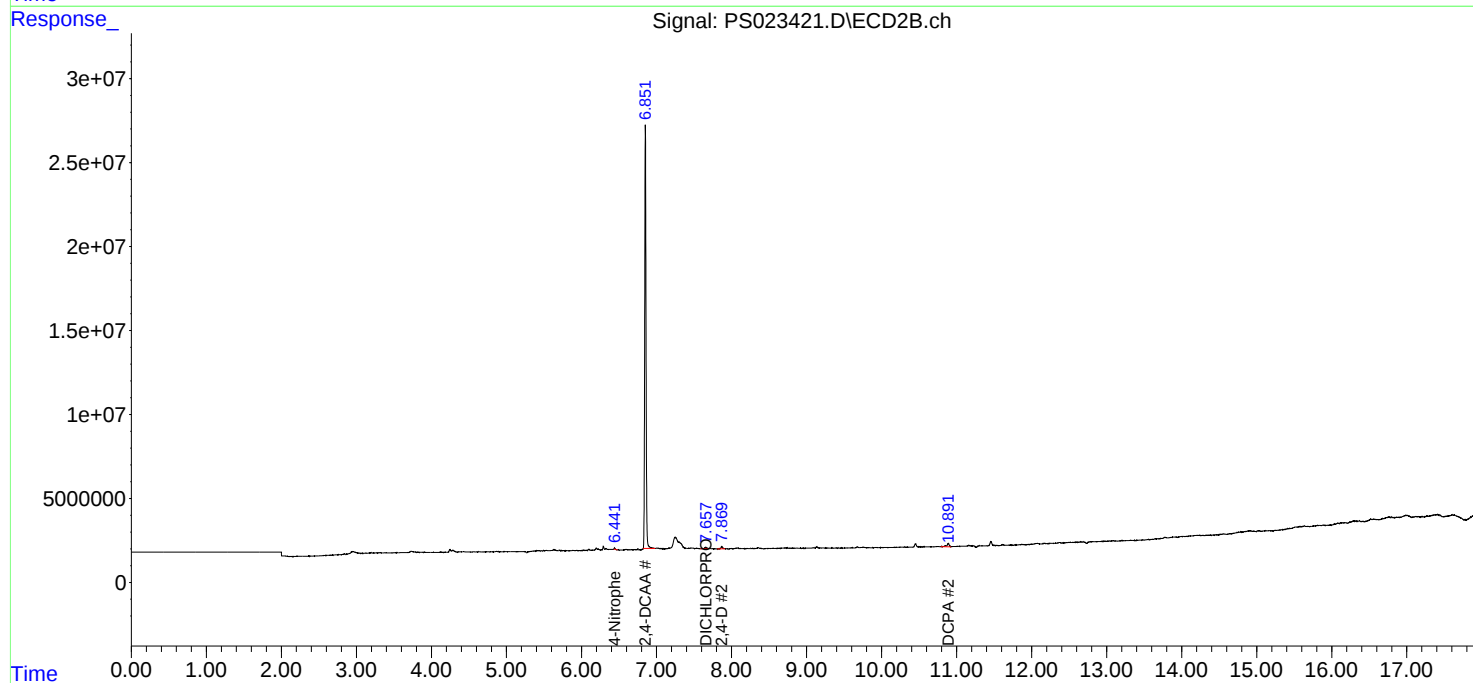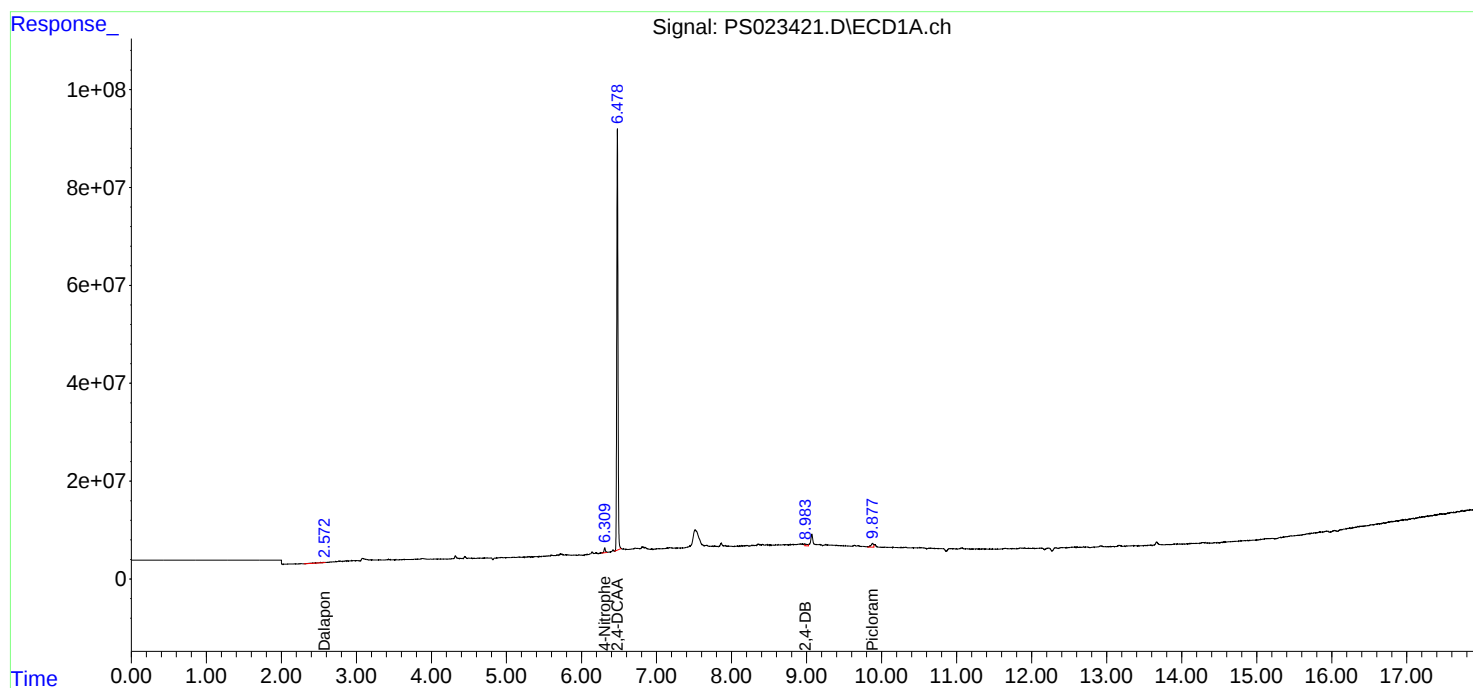


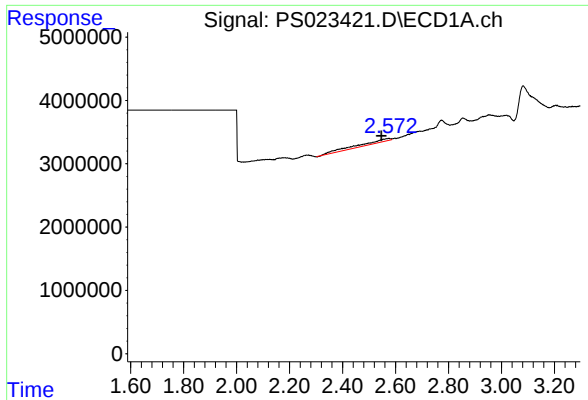

#1 Dalapon


R.T.: 2.575 min
Delta R.T.: 0.028 min
Response: 4568039
Conc: 2.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

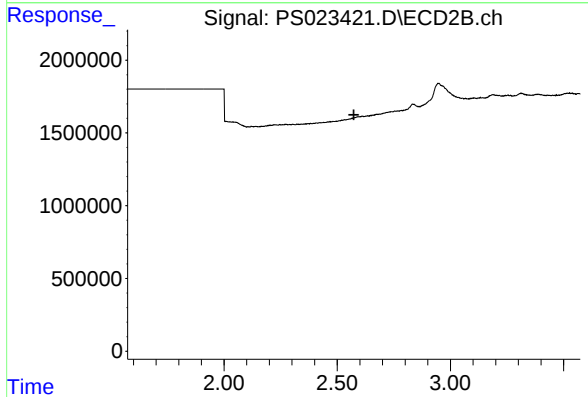


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

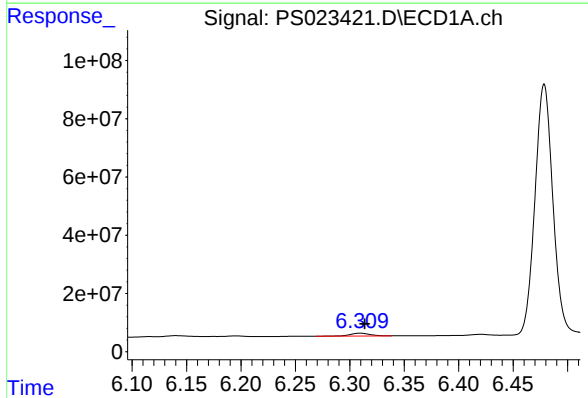


#3 4-Nitrophenol

R.T.: 6.310 min
Delta R.T.: -0.004 min
Response: 12845121
Conc: 9.97 ng/ml

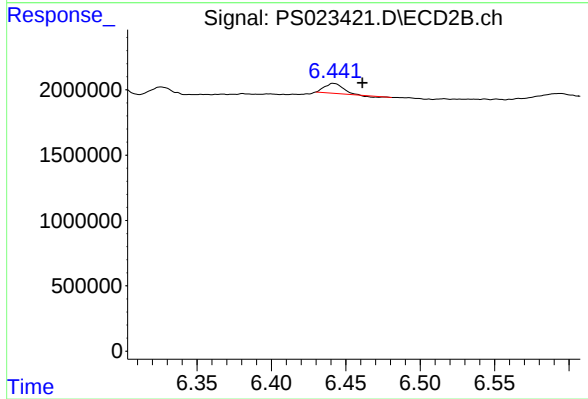

#3 4-Nitrophenol


R.T.: 6.442 min
Delta R.T.: -0.019 min
Response: 615767
Conc: 1.80 ng/ml

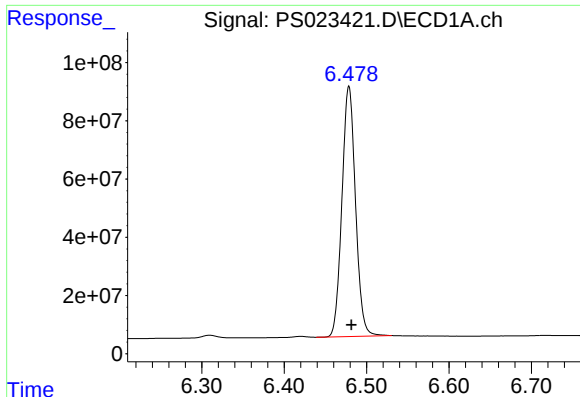

#4 2,4-DCAA


R.T.: 6.479 min
Delta R.T.: -0.003 min
Response: 984052843
Conc: 556.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

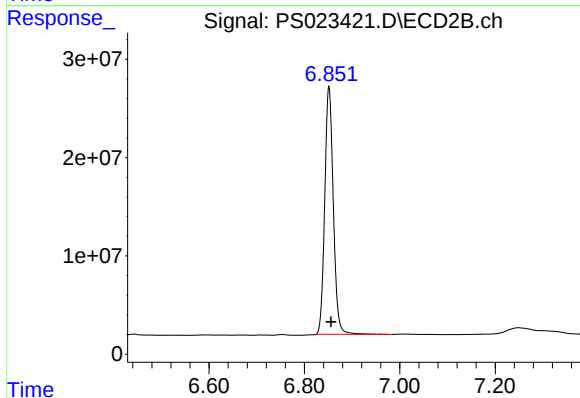


#4 2,4-DCAA

R.T.: 6.851 min
Delta R.T.: -0.005 min
Response: 313971208
Conc: 553.06 ng/ml

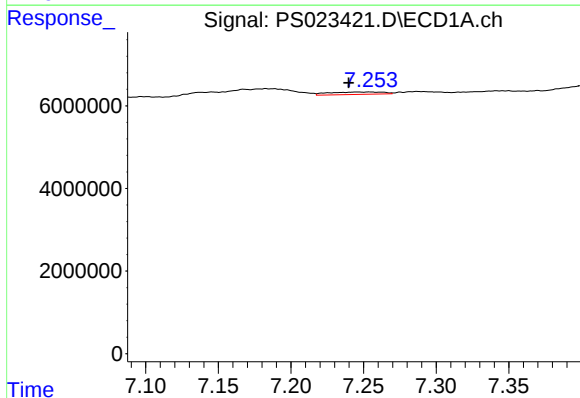


#8 DICHLORPROP

R.T.: 7.255 min
Delta R.T.: 0.015 min
Response: 1489069
Conc: N.D.

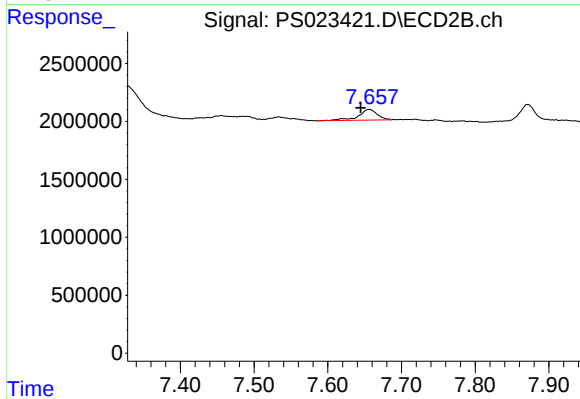

#8 DICHLORPROP


R.T.: 7.656 min
Delta R.T.: 0.012 min
Response: 1613241
Conc: 2.61 ng/ml

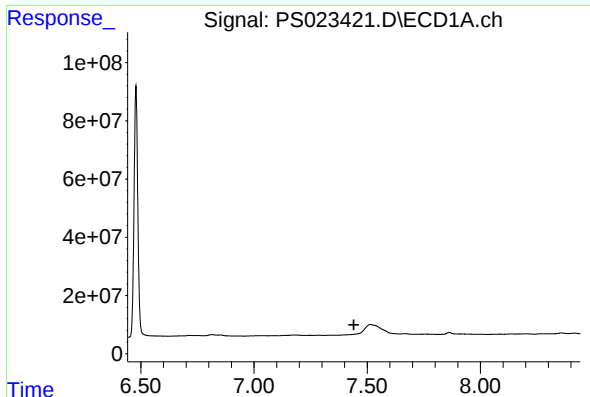

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

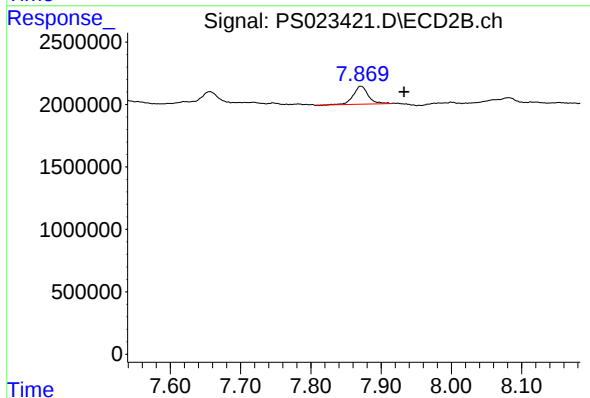


#9 2,4-D

R.T.: 7.871 min
Delta R.T.: -0.061 min
Response: 2101755
Conc: 3.03 ng/ml

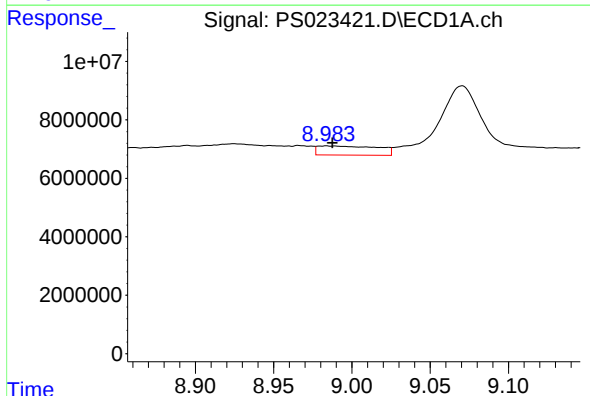


#13 2,4-DB

R.T.: 8.984 min
Delta R.T.: -0.004 min
Response: 8335671
Conc: 3.54 ng/ml

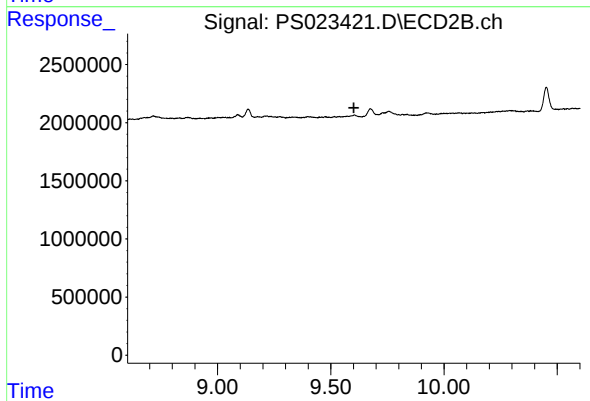

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.

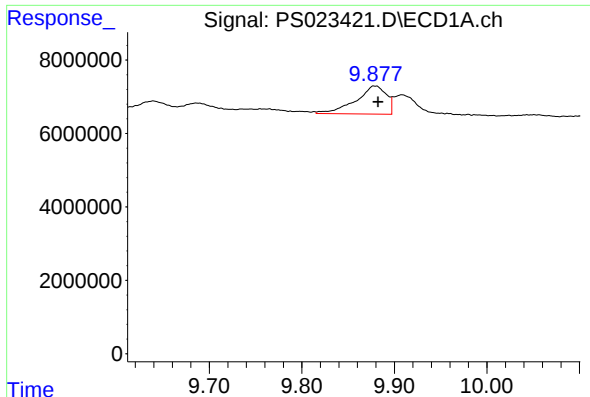

#15 Picloram


R.T.: 9.879 min
Delta R.T.: -0.004 min
Response: 17612383
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

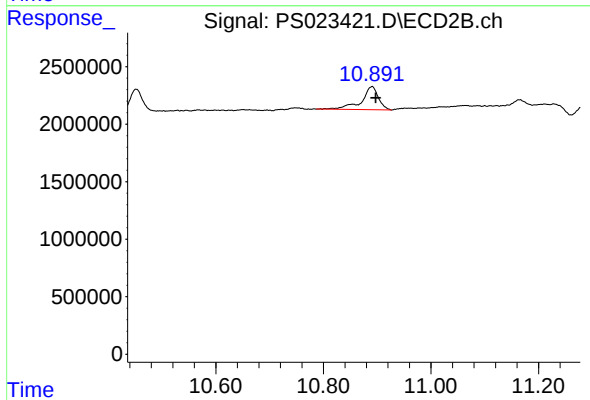


#15 Picloram

R.T.: 10.891 min
Delta R.T.: -0.007 min
Response: 4391546
Conc: N.D.

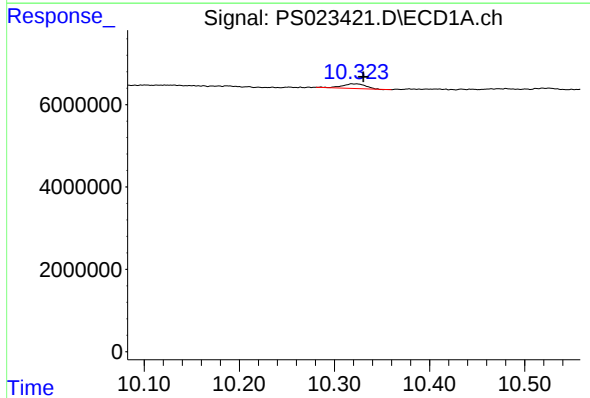

#16 DCPA

R.T.: 10.323 min
Delta R.T.: -0.007 min
Response: 1868888
Conc: N.D.

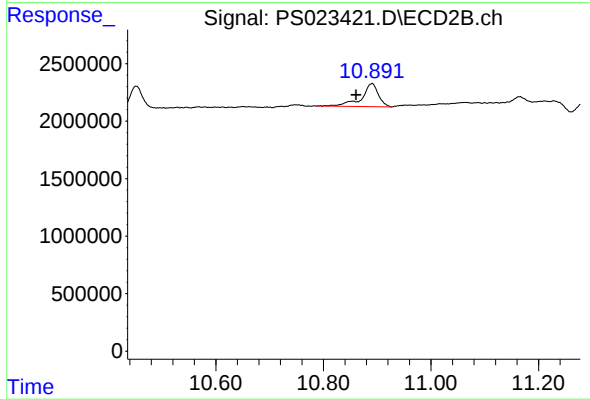

#16 DCPA

R.T.: 10.891 min
Delta R.T.: 0.030 min
Response: 4391546
Conc: 1.09 ng/ml