

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062523\
 Data File : PS023433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 05:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 07:18:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.478	6.850	1005.6E6	315.8E6	568.366	556.227
Target Compounds							
1) T	Dalapon	2.566	0.000	2817089	0	1.541	N.D. #
3) T	4-Nitroph...	6.311	0.000	10723320	0	8.320	N.D. #
5) T	DICAMBA	6.680f	0.000	1882346	0	<MDL	N.D. #
6) T	MCP	6.813	0.000	2597999	0	<MDL	N.D. #
7) T	MCPA	6.933	0.000	226118	0	<MDL	N.D. #
8) T	DICHLORPROP	7.242	7.655	1515081	1964444	<MDL	3.176 #
9) T	2,4-D	0.000	7.872f	0	1009101	N.D.	1.455
10) T	Pentachlo...	7.670	0.000	2170687	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.204	0.000	3468393	0	<MDL	N.D. #
12) T	2,4,5-T	8.470	9.135	3143660	1394450	<MDL	<MDL #
13) T	2,4-DB	8.966	0.000	2897994	0	1.231	N.D. #
14) T	DINOSEB	10.056	0.000	642608	0	<MDL	N.D. #
15) T	Picloram	9.882	10.888	17638753	4138617	1.016	<MDL #
16) T	DCPA	10.325	10.888	2264575	4138617	<MDL	1.032 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062523\
Data File : PS023433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 05:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 07:18:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

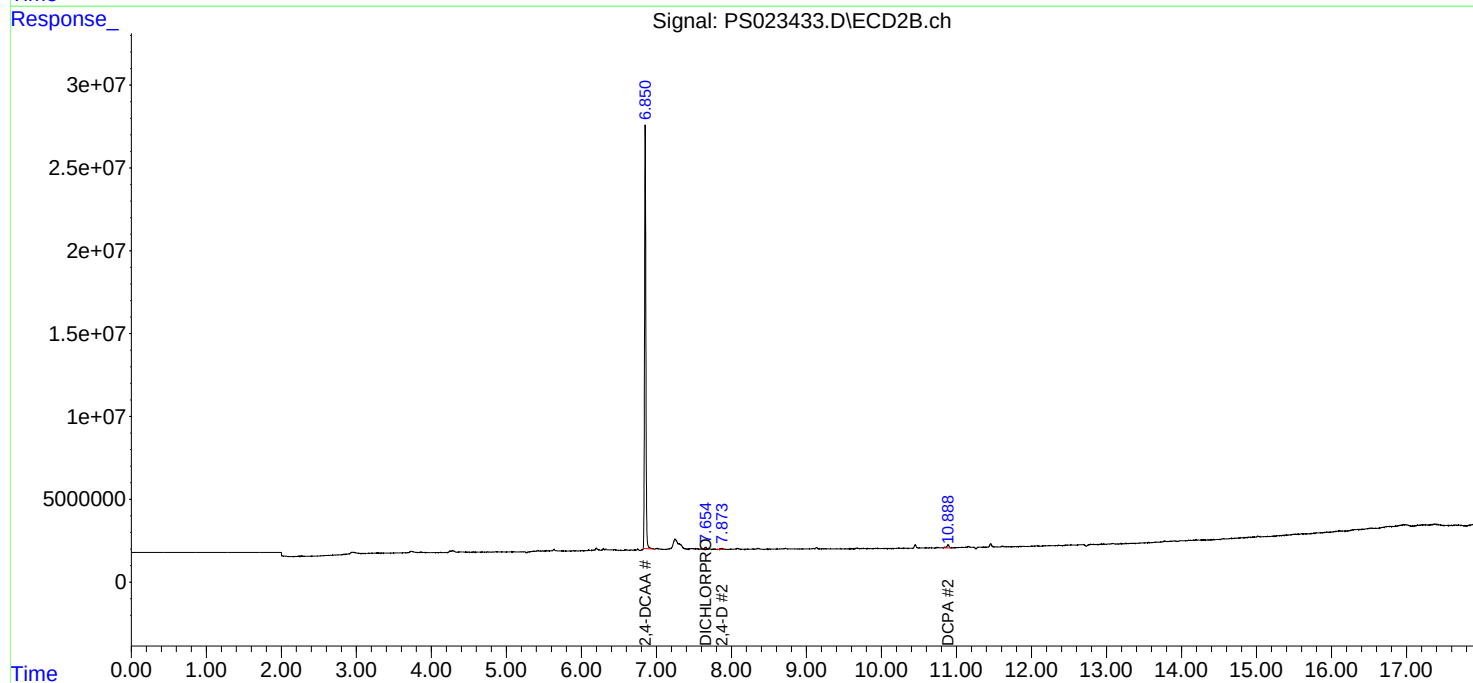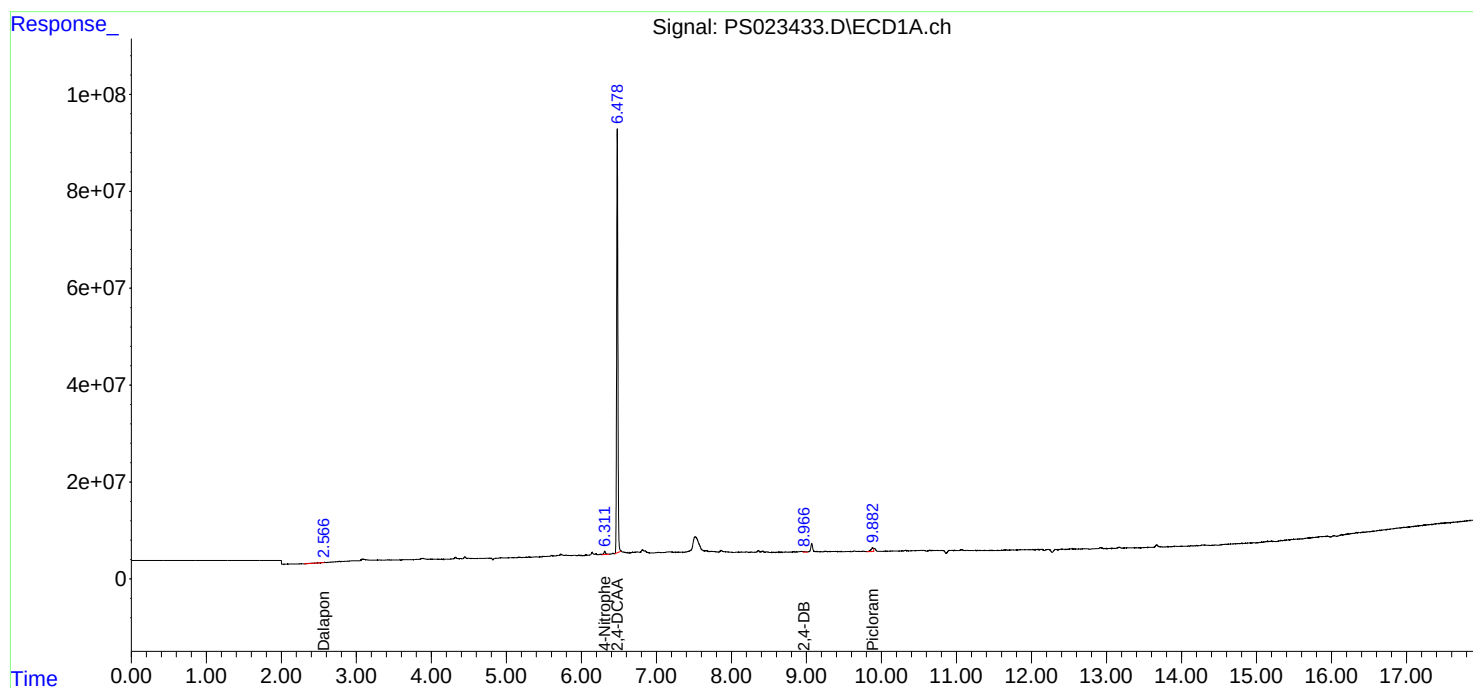


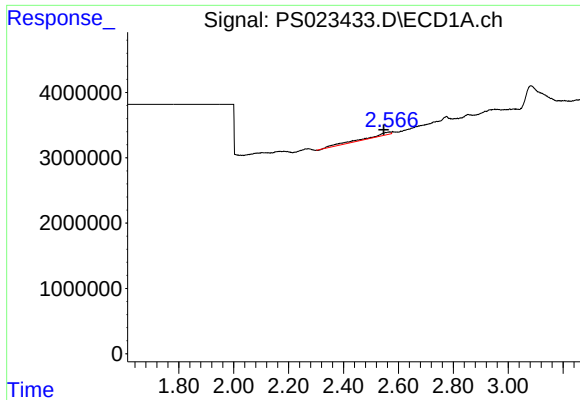

#1 Dalapon


R.T.: 2.566 min
Delta R.T.: 0.019 min
Response: 2817089
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

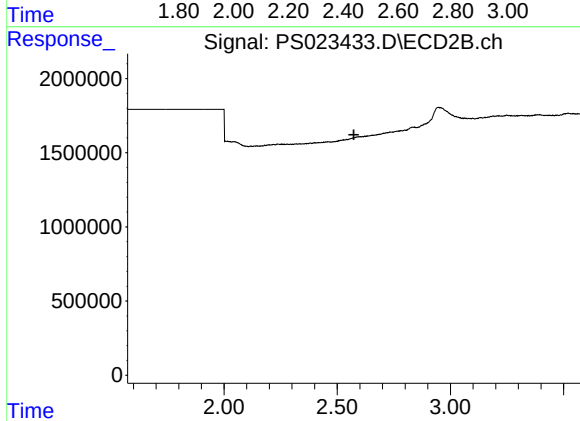


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

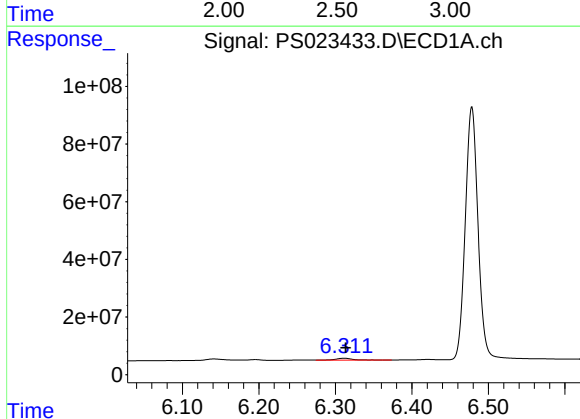


#3 4-Nitrophenol

R.T.: 6.311 min
Delta R.T.: -0.002 min
Response: 10723320
Conc: 8.32 ng/ml

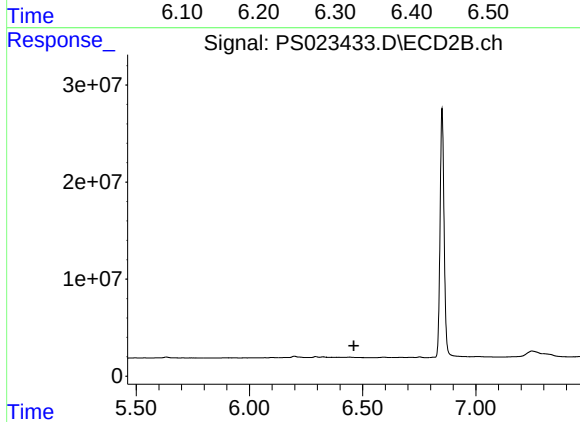

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

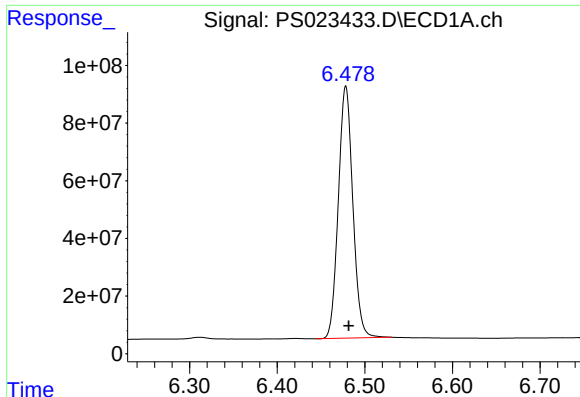

#4 2,4-DCAA


R.T.: 6.478 min
Delta R.T.: -0.003 min
Response: 1005584161
Conc: 568.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

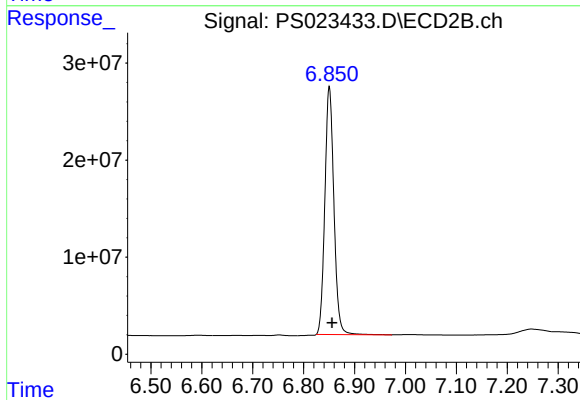


#4 2,4-DCAA

R.T.: 6.850 min
Delta R.T.: -0.006 min
Response: 315767742
Conc: 556.23 ng/ml

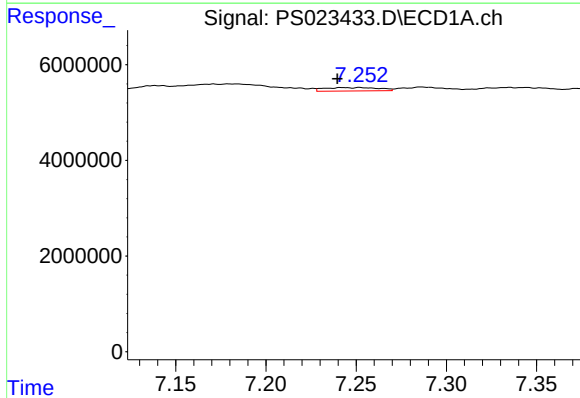


#8 DICHLORPROP

R.T.: 7.242 min
Delta R.T.: 0.003 min
Response: 1515081
Conc: N.D.

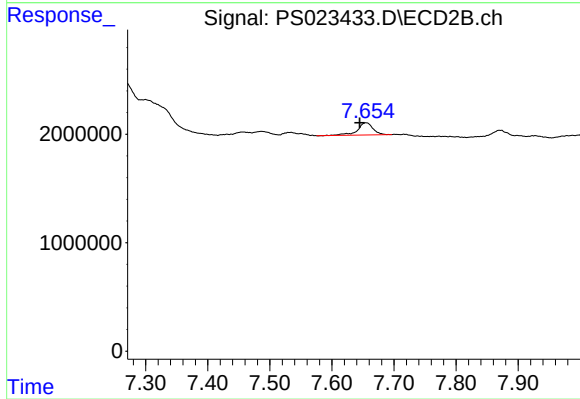

#8 DICHLORPROP


R.T.: 7.655 min
Delta R.T.: 0.011 min
Response: 1964444
Conc: 3.18 ng/ml

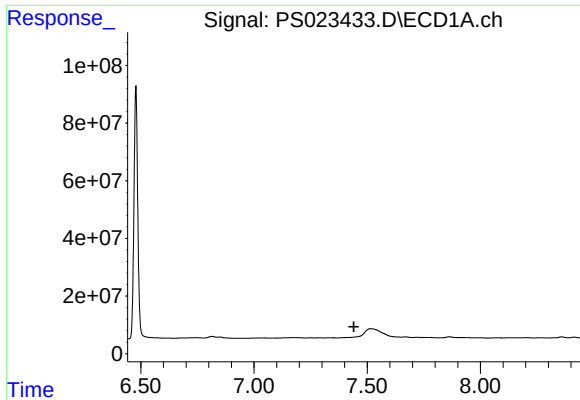

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

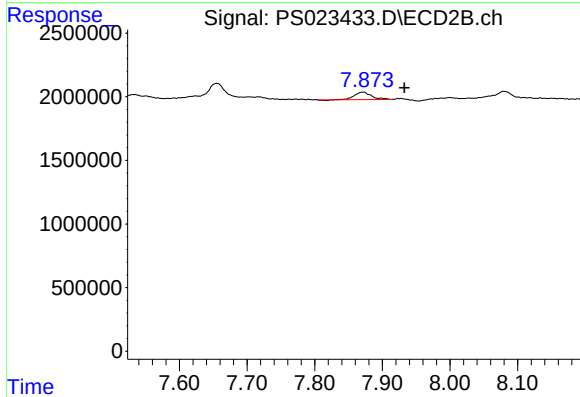


#9 2,4-D

R.T.: 7.872 min
Delta R.T.: -0.060 min
Response: 1009101
Conc: 1.46 ng/ml

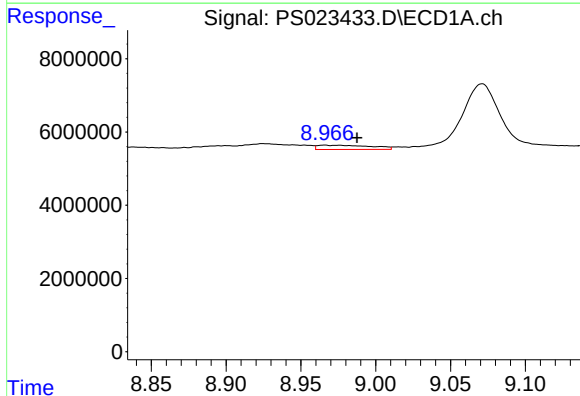


#13 2,4-DB

R.T.: 8.966 min
Delta R.T.: -0.022 min
Response: 2897994
Conc: 1.23 ng/ml

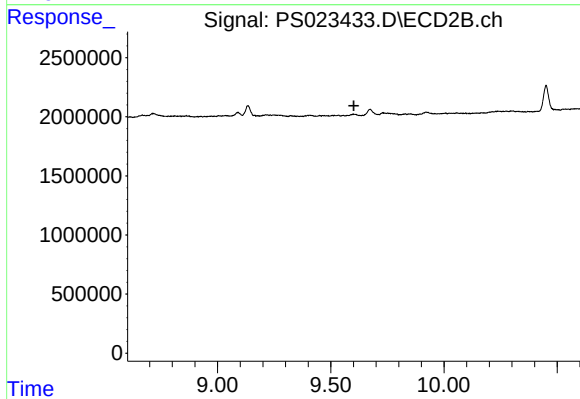

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.

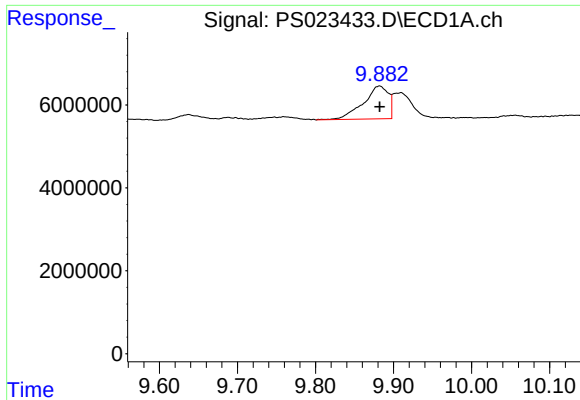

#15 Picloram


R.T.: 9.882 min
Delta R.T.: 0.000 min
Response: 17638753
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

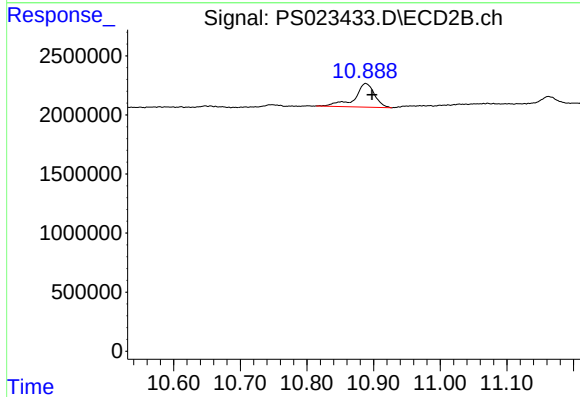


#15 Picloram

R.T.: 10.888 min
Delta R.T.: -0.009 min
Response: 4138617
Conc: N.D.

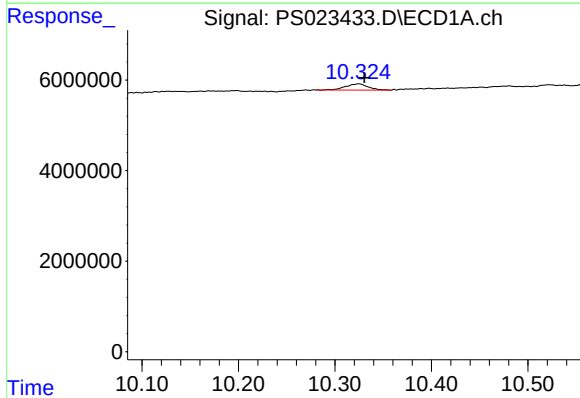

#16 DCPA

R.T.: 10.325 min
Delta R.T.: -0.006 min
Response: 2264575
Conc: N.D.

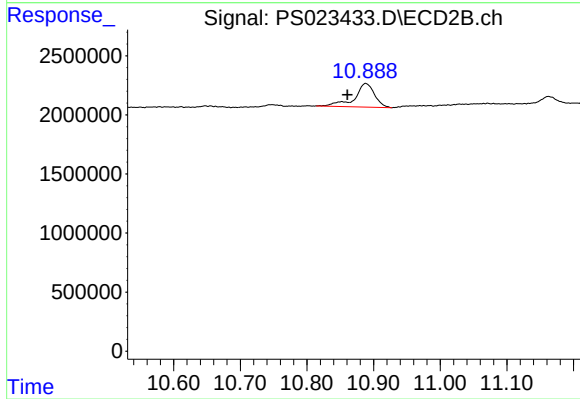

#16 DCPA

R.T.: 10.888 min
Delta R.T.: 0.028 min
Response: 4138617
Conc: 1.03 ng/ml