

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062524\
 Data File : PS027096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2024 12:05
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:31:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061724.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 18 02:58:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.230	7.781	888233	1473673	<MDL	<MDL	#
Target Compounds								
1) T	Dalapon	0.000	2.677	0	3210842	N.D.	<MDL	
2) T	3,5-DICHL...	6.370f	0.000	15107452	0	3.752	N.D.	#
3) T	4-Nitroph...	7.037	0.000	78399	0	<MDL	N.D.	#
5) T	DICAMBA	0.000	7.942	0	2598586	N.D.	<MDL	
6) T	MCP	7.543f	8.061	1679104	6504091	<MDL	<MDL	#
7) T	MCPA	7.727	0.000	654227	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.137	0.000	795303	0	<MDL	N.D.	#
9) T	2,4-D	8.345	0.000	56535127	0	19.024	N.D.	#
11) T	2,4,5-TP ...	0.000	9.926	0	1503763	N.D.	<MDL	
12) T	2,4,5-T	9.496	10.332	1000120	2074752	<MDL	<MDL	#
13) T	2,4-DB	10.098f	10.902	390139	-3810	<MDL	N.D.	#
14) T	DINOSEB	11.244f	0.000	597943	0	<MDL	N.D.	#
15) T	Picloram	11.083	12.367	10809870	14659391	<MDL	<MDL	#
16) T	DCPA	11.589	12.265f	80743	4110784	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062524\
Data File : PS027096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2024 12:05
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:31:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061724.M
Quant Title : 8080.M
QLast Update : Tue Jun 18 02:58:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

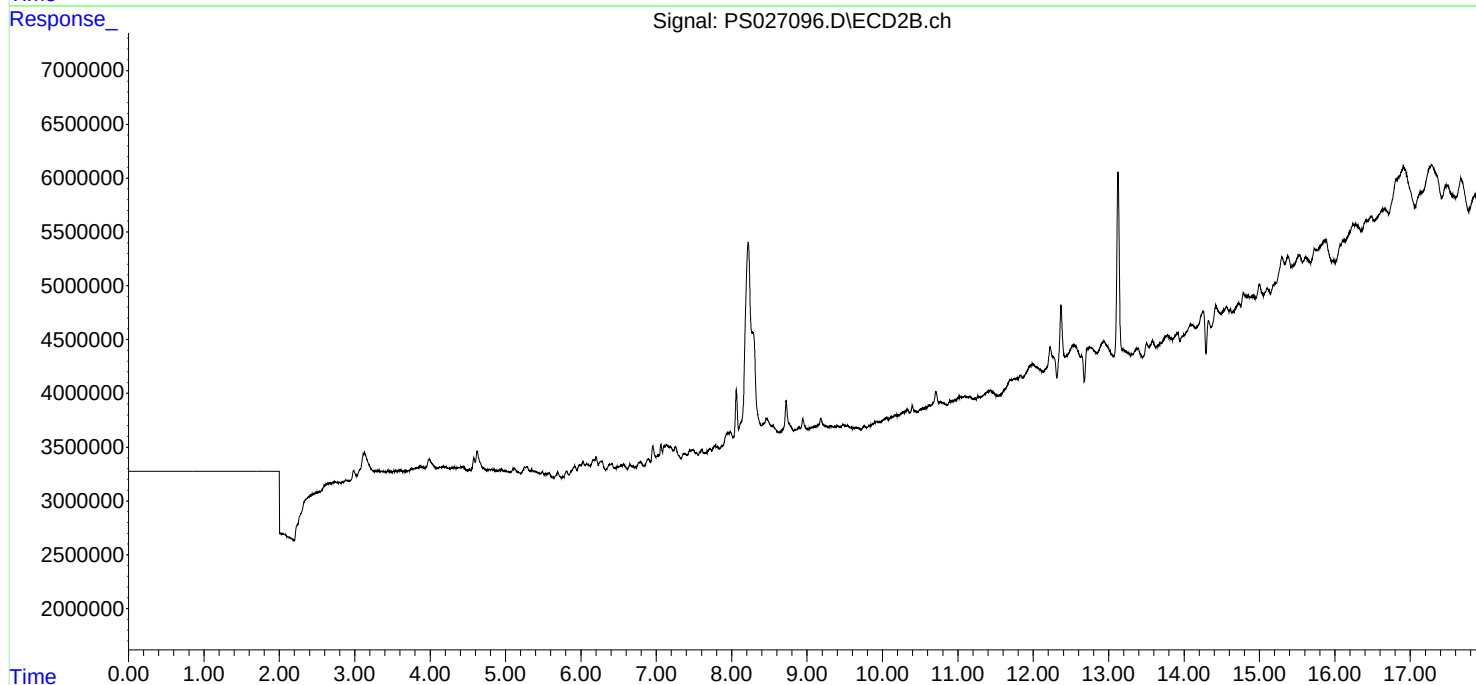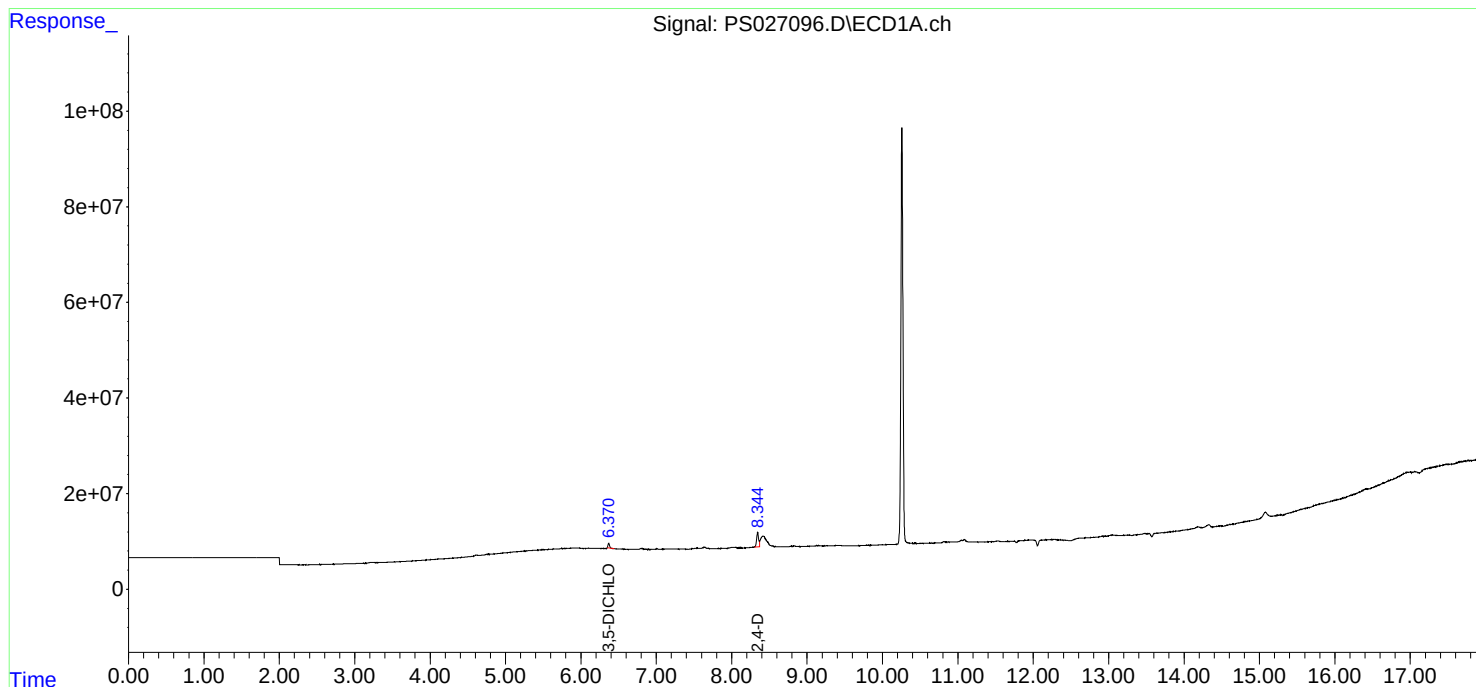


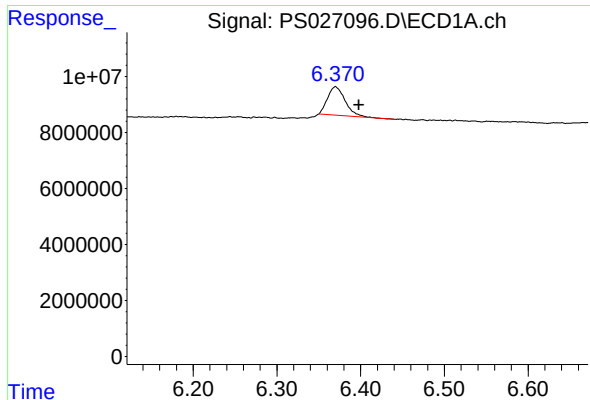

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.370 min
Delta R.T.: -0.028 min
Response: 15107452
Conc: 3.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

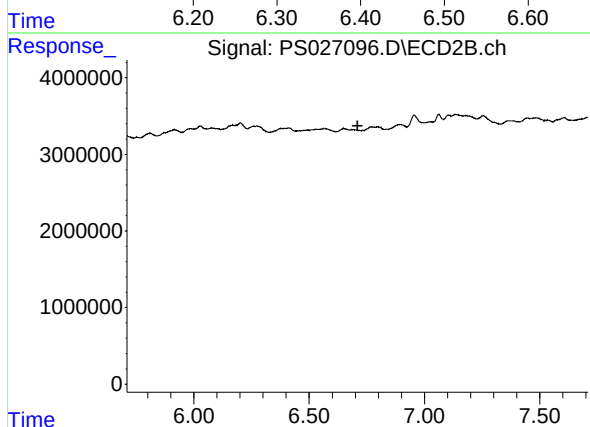


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

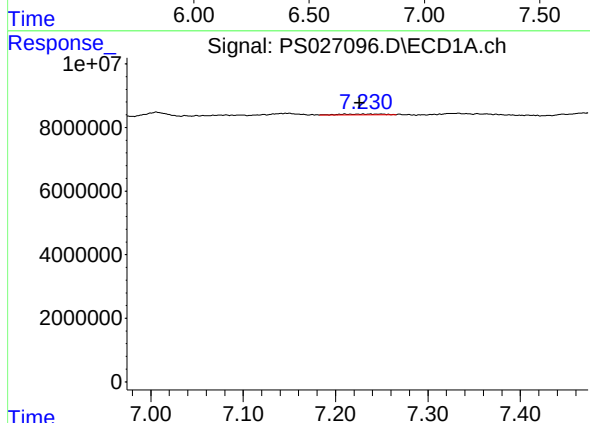


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.004 min
Response: 888233
Conc: N.D.

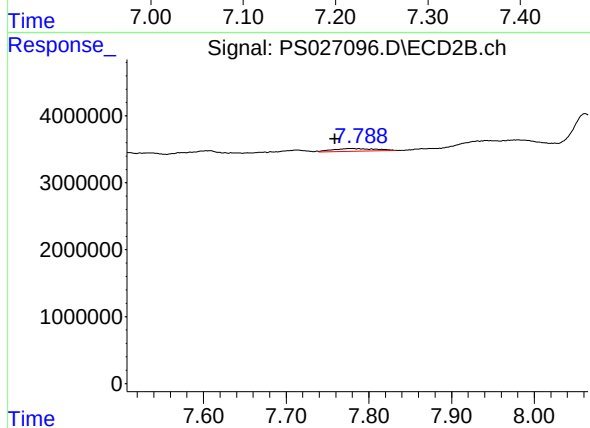

#4 2,4-DCAA


R.T.: 7.781 min
Delta R.T.: 0.021 min
Response: 1473673
Conc: N.D.

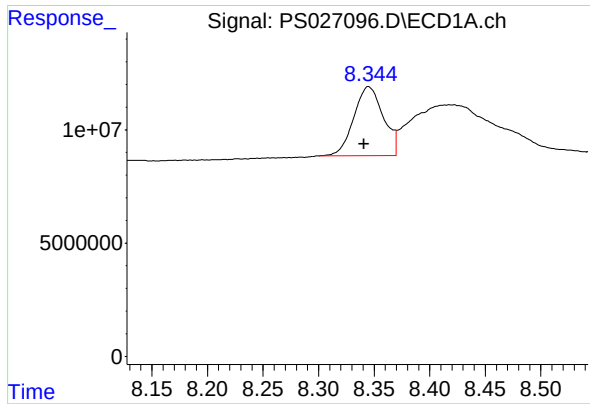

#9 2,4-D

R.T.: 8.345 min
Delta R.T.: 0.004 min
Response: 56535127
Conc: 19.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

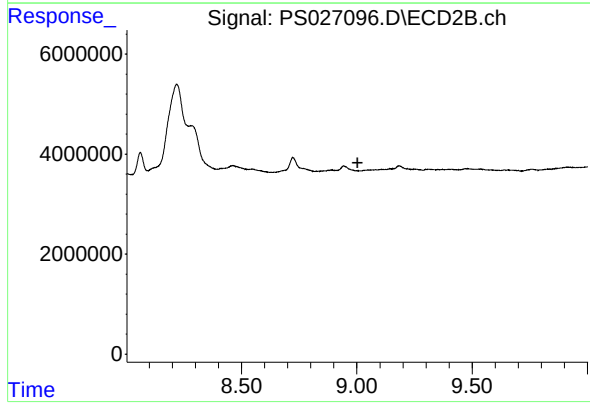

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 9.003 min
Response: 0
Conc: N.D.