

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062618\
 Data File : PS000642.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 09:52
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 15:57:50 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.817	11.181	185.3E6	156.0E6	491.945	458.435
Target Compounds							
1) T	Dalapon	0.000	2.559	0	31654	N.D.	0.073 #
3) T	4-Nitroph...	11.442	0.000	611367	0	2.601	N.D. #
6) T	MCP	12.520	0.000	60596	0	0.054	N.D. #
10) T	Pentachlo...	14.084	13.630	850063	615829	0.162	0.130
11) T	2,4,5-TP ...	14.952	14.239	626038	484343	0.288	0.249
12) T	2,4,5-T	15.361	14.817	580777	1063002	0.270	0.629 #
14) T	DINOSEB	17.613	15.887	479366	356587	0.322	0.273
15) T	Picloram	17.388	17.140	2589656	2070915	0.887	0.830
16) T	DCPA	17.951	17.078	831652	712966	0.325	0.309



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062618\
Data File : PS000642.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 09:52
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 15:57:50 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

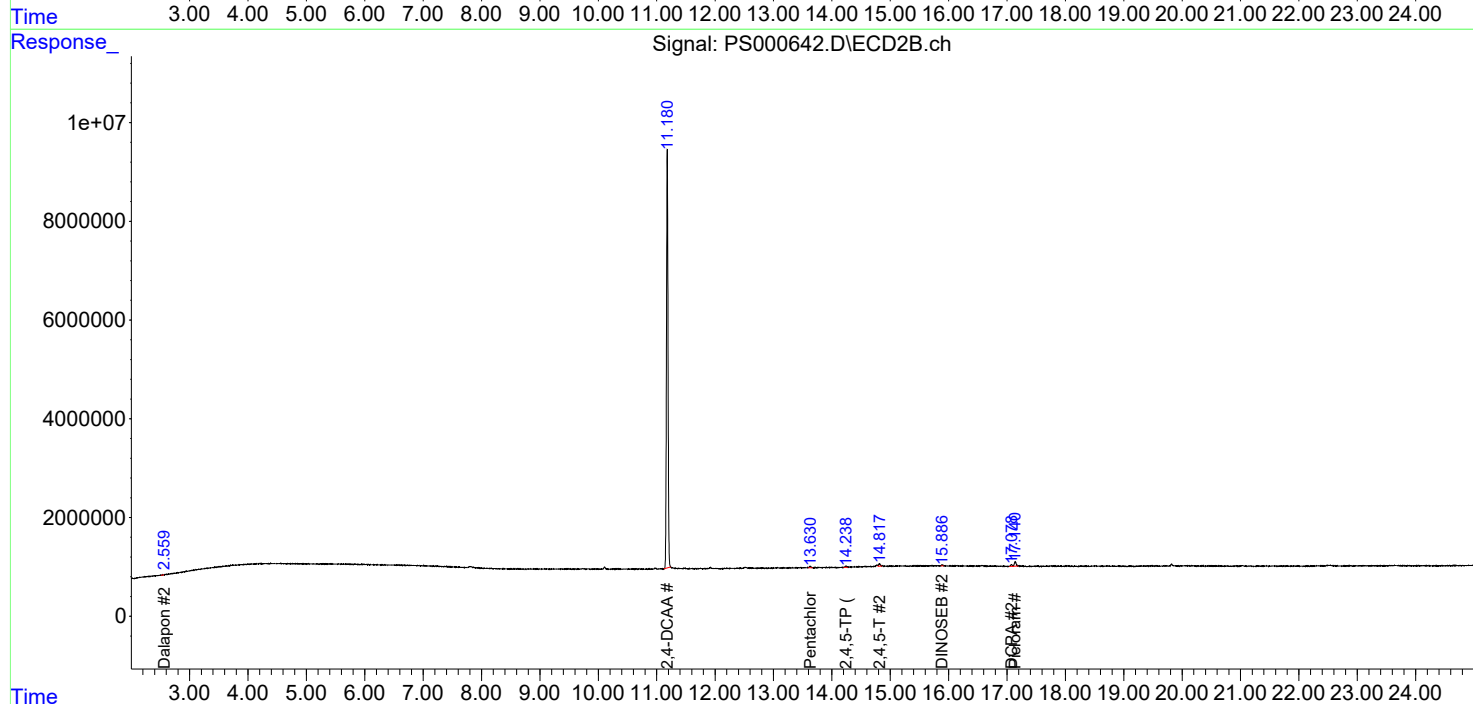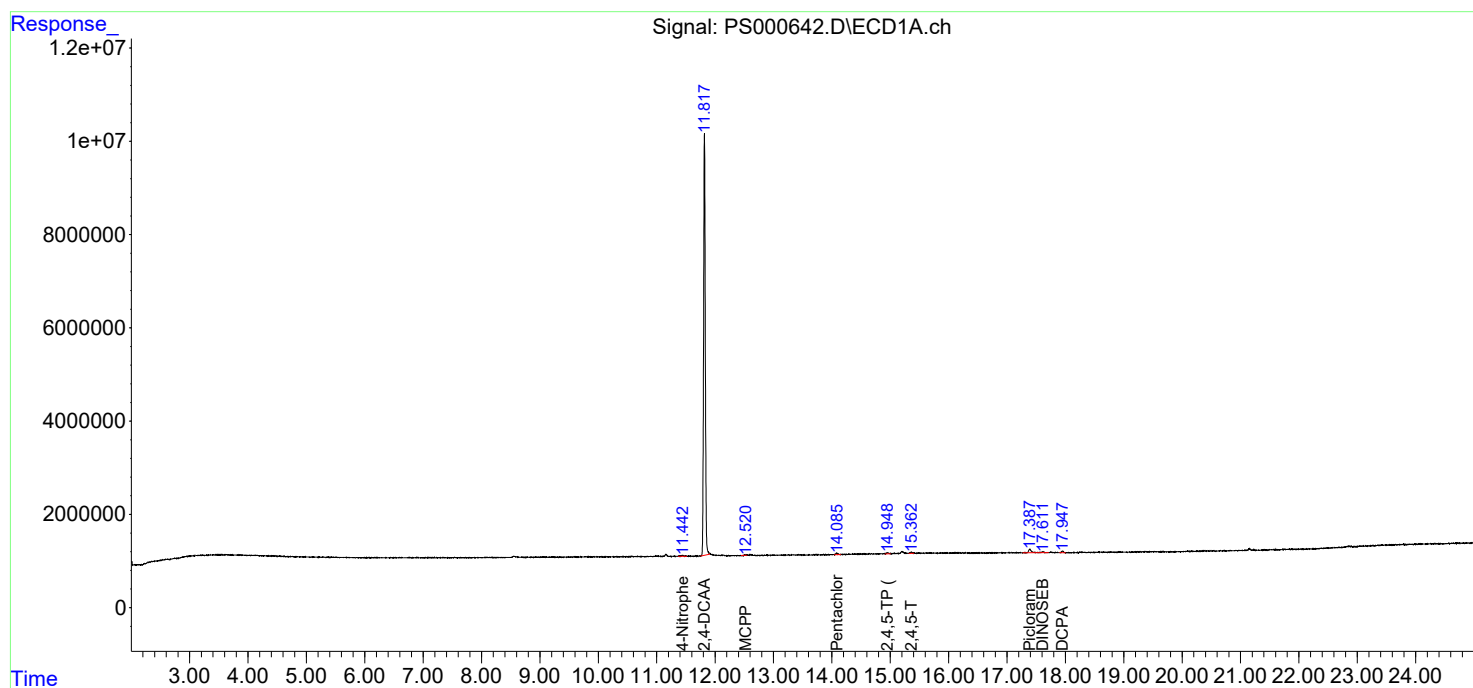


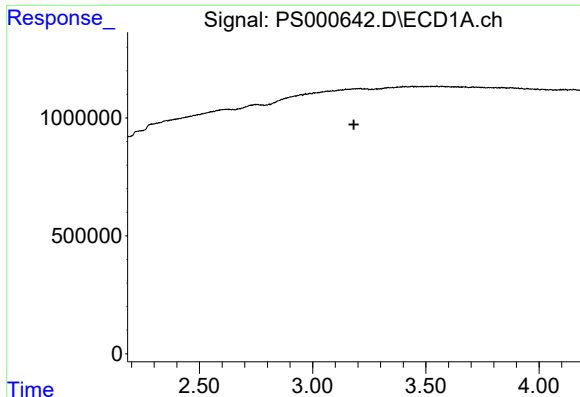

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

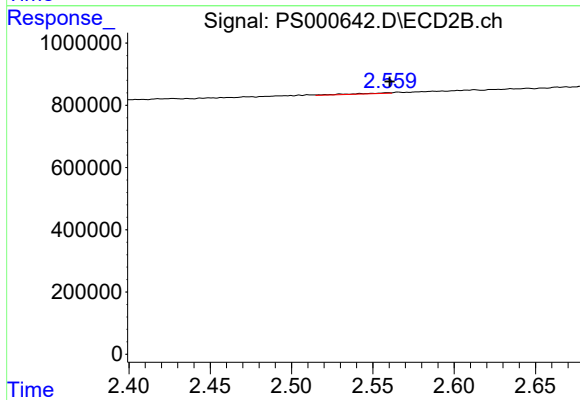


#1 Dalapon

R.T.: 2.559 min
Delta R.T.: -0.001 min
Response: 31654
Conc: 0.07 ng/ml

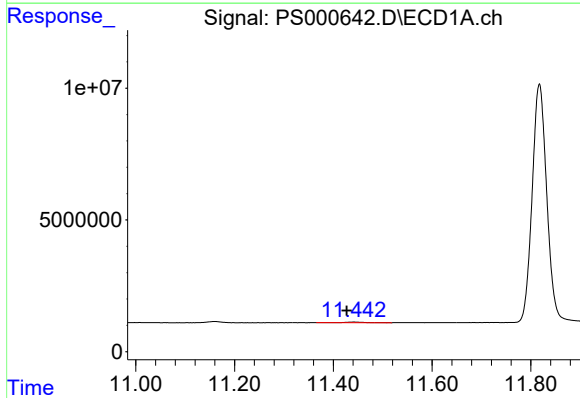


#3 4-Nitrophenol

R.T.: 11.442 min
Delta R.T.: 0.014 min
Response: 611367
Conc: 2.60 ng/ml

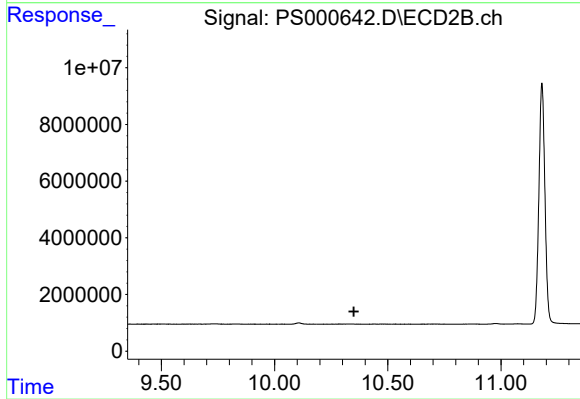

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.350 min
Response: 0
Conc: N.D.

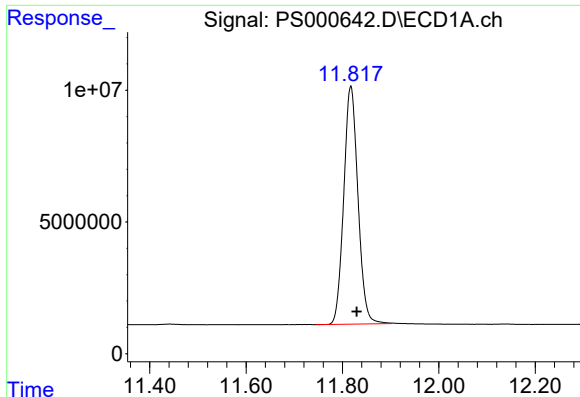

#4 2,4-DCAA


R.T.: 11.817 min
Delta R.T.: -0.012 min
Response: 185293267
Conc: 491.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

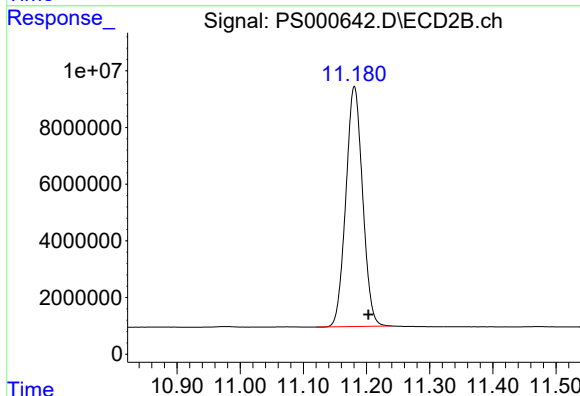


#4 2,4-DCAA

R.T.: 11.181 min
Delta R.T.: -0.022 min
Response: 156009503
Conc: 458.43 ng/ml

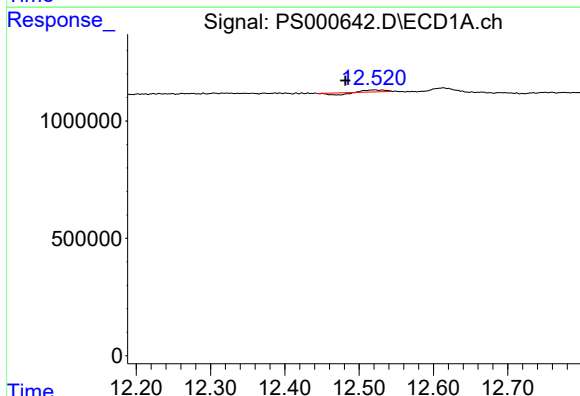


#6 MCP

R.T.: 12.520 min
Delta R.T.: 0.038 min
Response: 60596
Conc: 0.05 ug/ml

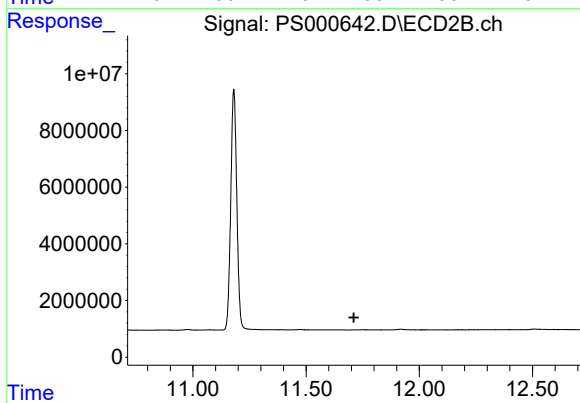

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.711 min
Response: 0
Conc: N.D.

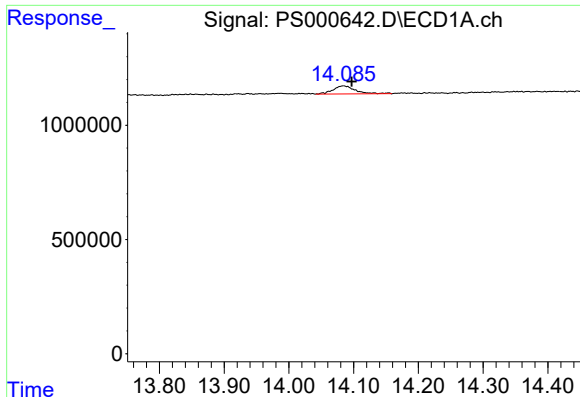

#10 Pentachlorophenol


R.T.: 14.084 min
Delta R.T.: -0.013 min
Response: 850063
Conc: 0.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

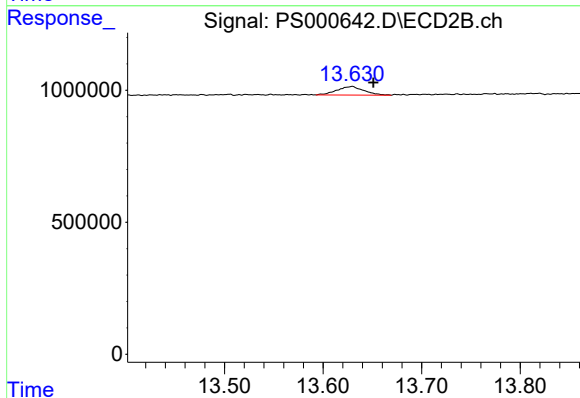


#10 Pentachlorophenol

R.T.: 13.630 min
Delta R.T.: -0.021 min
Response: 615829
Conc: 0.13 ng/ml

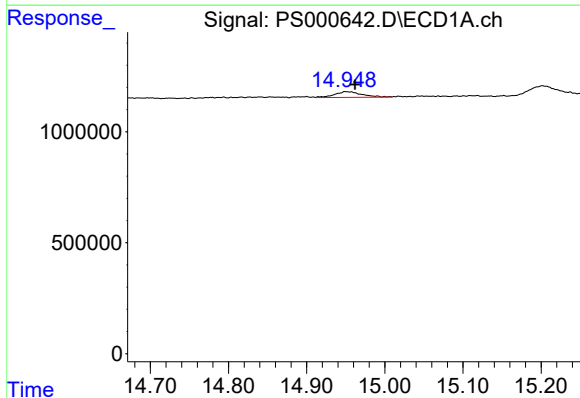


#11 2,4,5-TP (SILVEX)

R.T.: 14.952 min
Delta R.T.: -0.010 min
Response: 626038
Conc: 0.29 ng/ml

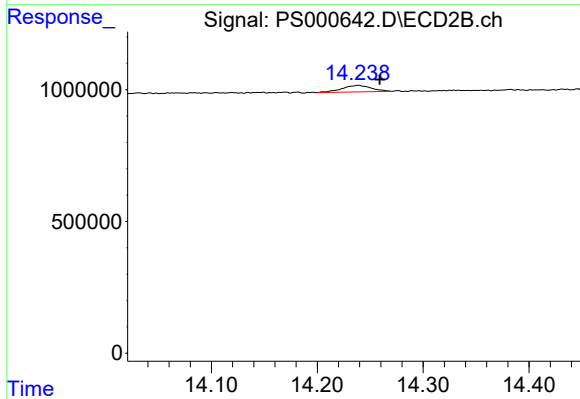

#11 2,4,5-TP (SILVEX)


R.T.: 14.239 min
Delta R.T.: -0.020 min
Response: 484343
Conc: 0.25 ng/ml

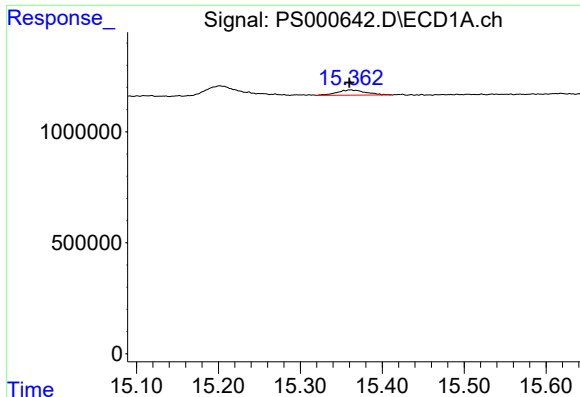

#12 2,4,5-T


R.T.: 15.361 min
Delta R.T.: 0.001 min
Response: 580777
Conc: 0.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

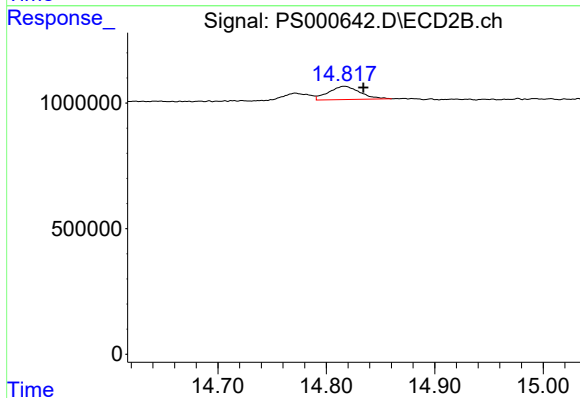


#12 2,4,5-T

R.T.: 14.817 min
Delta R.T.: -0.017 min
Response: 1063002
Conc: 0.63 ng/ml

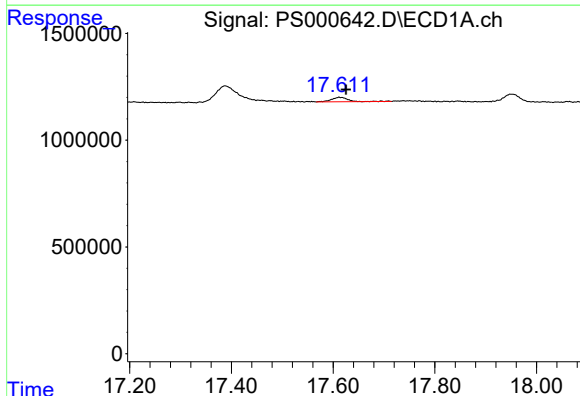


#14 DINOSEB

R.T.: 17.613 min
Delta R.T.: -0.012 min
Response: 479366
Conc: 0.32 ng/ml

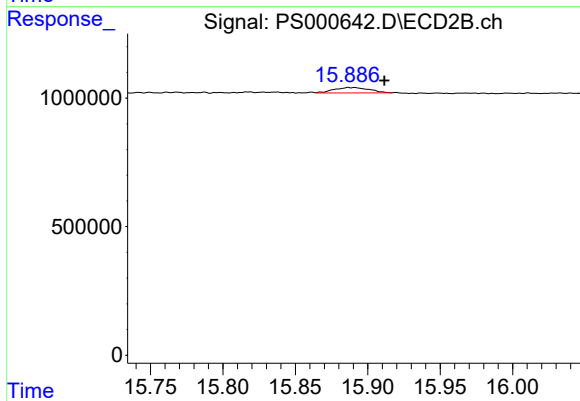

#14 DINOSEB


R.T.: 15.887 min
Delta R.T.: -0.025 min
Response: 356587
Conc: 0.27 ng/ml

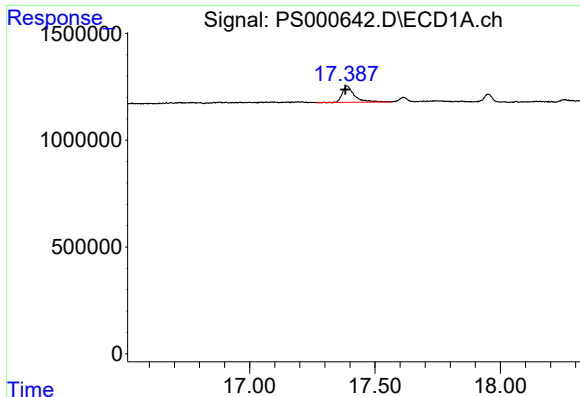

#15 Picloram


R.T.: 17.388 min
Delta R.T.: 0.006 min
Response: 2589656
Conc: 0.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

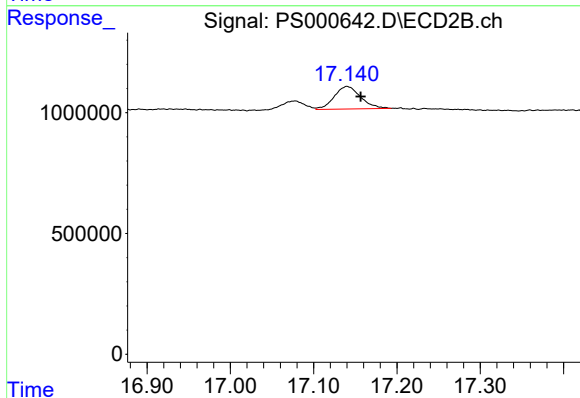


#15 Picloram

R.T.: 17.140 min
Delta R.T.: -0.016 min
Response: 2070915
Conc: 0.83 ng/ml

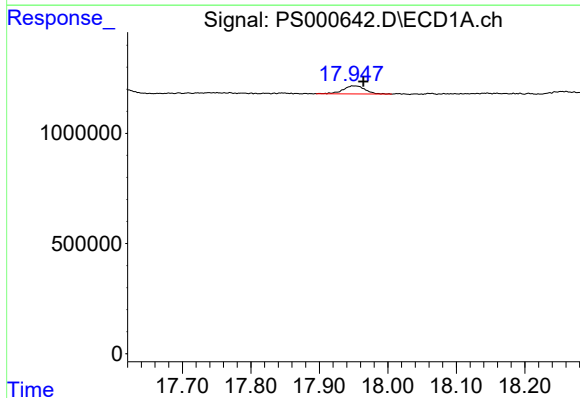

#16 DCPA

R.T.: 17.951 min
Delta R.T.: -0.013 min
Response: 831652
Conc: 0.32 ng/ml

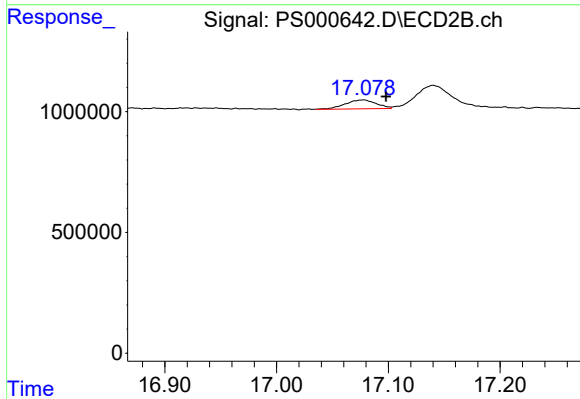

#16 DCPA

R.T.: 17.078 min
Delta R.T.: -0.020 min
Response: 712966
Conc: 0.31 ng/ml