

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062618\
 Data File : PS000655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2018 21:48
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 00:51:44 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.818	11.199	194.0E6	160.1E6	515.107	470.396
Target Compounds							
1) T	Dalapon	0.000	2.532	0	33775	N.D.	0.077 #
3) T	4-Nitroph...	11.441	0.000	402073	0	1.710	N.D. #
6) T	MCP	12.504	0.000	579072	0	0.511	N.D. #
7) T	MCPA	12.737	0.000	1823929	0	1.038	N.D. #
8) T	DICHLORPROP	13.368	0.000	1952433	0	5.190	N.D. #
10) T	Pentachlo...	14.085	0.000	595880	0	0.114	N.D. #
11) T	2,4,5-TP ...	0.000	14.250	0	2149005	N.D.	1.104 #
12) T	2,4,5-T	15.362	0.000	247134	0	0.115	N.D. #
14) T	DINOSEB	17.609	15.868	138853	1578985	0.093	1.210 #
15) T	Picloram	17.375	0.000	803373	0	0.275	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062618\
Data File : PS000655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2018 21:48
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 00:51:44 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

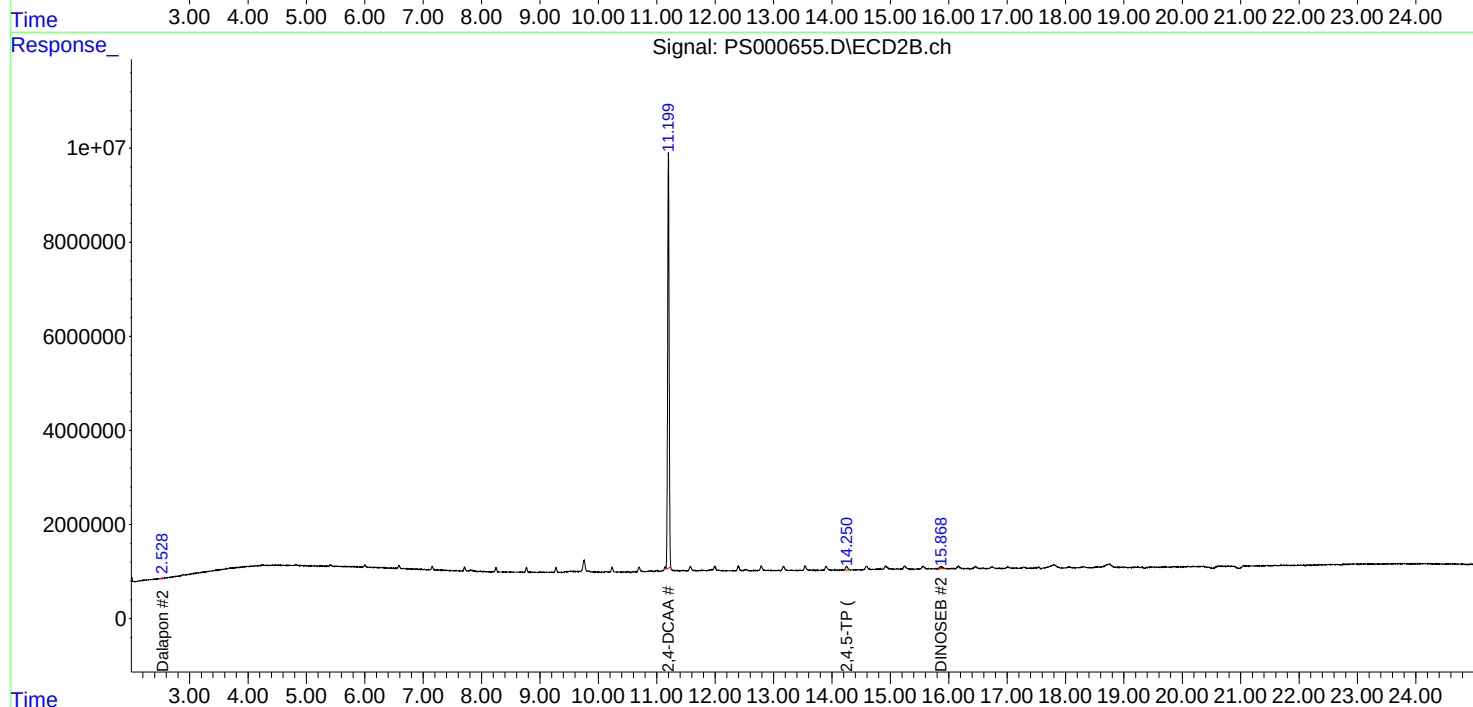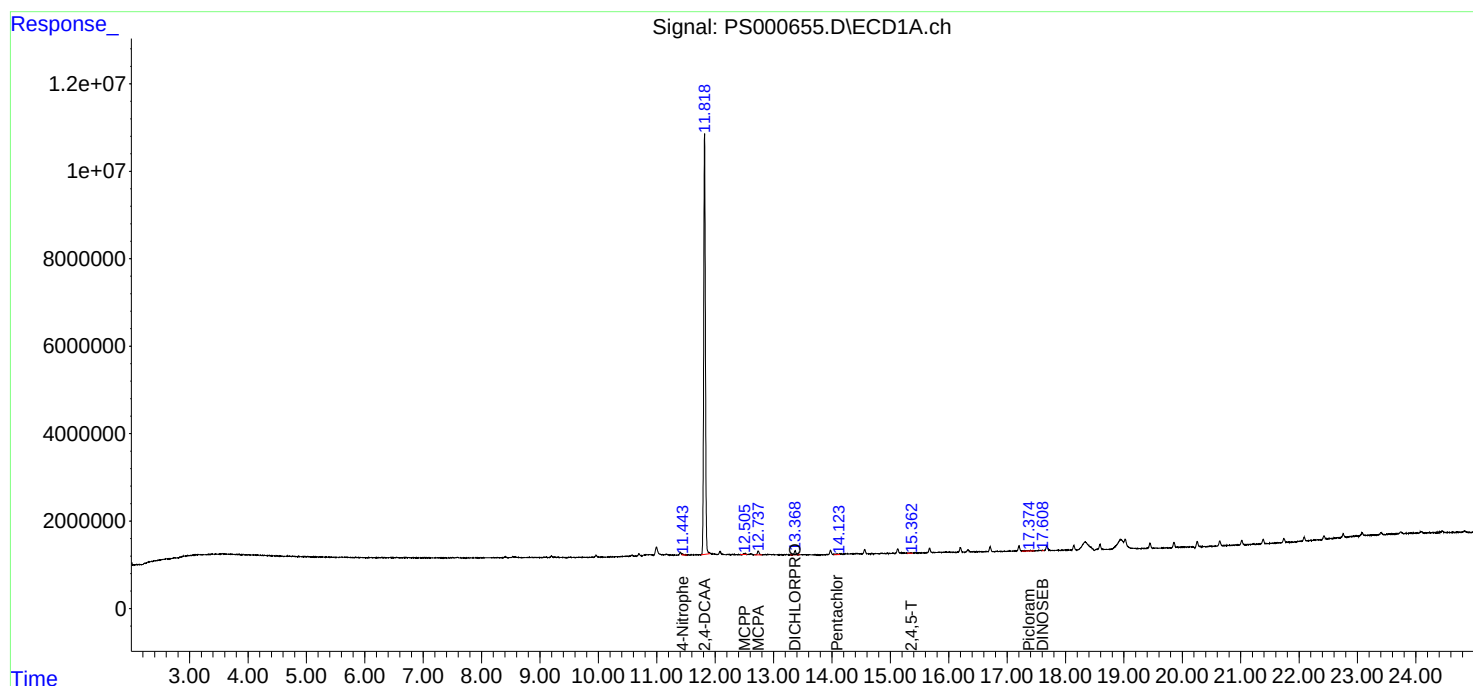


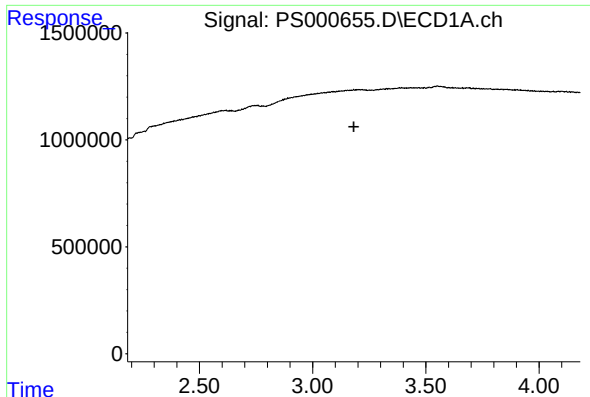

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

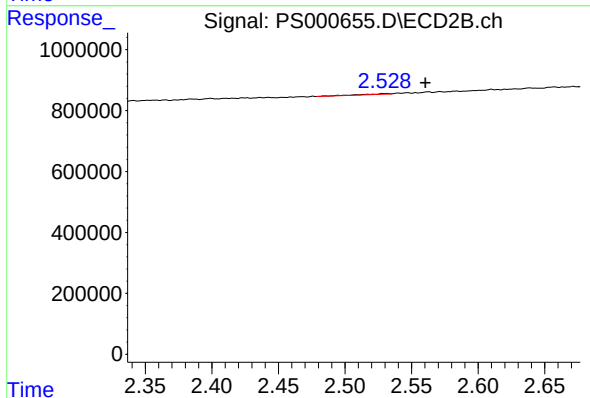


#1 Dalapon

R.T.: 2.532 min
Delta R.T.: -0.029 min
Response: 33775
Conc: 0.08 ng/ml

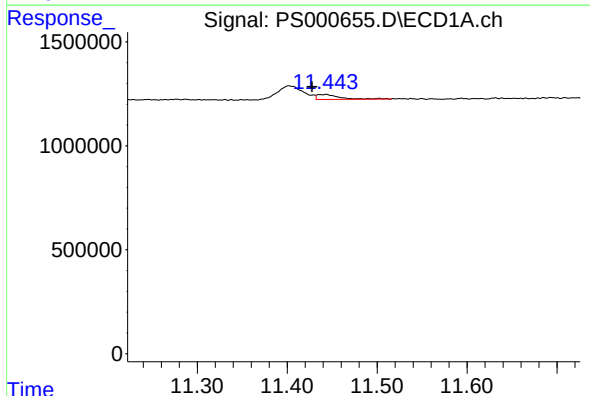


#3 4-Nitrophenol

R.T.: 11.441 min
Delta R.T.: 0.014 min
Response: 402073
Conc: 1.71 ng/ml

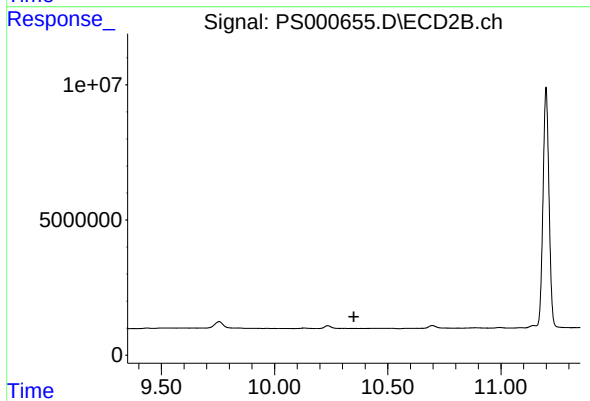

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

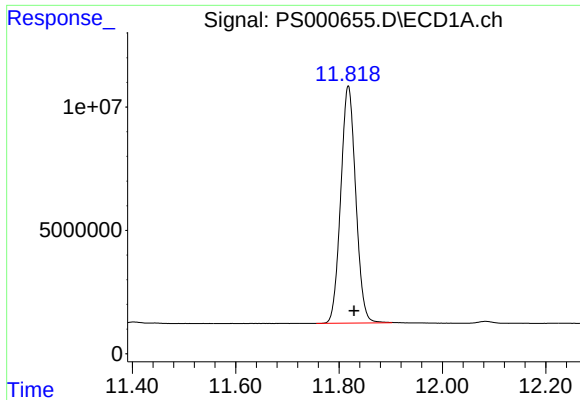

#4 2,4-DCAA


R.T.: 11.818 min
Delta R.T.: -0.011 min
Response: 194017339
Conc: 515.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

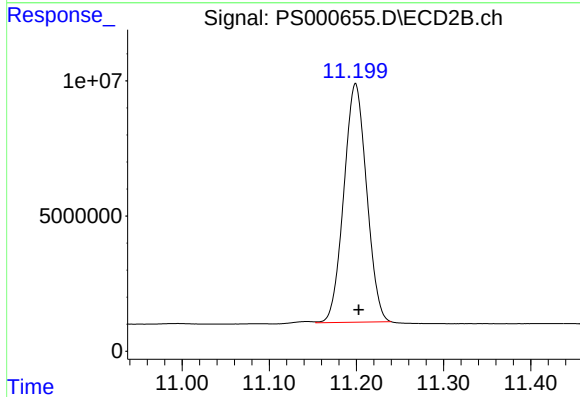


#4 2,4-DCAA

R.T.: 11.199 min
Delta R.T.: -0.004 min
Response: 160079835
Conc: 470.40 ng/ml

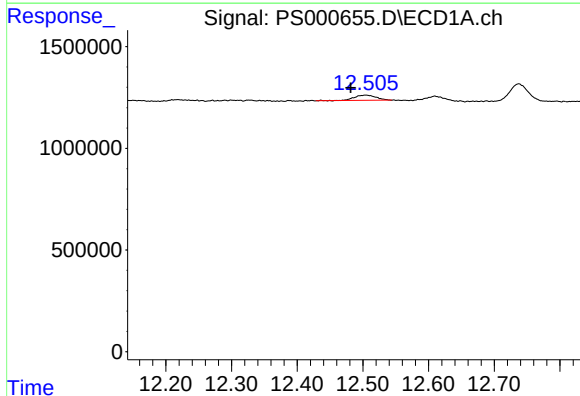


#6 MCP

R.T.: 12.504 min
Delta R.T.: 0.023 min
Response: 579072
Conc: 0.51 ug/ml

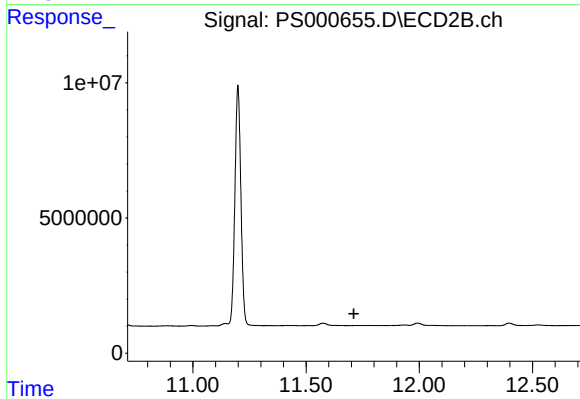

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.711 min
Response: 0
Conc: N.D.

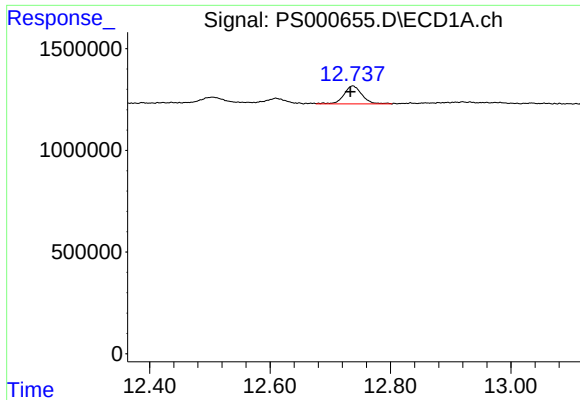

#7 MCPA


R.T.: 12.737 min
Delta R.T.: 0.004 min
Response: 1823929
Conc: 1.04 ug/ml

Instrument :
ECD_S
ClientSampleId :

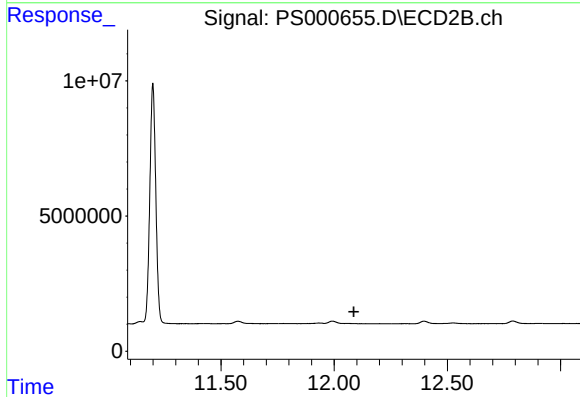


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.087 min
Response: 0
Conc: N.D.

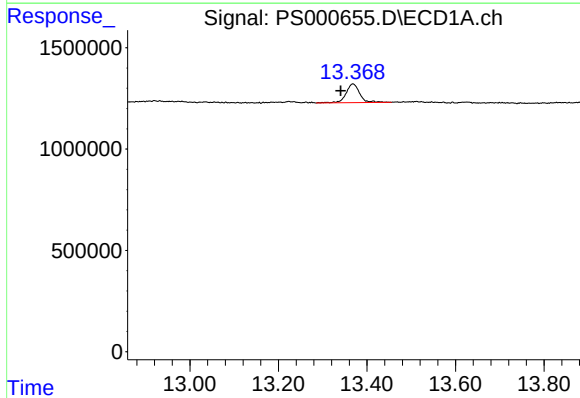


#8 DICHLORPROP

R.T.: 13.368 min
Delta R.T.: 0.027 min
Response: 1952433
Conc: 5.19 ng/ml

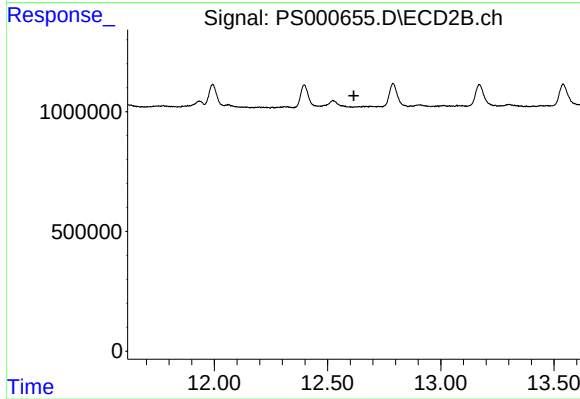

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.616 min
Response: 0
Conc: N.D.

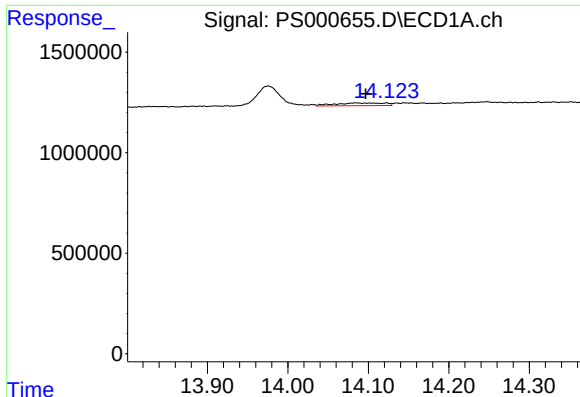

#10 Pentachlorophenol


R.T.: 14.085 min
Delta R.T.: -0.012 min
Response: 595880
Conc: 0.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

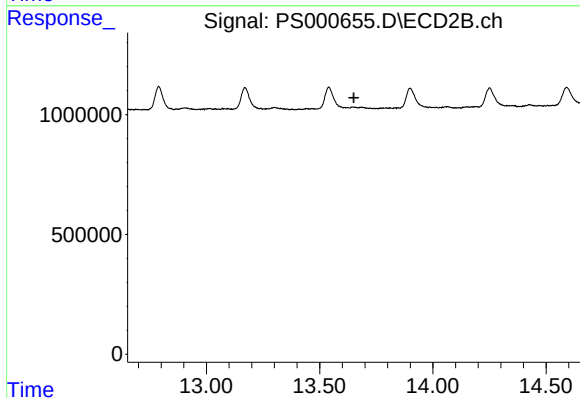


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.651 min
Response: 0
Conc: N.D.

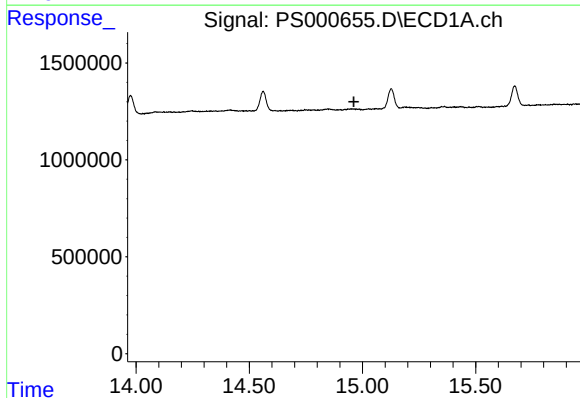


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.962 min
Response: 0
Conc: N.D.

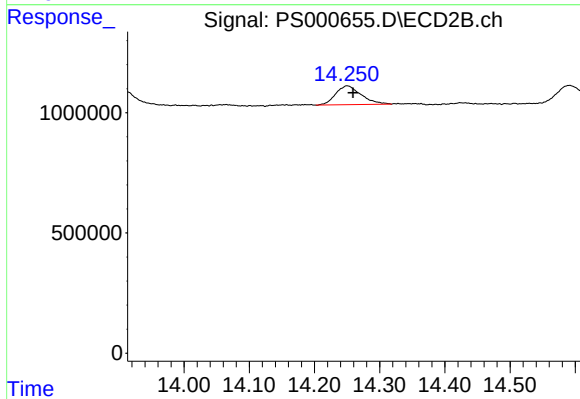

#11 2,4,5-TP (SILVEX)


R.T.: 14.250 min
Delta R.T.: -0.009 min
Response: 2149005
Conc: 1.10 ng/ml

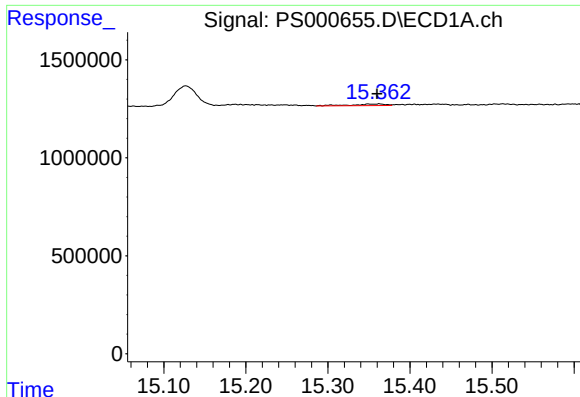

#12 2,4,5-T


R.T.: 15.362 min
Delta R.T.: 0.002 min
Response: 247134
Conc: 0.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

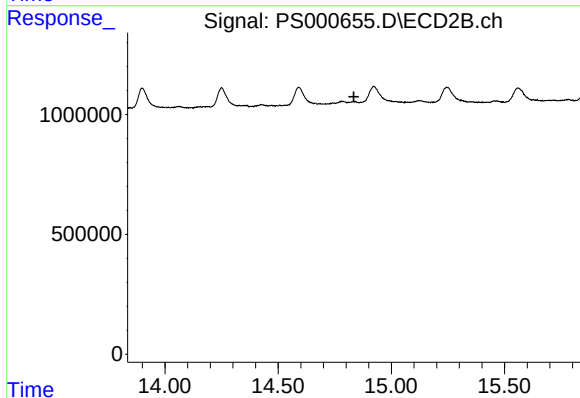


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.834 min
Response: 0
Conc: N.D.

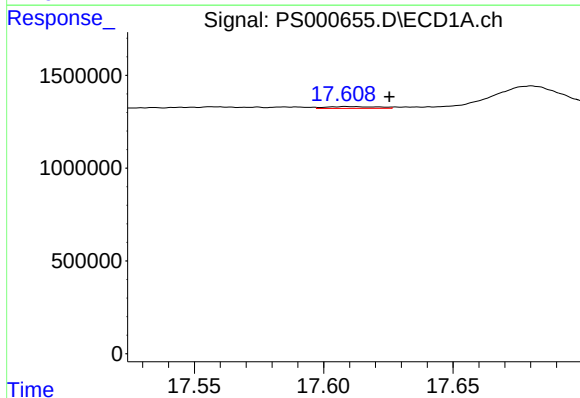


#14 DINOSEB

R.T.: 17.609 min
Delta R.T.: -0.016 min
Response: 138853
Conc: 0.09 ng/ml

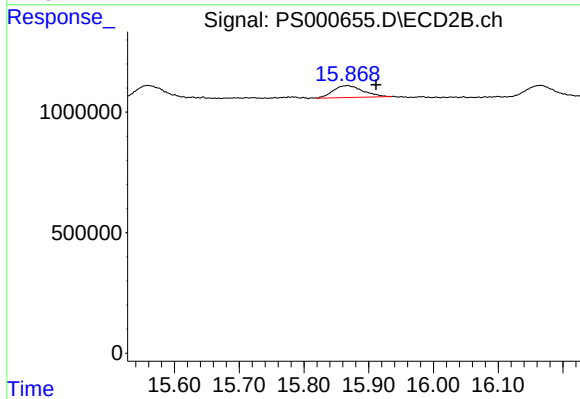

#14 DINOSEB


R.T.: 15.868 min
Delta R.T.: -0.043 min
Response: 1578985
Conc: 1.21 ng/ml

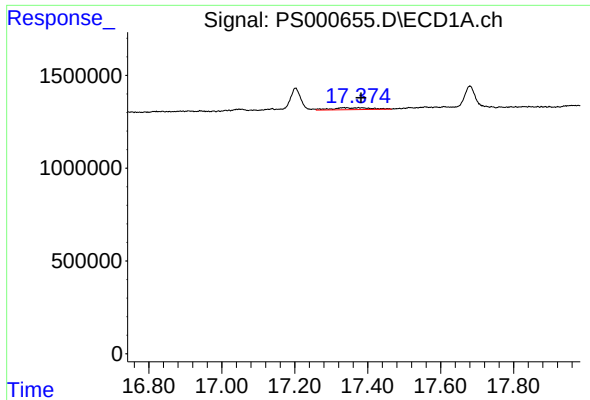

#15 Picloram

R.T.: 17.375 min
Delta R.T.: -0.007 min
Response: 803373
Conc: 0.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

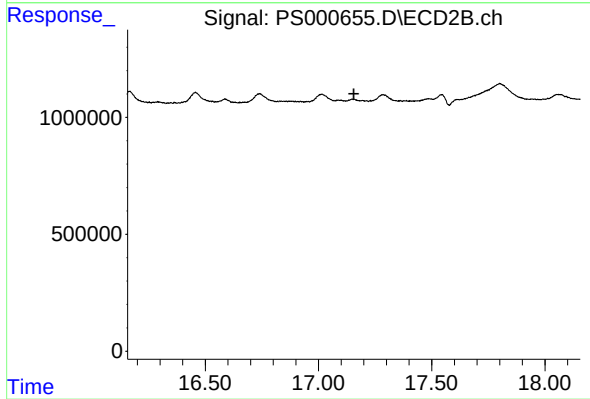

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.156 min
Response: 0
Conc: N.D.