

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
 Data File : PS005217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2019 10:06
 Operator : SM\AJ
 Sample : K3156-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-02-062419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 12:23:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.286	256.3E6	175.6E6	174.604	175.226
Target Compounds							
1) T	Dalapon	2.078	1.763	87047747	-14161318	47.224	N.D. #
2) T	3,5-DICHL...	0.000	4.562	0	8089225	N.D.	6.134
7) T	MCPA	5.966	0.000	18245995	0	2.906	N.D. #
8) T	DICHLORPROP	0.000	5.973	0	32589096	N.D.	33.752
10) T	Pentachlo...	0.000	6.552	0	16804369	N.D.	1.307
11) T	2,4,5-TP ...	0.000	6.940	0	84934229	N.D.	15.949
12) T	2,4,5-T	7.598	7.389	216.1E6	44972258	26.857	8.817 #
15) T	Picloram	9.140	9.096	276.0E6	191.2E6	24.019	25.338
16) T	DCPA	0.000	9.096	0	191.2E6	N.D.	28.088



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
Data File : PS005217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2019 10:06
Operator : SM\AJ
Sample : K3156-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HD-02-062419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 12:23:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

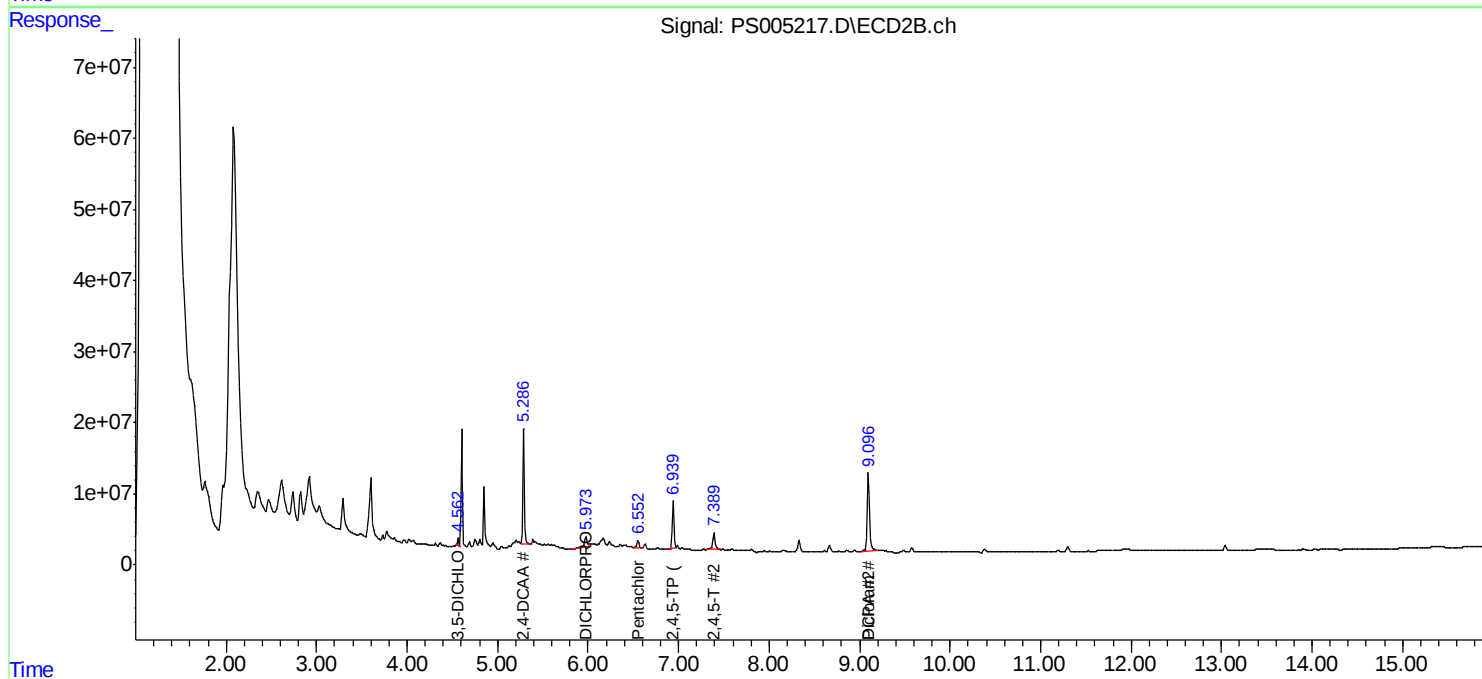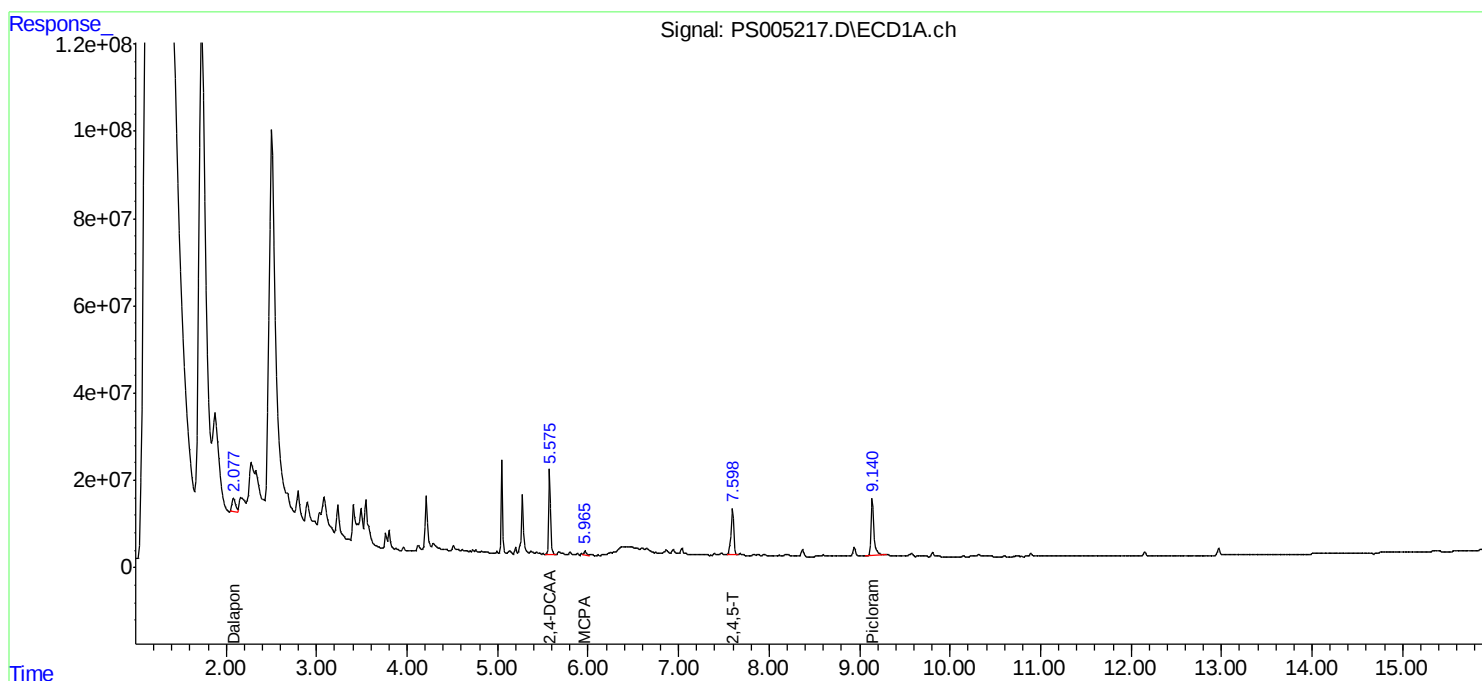


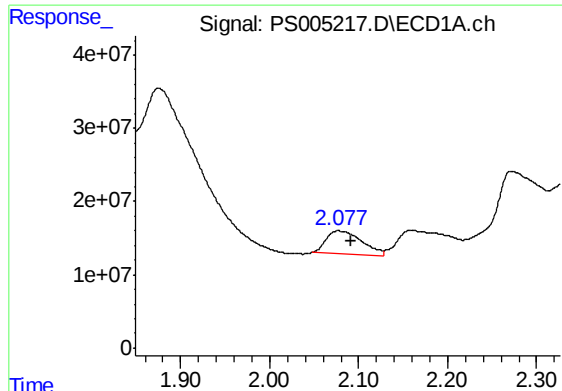

#1 Dalapon


R.T.: 2.078 min
Delta R.T.: -0.014 min
Response: 87047747
Conc: 47.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-062419

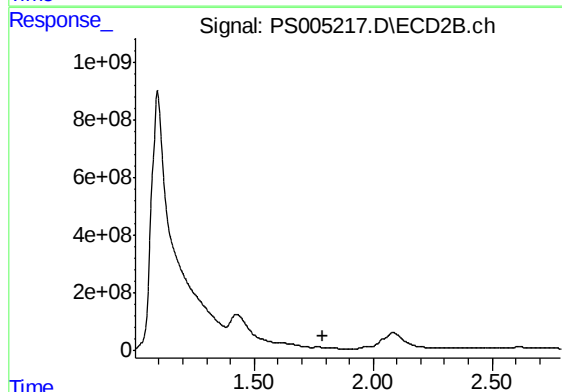


#1 Dalapon

R.T.: 1.763 min
Delta R.T.: -0.024 min
Response: -14161318
Conc: N.D.

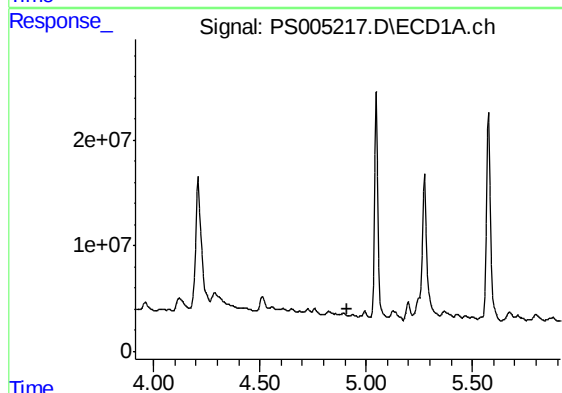


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

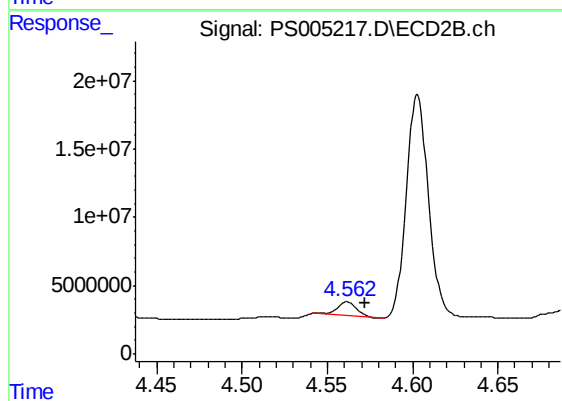

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.562 min
Delta R.T.: -0.011 min
Response: 8089225
Conc: 6.13 ng/ml

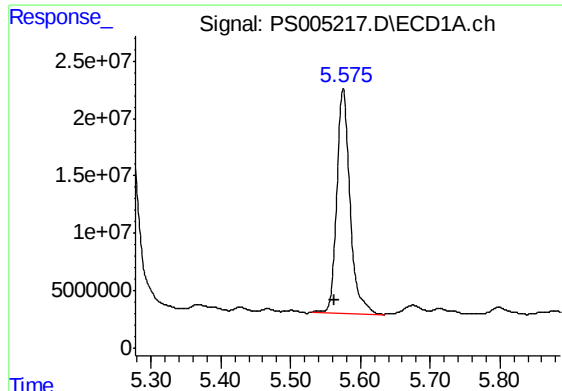

#4 2,4-DCAA


R.T.: 5.575 min
Delta R.T.: 0.012 min
Response: 256299835
Conc: 174.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-062419

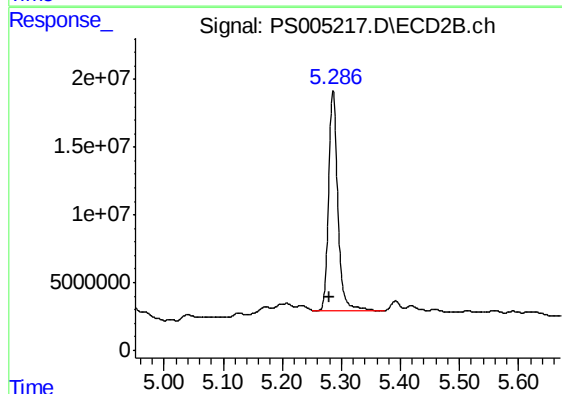


#4 2,4-DCAA

R.T.: 5.286 min
Delta R.T.: 0.007 min
Response: 175641450
Conc: 175.23 ng/ml

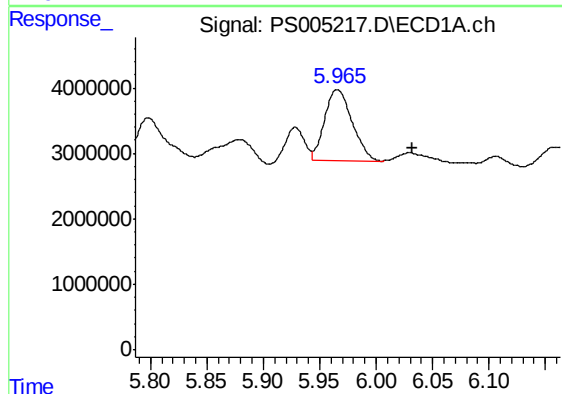


#7 MCPA

R.T.: 5.966 min
Delta R.T.: -0.067 min
Response: 18245995
Conc: 2.91 ug/ml

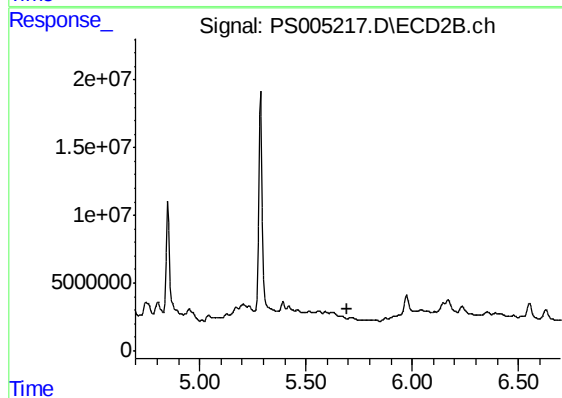

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.698 min
Response: 0
Conc: N.D.

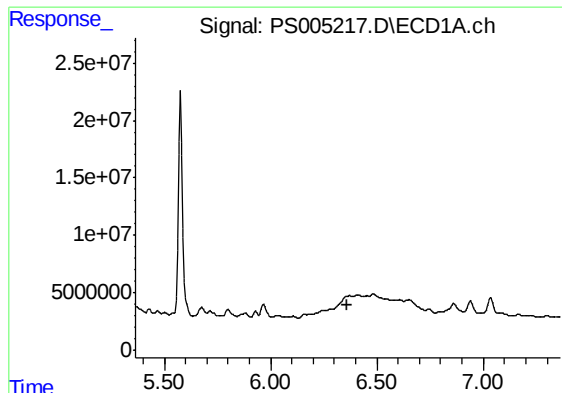

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-02-062419

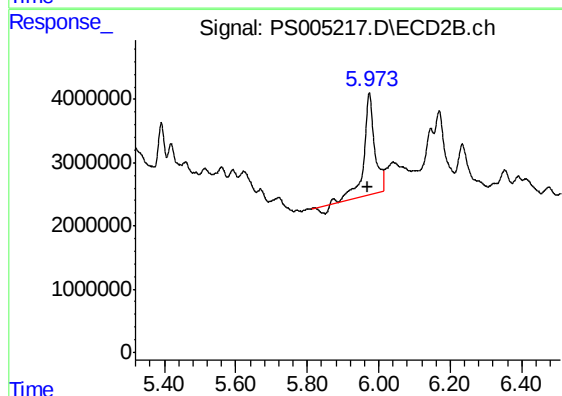


#8 DICHLORPROP

R.T.: 5.973 min
Delta R.T.: 0.004 min
Response: 32589096
Conc: 33.75 ng/ml

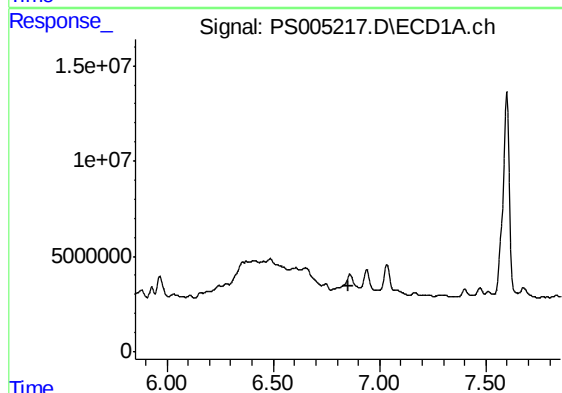


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

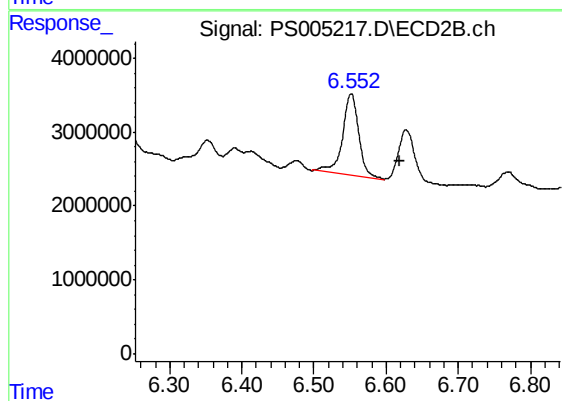

#10 Pentachlorophenol


R.T.: 6.552 min
Delta R.T.: -0.067 min
Response: 16804369
Conc: 1.31 ng/ml

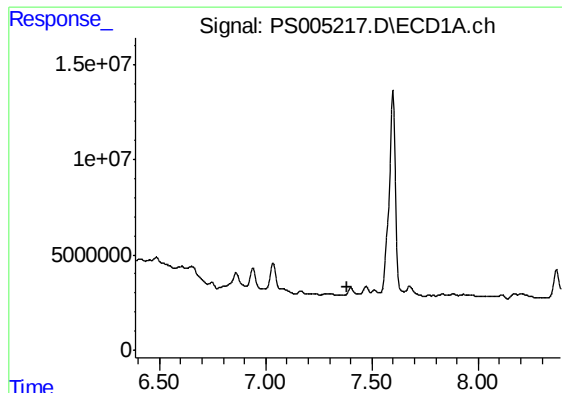

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-02-062419

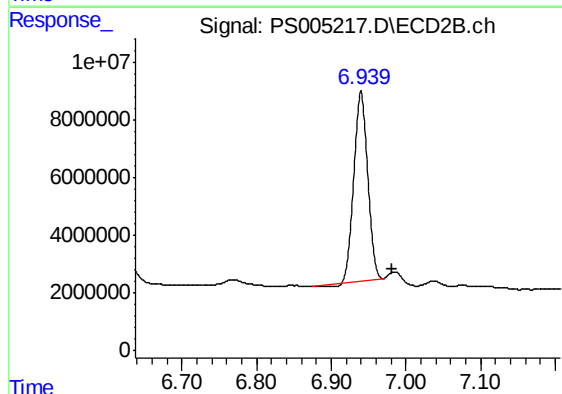


#11 2,4,5-TP (SILVEX)

R.T.: 6.940 min
Delta R.T.: -0.041 min
Response: 84934229
Conc: 15.95 ng/ml

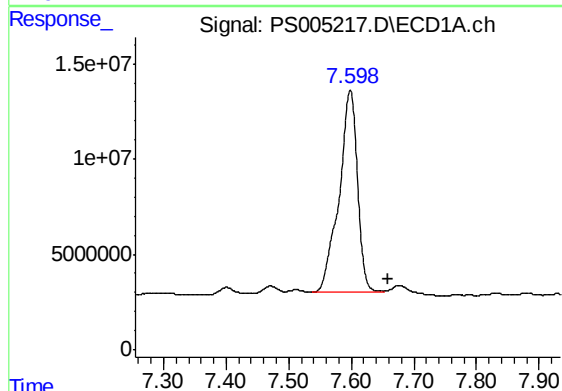


#12 2,4,5-T

R.T.: 7.598 min
Delta R.T.: -0.060 min
Response: 216136767
Conc: 26.86 ng/ml

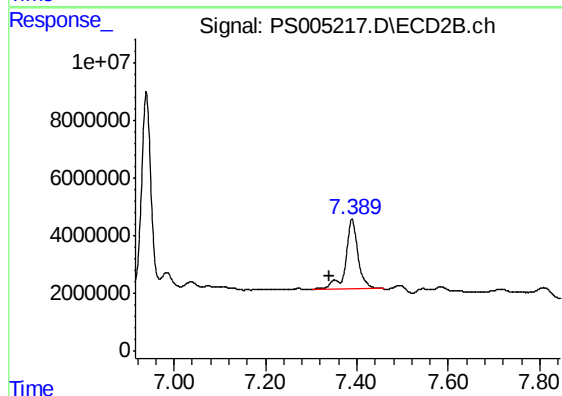

#12 2,4,5-T


R.T.: 7.389 min
Delta R.T.: 0.049 min
Response: 44972258
Conc: 8.82 ng/ml

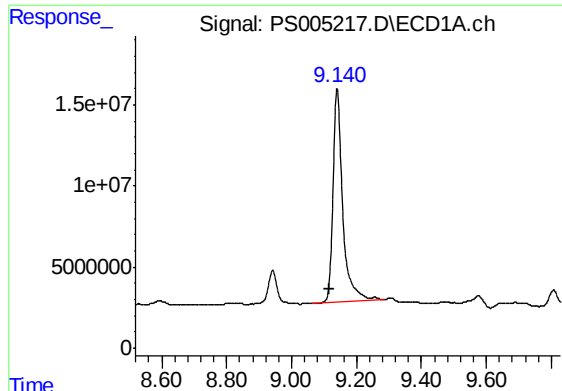

#15 Picloram


R.T.: 9.140 min
Delta R.T.: 0.024 min
Response: 276006362
Conc: 24.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-062419

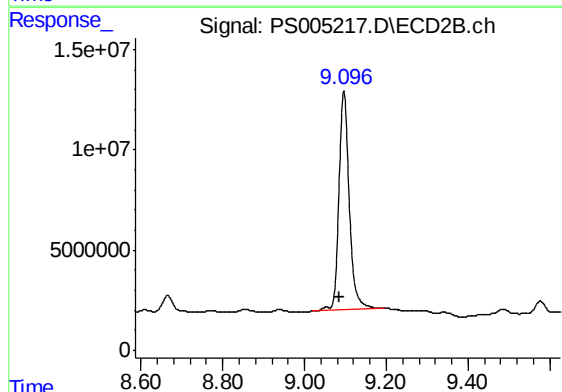


#15 Picloram

R.T.: 9.096 min
Delta R.T.: 0.011 min
Response: 191208038
Conc: 25.34 ng/ml

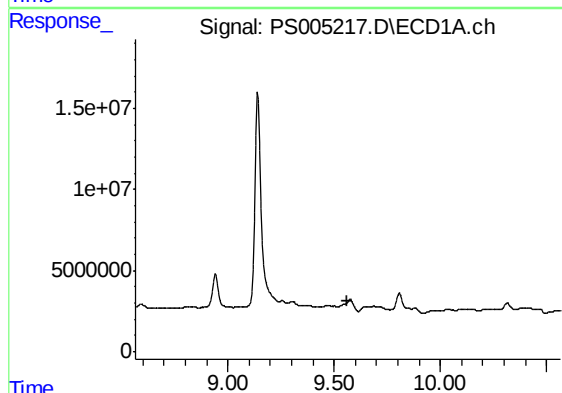

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

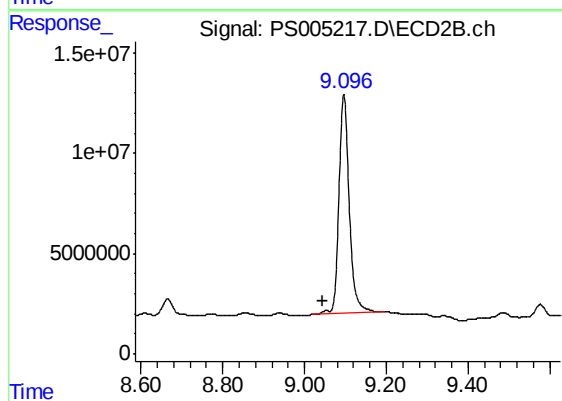

#16 DCPA

R.T.: 9.096 min
Delta R.T.: 0.050 min
Response: 191208038
Conc: 28.09 ng/ml