

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
 Data File : PS005219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2019 10:50
 Operator : SM\AJ
 Sample : K3155-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BAT-B11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 12:24:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.584	5.299	461.8E6	245.2E6	314.630	244.628
Target Compounds							
1) T	Dalapon	2.088	0.000	27749423	0	15.054	N.D. #
2) T	3,5-DICHL...	4.845	4.559	11912455	24012110	5.927	18.209 #
3) T	4-Nitroph...	5.387	4.954	14421961	100.8E6	19.912	201.087 #
5) T	DICAMBA	0.000	5.405	0	30903232	N.D.	8.256
6) T	MCPD	5.921	0.000	18882028	0	4.313	N.D. #
7) T	MCPA	6.078	5.690	23853558	41355426	3.798	10.209 #
8) T	DICHLORPROP	6.383	5.989	-4798787	13858696	N.D.	14.353
9) T	2,4-D	0.000	6.217	0	79035272	N.D.	70.866
10) T	Pentachlo...	6.858	6.602	136.0E6	79307220	6.911	6.169
11) T	2,4,5-TP ...	7.445	7.008	33771406	22933509	4.140	4.307
12) T	2,4,5-T	7.607	7.298	317.2E6	42420621	39.416	8.316 #
13) T	2,4-DB	8.179	7.860	11825540	148.5E6	10.181	227.499 #
14) T	DINOSEB	0.000	8.158	0	110.5E6	N.D.	27.321
15) T	Picloram	9.099	0.000	34265288	0	2.982	N.D. #
16) T	DCPA	9.535	0.000	70309535	0	7.048	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
Data File : PS005219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2019 10:50
Operator : SM\AJ
Sample : K3155-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BAT-B11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 12:24:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

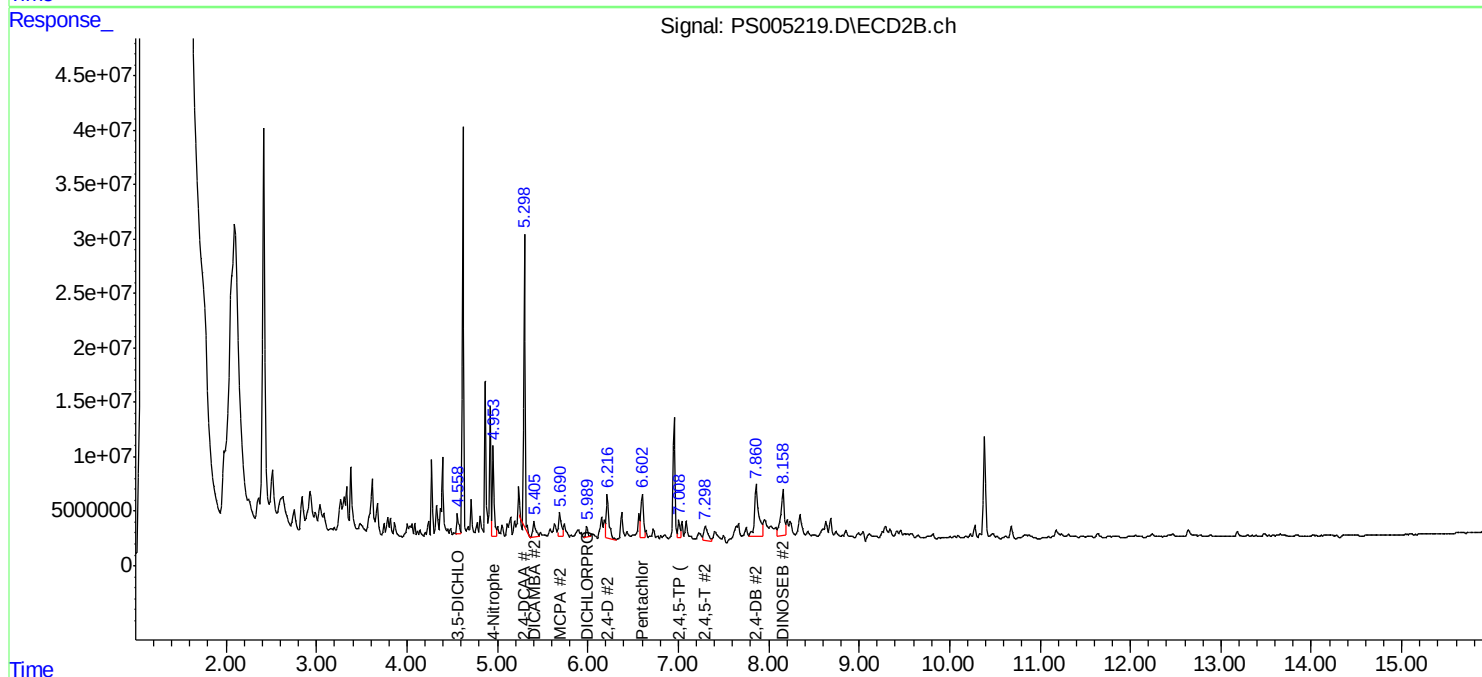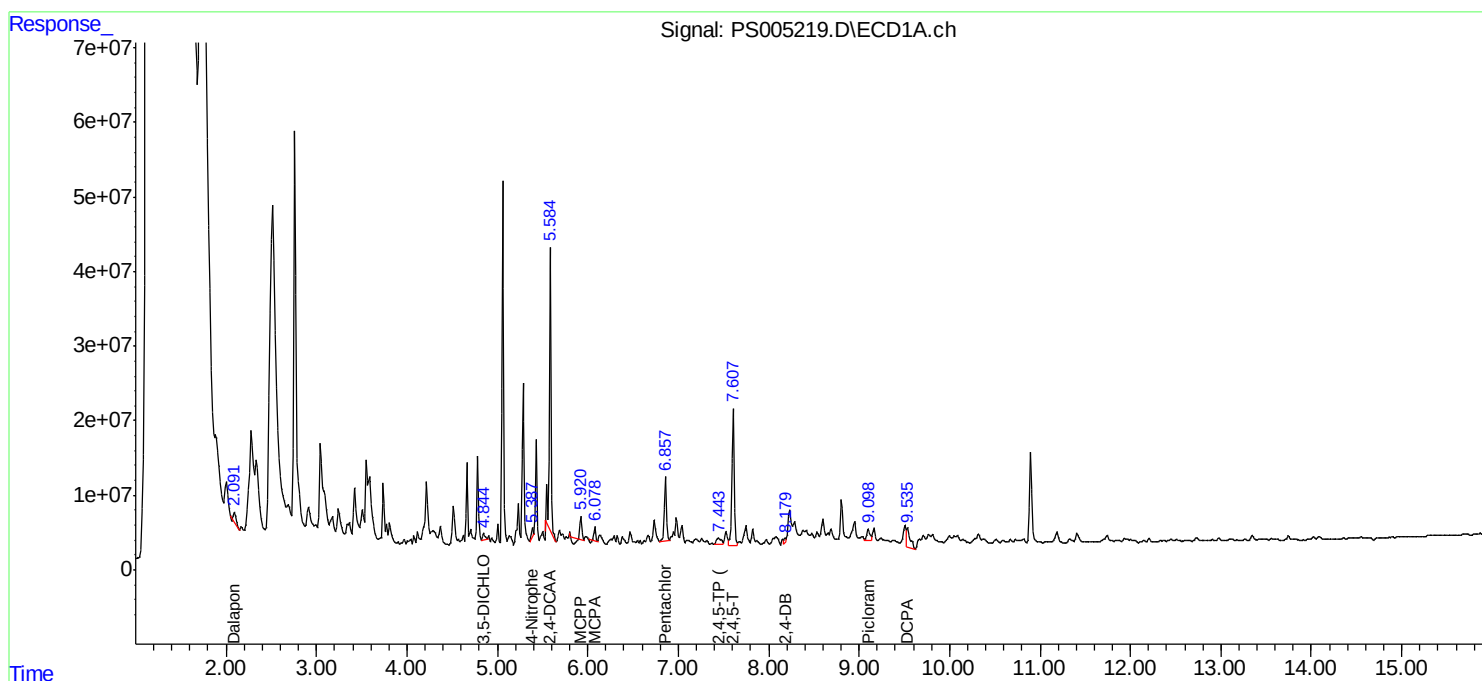


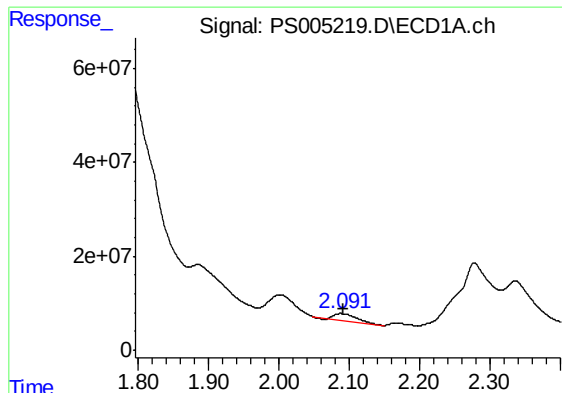

#1 Dalapon


R.T.: 2.088 min
Delta R.T.: -0.004 min
Response: 27749423
Conc: 15.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B11

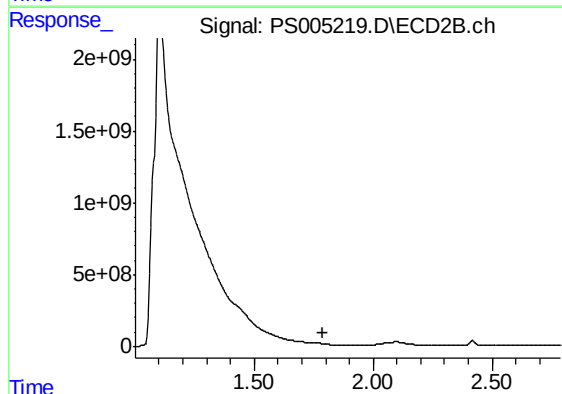


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

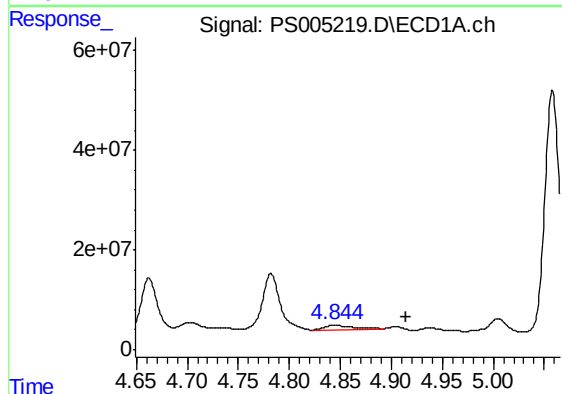


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.845 min
Delta R.T.: -0.070 min
Response: 11912455
Conc: 5.93 ng/ml

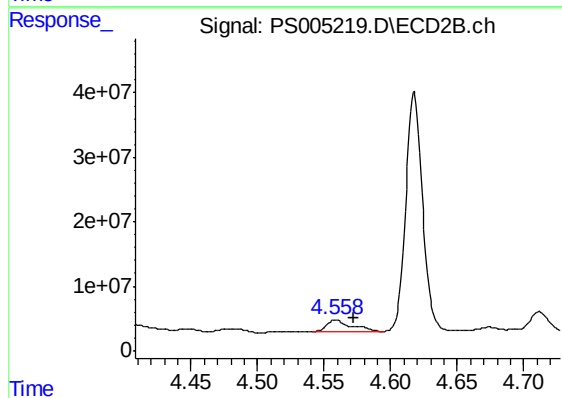

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.559 min
Delta R.T.: -0.014 min
Response: 24012110
Conc: 18.21 ng/ml

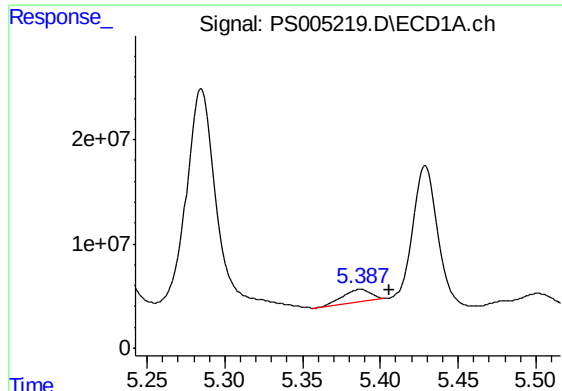

#3 4-Nitrophenol


R.T.: 5.387 min
Delta R.T.: -0.019 min
Response: 14421961
Conc: 19.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B11

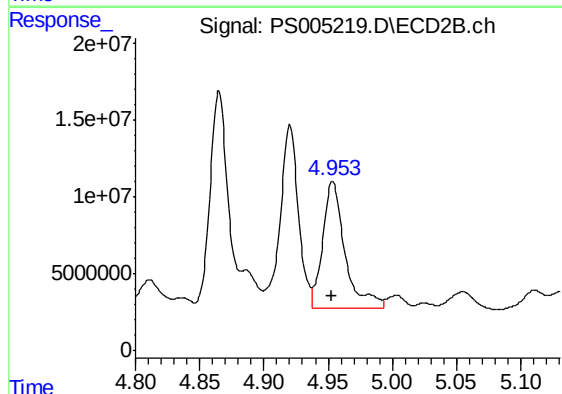


#3 4-Nitrophenol

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 100834961
Conc: 201.09 ng/ml

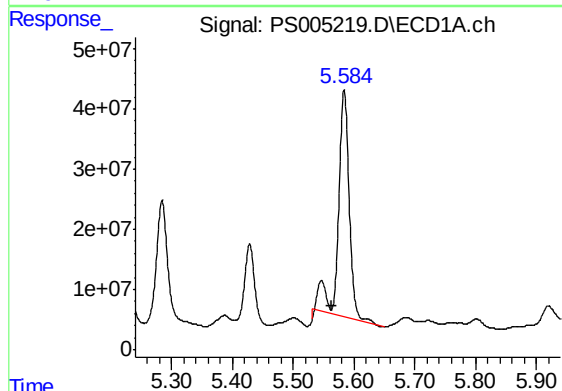


#4 2,4-DCAA

R.T.: 5.584 min
Delta R.T.: 0.021 min
Response: 461843825
Conc: 314.63 ng/ml

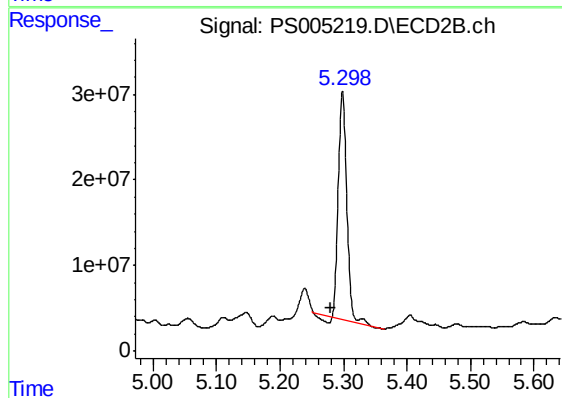

#4 2,4-DCAA


R.T.: 5.299 min
Delta R.T.: 0.019 min
Response: 245207030
Conc: 244.63 ng/ml

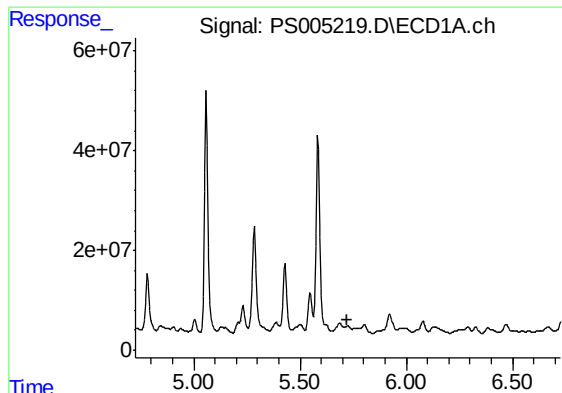

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B11

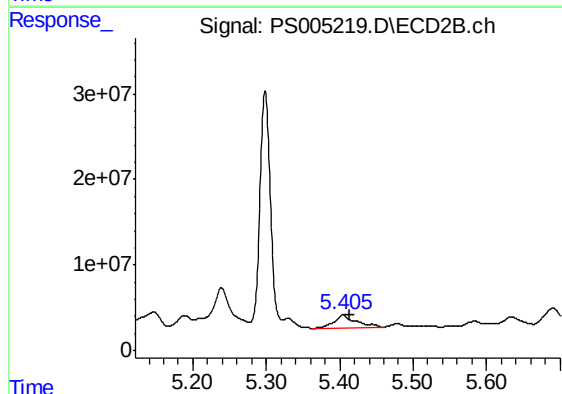


#5 DICAMBA

R.T.: 5.405 min
Delta R.T.: -0.009 min
Response: 30903232
Conc: 8.26 ng/ml

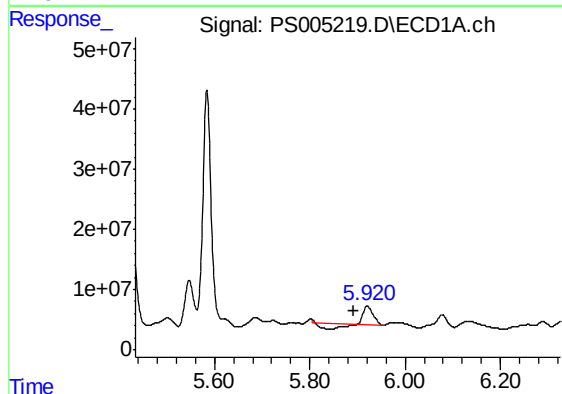


#6 MCPP

R.T.: 5.921 min
Delta R.T.: 0.029 min
Response: 18882028
Conc: 4.31 ug/ml

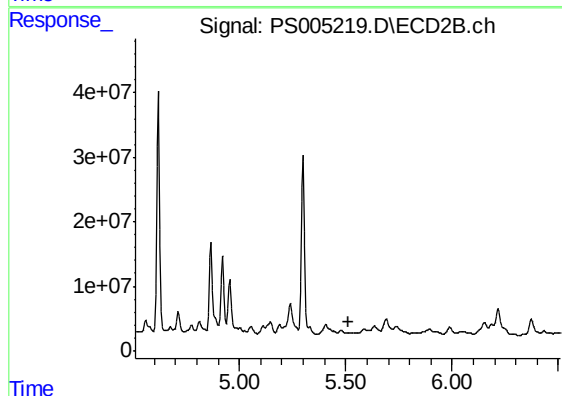

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

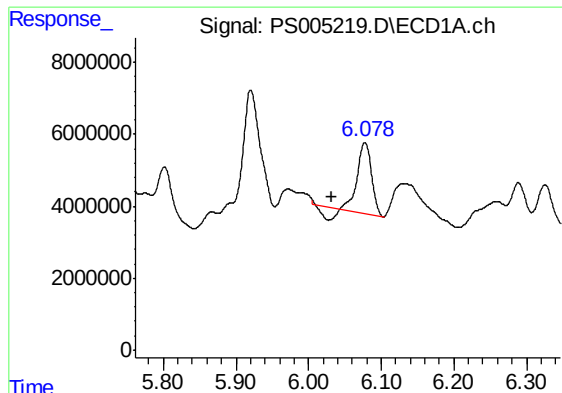

#7 MCPA


R.T.: 6.078 min
Delta R.T.: 0.046 min
Response: 23853558
Conc: 3.80 ug/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B11

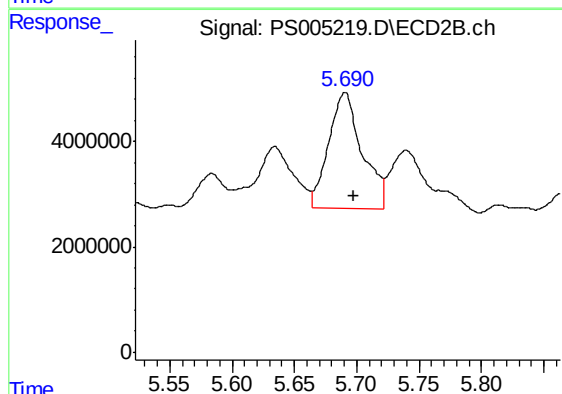


#7 MCPA

R.T.: 5.690 min
Delta R.T.: -0.007 min
Response: 41355426
Conc: 10.21 ug/ml

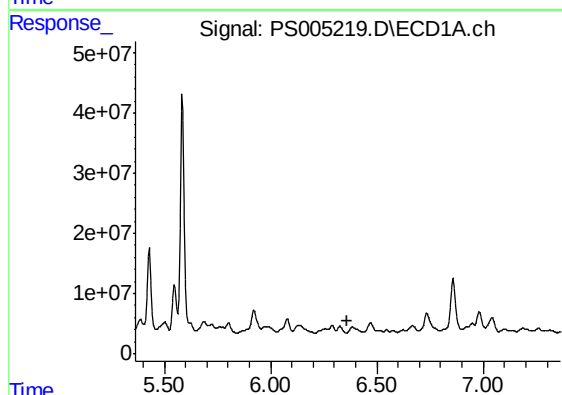


#8 DICHLORPROP

R.T.: 6.383 min
Delta R.T.: 0.020 min
Response: -4798787
Conc: N.D.

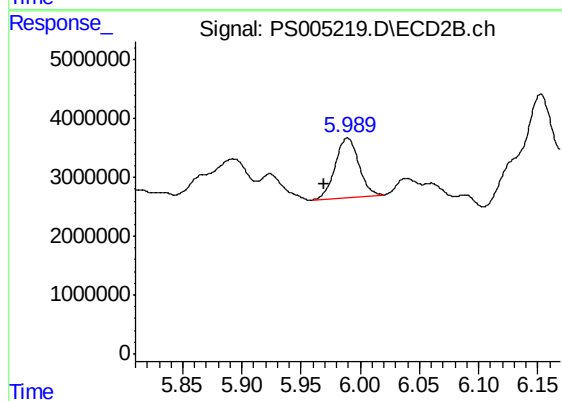

#8 DICHLORPROP


R.T.: 5.989 min
Delta R.T.: 0.020 min
Response: 13858696
Conc: 14.35 ng/ml

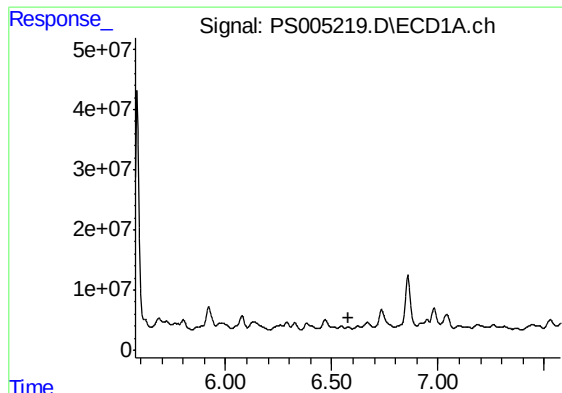

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B11

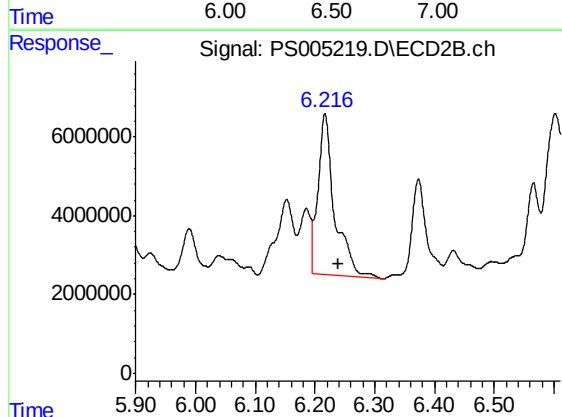


#9 2,4-D

R.T.: 6.217 min
Delta R.T.: -0.023 min
Response: 79035272
Conc: 70.87 ng/ml

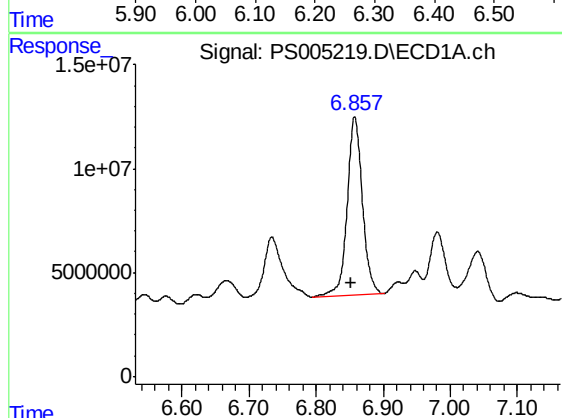


#10 Pentachlorophenol

R.T.: 6.858 min
Delta R.T.: 0.006 min
Response: 135977073
Conc: 6.91 ng/ml

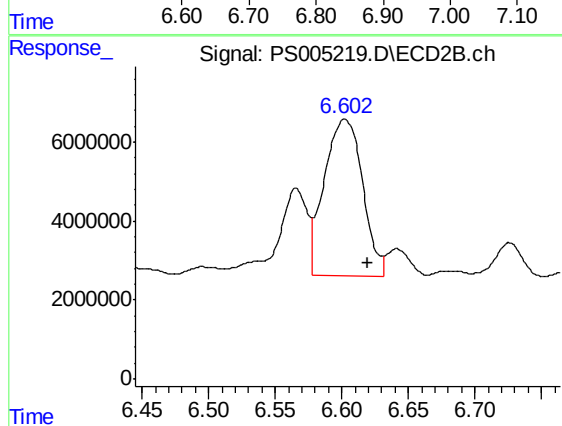

#10 Pentachlorophenol


R.T.: 6.602 min
Delta R.T.: -0.017 min
Response: 79307220
Conc: 6.17 ng/ml

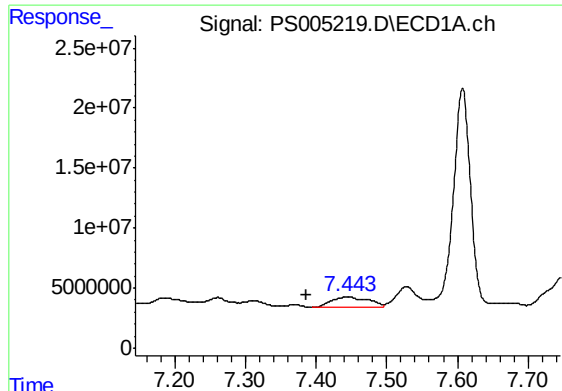

#11 2,4,5-TP (SILVEX)


R.T.: 7.445 min
Delta R.T.: 0.058 min
Response: 33771406
Conc: 4.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B11

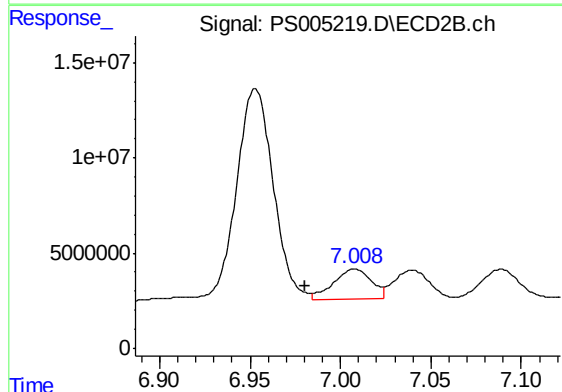


#11 2,4,5-TP (SILVEX)

R.T.: 7.008 min
Delta R.T.: 0.027 min
Response: 22933509
Conc: 4.31 ng/ml

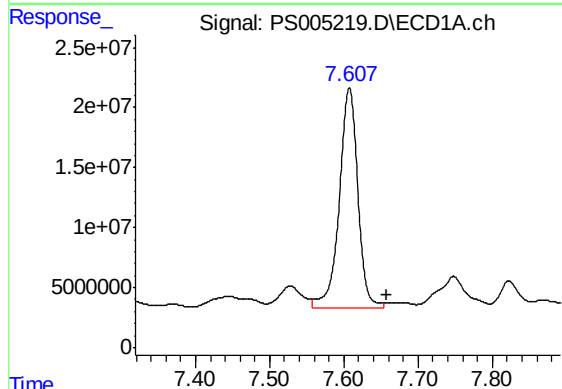


#12 2,4,5-T

R.T.: 7.607 min
Delta R.T.: -0.051 min
Response: 317216373
Conc: 39.42 ng/ml

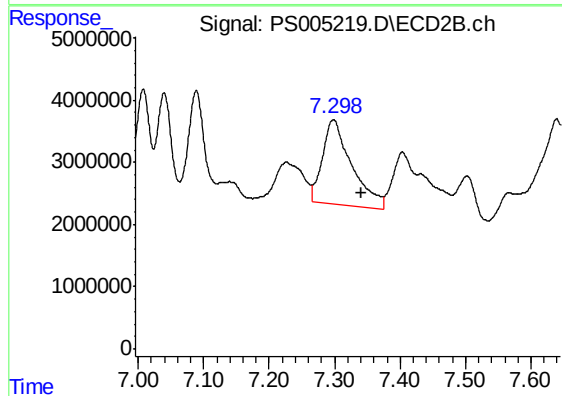

#12 2,4,5-T


R.T.: 7.298 min
Delta R.T.: -0.042 min
Response: 42420621
Conc: 8.32 ng/ml

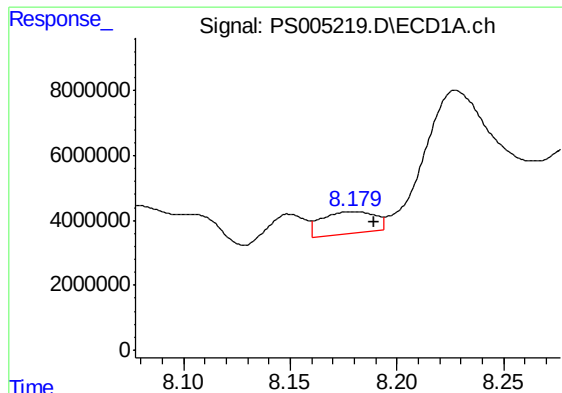

#13 2,4-DB


R.T.: 8.179 min
Delta R.T.: -0.010 min
Response: 11825540
Conc: 10.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B11

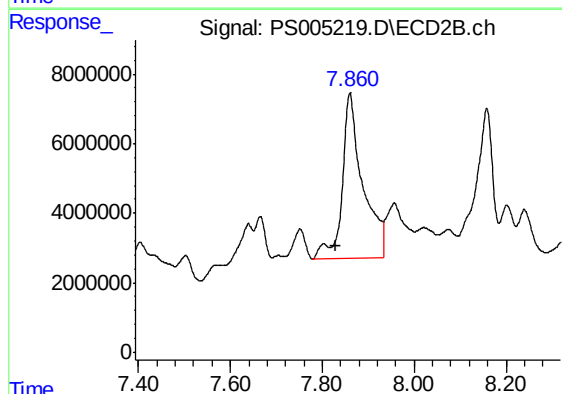


#13 2,4-DB

R.T.: 7.860 min
Delta R.T.: 0.031 min
Response: 148523151
Conc: 227.50 ng/ml

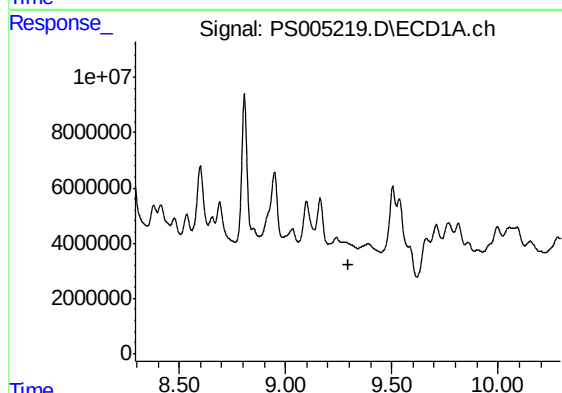


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.294 min
Response: 0
Conc: N.D.

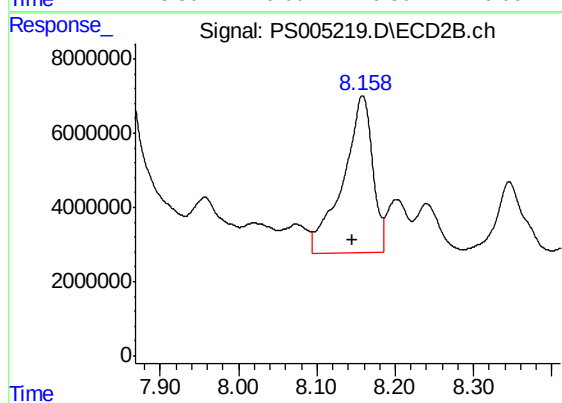

#14 DINOSEB


R.T.: 8.158 min
Delta R.T.: 0.012 min
Response: 110466389
Conc: 27.32 ng/ml

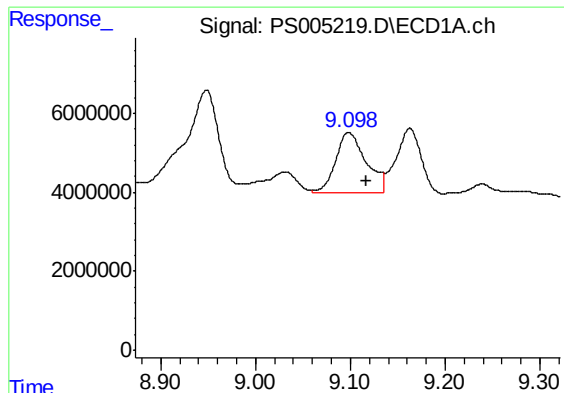

#15 Picloram


R.T.: 9.099 min
Delta R.T.: -0.018 min
Response: 34265288
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B11

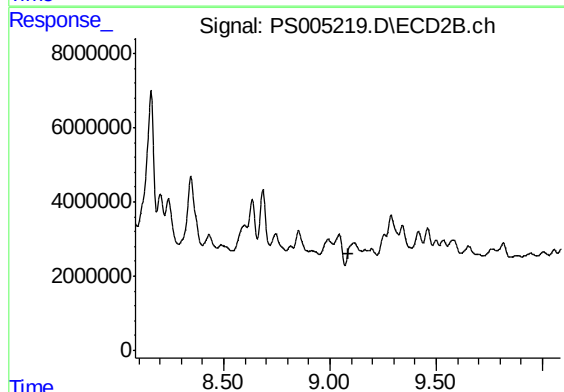


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.

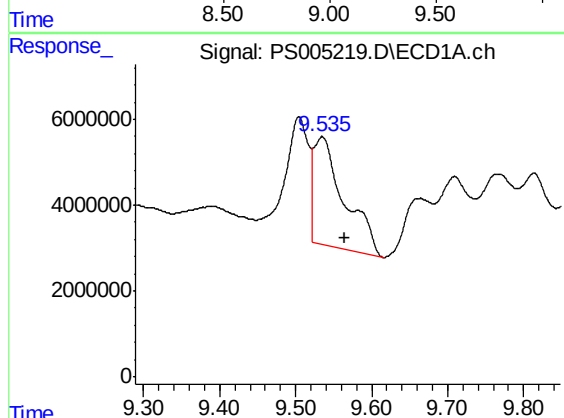

#16 DCPA

R.T.: 9.535 min
Delta R.T.: -0.030 min
Response: 70309535
Conc: 7.05 ng/ml

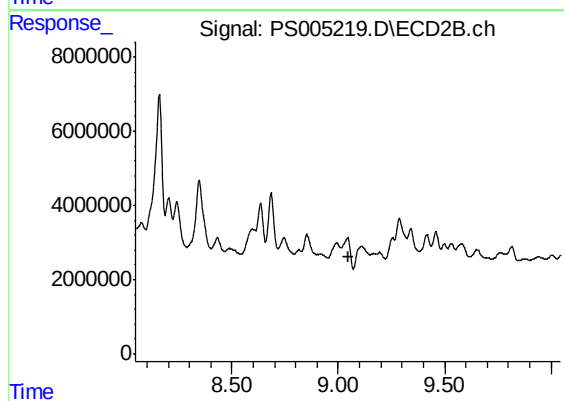

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.046 min
Response: 0
Conc: N.D.