

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
 Data File : PS005220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2019 11:12
 Operator : SM\AJ
 Sample : K3155-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BAT-B06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 12:24:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.549	5.264	30697827	45572082	20.913	45.464 #
Target Compounds							
1) T	Dalapon	0.000	1.746	0	696.9E6	N.D.	528.319
2) T	3,5-DICHL...	4.863	4.560	19364004	12136246	9.635	9.203
3) T	4-Nitroph...	5.387	4.955	8609688	54434155	11.887	108.554 #
5) T	DICAMBA	0.000	5.406	0	37010236	N.D.	9.887
6) T	MCPD	5.922	0.000	32013151	0	7.313	N.D. #
7) T	MCPA	6.077	5.713	34862698	117.3E6	5.552	28.967 #
8) T	DICHLORPROP	0.000	5.991	0	20539966	N.D.	21.273
9) T	2,4-D	6.578	6.247	16873376	26417150	10.854	23.687 #
10) T	Pentachlo...	6.859	6.595	127.6E6	338.8E6	6.487	26.355 #
11) T	2,4,5-TP ...	0.000	6.953	0	165.1E6	N.D.	31.008
12) T	2,4,5-T	7.607	0.000	326.6E6	0	40.580	N.D. #
13) T	2,4-DB	8.226	7.860	210.0E6	133.4E6	180.767	204.260
14) T	DINOSEB	0.000	8.159	0	69741773	N.D.	17.249
15) T	Picloram	9.101	0.000	35000465	0	3.046	N.D. #
16) T	DCPA	9.506	0.000	83212964	0	8.342	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
Data File : PS005220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2019 11:12
Operator : SM\AJ
Sample : K3155-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BAT-B06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 12:24:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

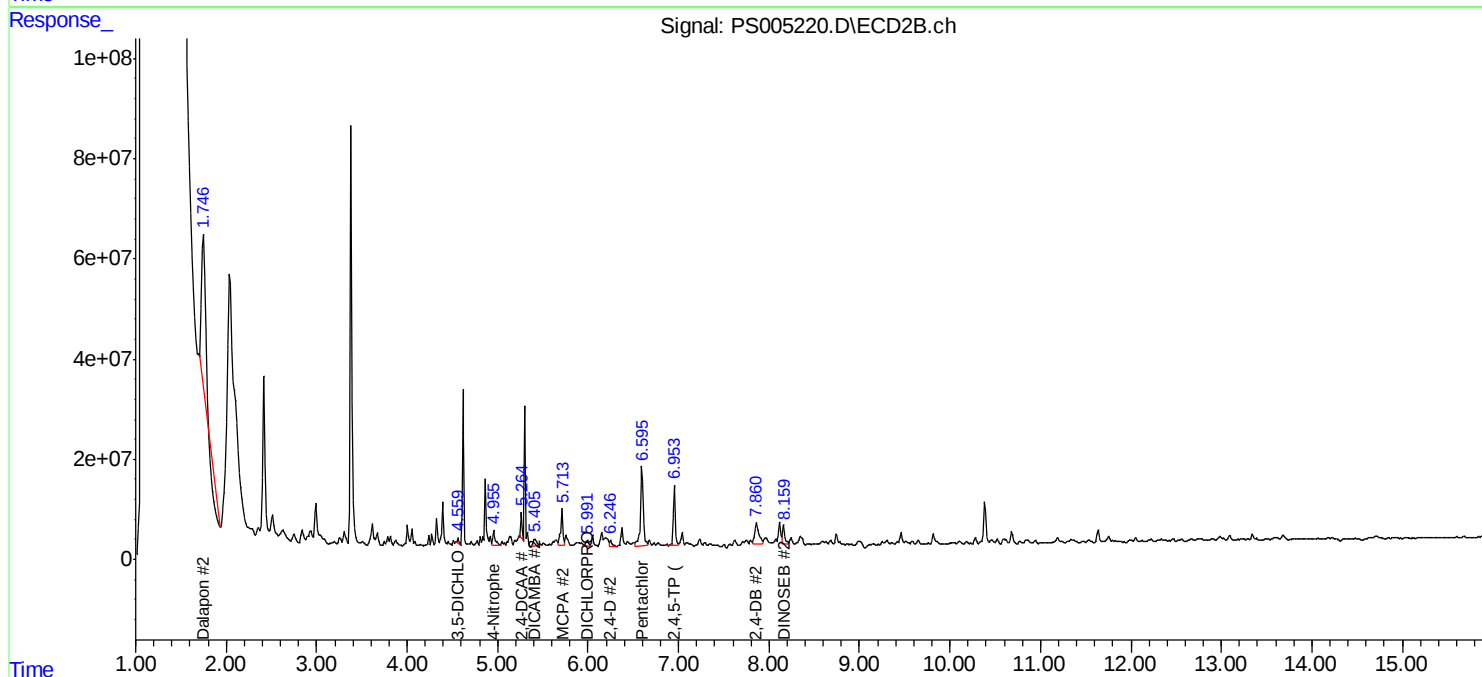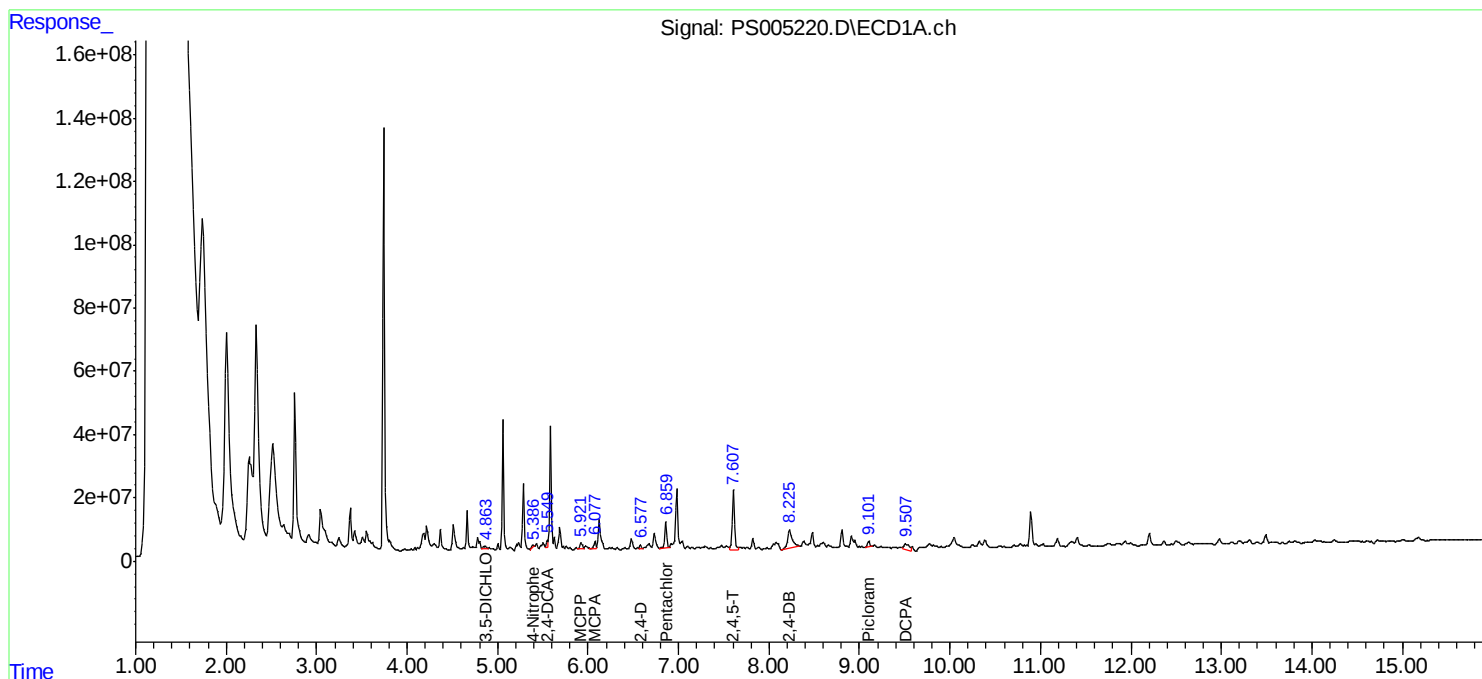


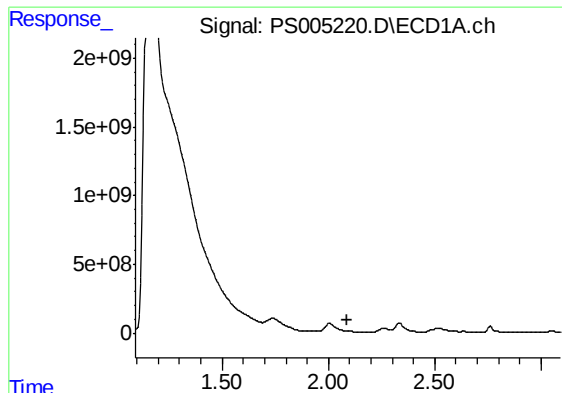

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B06

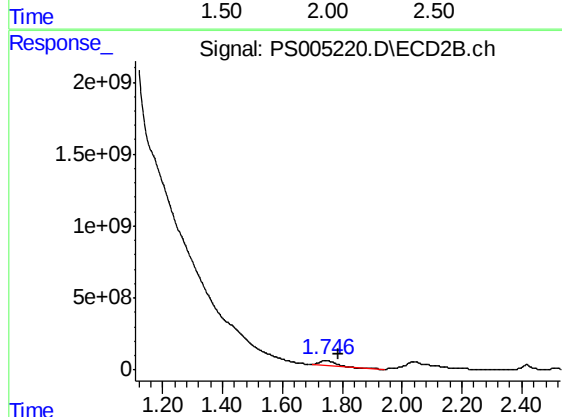


#1 Dalapon

R.T.: 1.746 min
Delta R.T.: -0.042 min
Response: 696887419
Conc: 528.32 ng/ml

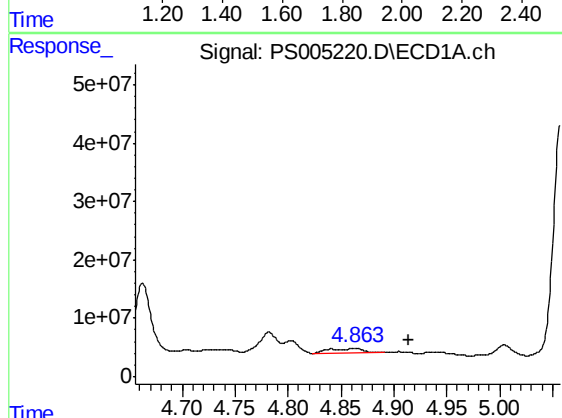


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.863 min
Delta R.T.: -0.051 min
Response: 19364004
Conc: 9.64 ng/ml

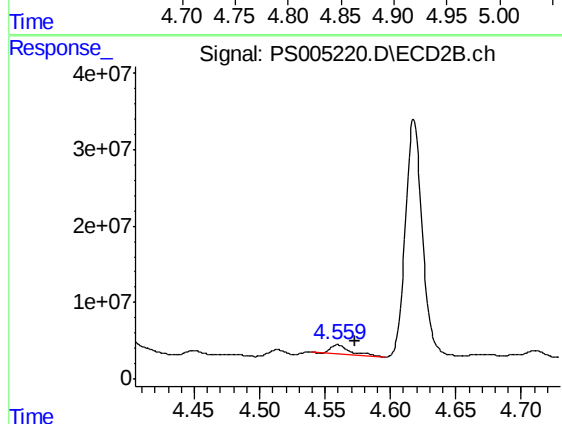

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.560 min
Delta R.T.: -0.013 min
Response: 12136246
Conc: 9.20 ng/ml

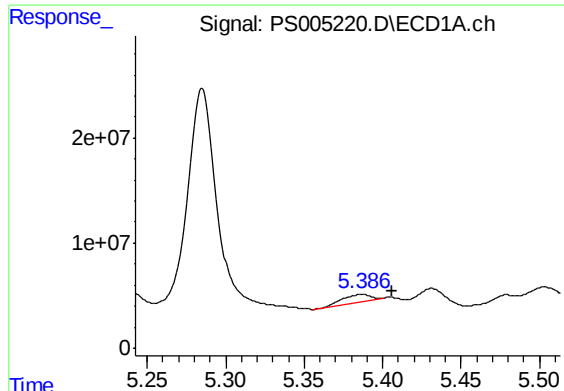

#3 4-Nitrophenol


R.T.: 5.387 min
Delta R.T.: -0.020 min
Response: 8609688
Conc: 11.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B06

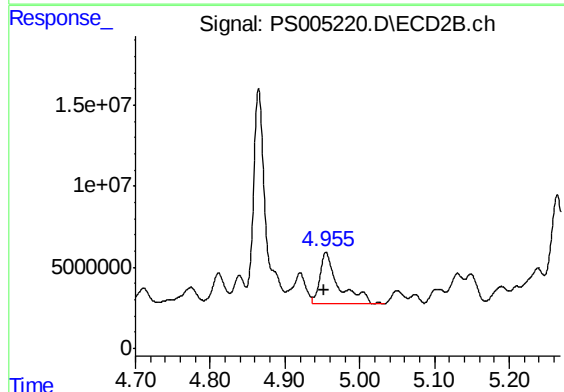


#3 4-Nitrophenol

R.T.: 4.955 min
Delta R.T.: 0.002 min
Response: 54434155
Conc: 108.55 ng/ml

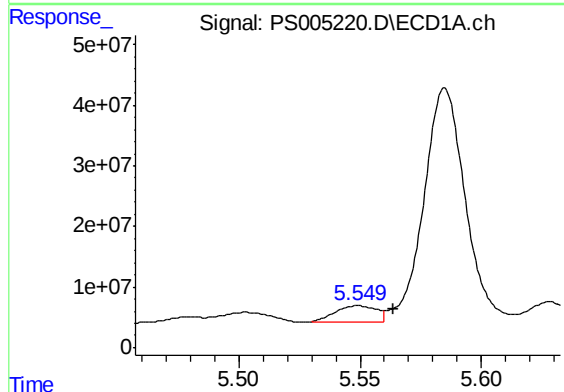


#4 2,4-DCAA

R.T.: 5.549 min
Delta R.T.: -0.014 min
Response: 30697827
Conc: 20.91 ng/ml

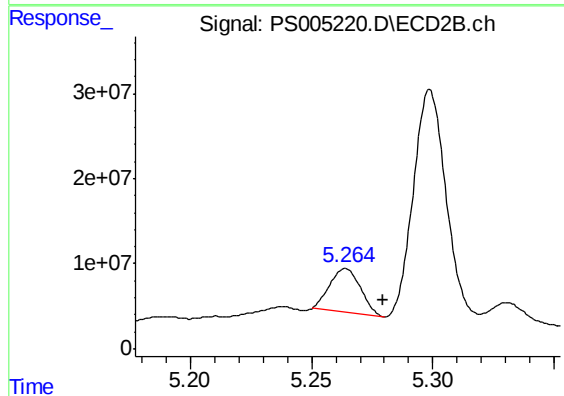

#4 2,4-DCAA


R.T.: 5.264 min
Delta R.T.: -0.016 min
Response: 45572082
Conc: 45.46 ng/ml

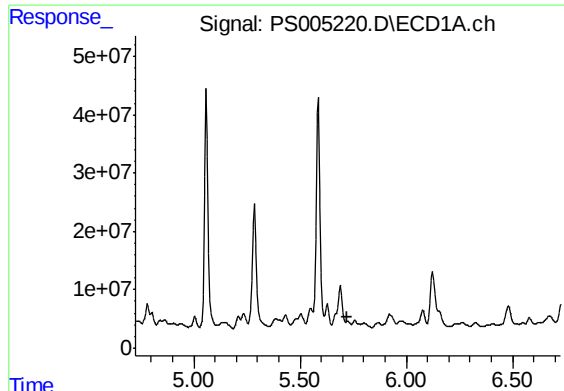

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B06

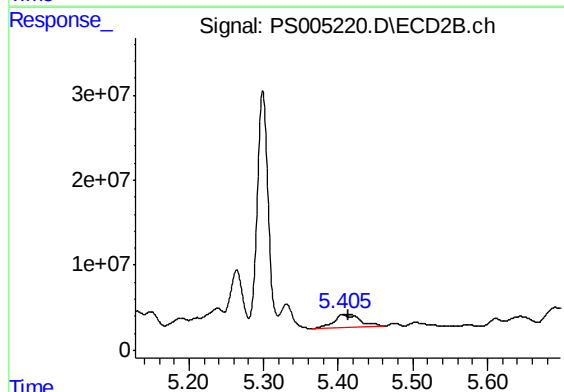


#5 DICAMBA

R.T.: 5.406 min
Delta R.T.: -0.008 min
Response: 37010236
Conc: 9.89 ng/ml

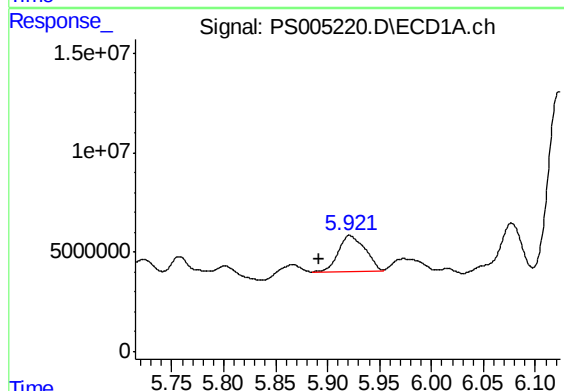


#6 MCPP

R.T.: 5.922 min
Delta R.T.: 0.030 min
Response: 32013151
Conc: 7.31 ug/ml

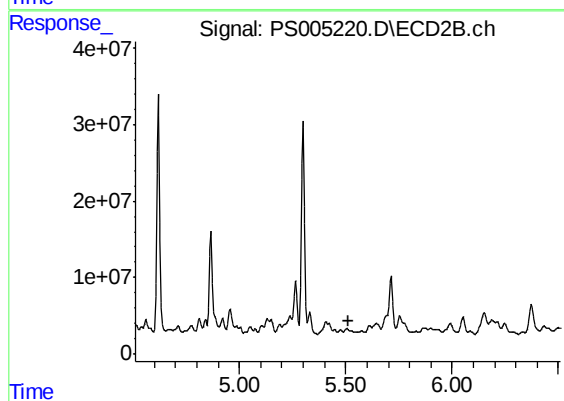

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

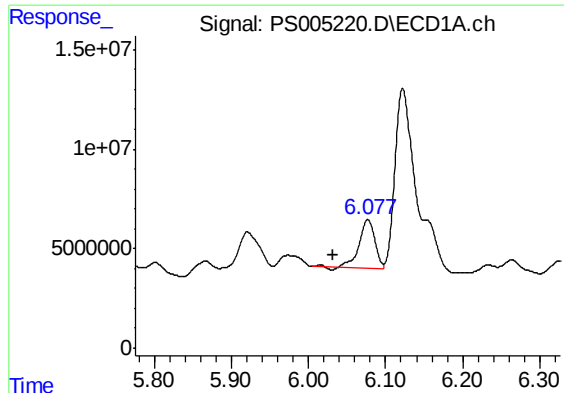

#7 MCPA


R.T.: 6.077 min
Delta R.T.: 0.045 min
Response: 34862698
Conc: 5.55 ug/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B06

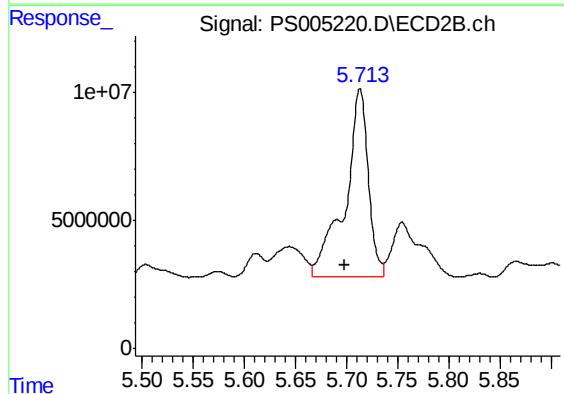


#7 MCPA

R.T.: 5.713 min
Delta R.T.: 0.015 min
Response: 117341888
Conc: 28.97 ug/ml

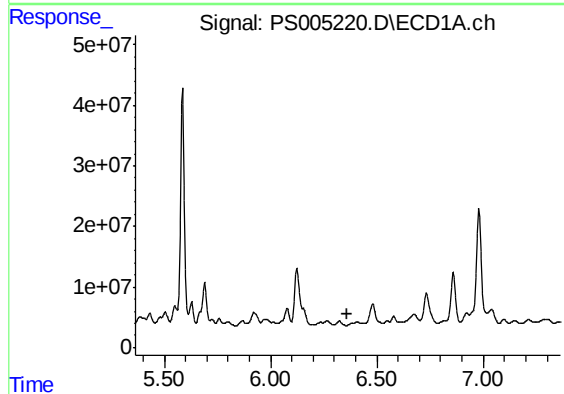


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

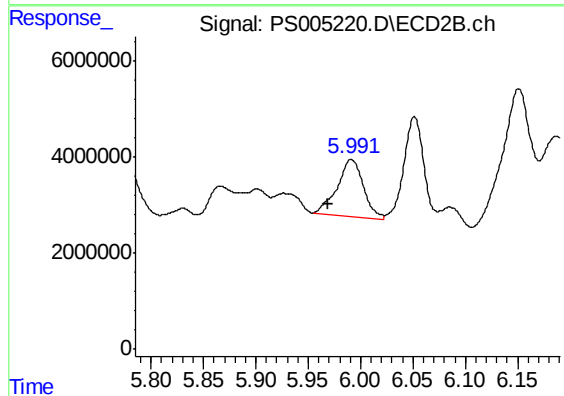

#8 DICHLORPROP


R.T.: 5.991 min
Delta R.T.: 0.022 min
Response: 20539966
Conc: 21.27 ng/ml

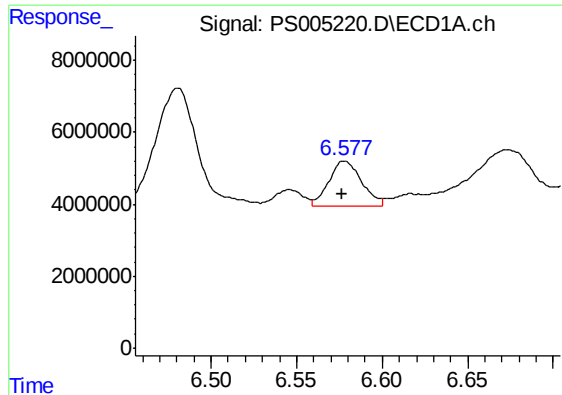

#9 2,4-D


R.T.: 6.578 min
Delta R.T.: 0.002 min
Response: 16873376
Conc: 10.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B06

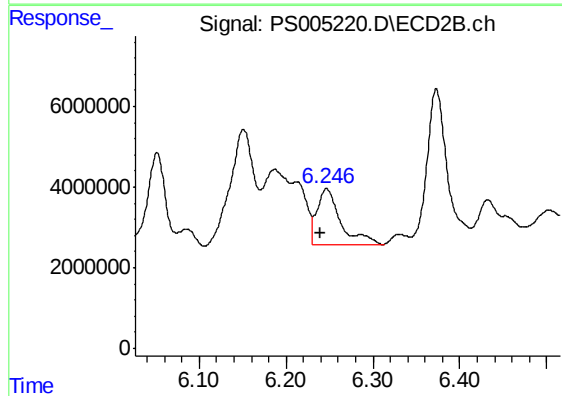


#9 2,4-D

R.T.: 6.247 min
Delta R.T.: 0.007 min
Response: 26417150
Conc: 23.69 ng/ml

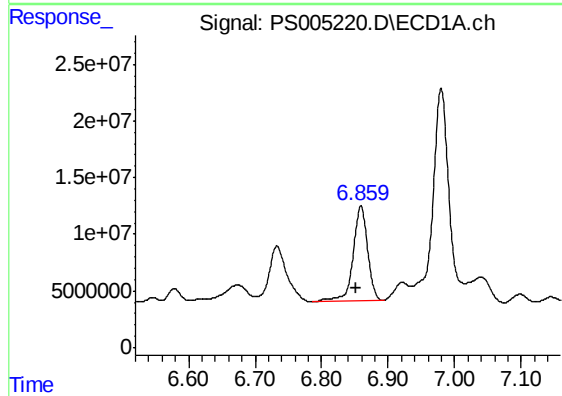


#10 Pentachlorophenol

R.T.: 6.859 min
Delta R.T.: 0.008 min
Response: 127631635
Conc: 6.49 ng/ml

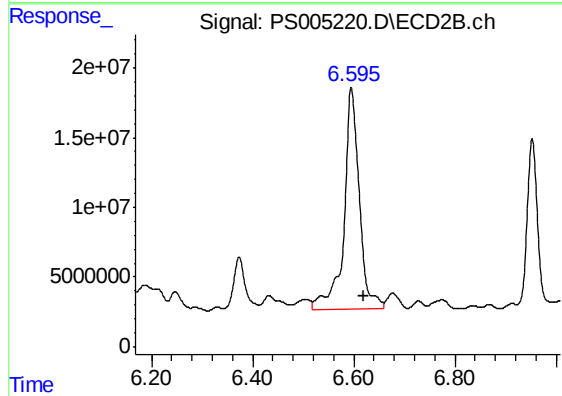

#10 Pentachlorophenol


R.T.: 6.595 min
Delta R.T.: -0.024 min
Response: 338832215
Conc: 26.36 ng/ml

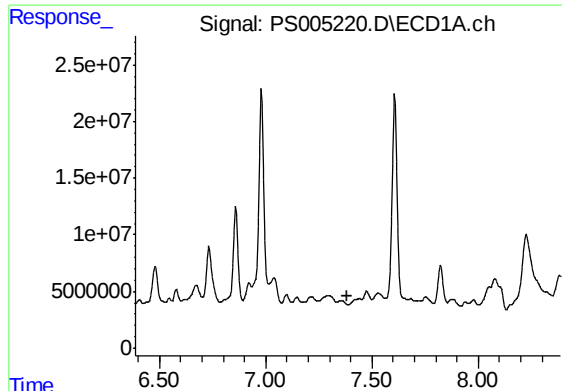

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B06

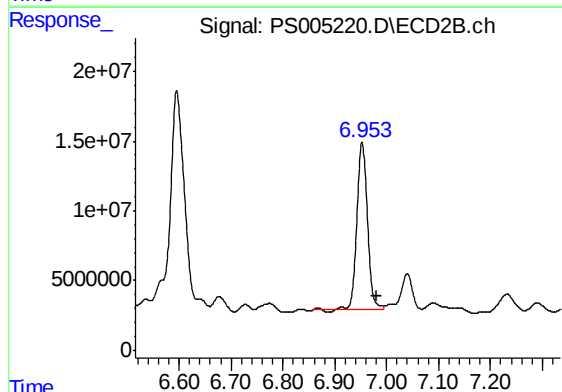


#11 2,4,5-TP (SILVEX)

R.T.: 6.953 min
Delta R.T.: -0.028 min
Response: 165125943
Conc: 31.01 ng/ml

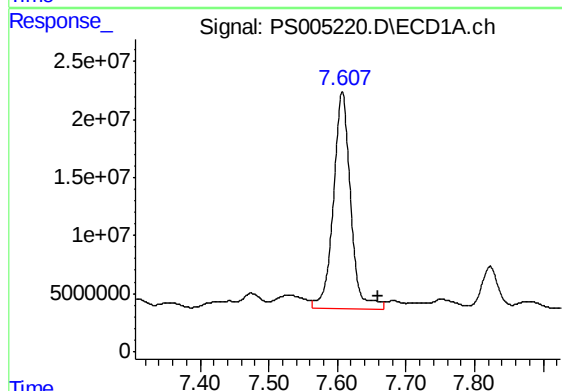


#12 2,4,5-T

R.T.: 7.607 min
Delta R.T.: -0.051 min
Response: 326577180
Conc: 40.58 ng/ml

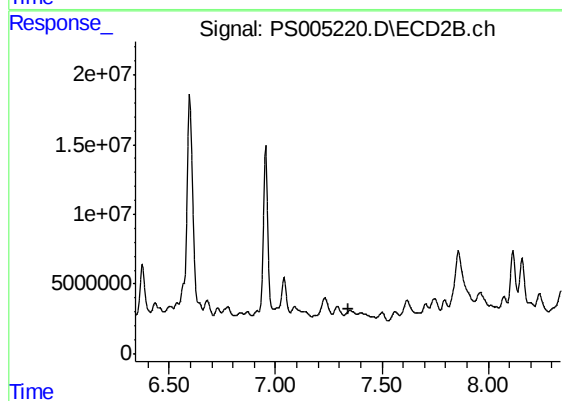

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

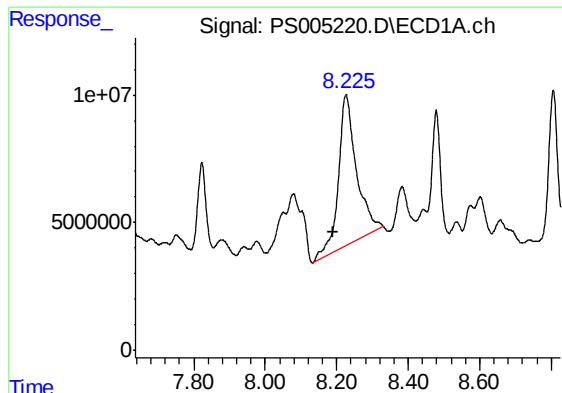

#13 2,4-DB


R.T.: 8.226 min
Delta R.T.: 0.036 min
Response: 209968952
Conc: 180.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B06

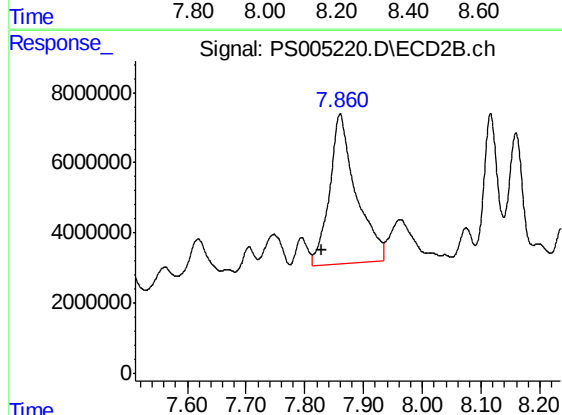


#13 2,4-DB

R.T.: 7.860 min
Delta R.T.: 0.030 min
Response: 133351554
Conc: 204.26 ng/ml

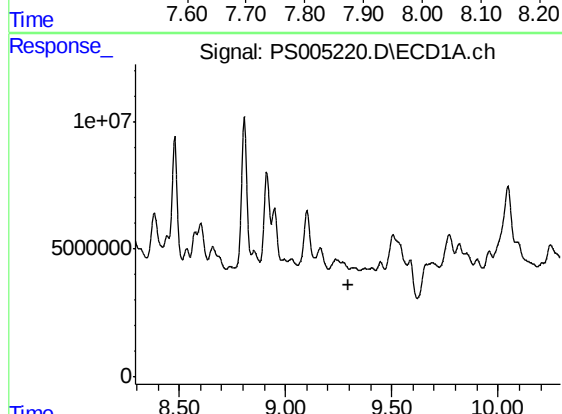


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

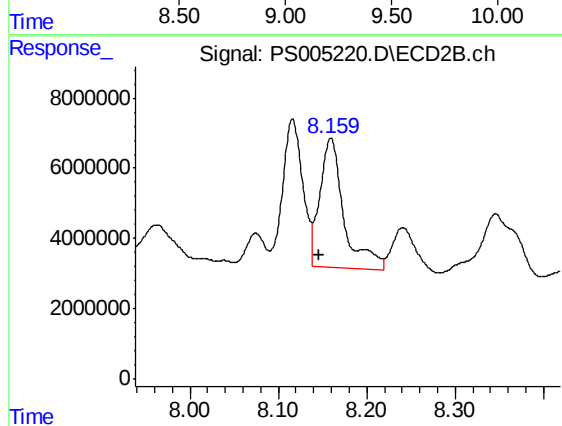

#14 DINOSEB


R.T.: 8.159 min
Delta R.T.: 0.013 min
Response: 69741773
Conc: 17.25 ng/ml

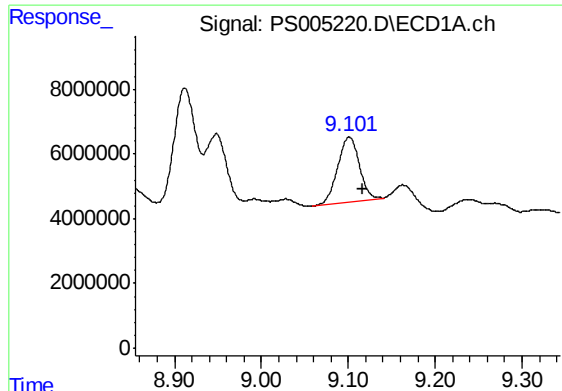

#15 Picloram


R.T.: 9.101 min
Delta R.T.: -0.015 min
Response: 35000465
Conc: 3.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B06

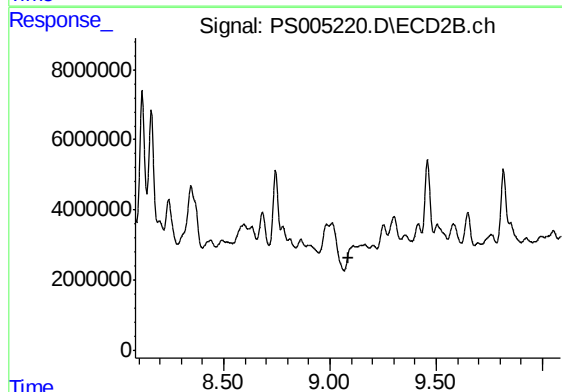


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.

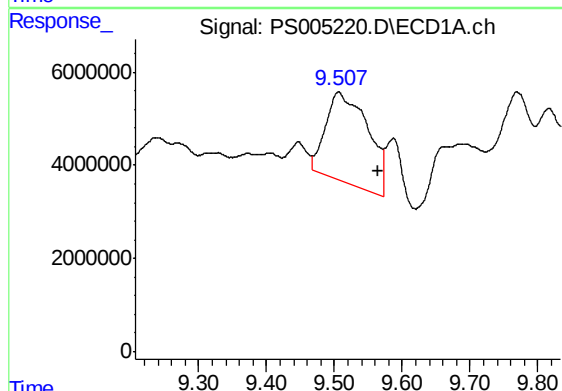

#16 DCPA

R.T.: 9.506 min
Delta R.T.: -0.059 min
Response: 83212964
Conc: 8.34 ng/ml

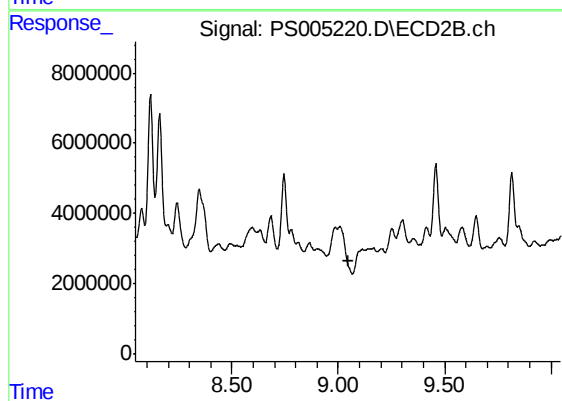

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.046 min
Response: 0
Conc: N.D.