

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
 Data File : PS005235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2019 16:42
 Operator : SM\AJ
 Sample : K3511-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 17:14:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.590	5.304	320.4E6	201.8E6	218.295	201.366
Target Compounds							
1) T	Dalapon	2.093	1.782	70618851	10480430	38.311	7.945 #
2) T	3,5-DICHL...	4.955	4.581	9143227	9168593	4.550	6.953 #
5) T	DICAMBA	0.000	5.457	0	15163020	N.D.	4.051
6) T	MCP	0.000	5.457	0	15163020	N.D.	5.444
9) T	2,4-D	0.000	6.252	0	11729966	N.D.	10.517
10) T	Pentachlo...	0.000	6.569	0	17957827	N.D.	1.397
11) T	2,4,5-TP ...	0.000	6.958	0	100.7E6	N.D.	18.911
12) T	2,4,5-T	7.613	0.000	178.7E6	0	22.203	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
Data File : PS005235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2019 16:42
Operator : SM\AJ
Sample : K3511-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 17:14:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

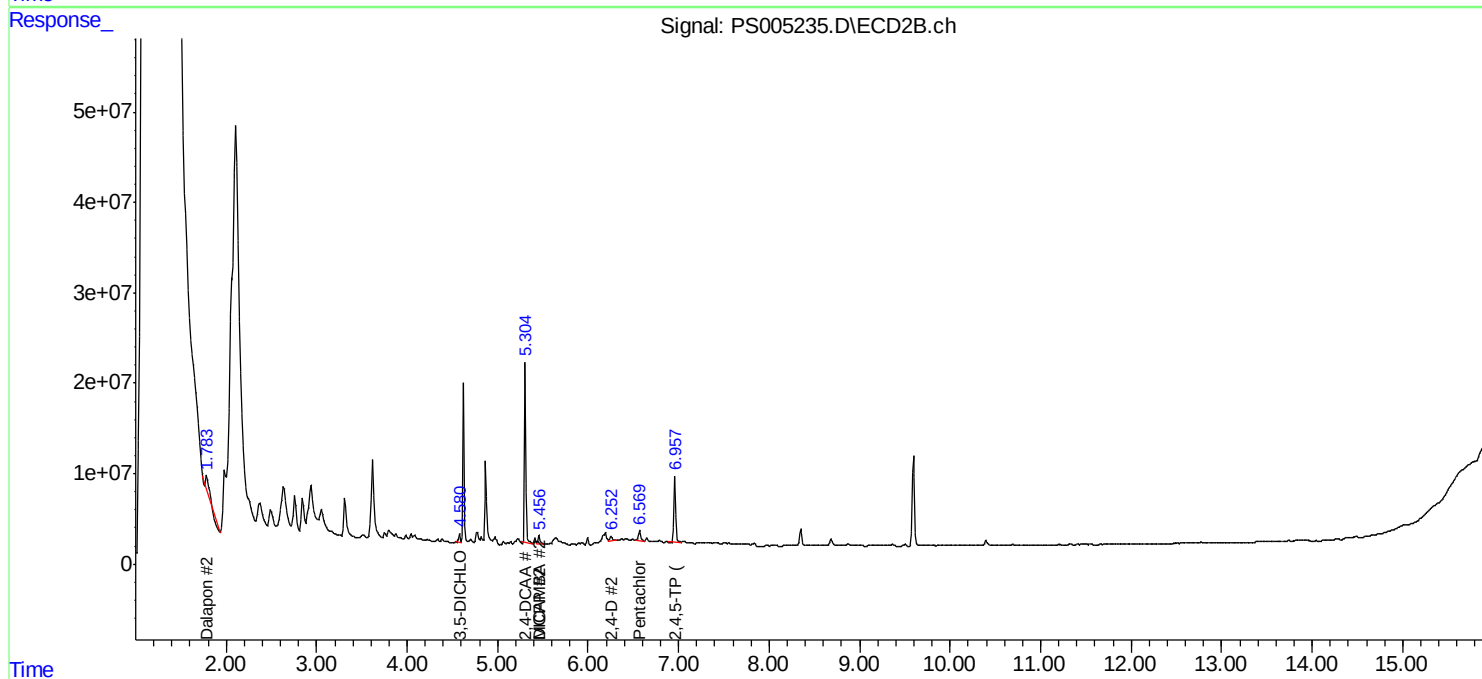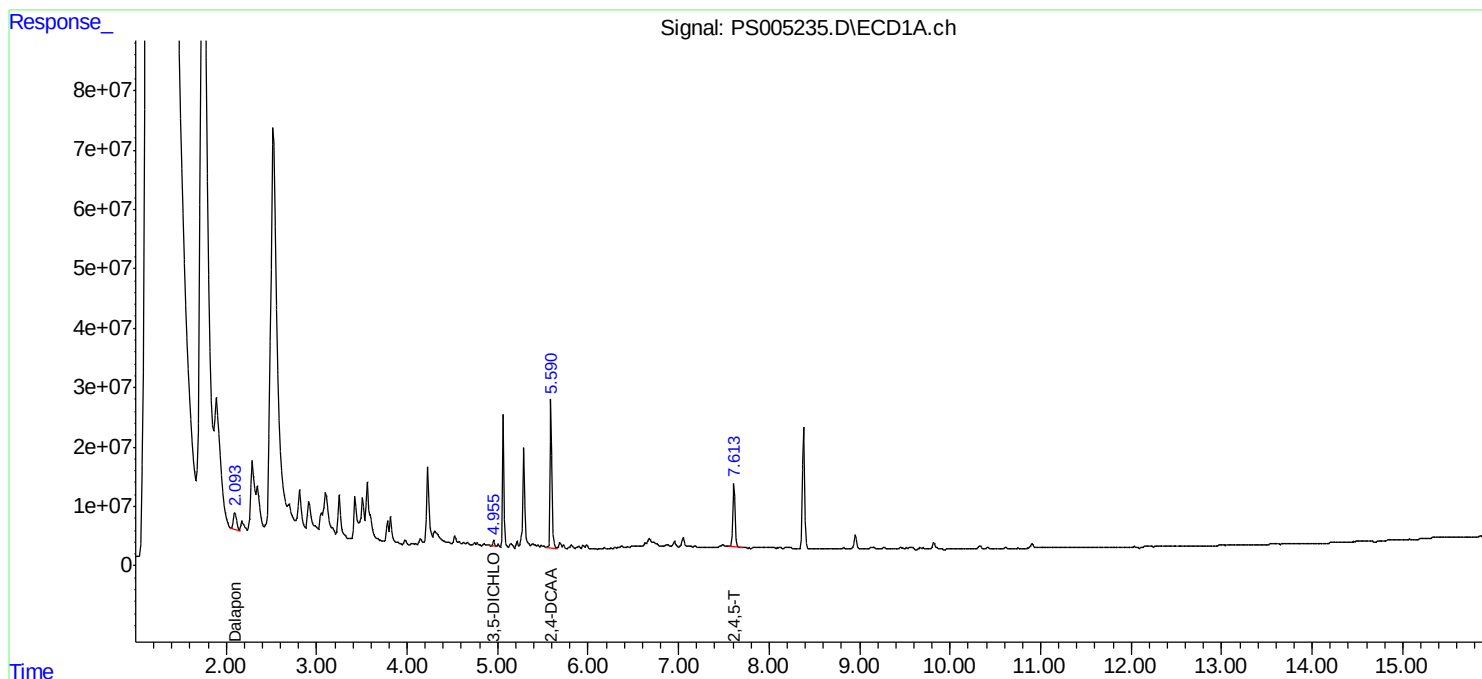


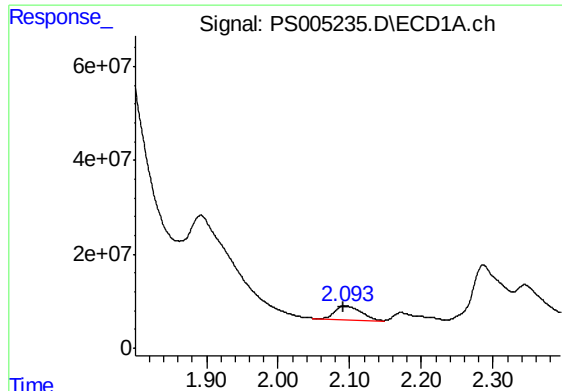

#1 Dalapon


R.T.: 2.093 min
Delta R.T.: 0.000 min
Response: 70618851
Conc: 38.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-2

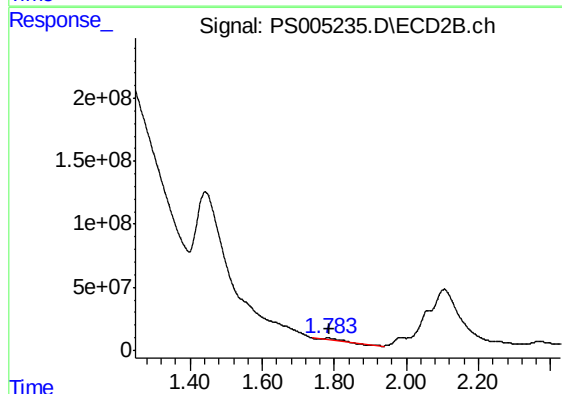


#1 Dalapon

R.T.: 1.782 min
Delta R.T.: -0.006 min
Response: 10480430
Conc: 7.95 ng/ml

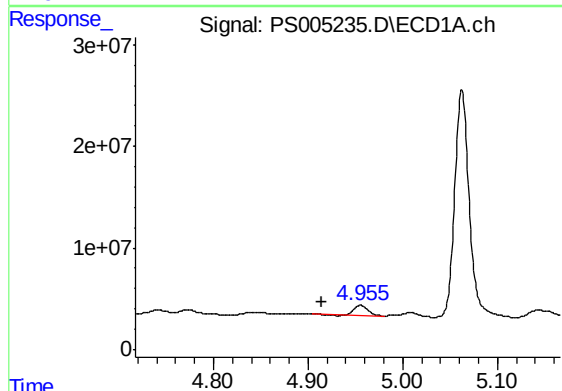


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.955 min
Delta R.T.: 0.041 min
Response: 9143227
Conc: 4.55 ng/ml

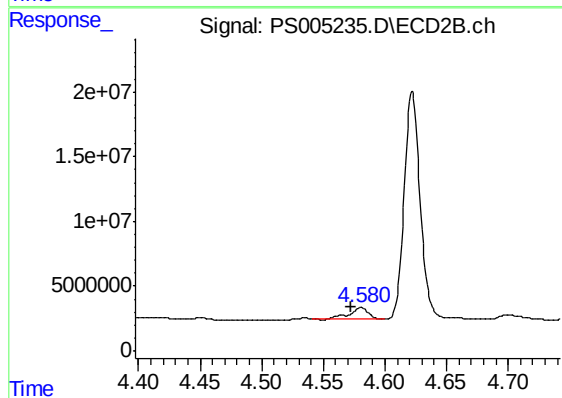

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.581 min
Delta R.T.: 0.008 min
Response: 9168593
Conc: 6.95 ng/ml

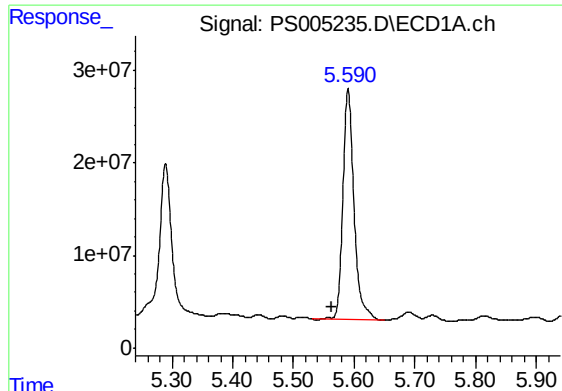

#4 2,4-DCAA


R.T.: 5.590 min
Delta R.T.: 0.026 min
Response: 320433218
Conc: 218.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-2

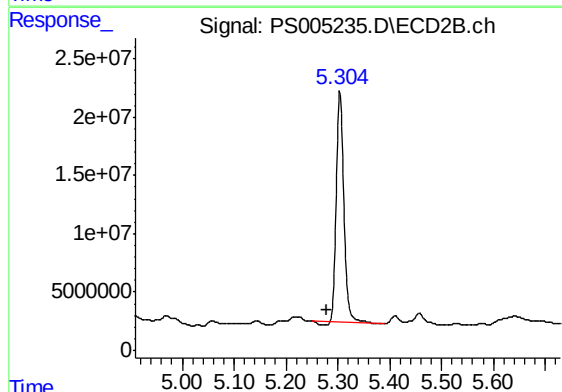


#4 2,4-DCAA

R.T.: 5.304 min
Delta R.T.: 0.024 min
Response: 201842564
Conc: 201.37 ng/ml

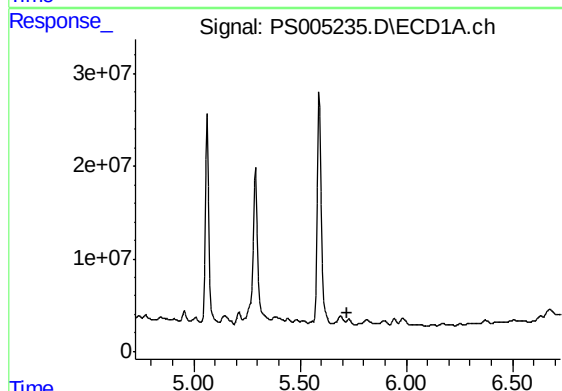


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

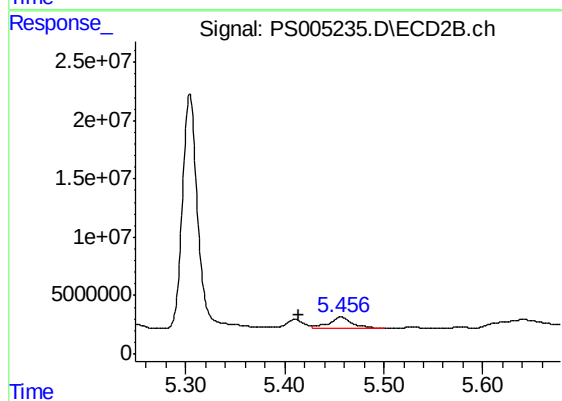

#5 DICAMBA


R.T.: 5.457 min
Delta R.T.: 0.043 min
Response: 15163020
Conc: 4.05 ng/ml

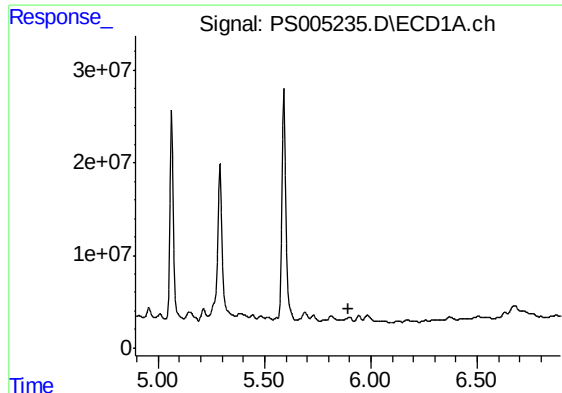

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.892 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-2

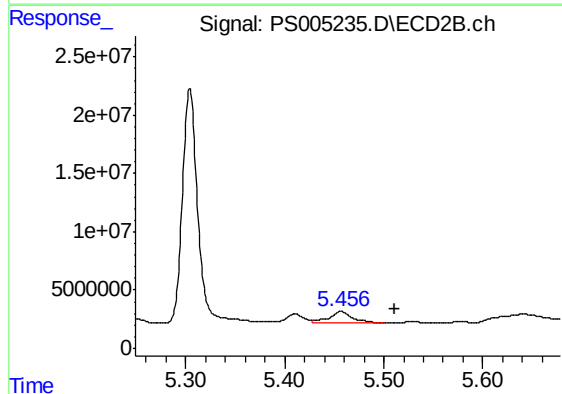


#6 MCP

R.T.: 5.457 min
Delta R.T.: -0.054 min
Response: 15163020
Conc: 5.44 ug/ml

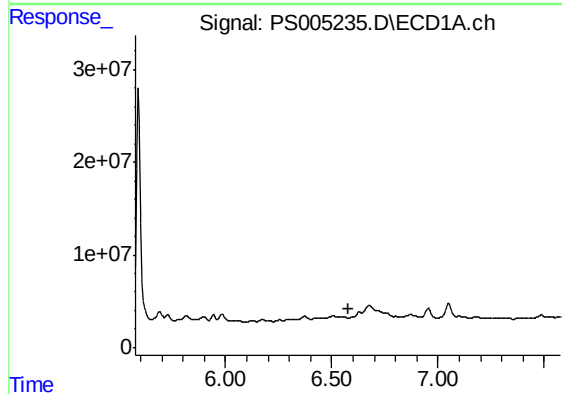


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

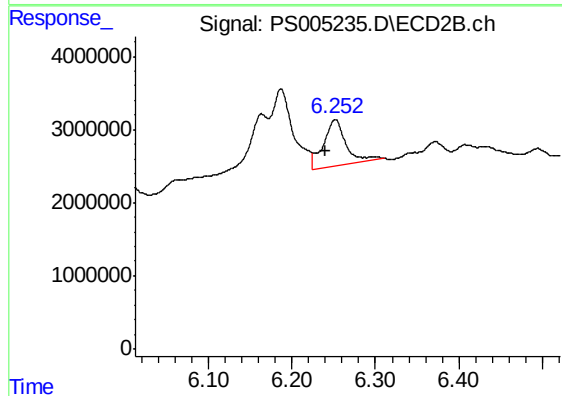

#9 2,4-D


R.T.: 6.252 min
Delta R.T.: 0.012 min
Response: 11729966
Conc: 10.52 ng/ml

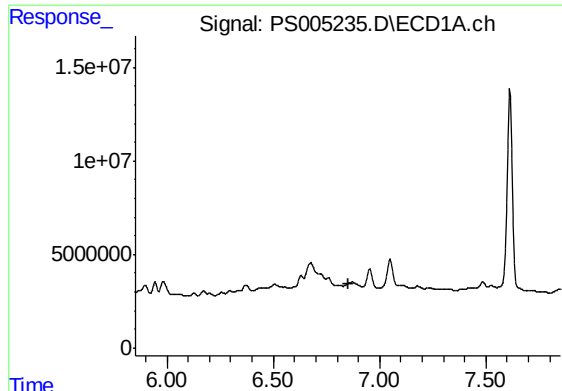

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-2

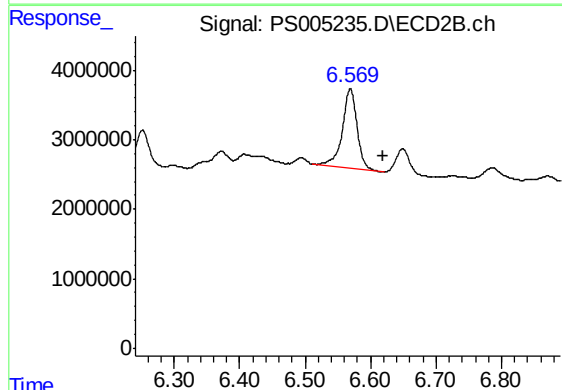


#10 Pentachlorophenol

R.T.: 6.569 min
Delta R.T.: -0.050 min
Response: 17957827
Conc: 1.40 ng/ml

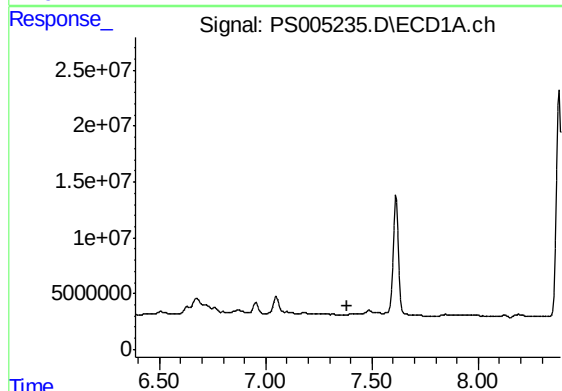


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

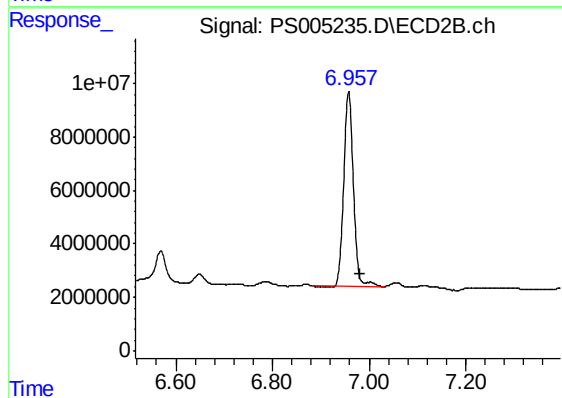

#11 2,4,5-TP (SILVEX)


R.T.: 6.958 min
Delta R.T.: -0.023 min
Response: 100705796
Conc: 18.91 ng/ml

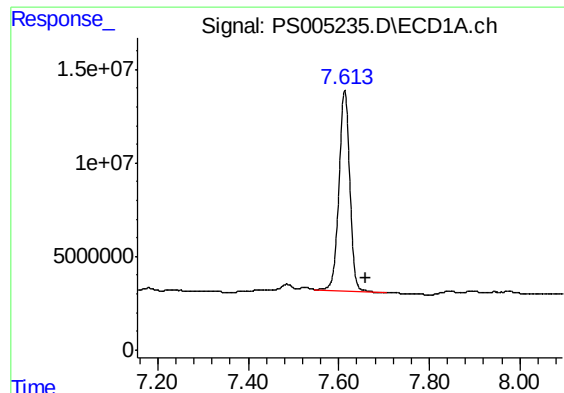

#12 2,4,5-T

R.T.: 7.613 min
Delta R.T.: -0.046 min
Response: 178688489
Conc: 22.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-2

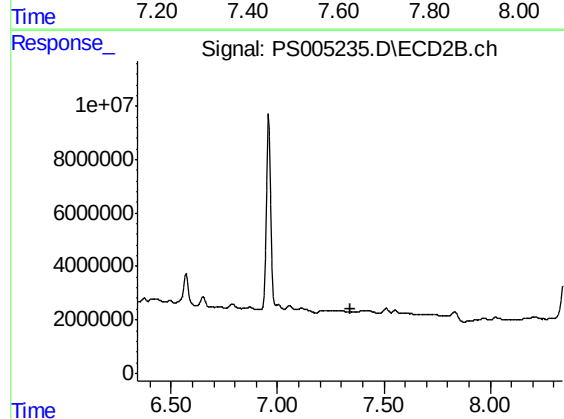

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.