

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
 Data File : PS005220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2019 11:12
 Operator : SM\AJ
 Sample : K3155-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BAT-B06

Manual Integrations
 APPROVED

Ankita
 6/27/2019 9:11:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 13:50:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.584	5.298	456.9E6	270.6E6	311.296m	269.912m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062619\
Data File : PS005220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2019 11:12
Operator : SM\AJ
Sample : K3155-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
BAT-B06


Manual Integrations
APPROVED

Ankita
6/27/2019 9:11:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 13:50:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

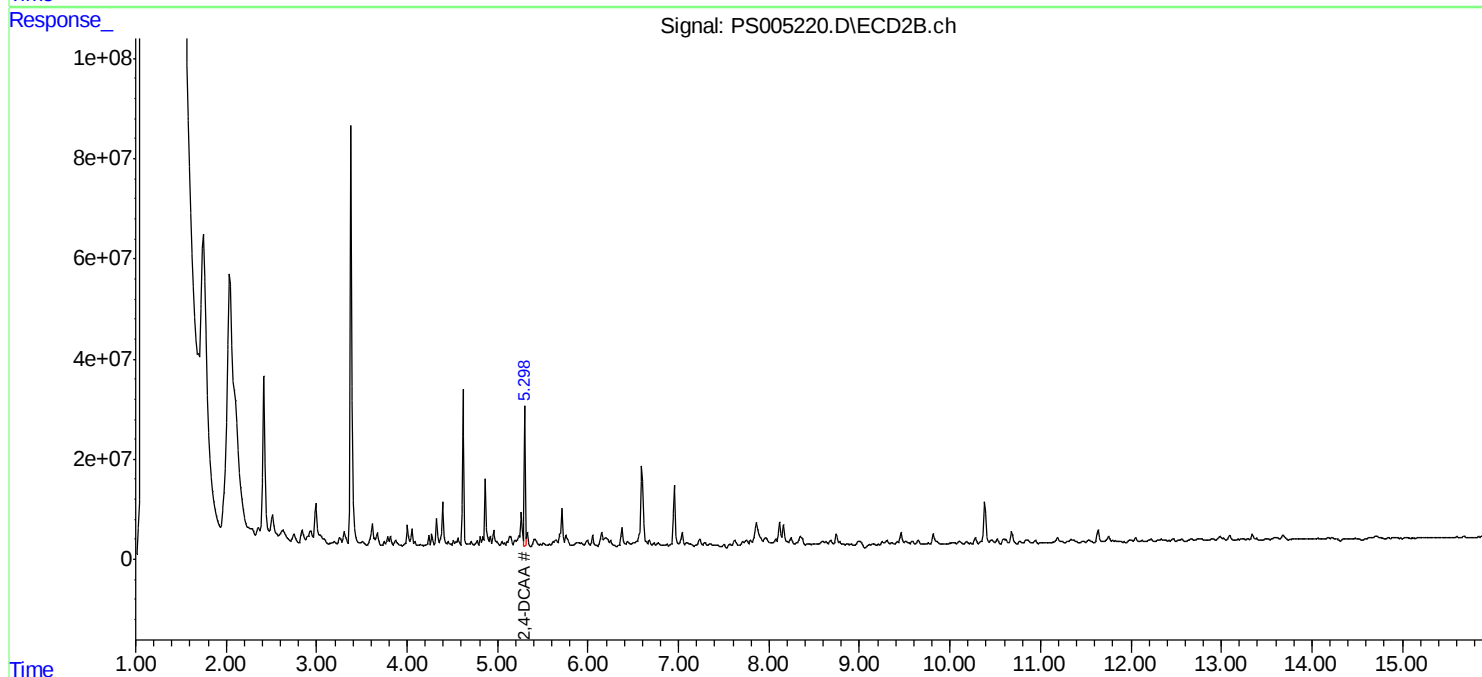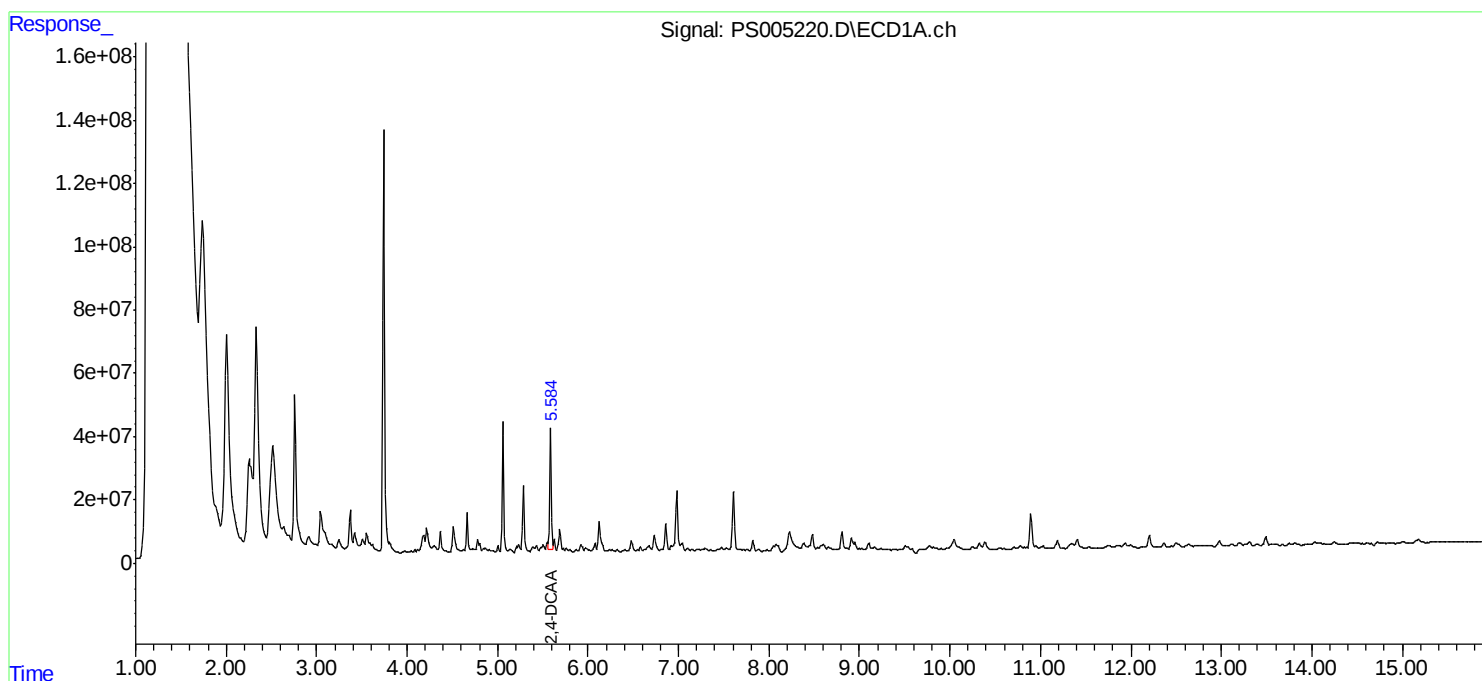

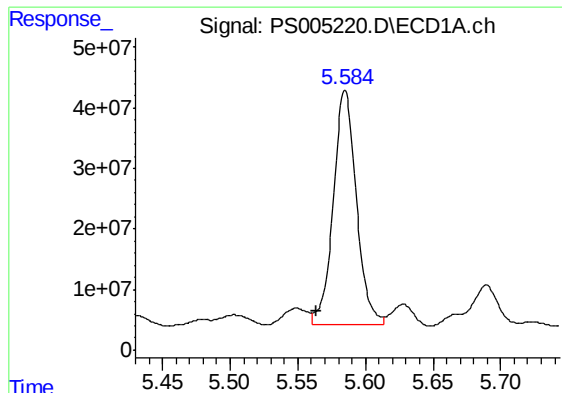


#4 2,4-DCAA

R.T.: 5.584 min
Delta R.T.: 0.021 min
Response: 456949625
Conc: 311.30 ng/ml m

Instrument :
ECD_S
ClientSampleId :
BAT-B06

Manual Integrations
APPROVED

Ankita
6/27/2019 9:11:48 AM

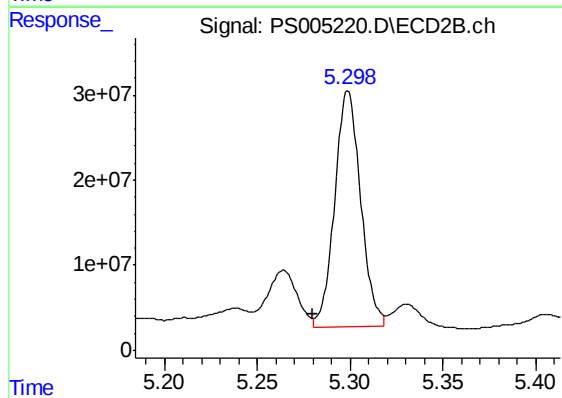

#4 2,4-DCAA

R.T.: 5.298 min
Delta R.T.: 0.019 min
Response: 270551670
Conc: 269.91 ng/ml m