

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
 Data File : PS010969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2020 19:20
 Operator : DD\AJ
 Sample : PB129801BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB129801BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 04:00:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.919	421.7E6	290.1E6	465.012	523.606
Target Compounds							
1) T	Dalapon	2.994	2.585	38938104	133.9E6	34.775	177.466 #
2) T	3,5-DICHL...	0.000	6.100	0	20741938	N.D.	24.906
7) T	MCPA	7.721	7.384	8903669	40308771	2.236	14.605 #
8) T	DICHLORPROP	0.000	7.739	0	6405112	N.D.	10.909
10) T	Pentachlo...	8.710	0.000	7876187	0	<MDL	N.D. #
12) T	2,4,5-T	9.509	0.000	5974069	0	1.283	N.D. #
13) T	2,4-DB	9.995	0.000	21801970	0	36.683	N.D. #
14) T	DINOSEB	11.168	10.036	9947713	6088051	2.778	2.924
15) T	Picloram	10.993	0.000	64522516	0	11.509	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
Data File : PS010969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2020 19:20
Operator : DD\AJ
Sample : PB129801BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
PB129801BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:00:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

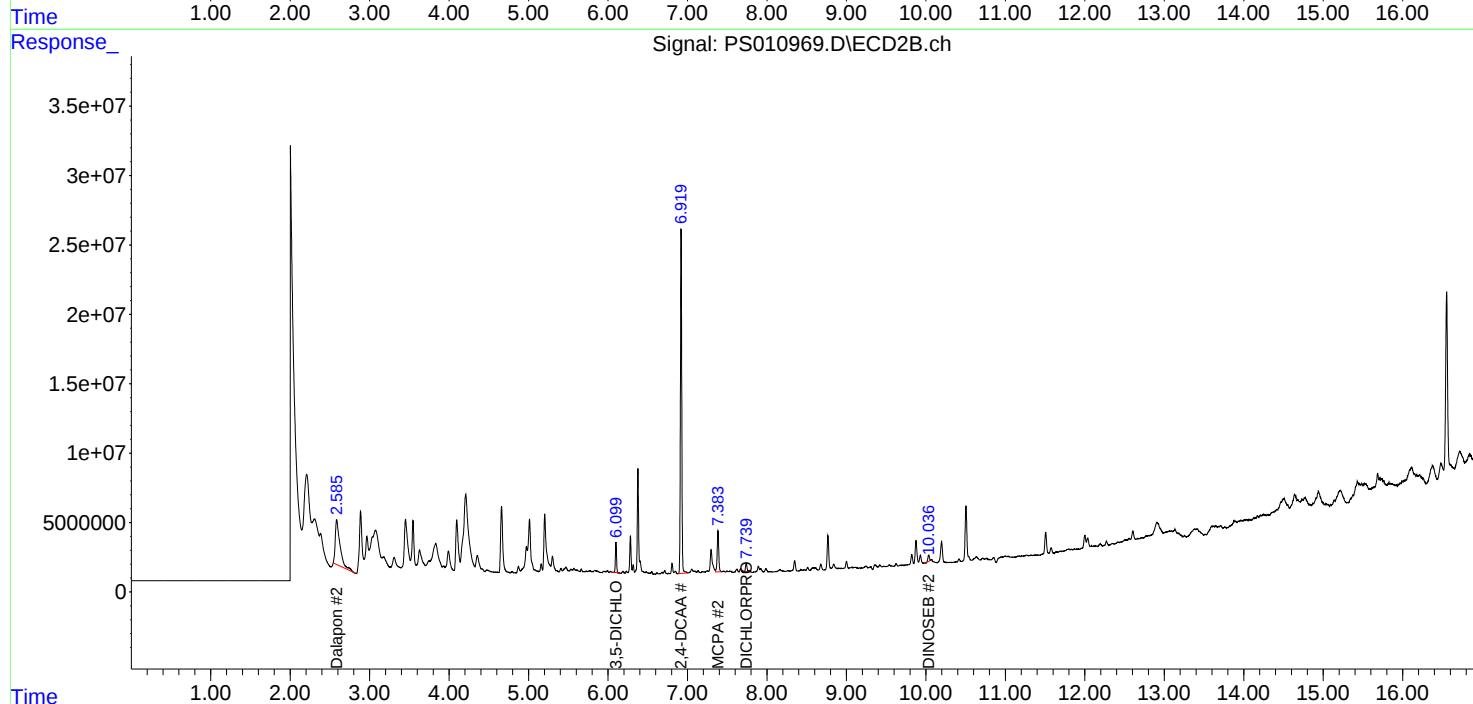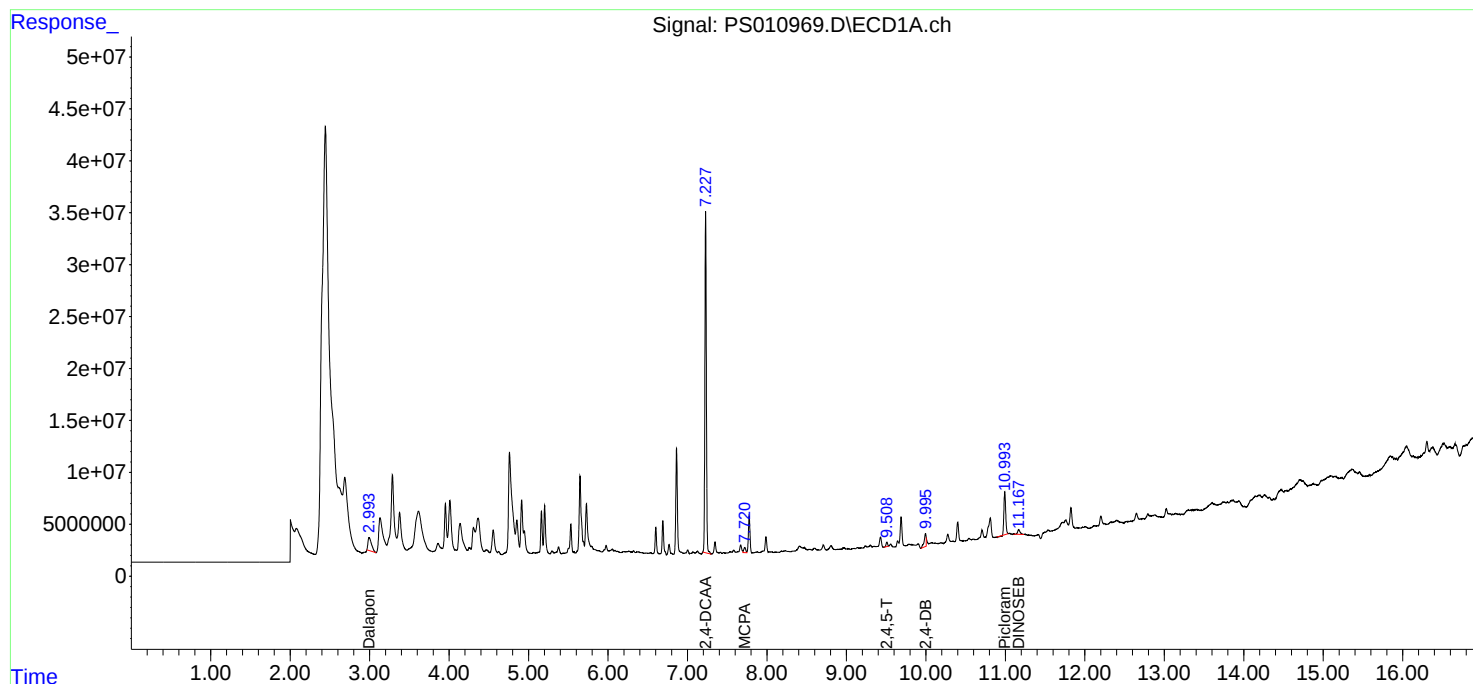


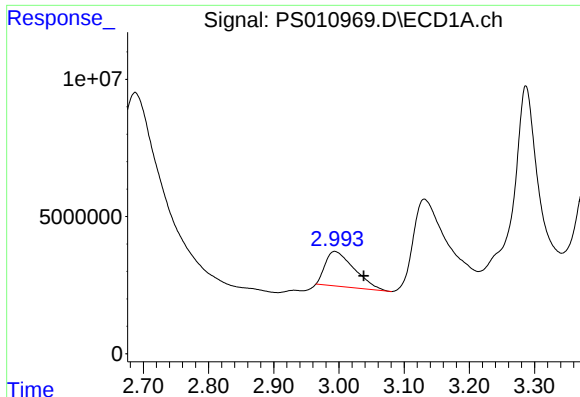

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.044 min
Response: 38938104
Conc: 34.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129801BL

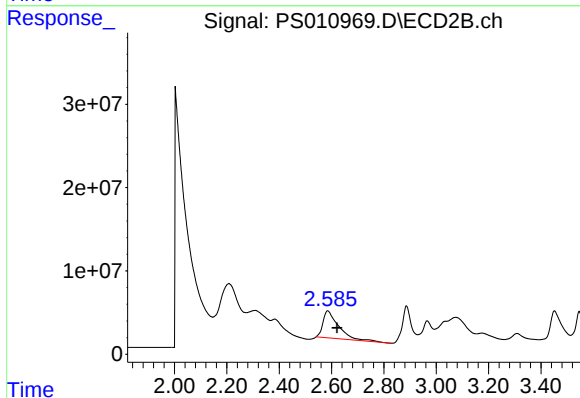


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.037 min
Response: 133873557
Conc: 177.47 ng/ml

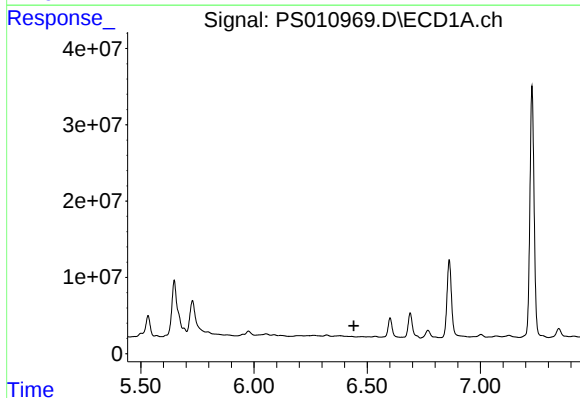


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

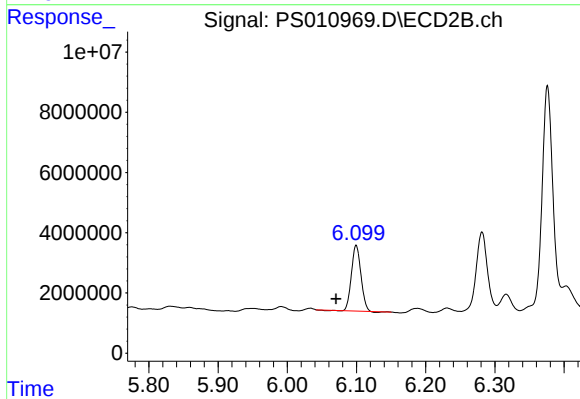

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 20741938
Conc: 24.91 ng/ml

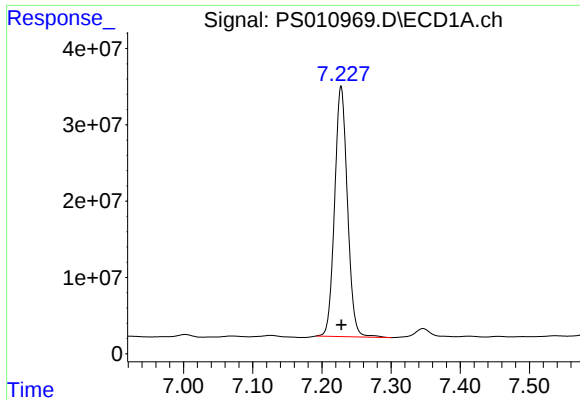

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 421681056
Conc: 465.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129801BL

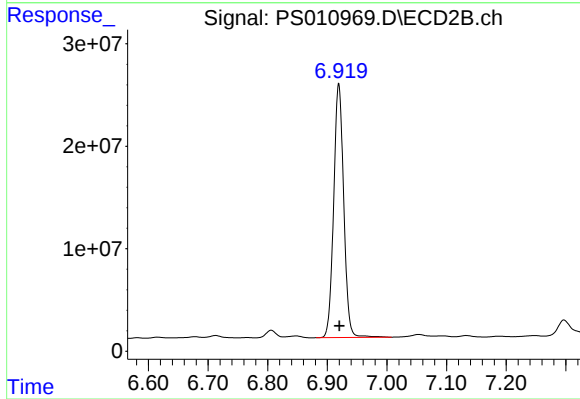


#4 2,4-DCAA

R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 290117791
Conc: 523.61 ng/ml

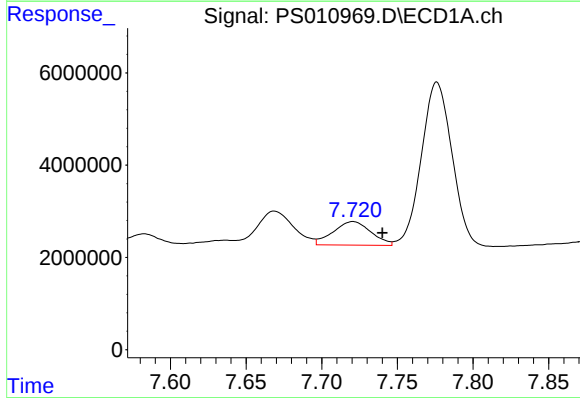


#7 MCPA

R.T.: 7.721 min
Delta R.T.: -0.020 min
Response: 8903669
Conc: 2.24 ug/ml

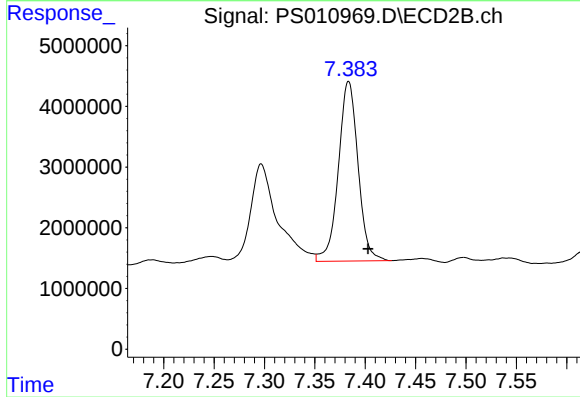

#7 MCPA


R.T.: 7.384 min
Delta R.T.: -0.019 min
Response: 40308771
Conc: 14.60 ug/ml

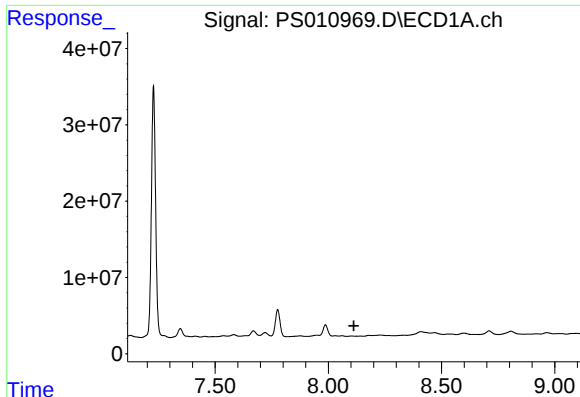

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB129801BL

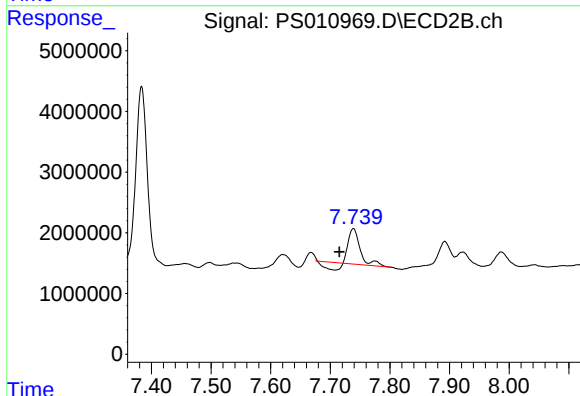


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.024 min
Response: 6405112
Conc: 10.91 ng/ml

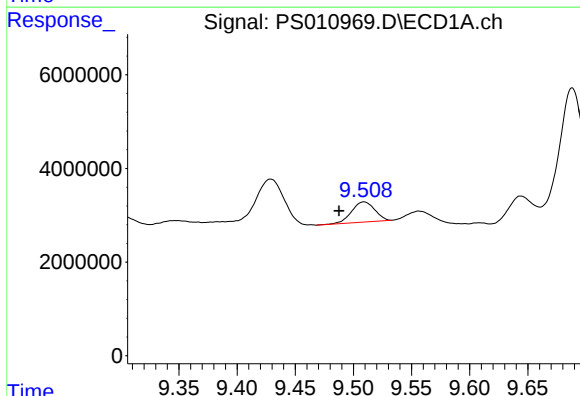


#12 2,4,5-T

R.T.: 9.509 min
Delta R.T.: 0.021 min
Response: 5974069
Conc: 1.28 ng/ml

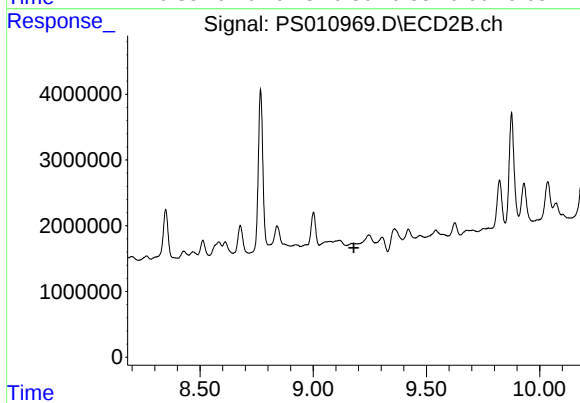

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

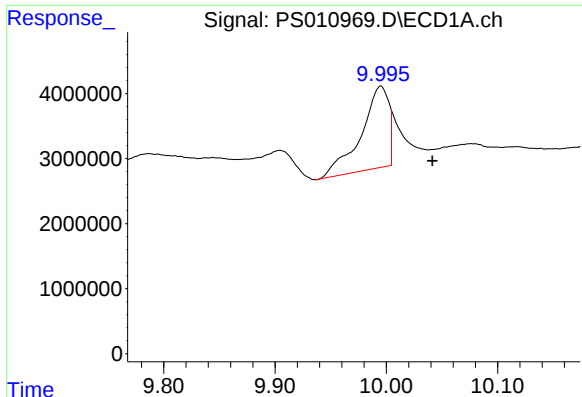

#13 2,4-DB


R.T.: 9.995 min
Delta R.T.: -0.046 min
Response: 21801970
Conc: 36.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129801BL

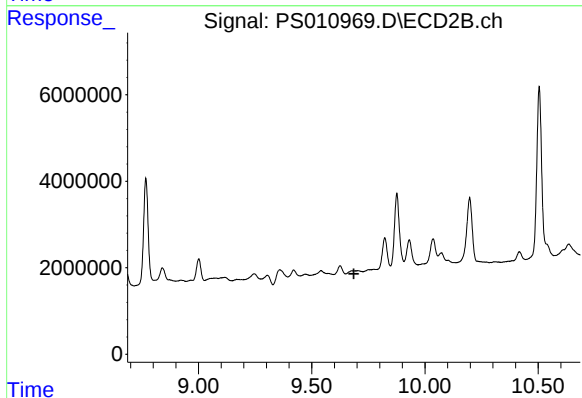


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.686 min
Response: 0
Conc: N.D.

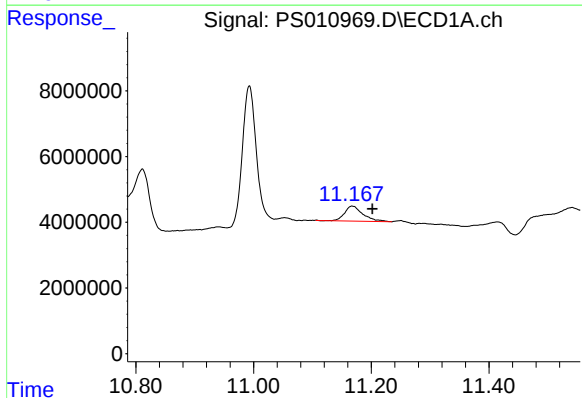


#14 DINOSEB

R.T.: 11.168 min
Delta R.T.: -0.034 min
Response: 9947713
Conc: 2.78 ng/ml

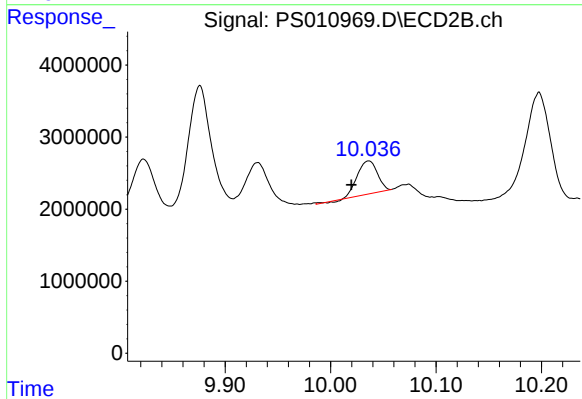

#14 DINOSEB


R.T.: 10.036 min
Delta R.T.: 0.016 min
Response: 6088051
Conc: 2.92 ng/ml

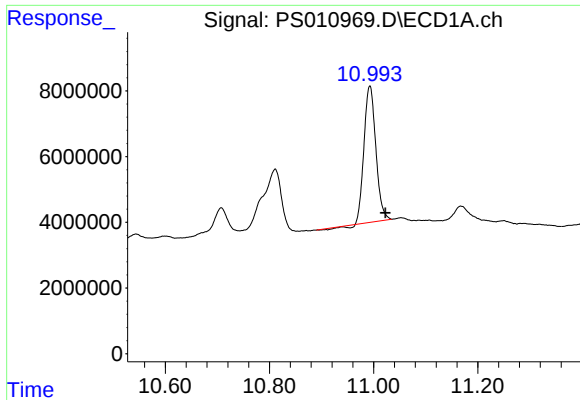

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.030 min
Response: 64522516
Conc: 11.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129801BL

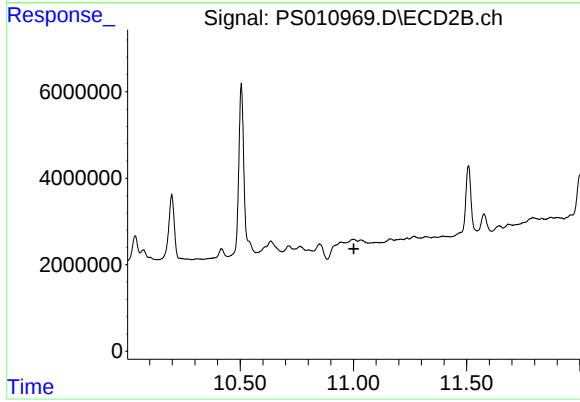

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.