

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
 Data File : PS010971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2020 20:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 04:01:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	400.5E6	278.4E6	441.629	502.496
Target Compounds							
9) T	2,4-D	0.000	7.944	0	12016265	N.D.	16.628
10) T	Pentachlo...	8.653	8.439	8099901	6214911	<MDL	<MDL #
12) T	2,4,5-T	9.490	9.182	8693447	7162331	1.866	2.405 #
15) T	Picloram	11.026	11.005	101.8E6	93248192	18.157	22.257
16) T	DCPA	11.467	10.948	7608994	6270298	1.245	1.684 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
Data File : PS010971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2020 20:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:01:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

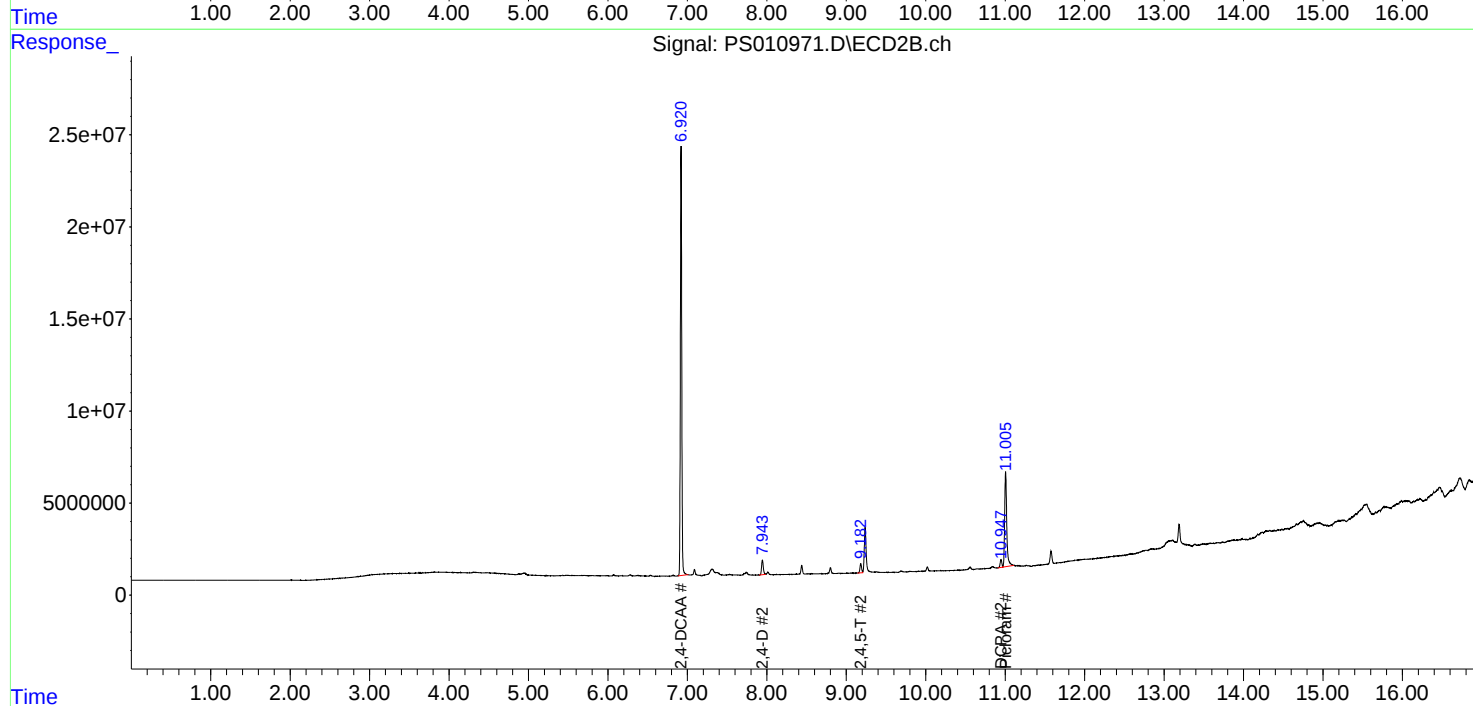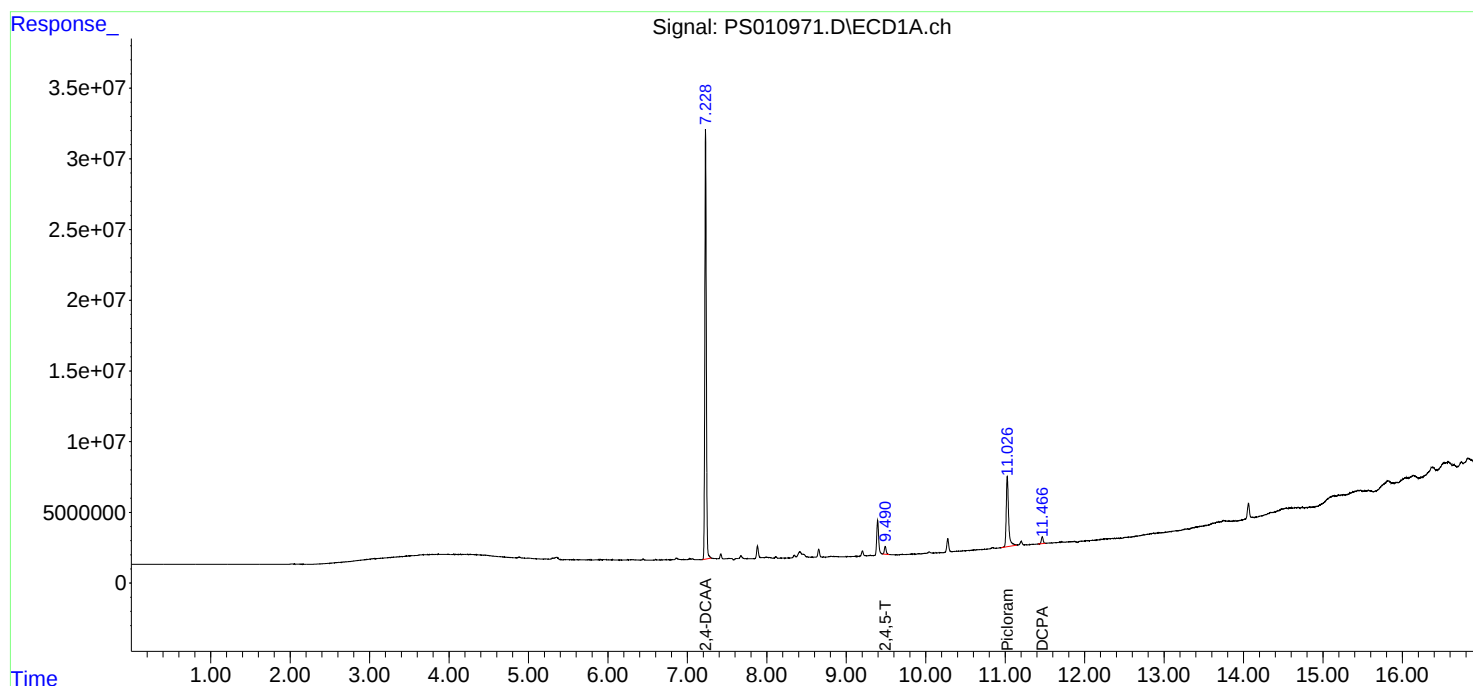


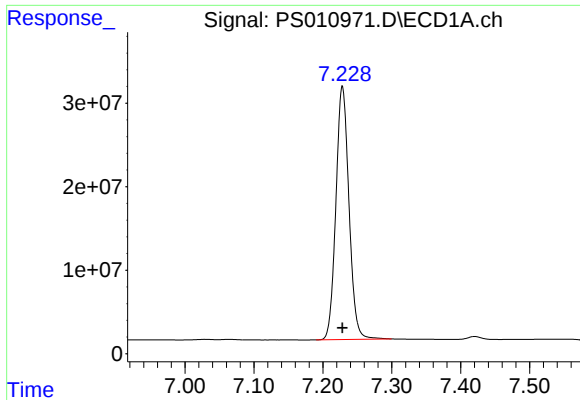

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 400477278
Conc: 441.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

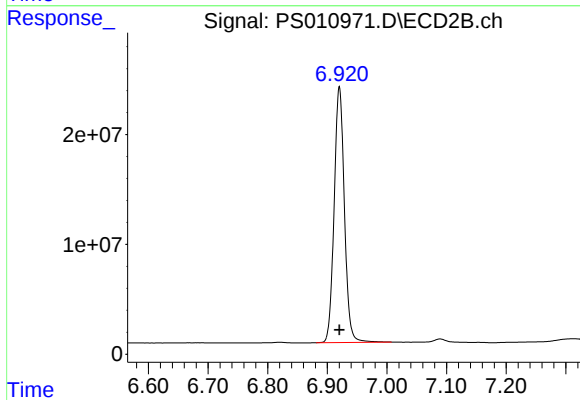


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 278421277
Conc: 502.50 ng/ml

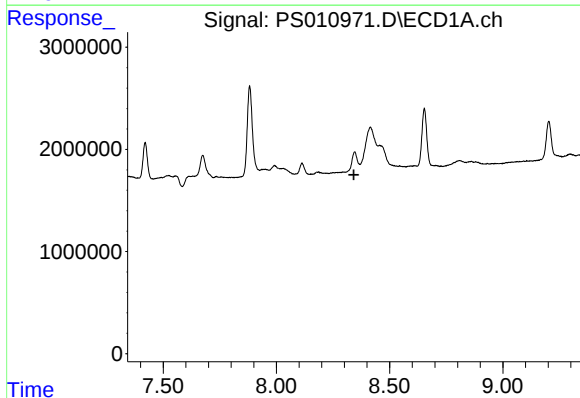


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

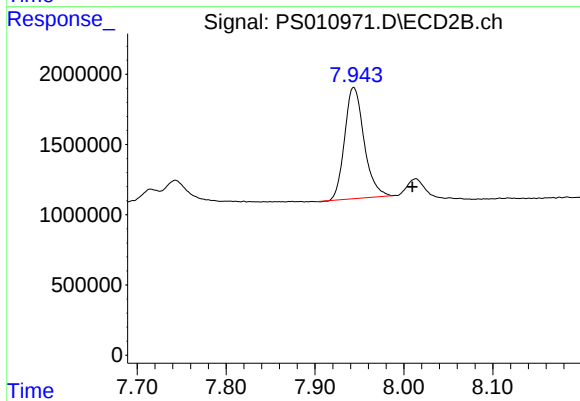

#9 2,4-D


R.T.: 7.944 min
Delta R.T.: -0.066 min
Response: 12016265
Conc: 16.63 ng/ml

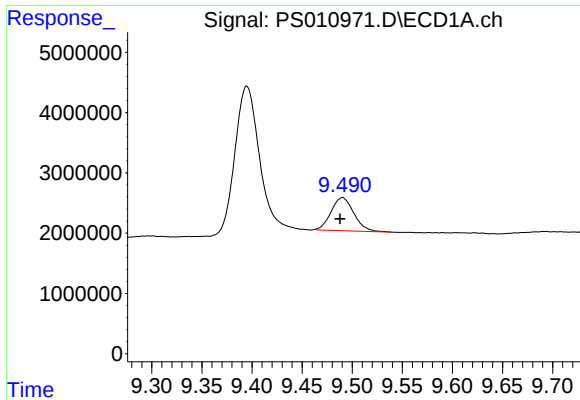

#12 2,4,5-T


R.T.: 9.490 min
Delta R.T.: 0.002 min
Response: 8693447
Conc: 1.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

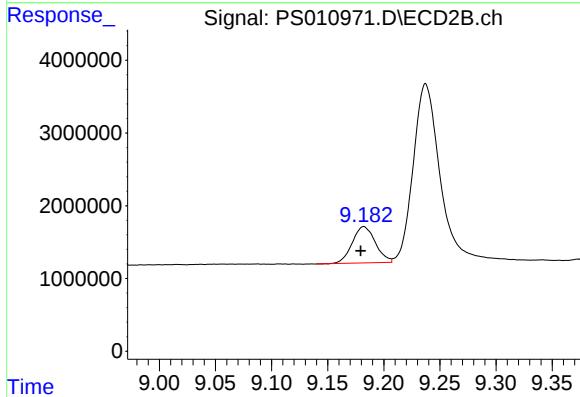


#12 2,4,5-T

R.T.: 9.182 min
Delta R.T.: 0.003 min
Response: 7162331
Conc: 2.41 ng/ml

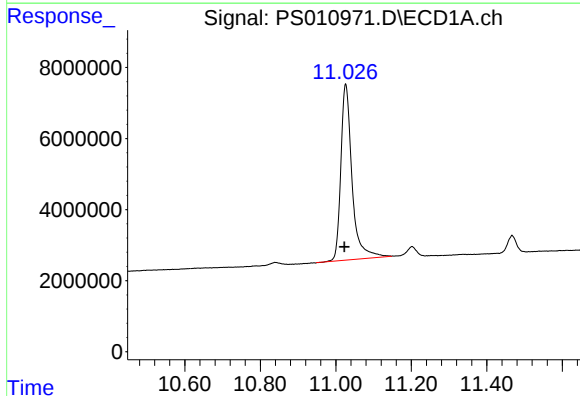


#15 Picloram

R.T.: 11.026 min
Delta R.T.: 0.004 min
Response: 101790995
Conc: 18.16 ng/ml

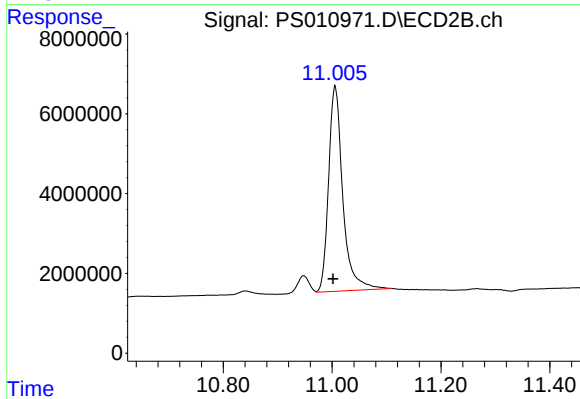

#15 Picloram


R.T.: 11.005 min
Delta R.T.: 0.003 min
Response: 93248192
Conc: 22.26 ng/ml

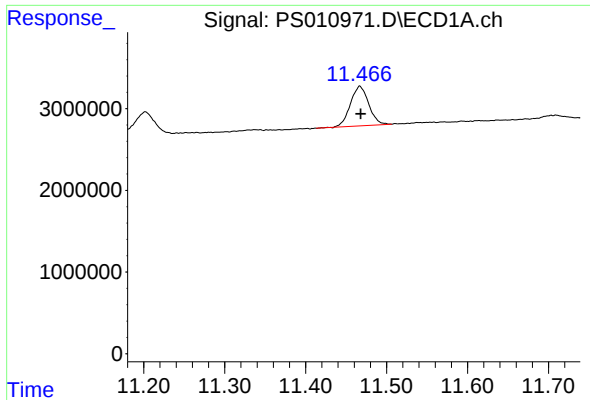

#16 DCPA

R.T.: 11.467 min
Delta R.T.: 0.000 min
Response: 7608994
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

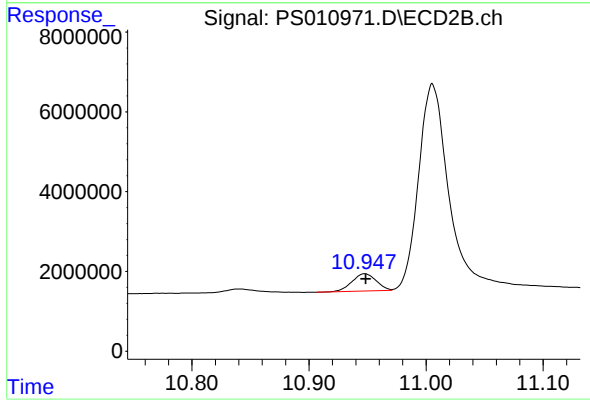

#16 DCPA

R.T.: 10.948 min
Delta R.T.: 0.000 min
Response: 6270298
Conc: 1.68 ng/ml