

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
 Data File : PS010975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2020 21:38
 Operator : DD\AJ
 Sample : PB129810BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB129810BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 04:02:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	411.1E6	281.3E6	453.289	507.744
Target Compounds							
1) T	Dalapon	2.998	2.586	35807361	85675941	31.979	113.574 #
2) T	3,5-DICHL...	0.000	6.100	0	70642432	N.D.	84.823
3) T	4-Nitroph...	7.002	0.000	4557214	0	11.417	N.D. #
7) T	MCPA	7.716	7.384	12887397	38152107	3.236	13.823 #
8) T	DICHLORPROP	0.000	7.740	0	9805891	N.D.	16.701
10) T	Pentachlo...	8.709	0.000	9058630	0	<MDL	N.D. #
12) T	2,4,5-T	9.509	0.000	6897132	0	1.481	N.D. #
14) T	DINOSEB	0.000	10.036	0	9834614	N.D.	4.723
15) T	Picloram	10.994	0.000	28964409	0	5.167	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062620\
Data File : PS010975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2020 21:38
Operator : DD\AJ
Sample : PB129810BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB129810BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:02:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

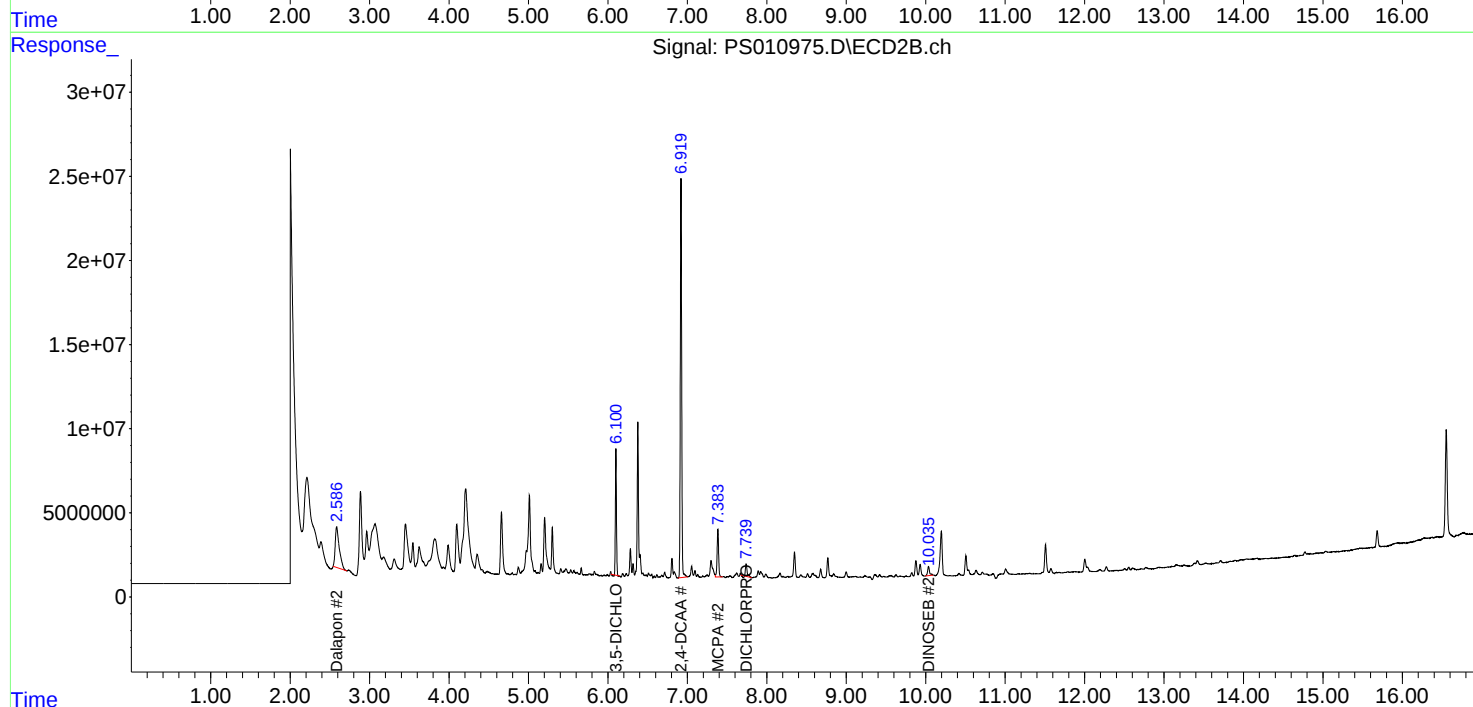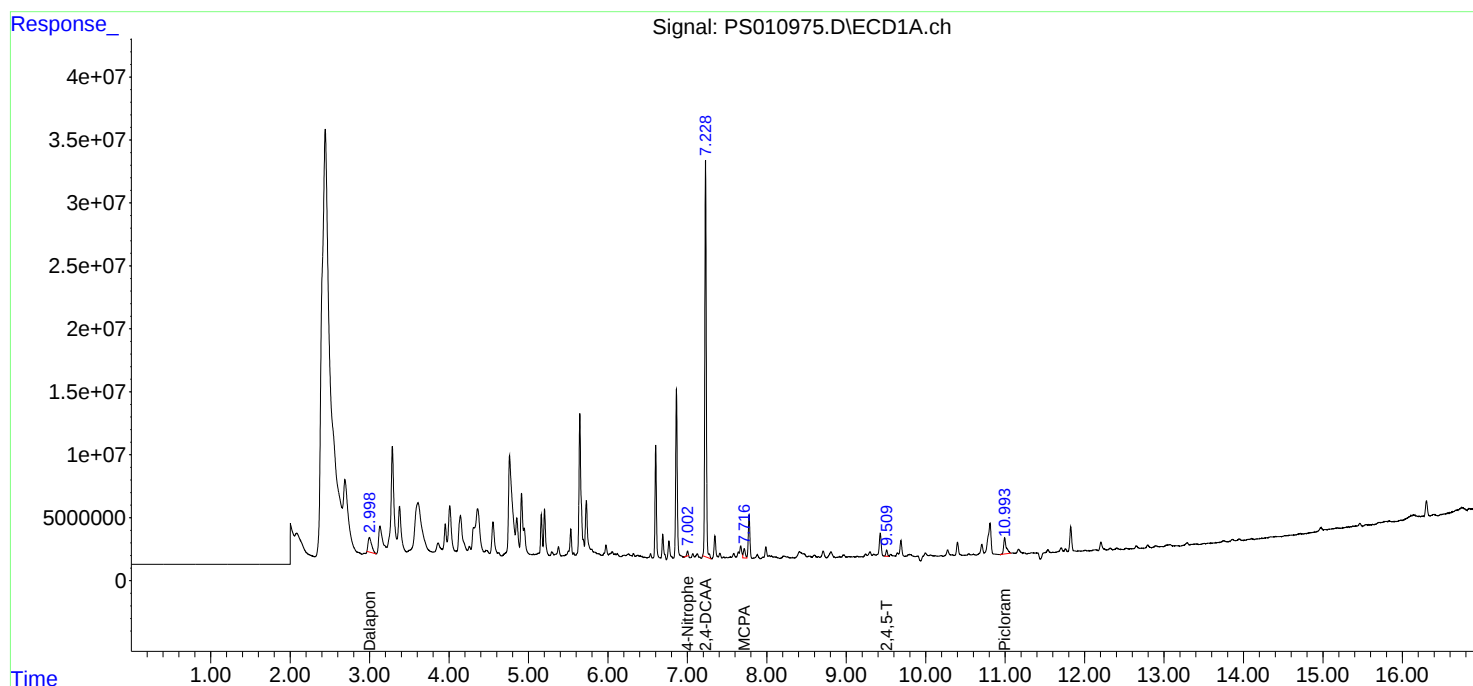


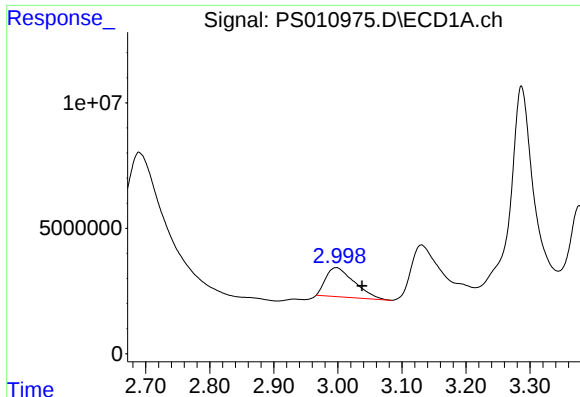

#1 Dalapon


R.T.: 2.998 min
Delta R.T.: -0.040 min
Response: 35807361
Conc: 31.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129810BL

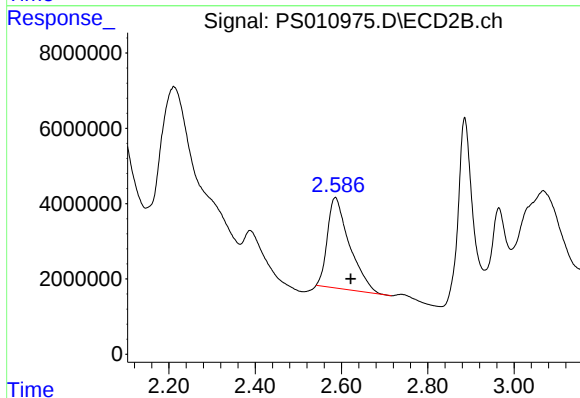


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 85675941
Conc: 113.57 ng/ml

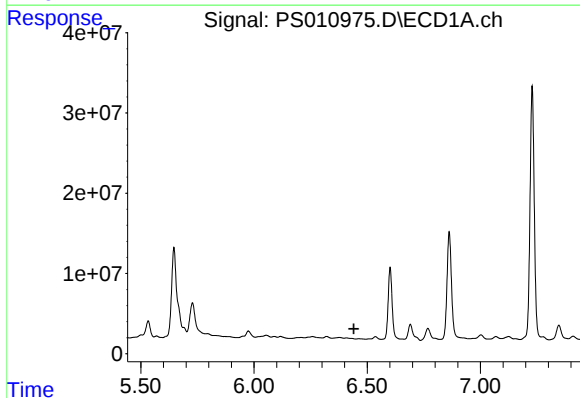


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

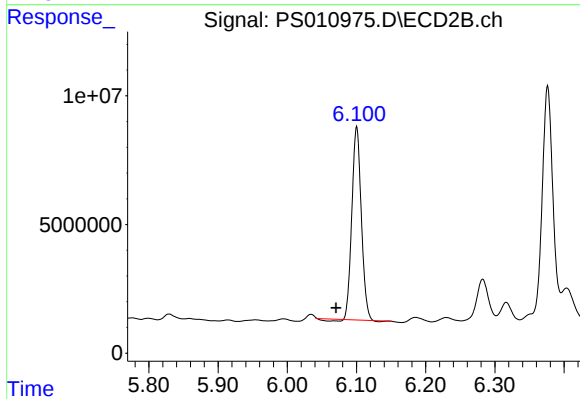

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 70642432
Conc: 84.82 ng/ml

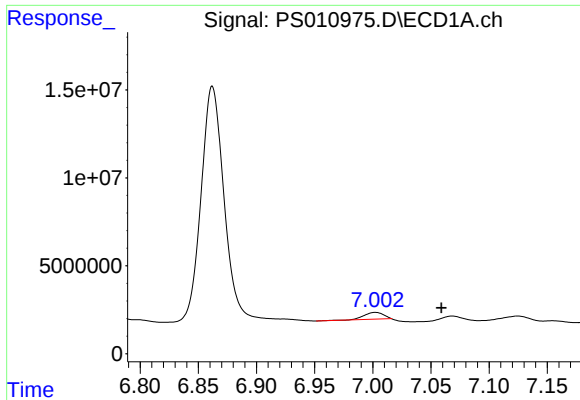

#3 4-Nitrophenol


R.T.: 7.002 min
Delta R.T.: -0.057 min
Response: 4557214
Conc: 11.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129810BL

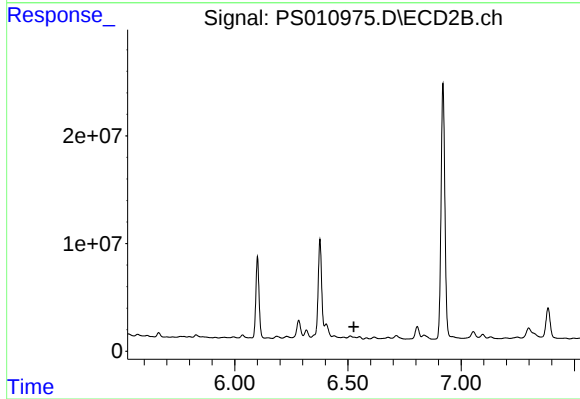


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.526 min
Response: 0
Conc: N.D.

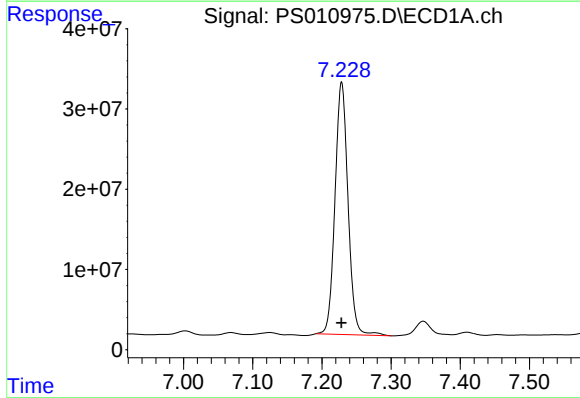


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 411050936
Conc: 453.29 ng/ml

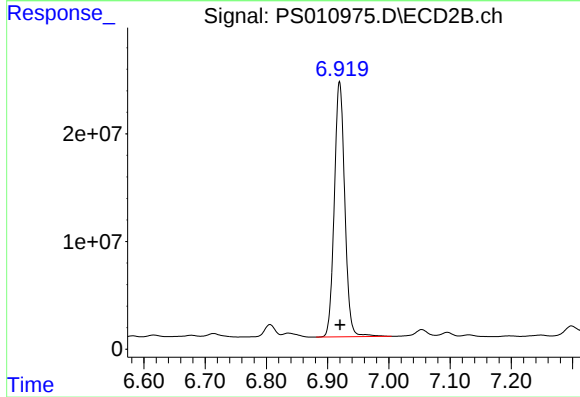

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 281328910
Conc: 507.74 ng/ml

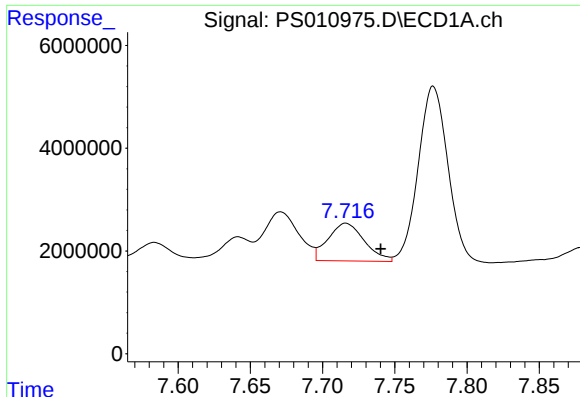

#7 MCPA


R.T.: 7.716 min
Delta R.T.: -0.024 min
Response: 12887397
Conc: 3.24 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB129810BL

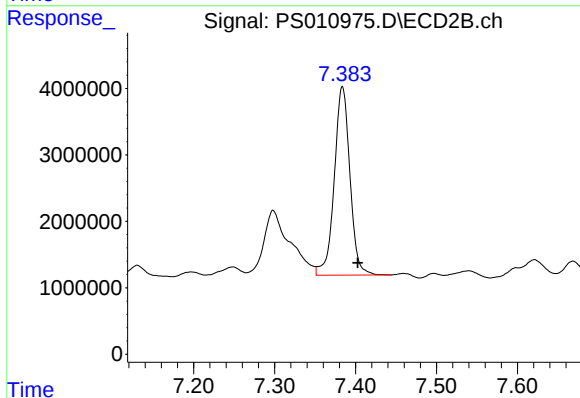


#7 MCPA

R.T.: 7.384 min
Delta R.T.: -0.019 min
Response: 38152107
Conc: 13.82 ug/ml

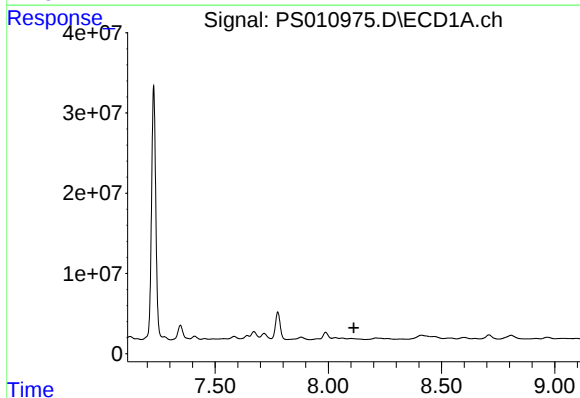


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

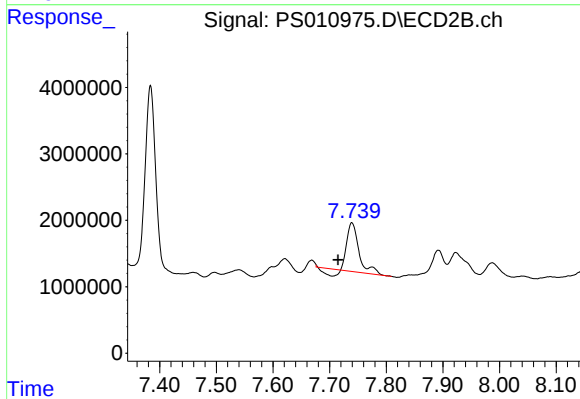

#8 DICHLORPROP


R.T.: 7.740 min
Delta R.T.: 0.024 min
Response: 9805891
Conc: 16.70 ng/ml

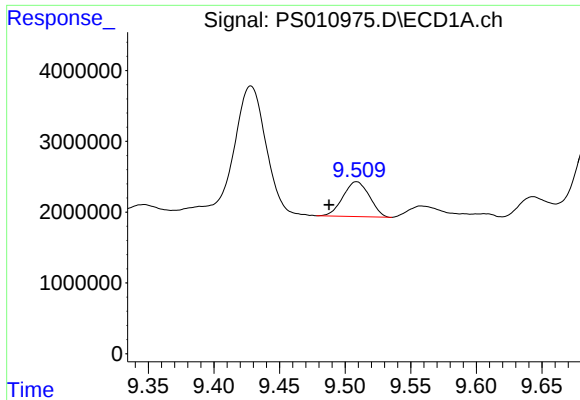

#12 2,4,5-T


R.T.: 9.509 min
Delta R.T.: 0.021 min
Response: 6897132
Conc: 1.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129810BL

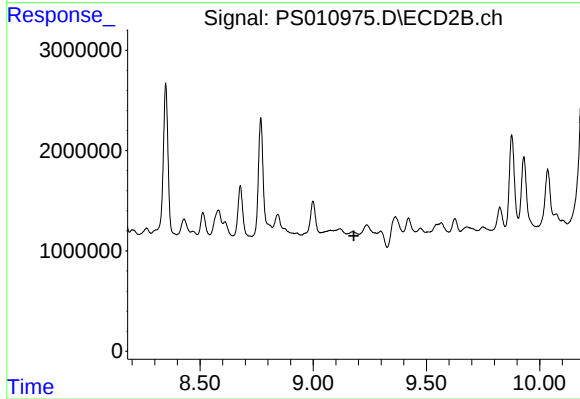


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

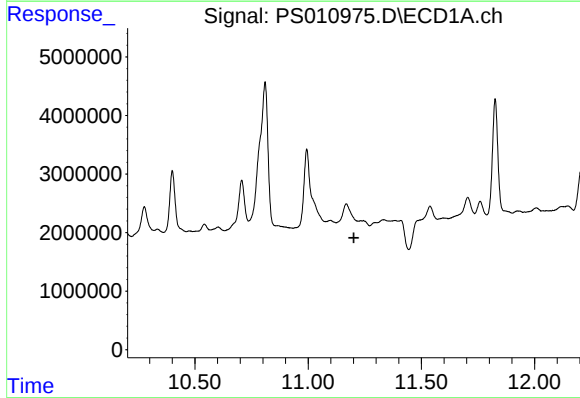


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.202 min
Response: 0
Conc: N.D.

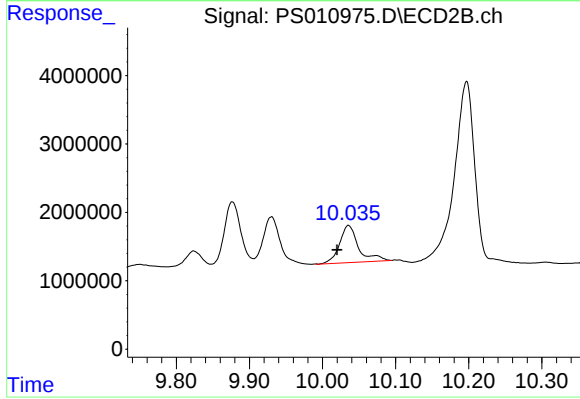

#14 DINOSEB


R.T.: 10.036 min
Delta R.T.: 0.016 min
Response: 9834614
Conc: 4.72 ng/ml

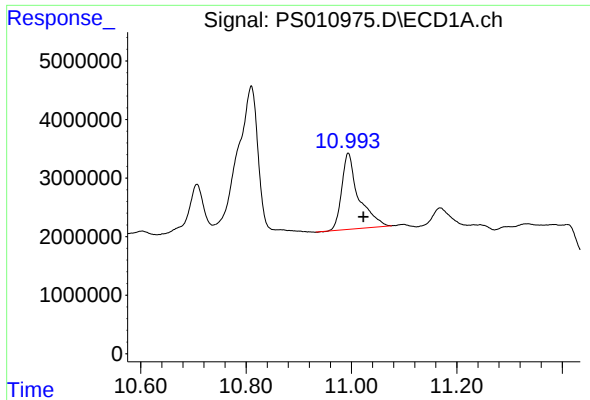

#15 Picloram

R.T.: 10.994 min
Delta R.T.: -0.029 min
Response: 28964409
Conc: 5.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB129810BL

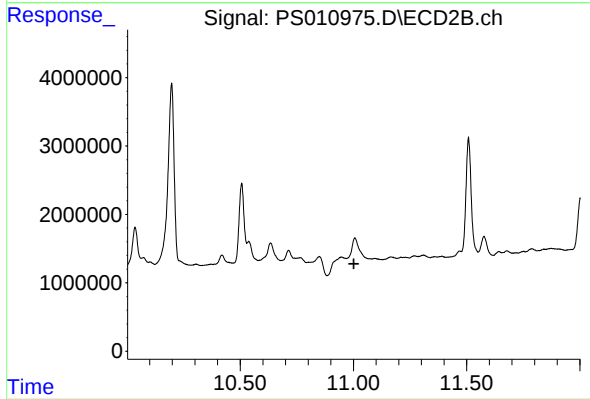

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.